

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032819\
 Data File : PS003818.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2019 17:32
 Operator : EI\SJ
 Sample : K2086-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 05:02:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.265	10.767	217.0E6	206.8E6	497.381	421.437
Target Compounds							
1) T	Dalapon	2.784	2.279	43710498	100.8E6	58.630	138.102 #
2) T	3,5-DICHL...	0.000	8.932	0	5010527	N.D.	7.855 #
3) T	4-Nitroph...	0.000	9.940	0	17866892	N.D.	78.697 #
5) T	DICAMBA	0.000	11.106	0	139576	N.D.	0.075 #
7) T	MCPA	12.215	11.674	78609846	985162	37.260	0.552 #
9) T	2,4-D	0.000	12.626	0	2005147	N.D.	3.770 #
10) T	Pentachlo...	0.000	13.174	0	861616	N.D.	0.125 #
11) T	2,4,5-TP ...	0.000	13.801	0	1089591	N.D.	0.411 #
12) T	2,4,5-T	0.000	14.402	0	10966072	N.D.	5.044 #
14) T	DINOSEB	0.000	15.496	0	2296266	N.D.	1.197 #
15) T	Picloram	0.000	16.706	0	15776164	N.D.	4.975 #
16) T	DCPA	0.000	16.619	0	3262059	N.D.	0.965 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032819\
Data File : PS003818.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2019 17:32
Operator : EI\SJ
Sample : K2086-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 05:02:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

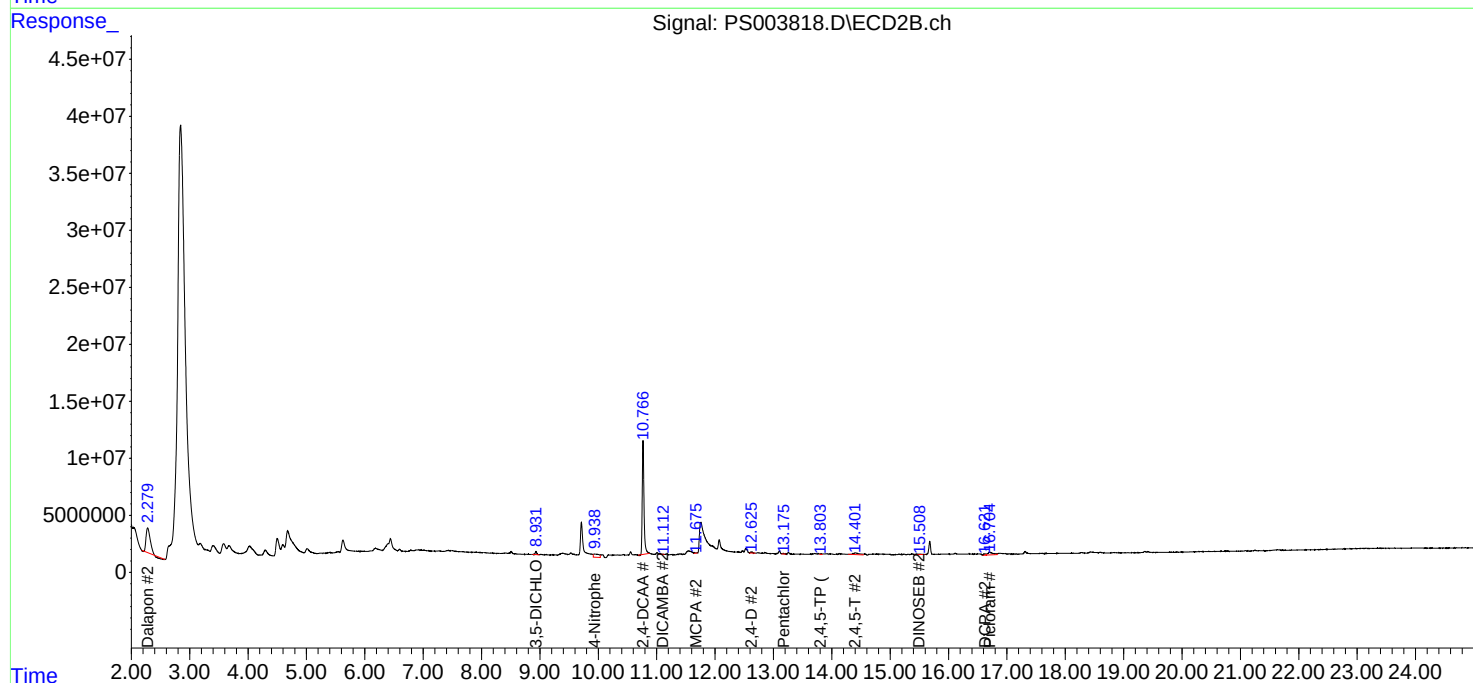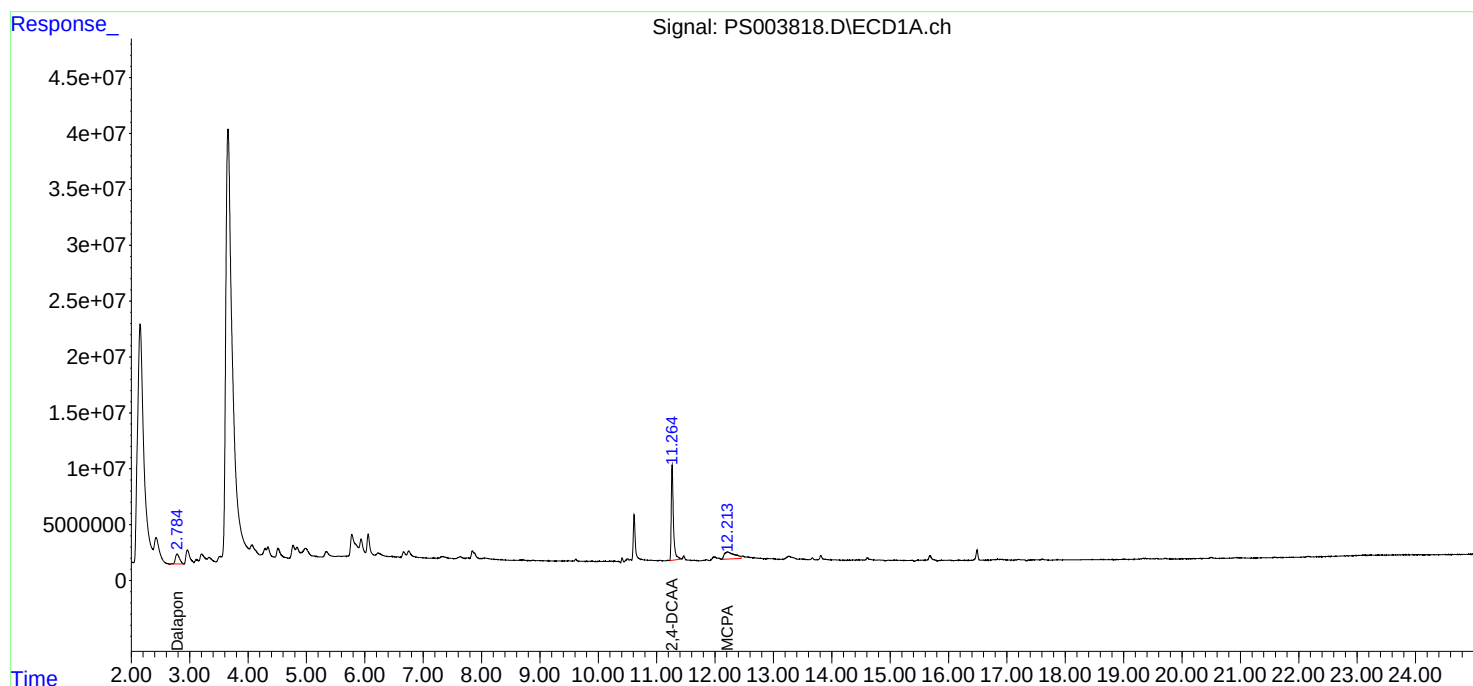


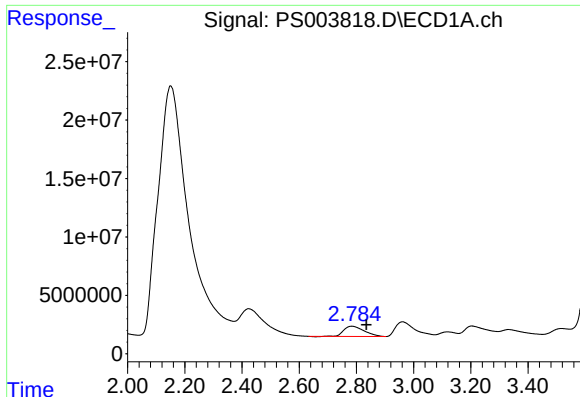

#1 Dalapon


R.T.: 2.784 min
Delta R.T.: -0.051 min
Response: 43710498
Conc: 58.63 ng/ml

Instrument :
ECD_S
ClientSampleId :

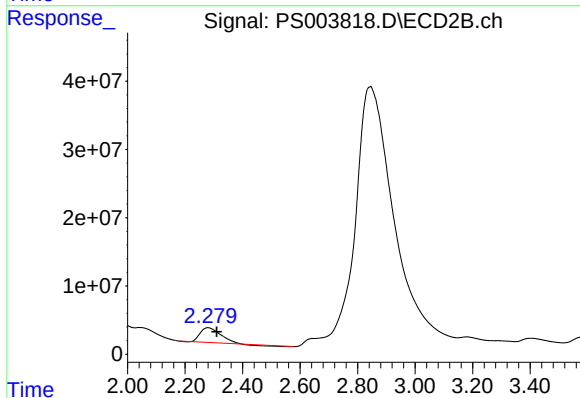


#1 Dalapon

R.T.: 2.279 min
Delta R.T.: -0.031 min
Response: 100763288
Conc: 138.10 ng/ml

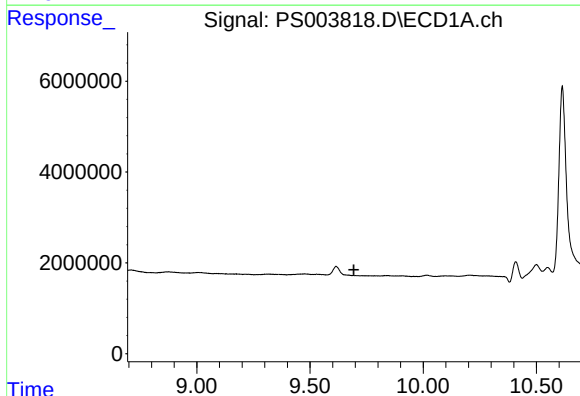


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

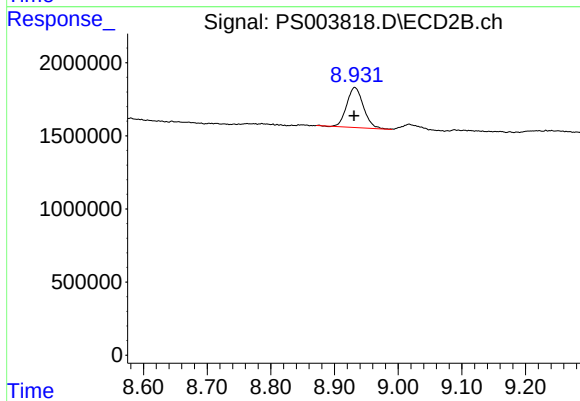

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.932 min
Delta R.T.: 0.000 min
Response: 5010527
Conc: 7.86 ng/ml

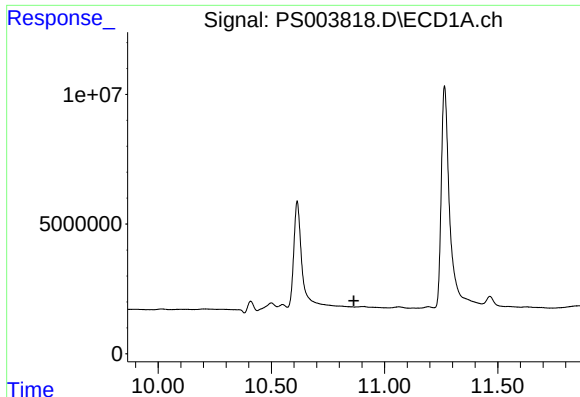

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

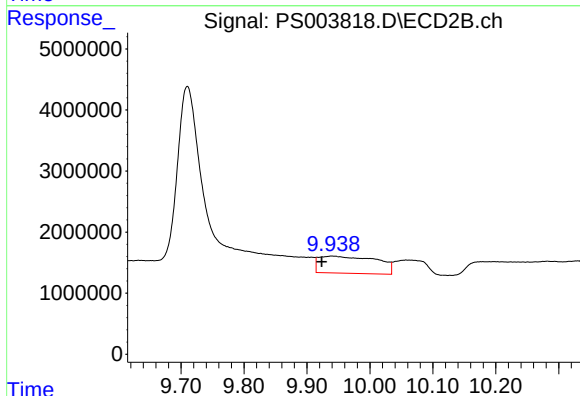


#3 4-Nitrophenol

R.T.: 9.940 min
Delta R.T.: 0.017 min
Response: 17866892
Conc: 78.70 ng/ml

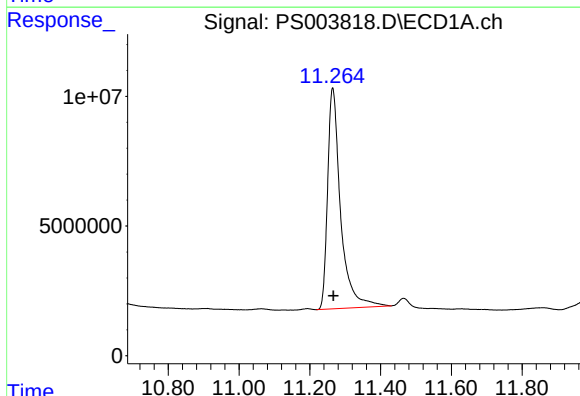


#4 2,4-DCAA

R.T.: 11.265 min
Delta R.T.: -0.001 min
Response: 216963636
Conc: 497.38 ng/ml

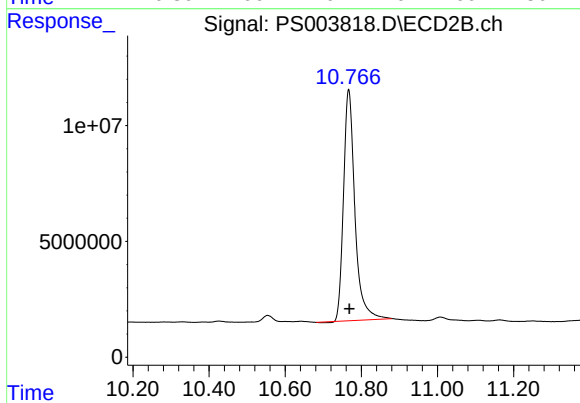

#4 2,4-DCAA


R.T.: 10.767 min
Delta R.T.: -0.002 min
Response: 206781560
Conc: 421.44 ng/ml

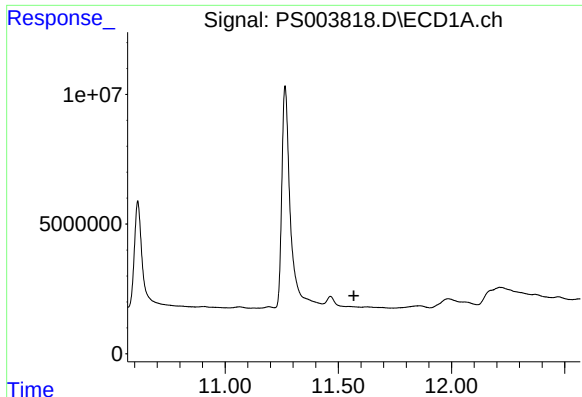

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

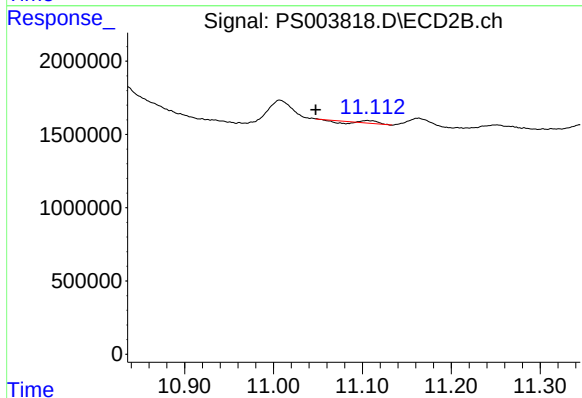


#5 DICAMBA

R.T.: 11.106 min
Delta R.T.: 0.059 min
Response: 139576
Conc: 0.08 ng/ml

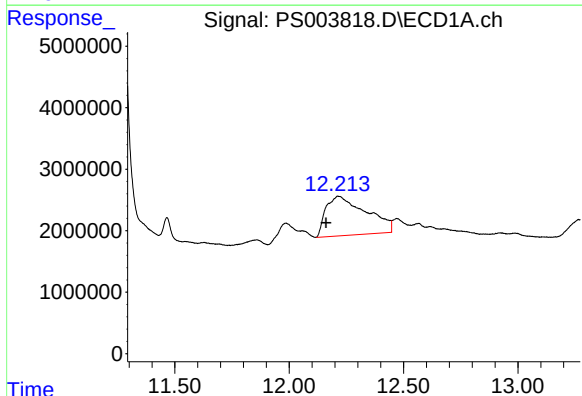


#7 MCPA

R.T.: 12.215 min
Delta R.T.: 0.054 min
Response: 78609846
Conc: 37.26 ug/ml

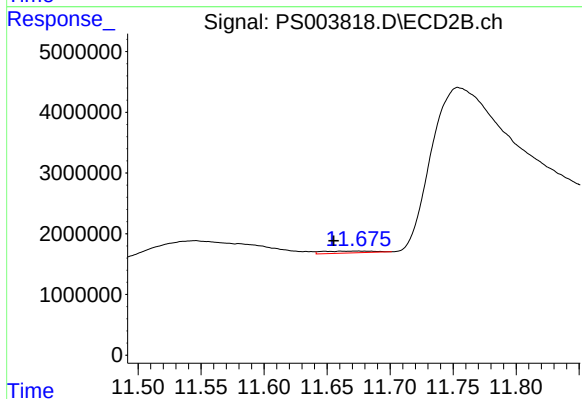

#7 MCPA


R.T.: 11.674 min
Delta R.T.: 0.019 min
Response: 985162
Conc: 0.55 ug/ml

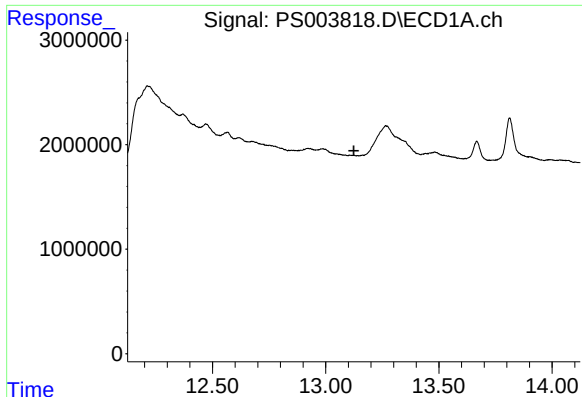

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

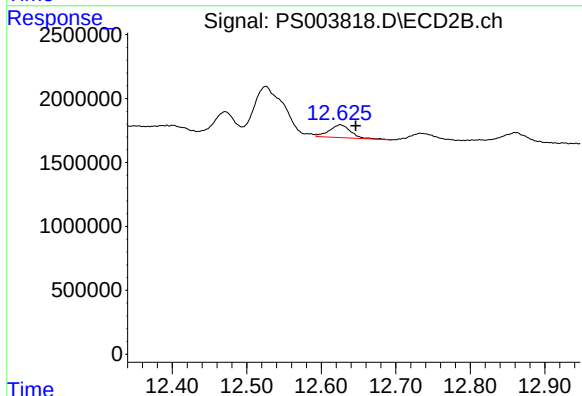


#9 2,4-D

R.T.: 12.626 min
Delta R.T.: -0.021 min
Response: 2005147
Conc: 3.77 ng/ml

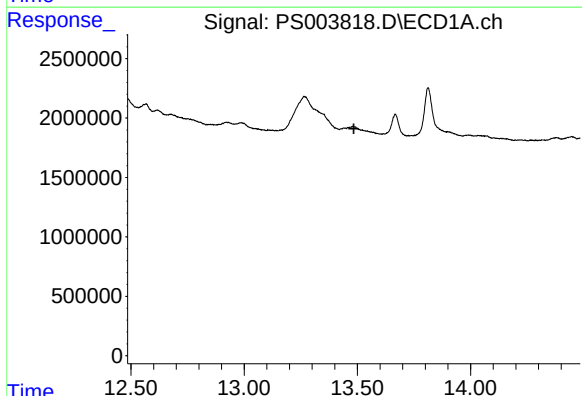


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.485 min
Response: 0
Conc: N.D.

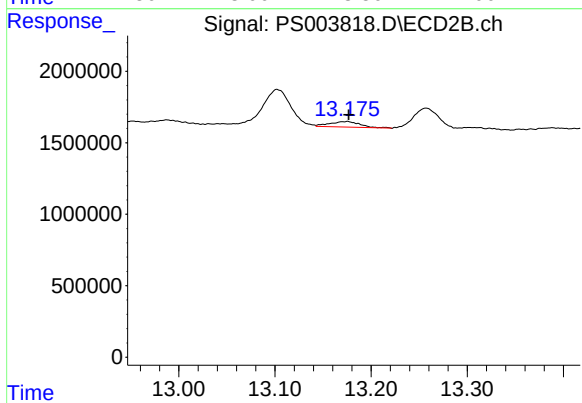

#10 Pentachlorophenol


R.T.: 13.174 min
Delta R.T.: -0.003 min
Response: 861616
Conc: 0.12 ng/ml

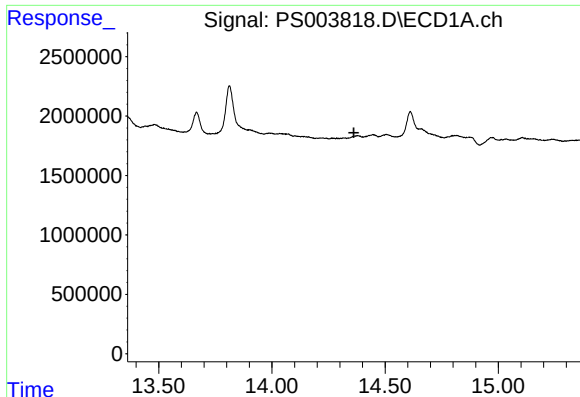

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

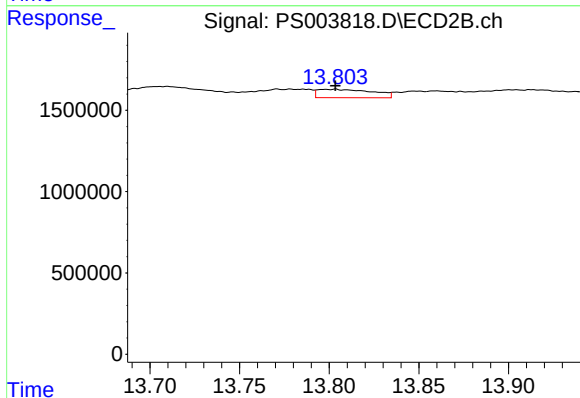


#11 2,4,5-TP (SILVEX)

R.T.: 13.801 min
Delta R.T.: -0.002 min
Response: 1089591
Conc: 0.41 ng/ml

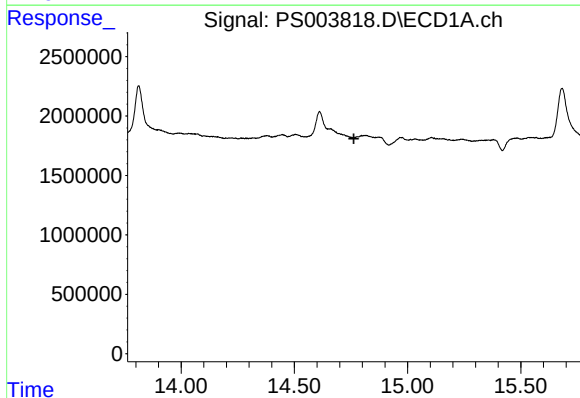


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.763 min
Response: 0
Conc: N.D.

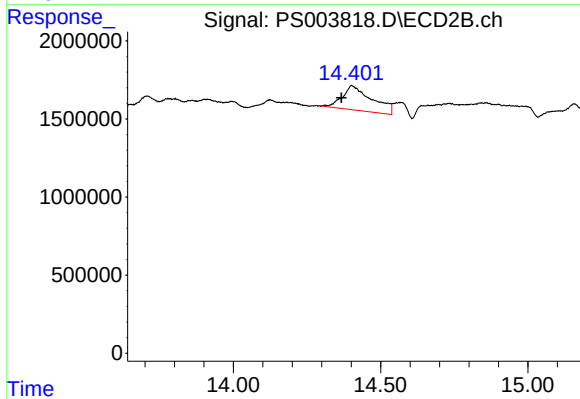

#12 2,4,5-T


R.T.: 14.402 min
Delta R.T.: 0.035 min
Response: 10966072
Conc: 5.04 ng/ml

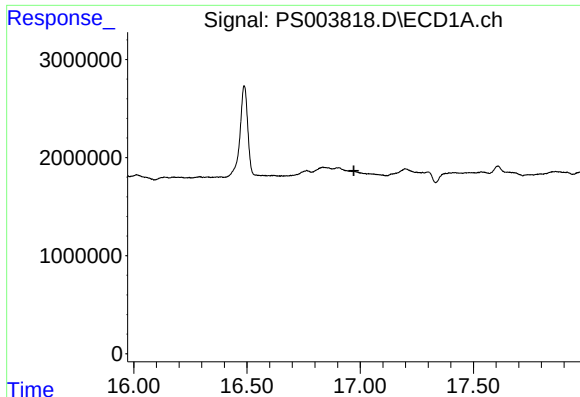

#14 DINoseb


R.T.: 0.000 min
Exp R.T. : 16.972 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

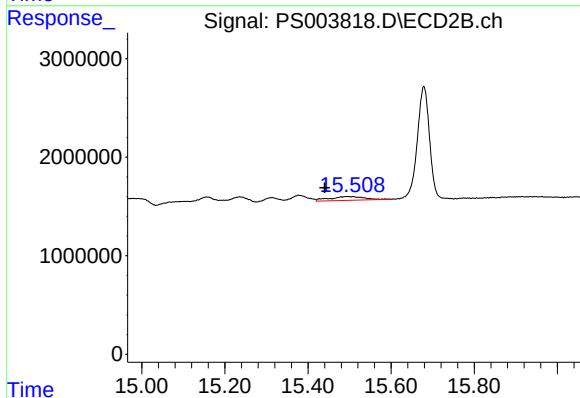


#14 DINoseb

R.T.: 15.496 min
Delta R.T.: 0.056 min
Response: 2296266
Conc: 1.20 ng/ml

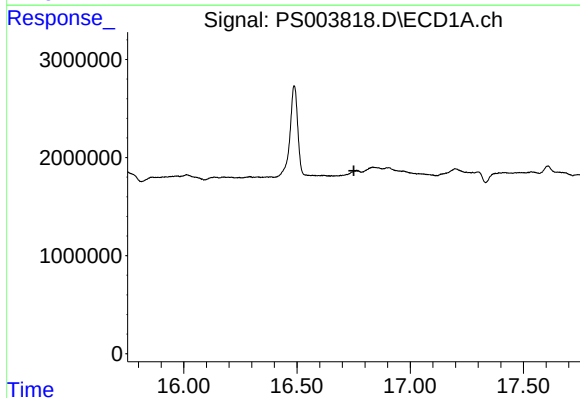


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.752 min
Response: 0
Conc: N.D.

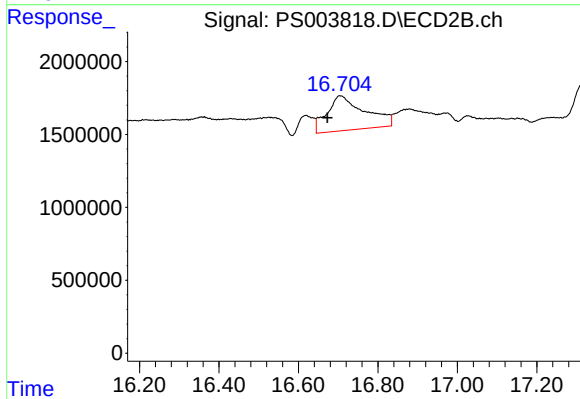

#15 Picloram


R.T.: 16.706 min
Delta R.T.: 0.033 min
Response: 15776164
Conc: 4.97 ng/ml

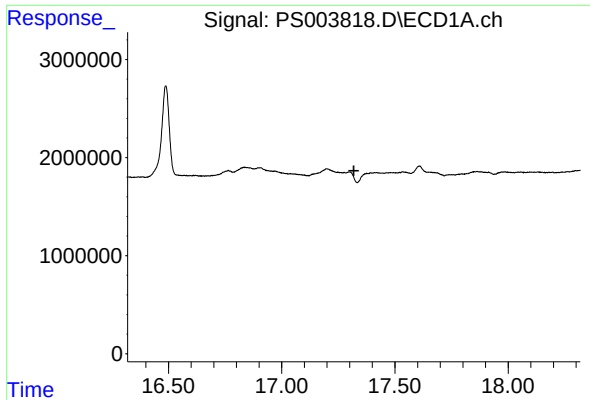

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

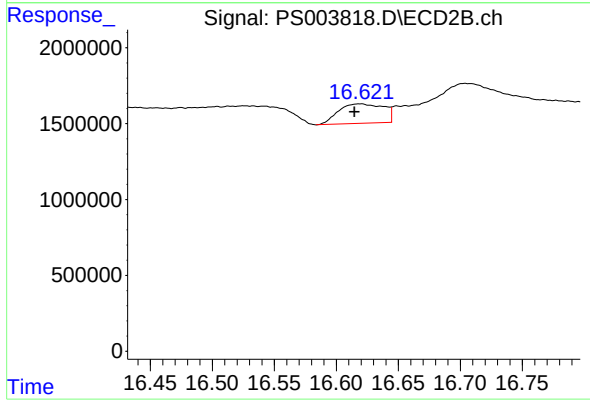

#16 DCPA

R.T.: 16.619 min
Delta R.T.: 0.005 min
Response: 3262059
Conc: 0.97 ng/ml