

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032819\
 Data File : PS003820.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2019 18:35
 Operator : EI\SJ
 Sample : K2086-13
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 05:03:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.265	10.768	216.5E6	205.0E6	496.304	417.734
Target Compounds							
1) T	Dalapon	2.782	2.283	46425566	120.7E6	62.272	165.404 #
2) T	3,5-DICHL...	0.000	8.931	0	4804092	N.D.	7.532 #
3) T	4-Nitroph...	0.000	9.940	0	17887283	N.D.	78.787 #
7) T	MCPA	12.163	11.671	34229978	637497	16.224	0.357 #
9) T	2,4-D	0.000	12.626	0	2344566	N.D.	4.408 #
10) T	Pentachlo...	0.000	13.172	0	635244	N.D.	0.092 #
11) T	2,4,5-TP ...	0.000	13.777	0	2556299	N.D.	0.965 #
12) T	2,4,5-T	0.000	14.434	0	8055277	N.D.	3.705 #
13) T	2,4-DB	0.000	14.996	0	1573991	N.D.	5.301 #
14) T	DINOSEB	0.000	15.492	0	2824027	N.D.	1.472 #
15) T	Picloram	0.000	16.715	0	8637420	N.D.	2.724 #
16) T	DCPA	0.000	16.620	0	3979462	N.D.	1.177 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032819\
Data File : PS003820.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2019 18:35
Operator : EI\SJ
Sample : K2086-13
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 05:03:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

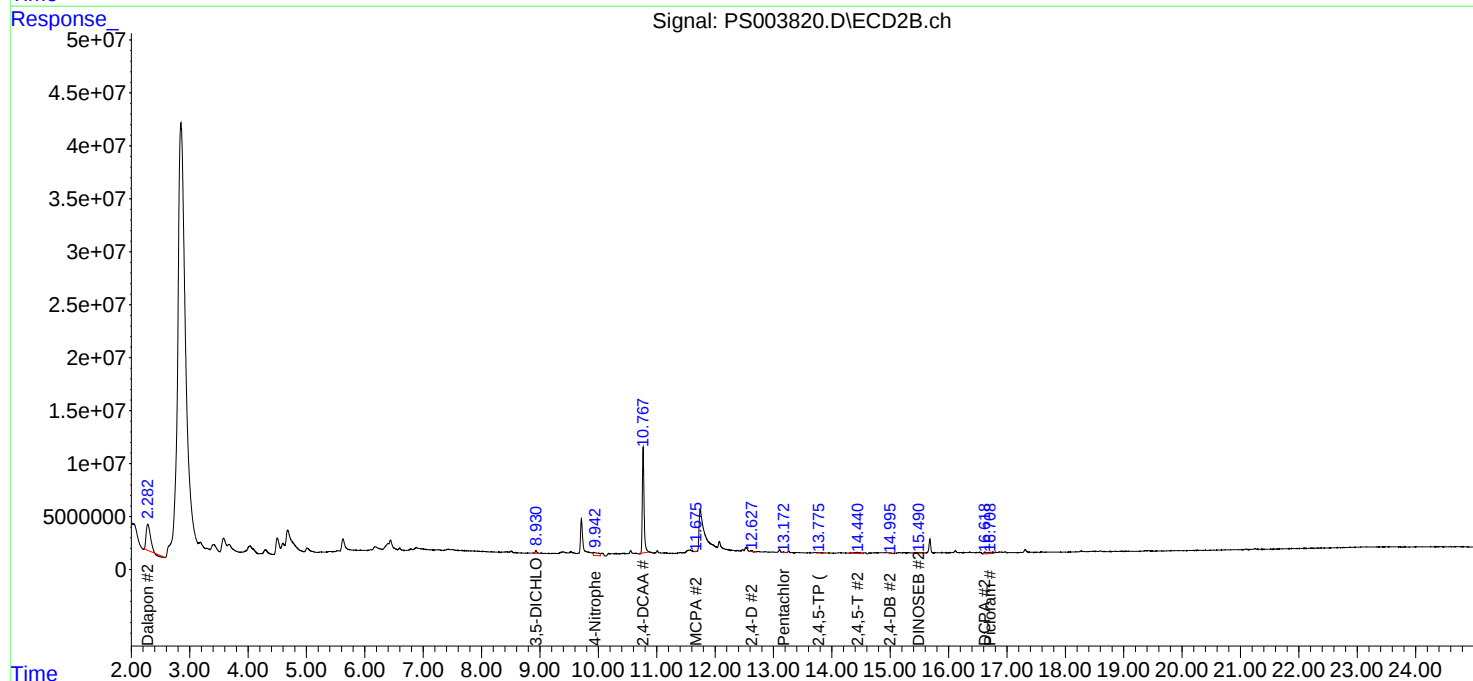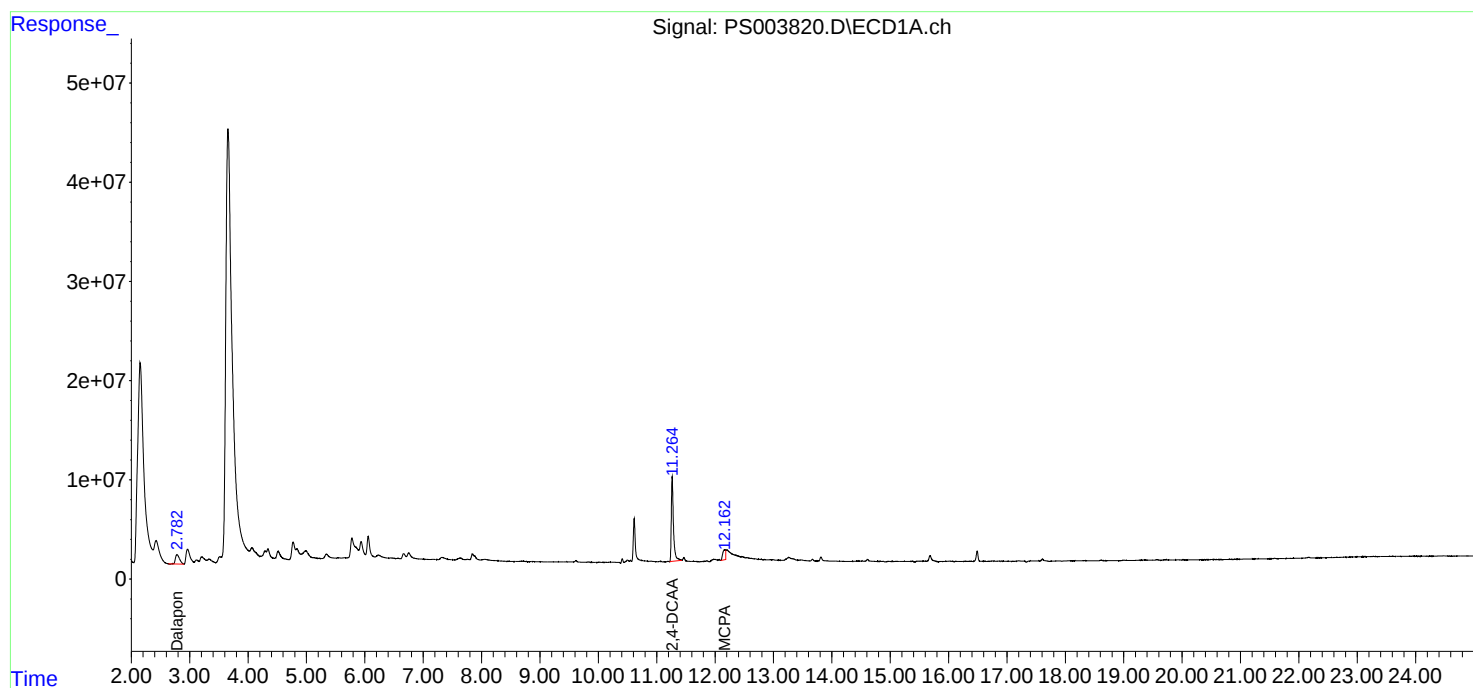


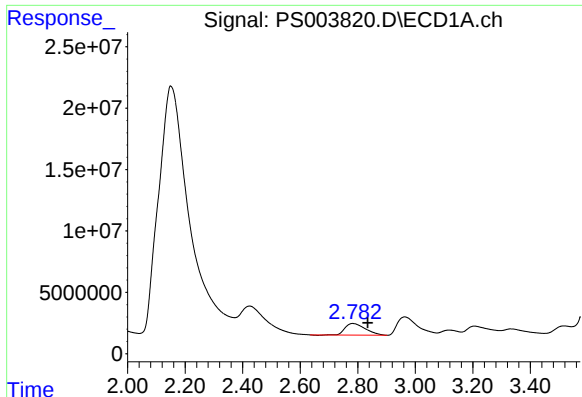

#1 Dalapon


R.T.: 2.782 min
Delta R.T.: -0.053 min
Response: 46425566
Conc: 62.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

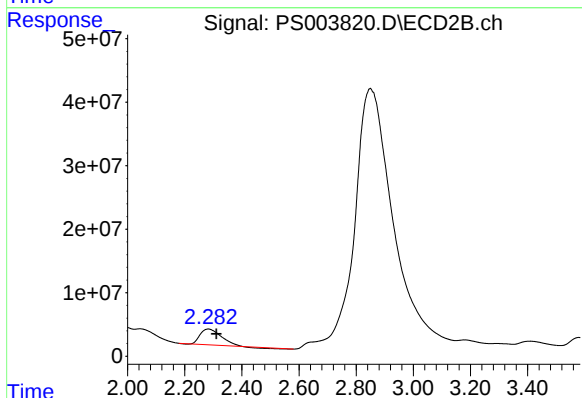


#1 Dalapon

R.T.: 2.283 min
Delta R.T.: -0.028 min
Response: 120683705
Conc: 165.40 ng/ml

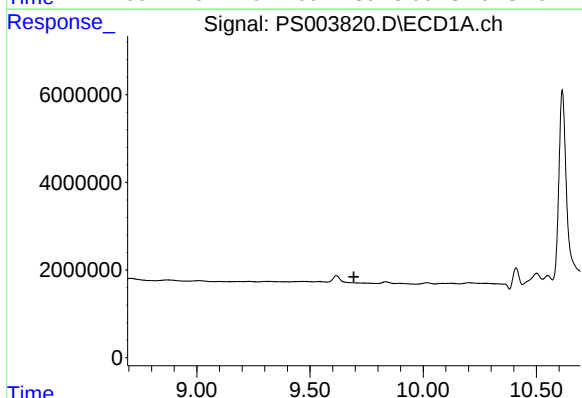


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

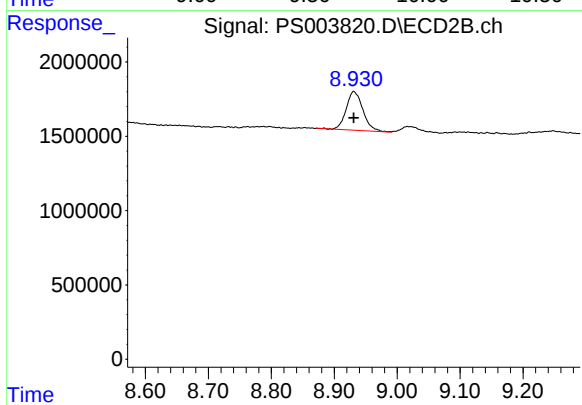

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.931 min
Delta R.T.: 0.000 min
Response: 4804092
Conc: 7.53 ng/ml

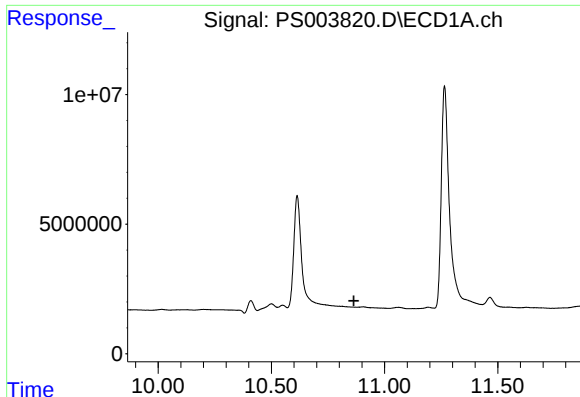

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

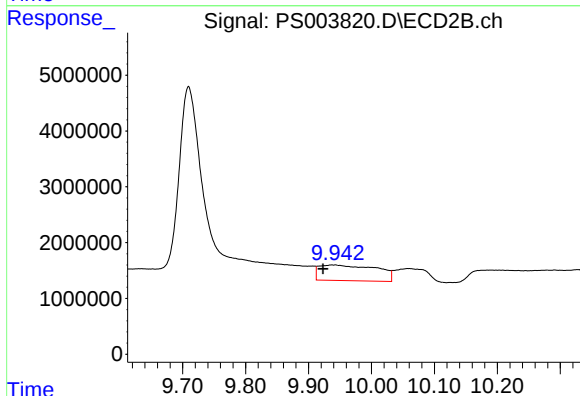


#3 4-Nitrophenol

R.T.: 9.940 min
Delta R.T.: 0.016 min
Response: 17887283
Conc: 78.79 ng/ml

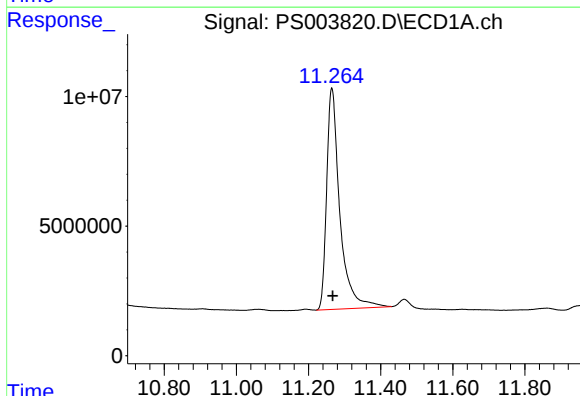


#4 2,4-DCAA

R.T.: 11.265 min
Delta R.T.: -0.002 min
Response: 216493913
Conc: 496.30 ng/ml

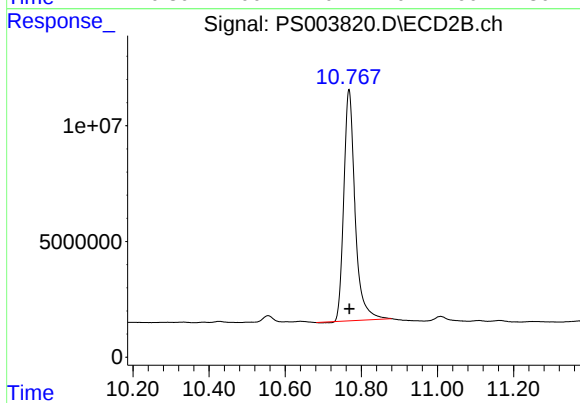

#4 2,4-DCAA


R.T.: 10.768 min
Delta R.T.: -0.001 min
Response: 204964851
Conc: 417.73 ng/ml

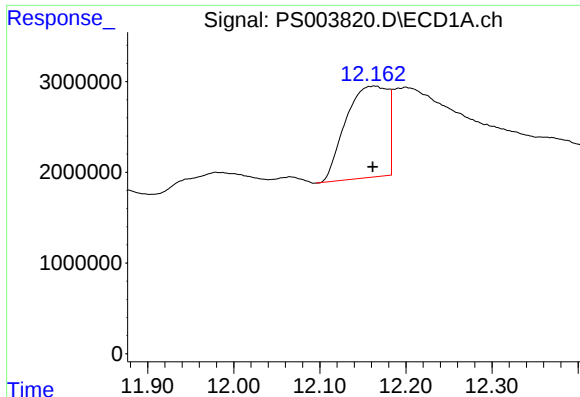

#7 MCPA


R.T.: 12.163 min
Delta R.T.: 0.001 min
Response: 34229978
Conc: 16.22 ug/ml

Instrument :
ECD_S
ClientSampleId :

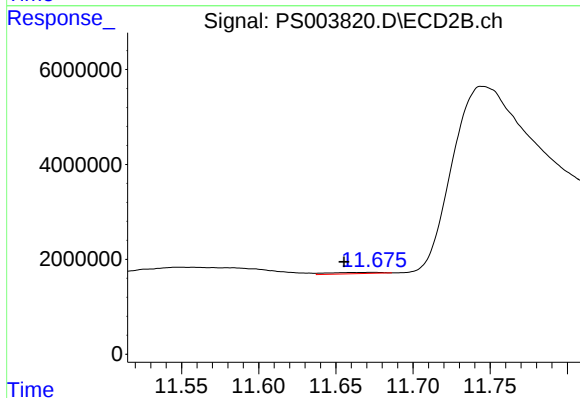


#7 MCPA

R.T.: 11.671 min
Delta R.T.: 0.016 min
Response: 637497
Conc: 0.36 ug/ml

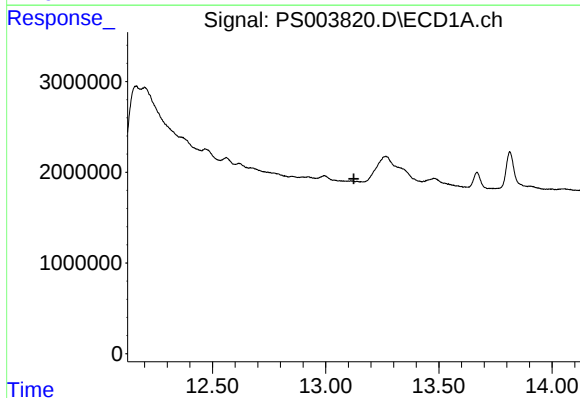


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.125 min
Response: 0
Conc: N.D.

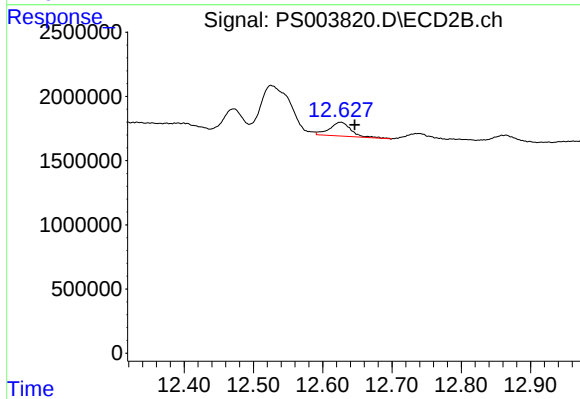

#9 2,4-D


R.T.: 12.626 min
Delta R.T.: -0.021 min
Response: 2344566
Conc: 4.41 ng/ml

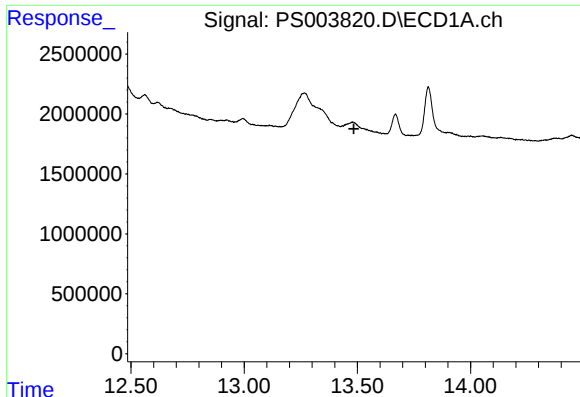

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.485 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

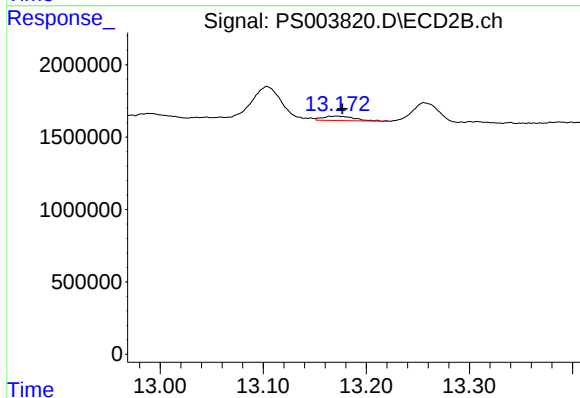


#10 Pentachlorophenol

R.T.: 13.172 min
Delta R.T.: -0.005 min
Response: 635244
Conc: 0.09 ng/ml

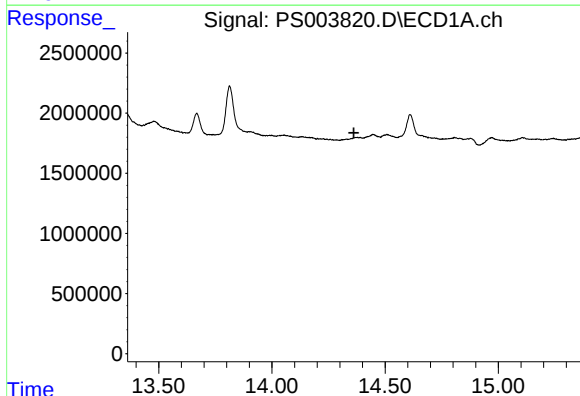


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

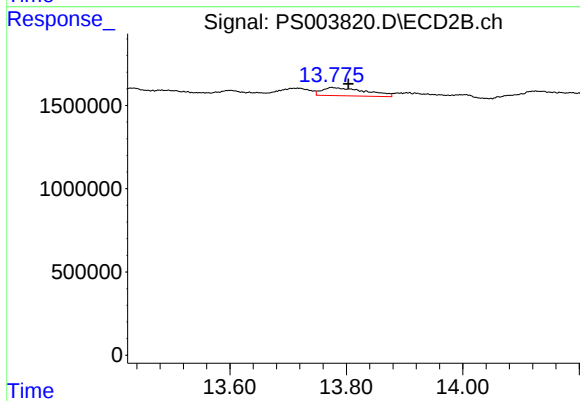

#11 2,4,5-TP (SILVEX)


R.T.: 13.777 min
Delta R.T.: -0.026 min
Response: 2556299
Conc: 0.97 ng/ml

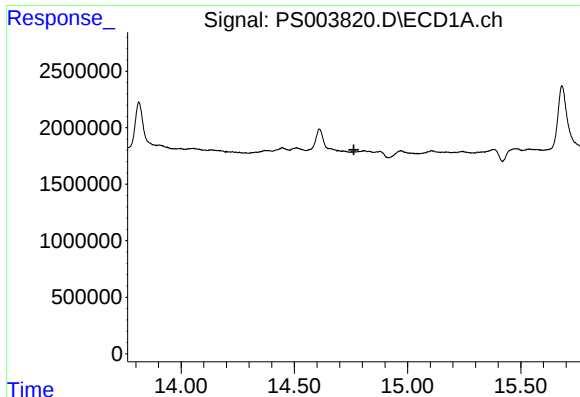

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.763 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

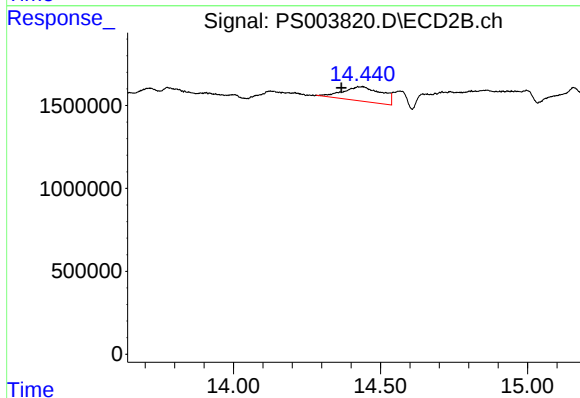


#12 2,4,5-T

R.T.: 14.434 min
Delta R.T.: 0.067 min
Response: 8055277
Conc: 3.71 ng/ml

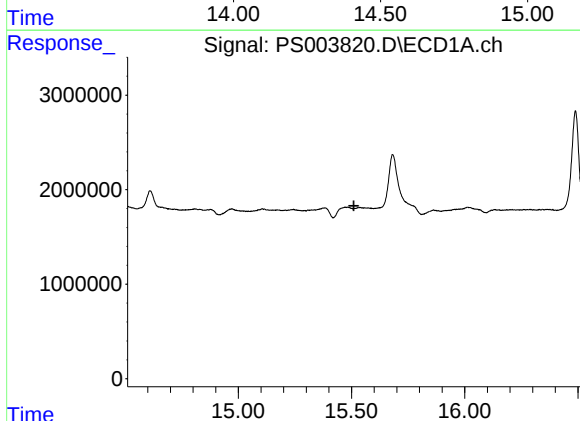


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

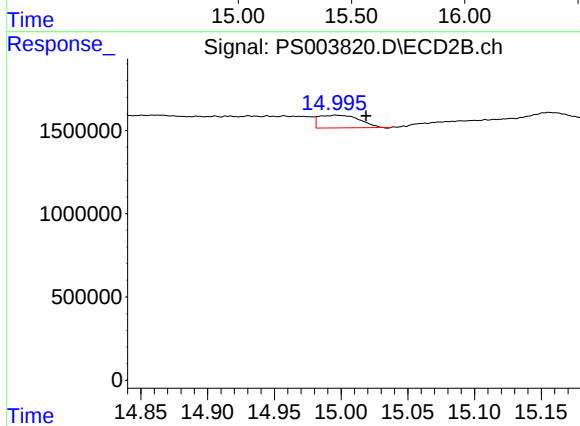

#13 2,4-DB


R.T.: 14.996 min
Delta R.T.: -0.023 min
Response: 1573991
Conc: 5.30 ng/ml

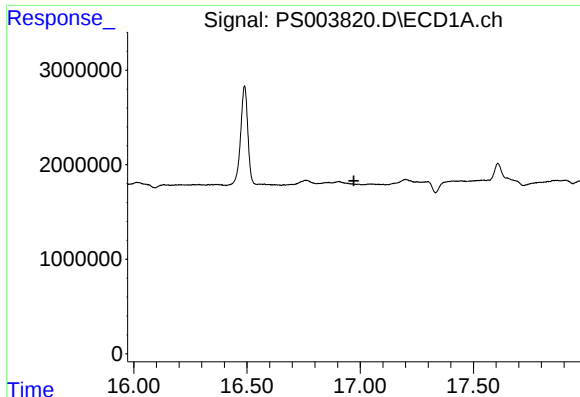

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 16.972 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

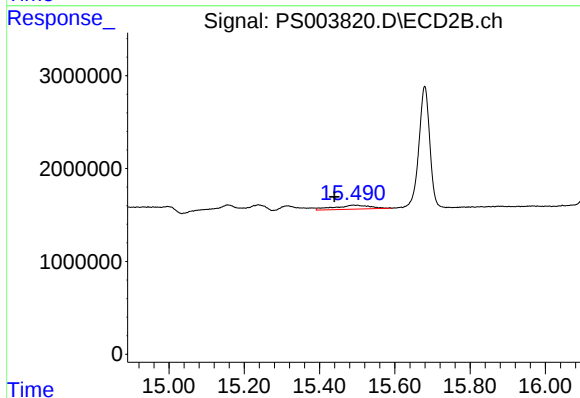


#14 DINOSEB

R.T.: 15.492 min
Delta R.T.: 0.052 min
Response: 2824027
Conc: 1.47 ng/ml

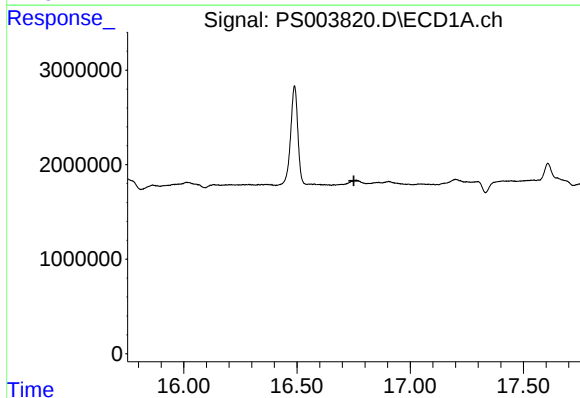


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.752 min
Response: 0
Conc: N.D.

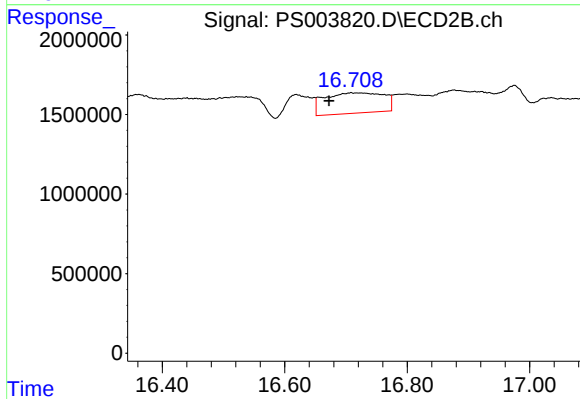

#15 Picloram


R.T.: 16.715 min
Delta R.T.: 0.042 min
Response: 8637420
Conc: 2.72 ng/ml

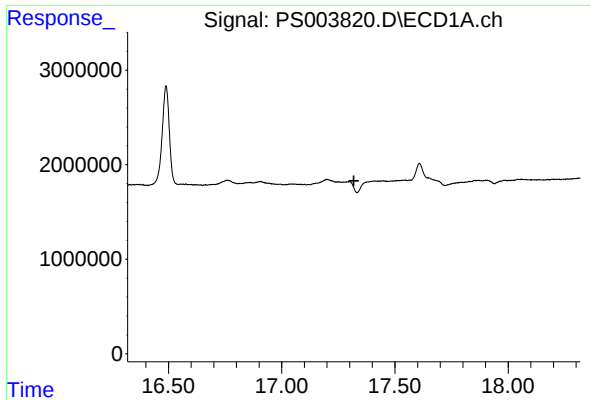

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

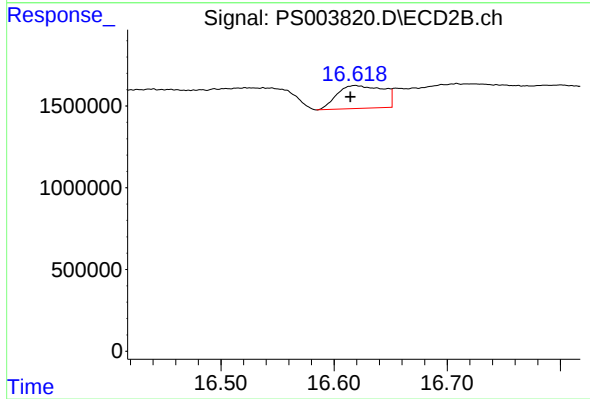

#16 DCPA

R.T.: 16.620 min
Delta R.T.: 0.006 min
Response: 3979462
Conc: 1.18 ng/ml