

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032819\
 Data File : PS003821.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2019 19:06
 Operator : EI\SJ
 Sample : K2086-14
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 05:03:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.264	10.767	248.8E6	234.3E6	570.442	477.427
Target Compounds							
1) T	Dalapon	2.784	2.283	48189033	109.5E6	64.637	150.063 #
2) T	3,5-DICHL...	0.000	8.932	0	4874912	N.D.	7.643 #
3) T	4-Nitroph...	0.000	9.938	0	17033739	N.D.	75.027 #
7) T	MCPA	12.158	0.000	38760199	0	18.372	N.D. #
9) T	2,4-D	0.000	12.626	0	2342052	N.D.	4.403 #
10) T	Pentachlo...	13.485	13.175	11252241	7472987	1.461	1.080 #
11) T	2,4,5-TP ...	0.000	13.779	0	2737087	N.D.	1.033 #
12) T	2,4,5-T	0.000	14.425	0	8187047	N.D.	3.766 #
13) T	2,4-DB	0.000	14.994	0	1426467	N.D.	4.804 #
14) T	DINOSEB	0.000	15.487	0	3046235	N.D.	1.588 #
15) T	Picloram	0.000	16.619	0	3995755	N.D.	1.260 #
16) T	DCPA	0.000	16.619	0	3995755	N.D.	1.182 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032819\
Data File : PS003821.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2019 19:06
Operator : EI\SJ
Sample : K2086-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 05:03:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

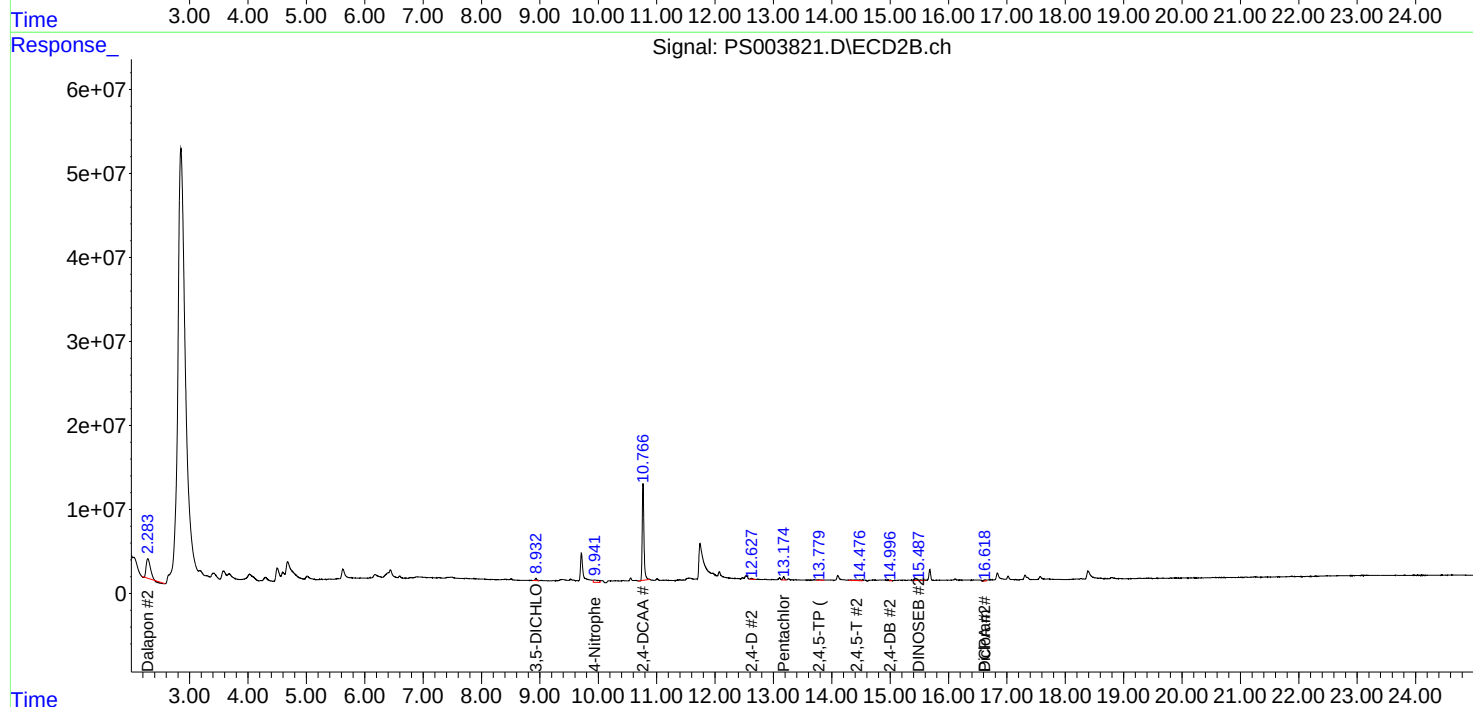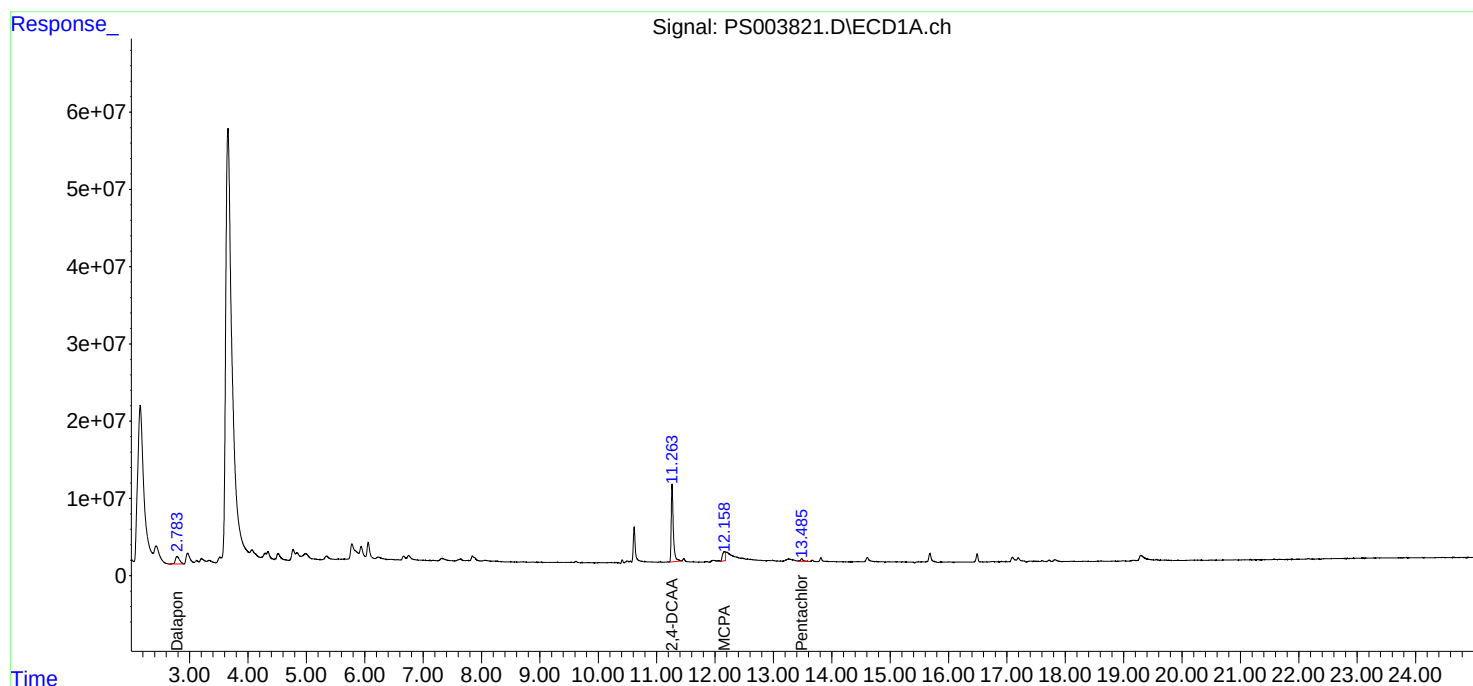


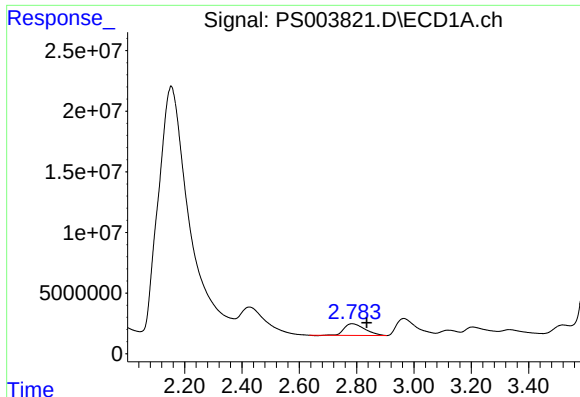

#1 Dalapon


R.T.: 2.784 min
Delta R.T.: -0.051 min
Response: 48189033
Conc: 64.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

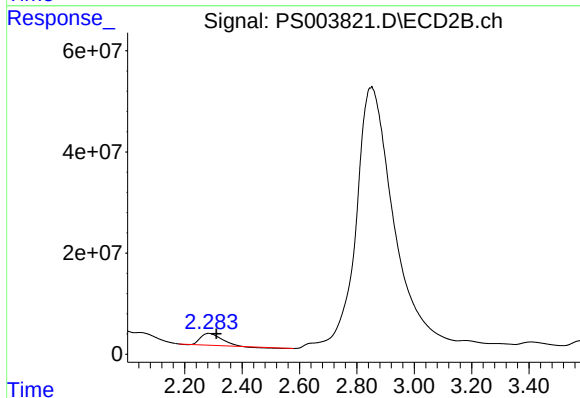


#1 Dalapon

R.T.: 2.283 min
Delta R.T.: -0.027 min
Response: 109490082
Conc: 150.06 ng/ml

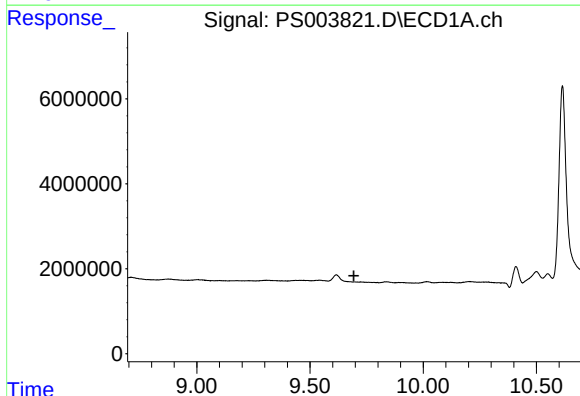


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

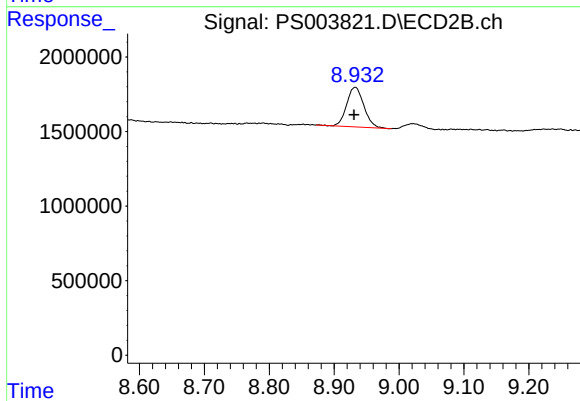

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.932 min
Delta R.T.: 0.001 min
Response: 4874912
Conc: 7.64 ng/ml

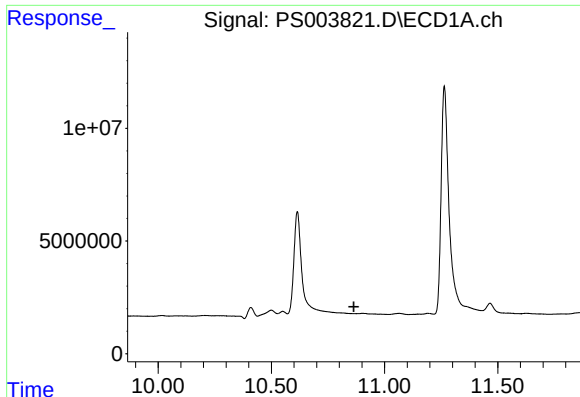

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

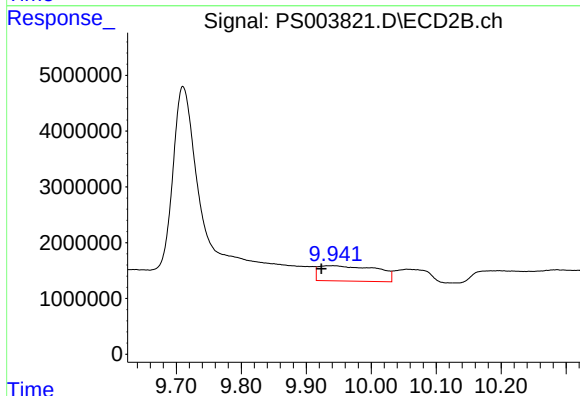


#3 4-Nitrophenol

R.T.: 9.938 min
Delta R.T.: 0.015 min
Response: 17033739
Conc: 75.03 ng/ml

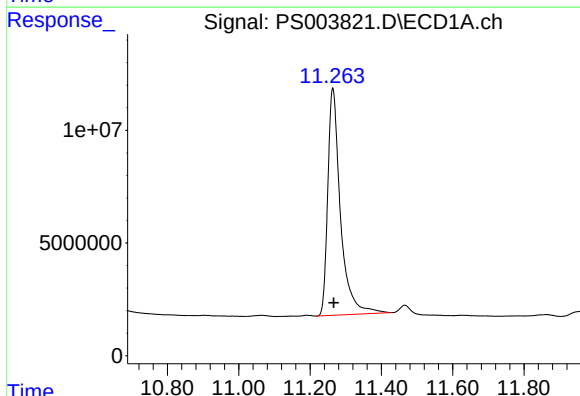


#4 2,4-DCAA

R.T.: 11.264 min
Delta R.T.: -0.003 min
Response: 248833873
Conc: 570.44 ng/ml

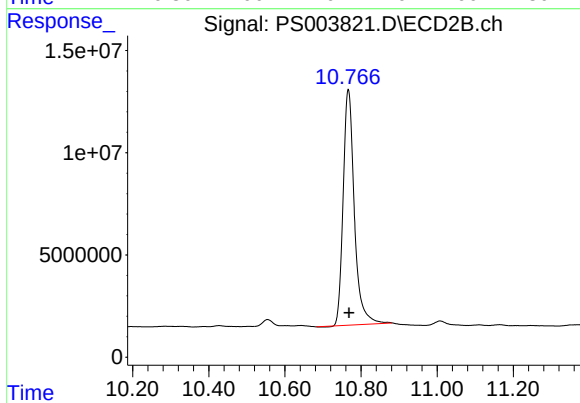

#4 2,4-DCAA


R.T.: 10.767 min
Delta R.T.: -0.002 min
Response: 234253615
Conc: 477.43 ng/ml

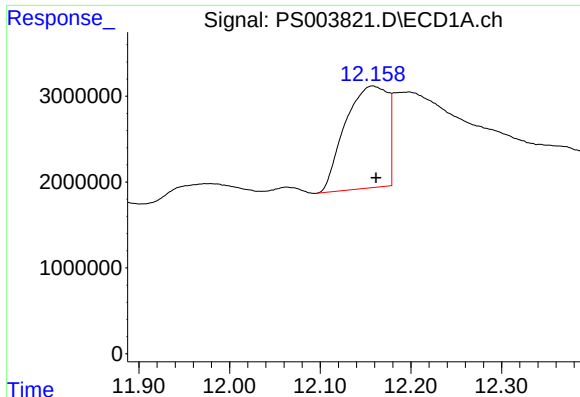

#7 MCPA


R.T.: 12.158 min
Delta R.T.: -0.004 min
Response: 38760199
Conc: 18.37 ug/ml

Instrument :
ECD_S
ClientSampleId :

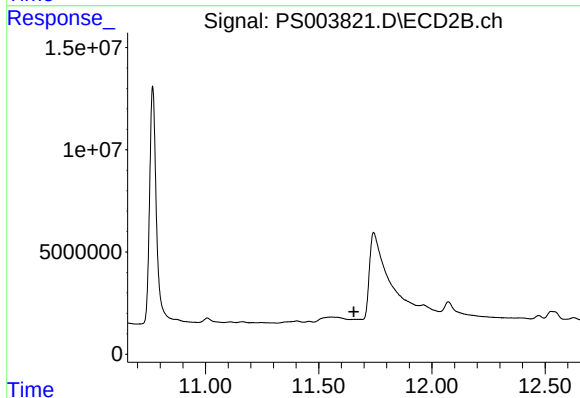


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.655 min
Response: 0
Conc: N.D.

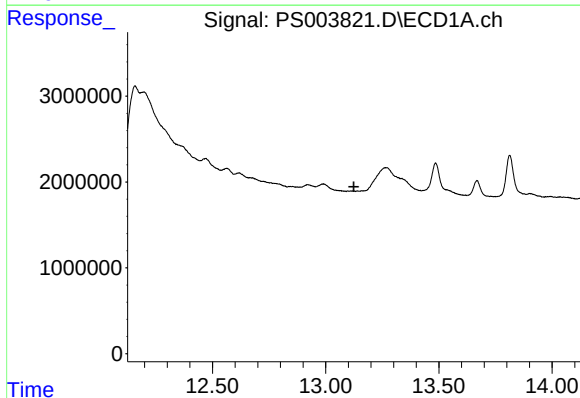


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.125 min
Response: 0
Conc: N.D.

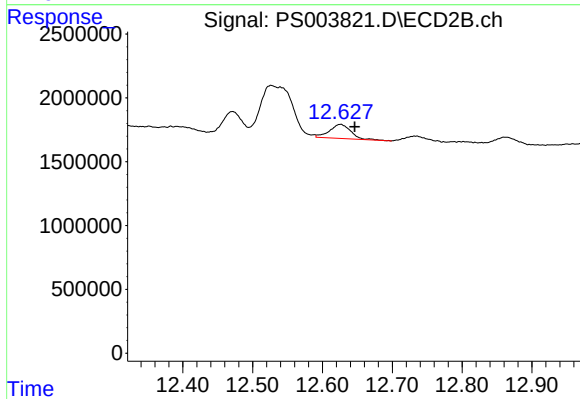

#9 2,4-D


R.T.: 12.626 min
Delta R.T.: -0.021 min
Response: 2342052
Conc: 4.40 ng/ml

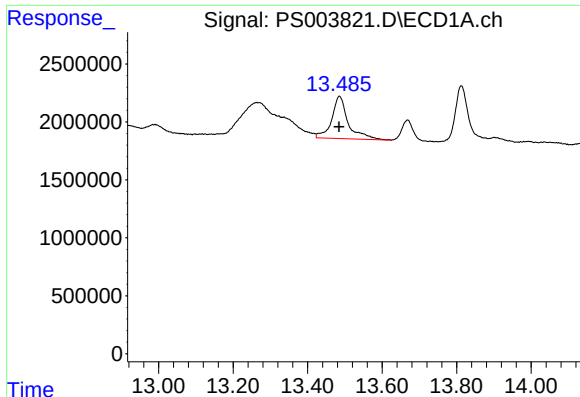

#10 Pentachlorophenol


R.T.: 13.485 min
Delta R.T.: 0.000 min
Response: 11252241
Conc: 1.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

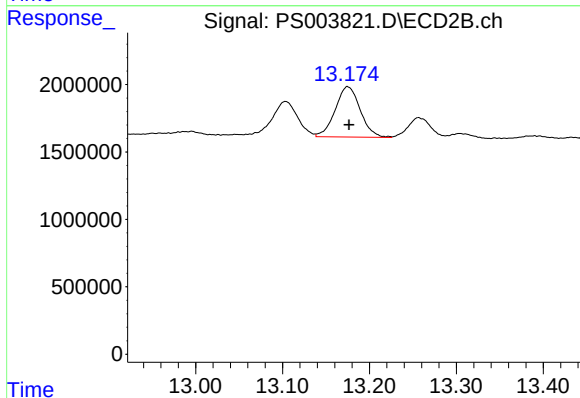


#10 Pentachlorophenol

R.T.: 13.175 min
Delta R.T.: -0.001 min
Response: 7472987
Conc: 1.08 ng/ml

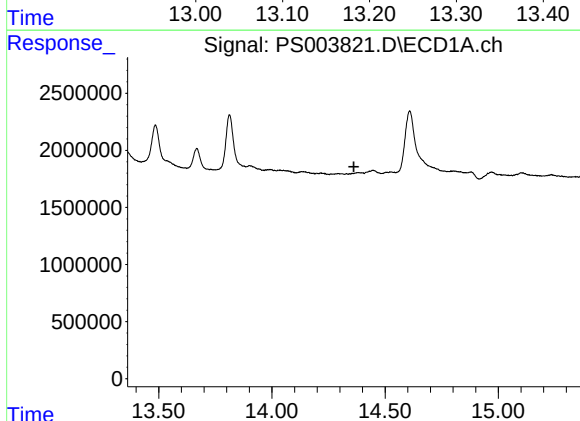


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.362 min
Response: 0
Conc: N.D.

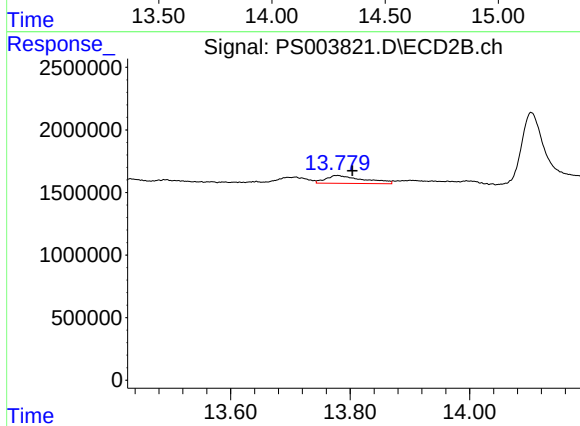

#11 2,4,5-TP (SILVEX)


R.T.: 13.779 min
Delta R.T.: -0.024 min
Response: 2737087
Conc: 1.03 ng/ml

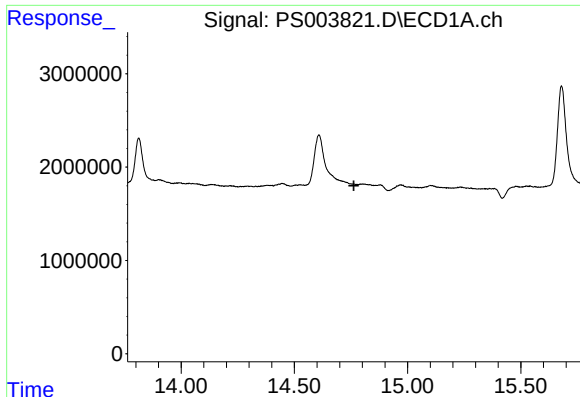

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.763 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

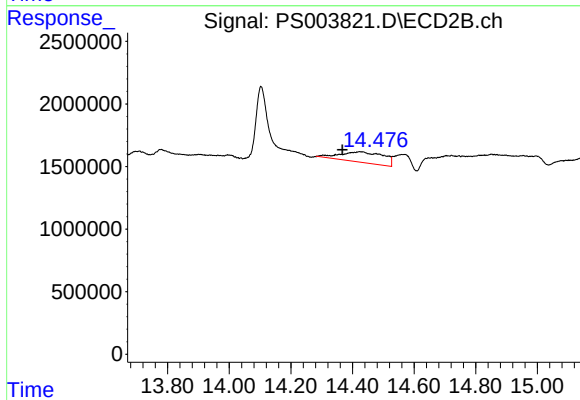


#12 2,4,5-T

R.T.: 14.425 min
Delta R.T.: 0.058 min
Response: 8187047
Conc: 3.77 ng/ml

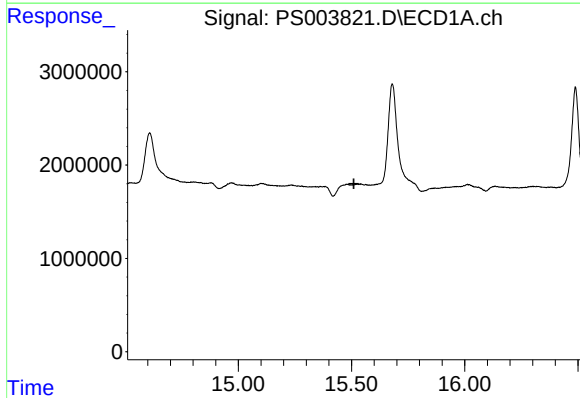


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

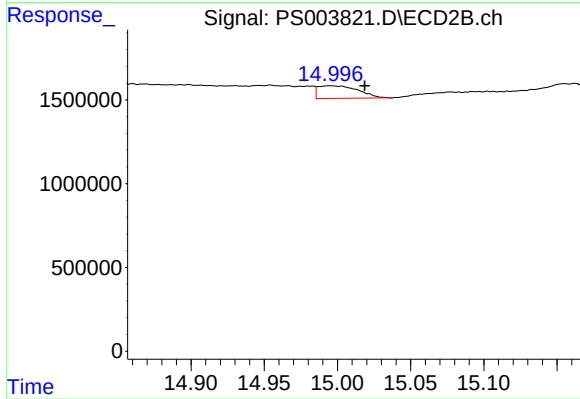

#13 2,4-DB


R.T.: 14.994 min
Delta R.T.: -0.025 min
Response: 1426467
Conc: 4.80 ng/ml

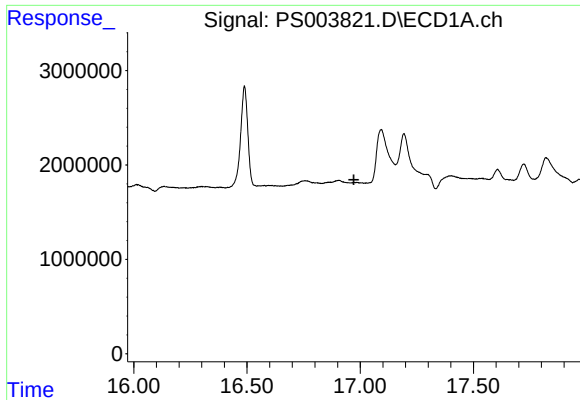

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.972 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

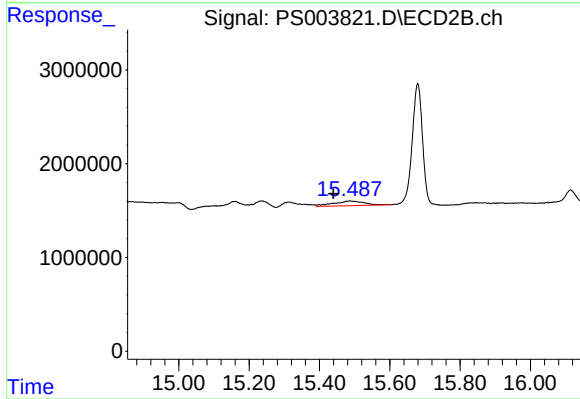


#14 DINOSEB

R.T.: 15.487 min
Delta R.T.: 0.047 min
Response: 3046235
Conc: 1.59 ng/ml

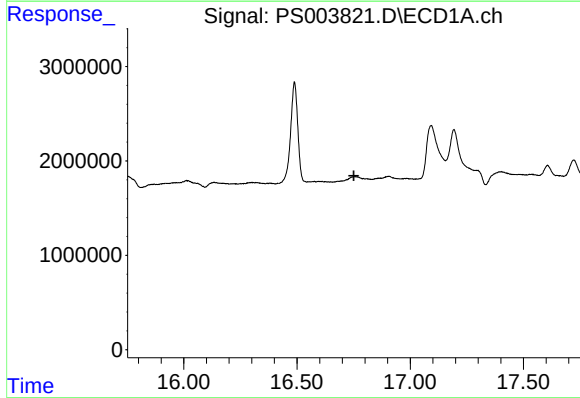


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.752 min
Response: 0
Conc: N.D.

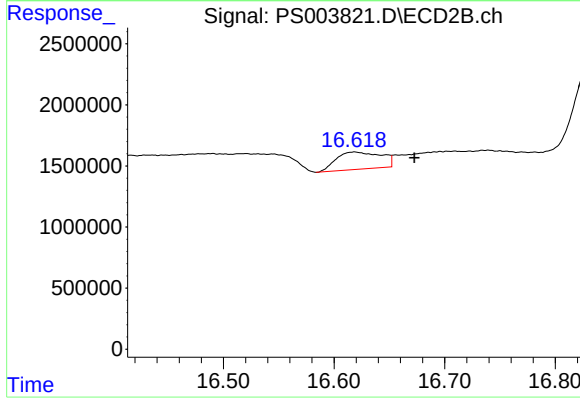

#15 Picloram


R.T.: 16.619 min
Delta R.T.: -0.053 min
Response: 3995755
Conc: 1.26 ng/ml

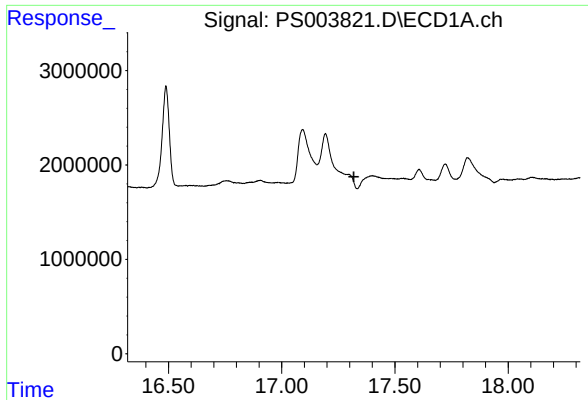

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

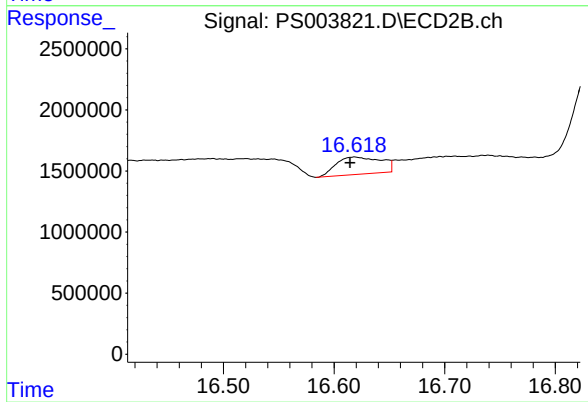

#16 DCPA

R.T.: 16.619 min
Delta R.T.: 0.005 min
Response: 3995755
Conc: 1.18 ng/ml