

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032822\
 Data File : PS018789.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2022 13:49
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 17:41:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.226	6.808	1395.3E6	372.2E6	490.288	528.978
Target Compounds							
6) T	MCP	7.670f	0.000	12153540	0	1.432	N.D. #
8) T	DICHLORPROP	0.000	7.543f	0	3947351	N.D.	4.986
9) T	2,4-D	8.416f	0.000	11727964	0	3.500	N.D. #
11) T	2,4,5-TP ...	9.265f	8.638f	13676544	3593416	<MDL	<MDL #
12) T	2,4,5-T	9.469	9.053	8559396	3260007	<MDL	<MDL #
13) T	2,4-DB	9.999f	0.000	2353947	0	<MDL	N.D. #
14) T	DINOSEB	11.256	0.000	11383342	0	1.065	N.D. #
15) T	Picloram	11.027	10.876	58433635	11988124	2.843	2.255
16) T	DCPA	11.481	10.876f	2643362	11988124	<MDL	2.279 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032822\
Data File : PS018789.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2022 13:49
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 17:41:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

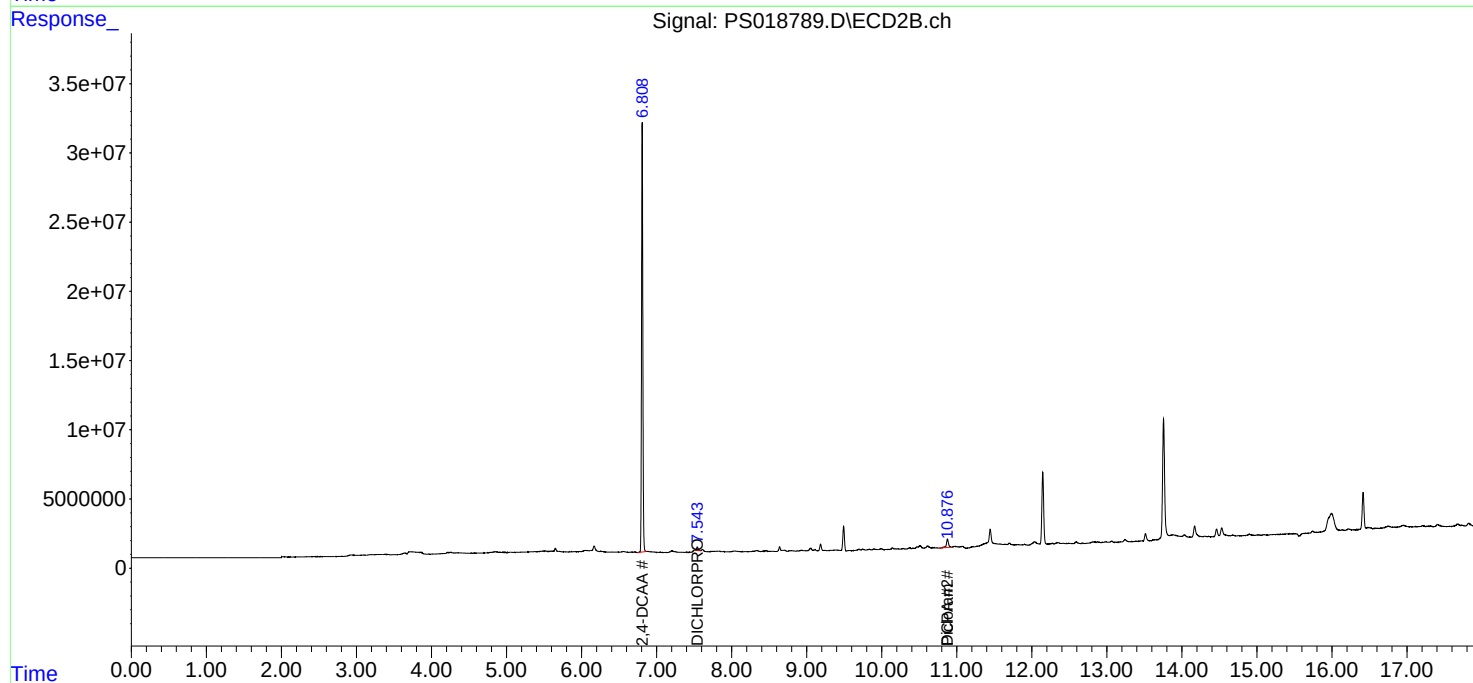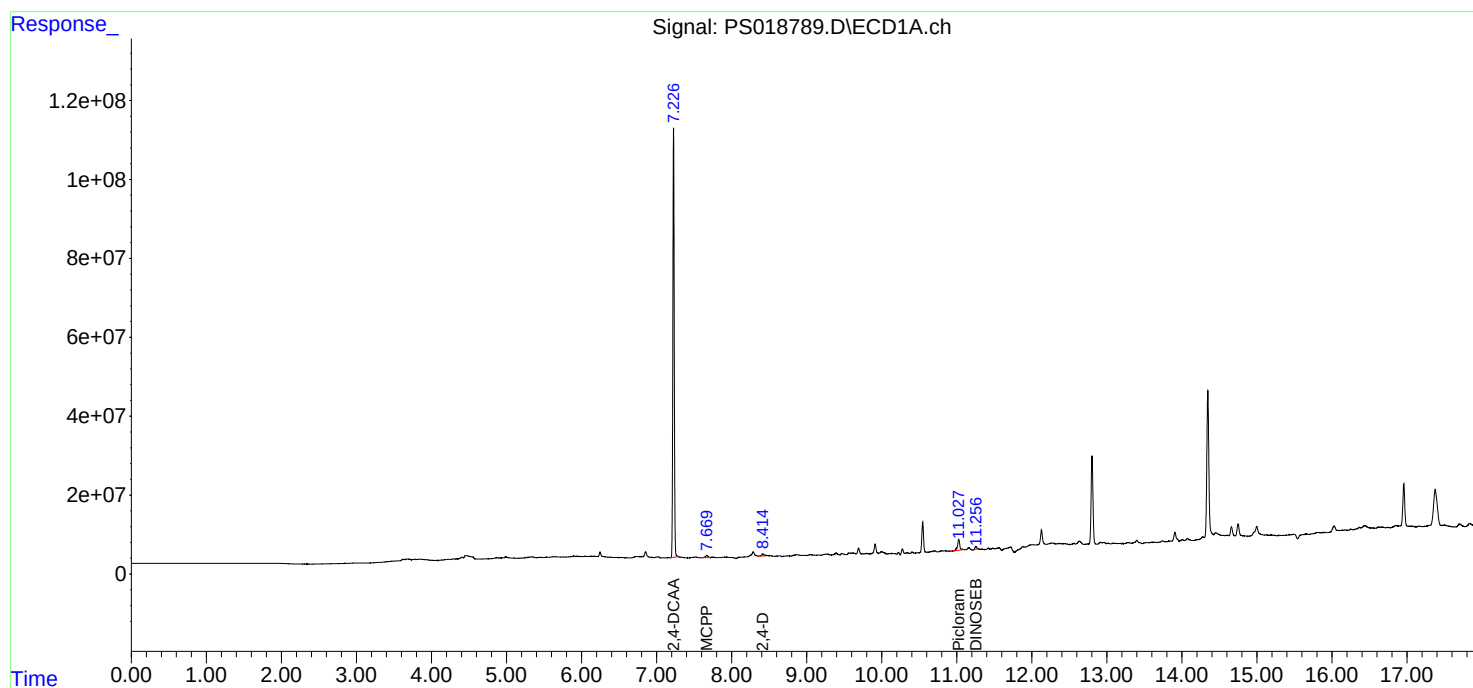


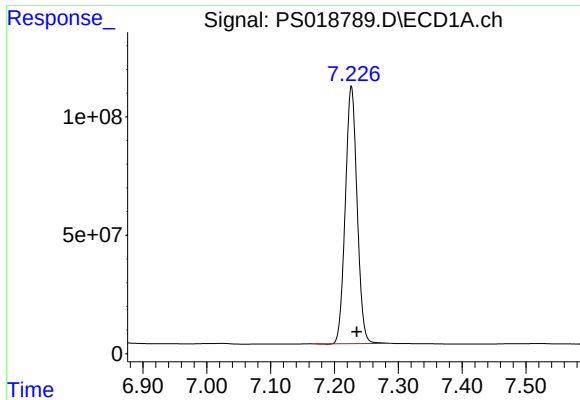

#4 2,4-DCAA


R.T.: 7.226 min
Delta R.T.: -0.009 min
Response: 1395318898
Conc: 490.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

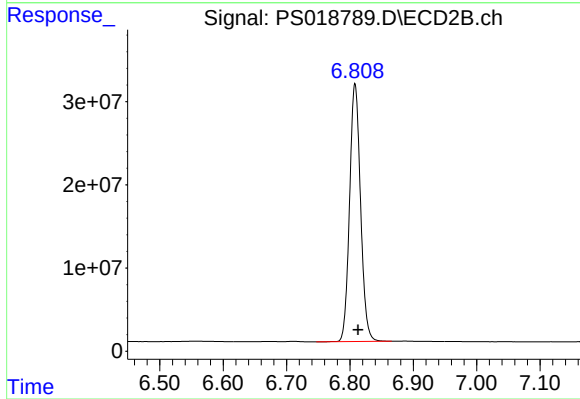


#4 2,4-DCAA

R.T.: 6.808 min
Delta R.T.: -0.005 min
Response: 372218062
Conc: 528.98 ng/ml

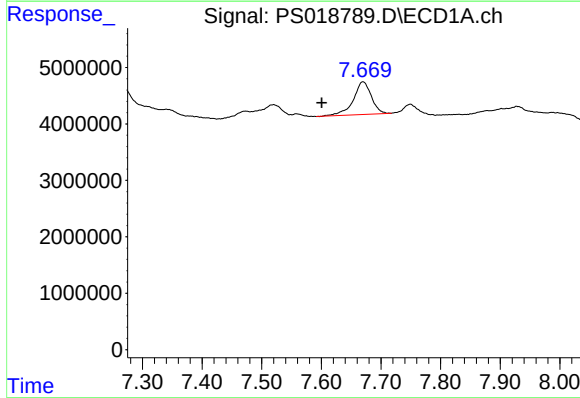


#6 MCP

R.T.: 7.670 min
Delta R.T.: 0.069 min
Response: 12153540
Conc: 1.43 ug/ml

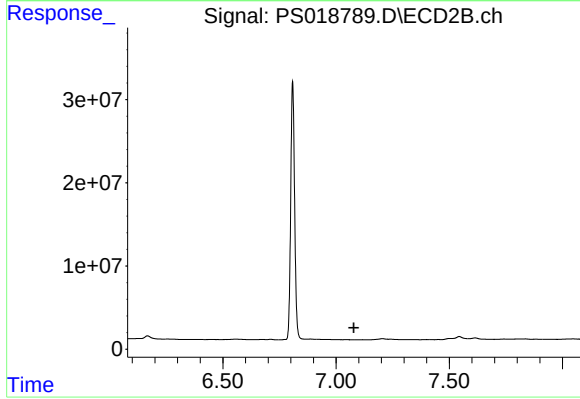

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.079 min
Response: 0
Conc: N.D.

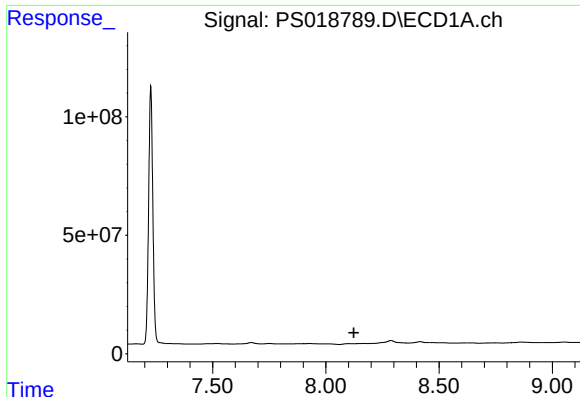

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.124 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

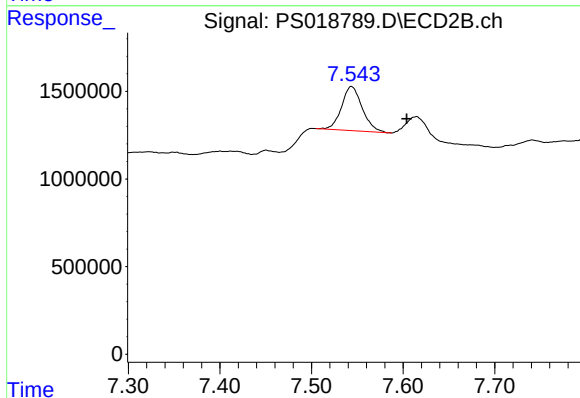


#8 DICHLORPROP

R.T.: 7.543 min
Delta R.T.: -0.061 min
Response: 3947351
Conc: 4.99 ng/ml

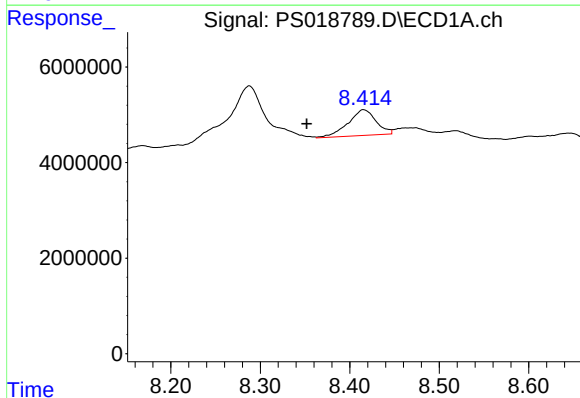


#9 2,4-D

R.T.: 8.416 min
Delta R.T.: 0.064 min
Response: 11727964
Conc: 3.50 ng/ml

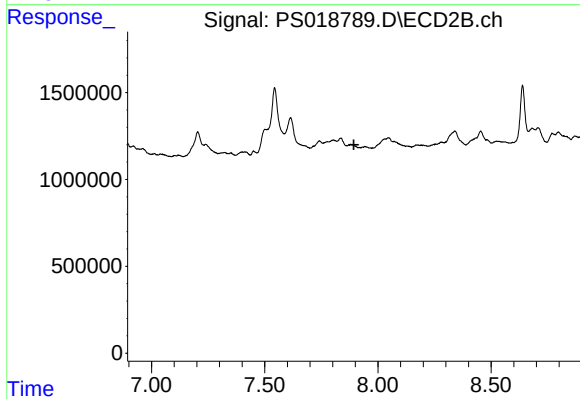

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.894 min
Response: 0
Conc: N.D.

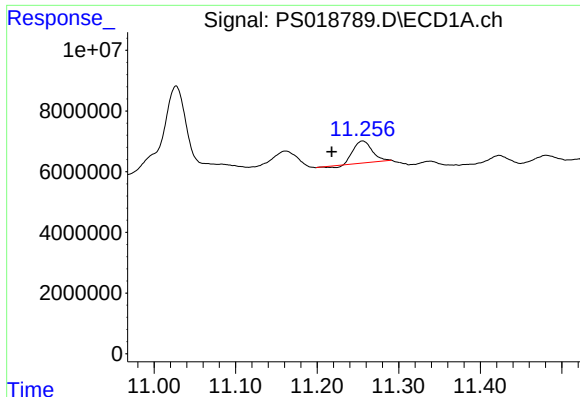

#14 DINOSEB


R.T.: 11.256 min
Delta R.T.: 0.038 min
Response: 11383342
Conc: 1.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

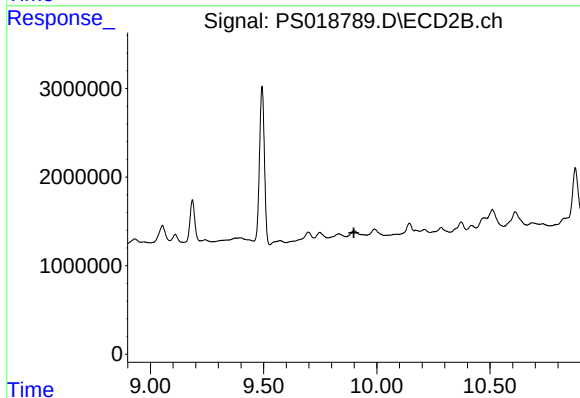


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.899 min
Response: 0
Conc: N.D.

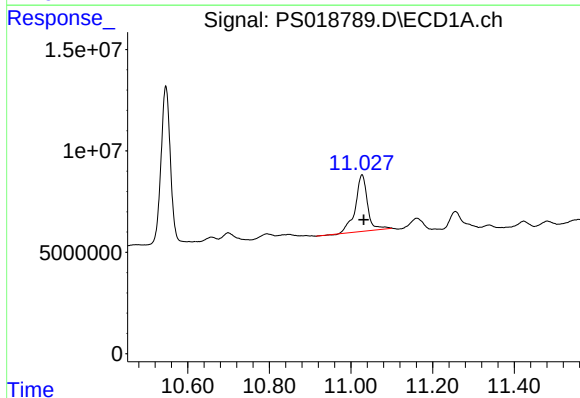


#15 Picloram

R.T.: 11.027 min
Delta R.T.: -0.004 min
Response: 58433635
Conc: 2.84 ng/ml

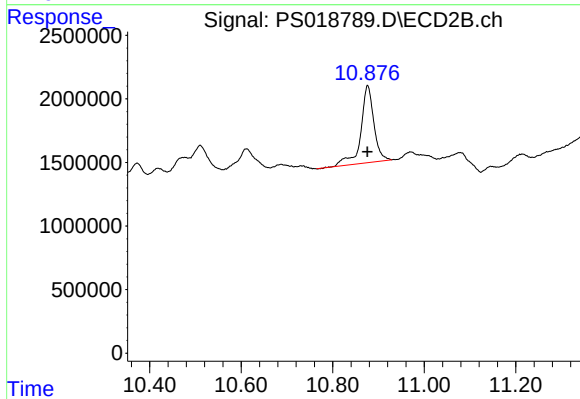

#15 Picloram


R.T.: 10.876 min
Delta R.T.: 0.000 min
Response: 11988124
Conc: 2.26 ng/ml

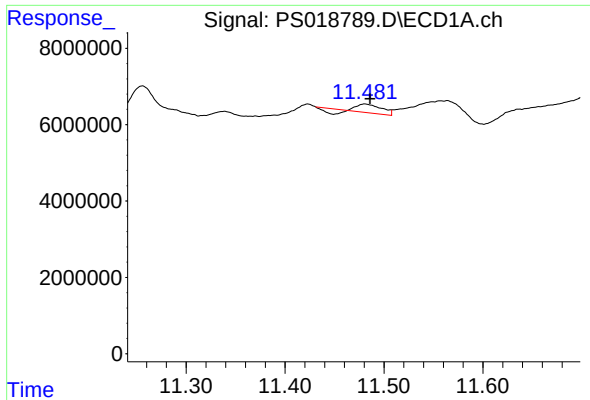

#16 DCPA

R.T.: 11.481 min
Delta R.T.: -0.005 min
Response: 2643362
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

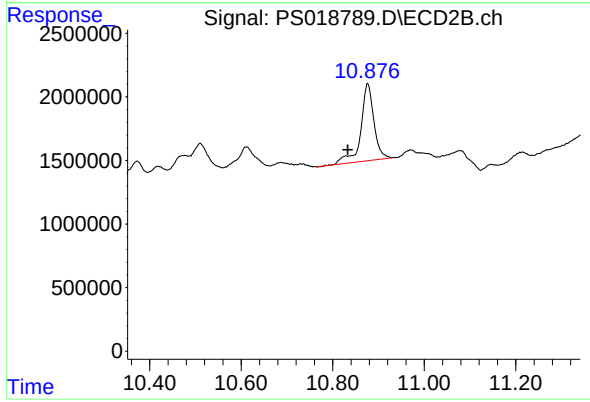

#16 DCPA

R.T.: 10.876 min
Delta R.T.: 0.043 min
Response: 11988124
Conc: 2.28 ng/ml