

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032822\
 Data File : PS018803.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2022 21:57
 Operator : AJ\MA
 Sample : N2125-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 01:12:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.226	6.810	1081.1E6	443.7E6	379.895	630.581 #
Target Compounds							
1) T	Dalapon	2.979f	2.496	297.9E6	431.7E6	76.605	522.288 #
2) T	3,5-DICHL...	0.000	5.961	0	3966307	N.D.	3.791
3) T	4-Nitroph...	7.062	6.407	26710834	91833187	15.501	226.037 #
5) T	DICAMBA	7.465	6.991	70654427	11343033	6.478	3.808 #
6) T	MCPD	7.640	7.108	712.4E6	9884339	83.921	4.038 #
7) T	MCPA	7.691f	7.334f	282.4E6	-7607750	23.353	N.D. #
8) T	DICHLORPROP	8.102	7.637	68965376	3680.7E6	25.038	4649.680 #
9) T	2,4-D	8.353	7.877	57946071	27931652	17.294	29.841 #
10) T	Pentachlo...	8.657	8.325	211.6E6	53397773	5.844	5.437
11) T	2,4,5-TP ...	9.272f	8.647f	7277.9E6	21218.2E6	478.549	4864.342 #
12) T	2,4,5-T	9.464	9.080	4364.6E6	1355.2E6	292.168	327.173
13) T	2,4-DB	10.037	9.555	3664.3E6	73389.5E6	1339.596	129264.084 #
14) T	DINOSEB	0.000	9.886	0	44168821	N.D.	14.416
15) T	Picloram	10.970f	10.824f	462.5E6	1120.0E6	22.502	210.677 #
16) T	DCPA	11.484	10.824	533.7E6	1120.0E6	29.833	212.953 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032822\
Data File : PS018803.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2022 21:57
Operator : AJ\MA
Sample : N2125-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 01:12:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

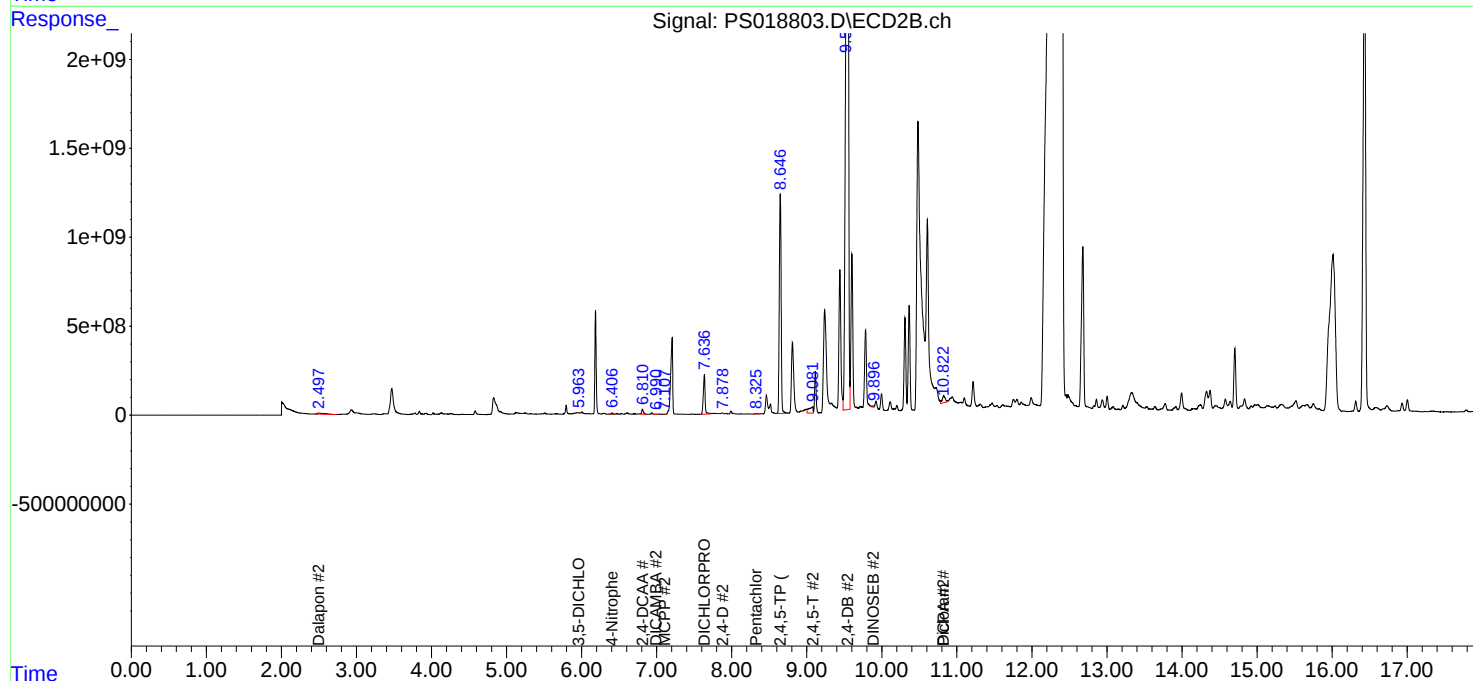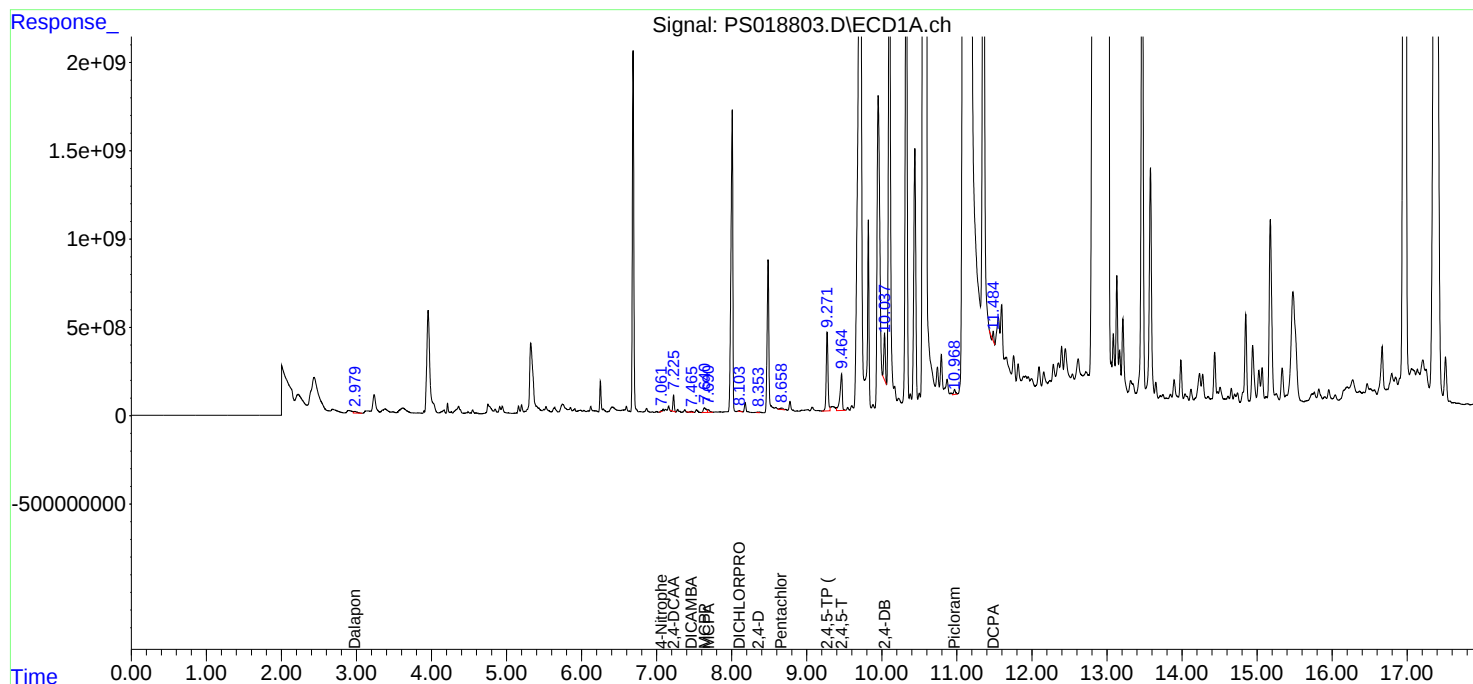


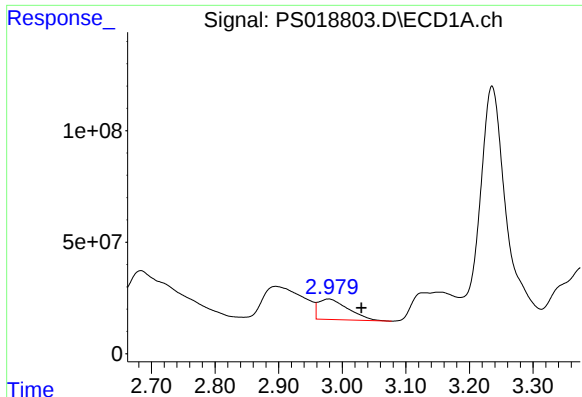

#1 Dalapon


R.T.: 2.979 min
Delta R.T.: -0.051 min
Response: 297876101
Conc: 76.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

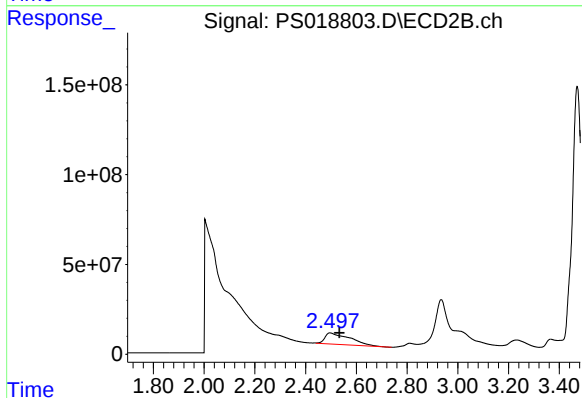


#1 Dalapon

R.T.: 2.496 min
Delta R.T.: -0.037 min
Response: 431653656
Conc: 522.29 ng/ml

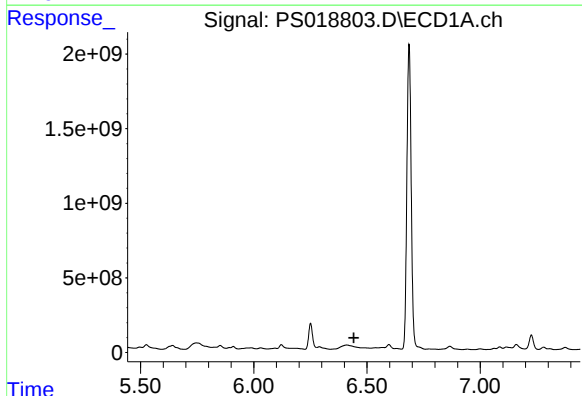


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.442 min
Response: 0
Conc: N.D.

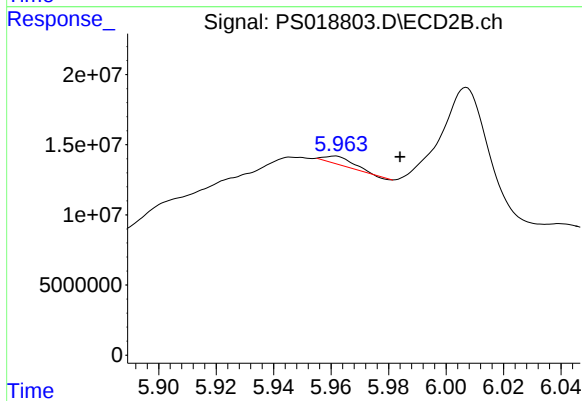

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.961 min
Delta R.T.: -0.023 min
Response: 3966307
Conc: 3.79 ng/ml

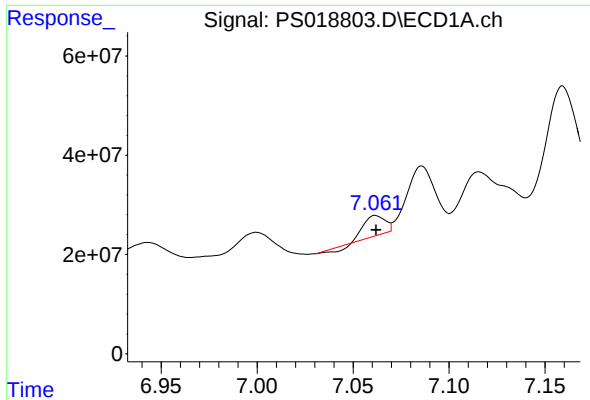

#3 4-Nitrophenol


R.T.: 7.062 min
Delta R.T.: 0.000 min
Response: 26710834
Conc: 15.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

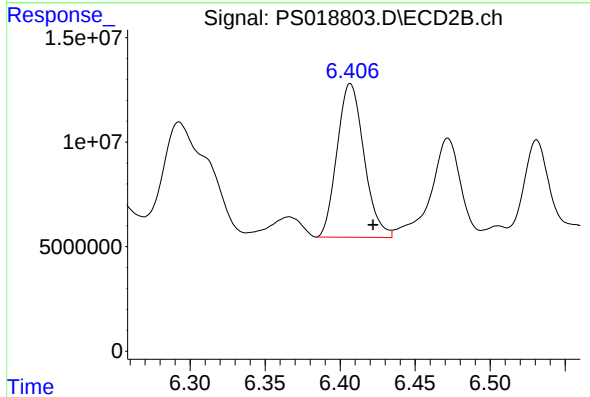


#3 4-Nitrophenol

R.T.: 6.407 min
Delta R.T.: -0.015 min
Response: 91833187
Conc: 226.04 ng/ml

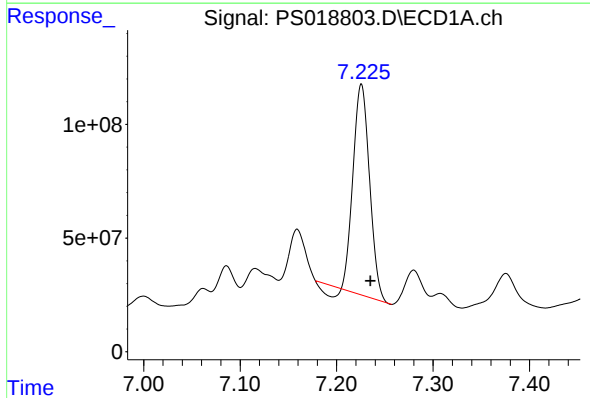


#4 2,4-DCAA

R.T.: 7.226 min
Delta R.T.: -0.009 min
Response: 1081149636
Conc: 379.90 ng/ml

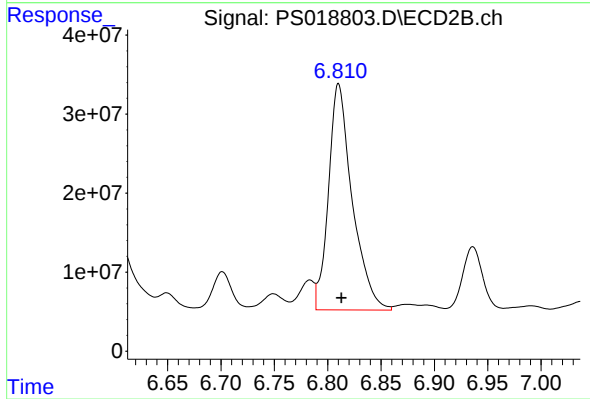

#4 2,4-DCAA


R.T.: 6.810 min
Delta R.T.: -0.003 min
Response: 443711751
Conc: 630.58 ng/ml

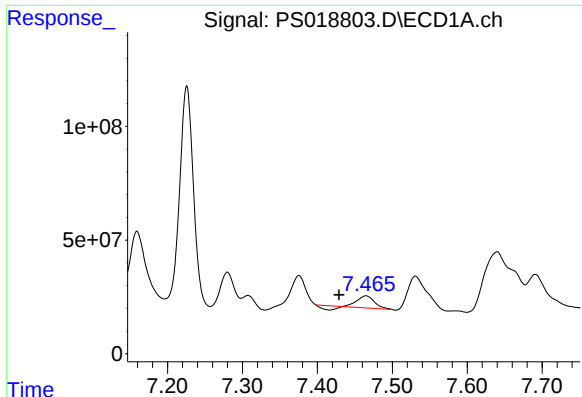

#5 DICAMBA


R.T.: 7.465 min
Delta R.T.: 0.036 min
Response: 70654427
Conc: 6.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

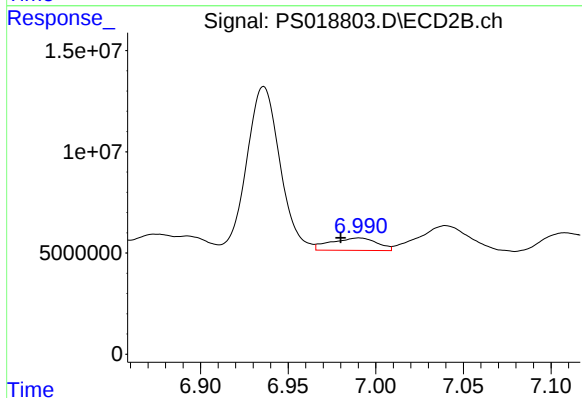


#5 DICAMBA

R.T.: 6.991 min
Delta R.T.: 0.011 min
Response: 11343033
Conc: 3.81 ng/ml

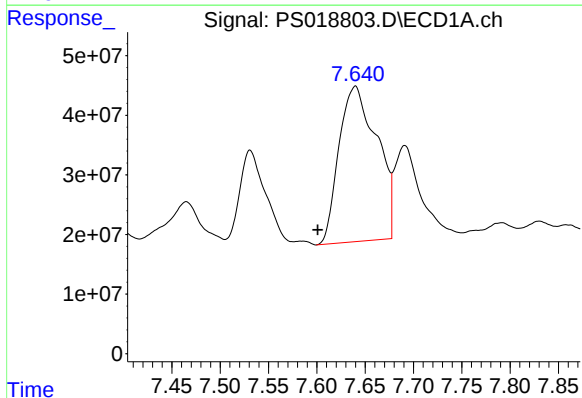


#6 MCP

R.T.: 7.640 min
Delta R.T.: 0.039 min
Response: 712359787
Conc: 83.92 ug/ml

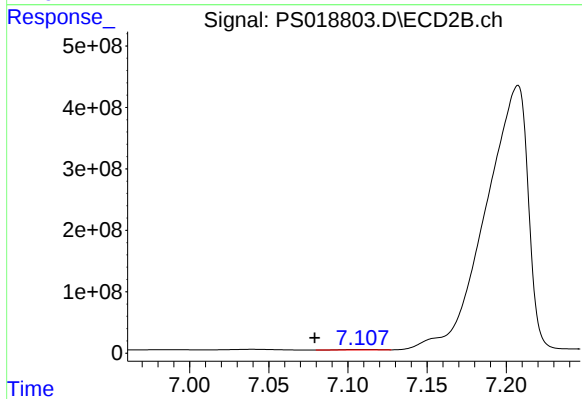

#6 MCP


R.T.: 7.108 min
Delta R.T.: 0.029 min
Response: 9884339
Conc: 4.04 ug/ml

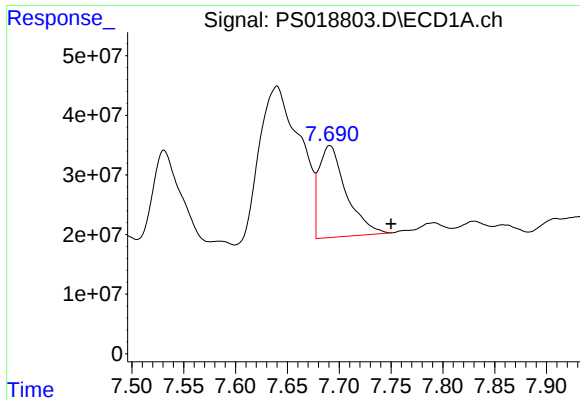

#7 MCPA


R.T.: 7.691 min
Delta R.T.: -0.059 min
Response: 282442097
Conc: 23.35 ug/ml

Instrument :
ECD_S
ClientSampleId :

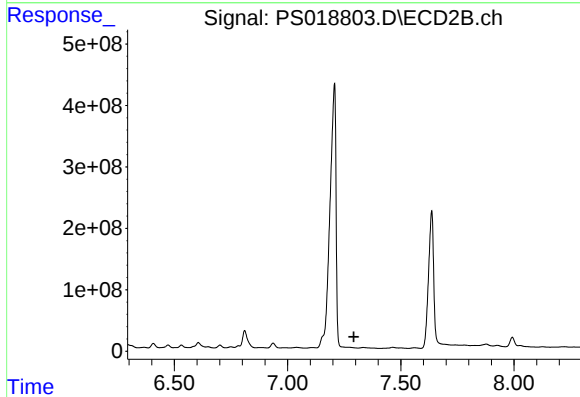


#7 MCPA

R.T.: 7.334 min
Delta R.T.: 0.041 min
Response: -7607750
Conc: N.D.

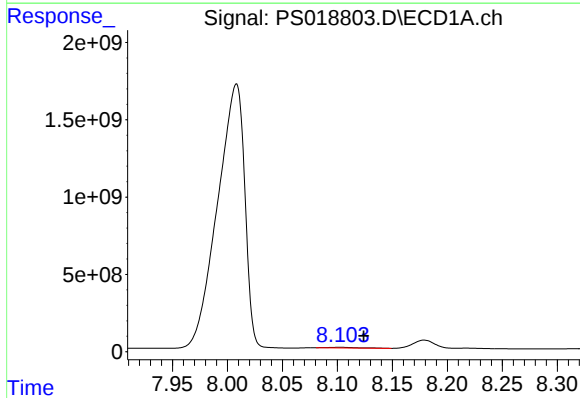


#8 DICHLORPROP

R.T.: 8.102 min
Delta R.T.: -0.022 min
Response: 68965376
Conc: 25.04 ng/ml

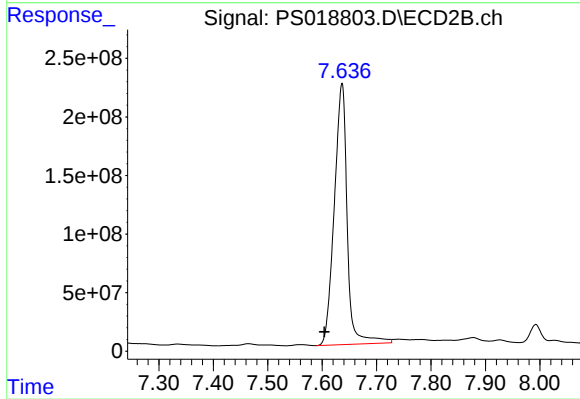

#8 DICHLORPROP


R.T.: 7.637 min
Delta R.T.: 0.033 min
Response: 3680746431
Conc: 4649.68 ng/ml

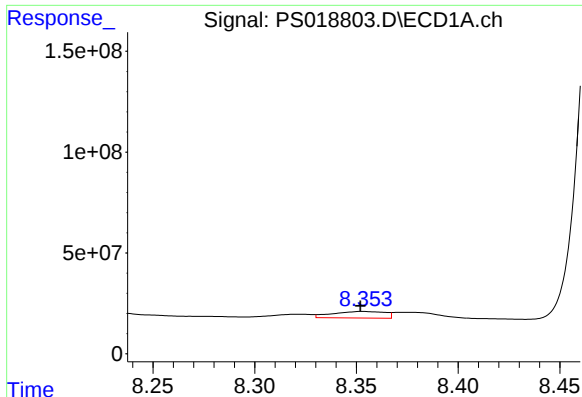

#9 2,4-D


R.T.: 8.353 min
Delta R.T.: 0.000 min
Response: 57946071
Conc: 17.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

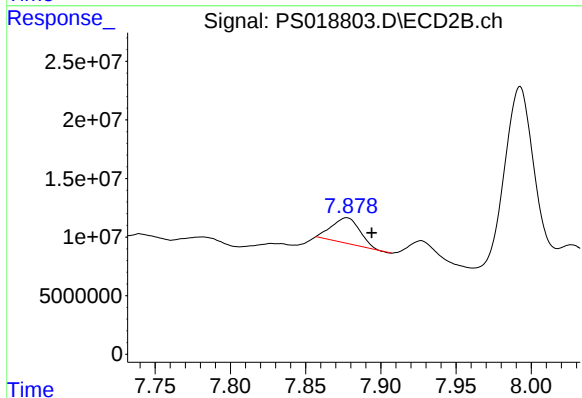


#9 2,4-D

R.T.: 7.877 min
Delta R.T.: -0.017 min
Response: 27931652
Conc: 29.84 ng/ml

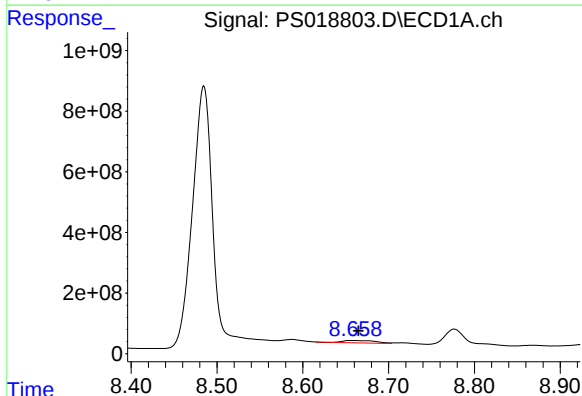


#10 Pentachlorophenol

R.T.: 8.657 min
Delta R.T.: -0.008 min
Response: 211581109
Conc: 5.84 ng/ml

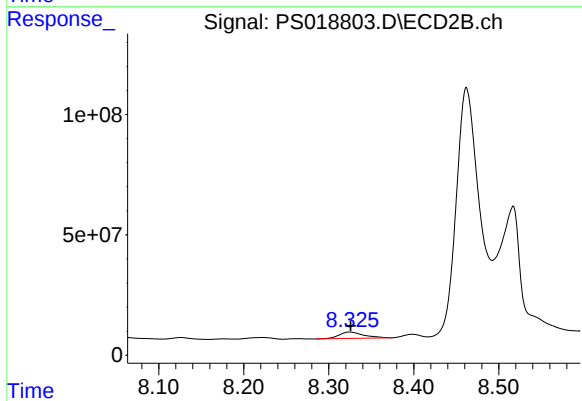

#10 Pentachlorophenol


R.T.: 8.325 min
Delta R.T.: -0.001 min
Response: 53397773
Conc: 5.44 ng/ml

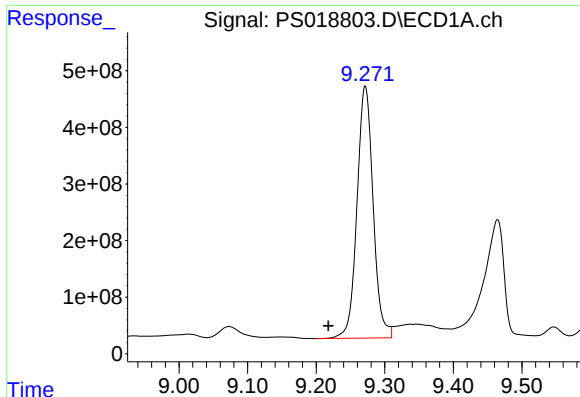

#11 2,4,5-TP (SILVEX)


R.T.: 9.272 min
Delta R.T.: 0.054 min
Response: 7277861221
Conc: 478.55 ng/ml

Instrument :
ECD_S
ClientSampleId :

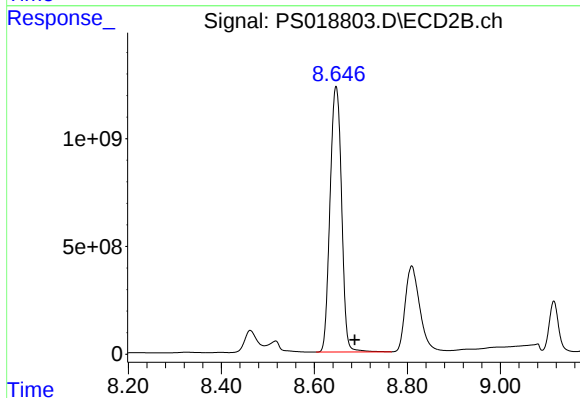


#11 2,4,5-TP (SILVEX)

R.T.: 8.647 min
Delta R.T.: -0.040 min
Response: 21218248395
Conc: 4864.34 ng/ml

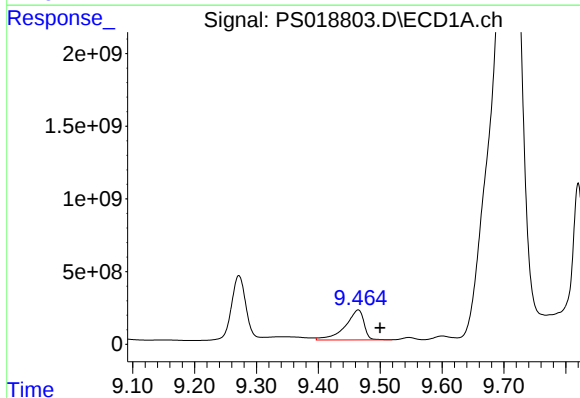


#12 2,4,5-T

R.T.: 9.464 min
Delta R.T.: -0.036 min
Response: 4364623482
Conc: 292.17 ng/ml

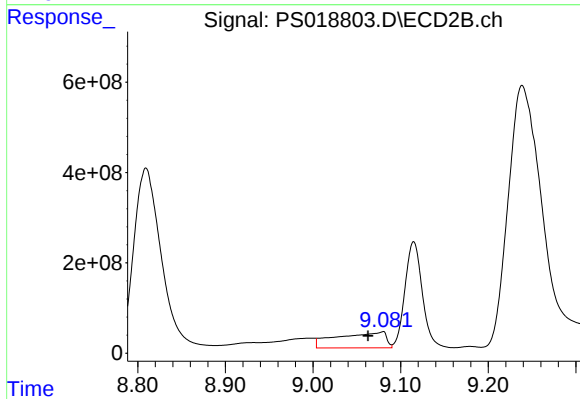

#12 2,4,5-T


R.T.: 9.080 min
Delta R.T.: 0.017 min
Response: 1355210861
Conc: 327.17 ng/ml

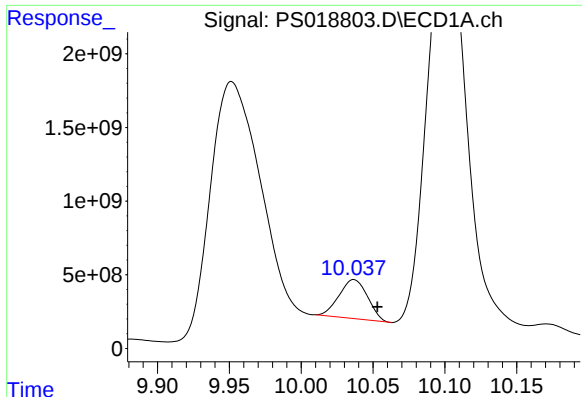

#13 2,4-DB


R.T.: 10.037 min
Delta R.T.: -0.016 min
Response: 3664342804
Conc: 1339.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

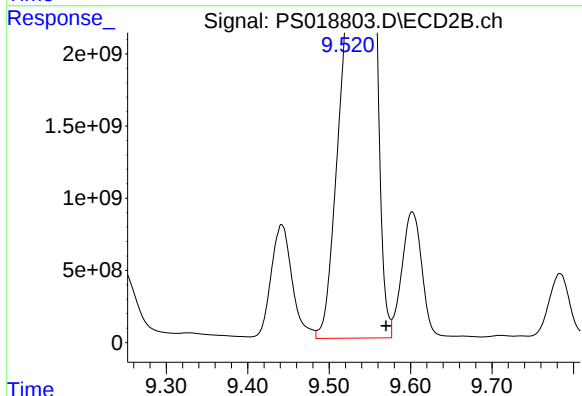


#13 2,4-DB

R.T.: 9.555 min
Delta R.T.: -0.015 min
Response: 73389472314
Conc: 129264.08 ng/ml

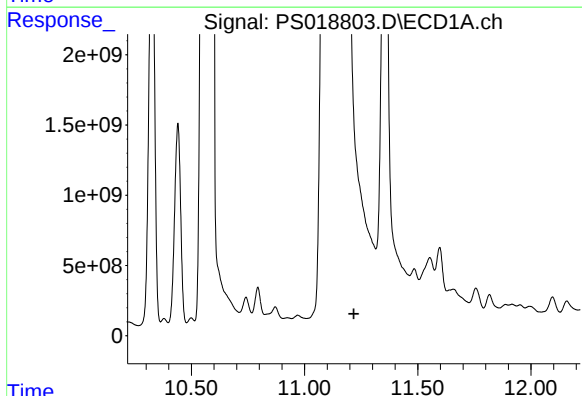


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.218 min
Response: 0
Conc: N.D.

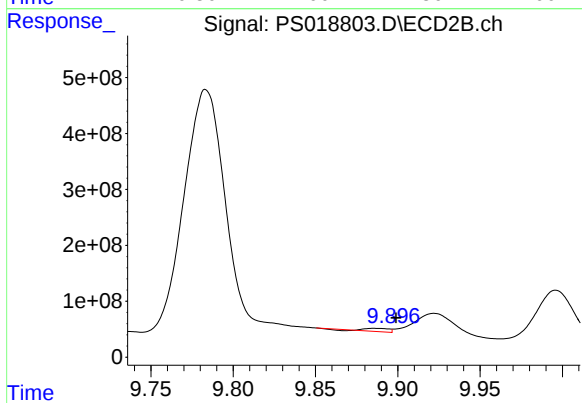

#14 DINOSEB


R.T.: 9.886 min
Delta R.T.: -0.013 min
Response: 44168821
Conc: 14.42 ng/ml

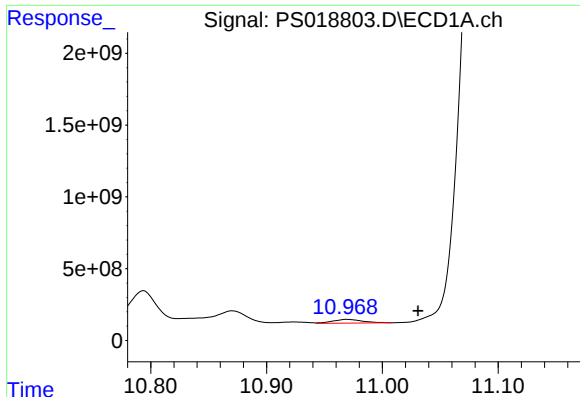

#15 Picloram


R.T.: 10.970 min
Delta R.T.: -0.061 min
Response: 462547465
Conc: 22.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

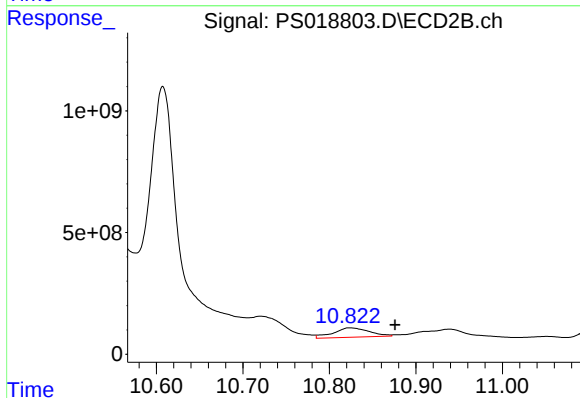


#15 Picloram

R.T.: 10.824 min
Delta R.T.: -0.052 min
Response: 1119980321
Conc: 210.68 ng/ml

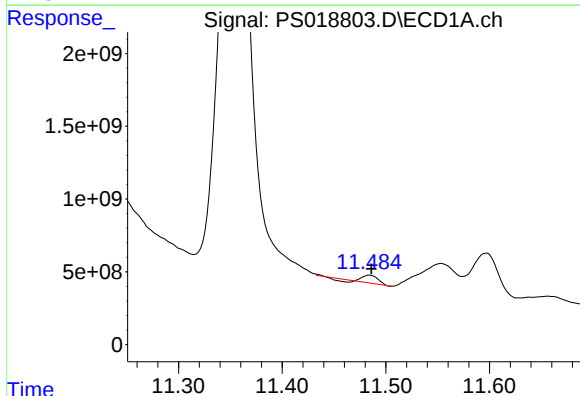

#16 DCPA

R.T.: 11.484 min
Delta R.T.: -0.002 min
Response: 533728369
Conc: 29.83 ng/ml

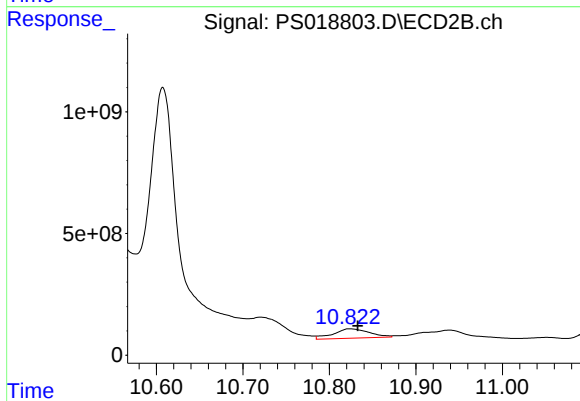

#16 DCPA

R.T.: 10.824 min
Delta R.T.: -0.009 min
Response: 1119980321
Conc: 212.95 ng/ml