

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032822\
 Data File : PS018806.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2022 23:09
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 01:13:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.226	6.809	1421.7E6	372.4E6	499.571	529.295
Target Compounds							
6) T	MCP	7.669f	7.130f	14771412	598722	1.740	<MDL #
7) T	MCPA	7.772	0.000	1924723	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.620	0	10979162	N.D.	13.869
11) T	2,4,5-TP ...	9.267f	8.712	59197316	3978195	3.892	<MDL #
12) T	2,4,5-T	9.480	9.066	30592363	2868579	2.048	<MDL #
13) T	2,4-DB	10.084	0.000	4539638	0	1.660	N.D. #
14) T	DINOSEB	11.165f	9.832f	62282325	448571	5.825	<MDL #
15) T	Picloram	11.026	10.878	44193293	12144085	2.150	2.284
16) T	DCPA	0.000	10.828	0	5708384	N.D.	1.085


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032822\
Data File : PS018806.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2022 23:09
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 01:13:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

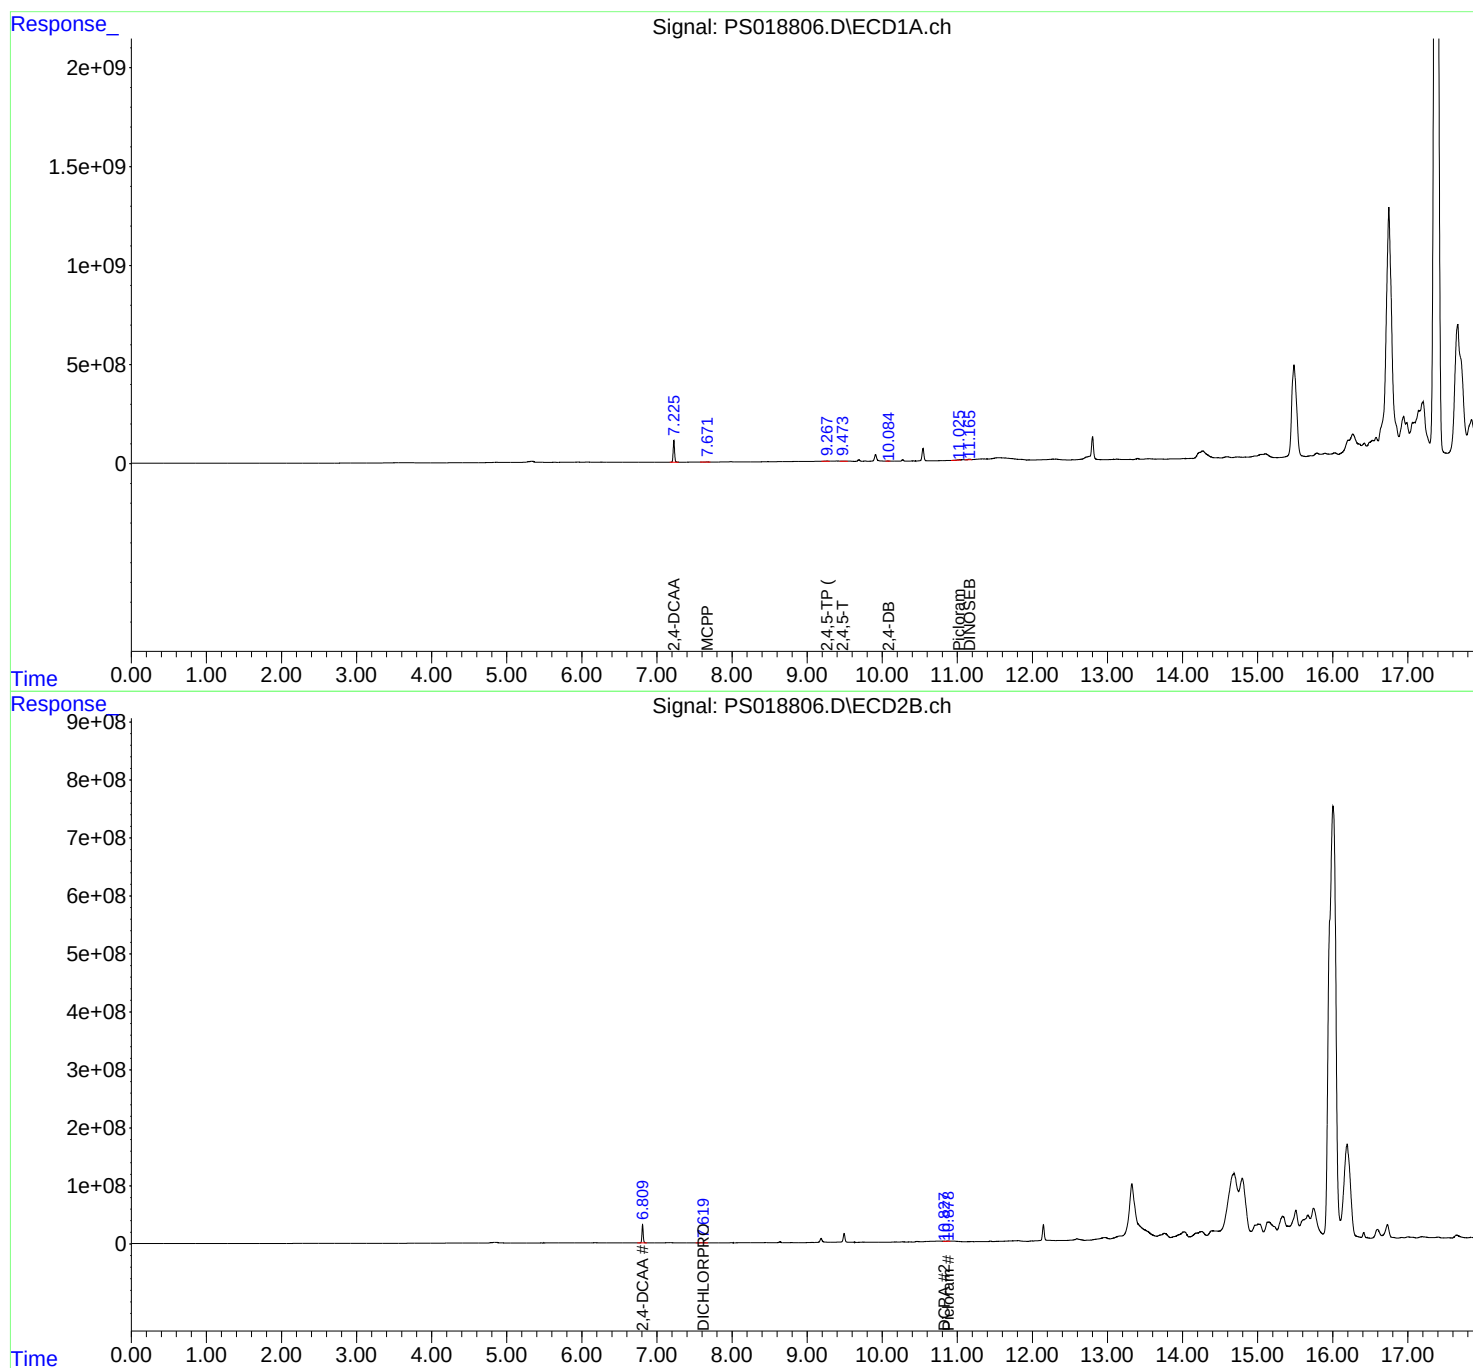


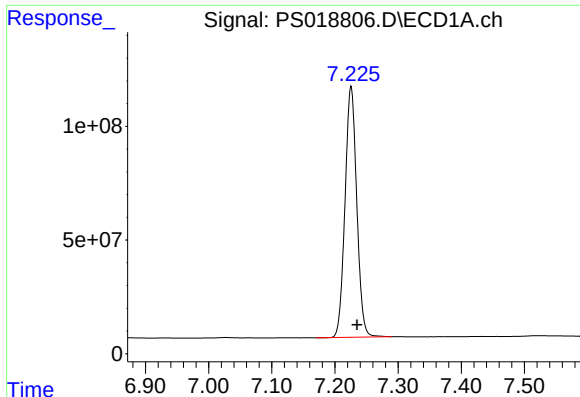

#4 2,4-DCAA


R.T.: 7.226 min
Delta R.T.: -0.009 min
Response: 1421737414
Conc: 499.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

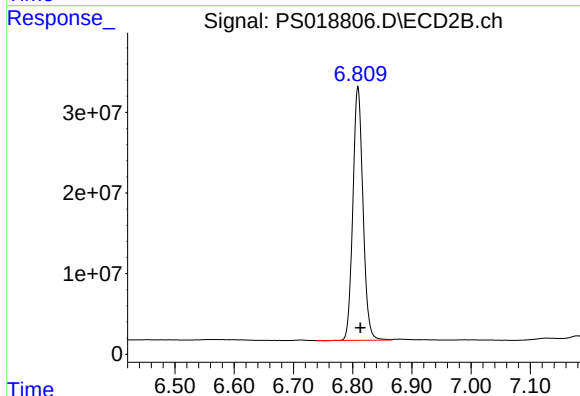


#4 2,4-DCAA

R.T.: 6.809 min
Delta R.T.: -0.004 min
Response: 372440860
Conc: 529.29 ng/ml

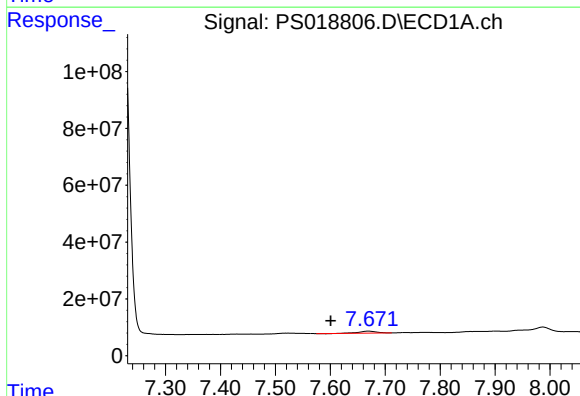


#6 MCP

R.T.: 7.669 min
Delta R.T.: 0.068 min
Response: 14771412
Conc: 1.74 ug/ml

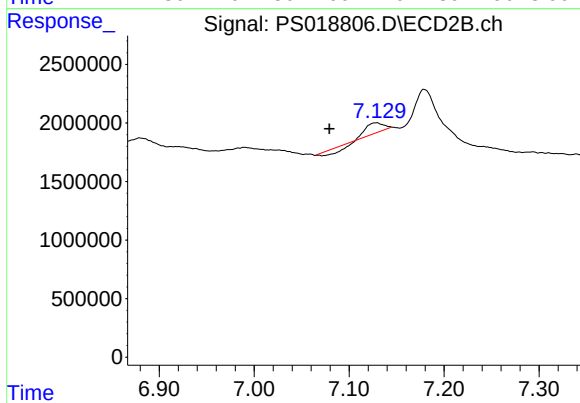

#6 MCP


R.T.: 7.130 min
Delta R.T.: 0.051 min
Response: 598722
Conc: N.D.

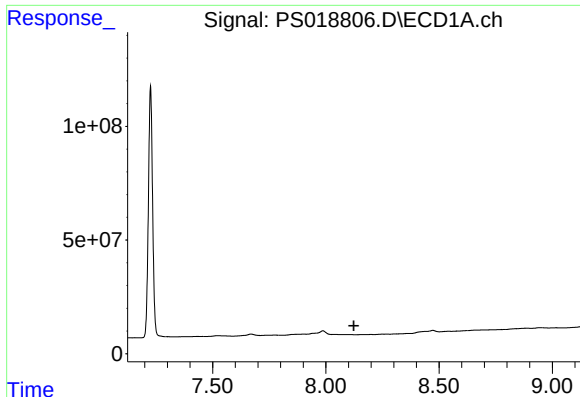

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.124 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

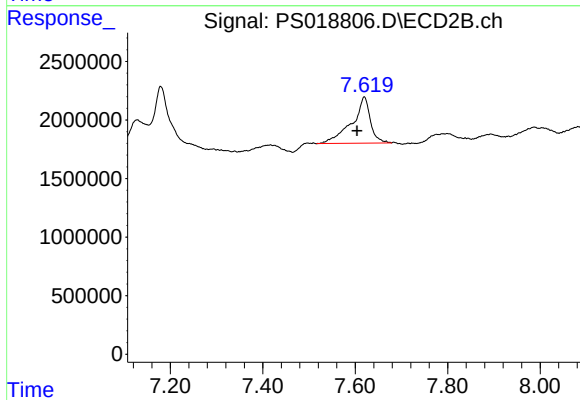


#8 DICHLORPROP

R.T.: 7.620 min
Delta R.T.: 0.016 min
Response: 10979162
Conc: 13.87 ng/ml

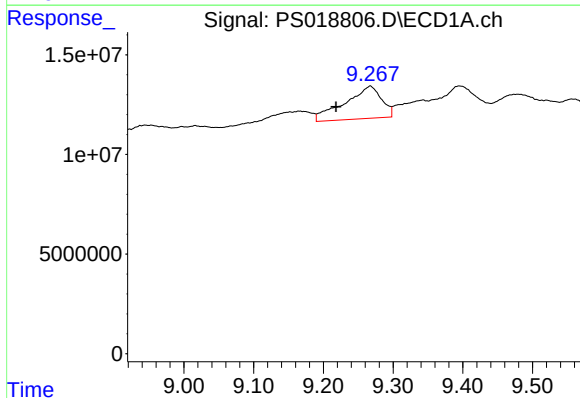


#11 2,4,5-TP (SILVEX)

R.T.: 9.267 min
Delta R.T.: 0.049 min
Response: 59197316
Conc: 3.89 ng/ml

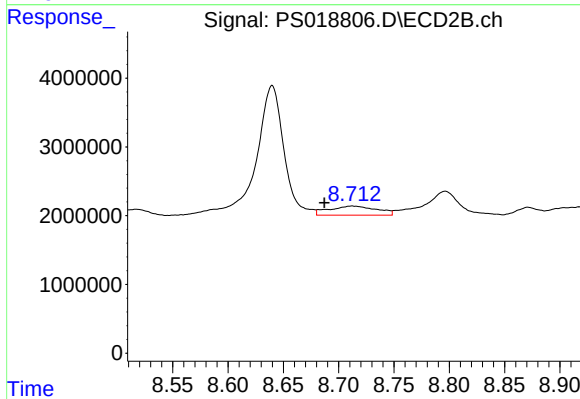

#11 2,4,5-TP (SILVEX)


R.T.: 8.712 min
Delta R.T.: 0.025 min
Response: 3978195
Conc: N.D.

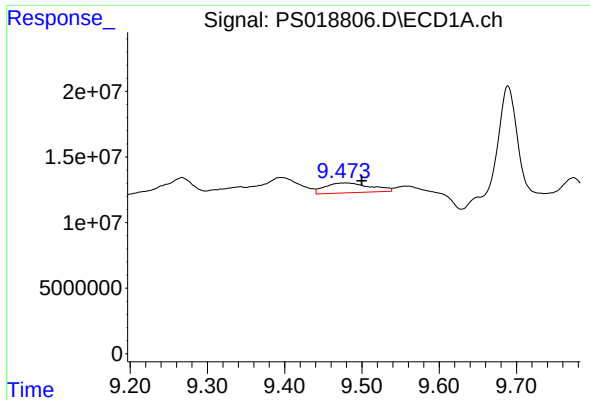

#12 2,4,5-T


R.T.: 9.480 min
Delta R.T.: -0.020 min
Response: 30592363
Conc: 2.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

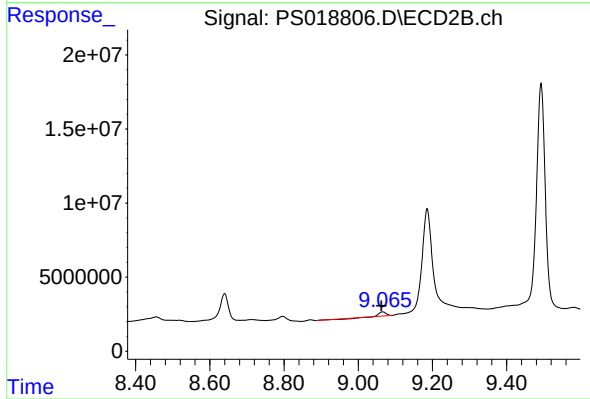


#12 2,4,5-T

R.T.: 9.066 min
Delta R.T.: 0.003 min
Response: 2868579
Conc: N.D.

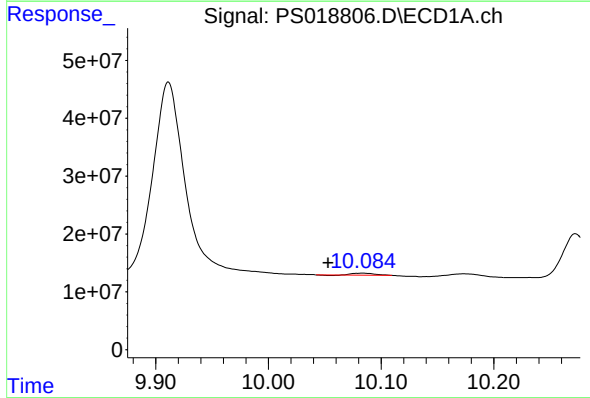


#13 2,4-DB

R.T.: 10.084 min
Delta R.T.: 0.031 min
Response: 4539638
Conc: 1.66 ng/ml

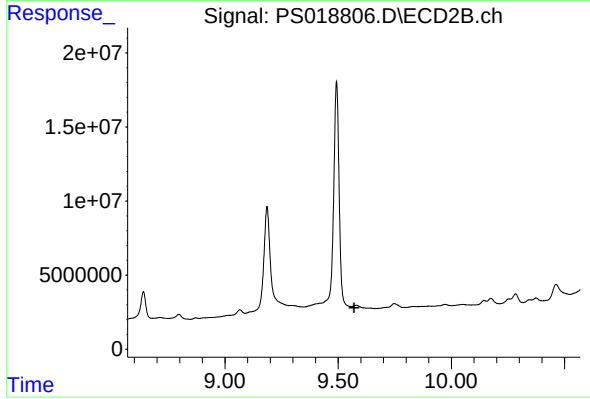

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.570 min
Response: 0
Conc: N.D.

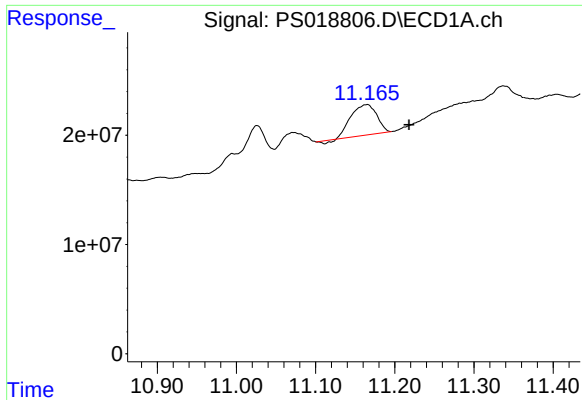

#14 DINOSEB


R.T.: 11.165 min
Delta R.T.: -0.053 min
Response: 62282325
Conc: 5.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

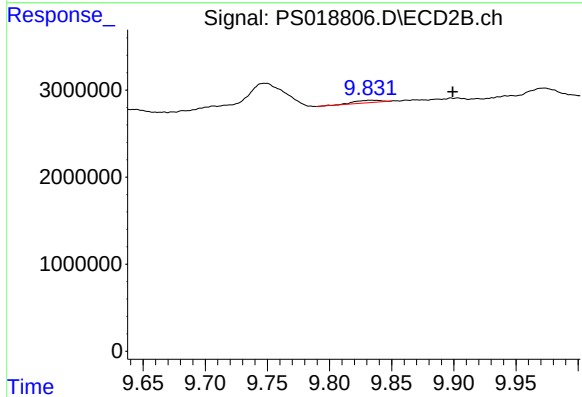


#14 DINOSEB

R.T.: 9.832 min
Delta R.T.: -0.067 min
Response: 448571
Conc: N.D.

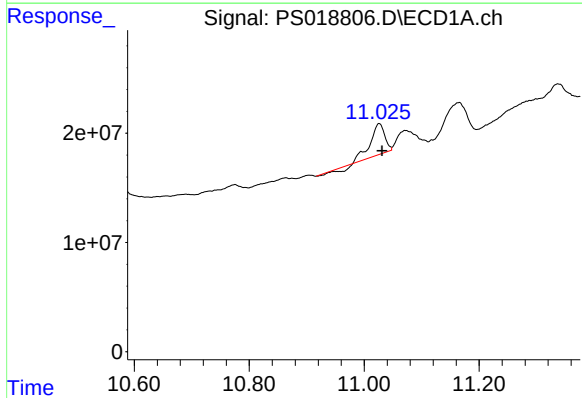


#15 Picloram

R.T.: 11.026 min
Delta R.T.: -0.005 min
Response: 44193293
Conc: 2.15 ng/ml

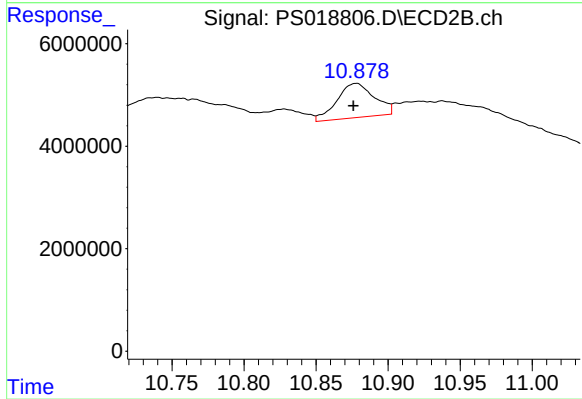

#15 Picloram


R.T.: 10.878 min
Delta R.T.: 0.002 min
Response: 12144085
Conc: 2.28 ng/ml

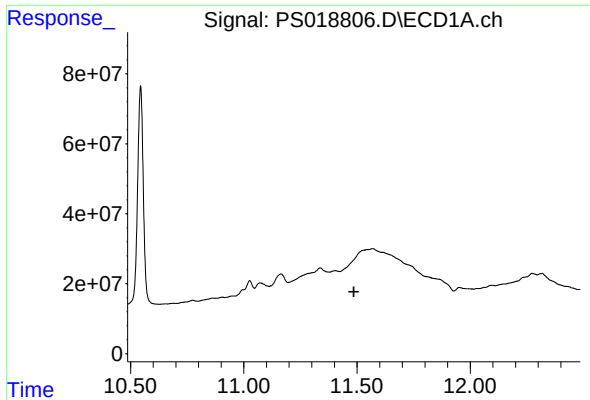

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.486 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

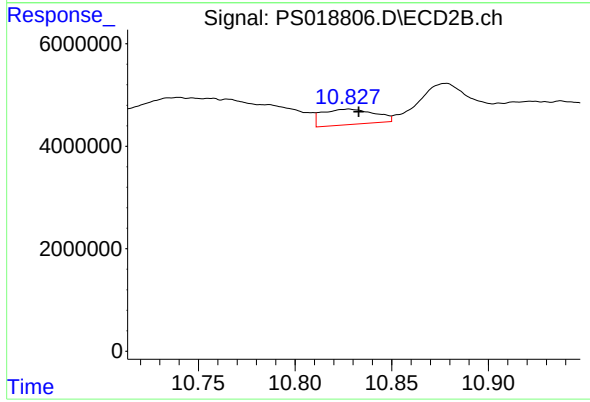

#16 DCPA

R.T.: 10.828 min
Delta R.T.: -0.005 min
Response: 5708384
Conc: 1.09 ng/ml