

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032825\
 Data File : PS029608.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2025 07:39
 Operator : AR\AJ
 Sample : Q1642-01
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PAT-1-032525

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/28/2025
 Supervised By : mohammad ahmed 04/01/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 08:07:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032825.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 27 12:24:58 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	7.114	7.534	1208.3E6	277.7E6	314.663m	321.681
------	----------	-------	-------	----------	---------	----------	---------

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032825\
Data File : PS029608.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2025 07:39
Operator : AR\AJ
Sample : Q1642-01
Misc :
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
PAT-1-032525


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/28/2025
Supervised By : mohammad ahmed 04/01/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 08:07:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032825.M
Quant Title : 8080.M
QLast Update : Thu Mar 27 12:24:58 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

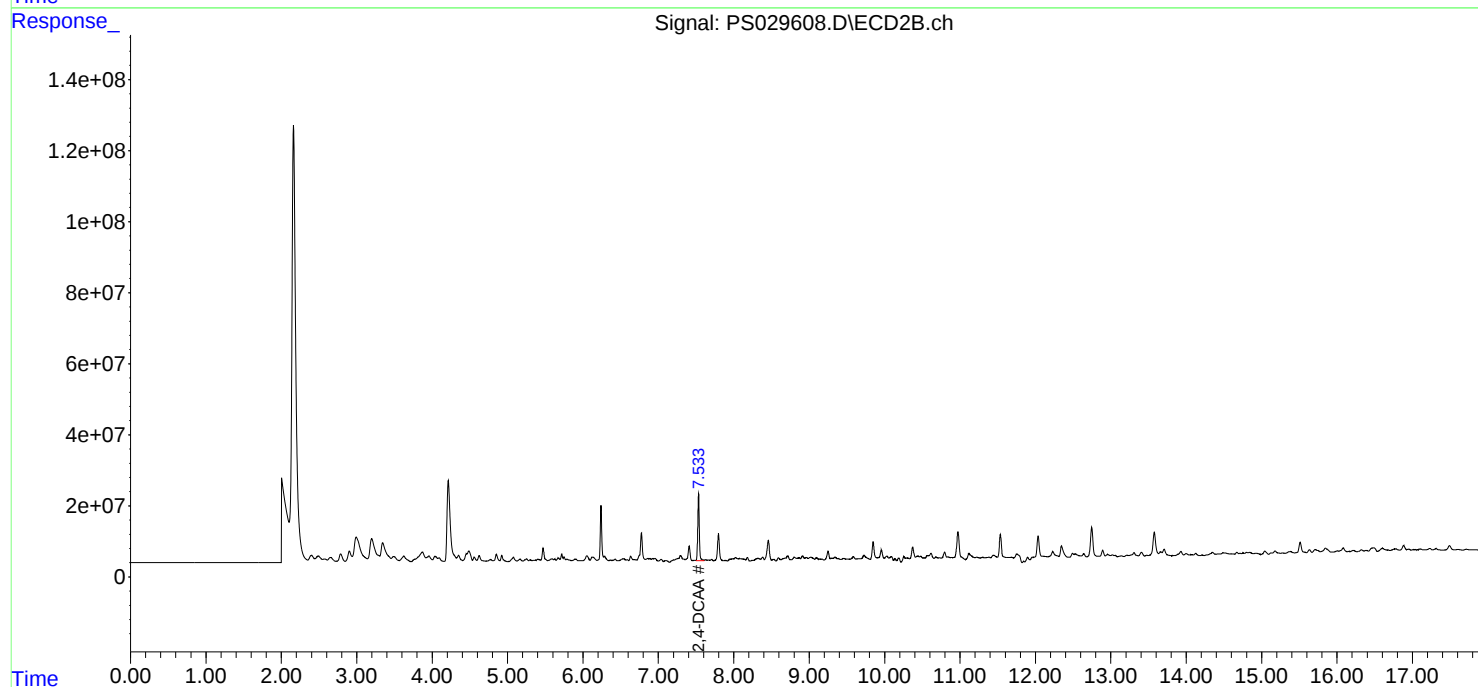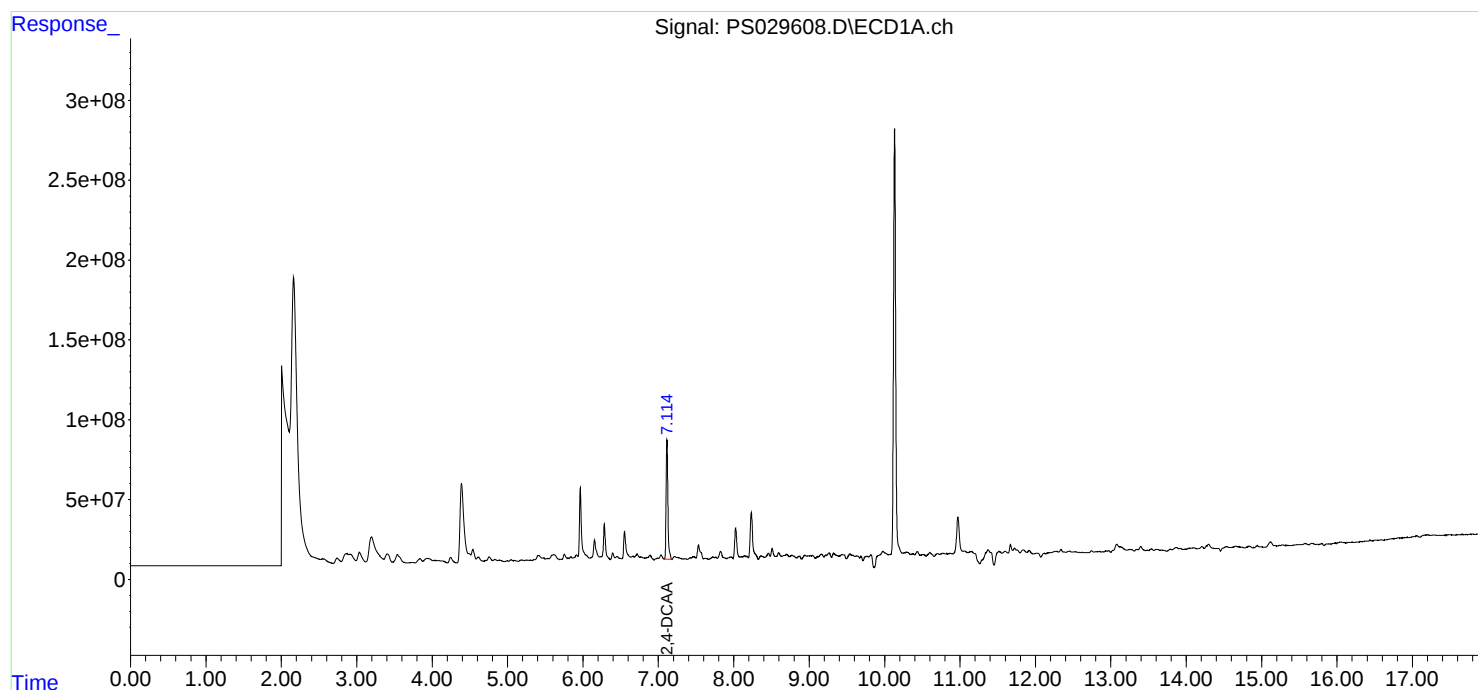

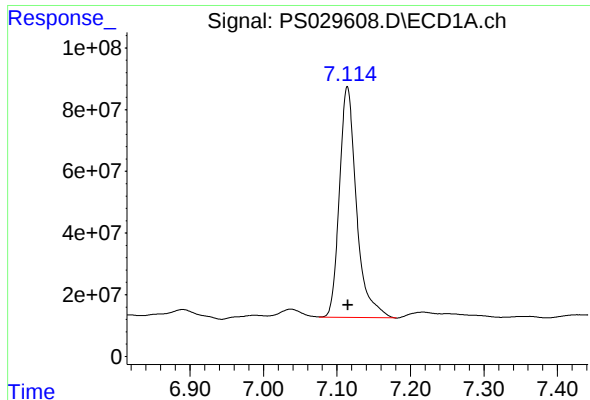


#4 2,4-DCAA

R.T.: 7.114 min
Delta R.T.: -0.001 min
Response: 1208334393
Conc: 314.66 ng/ml

Instrument :
ECD_S
ClientSampleId :
PAT-1-032525

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/28/2025
Supervised By :mohammad ahmed 04/01/2025

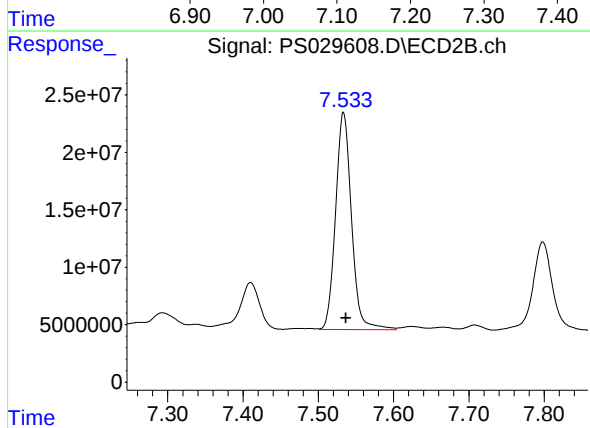

#4 2,4-DCAA

R.T.: 7.534 min
Delta R.T.: -0.003 min
Response: 277706375
Conc: 321.68 ng/ml