

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032919\
 Data File : PS003828.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Mar 2019 08:32
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 02:21:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.771	0	46893	N.D.	0.096 #
Target Compounds							
3) T	4-Nitroph...	0.000	9.934	0	119639	N.D.	0.527 #
5) T	DICAMBA	0.000	11.066	0	163392	N.D.	0.088 #
6) T	MCP	0.000	11.252	0	307585	N.D.	0.261 #
7) T	MCPA	0.000	11.598	0	3888493	N.D.	2.180 #
8) T	DICHLORPROP	0.000	12.111	0	410991	N.D.	0.883 #
9) T	2,4-D	0.000	12.648	0	160737	N.D.	0.302 #
10) T	Pentachlo...	0.000	13.172	0	100901	N.D.	0.015 #
11) T	2,4,5-TP ...	0.000	13.810	0	255996	N.D.	0.097 #
12) T	2,4,5-T	0.000	14.337	0	408863	N.D.	0.188 #
13) T	2,4-DB	0.000	15.005	0	201535	N.D.	0.679 #
14) T	DINOSEB	0.000	15.468	0	231111	N.D.	0.120 #
15) T	Picloram	0.000	16.644	0	8701867	N.D.	2.744 #
16) T	DCPA	0.000	16.644	0	8701867	N.D.	2.574 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032919\
Data File : PS003828.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Mar 2019 08:32
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 02:21:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

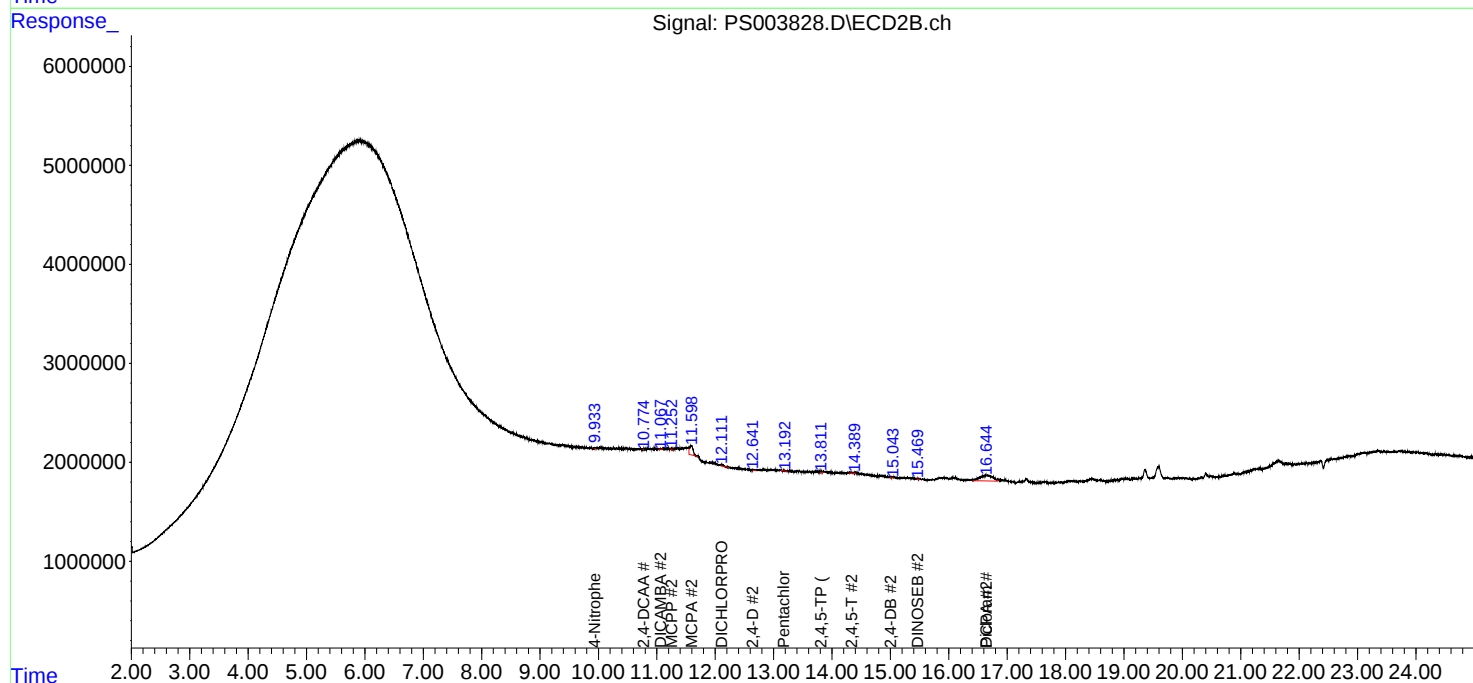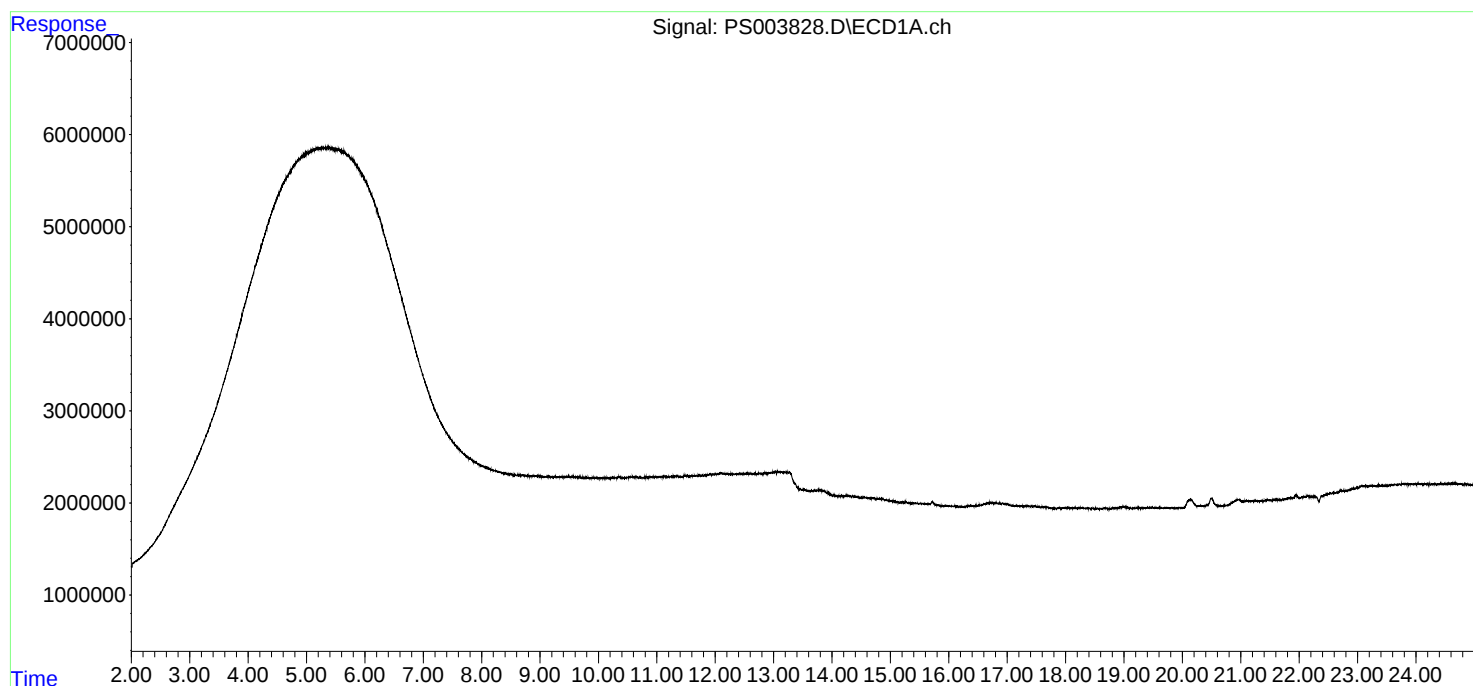


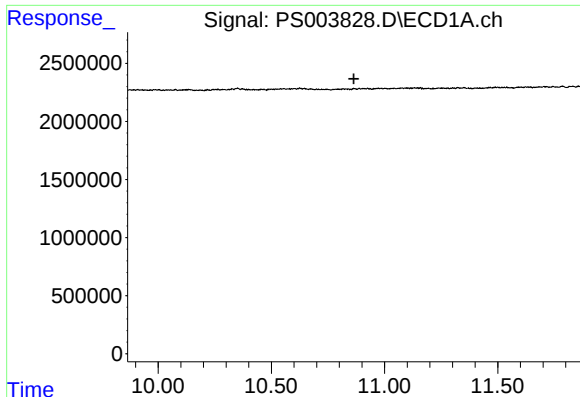

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

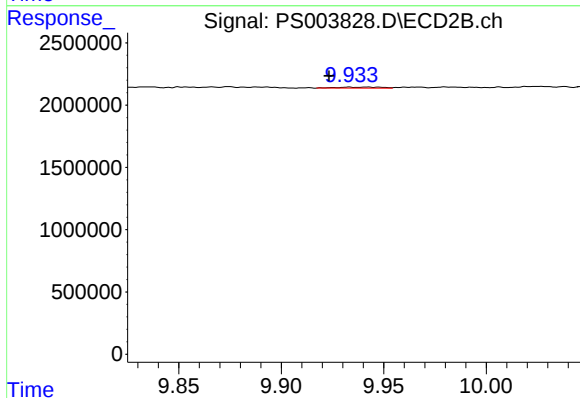


#3 4-Nitrophenol

R.T.: 9.934 min
Delta R.T.: 0.011 min
Response: 119639
Conc: 0.53 ng/ml

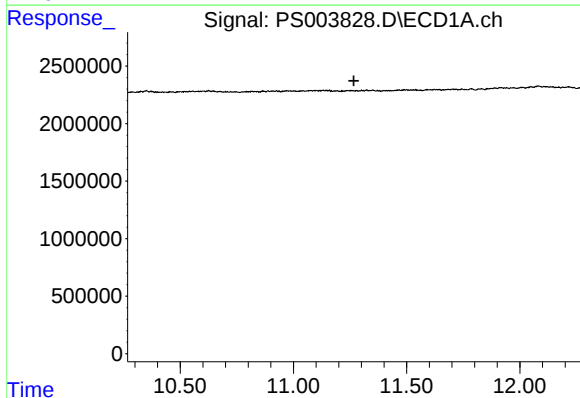


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 11.267 min
Response: 0
Conc: N.D.

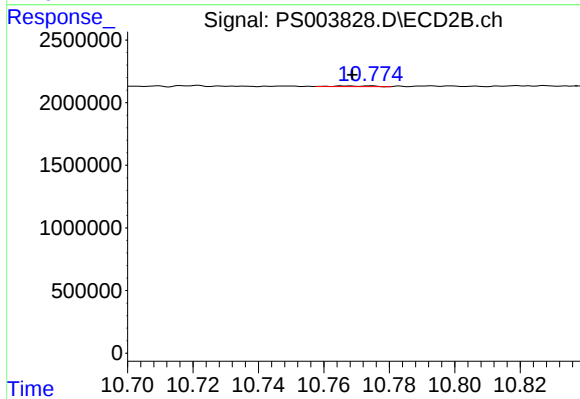

#4 2,4-DCAA


R.T.: 10.771 min
Delta R.T.: 0.003 min
Response: 46893
Conc: 0.10 ng/ml

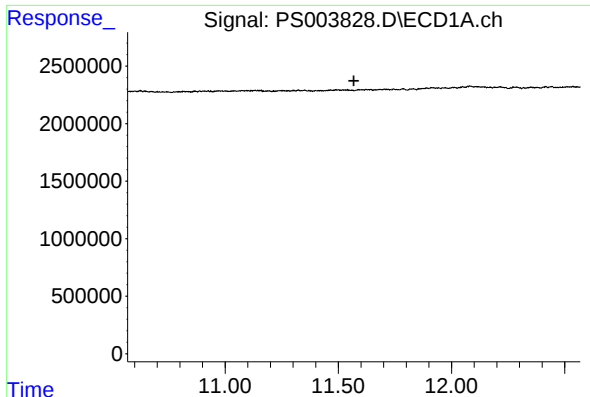

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 11.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

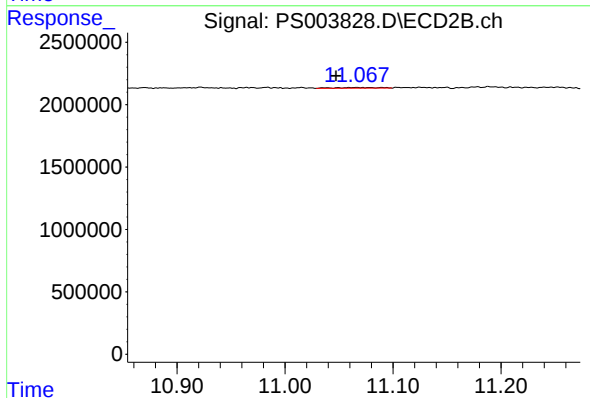


#5 DICAMBA

R.T.: 11.066 min
Delta R.T.: 0.019 min
Response: 163392
Conc: 0.09 ng/ml

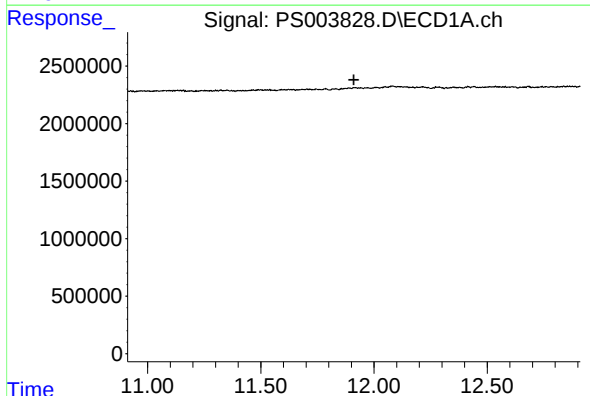


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.911 min
Response: 0
Conc: N.D.

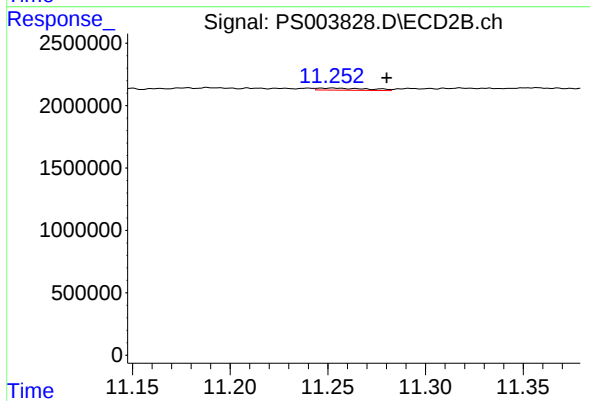

#6 MCP


R.T.: 11.252 min
Delta R.T.: -0.028 min
Response: 307585
Conc: 0.26 ug/ml

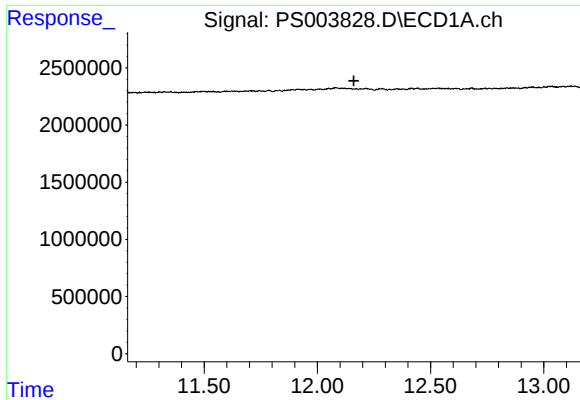

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.162 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

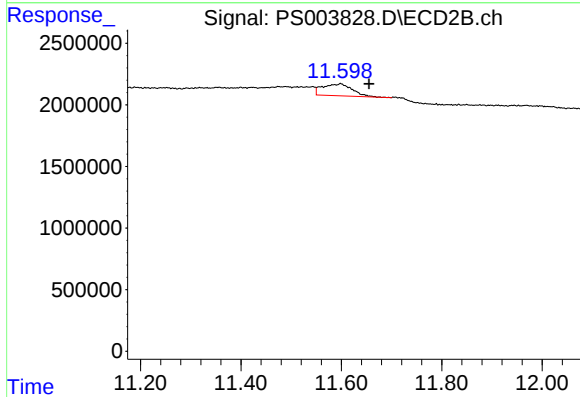


#7 MCPA

R.T.: 11.598 min
Delta R.T.: -0.057 min
Response: 3888493
Conc: 2.18 ug/ml

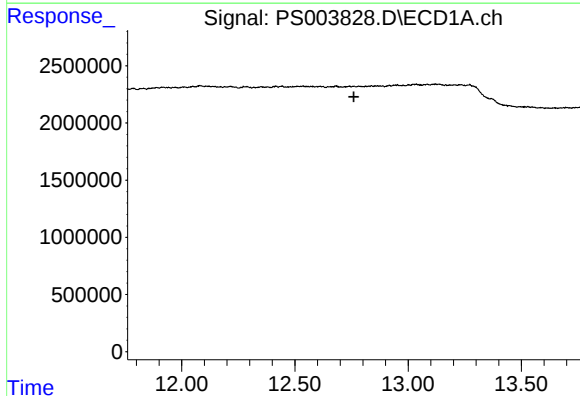


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.760 min
Response: 0
Conc: N.D.

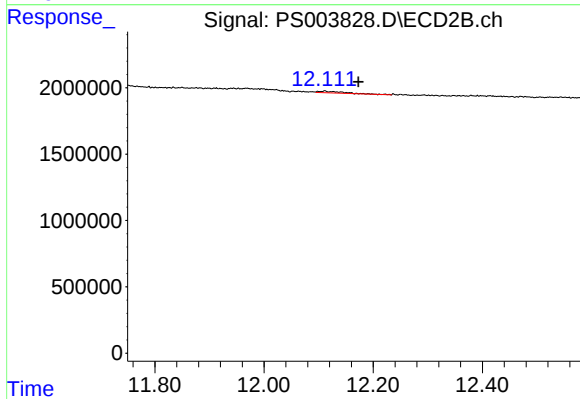

#8 DICHLORPROP


R.T.: 12.111 min
Delta R.T.: -0.062 min
Response: 410991
Conc: 0.88 ng/ml

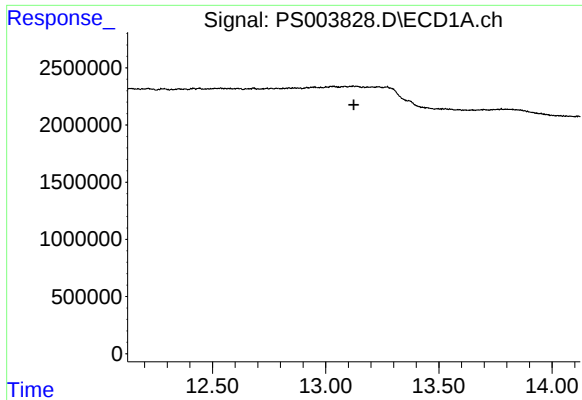

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

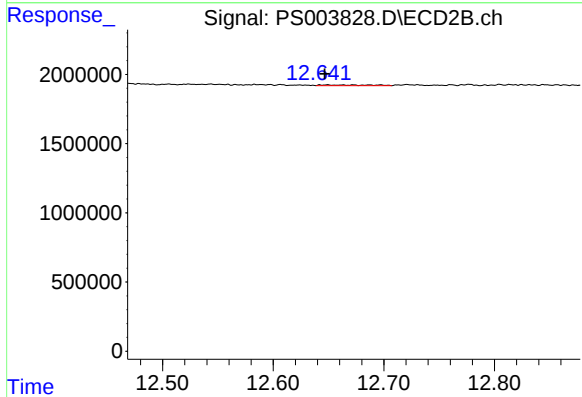


#9 2,4-D

R.T.: 12.648 min
Delta R.T.: 0.002 min
Response: 160737
Conc: 0.30 ng/ml

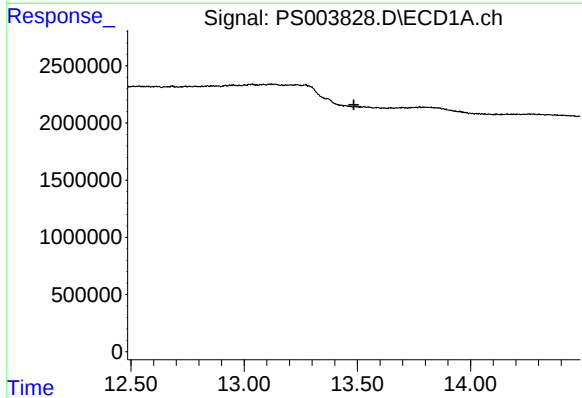


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.485 min
Response: 0
Conc: N.D.

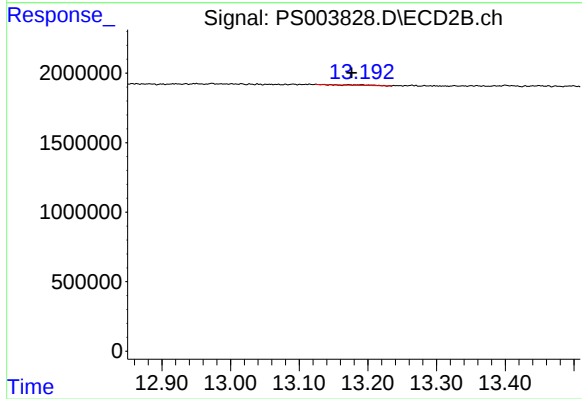

#10 Pentachlorophenol


R.T.: 13.172 min
Delta R.T.: -0.005 min
Response: 100901
Conc: 0.01 ng/ml

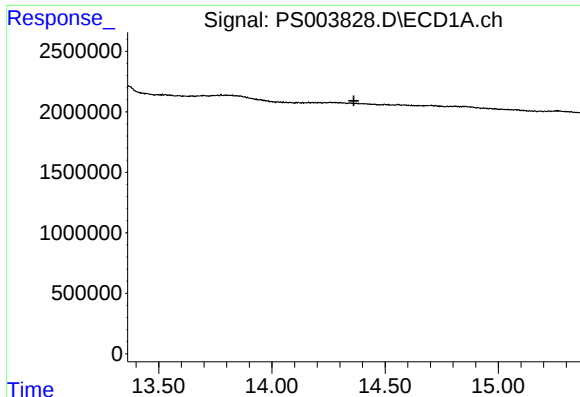

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

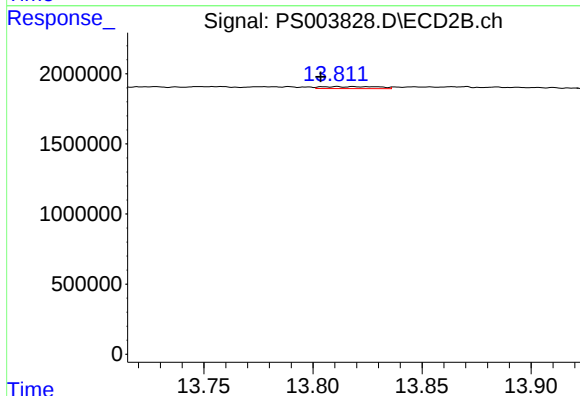


#11 2,4,5-TP (SILVEX)

R.T.: 13.810 min
Delta R.T.: 0.007 min
Response: 255996
Conc: 0.10 ng/ml

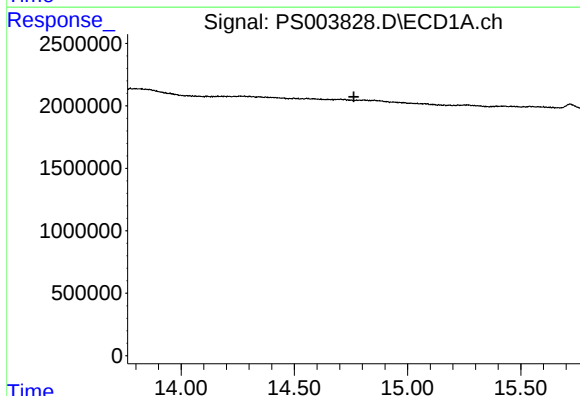


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.763 min
Response: 0
Conc: N.D.

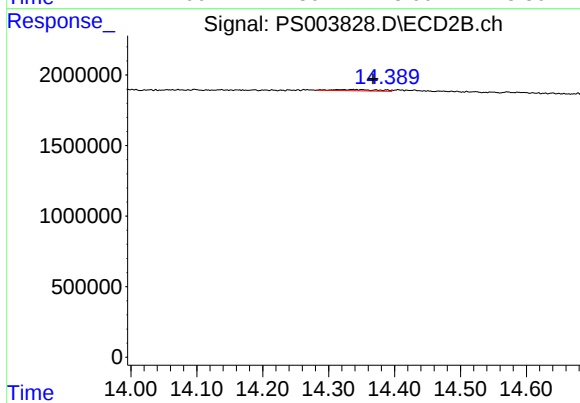

#12 2,4,5-T


R.T.: 14.337 min
Delta R.T.: -0.030 min
Response: 408863
Conc: 0.19 ng/ml

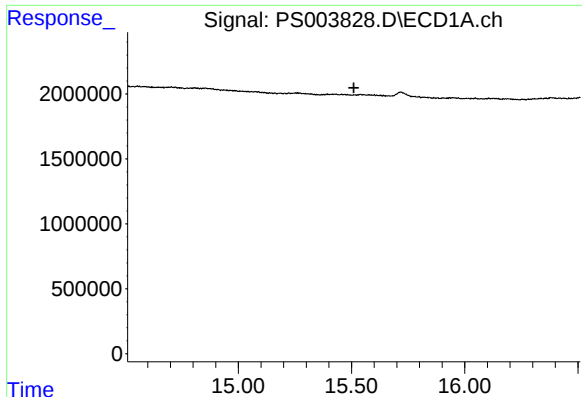

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

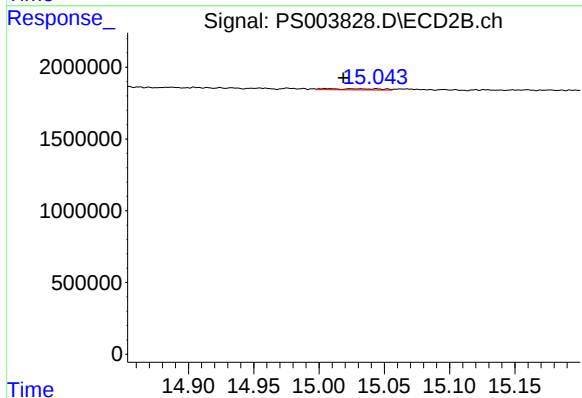


#13 2,4-DB

R.T.: 15.005 min
Delta R.T.: -0.014 min
Response: 201535
Conc: 0.68 ng/ml

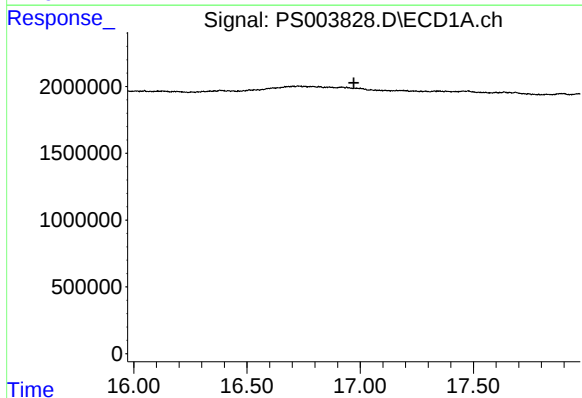


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.972 min
Response: 0
Conc: N.D.

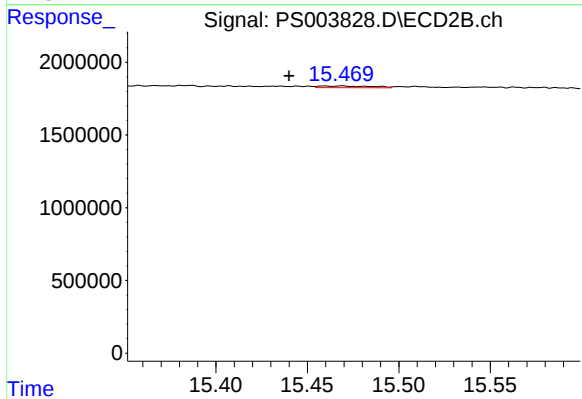

#14 DINOSEB


R.T.: 15.468 min
Delta R.T.: 0.028 min
Response: 231111
Conc: 0.12 ng/ml

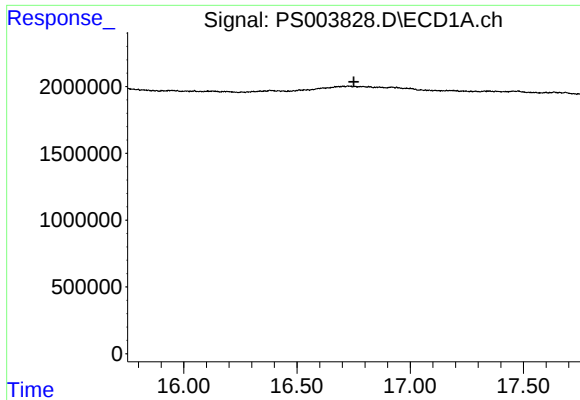

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.752 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

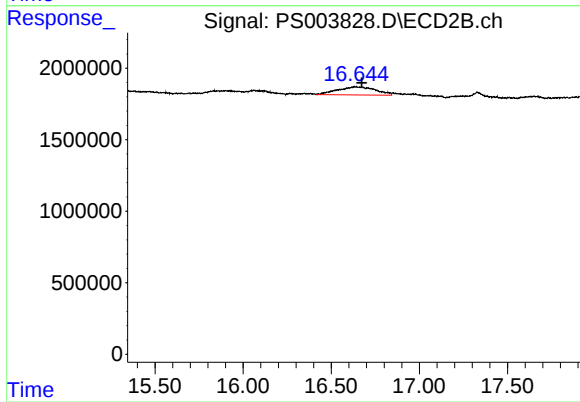


#15 Picloram

R.T.: 16.644 min
Delta R.T.: -0.029 min
Response: 8701867
Conc: 2.74 ng/ml

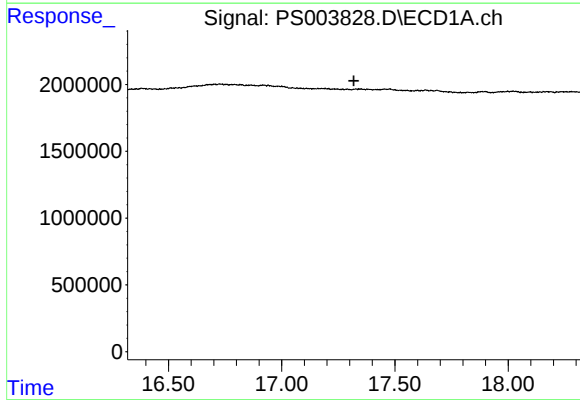

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.319 min
Response: 0
Conc: N.D.

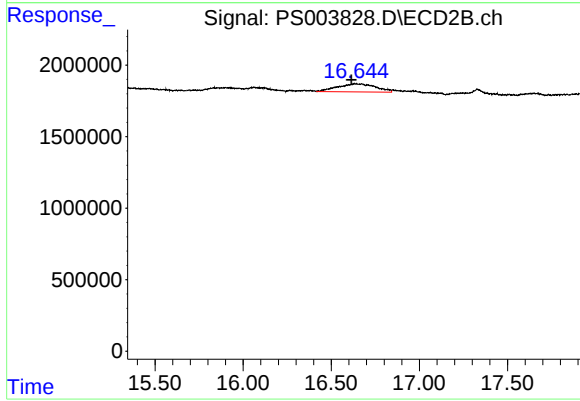

#16 DCPA

R.T.: 16.644 min
Delta R.T.: 0.029 min
Response: 8701867
Conc: 2.57 ng/ml