

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032919\
 Data File : PS003831.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Mar 2019 11:45
 Operator : EI\SJ
 Sample : PB118327BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB118327BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 02:22:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.264	10.758	247.1E6	242.8E6	566.481	494.781
Target Compounds							
1) T	Dalapon	2.785	2.276	78980973	133.2E6	105.939	182.556 #
2) T	3,5-DICHL...	0.000	8.921	0	5516905	N.D.	8.649 #
3) T	4-Nitroph...	0.000	9.931	0	19180242	N.D.	84.482 #
6) T	MCP	11.977	11.233	7889095	-230525	5.671	N.D. #
7) T	MCPA	12.221	0.000	59322191	0	28.118	N.D. #
9) T	2,4-D	0.000	12.618	0	2688072	N.D.	5.054 #
10) T	Pentachlo...	0.000	13.167	0	487406	N.D.	0.070 #
11) T	2,4,5-TP ...	0.000	13.771	0	1778695	N.D.	0.672 #
12) T	2,4,5-T	0.000	14.398	0	15353119	N.D.	7.063 #
13) T	2,4-DB	0.000	14.986	0	2075531	N.D.	6.989 #
14) T	DINOSEB	0.000	15.433	0	561869	N.D.	0.293 #
15) T	Picloram	0.000	16.706	0	29939998	N.D.	9.441 #
16) T	DCPA	0.000	16.623	0	4530951	N.D.	1.341 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032919\
Data File : PS003831.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Mar 2019 11:45
Operator : EI\SJ
Sample : PB118327BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB118327BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 02:22:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

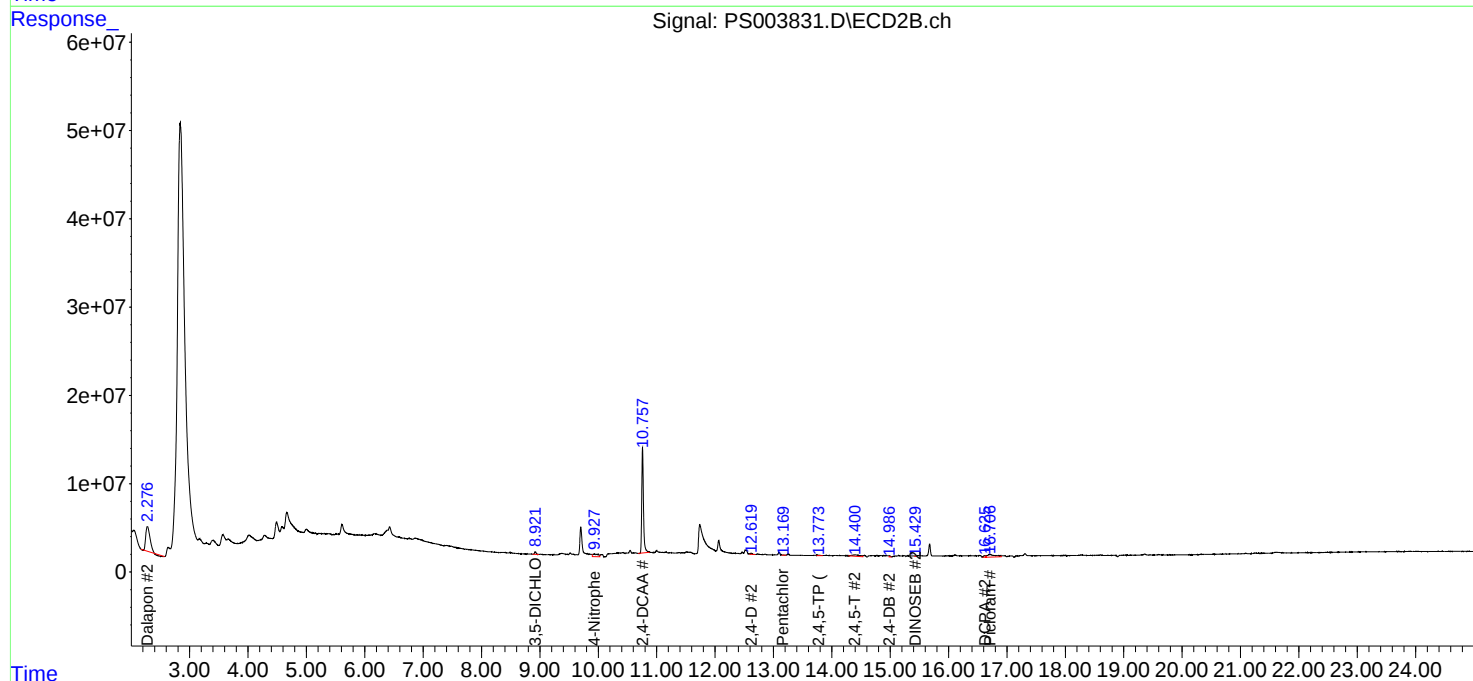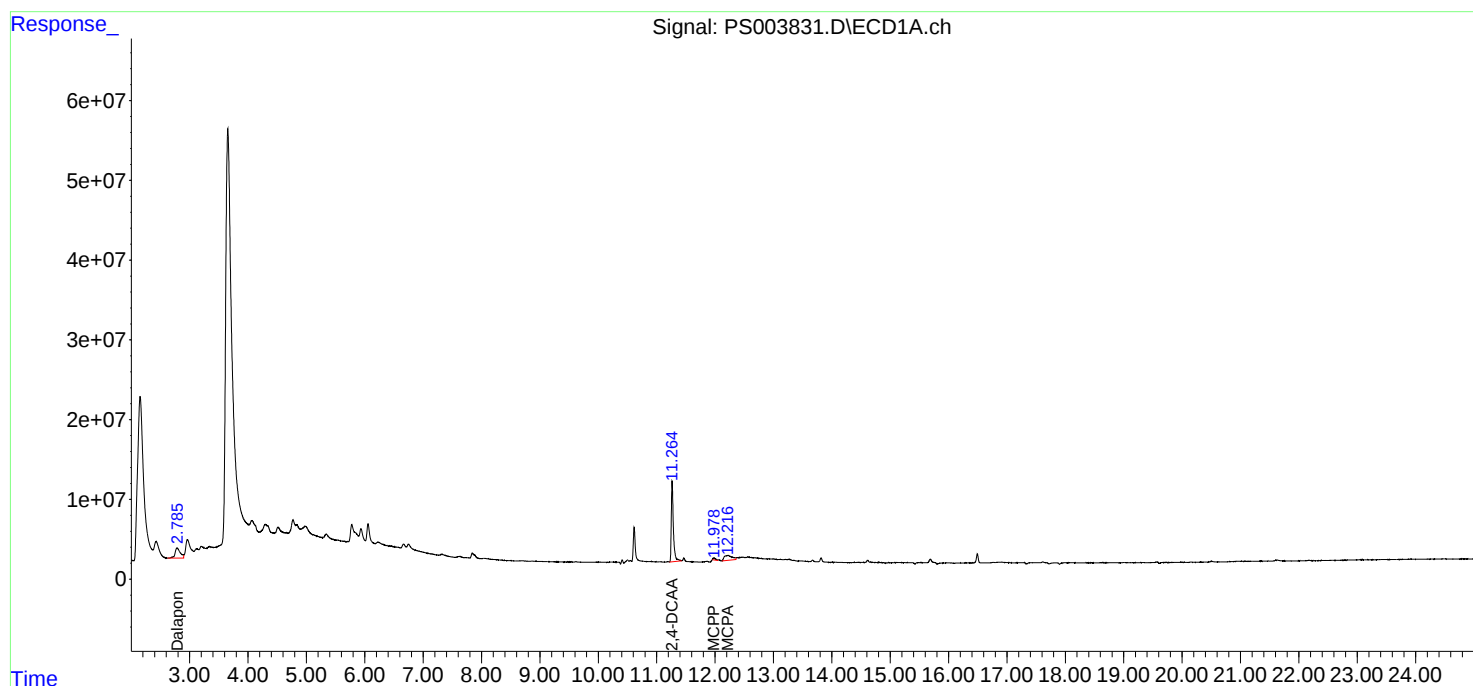


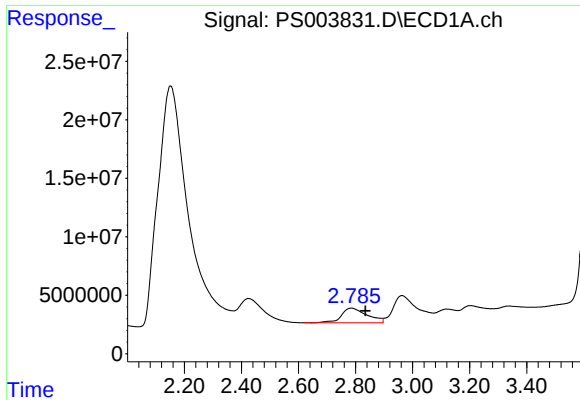

#1 Dalapon


R.T.: 2.785 min
Delta R.T.: -0.050 min
Response: 78980973
Conc: 105.94 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB118327BL

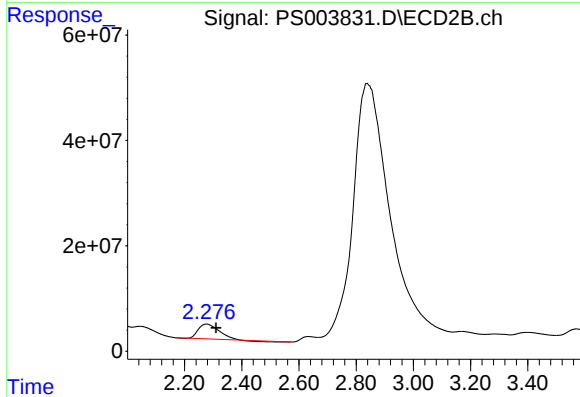


#1 Dalapon

R.T.: 2.276 min
Delta R.T.: -0.034 min
Response: 133198329
Conc: 182.56 ng/ml

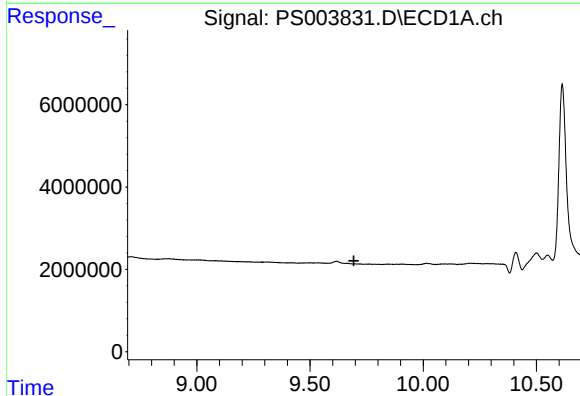


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

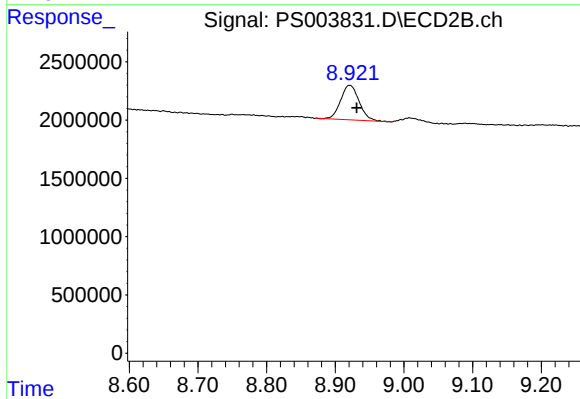

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.921 min
Delta R.T.: -0.010 min
Response: 5516905
Conc: 8.65 ng/ml

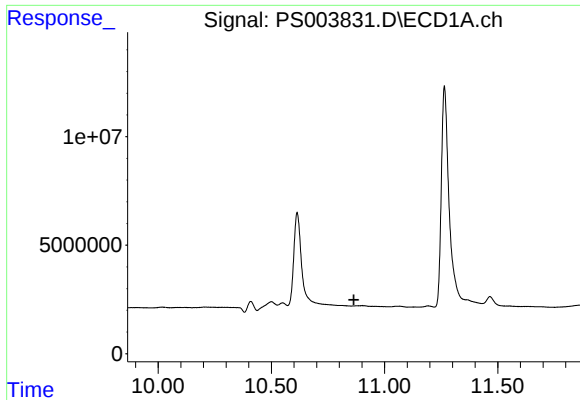

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB118327BL

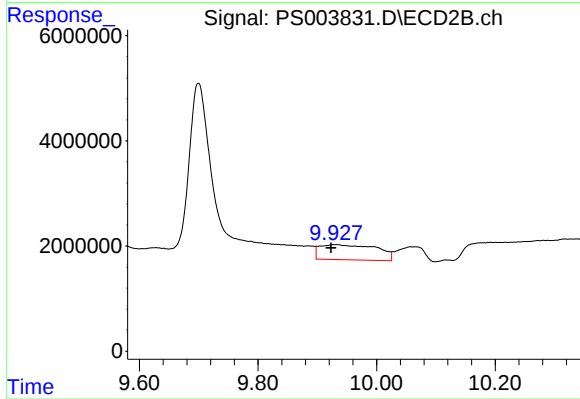


#3 4-Nitrophenol

R.T.: 9.931 min
Delta R.T.: 0.007 min
Response: 19180242
Conc: 84.48 ng/ml

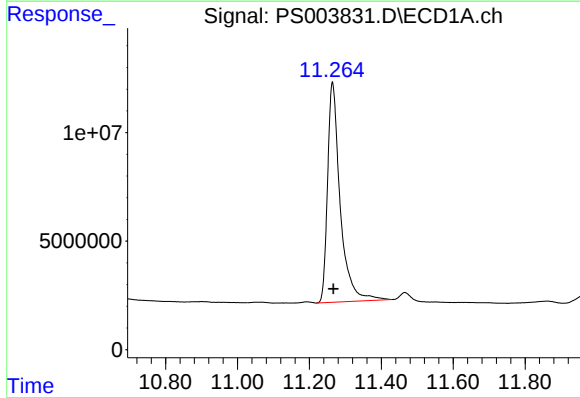


#4 2,4-DCAA

R.T.: 11.264 min
Delta R.T.: -0.002 min
Response: 247105856
Conc: 566.48 ng/ml

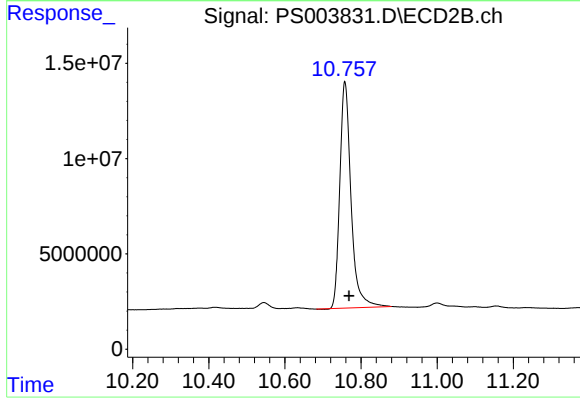

#4 2,4-DCAA


R.T.: 10.758 min
Delta R.T.: -0.011 min
Response: 242768420
Conc: 494.78 ng/ml

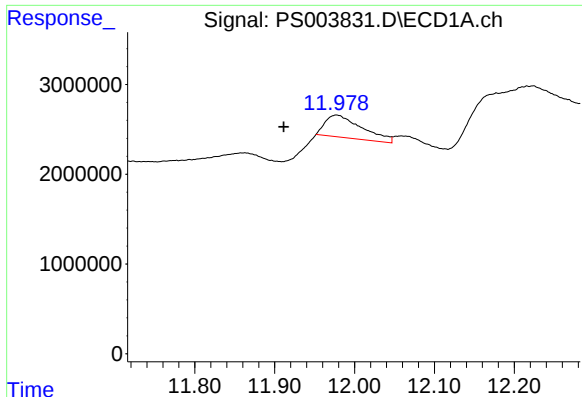

#6 MCPP


R.T.: 11.977 min
Delta R.T.: 0.066 min
Response: 7889095
Conc: 5.67 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB118327BL

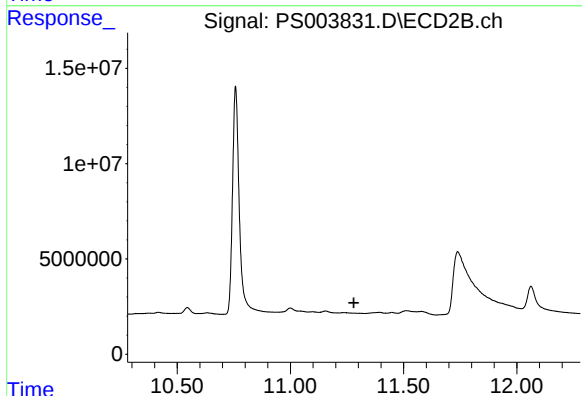


#6 MCPP

R.T.: 11.233 min
Delta R.T.: -0.047 min
Response: -230525
Conc: N.D.

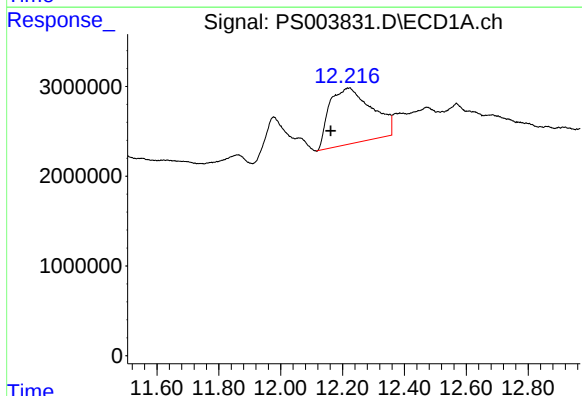


#7 MCPA

R.T.: 12.221 min
Delta R.T.: 0.060 min
Response: 59322191
Conc: 28.12 ug/ml

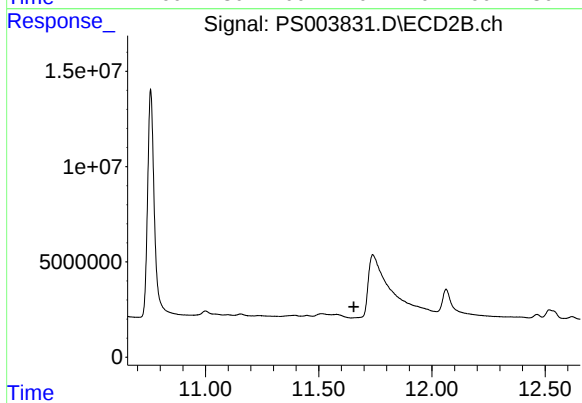

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 11.655 min
Response: 0
Conc: N.D.

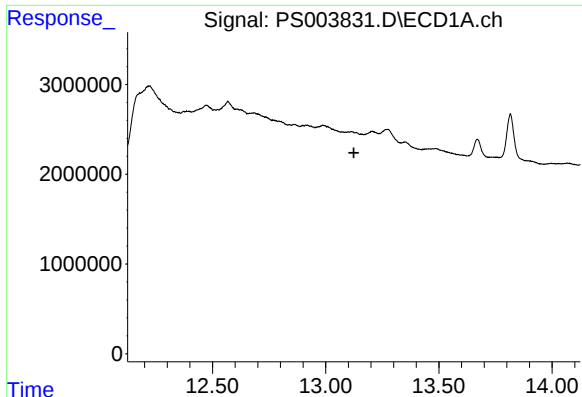

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB118327BL

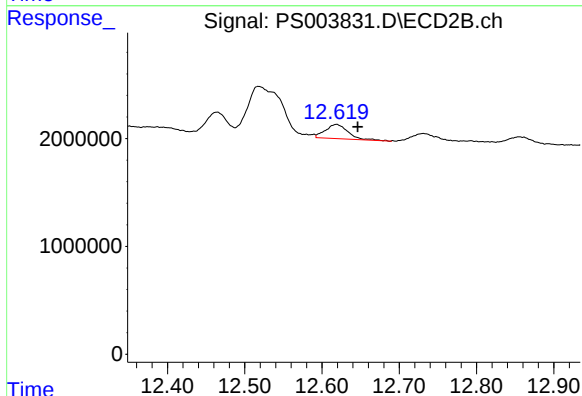


#9 2,4-D

R.T.: 12.618 min
Delta R.T.: -0.028 min
Response: 2688072
Conc: 5.05 ng/ml

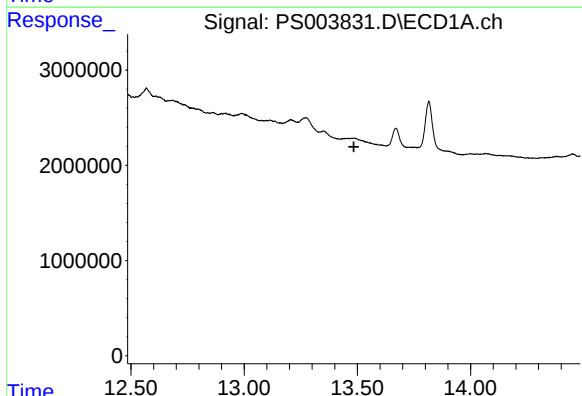


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.485 min
Response: 0
Conc: N.D.

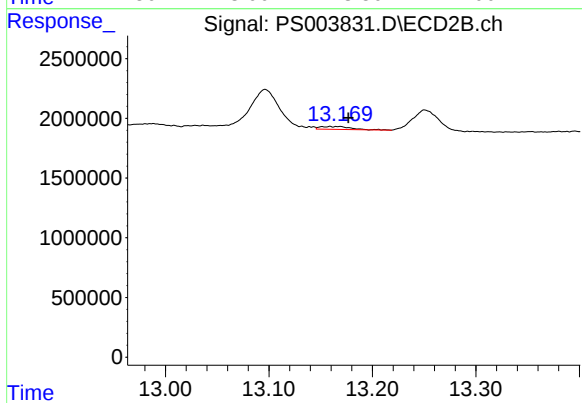

#10 Pentachlorophenol


R.T.: 13.167 min
Delta R.T.: -0.010 min
Response: 487406
Conc: 0.07 ng/ml

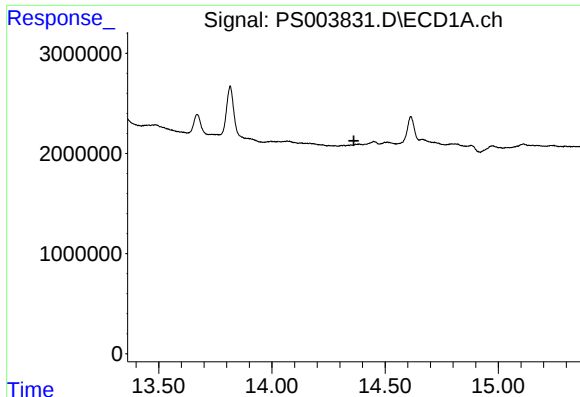

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB118327BL

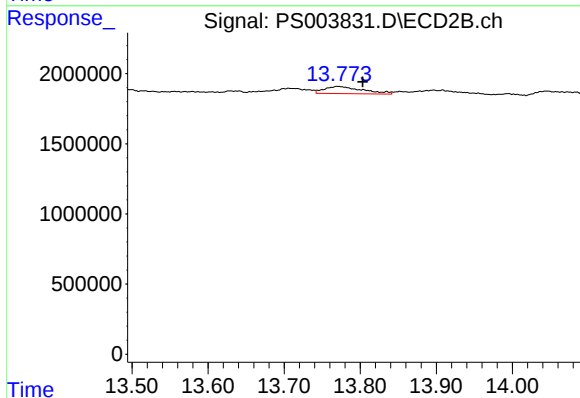


#11 2,4,5-TP (SILVEX)

R.T.: 13.771 min
Delta R.T.: -0.032 min
Response: 1778695
Conc: 0.67 ng/ml

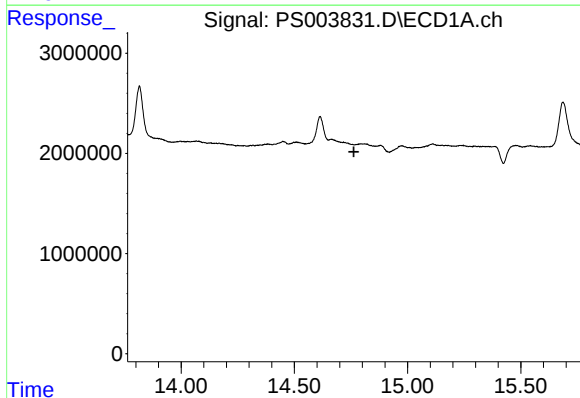


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.763 min
Response: 0
Conc: N.D.

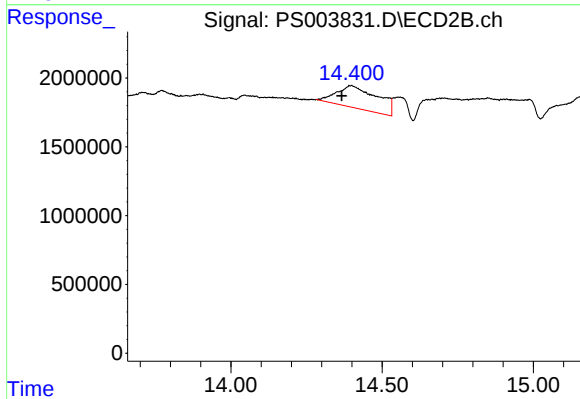

#12 2,4,5-T


R.T.: 14.398 min
Delta R.T.: 0.031 min
Response: 15353119
Conc: 7.06 ng/ml

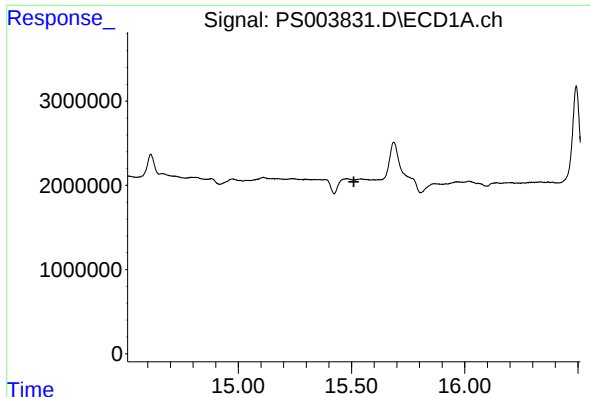

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB118327BL

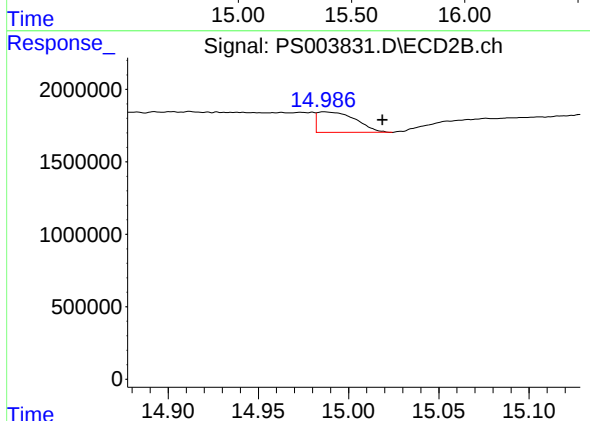


#13 2,4-DB

R.T.: 14.986 min
Delta R.T.: -0.032 min
Response: 2075531
Conc: 6.99 ng/ml

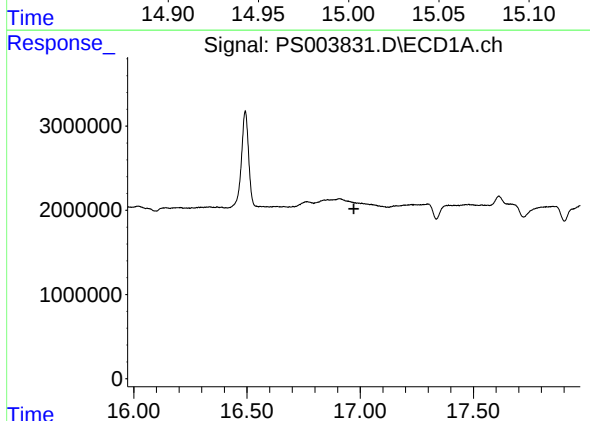


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.972 min
Response: 0
Conc: N.D.

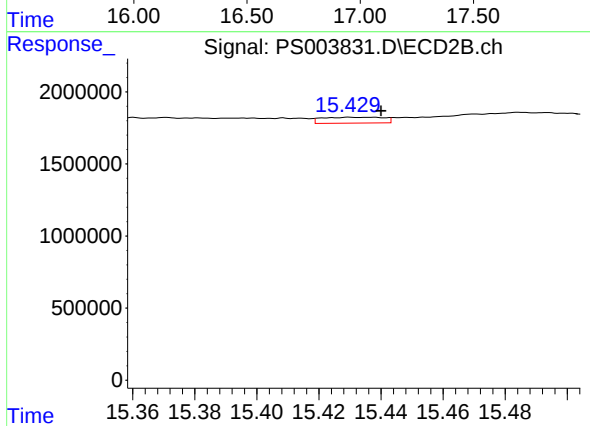

#14 DINOSEB


R.T.: 15.433 min
Delta R.T.: -0.007 min
Response: 561869
Conc: 0.29 ng/ml

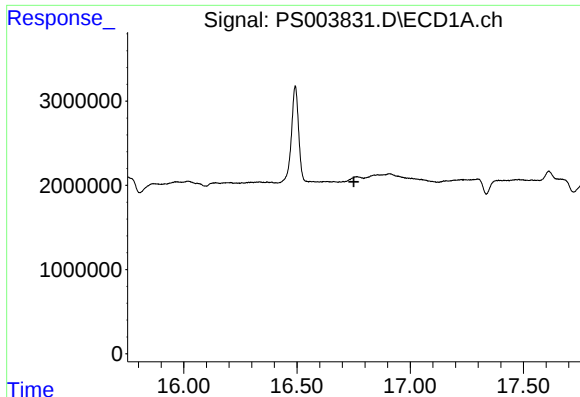

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.752 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB118327BL

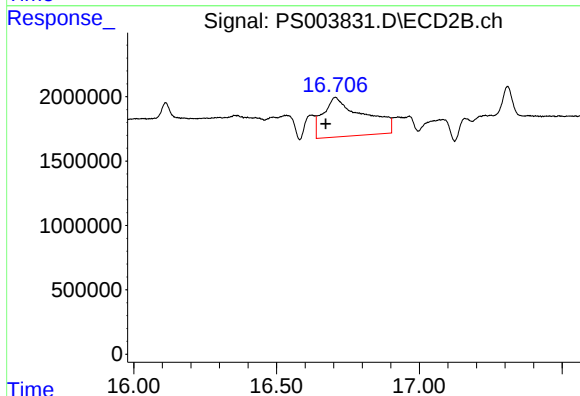


#15 Picloram

R.T.: 16.706 min
Delta R.T.: 0.033 min
Response: 29939998
Conc: 9.44 ng/ml

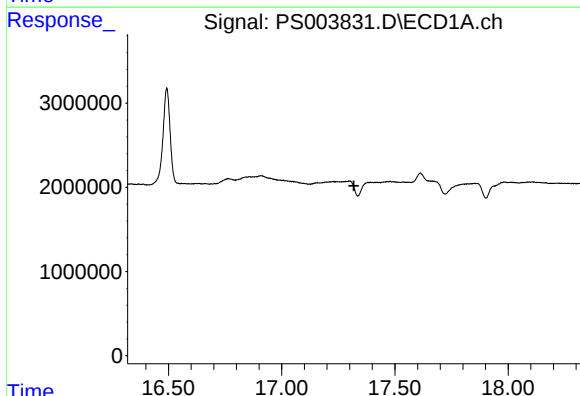

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.319 min
Response: 0
Conc: N.D.

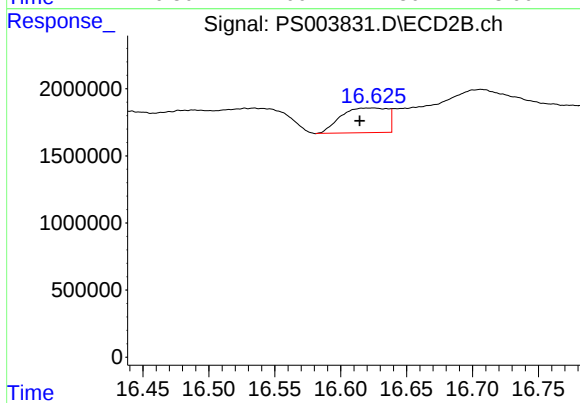

#16 DCPA

R.T.: 16.623 min
Delta R.T.: 0.008 min
Response: 4530951
Conc: 1.34 ng/ml