

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032919\
 Data File : PS003832.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Mar 2019 17:25
 Operator : EI\SJ
 Sample : K1698-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TR-05-032819

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 02:23:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.262	10.764	259.4E6	250.3E6	594.574	510.144
Target Compounds							
1) T	Dalapon	2.783	2.272	66479535	81641120	89.170	111.894 #
2) T	3,5-DICHL...	0.000	8.929	0	5527635	N.D.	8.666 #
3) T	4-Nitroph...	0.000	9.940	0	19044275	N.D.	83.883 #
7) T	MCPA	0.000	11.675	0	698064	N.D.	0.391 #
9) T	2,4-D	0.000	12.606	0	5725287	N.D.	10.764 #
11) T	2,4,5-TP ...	0.000	13.773	0	1936629	N.D.	0.731 #
12) T	2,4,5-T	0.000	14.360	0	1293621	N.D.	0.595 #
13) T	2,4-DB	0.000	14.955	0	2869735	N.D.	9.664 #
14) T	DINOSEB	0.000	15.491	0	3595285	N.D.	1.874 #
15) T	Picloram	0.000	16.617	0	5261774	N.D.	1.659 #
16) T	DCPA	0.000	16.617	0	5261774	N.D.	1.557 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032919\
Data File : PS003832.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Mar 2019 17:25
Operator : EI\SJ
Sample : K1698-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TR-05-032819

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 02:23:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

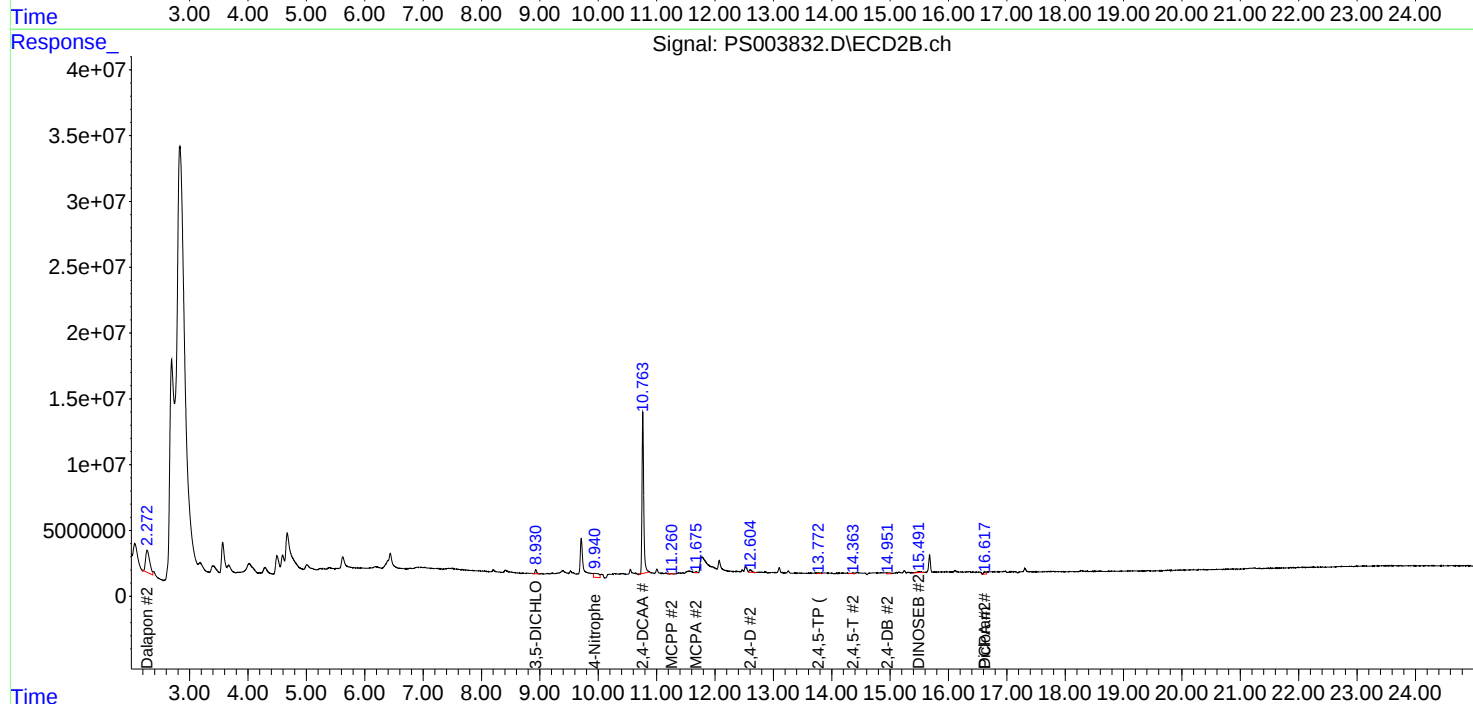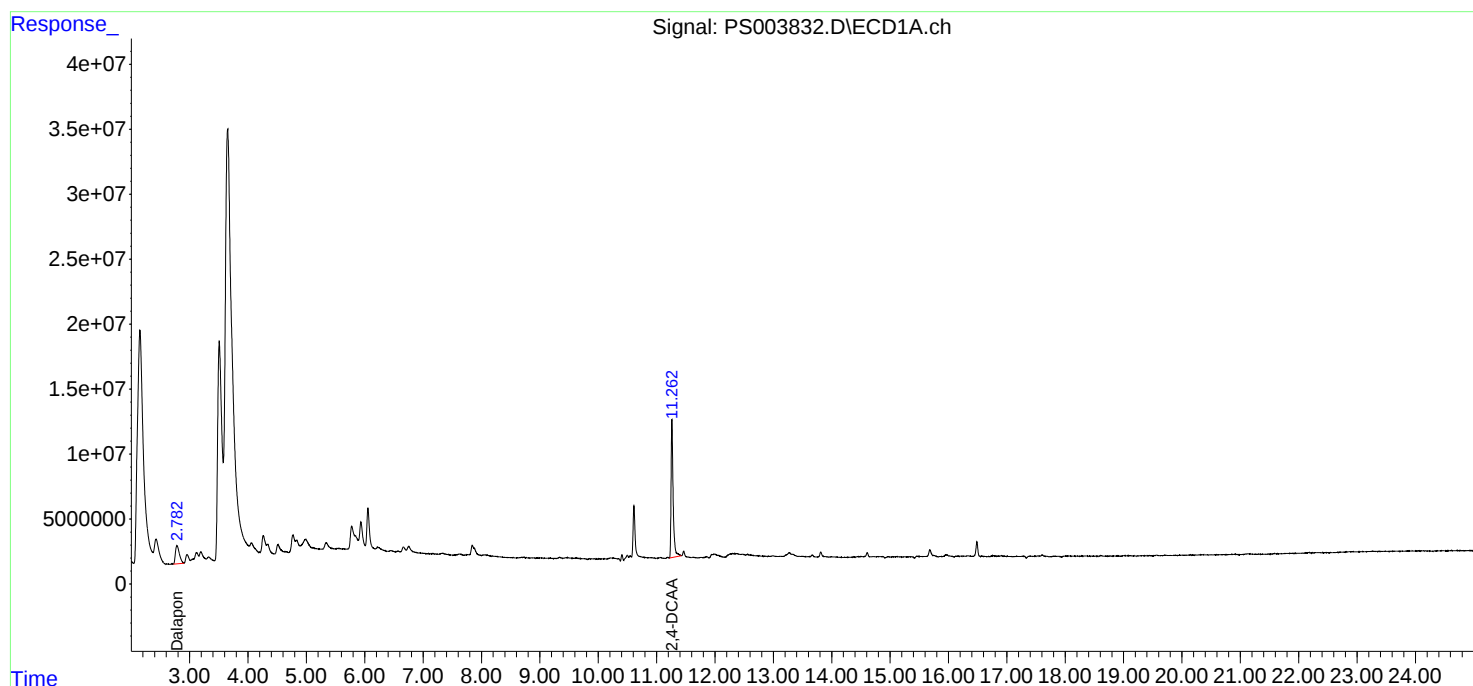


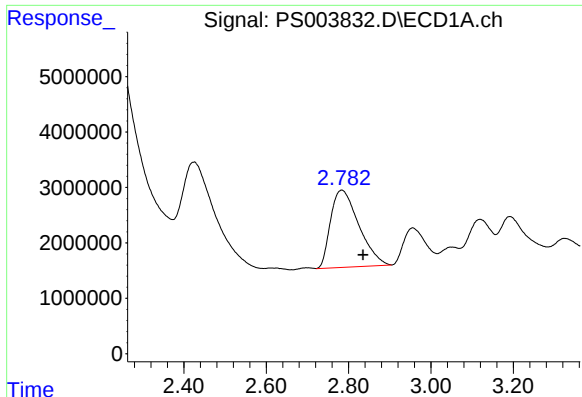

#1 Dalapon


R.T.: 2.783 min
Delta R.T.: -0.052 min
Response: 66479535
Conc: 89.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-05-032819

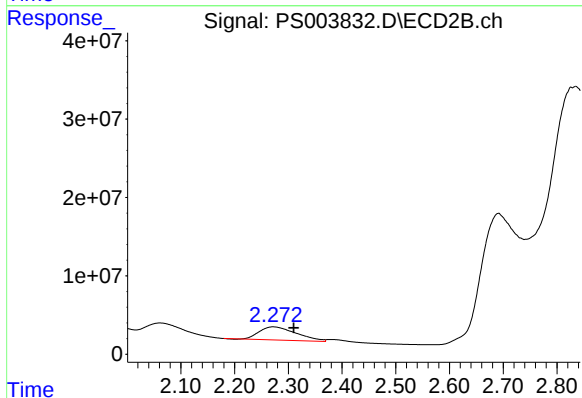


#1 Dalapon

R.T.: 2.272 min
Delta R.T.: -0.039 min
Response: 81641120
Conc: 111.89 ng/ml

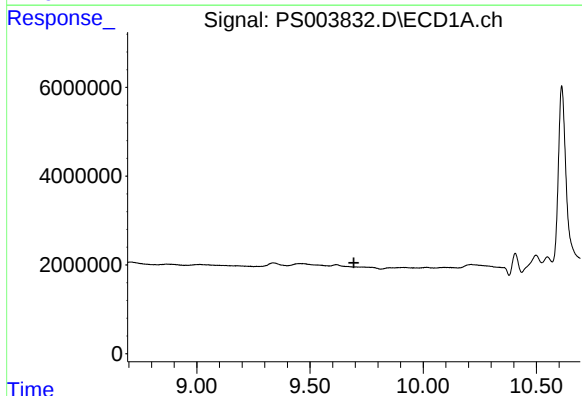


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

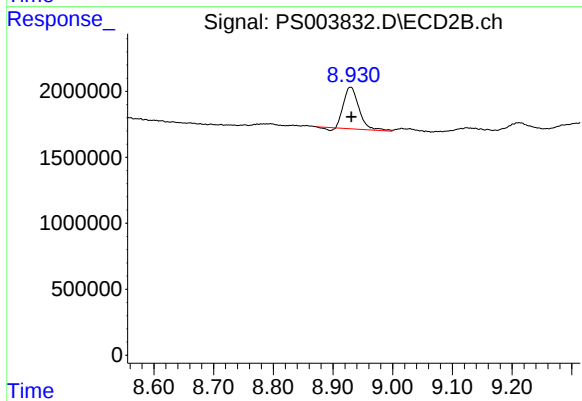

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.929 min
Delta R.T.: -0.002 min
Response: 5527635
Conc: 8.67 ng/ml

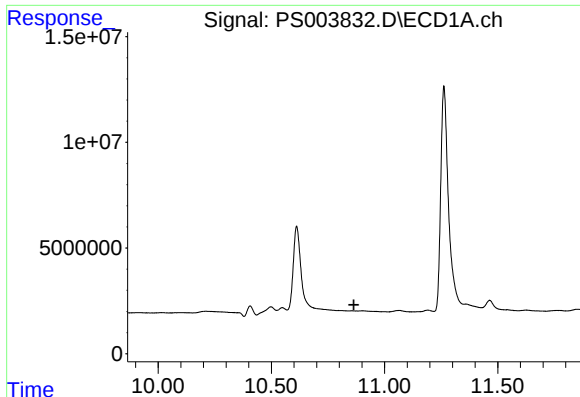

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TR-05-032819

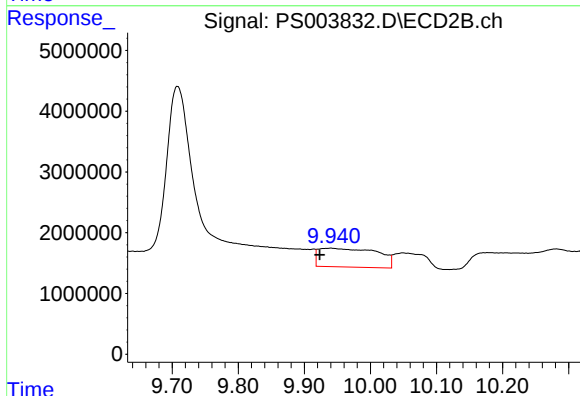


#3 4-Nitrophenol

R.T.: 9.940 min
Delta R.T.: 0.017 min
Response: 19044275
Conc: 83.88 ng/ml

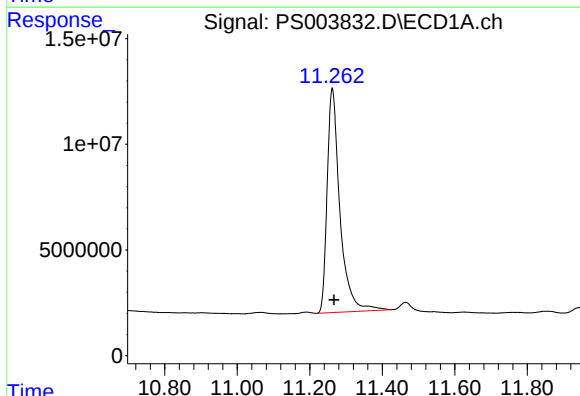


#4 2,4-DCAA

R.T.: 11.262 min
Delta R.T.: -0.005 min
Response: 259360573
Conc: 594.57 ng/ml

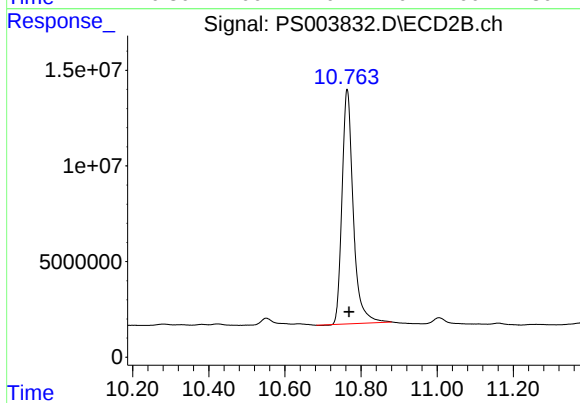

#4 2,4-DCAA


R.T.: 10.764 min
Delta R.T.: -0.005 min
Response: 250306319
Conc: 510.14 ng/ml

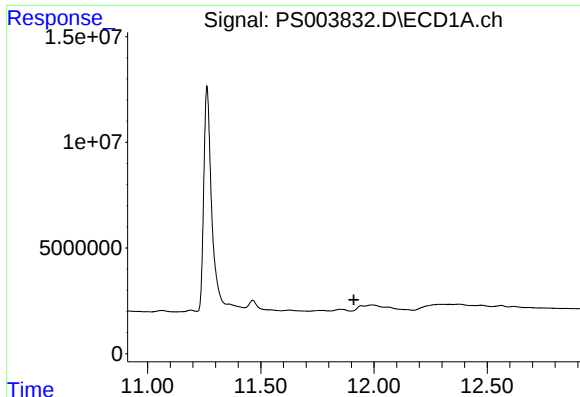

#6 MCPP


R.T.: 11.943 min
Delta R.T.: 0.032 min
Response: -2361057
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TR-05-032819

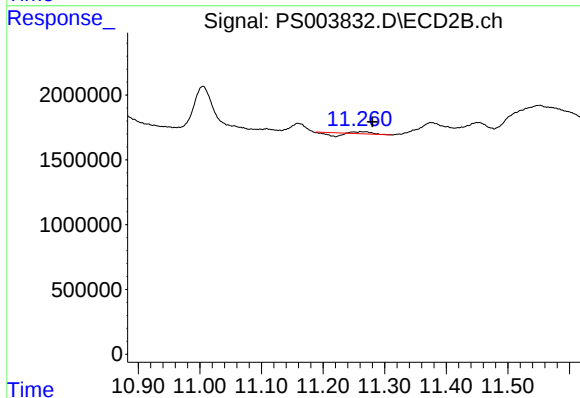


#6 MCPP

R.T.: 11.267 min
Delta R.T.: -0.013 min
Response: 45100
Conc: 0.04 ug/ml

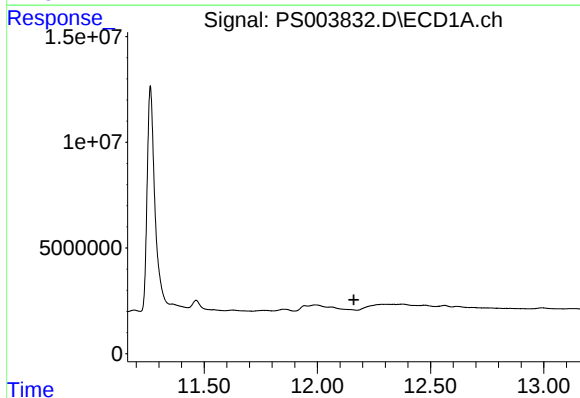


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.162 min
Response: 0
Conc: N.D.

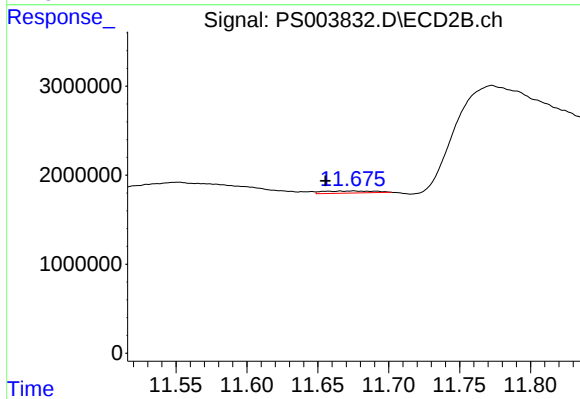

#7 MCPA


R.T.: 11.675 min
Delta R.T.: 0.020 min
Response: 698064
Conc: 0.39 ug/ml

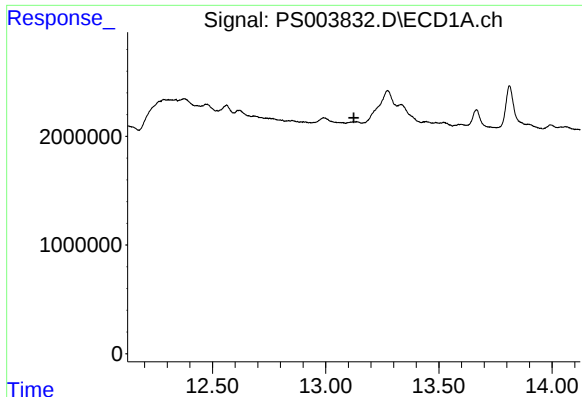

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TR-05-032819

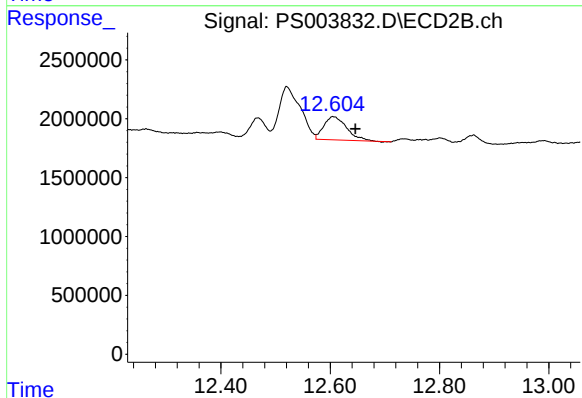


#9 2,4-D

R.T.: 12.606 min
Delta R.T.: -0.041 min
Response: 5725287
Conc: 10.76 ng/ml

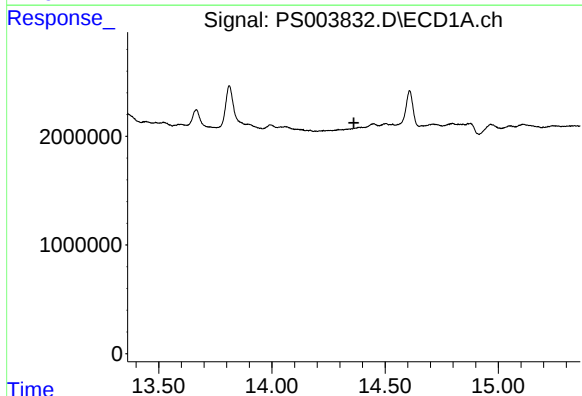


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.362 min
Response: 0
Conc: N.D.

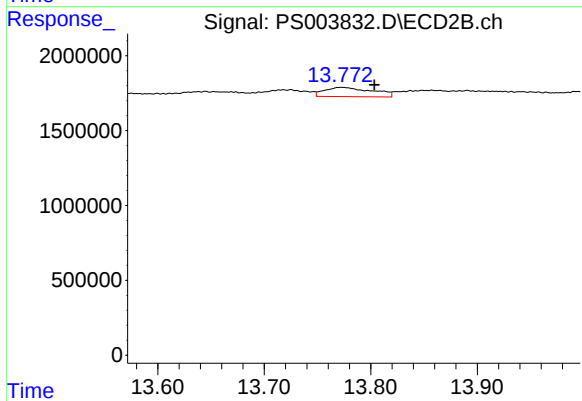

#11 2,4,5-TP (SILVEX)


R.T.: 13.773 min
Delta R.T.: -0.031 min
Response: 1936629
Conc: 0.73 ng/ml

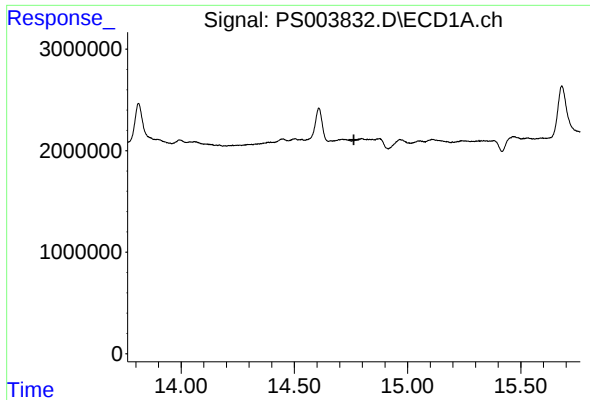

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.763 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TR-05-032819

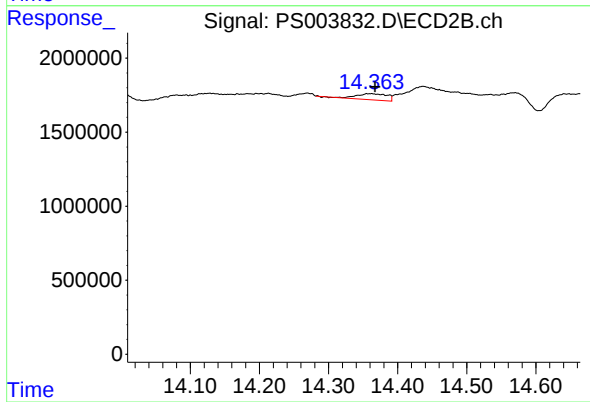


#12 2,4,5-T

R.T.: 14.360 min
Delta R.T.: -0.007 min
Response: 1293621
Conc: 0.60 ng/ml

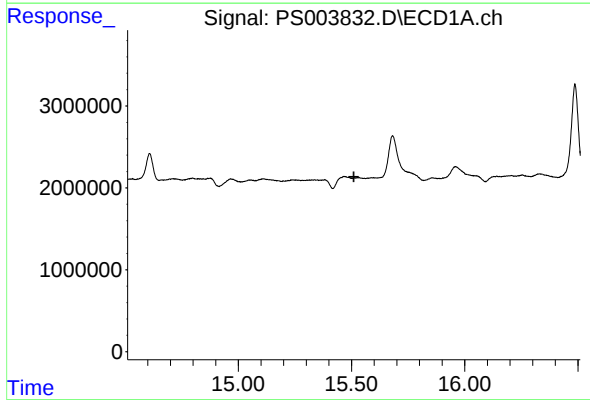


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

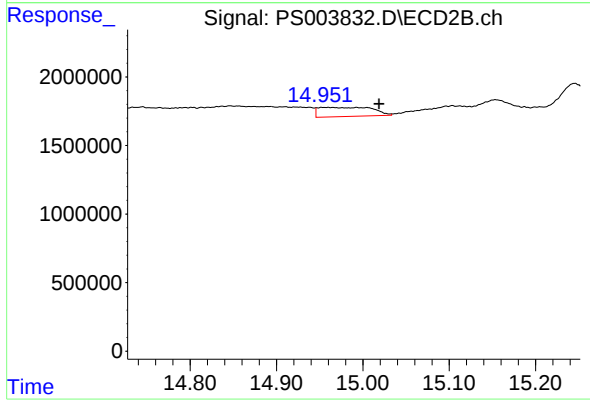

#13 2,4-DB


R.T.: 14.955 min
Delta R.T.: -0.063 min
Response: 2869735
Conc: 9.66 ng/ml

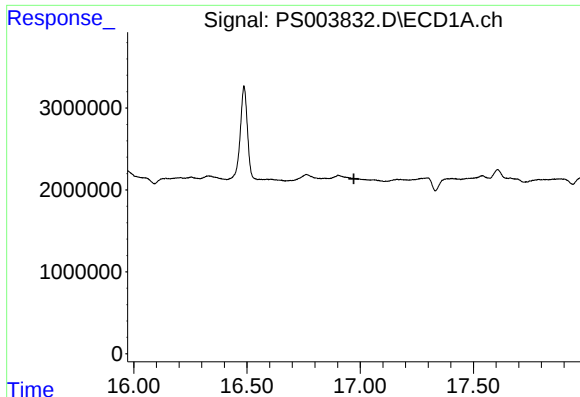

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 16.972 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TR-05-032819

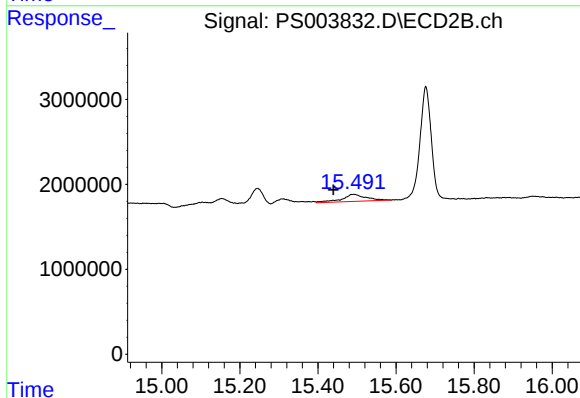


#14 DINOSEB

R.T.: 15.491 min
Delta R.T.: 0.051 min
Response: 3595285
Conc: 1.87 ng/ml

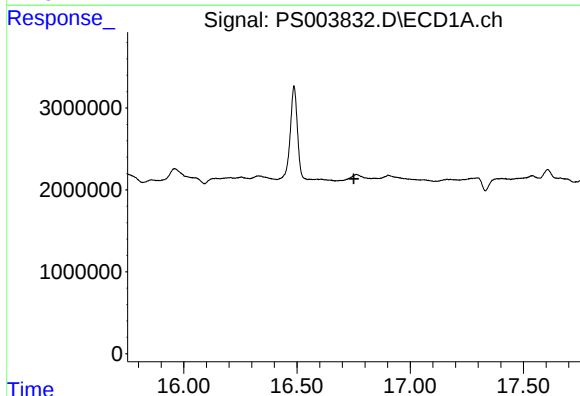


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.752 min
Response: 0
Conc: N.D.

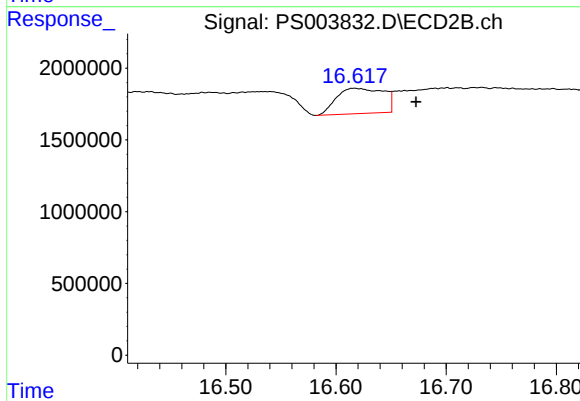

#15 Picloram


R.T.: 16.617 min
Delta R.T.: -0.055 min
Response: 5261774
Conc: 1.66 ng/ml

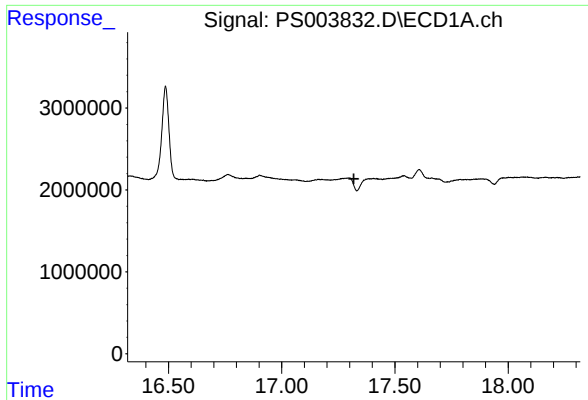

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TR-05-032819

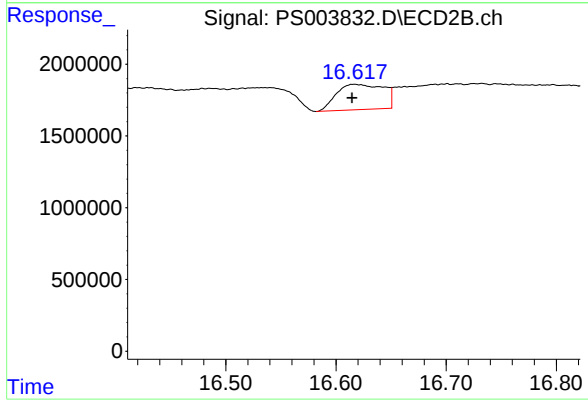

#16 DCPA

R.T.: 16.617 min
Delta R.T.: 0.003 min
Response: 5261774
Conc: 1.56 ng/ml