

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032919\
 Data File : PS003836.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Mar 2019 19:30
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 02:24:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.274	10.772	180.9E6	173.9E6	414.604	354.368
Target Compounds							
2) T	3,5-DICHL...	0.000	8.905	0	25543	N.D.	0.040 #
3) T	4-Nitroph...	0.000	9.910	0	262737	N.D.	1.157 #
6) T	MCP	0.000	11.280	0	59105	N.D.	0.050 #
7) T	MCPA	0.000	11.659	0	1362308	N.D.	0.764 #
8) T	DICHLORPROP	0.000	12.203	0	132496	N.D.	0.285 #
9) T	2,4-D	0.000	12.654	0	131881	N.D.	0.248 #
10) T	Pentachlo...	0.000	13.189	0	1302587	N.D.	0.188 #
11) T	2,4,5-TP ...	0.000	13.804	0	51138	N.D.	0.019 #
12) T	2,4,5-T	0.000	14.351	0	61381	N.D.	0.028 #
13) T	2,4-DB	0.000	15.088	0	171027	N.D.	0.576 #
14) T	DINOSEB	0.000	15.408	0	232935	N.D.	0.121 #
15) T	Picloram	0.000	16.646	0	409079	N.D.	0.129 #
16) T	DCPA	0.000	16.619	0	535829	N.D.	0.159 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032919\
Data File : PS003836.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Mar 2019 19:30
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 02:24:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

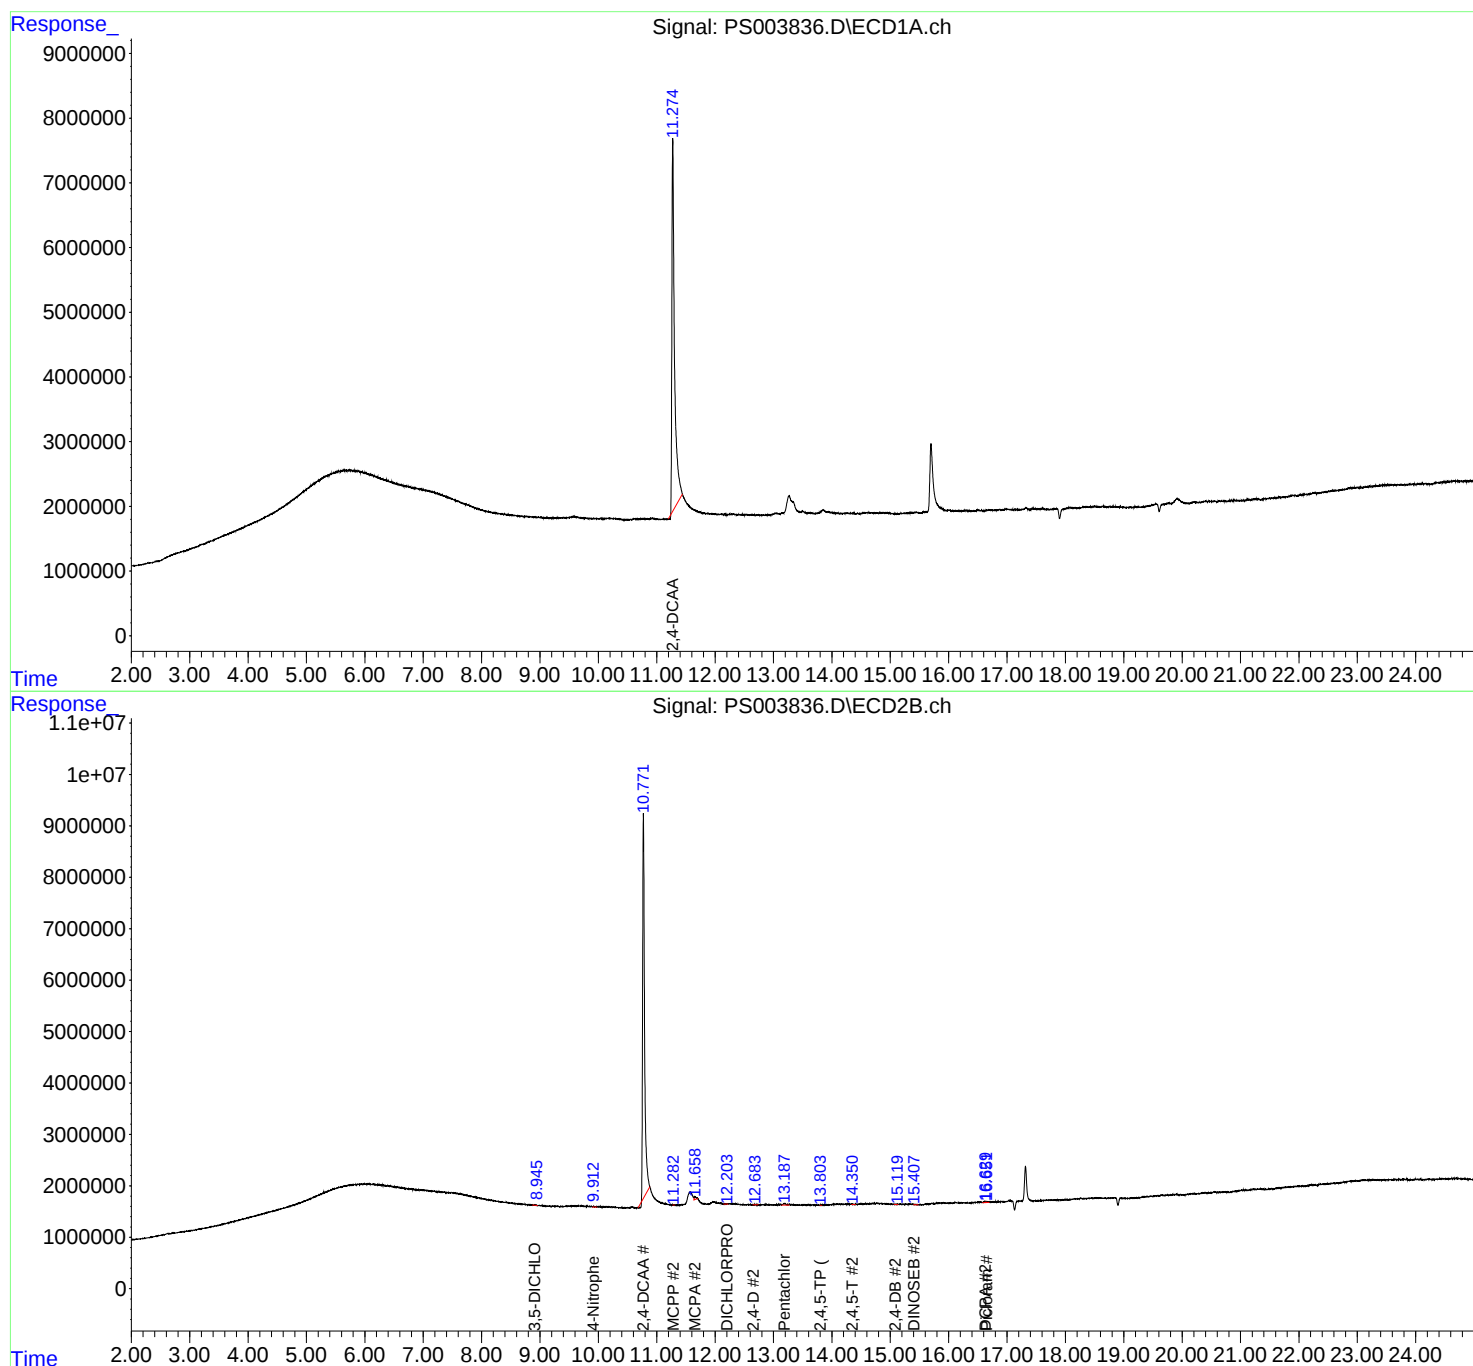


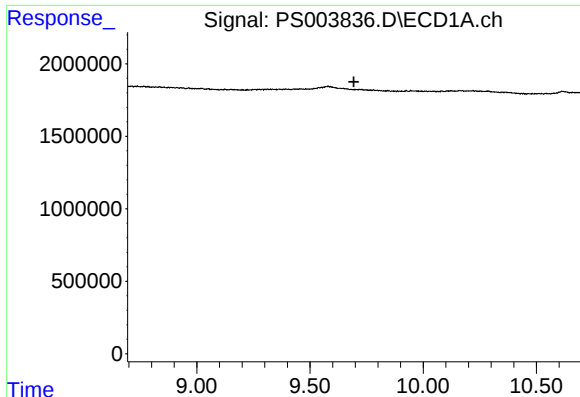

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.693 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

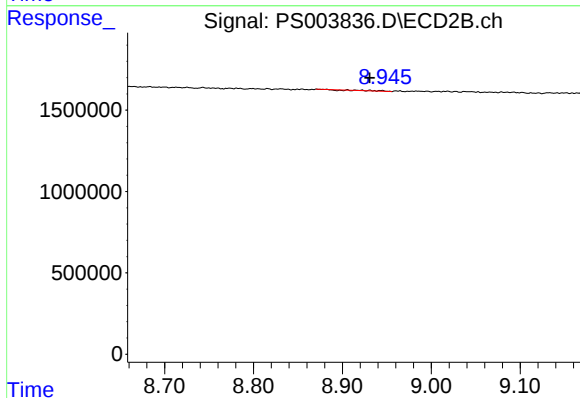


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.905 min
Delta R.T.: -0.026 min
Response: 25543
Conc: 0.04 ng/ml

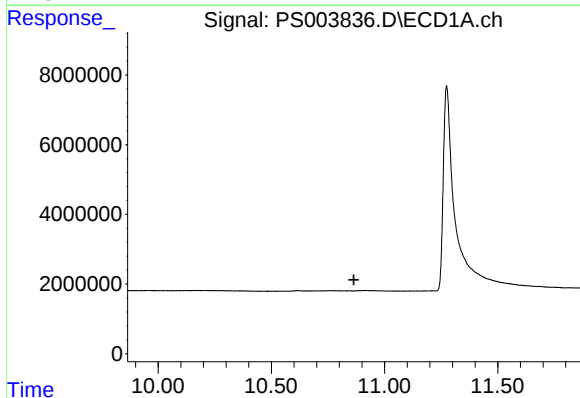


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

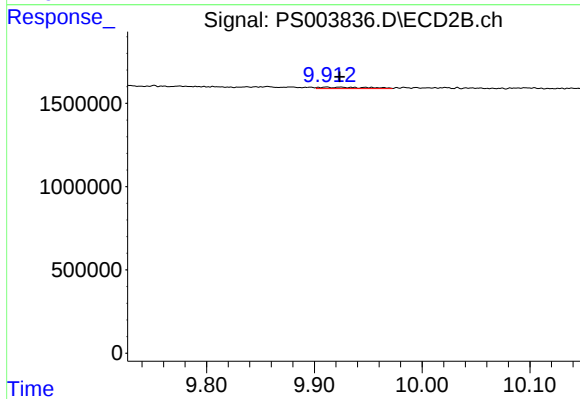

#3 4-Nitrophenol


R.T.: 9.910 min
Delta R.T.: -0.013 min
Response: 262737
Conc: 1.16 ng/ml

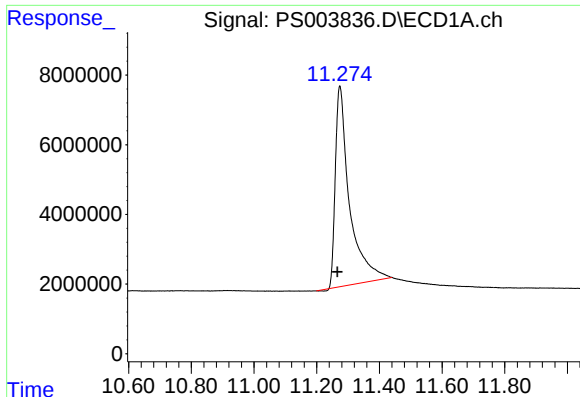

#4 2,4-DCAA


R.T.: 11.274 min
Delta R.T.: 0.007 min
Response: 180855467
Conc: 414.60 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

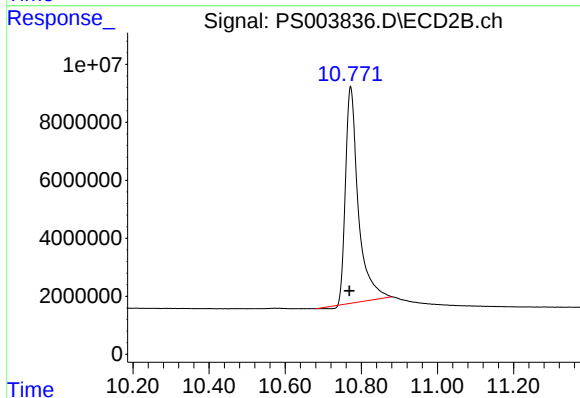


#4 2,4-DCAA

R.T.: 10.772 min
Delta R.T.: 0.003 min
Response: 173873504
Conc: 354.37 ng/ml

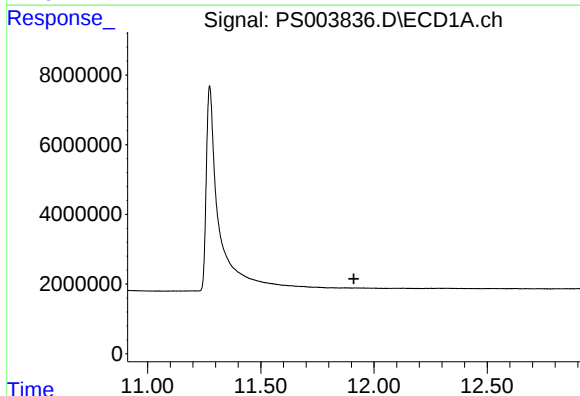


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.911 min
Response: 0
Conc: N.D.

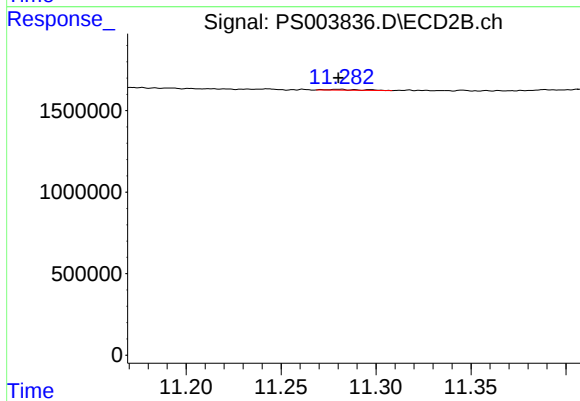

#6 MCP


R.T.: 11.280 min
Delta R.T.: 0.000 min
Response: 59105
Conc: 0.05 ug/ml

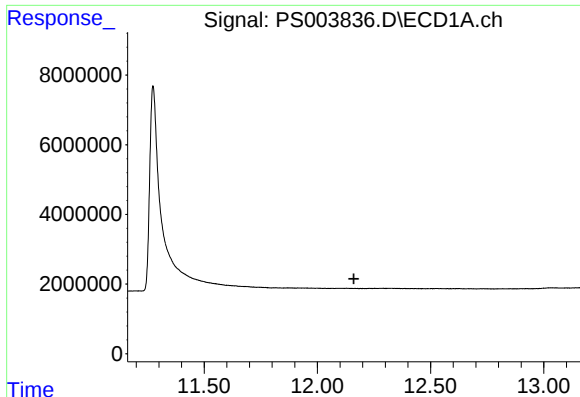

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.162 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

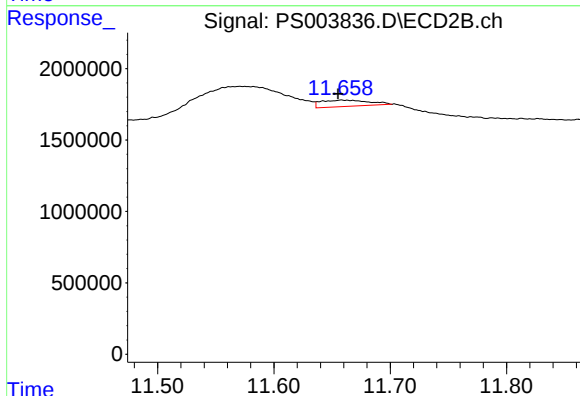


#7 MCPA

R.T.: 11.659 min
Delta R.T.: 0.004 min
Response: 1362308
Conc: 0.76 ug/ml

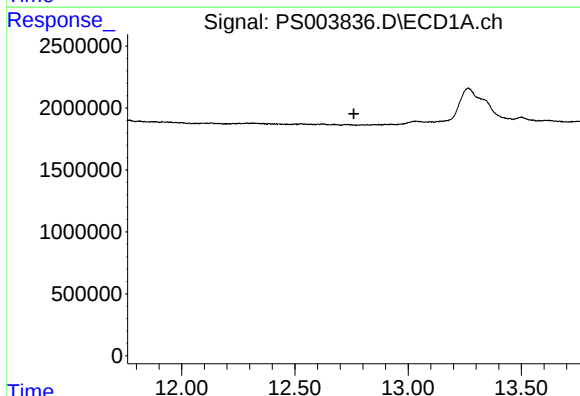


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.760 min
Response: 0
Conc: N.D.

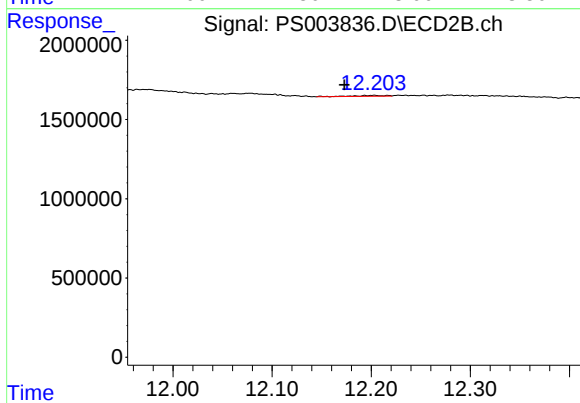

#8 DICHLORPROP


R.T.: 12.203 min
Delta R.T.: 0.030 min
Response: 132496
Conc: 0.28 ng/ml

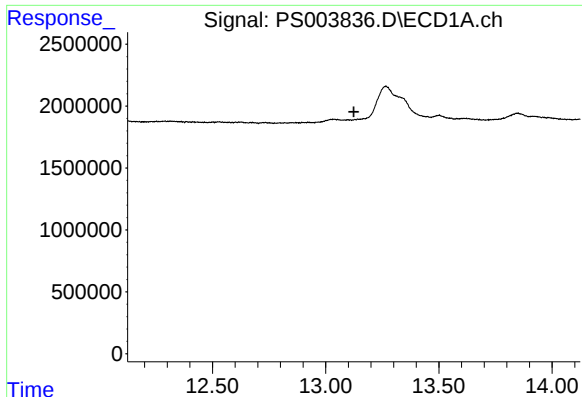

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

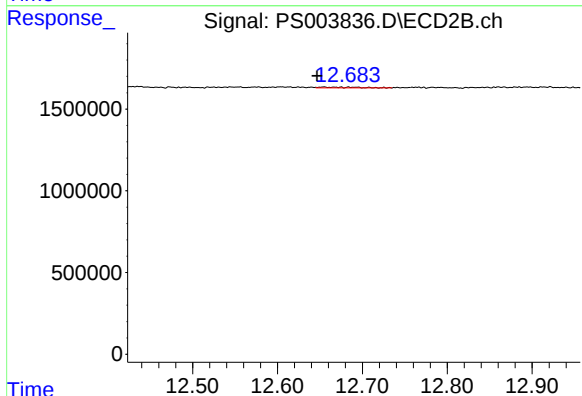


#9 2,4-D

R.T.: 12.654 min
Delta R.T.: 0.008 min
Response: 131881
Conc: 0.25 ng/ml

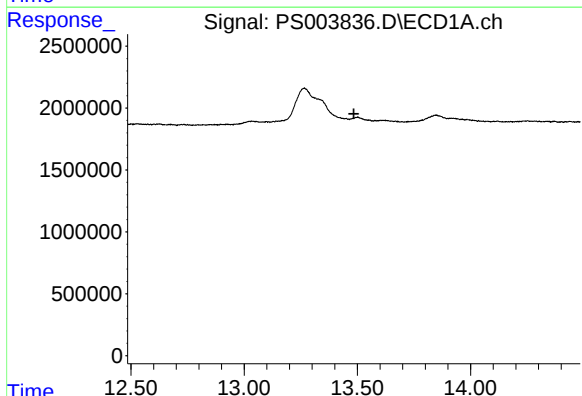


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.485 min
Response: 0
Conc: N.D.

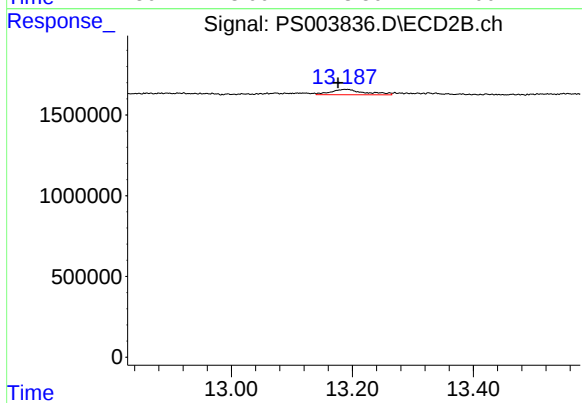

#10 Pentachlorophenol


R.T.: 13.189 min
Delta R.T.: 0.012 min
Response: 1302587
Conc: 0.19 ng/ml

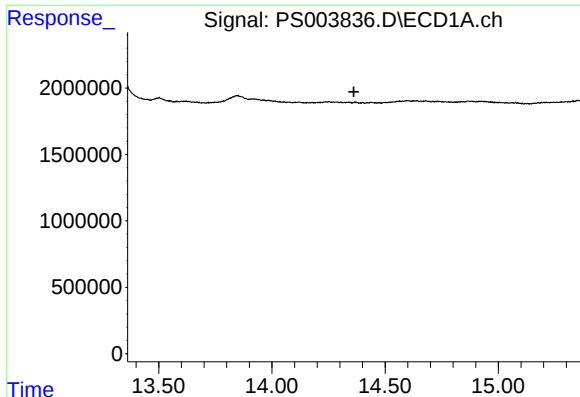

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

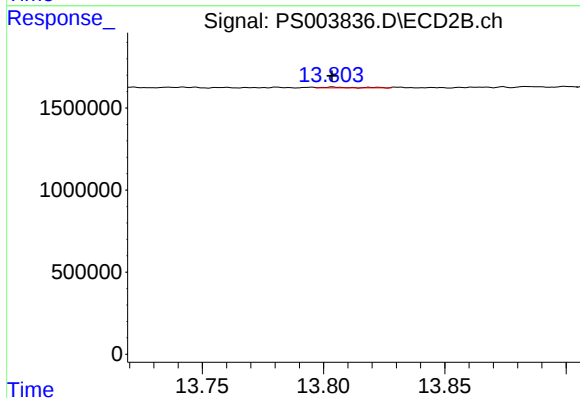


#11 2,4,5-TP (SILVEX)

R.T.: 13.804 min
Delta R.T.: 0.000 min
Response: 51138
Conc: 0.02 ng/ml

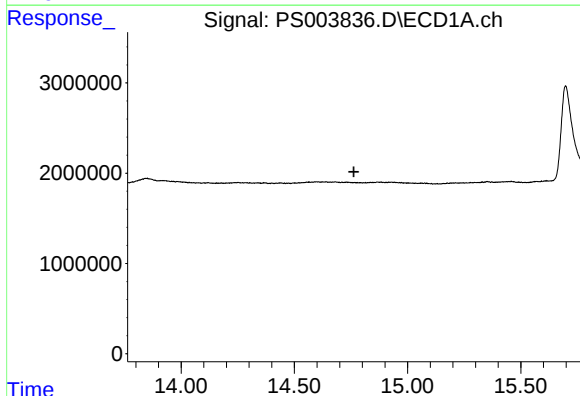


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.763 min
Response: 0
Conc: N.D.

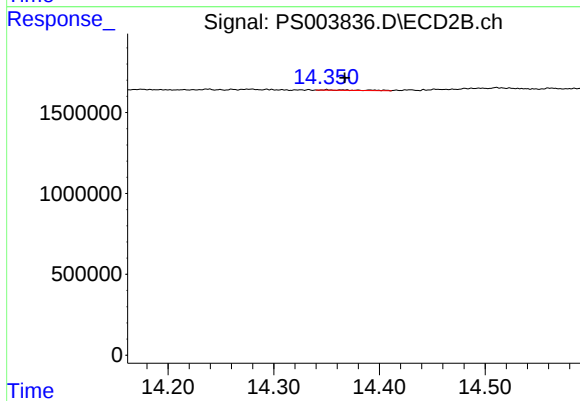

#12 2,4,5-T


R.T.: 14.351 min
Delta R.T.: -0.017 min
Response: 61381
Conc: 0.03 ng/ml

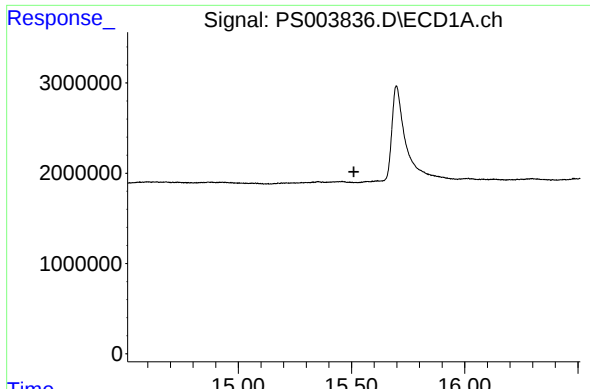

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

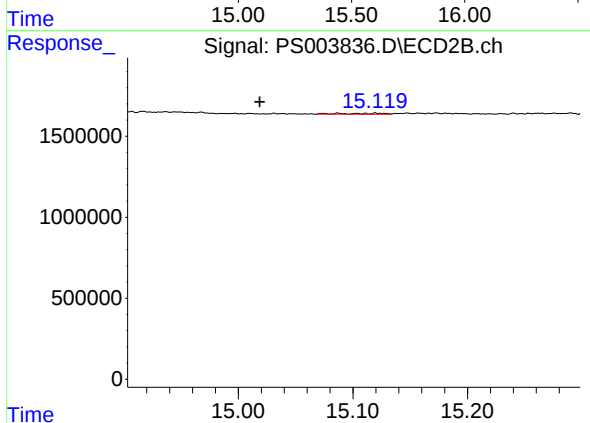


#13 2,4-DB

R.T.: 15.088 min
Delta R.T.: 0.069 min
Response: 171027
Conc: 0.58 ng/ml

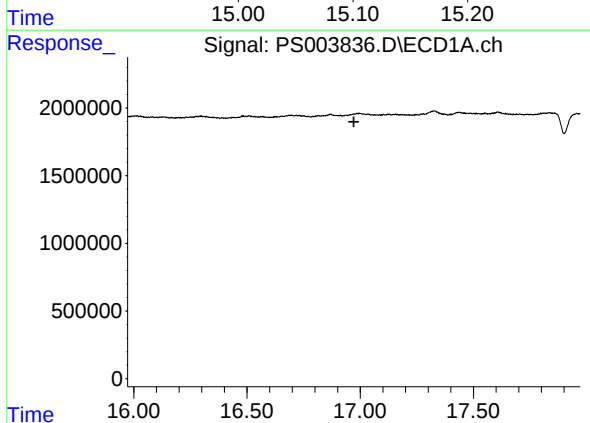


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.972 min
Response: 0
Conc: N.D.

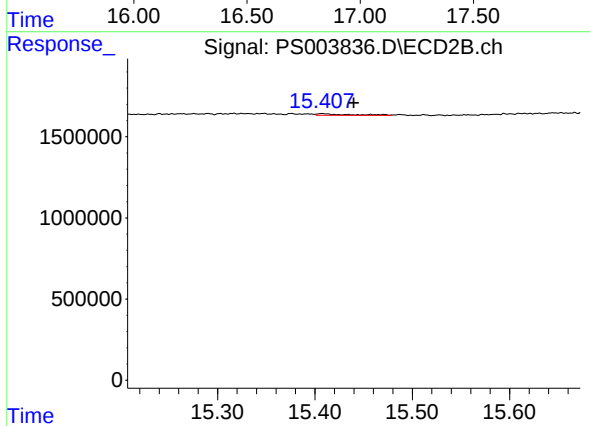

#14 DINOSEB


R.T.: 15.408 min
Delta R.T.: -0.032 min
Response: 232935
Conc: 0.12 ng/ml

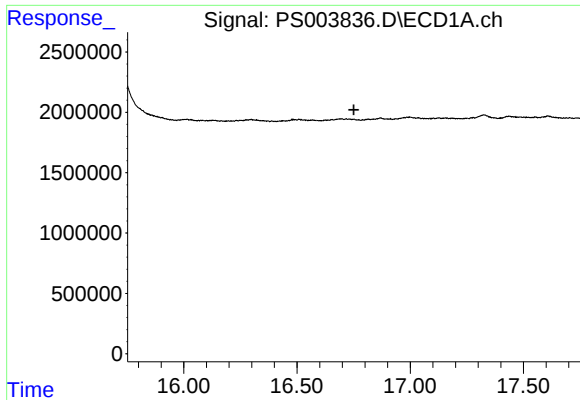

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.752 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

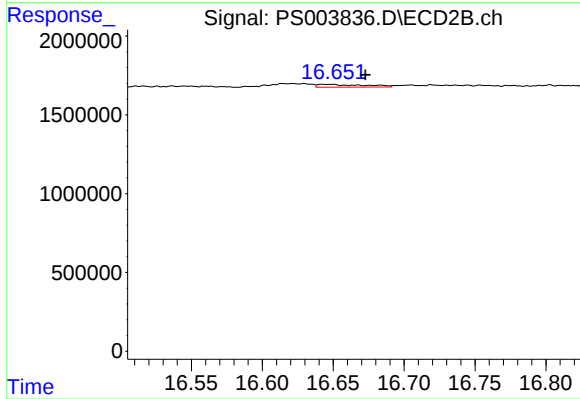


#15 Picloram

R.T.: 16.646 min
Delta R.T.: -0.026 min
Response: 409079
Conc: 0.13 ng/ml

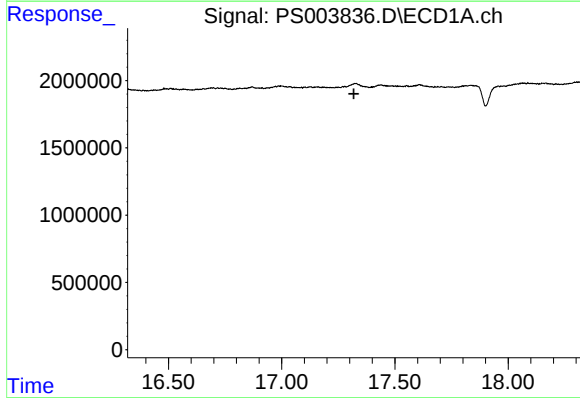

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.319 min
Response: 0
Conc: N.D.

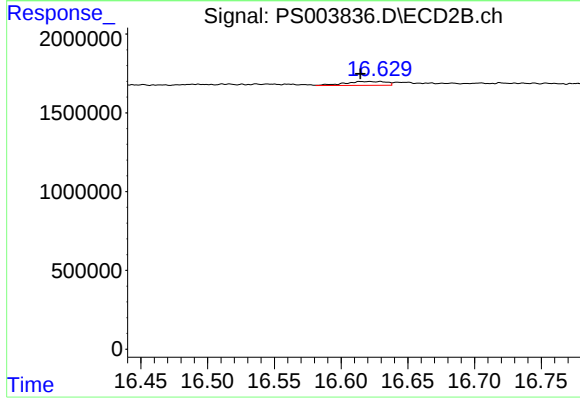

#16 DCPA

R.T.: 16.619 min
Delta R.T.: 0.005 min
Response: 535829
Conc: 0.16 ng/ml