

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032919\
 Data File : PS003838.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Mar 2019 20:32
 Operator : EI\SJ
 Sample : PB118306BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB118306BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 02:25:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.262	10.752	321.0E6	315.7E6	735.867	643.345
Target Compounds							
1) T	Dalapon	2.781	2.260	41496772	75451834	55.660	103.411 #
2) T	3,5-DICHL...	0.000	8.918	0	1174960	N.D.	1.842 #
3) T	4-Nitroph...	0.000	9.927	0	19116663	N.D.	84.201 #
7) T	MCPA	12.216	11.673	7115374	942238	3.373	0.528 #
9) T	2,4-D	0.000	12.611	0	3923957	N.D.	7.377 #
10) T	Pentachlo...	0.000	13.163	0	1042275	N.D.	0.151 #
11) T	2,4,5-TP ...	0.000	13.760	0	4068475	N.D.	1.536 #
12) T	2,4,5-T	0.000	14.427	0	15348852	N.D.	7.061 #
13) T	2,4-DB	0.000	14.999	0	14385943	N.D.	48.446 #
14) T	DINOSEB	0.000	15.428	0	2057930	N.D.	1.073 #
15) T	Picloram	0.000	16.724	0	36517301	N.D.	11.515 #
16) T	DCPA	0.000	16.609	0	9465010	N.D.	2.800 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032919\
Data File : PS003838.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Mar 2019 20:32
Operator : EI\SJ
Sample : PB118306BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB118306BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 02:25:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

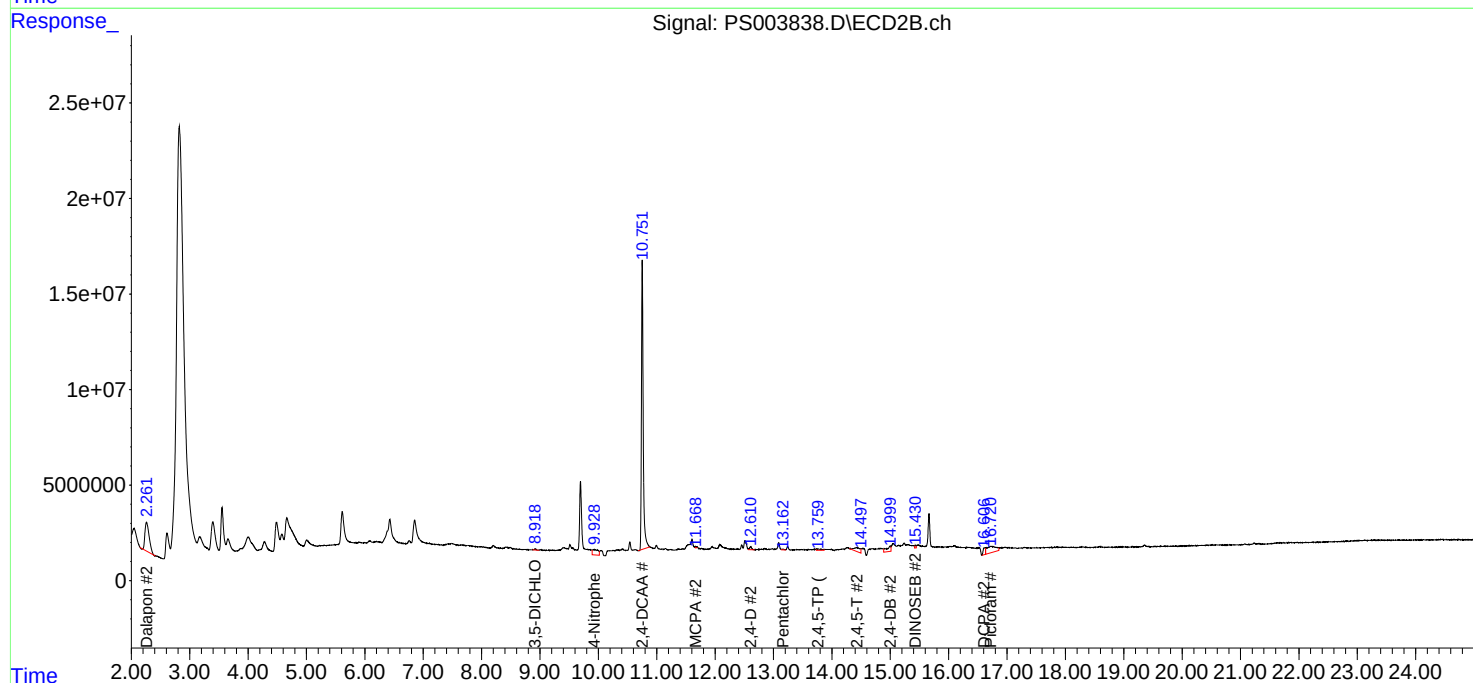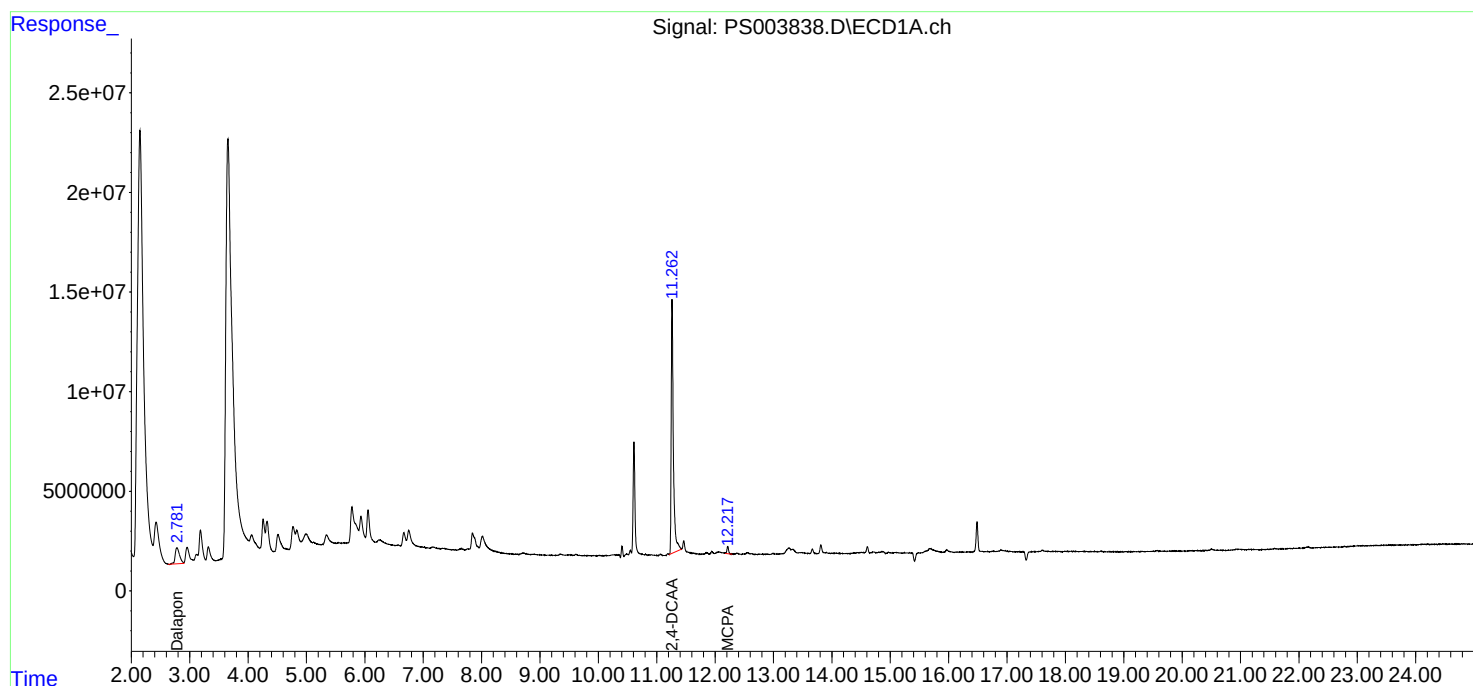


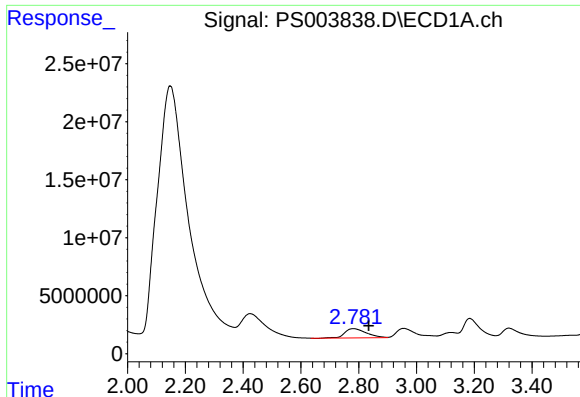

#1 Dalapon


R.T.: 2.781 min
Delta R.T.: -0.054 min
Response: 41496772
Conc: 55.66 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB118306BL

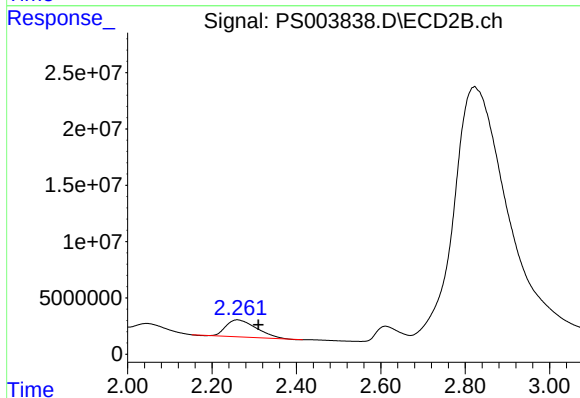


#1 Dalapon

R.T.: 2.260 min
Delta R.T.: -0.050 min
Response: 75451834
Conc: 103.41 ng/ml

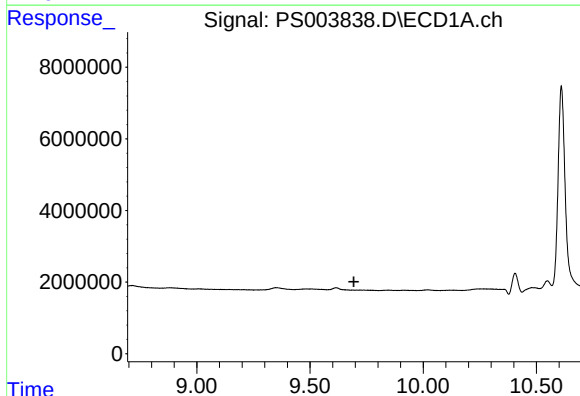


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

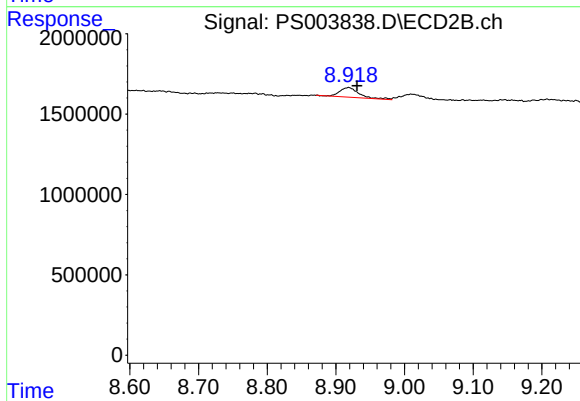

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.918 min
Delta R.T.: -0.013 min
Response: 1174960
Conc: 1.84 ng/ml

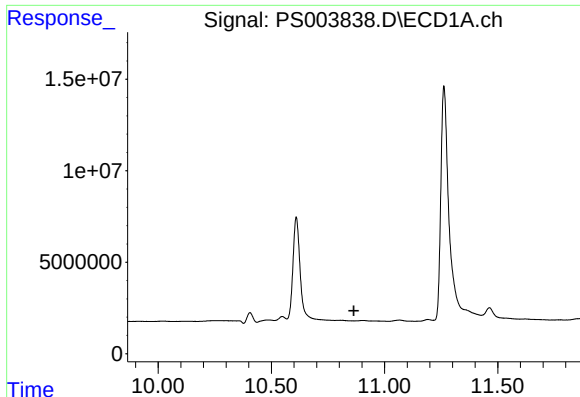

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB118306BL

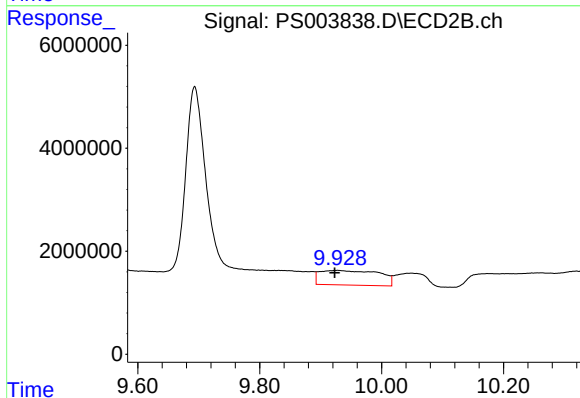


#3 4-Nitrophenol

R.T.: 9.927 min
Delta R.T.: 0.004 min
Response: 19116663
Conc: 84.20 ng/ml

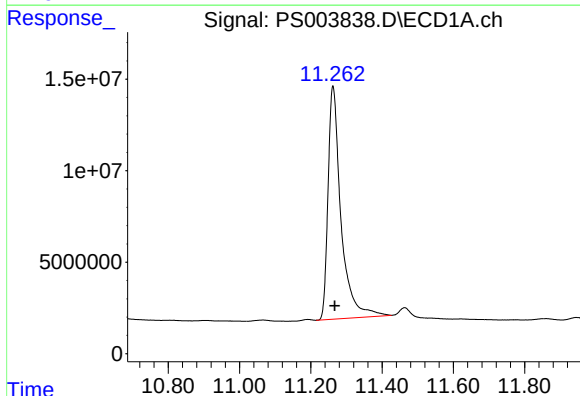


#4 2,4-DCAA

R.T.: 11.262 min
Delta R.T.: -0.004 min
Response: 320994072
Conc: 735.87 ng/ml

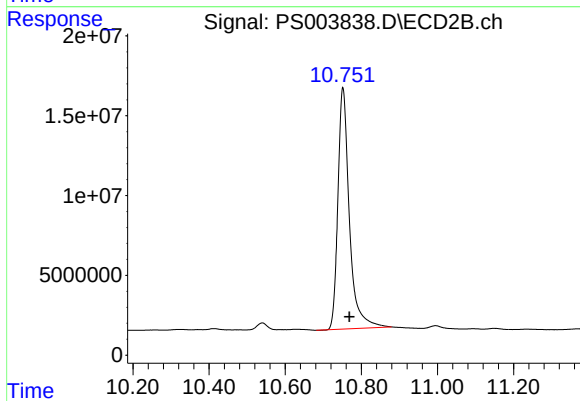

#4 2,4-DCAA


R.T.: 10.752 min
Delta R.T.: -0.017 min
Response: 315662566
Conc: 643.34 ng/ml

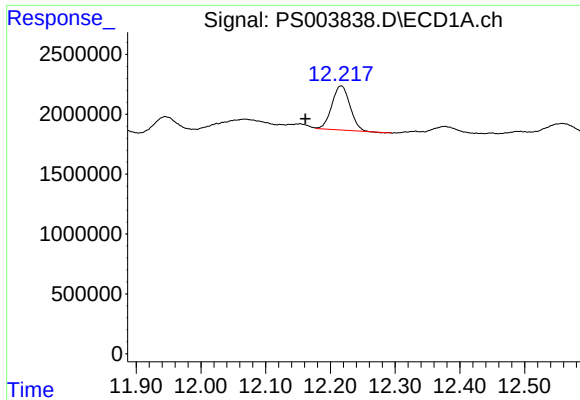

#7 MCPA


R.T.: 12.216 min
Delta R.T.: 0.055 min
Response: 7115374
Conc: 3.37 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB118306BL

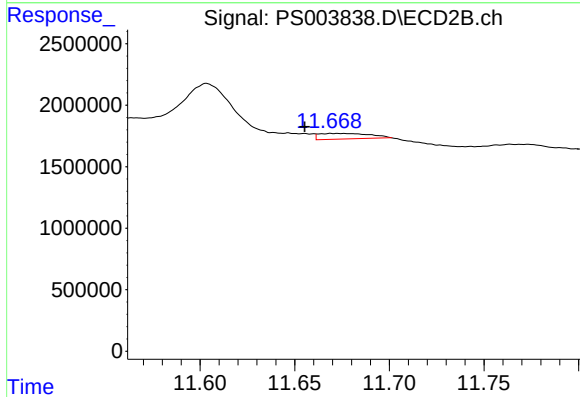


#7 MCPA

R.T.: 11.673 min
Delta R.T.: 0.018 min
Response: 942238
Conc: 0.53 ug/ml

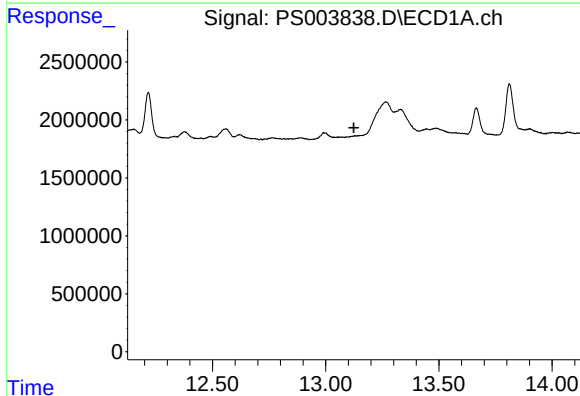


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.125 min
Response: 0
Conc: N.D.

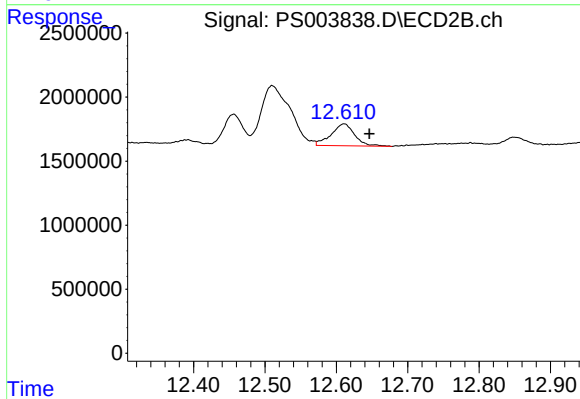

#9 2,4-D


R.T.: 12.611 min
Delta R.T.: -0.036 min
Response: 3923957
Conc: 7.38 ng/ml

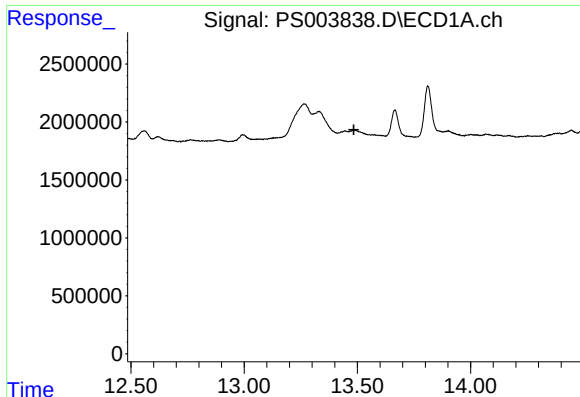

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.485 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB118306BL

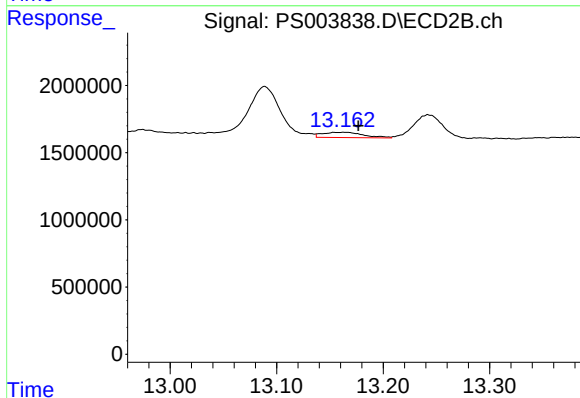


#10 Pentachlorophenol

R.T.: 13.163 min
Delta R.T.: -0.013 min
Response: 1042275
Conc: 0.15 ng/ml

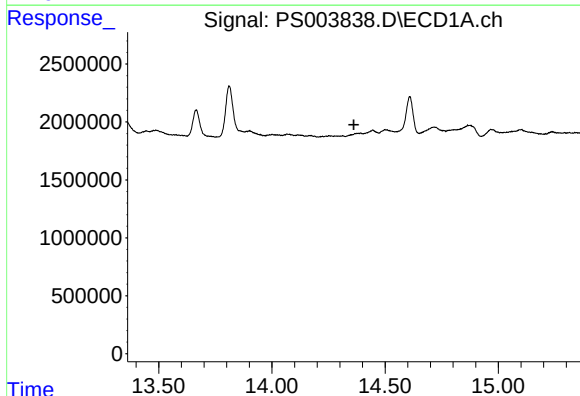


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

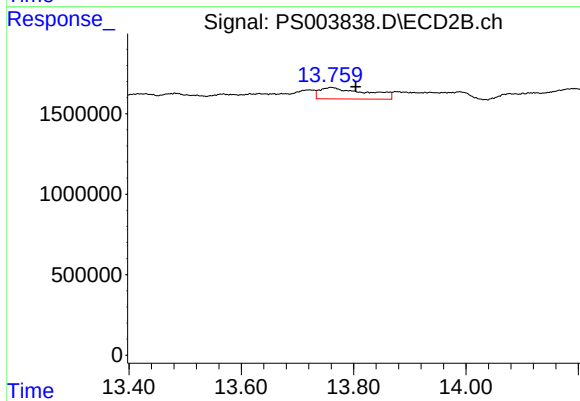

#11 2,4,5-TP (SILVEX)


R.T.: 13.760 min
Delta R.T.: -0.043 min
Response: 4068475
Conc: 1.54 ng/ml

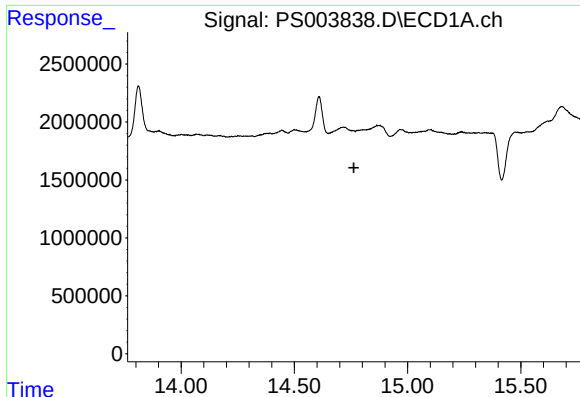

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.763 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB118306BL

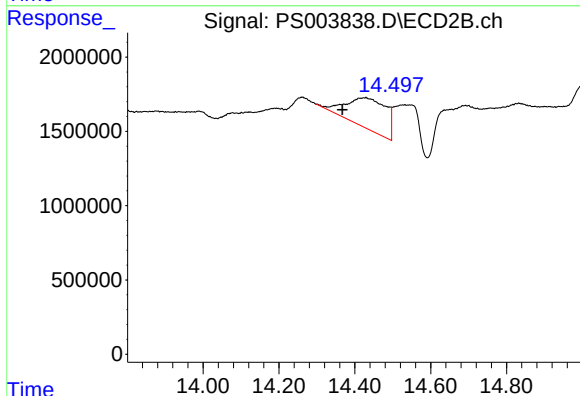


#12 2,4,5-T

R.T.: 14.427 min
Delta R.T.: 0.060 min
Response: 15348852
Conc: 7.06 ng/ml

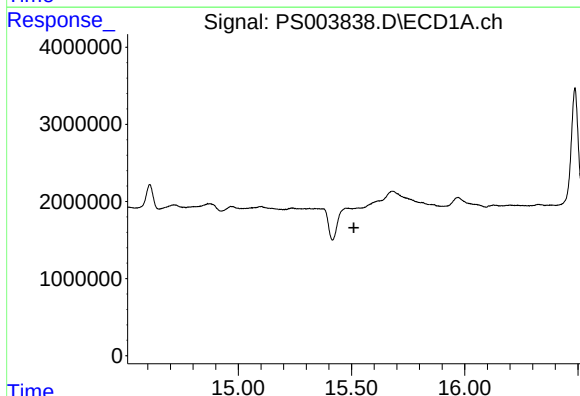


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 15.510 min
Response: 0
Conc: N.D.

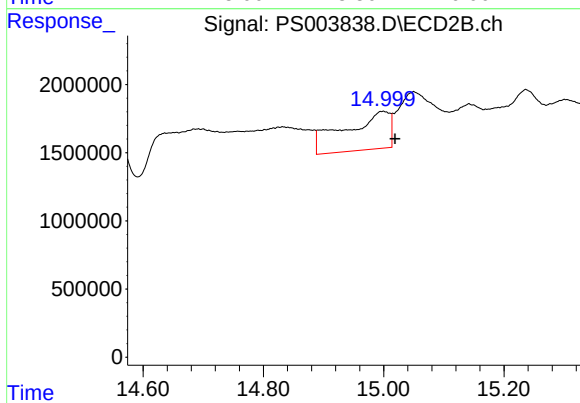

#13 2,4-DB


R.T.: 14.999 min
Delta R.T.: -0.020 min
Response: 14385943
Conc: 48.45 ng/ml

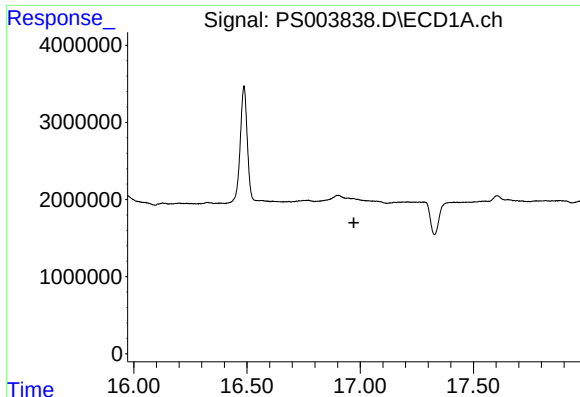

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 16.972 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB118306BL

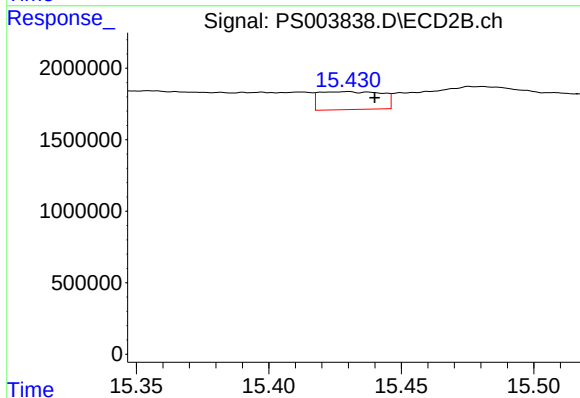


#14 DINOSEB

R.T.: 15.428 min
Delta R.T.: -0.012 min
Response: 2057930
Conc: 1.07 ng/ml

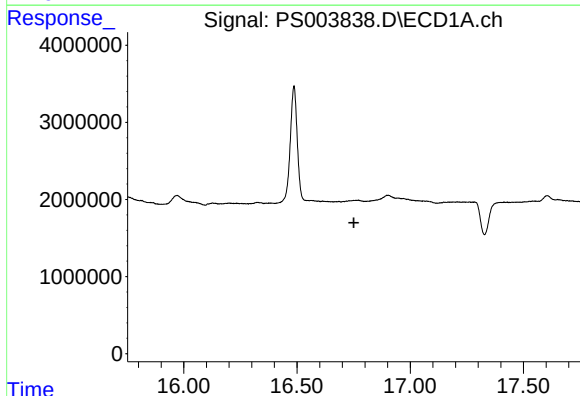


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.752 min
Response: 0
Conc: N.D.

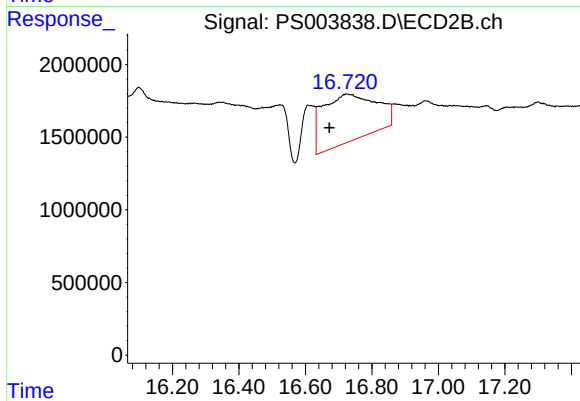

#15 Picloram


R.T.: 16.724 min
Delta R.T.: 0.051 min
Response: 36517301
Conc: 11.52 ng/ml

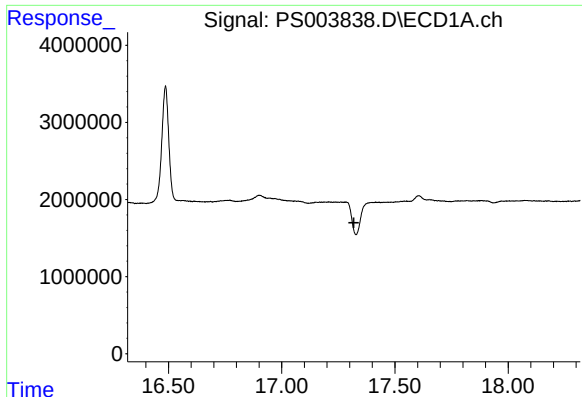

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB118306BL

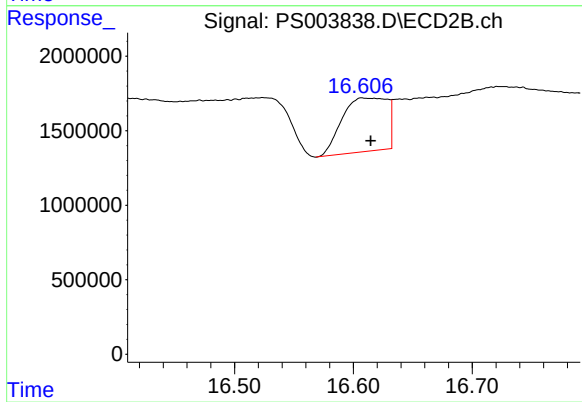

#16 DCPA

R.T.: 16.609 min
Delta R.T.: -0.005 min
Response: 9465010
Conc: 2.80 ng/ml