

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032919\
 Data File : PS003848.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2019 01:45
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 02:28:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.287	10.788	206.9E6	190.6E6	474.236	388.551
Target Compounds							
2) T	3,5-DICHL...	0.000	8.948	0	122783	N.D.	0.192 #
3) T	4-Nitroph...	0.000	9.975	0	250407	N.D.	1.103 #
6) T	MCP	0.000	11.269	0	7389	N.D.	0.006 #
7) T	MCPA	0.000	11.677	0	612009	N.D.	0.343 #
8) T	DICHLORPROP	0.000	12.144	0	5796504	N.D.	12.451 #
9) T	2,4-D	0.000	12.636	0	84305	N.D.	0.158 #
10) T	Pentachlo...	0.000	13.197	0	1235350	N.D.	0.179 #
11) T	2,4,5-TP ...	0.000	13.865	0	3530679	N.D.	1.333 #
12) T	2,4,5-T	0.000	14.383	0	65655	N.D.	0.030 #
13) T	2,4-DB	0.000	15.063	0	1102993	N.D.	3.714 #
14) T	DINOSEB	0.000	15.424	0	311932	N.D.	0.163 #
15) T	Picloram	0.000	16.637	0	649045	N.D.	0.205 #
16) T	DCPA	0.000	16.637	0	649045	N.D.	0.192 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032919\
Data File : PS003848.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Mar 2019 01:45
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 02:28:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

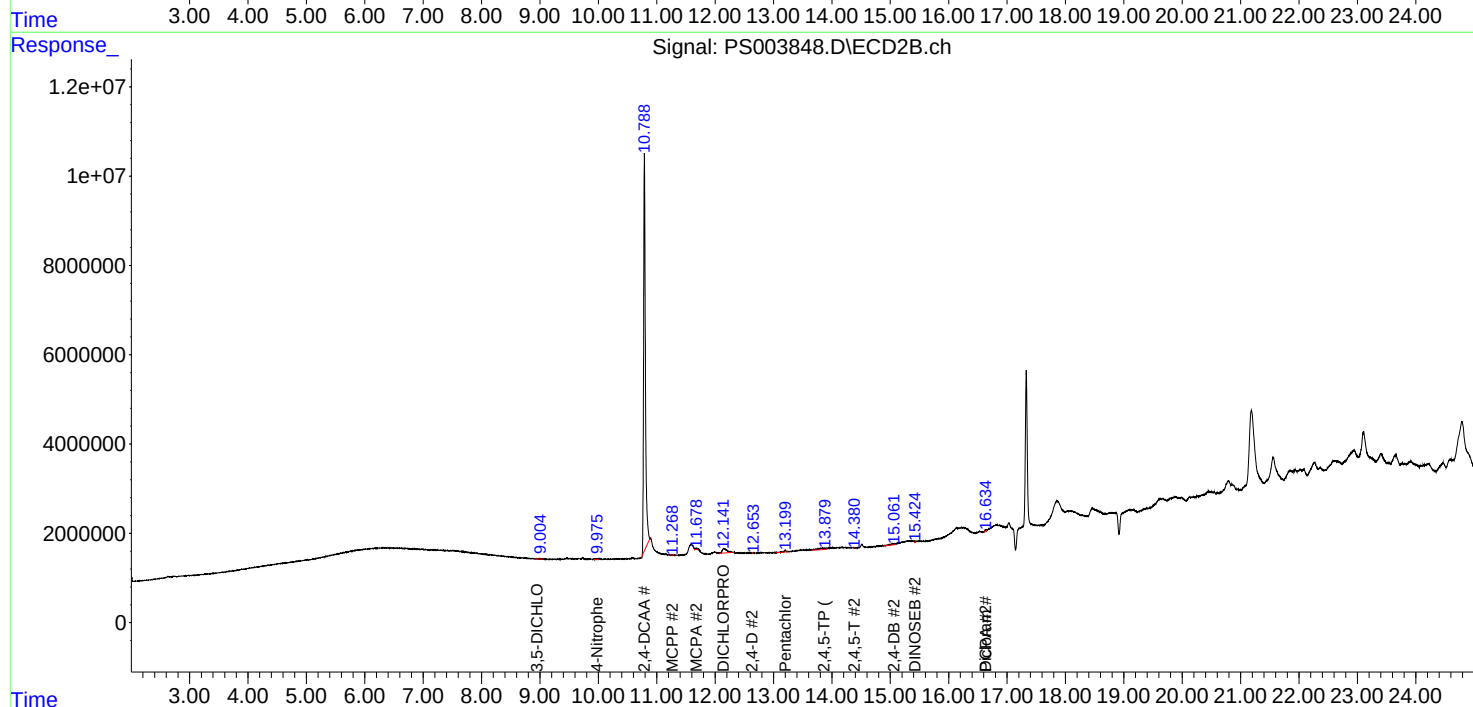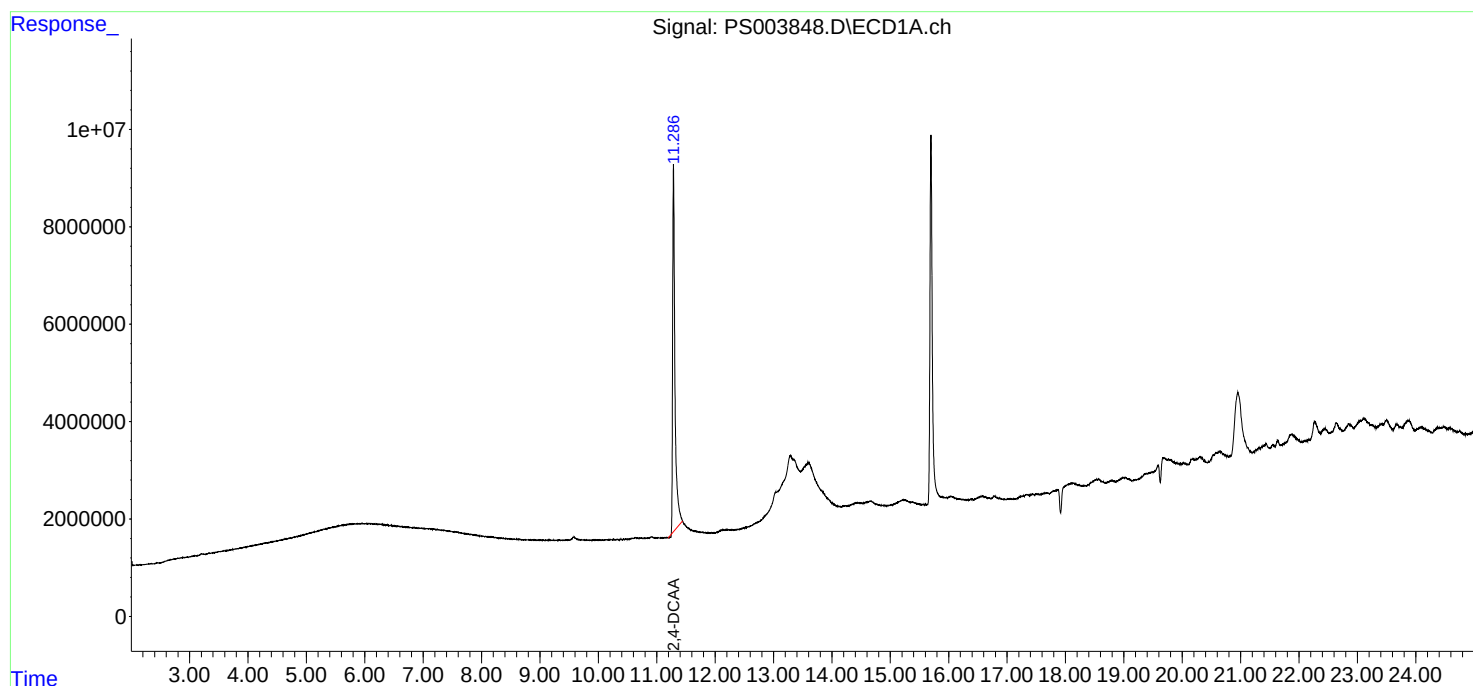


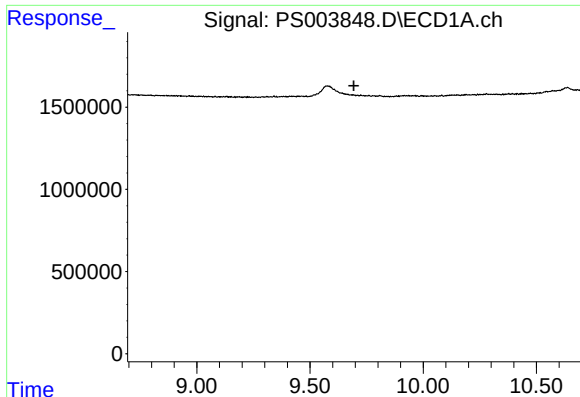

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.693 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

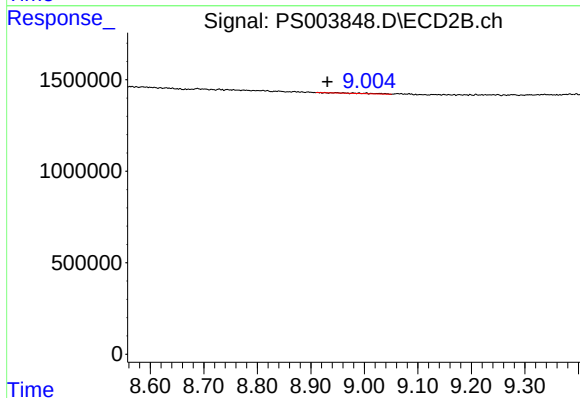


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.948 min
Delta R.T.: 0.017 min
Response: 122783
Conc: 0.19 ng/ml

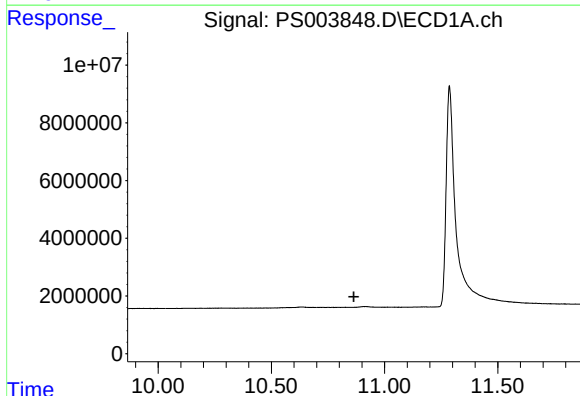


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

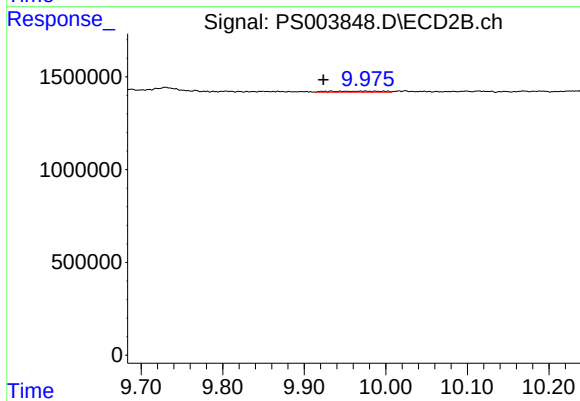

#3 4-Nitrophenol


R.T.: 9.975 min
Delta R.T.: 0.052 min
Response: 250407
Conc: 1.10 ng/ml

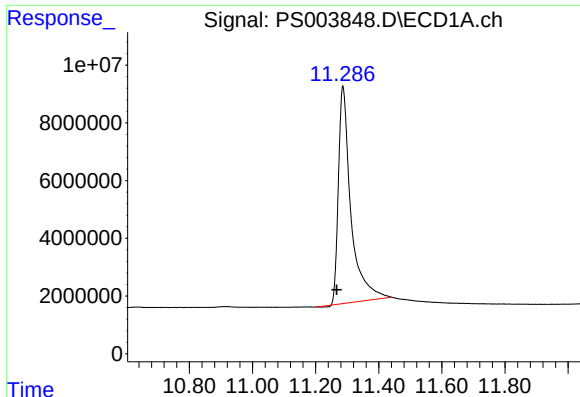

#4 2,4-DCAA


R.T.: 11.287 min
Delta R.T.: 0.020 min
Response: 206867787
Conc: 474.24 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

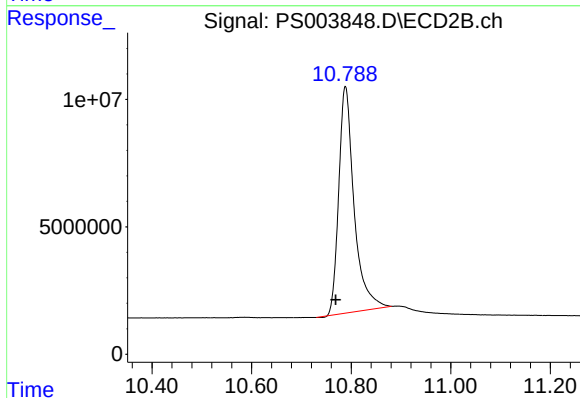


#4 2,4-DCAA

R.T.: 10.788 min
Delta R.T.: 0.020 min
Response: 190645855
Conc: 388.55 ng/ml

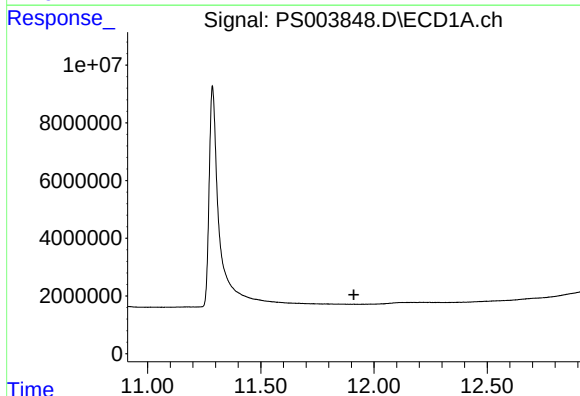


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.911 min
Response: 0
Conc: N.D.

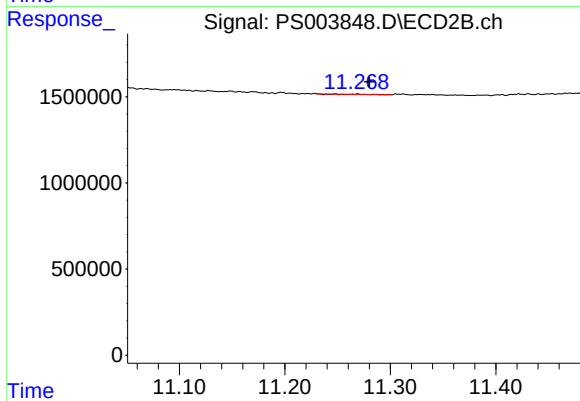

#6 MCP


R.T.: 11.269 min
Delta R.T.: -0.011 min
Response: 7389
Conc: 0.01 ug/ml

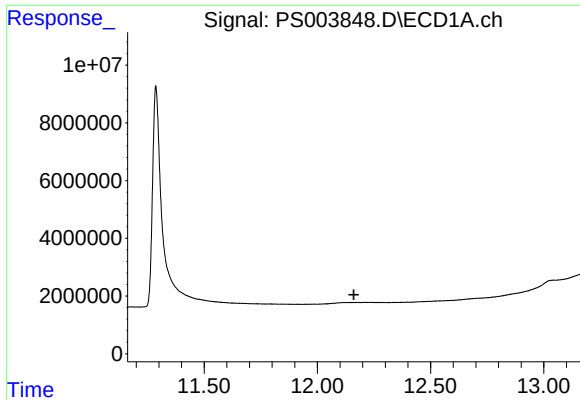

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.162 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

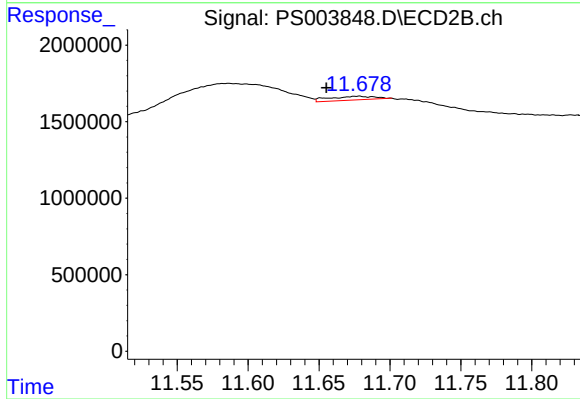


#7 MCPA

R.T.: 11.677 min
Delta R.T.: 0.022 min
Response: 612009
Conc: 0.34 ug/ml

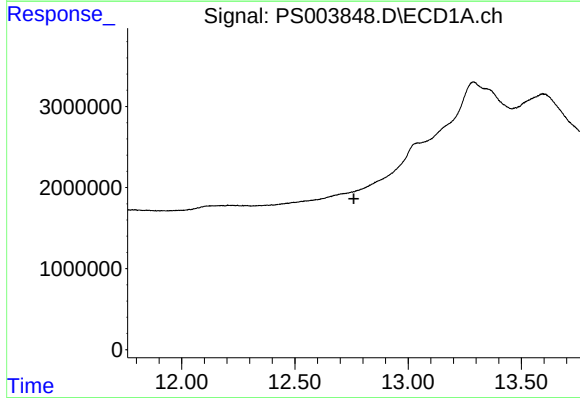


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.760 min
Response: 0
Conc: N.D.

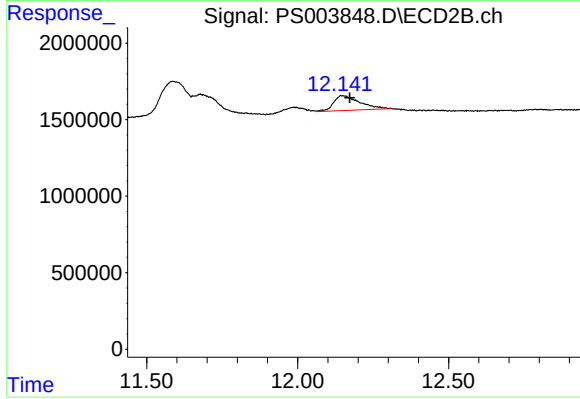

#8 DICHLORPROP


R.T.: 12.144 min
Delta R.T.: -0.028 min
Response: 5796504
Conc: 12.45 ng/ml

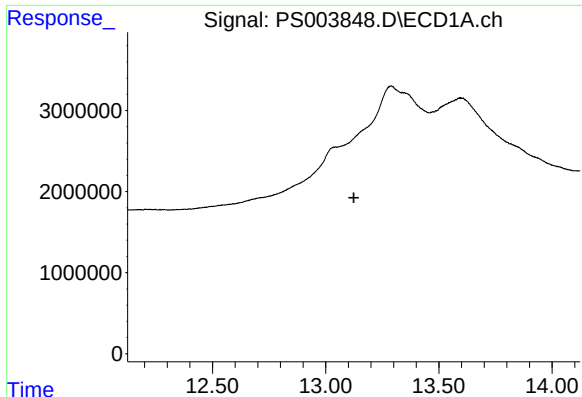

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

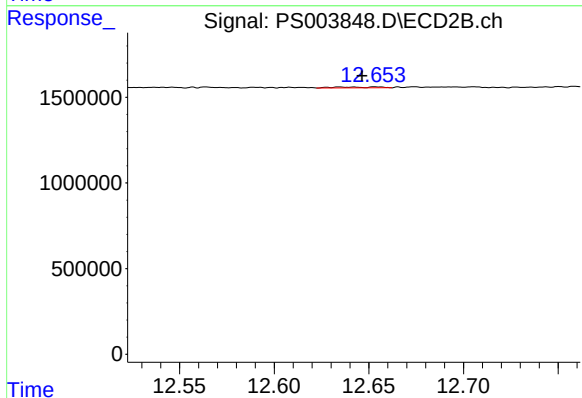


#9 2,4-D

R.T.: 12.636 min
Delta R.T.: -0.011 min
Response: 84305
Conc: 0.16 ng/ml

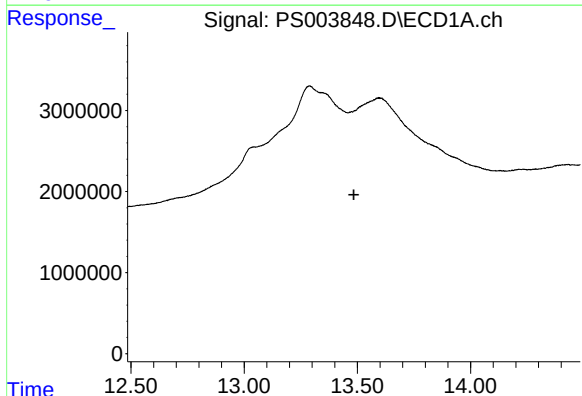


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.485 min
Response: 0
Conc: N.D.

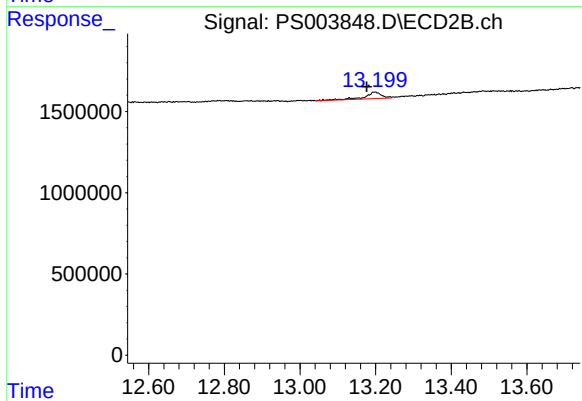

#10 Pentachlorophenol


R.T.: 13.197 min
Delta R.T.: 0.020 min
Response: 1235350
Conc: 0.18 ng/ml

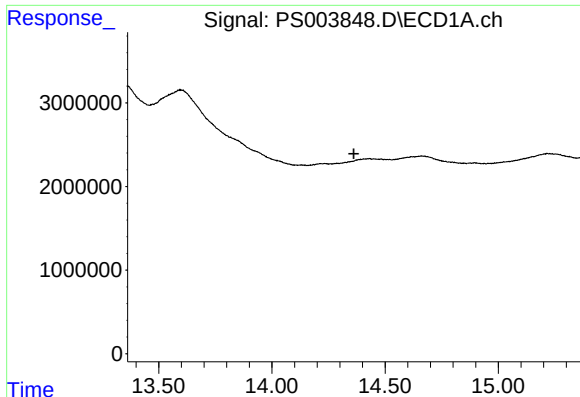

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

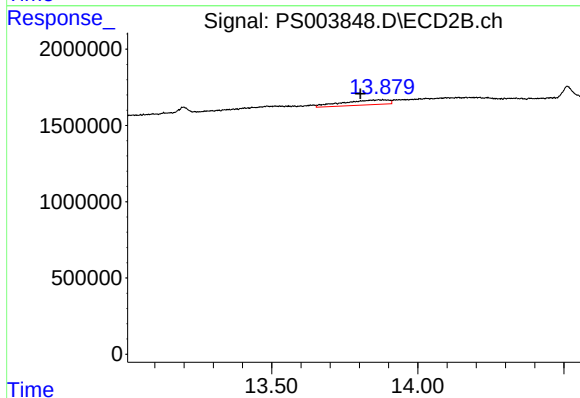


#11 2,4,5-TP (SILVEX)

R.T.: 13.865 min
Delta R.T.: 0.062 min
Response: 3530679
Conc: 1.33 ng/ml

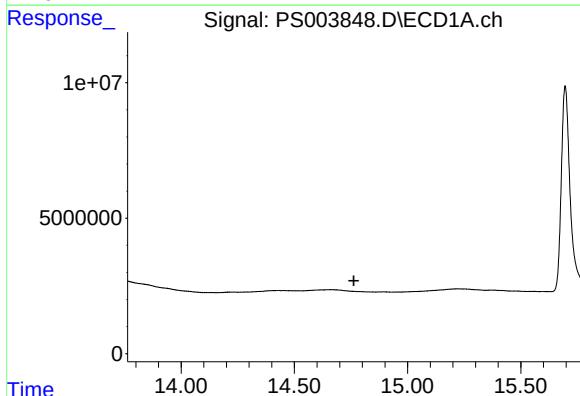


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.763 min
Response: 0
Conc: N.D.

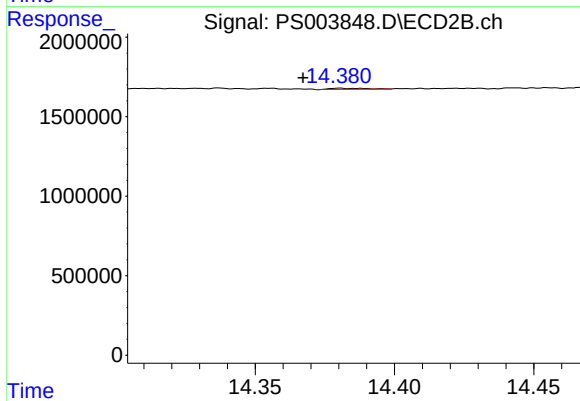

#12 2,4,5-T


R.T.: 14.383 min
Delta R.T.: 0.016 min
Response: 65655
Conc: 0.03 ng/ml

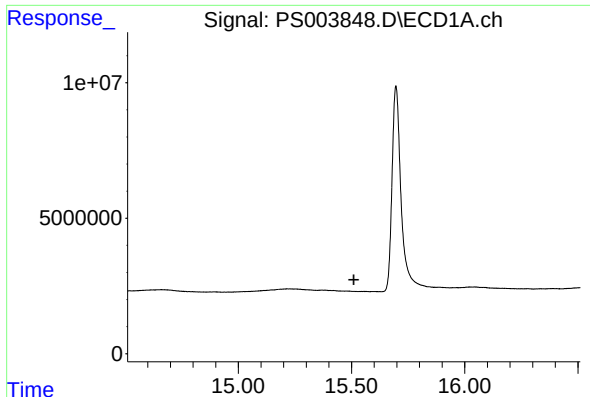

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

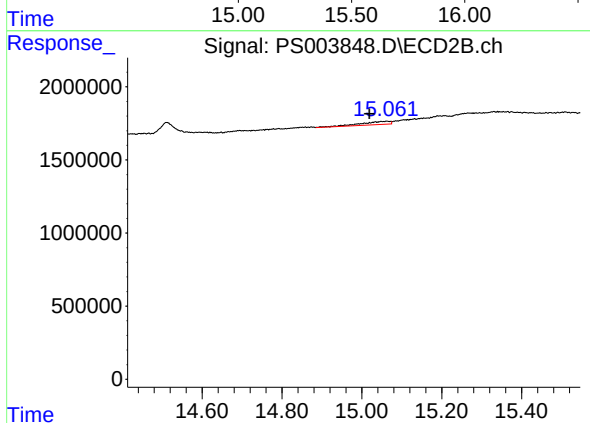


#13 2,4-DB

R.T.: 15.063 min
Delta R.T.: 0.044 min
Response: 1102993
Conc: 3.71 ng/ml

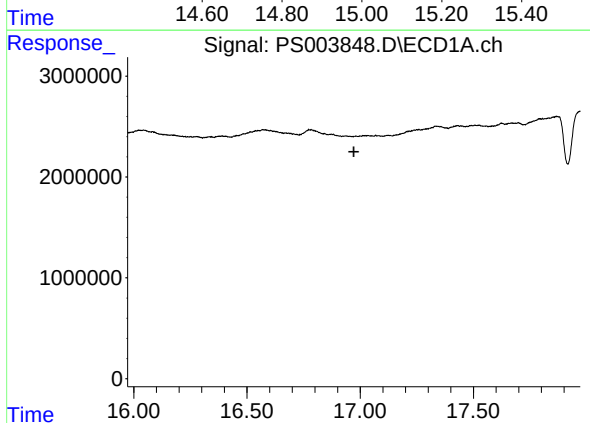


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.972 min
Response: 0
Conc: N.D.

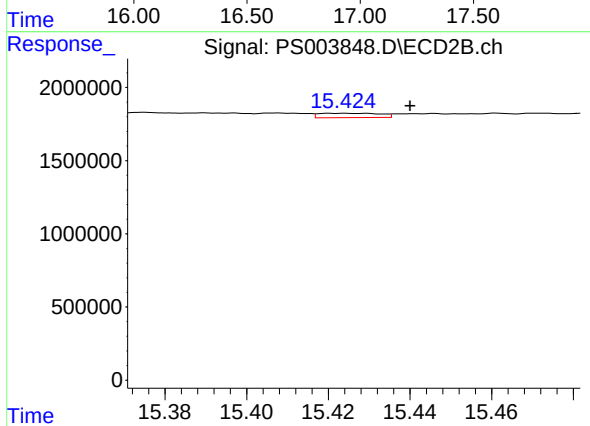

#14 DINOSEB


R.T.: 15.424 min
Delta R.T.: -0.016 min
Response: 311932
Conc: 0.16 ng/ml

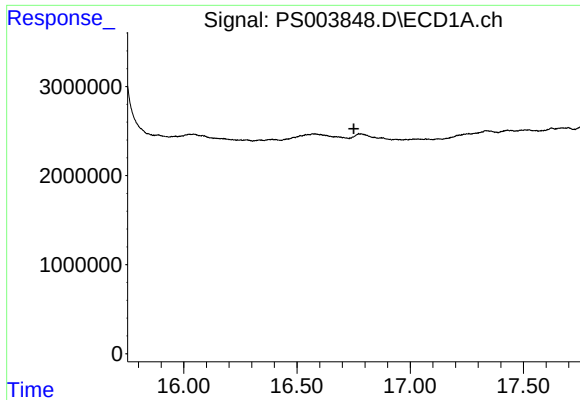

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.752 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

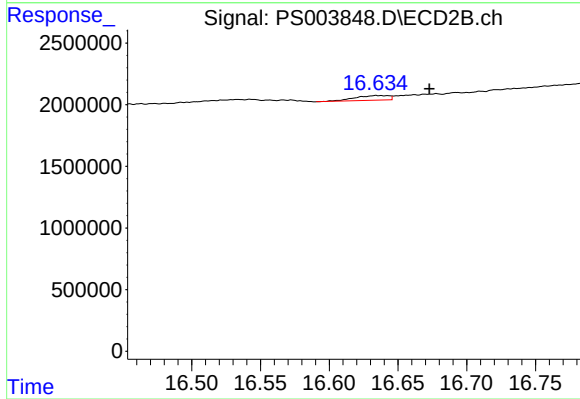


#15 Picloram

R.T.: 16.637 min
Delta R.T.: -0.036 min
Response: 649045
Conc: 0.20 ng/ml

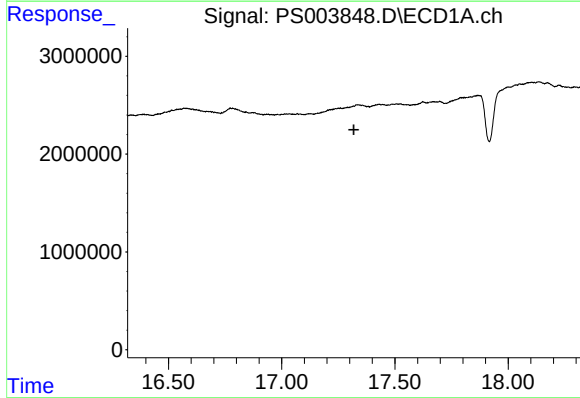

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

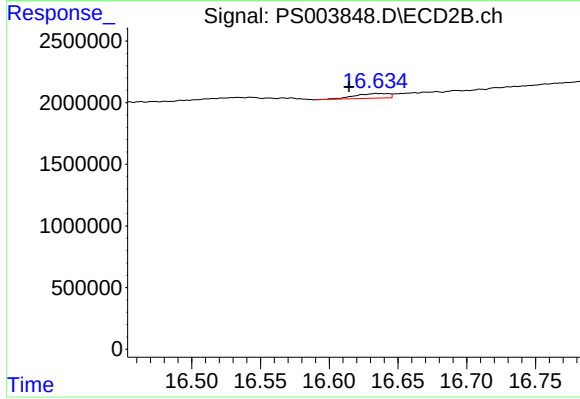

#16 DCPA

R.T.: 16.637 min
Delta R.T.: 0.022 min
Response: 649045
Conc: 0.19 ng/ml