

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032921\
 Data File : PS014397.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2021 03:28
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 06:20:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 18 02:23:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.165	6.890	621.4E6	249.6E6	434.886	529.081
Target Compounds							
5) T	DICAMBA	0.000	7.059	0	1610499	N.D.	<MDL
9) T	2,4-D	8.339f	0.000	3926765	0	2.664	N.D. #
10) T	Pentachlo...	8.582	8.408	4917662	2251456	<MDL	<MDL #
15) T	Picloram	0.000	10.906f	0	1940008	N.D.	<MDL
16) T	DCPA	11.371	10.906	3594991	1940008	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032921\
Data File : PS014397.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Mar 2021 03:28
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 06:20:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
Quant Title : 8080.M
QLast Update : Thu Mar 18 02:23:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

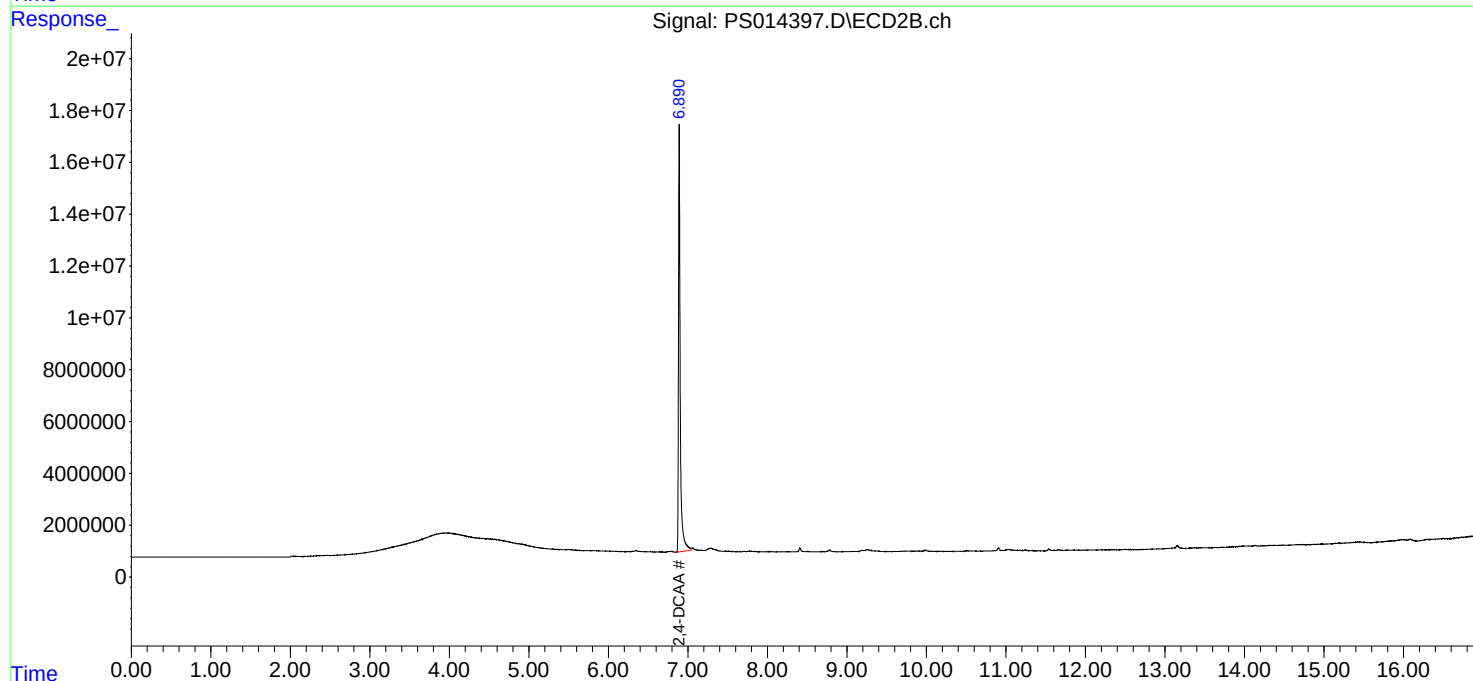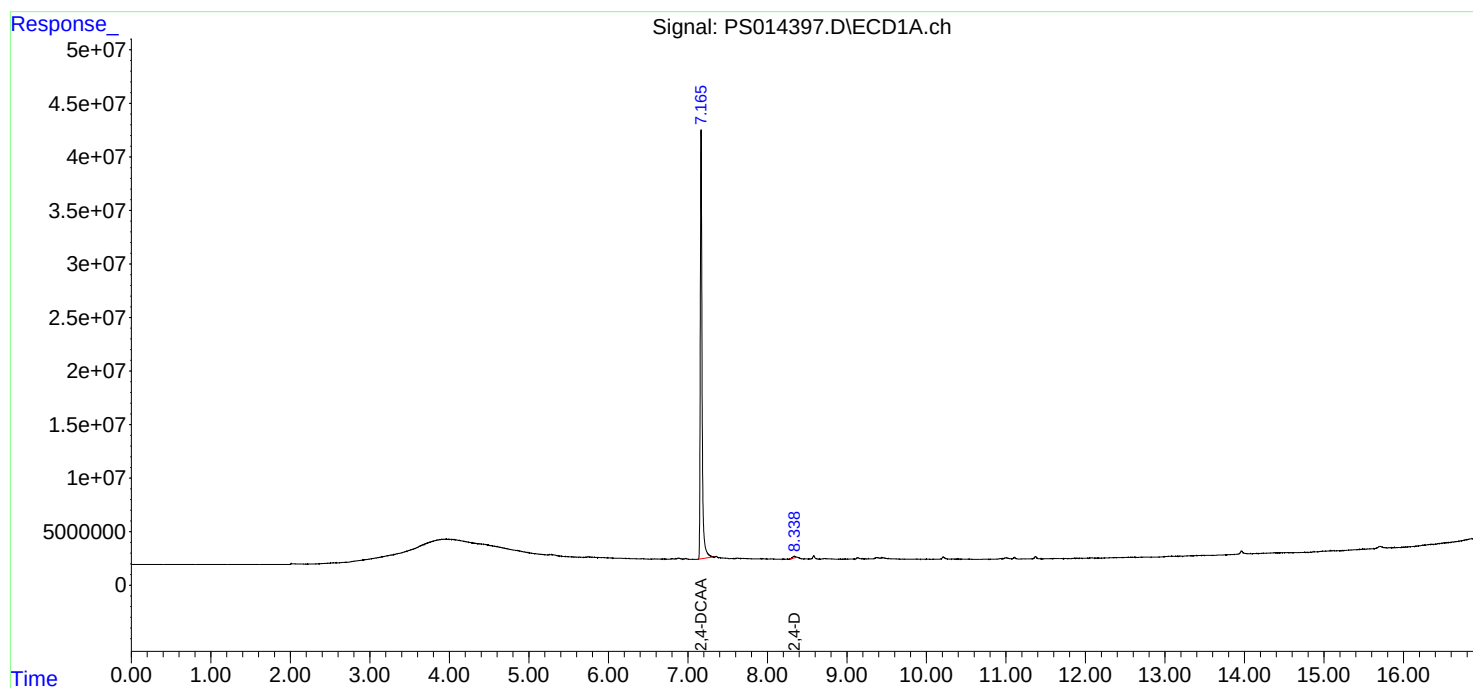


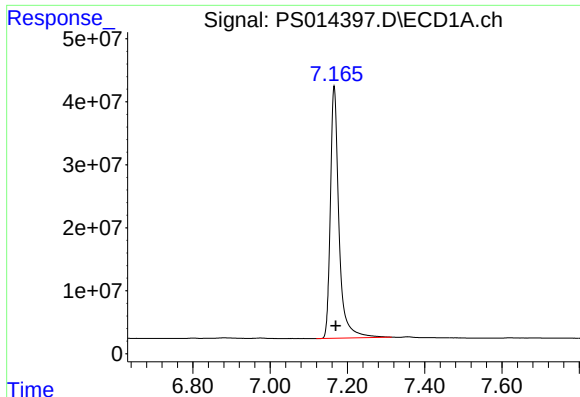

#4 2,4-DCAA


R.T.: 7.165 min
Delta R.T.: -0.005 min
Response: 621383032
Conc: 434.89 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

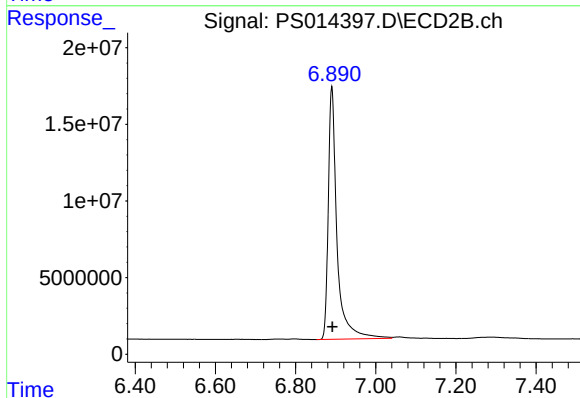


#4 2,4-DCAA

R.T.: 6.890 min
Delta R.T.: -0.002 min
Response: 249603816
Conc: 529.08 ng/ml

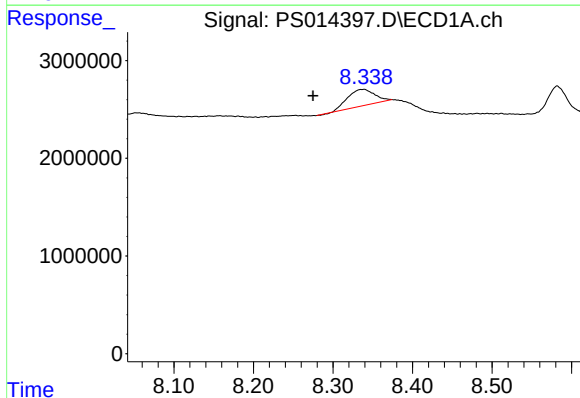

#9 2,4-D

R.T.: 8.339 min
Delta R.T.: 0.064 min
Response: 3926765
Conc: 2.66 ng/ml

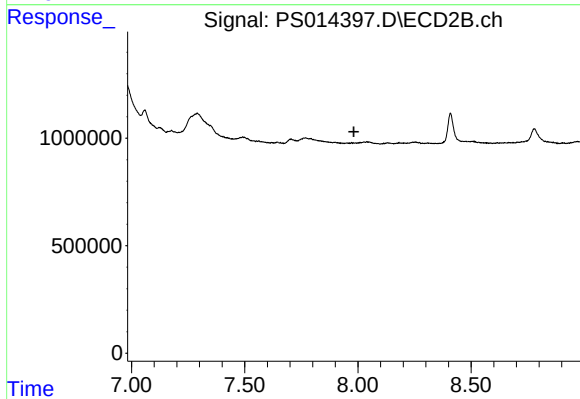

#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.982 min
Response: 0
Conc: N.D.