

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032922\
 Data File : PS018808.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Mar 2022 08:51
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 14:29:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	6.765f	0	9181889	N.D.	13.049
Target Compounds							
6) T	MCP	7.670f	0.000	6354916	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.619	0	3269342	N.D.	4.130
9) T	2,4-D	8.411f	0.000	6902070	0	2.060	N.D. #
11) T	2,4,5-TP ...	9.274f	8.639f	7539555	212.3E6	<MDL	48.660 #
12) T	2,4,5-T	9.502	9.067	4706431	12016529	<MDL	2.901 #
13) T	2,4-DB	10.036	9.609	4887977	3375828	1.787	5.946 #
14) T	DINOSEB	11.162f	9.841f	24902938	1815484	2.329	<MDL #
15) T	Picloram	11.027	10.876	335.4E6	22821728	16.317	4.293 #
16) T	DCPA	11.468	10.876f	63474982	22821728	3.548	4.339


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032922\
Data File : PS018808.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Mar 2022 08:51
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 14:29:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

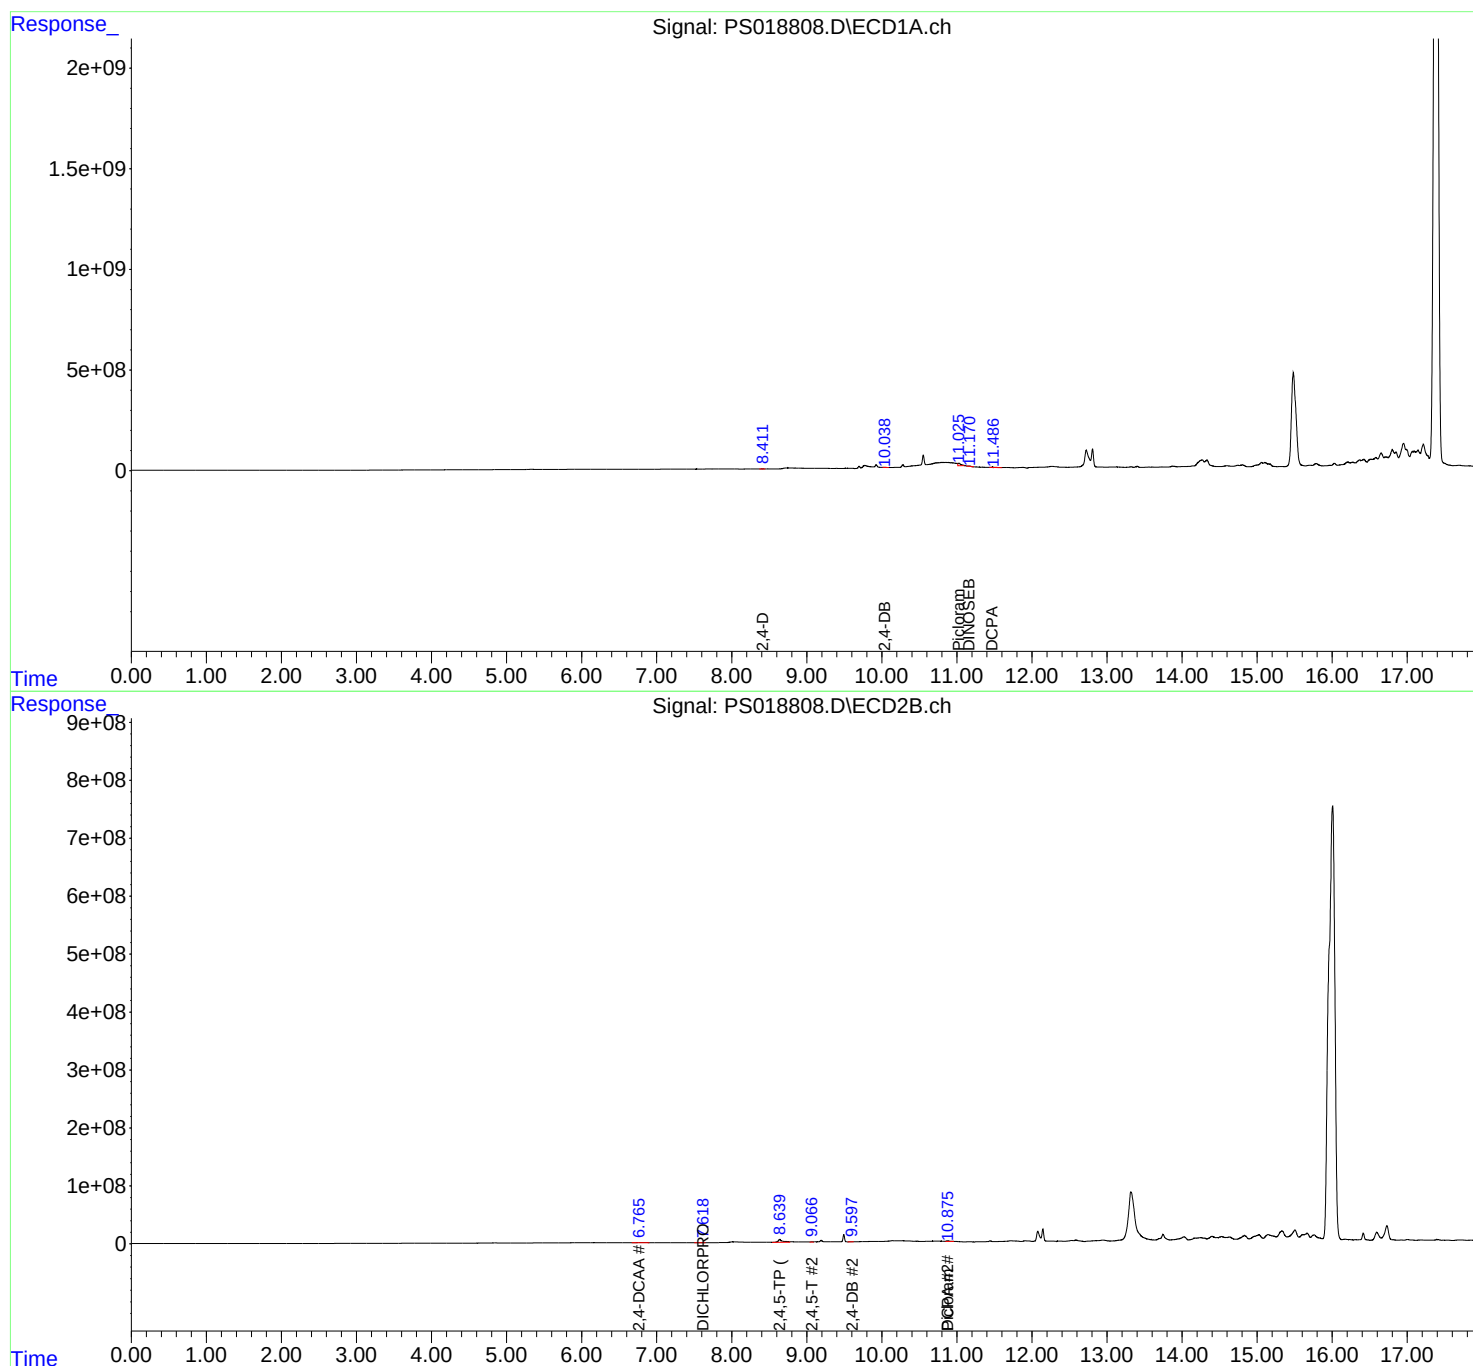


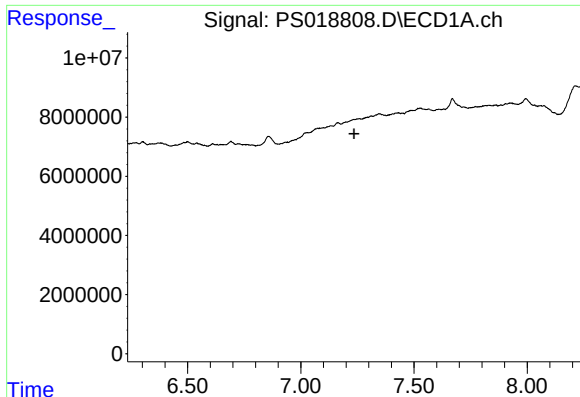

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.235 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

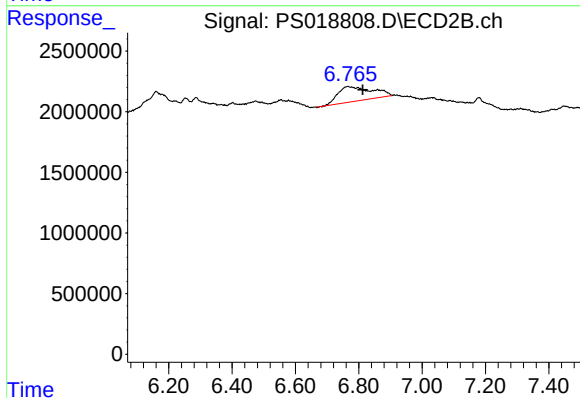


#4 2,4-DCAA

R.T.: 6.765 min
Delta R.T.: -0.048 min
Response: 9181889
Conc: 13.05 ng/ml

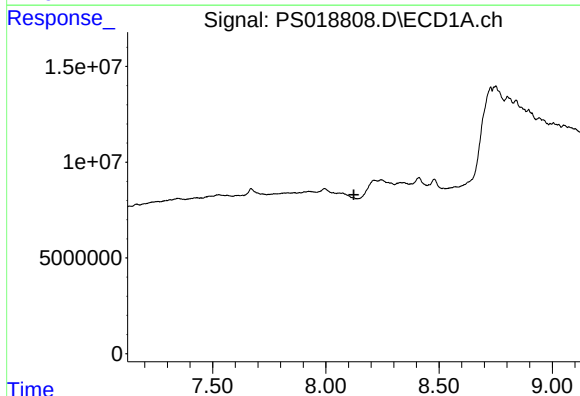


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.124 min
Response: 0
Conc: N.D.

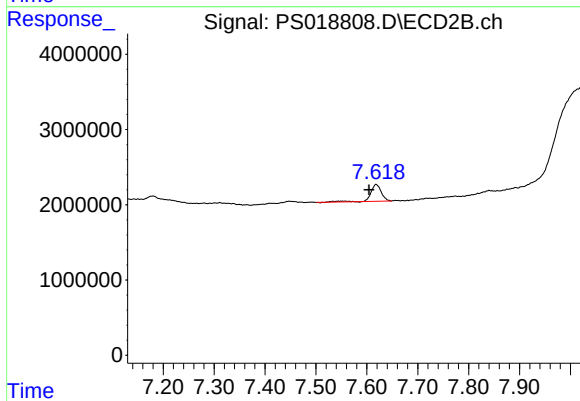

#8 DICHLORPROP


R.T.: 7.619 min
Delta R.T.: 0.014 min
Response: 3269342
Conc: 4.13 ng/ml

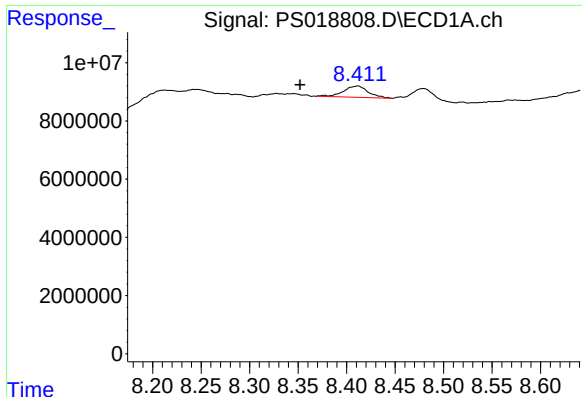

#9 2,4-D


R.T.: 8.411 min
Delta R.T.: 0.059 min
Response: 6902070
Conc: 2.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

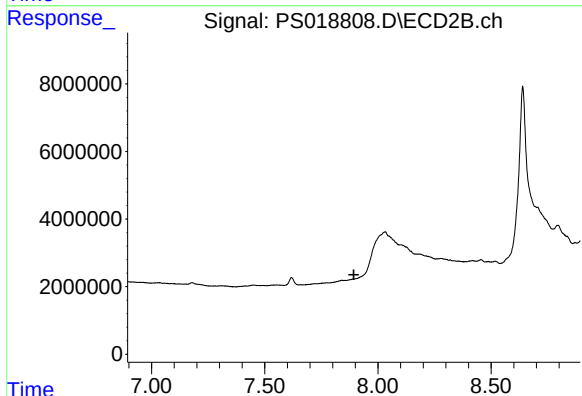


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.894 min
Response: 0
Conc: N.D.

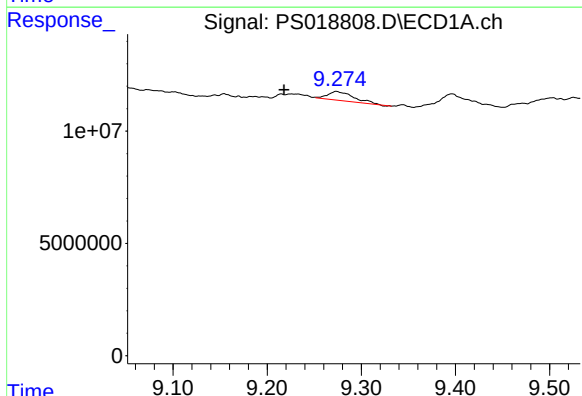


#11 2,4,5-TP (SILVEX)

R.T.: 9.274 min
Delta R.T.: 0.056 min
Response: 7539555
Conc: N.D.

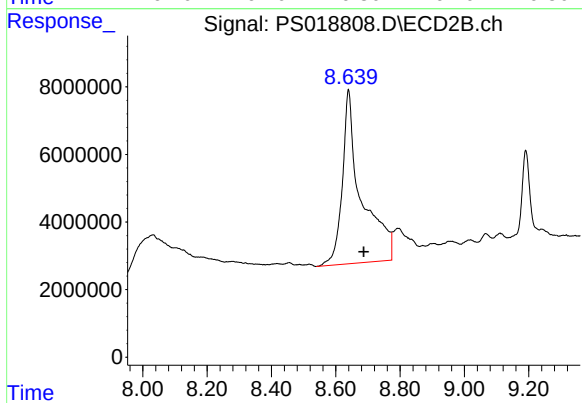

#11 2,4,5-TP (SILVEX)


R.T.: 8.639 min
Delta R.T.: -0.048 min
Response: 212256392
Conc: 48.66 ng/ml

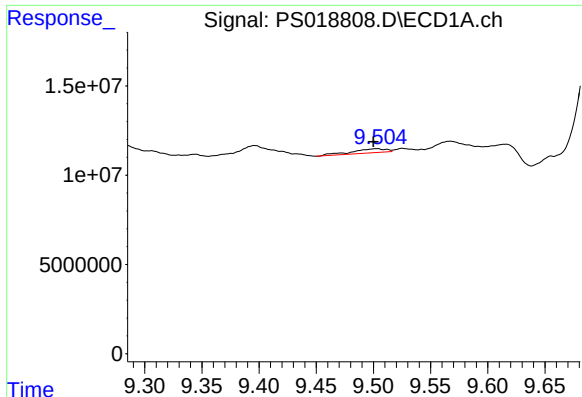

#12 2,4,5-T


R.T.: 9.502 min
Delta R.T.: 0.002 min
Response: 4706431
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

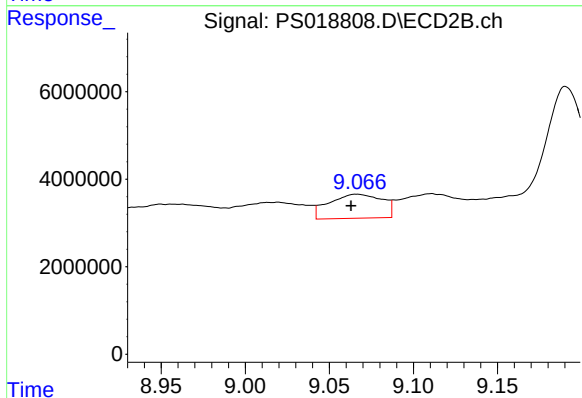


#12 2,4,5-T

R.T.: 9.067 min
Delta R.T.: 0.004 min
Response: 12016529
Conc: 2.90 ng/ml

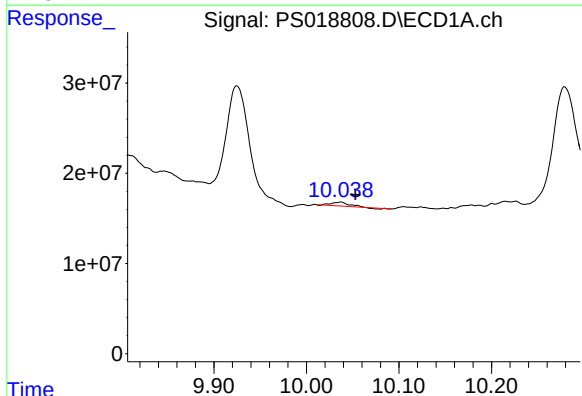


#13 2,4-DB

R.T.: 10.036 min
Delta R.T.: -0.017 min
Response: 4887977
Conc: 1.79 ng/ml

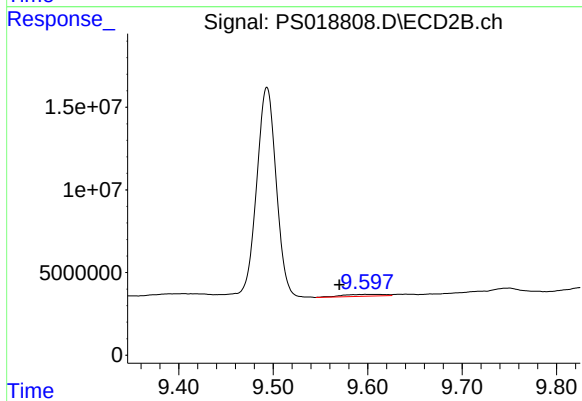

#13 2,4-DB


R.T.: 9.609 min
Delta R.T.: 0.039 min
Response: 3375828
Conc: 5.95 ng/ml

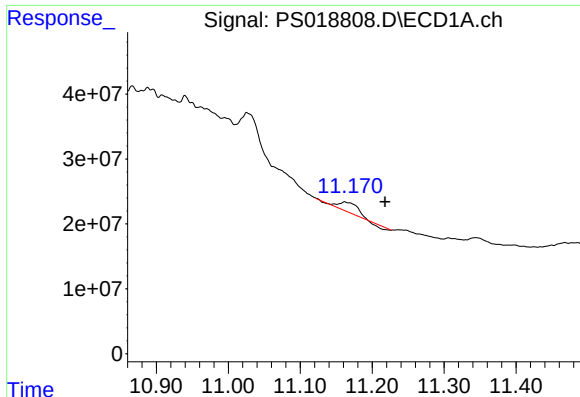

#14 DINOSEB


R.T.: 11.162 min
Delta R.T.: -0.056 min
Response: 24902938
Conc: 2.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

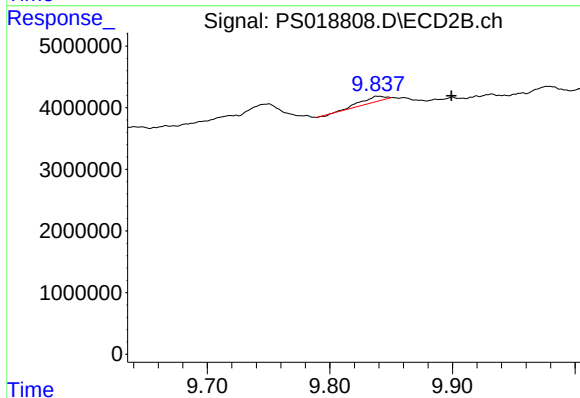


#14 DINOSEB

R.T.: 9.841 min
Delta R.T.: -0.058 min
Response: 1815484
Conc: N.D.

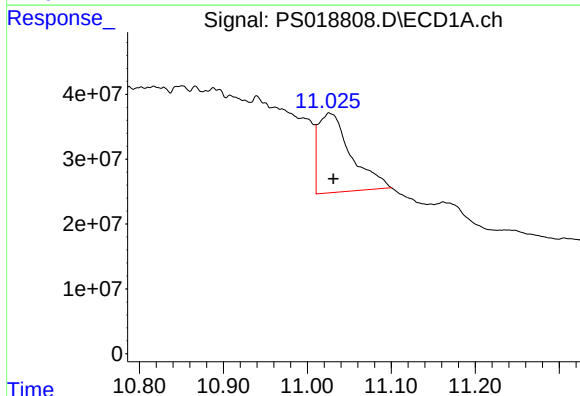


#15 Picloram

R.T.: 11.027 min
Delta R.T.: -0.004 min
Response: 335416215
Conc: 16.32 ng/ml

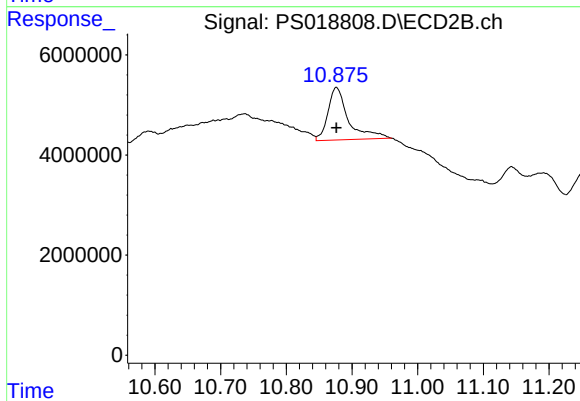

#15 Picloram


R.T.: 10.876 min
Delta R.T.: 0.000 min
Response: 22821728
Conc: 4.29 ng/ml

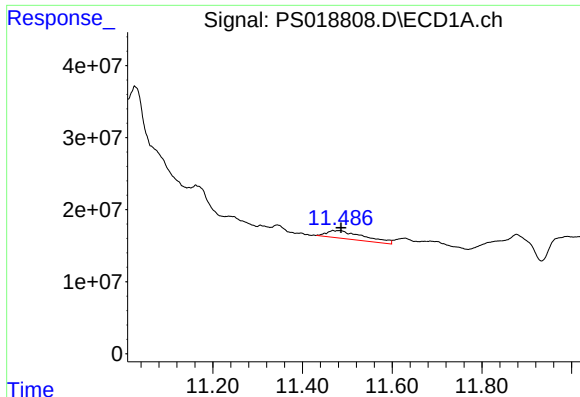

#16 DCPA

R.T.: 11.468 min
Delta R.T.: -0.018 min
Response: 63474982
Conc: 3.55 ng/ml

Instrument :
ECD_S
ClientSampleId :

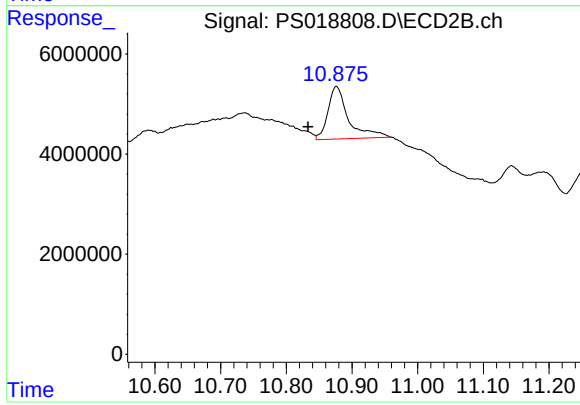

#16 DCPA

R.T.: 10.876 min
Delta R.T.: 0.043 min
Response: 22821728
Conc: 4.34 ng/ml