

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032922\
 Data File : PS018809.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Mar 2022 09:15
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 14:30:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.225	6.807	1381.2E6	365.2E6	485.316	518.989
Target Compounds							
8) T	DICHLORPROP	0.000	7.619	0	2439344	N.D.	3.081
11) T	2,4,5-TP ...	9.173f	8.638f	-1826327	13934283	N.D.	3.194
12) T	2,4,5-T	9.476	0.000	31325986	0	2.097	N.D. #
13) T	2,4-DB	9.995f	0.000	1620380	0	<MDL	N.D. #
14) T	DINOSEB	11.174f	0.000	13096072	0	1.225	N.D. #
15) T	Picloram	11.032	10.880	20559774	9986517	1.000	1.879 #
16) T	DCPA	0.000	10.880f	0	9986517	N.D.	1.899



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032922\
Data File : PS018809.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Mar 2022 09:15
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 14:30:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

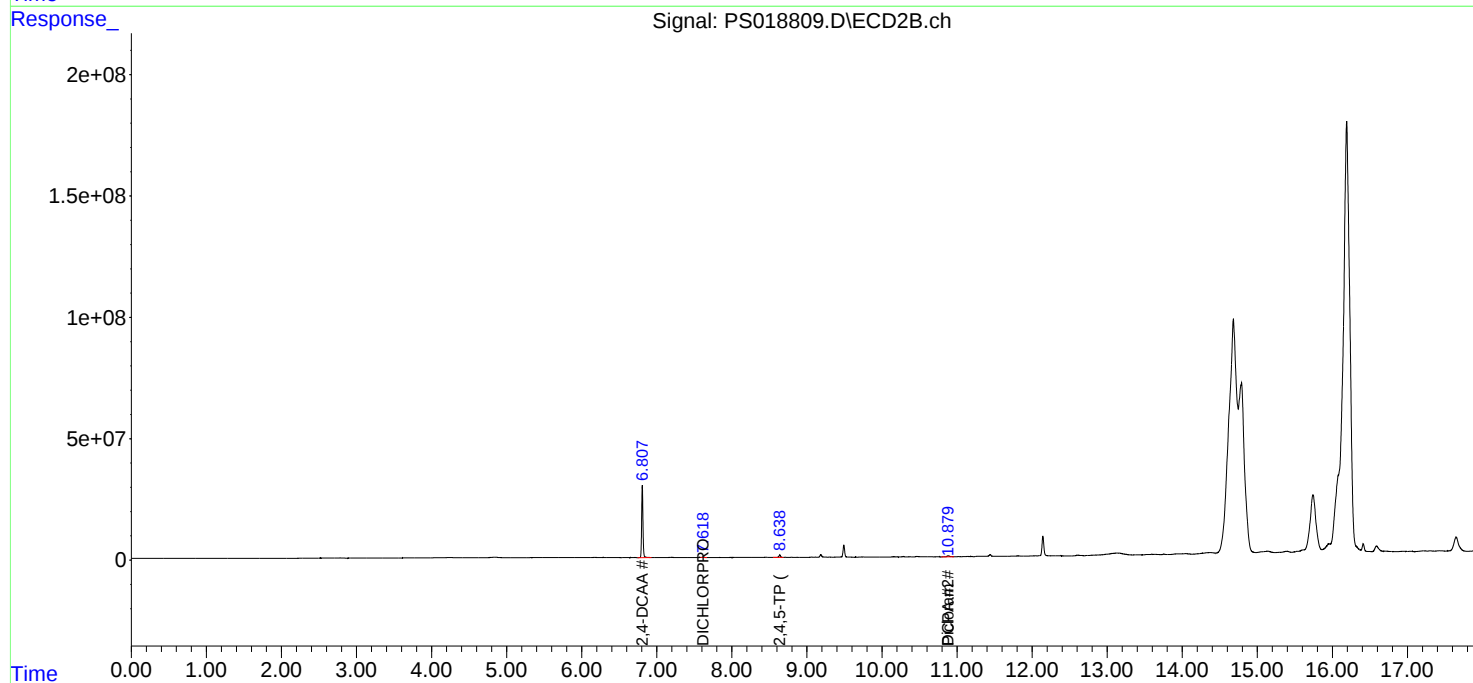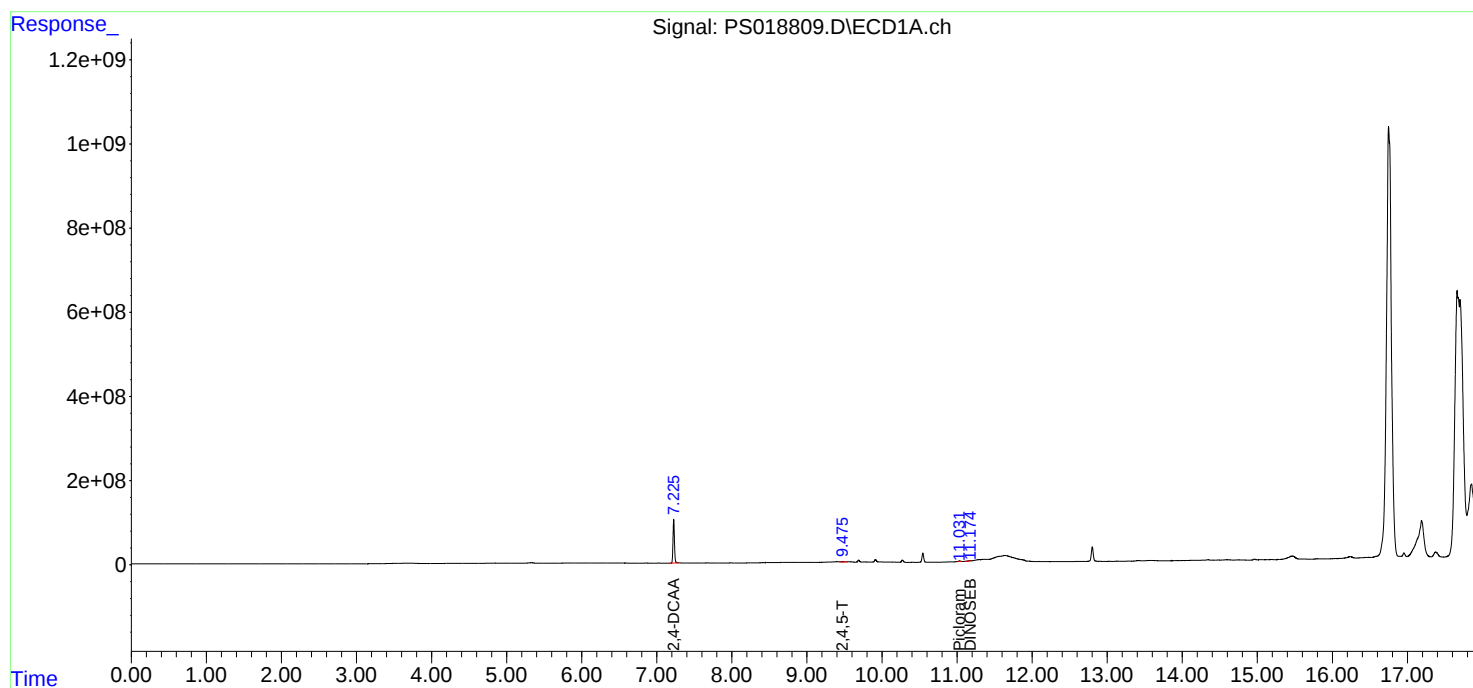


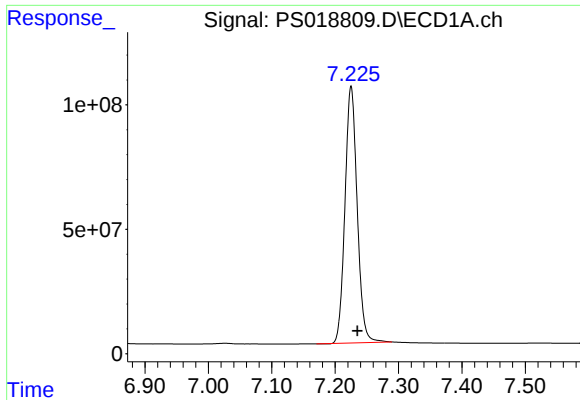

#4 2,4-DCAA


R.T.: 7.225 min
Delta R.T.: -0.010 min
Response: 1381167388
Conc: 485.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

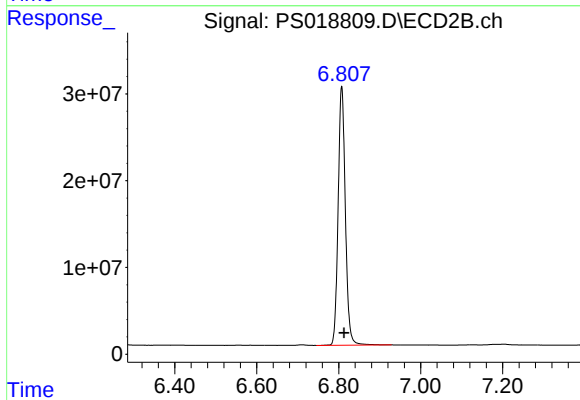


#4 2,4-DCAA

R.T.: 6.807 min
Delta R.T.: -0.006 min
Response: 365189412
Conc: 518.99 ng/ml

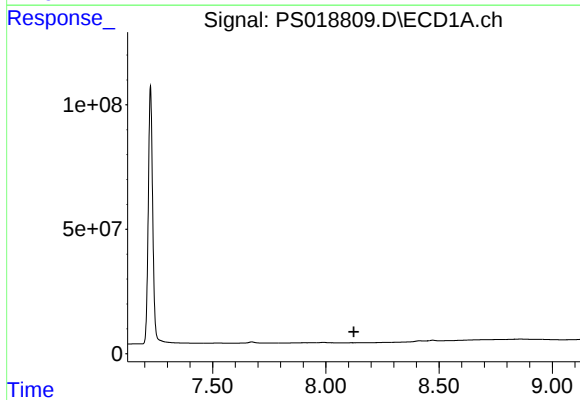


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.124 min
Response: 0
Conc: N.D.

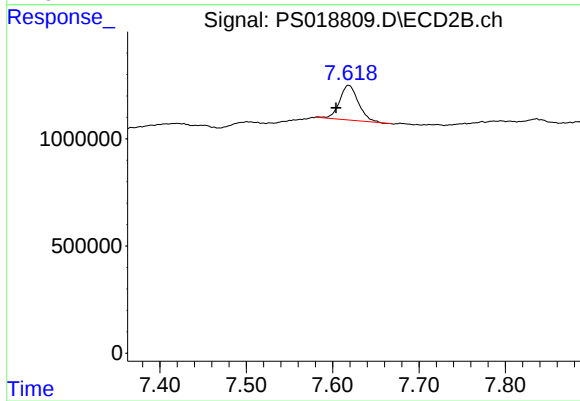

#8 DICHLORPROP


R.T.: 7.619 min
Delta R.T.: 0.015 min
Response: 2439344
Conc: 3.08 ng/ml

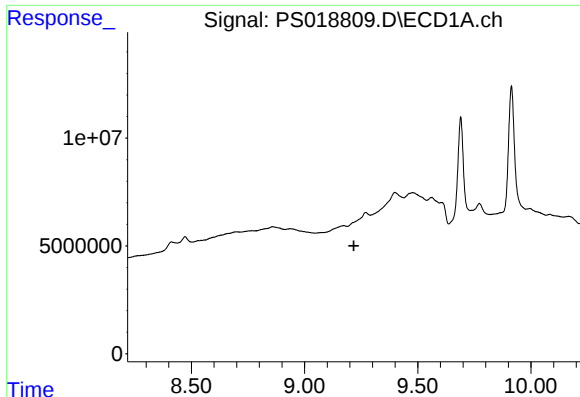

#11 2,4,5-TP (SILVEX)


R.T.: 9.173 min
Delta R.T.: -0.045 min
Response: -1826327
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

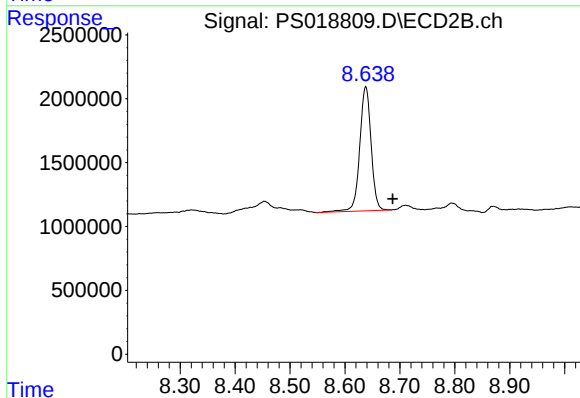


#11 2,4,5-TP (SILVEX)

R.T.: 8.638 min
Delta R.T.: -0.049 min
Response: 13934283
Conc: 3.19 ng/ml

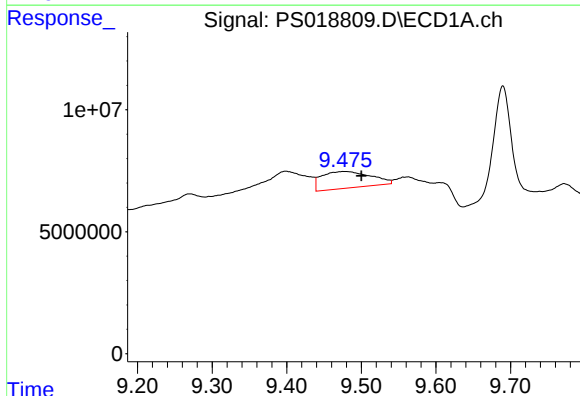


#12 2,4,5-T

R.T.: 9.476 min
Delta R.T.: -0.024 min
Response: 31325986
Conc: 2.10 ng/ml

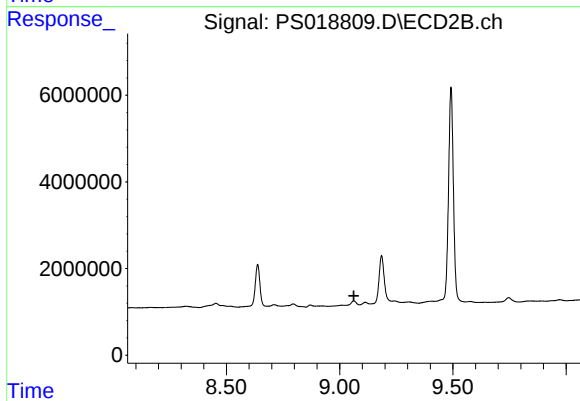

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.063 min
Response: 0
Conc: N.D.

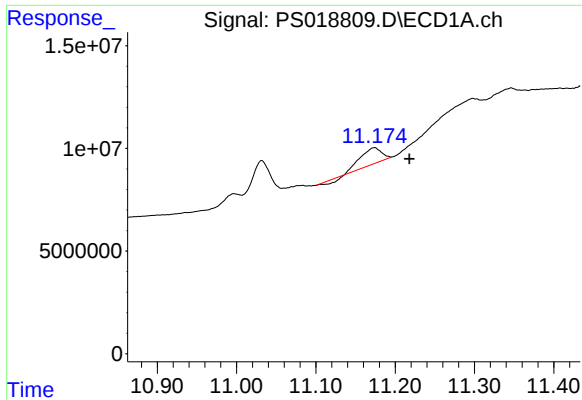

#14 DINOSEB


R.T.: 11.174 min
Delta R.T.: -0.044 min
Response: 13096072
Conc: 1.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

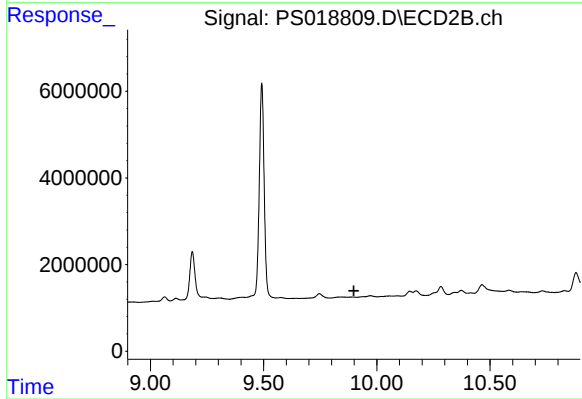


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.899 min
Response: 0
Conc: N.D.

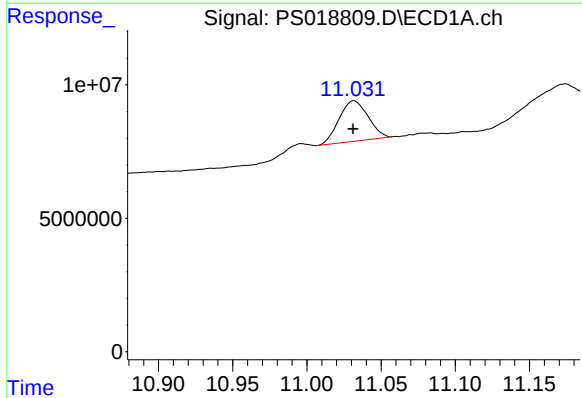


#15 Picloram

R.T.: 11.032 min
Delta R.T.: 0.000 min
Response: 20559774
Conc: 1.00 ng/ml

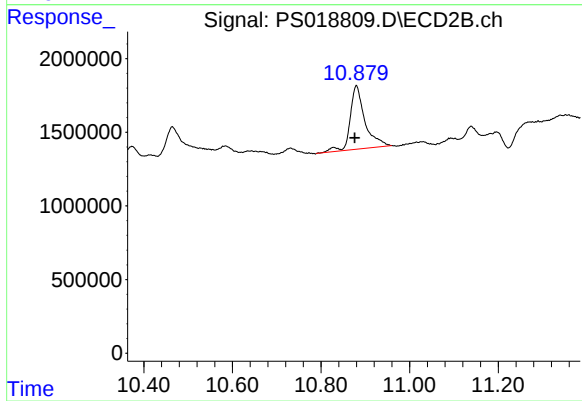

#15 Picloram


R.T.: 10.880 min
Delta R.T.: 0.004 min
Response: 9986517
Conc: 1.88 ng/ml

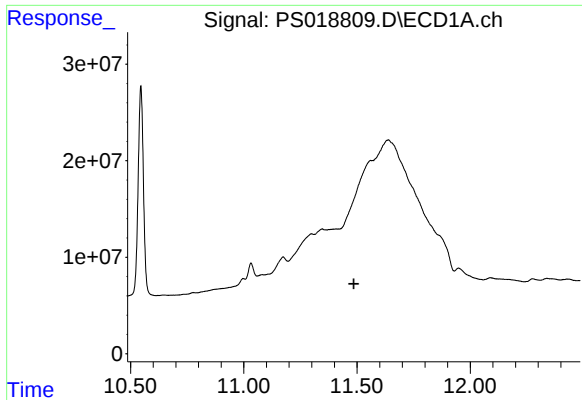

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.486 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

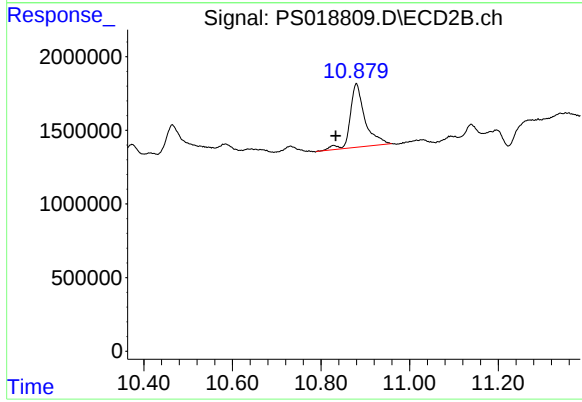

#16 DCPA

R.T.: 10.880 min
Delta R.T.: 0.047 min
Response: 9986517
Conc: 1.90 ng/ml