

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032922\
 Data File : PS018818.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2022 01:01
 Operator : AJ\MA
 Sample : PB143634TB
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 01:23:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.808	1312.8E6	481.9E6	461.287	684.826 #
Target Compounds							
1) T	Dalapon	2.977f	2.490f	266.7E6	466.1E6	68.576	564.019 #
2) T	3,5-DICHL...	6.462	6.006	-13350106	134.7E6	N.D.	128.772
3) T	4-Nitroph...	7.065	6.404	-7295052	82211923	N.D.	202.356
5) T	DICAMBA	7.469f	6.990	11097117	11684374	1.017	3.923 #
6) T	MCPD	7.588	7.114	5295217	4411835	<MDL	1.802 #
7) T	MCPA	7.739	7.328	153.7E6	5991203	12.706	1.716 #
8) T	DICHLORPROP	8.105	7.634	52163611	3482.3E6	18.938	4398.991 #
9) T	2,4-D	8.359	7.877	50976312	18864086	15.214	20.154 #
10) T	Pentachlo...	8.659	8.331	21365112	17260948	<MDL	1.758 #
11) T	2,4,5-TP ...	9.276f	8.645f	7012.2E6	21094.1E6	461.081	4835.884 #
12) T	2,4,5-T	9.469	9.075	4537.7E6	2268.5E6	303.752	547.661 #
13) T	2,4-DB	10.039	9.554	1884.8E6	73033.9E6	689.027	128637.800 #
14) T	DINOSEB	11.204	9.918	10506.0E6	-14893000	982.497	N.D. #
15) T	Picloram	10.980f	10.903	304.1E6	304.9E6	14.795	57.346 #
16) T	DCPA	11.492	10.834	501.3E6	556.2E6	28.022	105.765 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032922\
Data File : PS018818.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Mar 2022 01:01
Operator : AJ\MA
Sample : PB143634TB
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 01:23:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

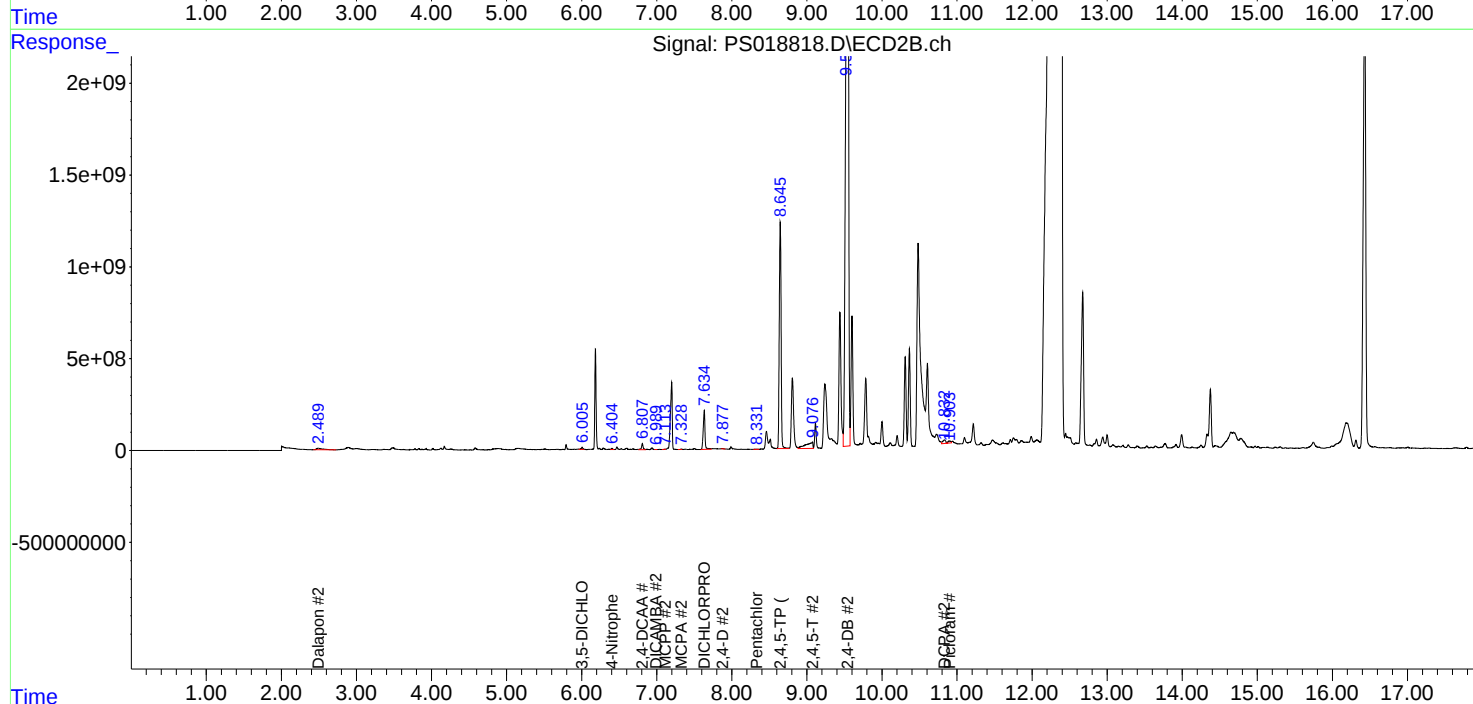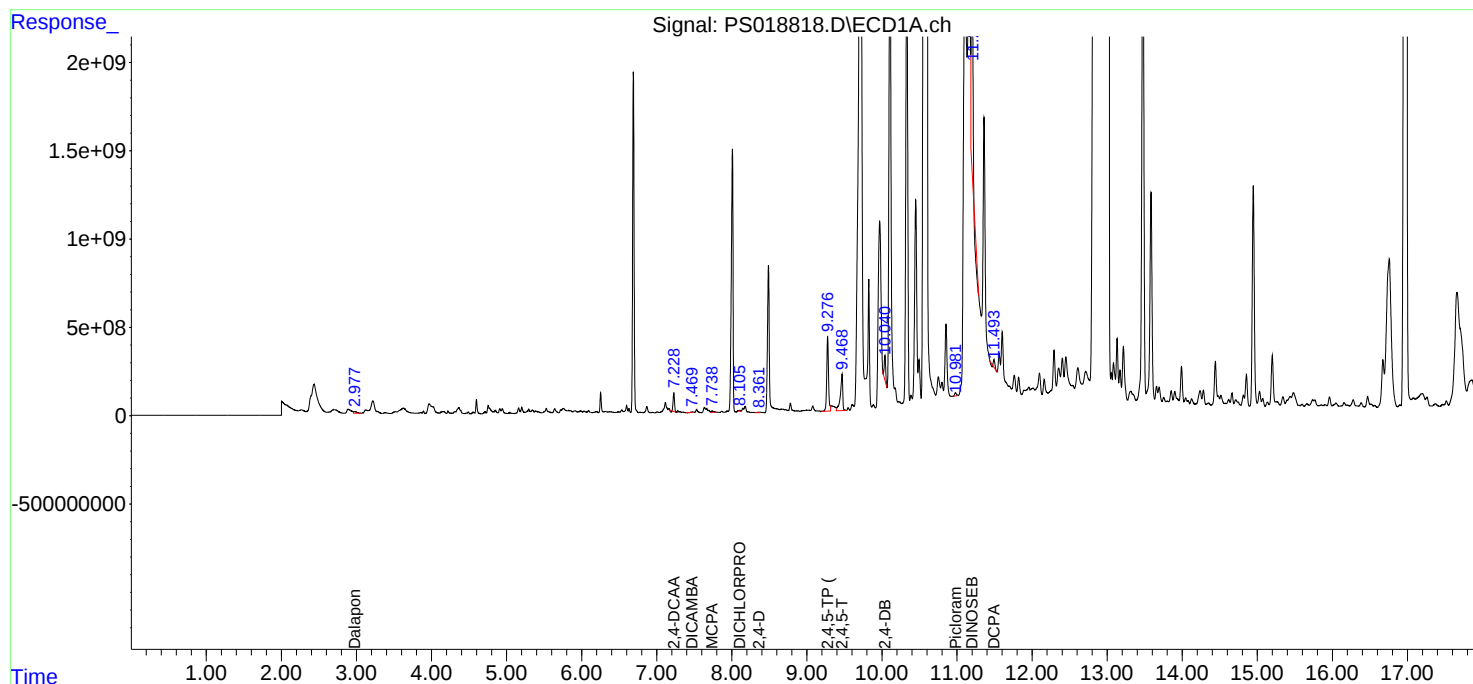


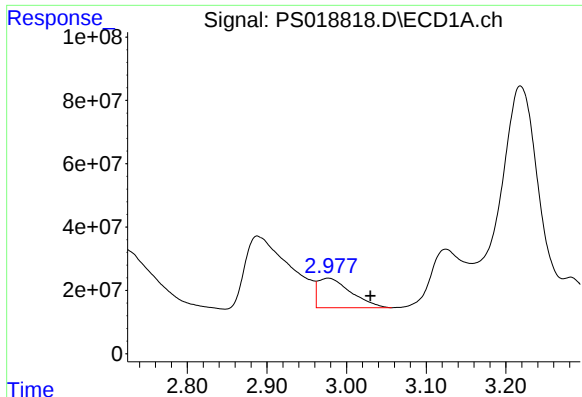

#1 Dalapon


R.T.: 2.977 min
Delta R.T.: -0.053 min
Response: 266658765
Conc: 68.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

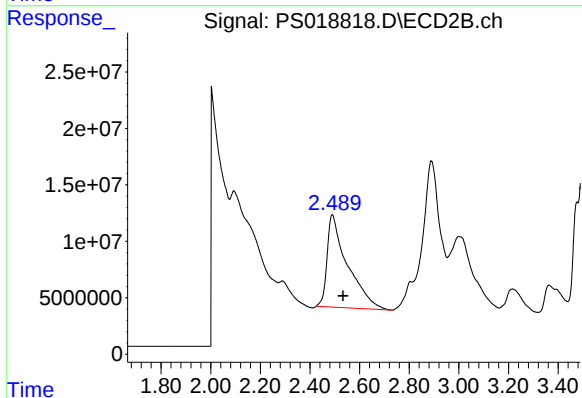


#1 Dalapon

R.T.: 2.490 min
Delta R.T.: -0.043 min
Response: 466142723
Conc: 564.02 ng/ml

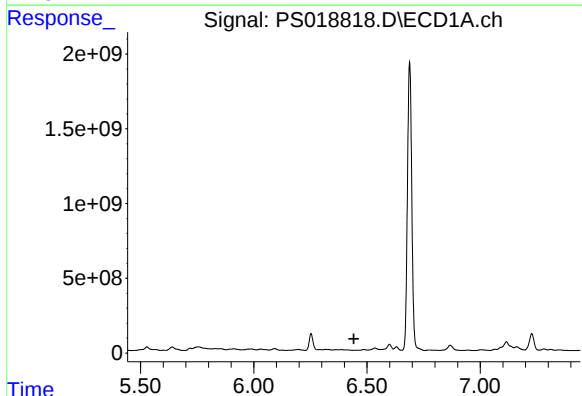


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.462 min
Delta R.T.: 0.020 min
Response: -13350106
Conc: N.D.

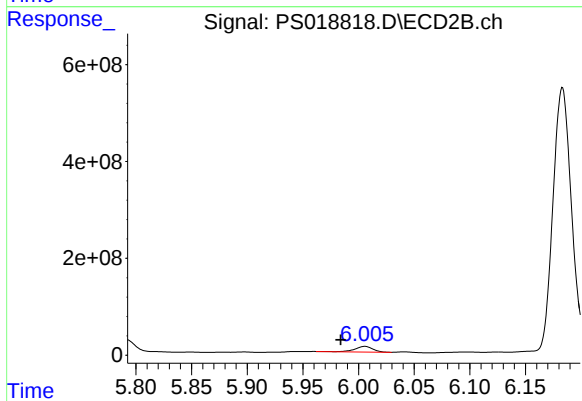

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.006 min
Delta R.T.: 0.022 min
Response: 134710129
Conc: 128.77 ng/ml

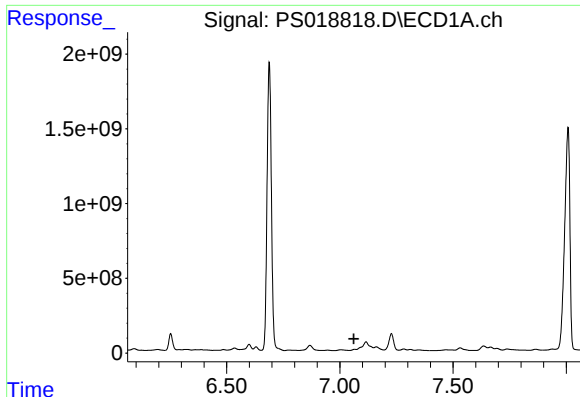

#3 4-Nitrophenol


R.T.: 7.065 min
Delta R.T.: 0.003 min
Response: -7295052
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

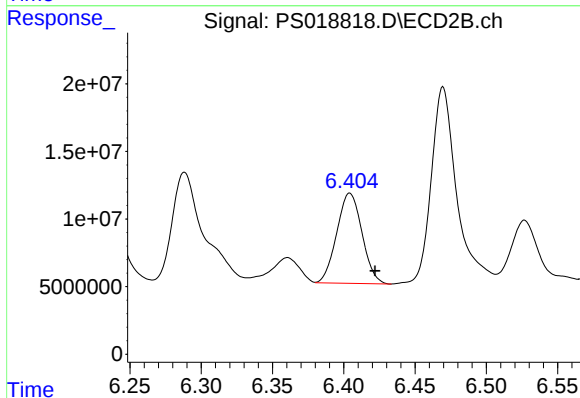


#3 4-Nitrophenol

R.T.: 6.404 min
Delta R.T.: -0.018 min
Response: 82211923
Conc: 202.36 ng/ml

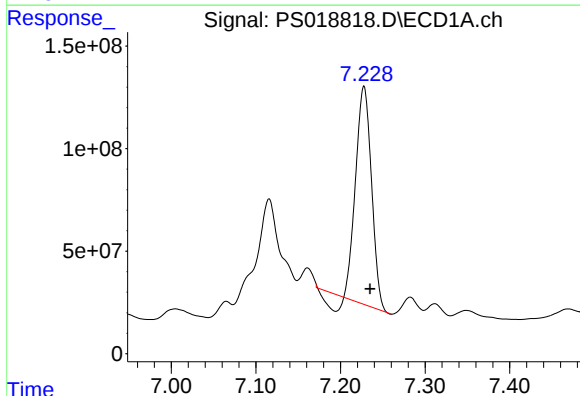


#4 2,4-DCAA

R.T.: 7.228 min
Delta R.T.: -0.007 min
Response: 1312783640
Conc: 461.29 ng/ml

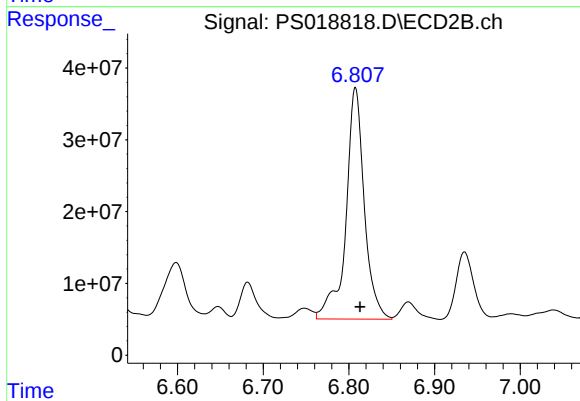

#4 2,4-DCAA


R.T.: 6.808 min
Delta R.T.: -0.005 min
Response: 481881162
Conc: 684.83 ng/ml

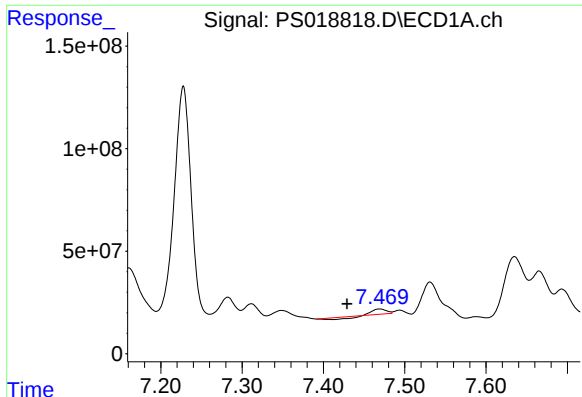

#5 DICAMBA


R.T.: 7.469 min
Delta R.T.: 0.040 min
Response: 11097117
Conc: 1.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

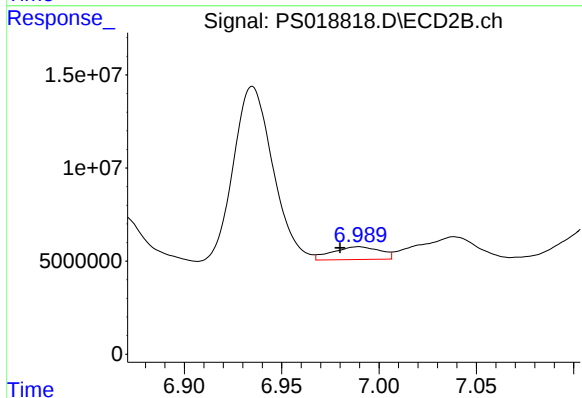


#5 DICAMBA

R.T.: 6.990 min
Delta R.T.: 0.010 min
Response: 11684374
Conc: 3.92 ng/ml

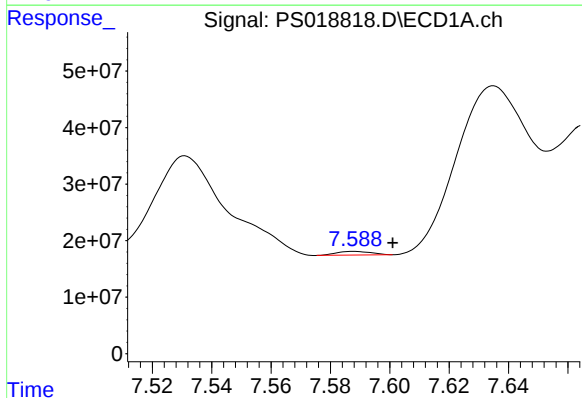


#6 MCP

R.T.: 7.588 min
Delta R.T.: -0.013 min
Response: 5295217
Conc: N.D.

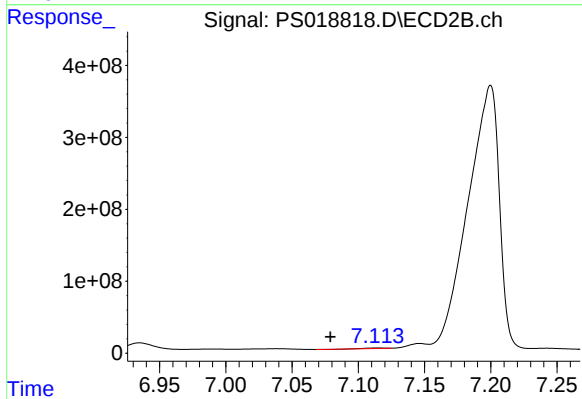

#6 MCP


R.T.: 7.114 min
Delta R.T.: 0.035 min
Response: 4411835
Conc: 1.80 ug/ml

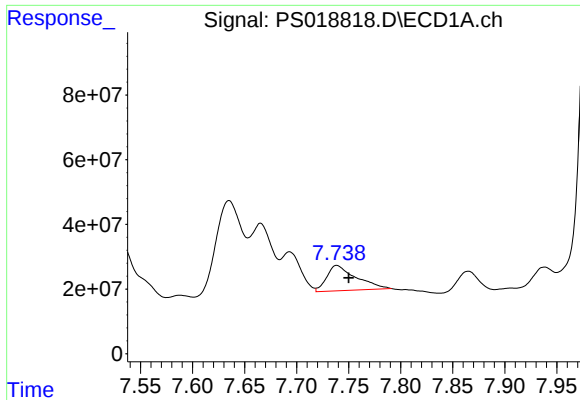

#7 MCPA


R.T.: 7.739 min
Delta R.T.: -0.011 min
Response: 153667832
Conc: 12.71 ug/ml

Instrument :
ECD_S
ClientSampleId :

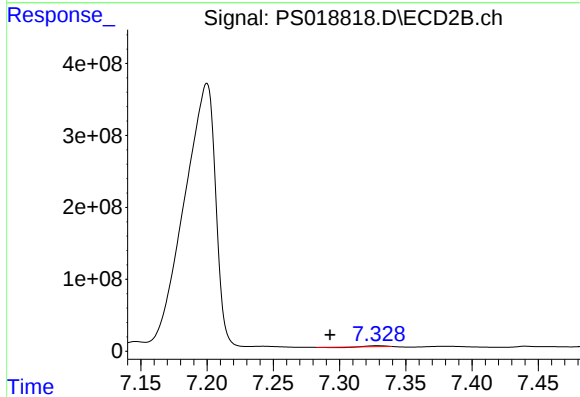


#7 MCPA

R.T.: 7.328 min
Delta R.T.: 0.035 min
Response: 5991203
Conc: 1.72 ug/ml

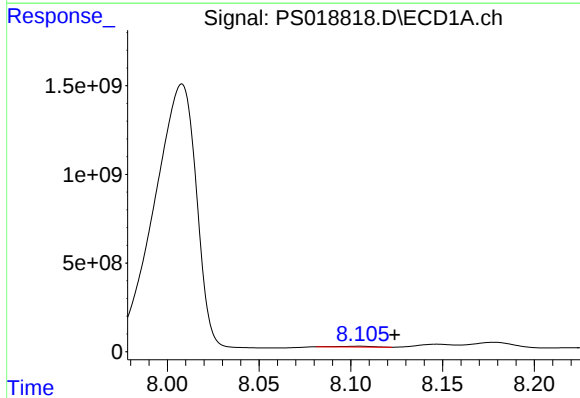


#8 DICHLORPROP

R.T.: 8.105 min
Delta R.T.: -0.019 min
Response: 52163611
Conc: 18.94 ng/ml

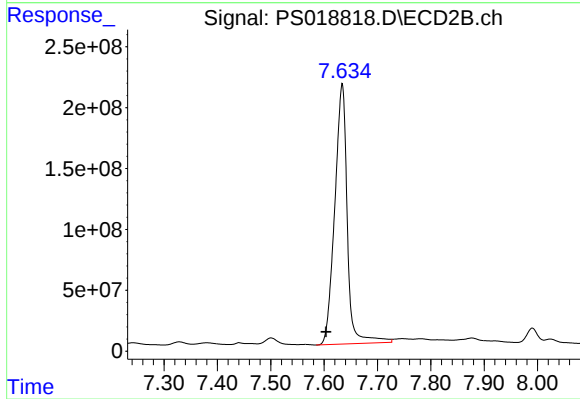

#8 DICHLORPROP


R.T.: 7.634 min
Delta R.T.: 0.030 min
Response: 3482298203
Conc: 4398.99 ng/ml

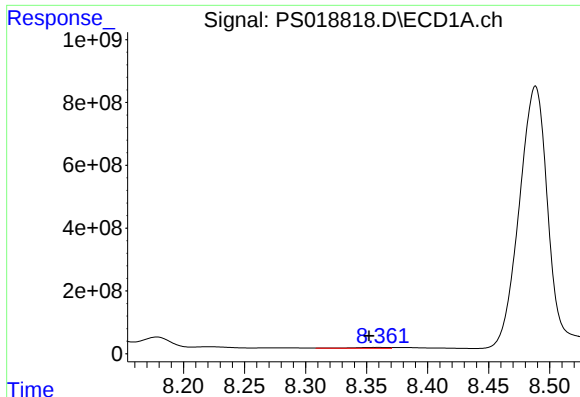

#9 2,4-D


R.T.: 8.359 min
Delta R.T.: 0.007 min
Response: 50976312
Conc: 15.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

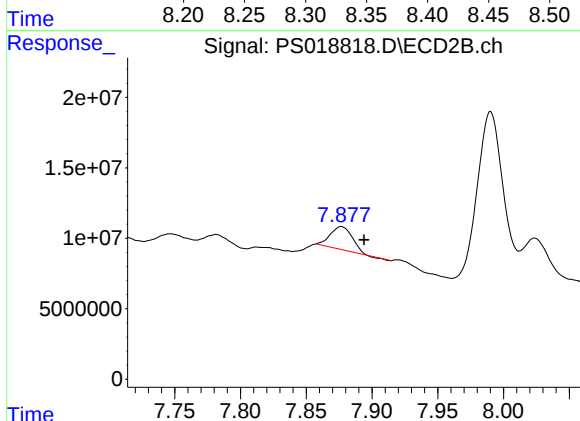


#9 2,4-D

R.T.: 7.877 min
Delta R.T.: -0.017 min
Response: 18864086
Conc: 20.15 ng/ml

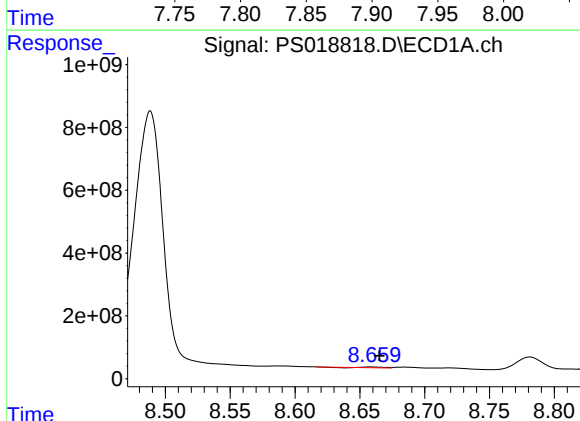


#10 Pentachlorophenol

R.T.: 8.659 min
Delta R.T.: -0.006 min
Response: 21365112
Conc: N.D.

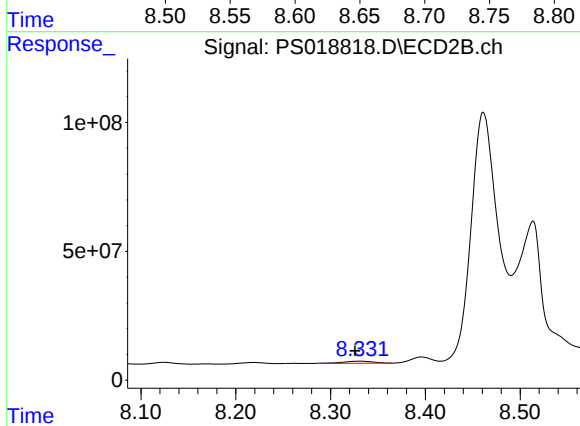

#10 Pentachlorophenol


R.T.: 8.331 min
Delta R.T.: 0.005 min
Response: 17260948
Conc: 1.76 ng/ml

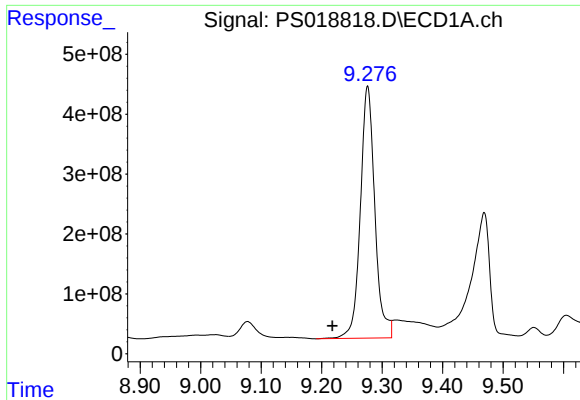

#11 2,4,5-TP (SILVEX)


R.T.: 9.276 min
Delta R.T.: 0.058 min
Response: 7012213055
Conc: 461.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

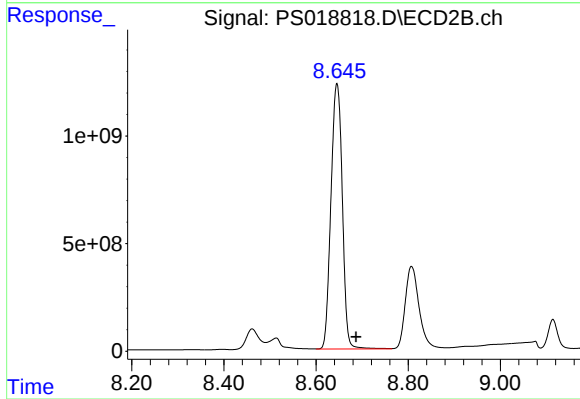


#11 2,4,5-TP (SILVEX)

R.T.: 8.645 min
Delta R.T.: -0.042 min
Response: 21094112301
Conc: 4835.88 ng/ml

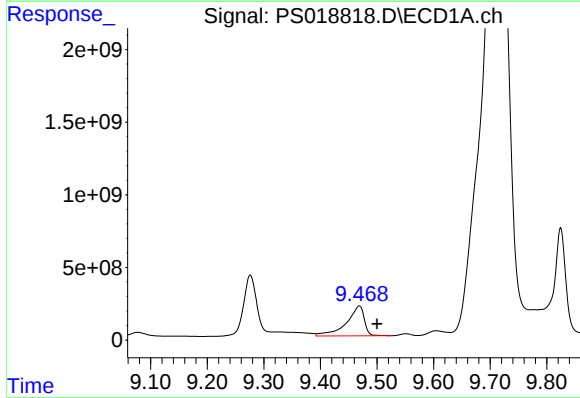


#12 2,4,5-T

R.T.: 9.469 min
Delta R.T.: -0.031 min
Response: 4537672582
Conc: 303.75 ng/ml

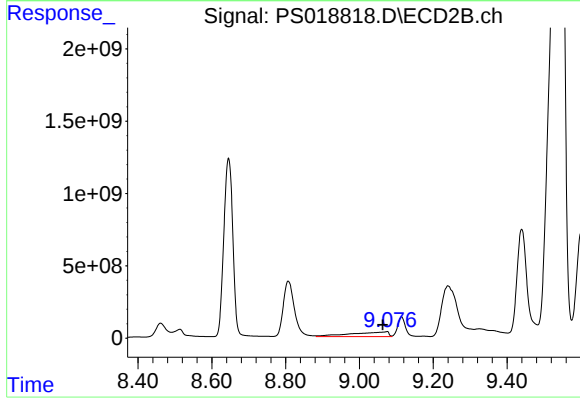

#12 2,4,5-T


R.T.: 9.075 min
Delta R.T.: 0.012 min
Response: 2268515986
Conc: 547.66 ng/ml

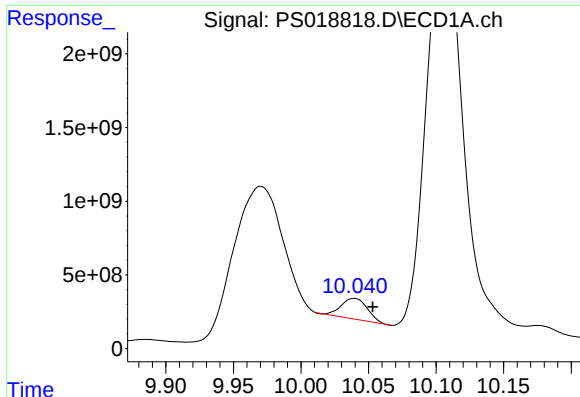

#13 2,4-DB


R.T.: 10.039 min
Delta R.T.: -0.014 min
Response: 1884770379
Conc: 689.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

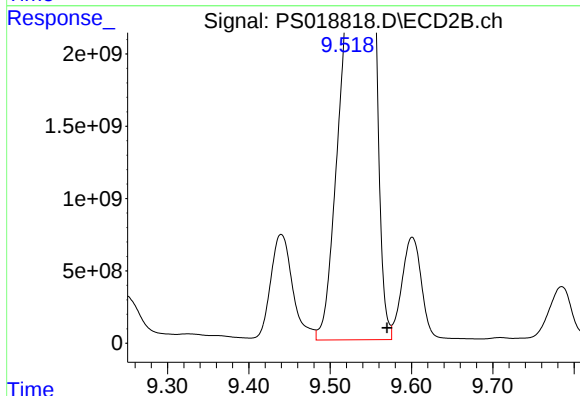


#13 2,4-DB

R.T.: 9.554 min
Delta R.T.: -0.016 min
Response: 73033900159
Conc: 128637.80 ng/ml

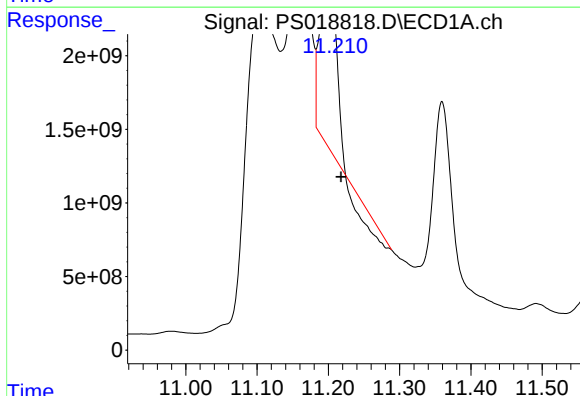


#14 DINOSEB

R.T.: 11.204 min
Delta R.T.: -0.014 min
Response: 10505972056
Conc: 982.50 ng/ml

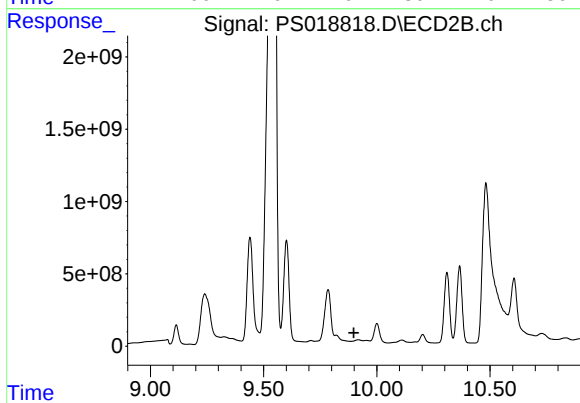

#14 DINOSEB


R.T.: 9.918 min
Delta R.T.: 0.019 min
Response: -14893000
Conc: N.D.

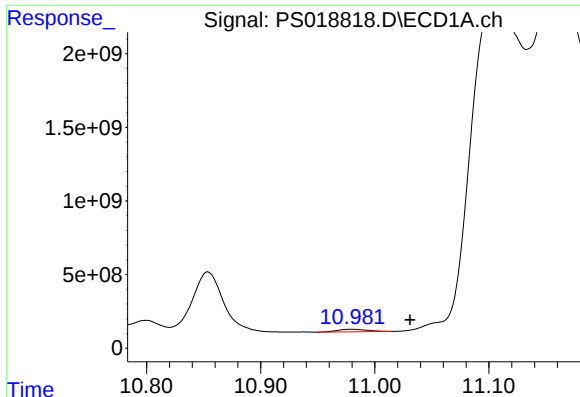

#15 Picloram


R.T.: 10.980 min
Delta R.T.: -0.051 min
Response: 304130173
Conc: 14.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

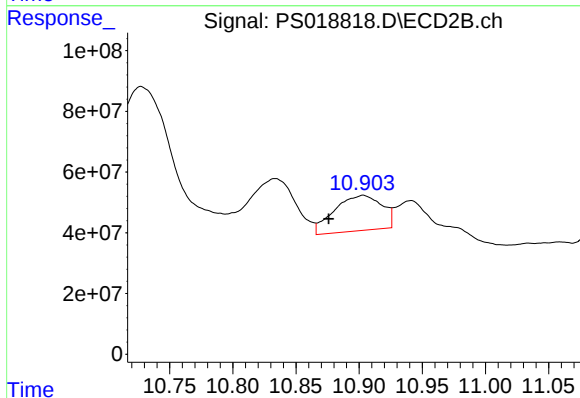


#15 Picloram

R.T.: 10.903 min
Delta R.T.: 0.027 min
Response: 304859341
Conc: 57.35 ng/ml

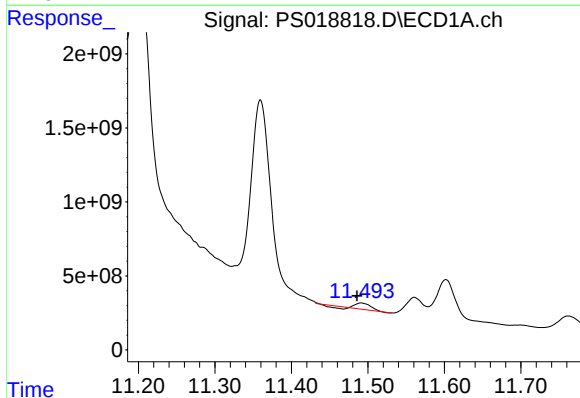

#16 DCPA

R.T.: 11.492 min
Delta R.T.: 0.006 min
Response: 501329475
Conc: 28.02 ng/ml

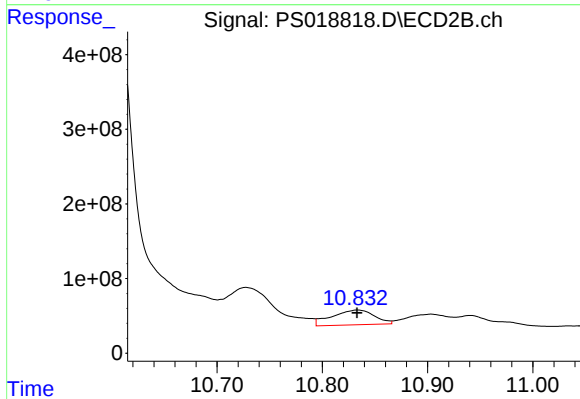

#16 DCPA

R.T.: 10.834 min
Delta R.T.: 0.000 min
Response: 556247072
Conc: 105.76 ng/ml