

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032922\
 Data File : PS018820.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2022 01:49
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 05:45:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.224	6.807	1492.7E6	385.6E6	524.516	547.926
Target Compounds							
3) T	4-Nitroph...	7.019f	0.000	863837	0	<MDL	N.D. #
5) T	DICAMBA	7.417	6.974	6719329	2057074	<MDL	<MDL #
6) T	MCP	7.623	7.131f	10475407	1095454	1.234	<MDL #
8) T	DICHLORPROP	8.108	7.617	6205175	65879575	2.253	83.222 #
9) T	2,4-D	8.340	7.889	14944266	3744316	4.460	4.000
10) T	Pentachlo...	8.651	8.318	24549764	6181572	<MDL	<MDL #
11) T	2,4,5-TP ...	9.204	8.679	57945358	15637243	3.810	3.585
12) T	2,4,5-T	9.488	9.058	141.4E6	33770823	9.466	8.153
13) T	2,4-DB	10.083	9.576	368.7E6	134.7E6	134.800	237.316 #
14) T	DINOSEB	11.256	9.893	-2646825	14071125	N.D.	4.593
15) T	Picloram	11.024	10.875	-65606734	70587523	N.D.	13.278
16) T	DCPA	11.472	10.824	236.0E6	38196011	13.191	7.263 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032922\
Data File : PS018820.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Mar 2022 01:49
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 05:45:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

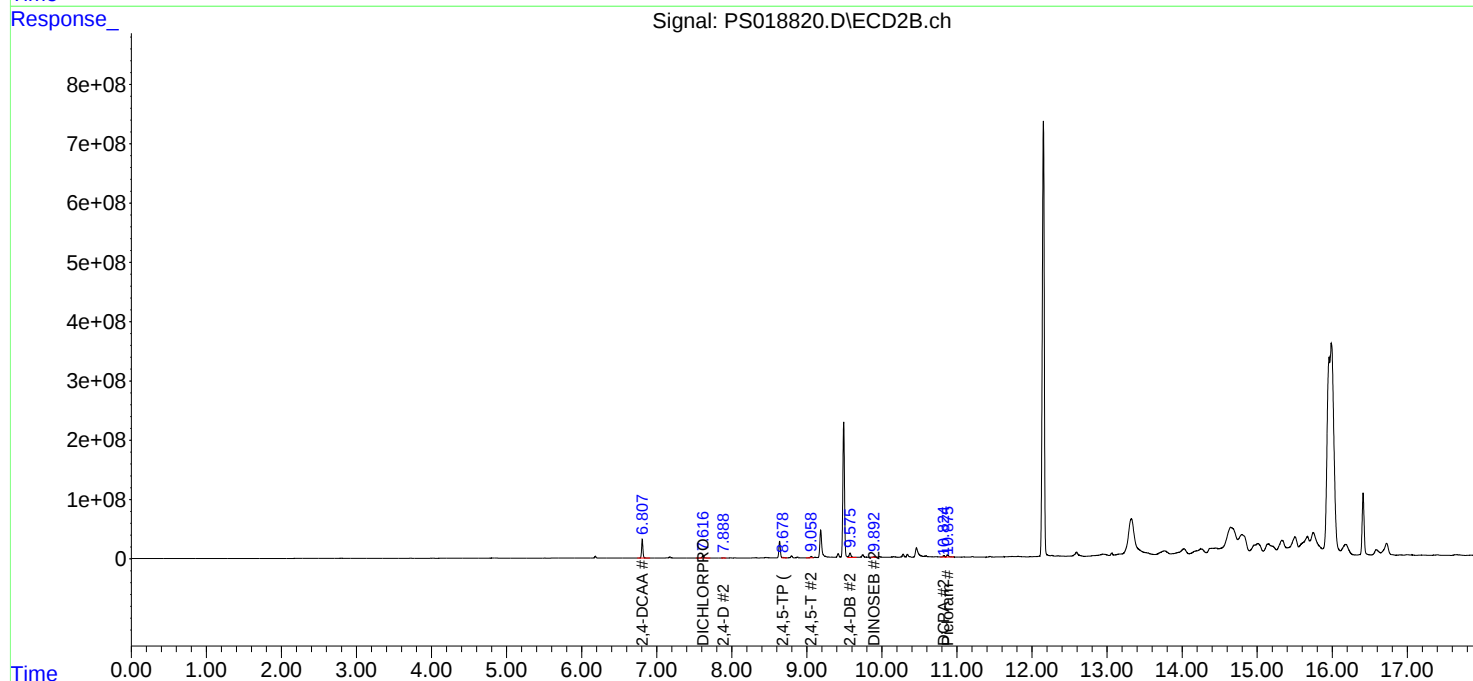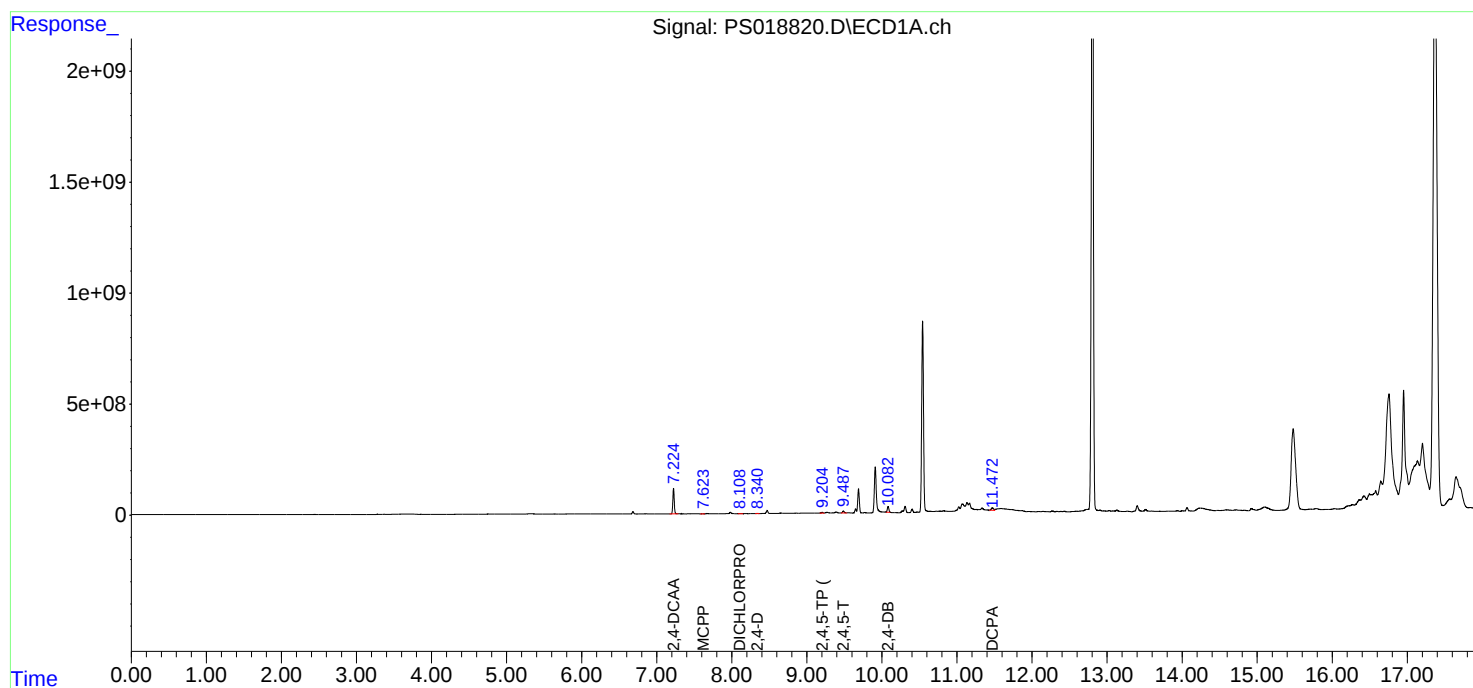


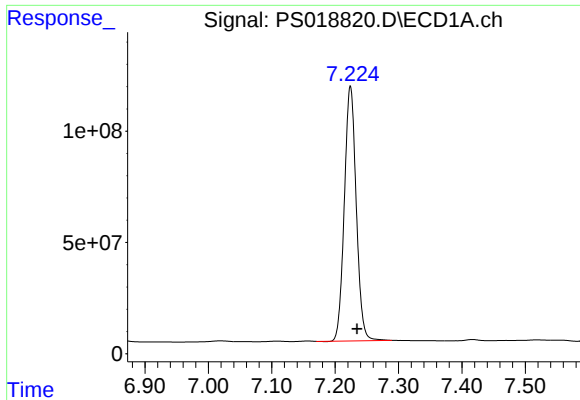

#4 2,4-DCAA


R.T.: 7.224 min
Delta R.T.: -0.011 min
Response: 1492728462
Conc: 524.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

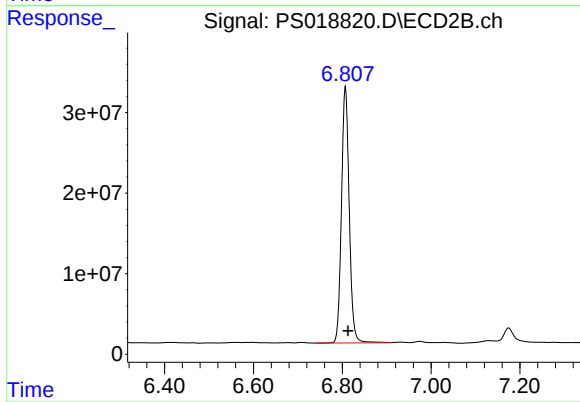


#4 2,4-DCAA

R.T.: 6.807 min
Delta R.T.: -0.006 min
Response: 385551074
Conc: 547.93 ng/ml

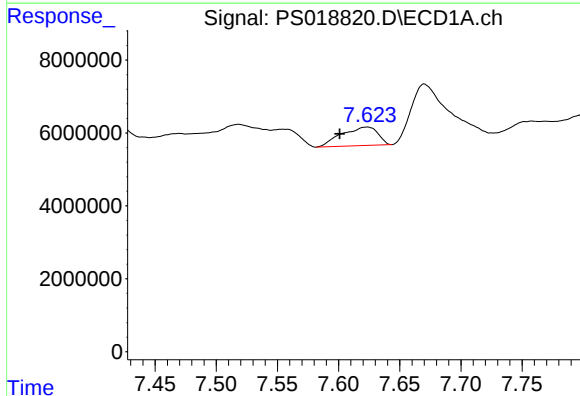


#6 MCP

R.T.: 7.623 min
Delta R.T.: 0.022 min
Response: 10475407
Conc: 1.23 ug/ml

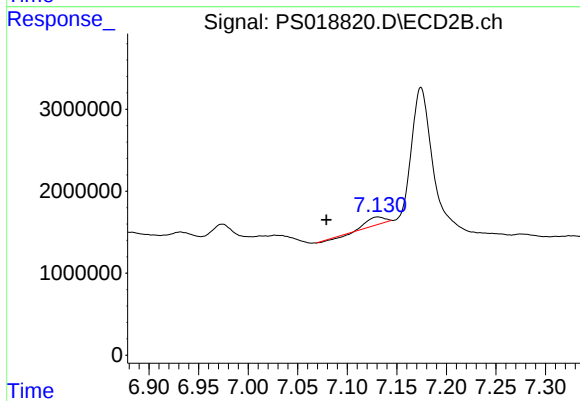

#6 MCP


R.T.: 7.131 min
Delta R.T.: 0.052 min
Response: 1095454
Conc: N.D.

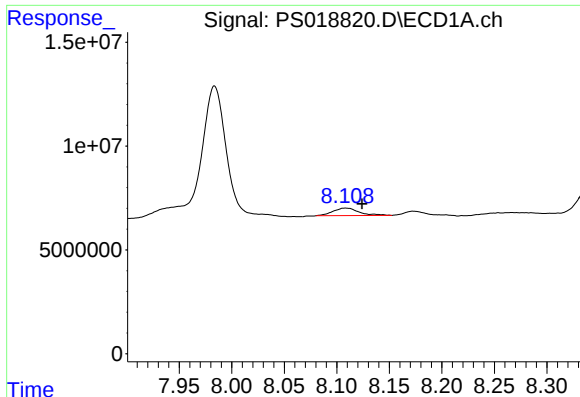

#8 DICHLORPROP


R.T.: 8.108 min
Delta R.T.: -0.016 min
Response: 6205175
Conc: 2.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

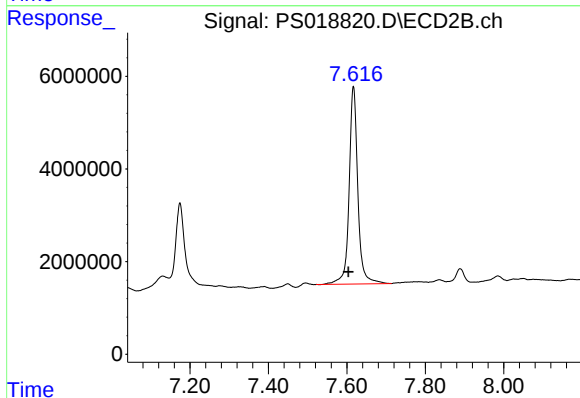


#8 DICHLORPROP

R.T.: 7.617 min
Delta R.T.: 0.013 min
Response: 65879575
Conc: 83.22 ng/ml

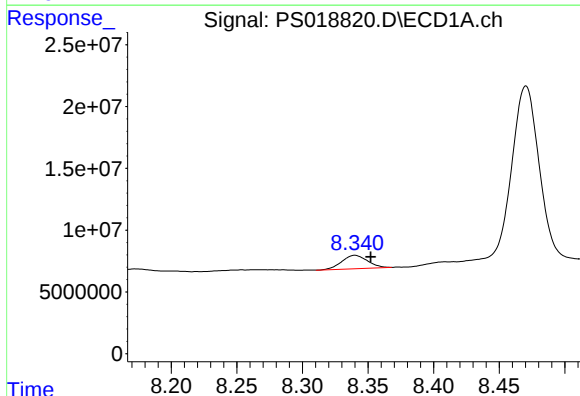


#9 2,4-D

R.T.: 8.340 min
Delta R.T.: -0.012 min
Response: 14944266
Conc: 4.46 ng/ml

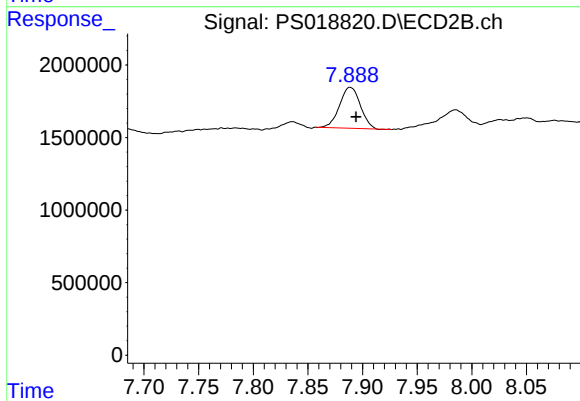

#9 2,4-D


R.T.: 7.889 min
Delta R.T.: -0.005 min
Response: 3744316
Conc: 4.00 ng/ml

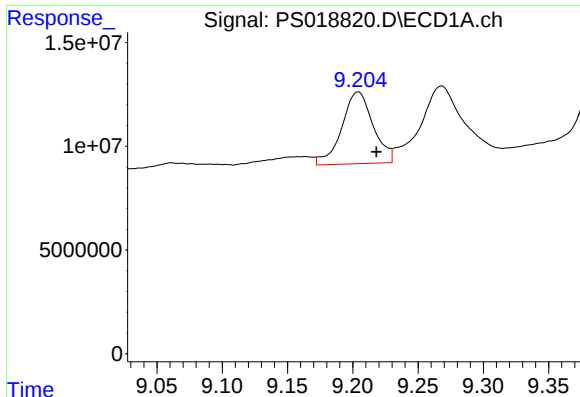

#11 2,4,5-TP (SILVEX)


R.T.: 9.204 min
Delta R.T.: -0.014 min
Response: 57945358
Conc: 3.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

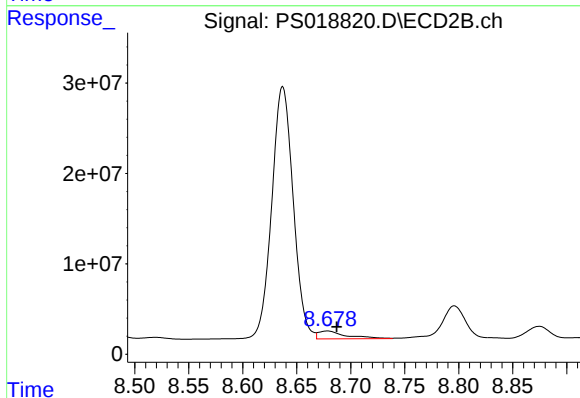


#11 2,4,5-TP (SILVEX)

R.T.: 8.679 min
Delta R.T.: -0.008 min
Response: 15637243
Conc: 3.58 ng/ml

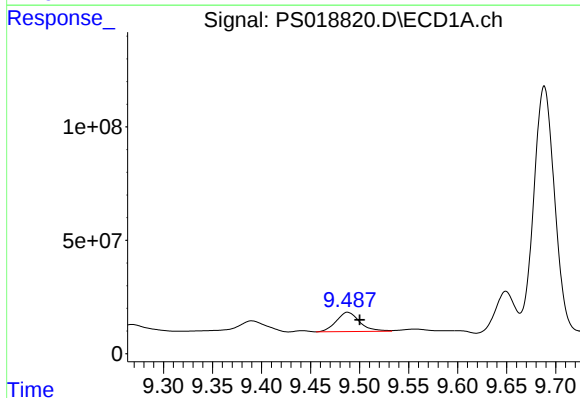


#12 2,4,5-T

R.T.: 9.488 min
Delta R.T.: -0.012 min
Response: 141408364
Conc: 9.47 ng/ml

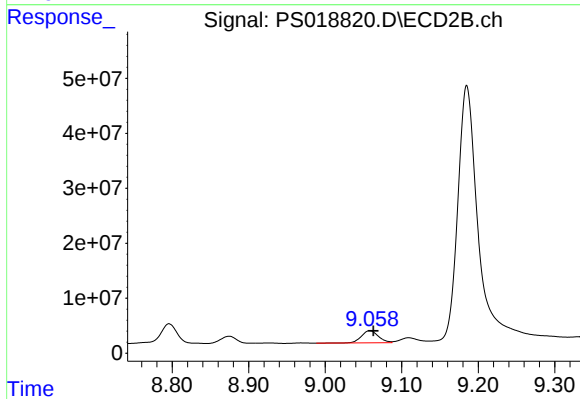

#12 2,4,5-T


R.T.: 9.058 min
Delta R.T.: -0.005 min
Response: 33770823
Conc: 8.15 ng/ml

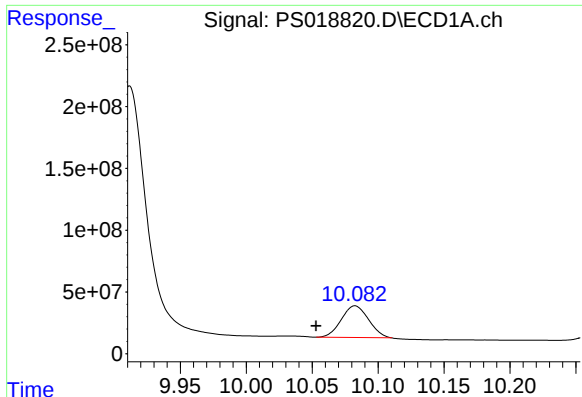

#13 2,4-DB


R.T.: 10.083 min
Delta R.T.: 0.030 min
Response: 368731959
Conc: 134.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

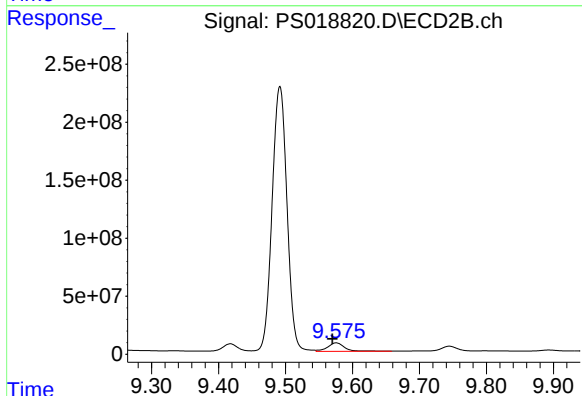


#13 2,4-DB

R.T.: 9.576 min
Delta R.T.: 0.006 min
Response: 134735963
Conc: 237.32 ng/ml

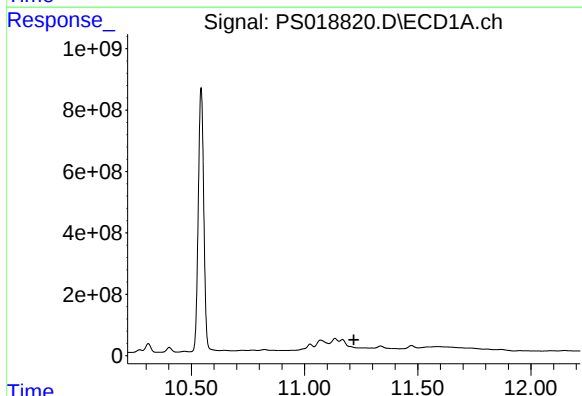


#14 DINOSEB

R.T.: 11.256 min
Delta R.T.: 0.038 min
Response: -2646825
Conc: N.D.

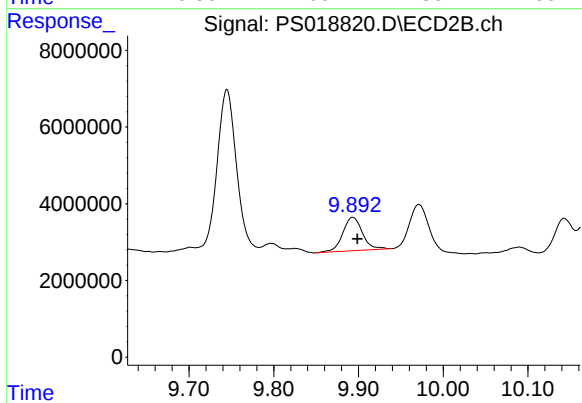

#14 DINOSEB


R.T.: 9.893 min
Delta R.T.: -0.006 min
Response: 14071125
Conc: 4.59 ng/ml

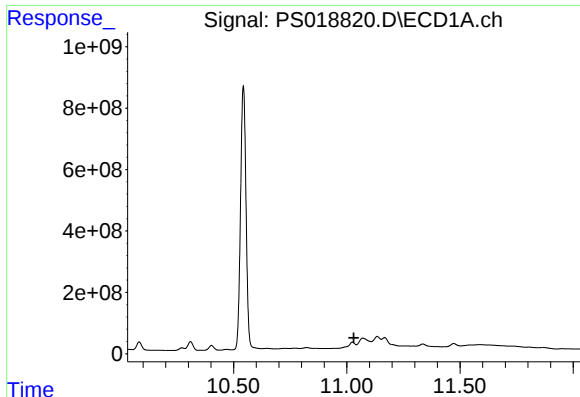

#15 Picloram


R.T.: 11.024 min
Delta R.T.: -0.007 min
Response: -65606734
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

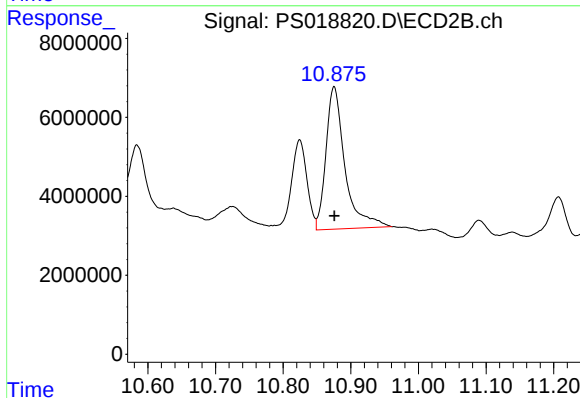


#15 Picloram

R.T.: 10.875 min
Delta R.T.: 0.000 min
Response: 70587523
Conc: 13.28 ng/ml

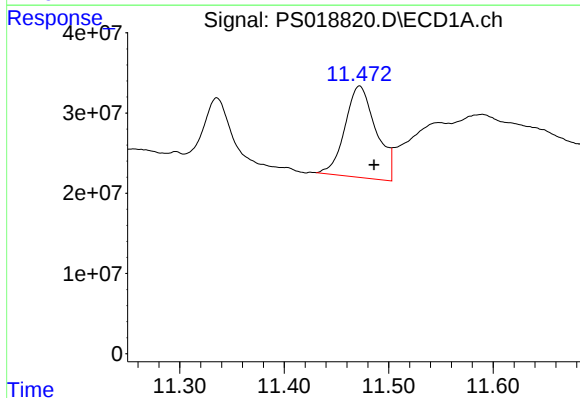

#16 DCPA

R.T.: 11.472 min
Delta R.T.: -0.014 min
Response: 235999379
Conc: 13.19 ng/ml

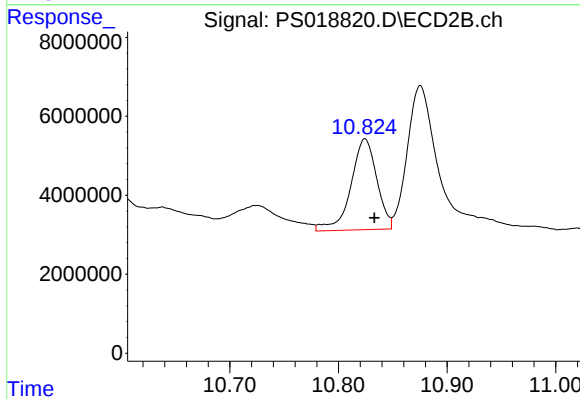

#16 DCPA

R.T.: 10.824 min
Delta R.T.: -0.009 min
Response: 38196011
Conc: 7.26 ng/ml