

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032922\
 Data File : PS018827.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2022 04:59
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 05:47:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.225	6.808	1530.4E6	373.3E6	537.738	530.558
Target Compounds							
8) T	DICHLORPROP	0.000	7.618	0	12536202	N.D.	15.836
10) T	Pentachlo...	8.653	0.000	2625546	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.268f	8.637f	42259776	24855007	2.779	5.698 #
12) T	2,4,5-T	9.488	0.000	10427468	0	<MDL	N.D. #
13) T	2,4-DB	10.084	9.575	9936550	4618672	3.633	8.135 #
14) T	DINOSEB	11.168f	0.000	87020982	0	8.138	N.D. #
15) T	Picloram	11.034	10.883	33684936	9089021	1.639	1.710
16) T	DCPA	11.472	10.827	7626484	1896592	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032922\
Data File : PS018827.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Mar 2022 04:59
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 05:47:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

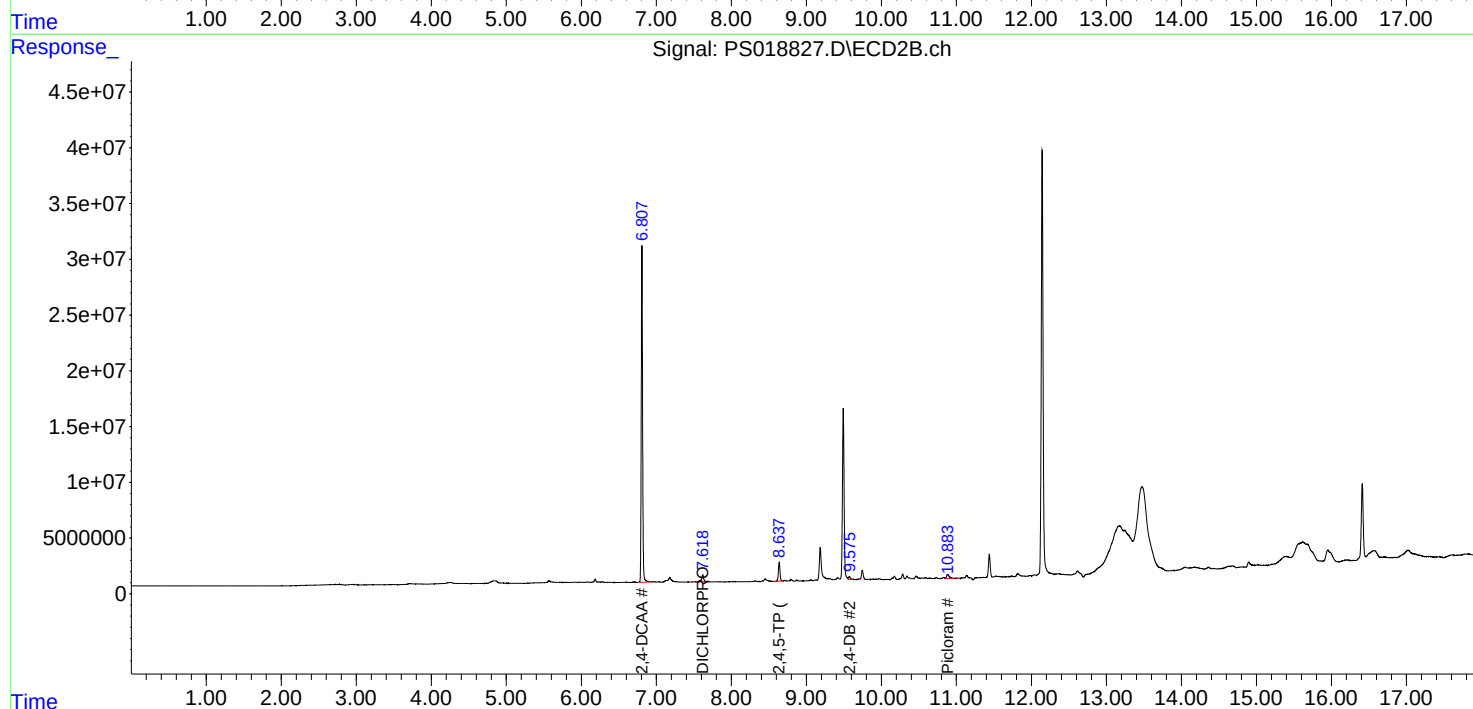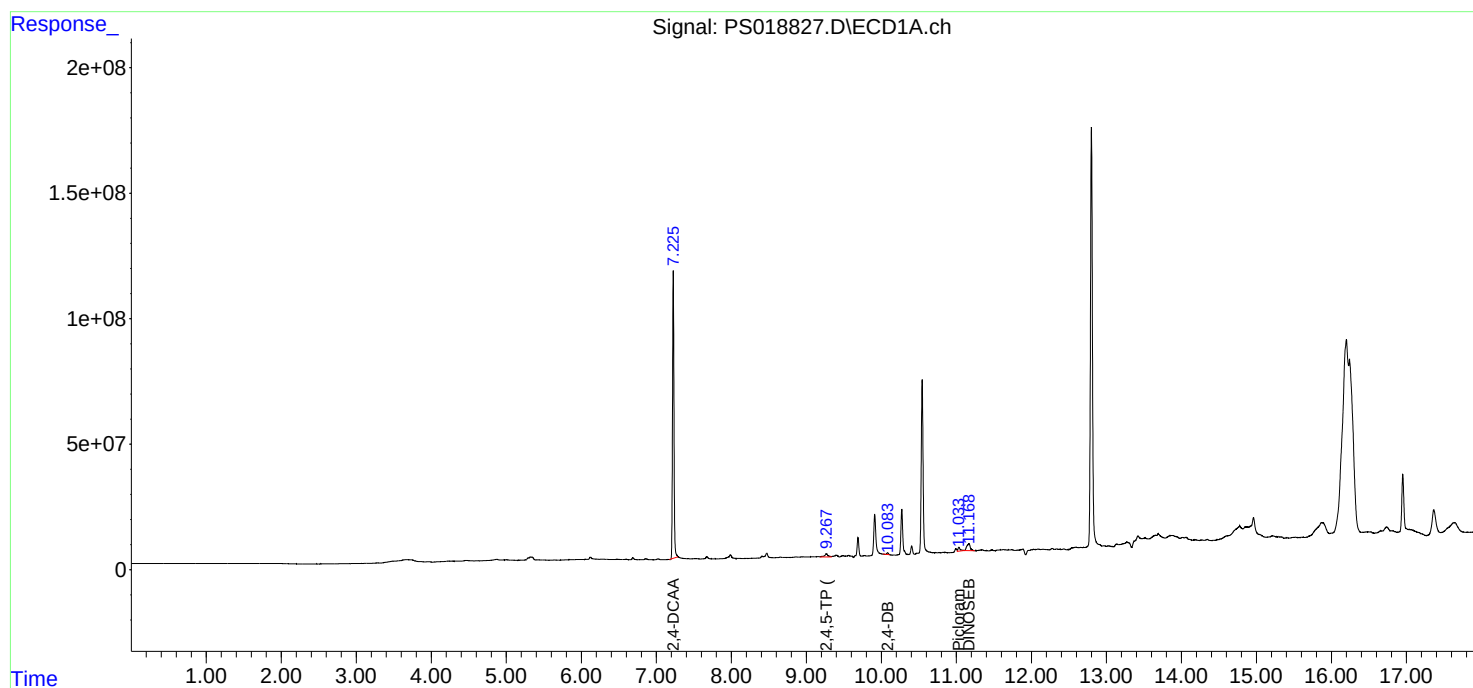


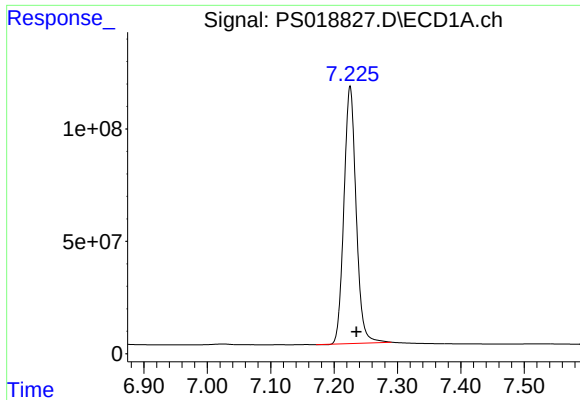

#4 2,4-DCAA


R.T.: 7.225 min
Delta R.T.: -0.010 min
Response: 1530356722
Conc: 537.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

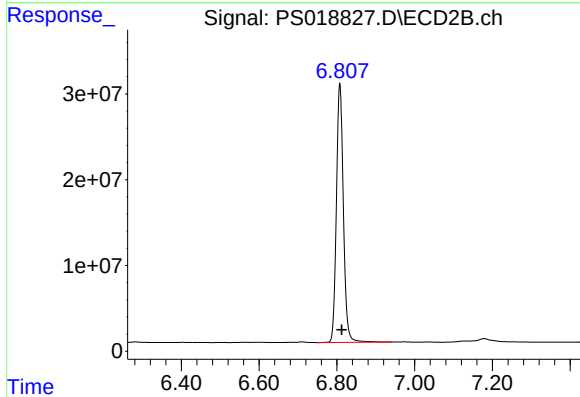


#4 2,4-DCAA

R.T.: 6.808 min
Delta R.T.: -0.005 min
Response: 373330082
Conc: 530.56 ng/ml

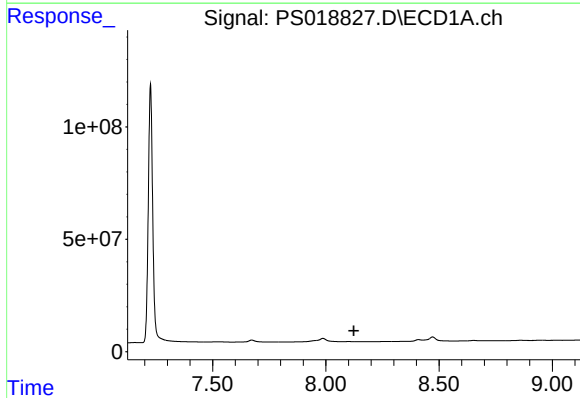


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.124 min
Response: 0
Conc: N.D.

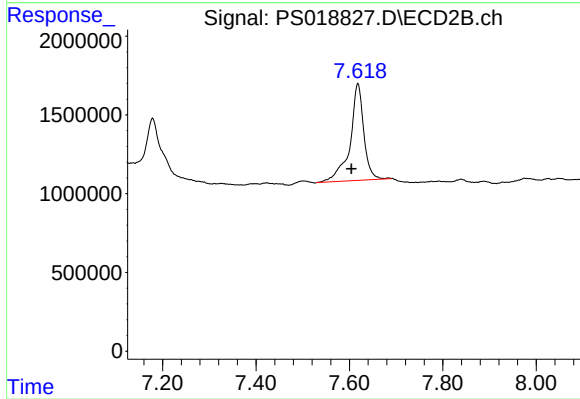

#8 DICHLORPROP


R.T.: 7.618 min
Delta R.T.: 0.014 min
Response: 12536202
Conc: 15.84 ng/ml

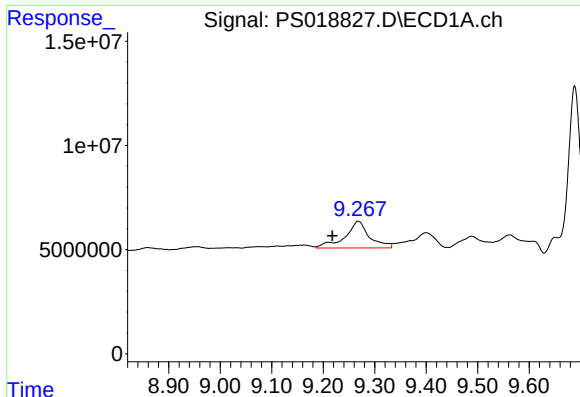

#11 2,4,5-TP (SILVEX)


R.T.: 9.268 min
Delta R.T.: 0.050 min
Response: 42259776
Conc: 2.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

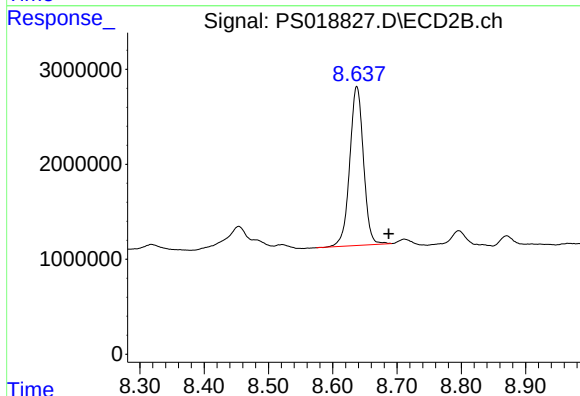


#11 2,4,5-TP (SILVEX)

R.T.: 8.637 min
Delta R.T.: -0.050 min
Response: 24855007
Conc: 5.70 ng/ml

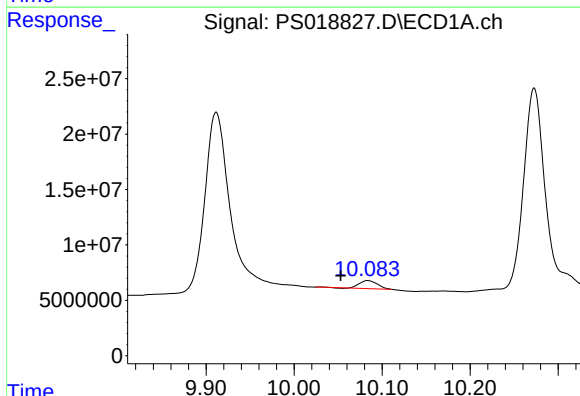


#13 2,4-DB

R.T.: 10.084 min
Delta R.T.: 0.031 min
Response: 9936550
Conc: 3.63 ng/ml

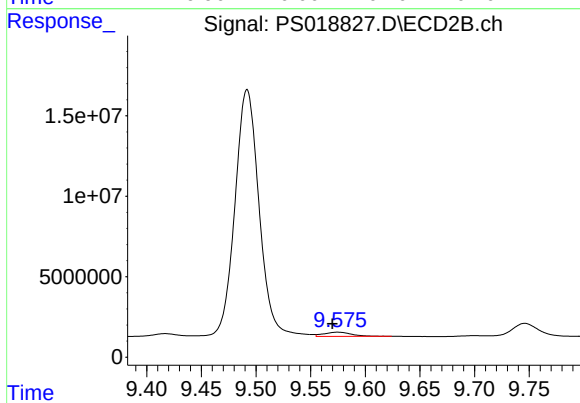

#13 2,4-DB


R.T.: 9.575 min
Delta R.T.: 0.005 min
Response: 4618672
Conc: 8.14 ng/ml

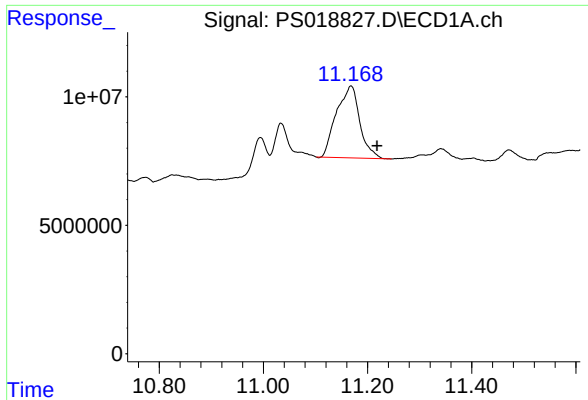

#14 DINOSEB


R.T.: 11.168 min
Delta R.T.: -0.050 min
Response: 87020982
Conc: 8.14 ng/ml

Instrument :
ECD_S
ClientSampleId :

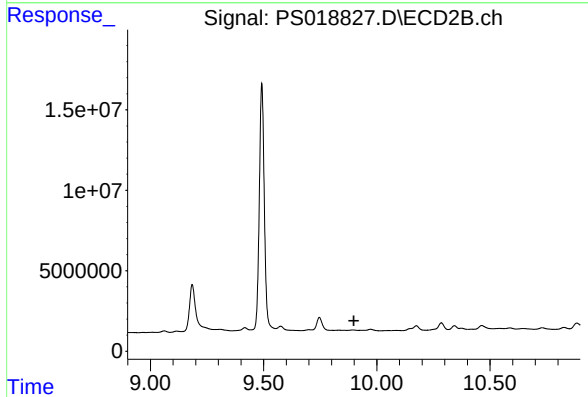


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.899 min
Response: 0
Conc: N.D.

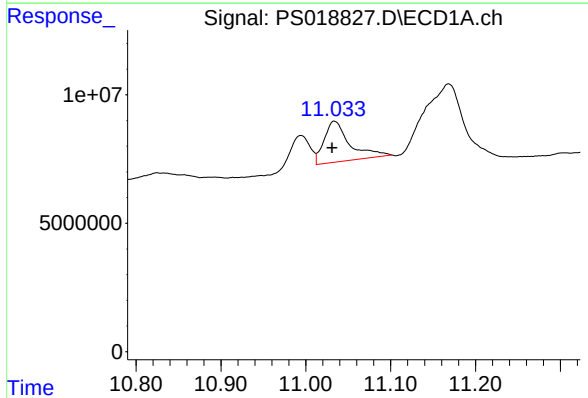

#15 Picloram

R.T.: 11.034 min
Delta R.T.: 0.003 min
Response: 33684936
Conc: 1.64 ng/ml

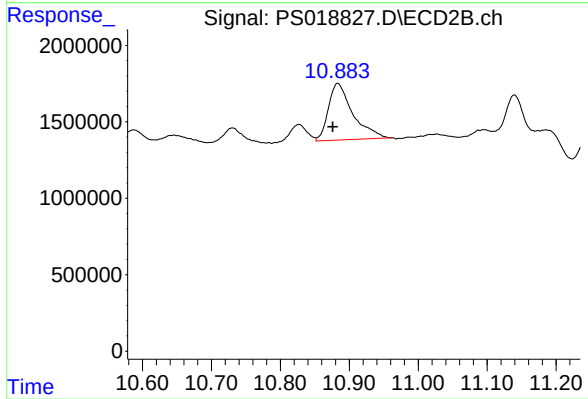

#15 Picloram

R.T.: 10.883 min
Delta R.T.: 0.007 min
Response: 9089021
Conc: 1.71 ng/ml