

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032922\
Data File : PS018819.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Mar 2022 01:25
Operator : AJ\MA
Sample : PB143700TB
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB143700TB

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/30/2022
Supervised By :mohammad ahmed 03/30/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 06:17:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.224	6.808	1579.4E6	395.9E6	554.976m	562.564m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032922\
Data File : PS018819.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Mar 2022 01:25
Operator : AJ\MA
Sample : PB143700TB
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
PB143700TB


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/30/2022
Supervised By : mohammad ahmed 03/30/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 06:17:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

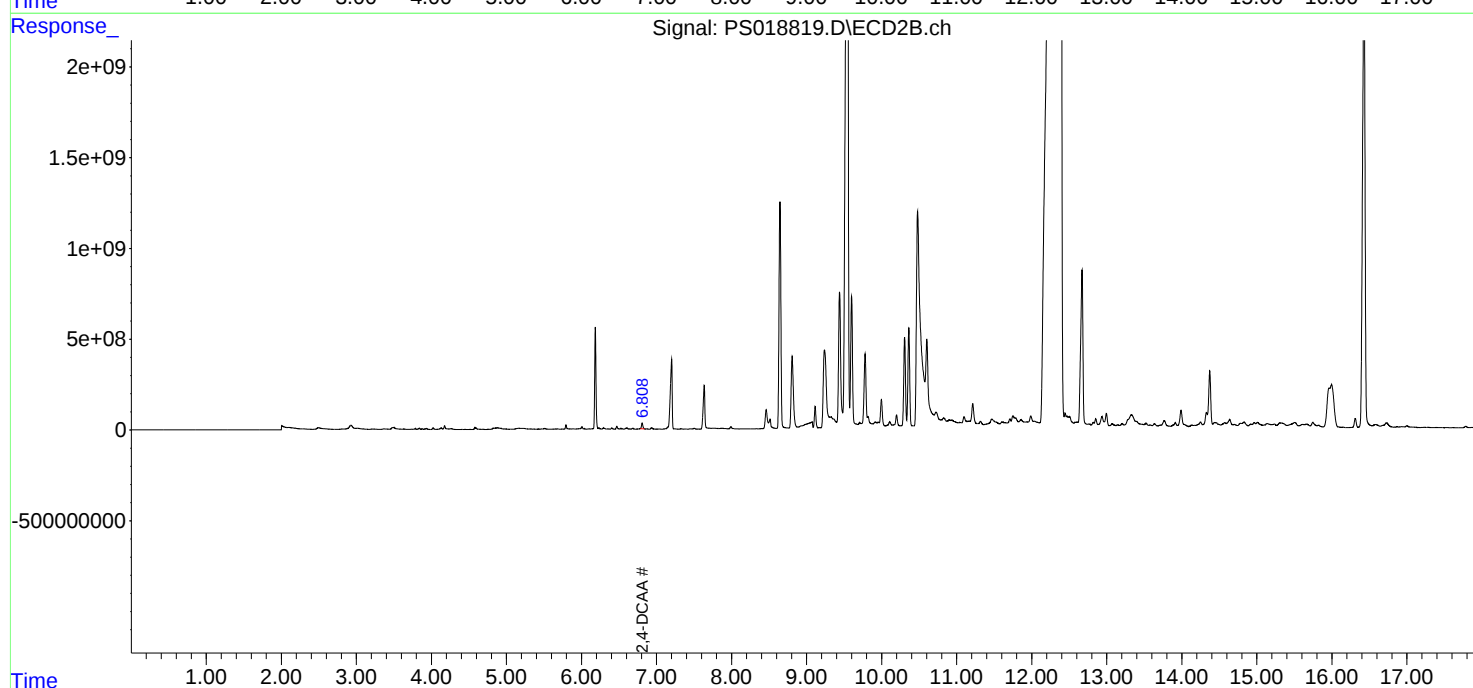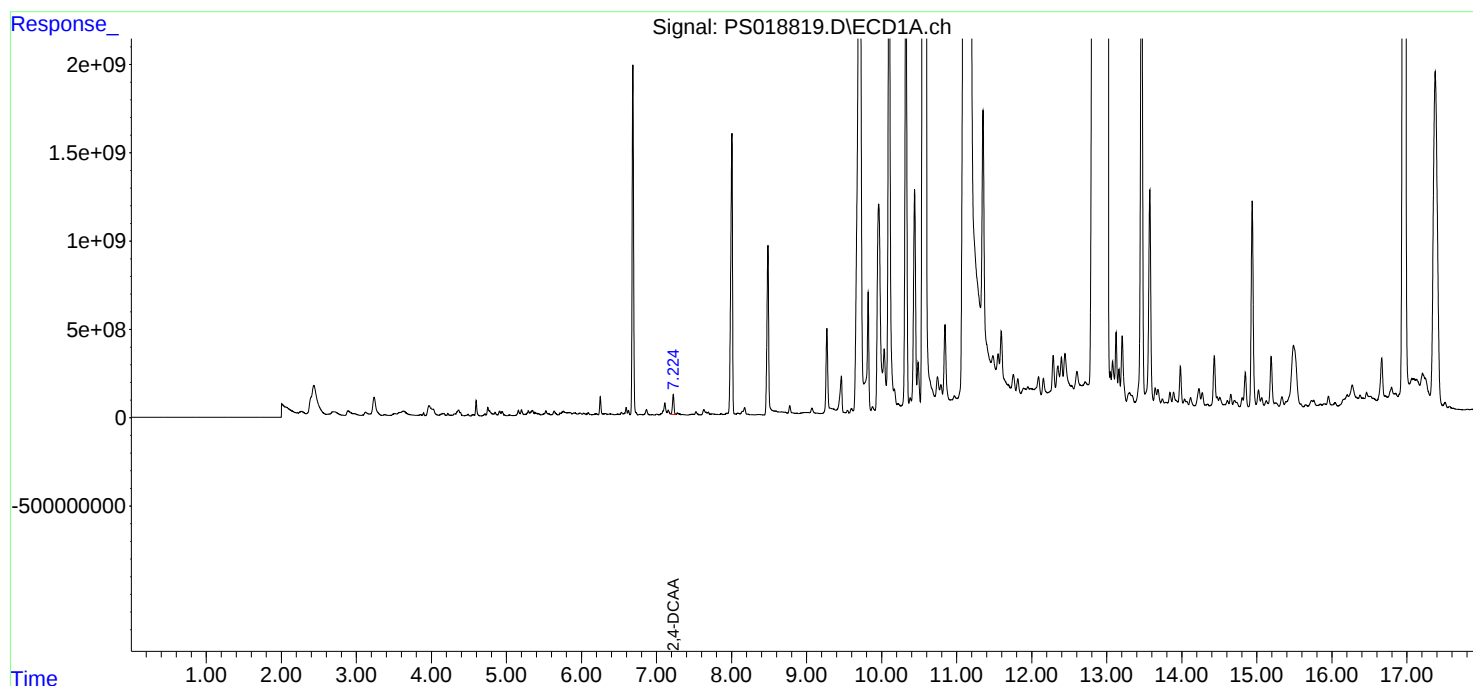

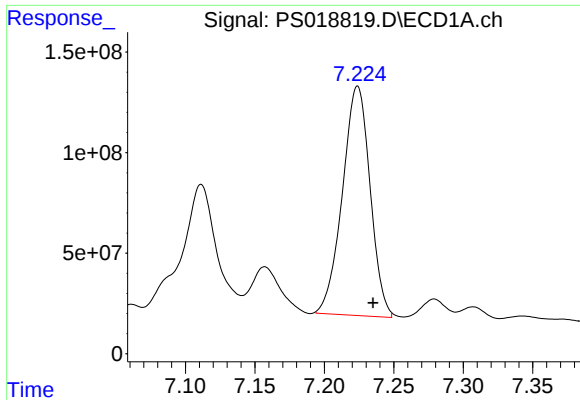


#4 2,4-DCAA

R.T.: 7.224 min
Delta R.T.: -0.011 min
Response: 1579414734
Conc: 554.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB143700TB

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/30/2022
Supervised By :mohammad ahmed 03/30/2022

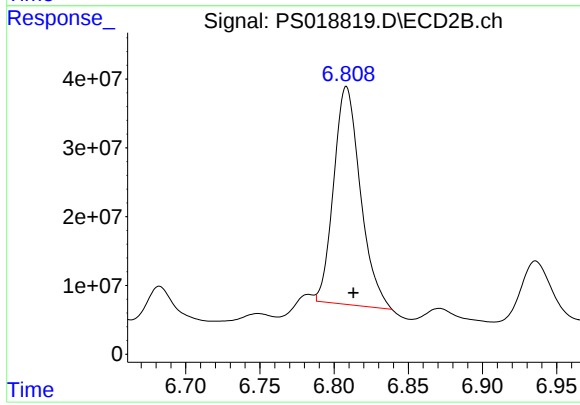

#4 2,4-DCAA

R.T.: 6.808 min
Delta R.T.: -0.005 min
Response: 395850665
Conc: 562.56 ng/ml m