

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032924\
 Data File : PS026283.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Mar 2024 09:44
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 04:24:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031924.M
 Quant Title : 8080.M
 QLast Update : Tue Mar 19 15:58:33 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.179	0.000	5033961	0	1.568	N.D. #
Target Compounds							
1) T	Dalapon	0.000	2.696	0	5268289	N.D.	2.772
2) T	3,5-DICHL...	6.348	0.000	10801169	0	2.311	N.D. #
3) T	4-Nitroph...	6.967	0.000	12642157	0	7.249	N.D. #
5) T	DICAMBA	7.368	7.872	871552	1292260	<MDL	<MDL #
6) T	MCP	7.600	7.973f	14757633	29551086	1.519	9.253 #
7) T	MCPA	7.729	0.000	1464206	0	<MDL	N.D. #
8) T	DICHLORPROP	8.106	8.633	2051341	2613148	<MDL	2.413 #
9) T	2,4-D	8.317	8.992f	314.4E6	1990113	88.042	1.933 #
10) T	Pentachlo...	8.628	9.498	2092871	276600	<MDL	<MDL #
11) T	2,4,5-TP ...	9.174	9.810	6063429	3032575	<MDL	<MDL #
12) T	2,4,5-T	9.469	10.287	6831366	2664089	<MDL	<MDL #
13) T	2,4-DB	10.037	10.862f	874493	1207394	<MDL	2.005 #
14) T	DINOSEB	11.240	11.164	4909111	1877896	<MDL	<MDL #
15) T	Picloram	11.032	12.251	109.1E6	3576358	4.785	<MDL #
16) T	DCPA	11.541	12.251	18457782	3576358	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032924\
Data File : PS026283.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Mar 2024 09:44
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 04:24:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031924.M
Quant Title : 8080.M
QLast Update : Tue Mar 19 15:58:33 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

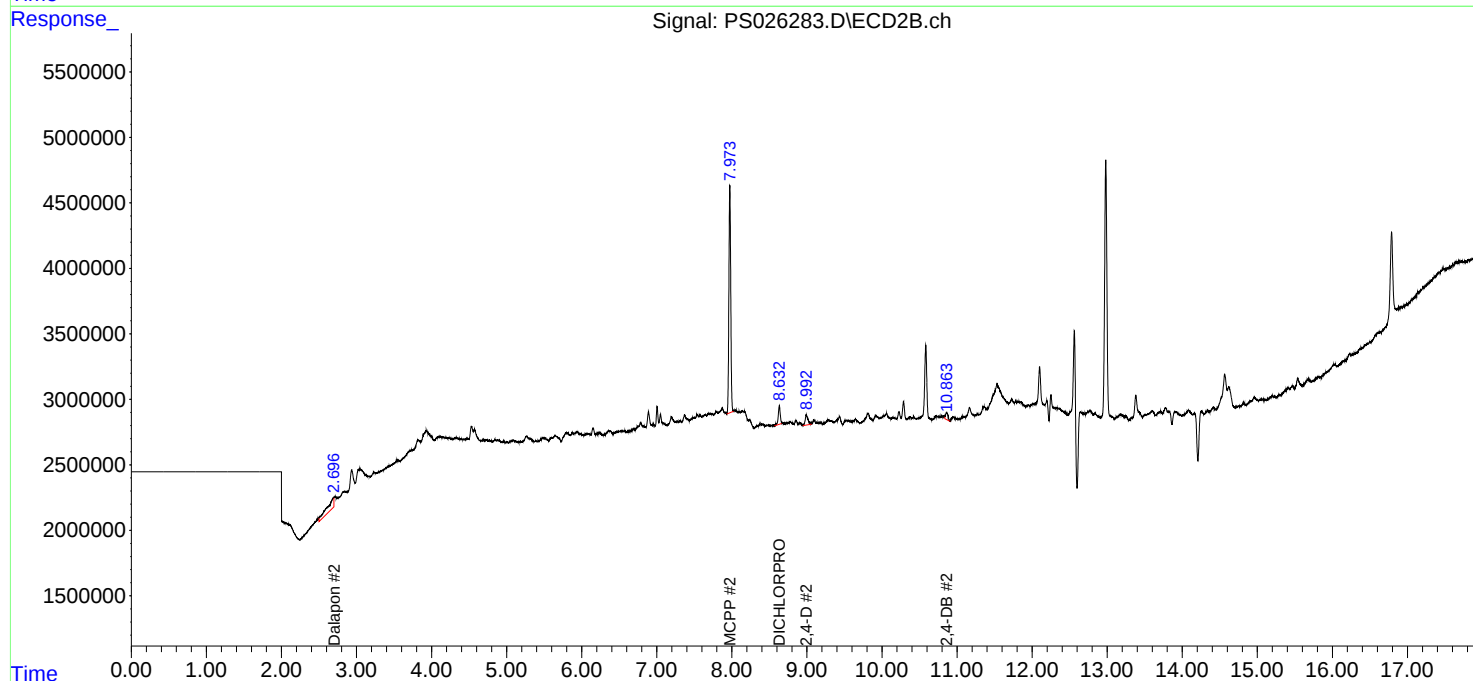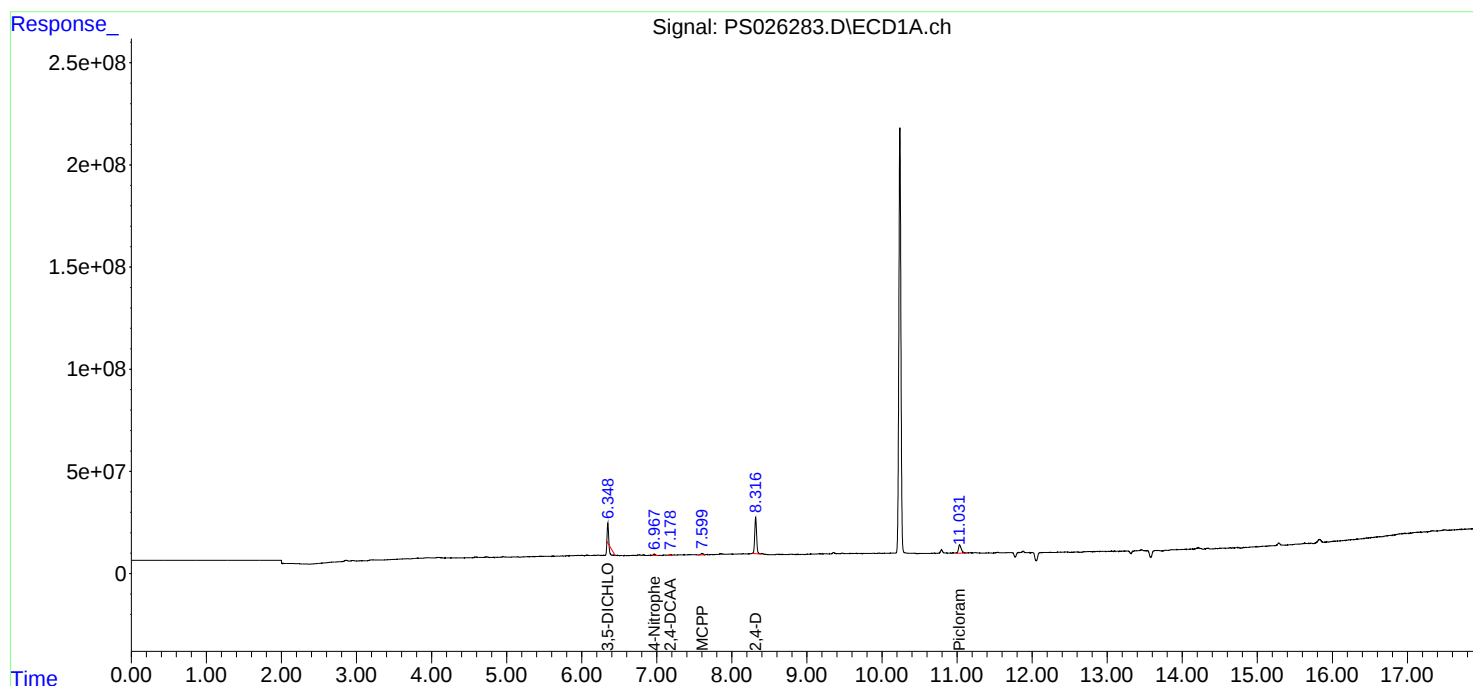


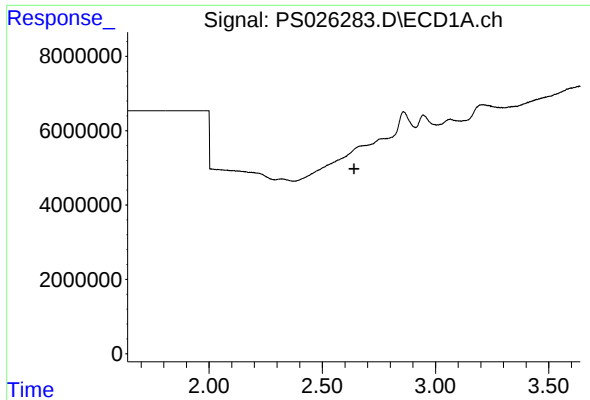

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.640 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

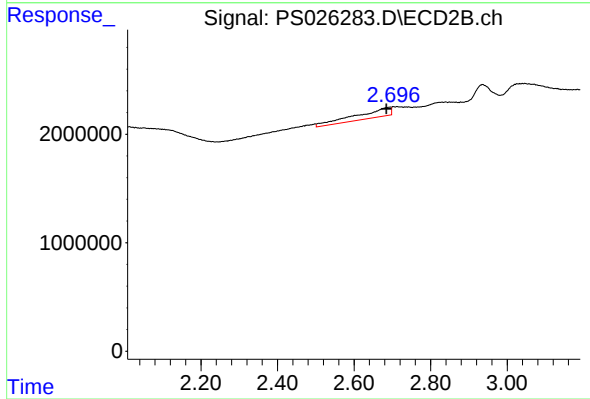


#1 Dalapon

R.T.: 2.696 min
Delta R.T.: 0.011 min
Response: 5268289
Conc: 2.77 ng/ml

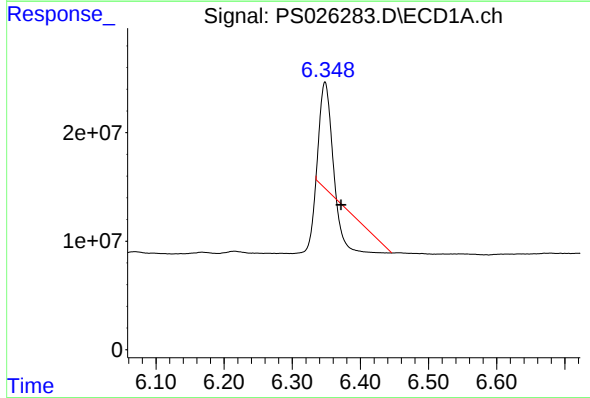


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.348 min
Delta R.T.: -0.024 min
Response: 10801169
Conc: 2.31 ng/ml

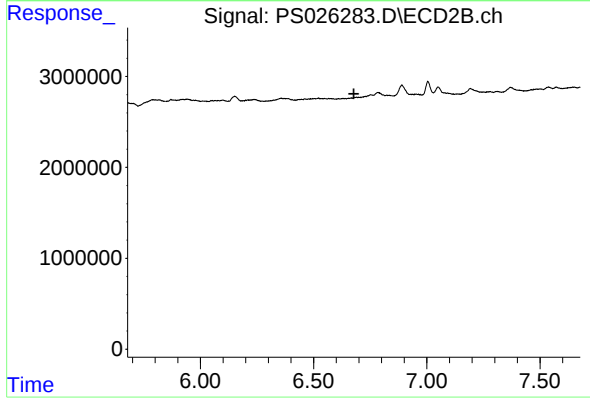

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.678 min
Response: 0
Conc: N.D.

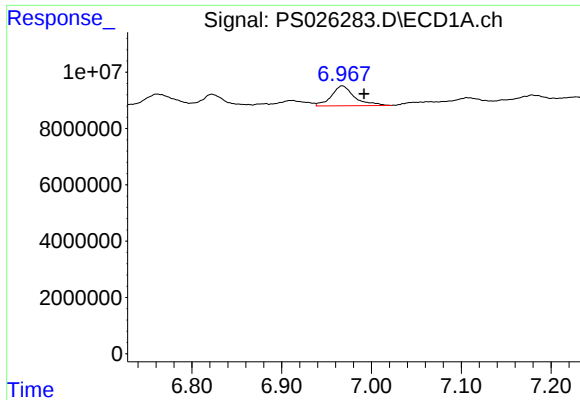

#3 4-Nitrophenol


R.T.: 6.967 min
Delta R.T.: -0.024 min
Response: 12642157
Conc: 7.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

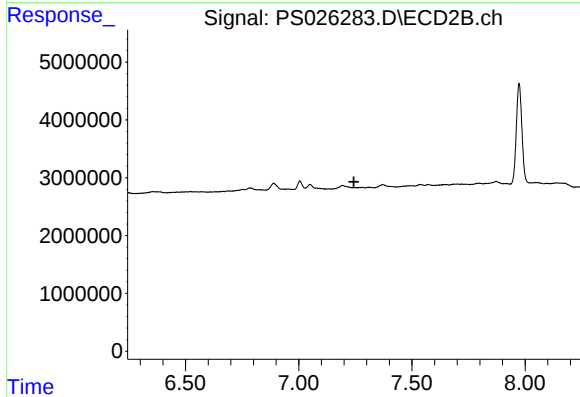


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.244 min
Response: 0
Conc: N.D.

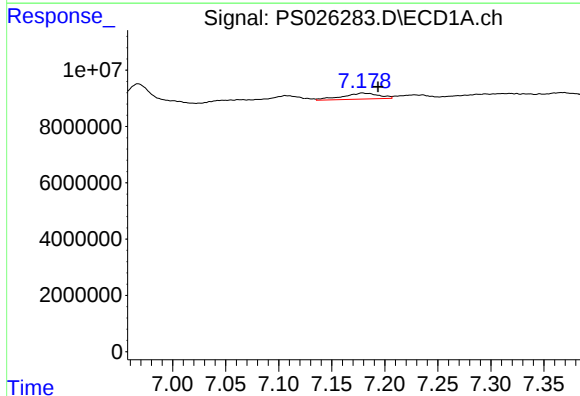


#4 2,4-DCAA

R.T.: 7.179 min
Delta R.T.: -0.015 min
Response: 5033961
Conc: 1.57 ng/ml

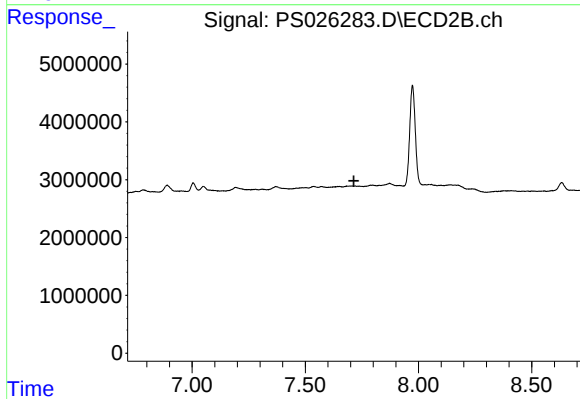

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.715 min
Response: 0
Conc: N.D.

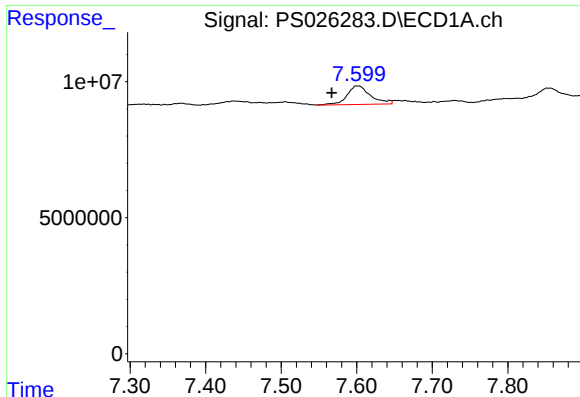

#6 MCP


R.T.: 7.600 min
Delta R.T.: 0.034 min
Response: 14757633
Conc: 1.52 ug/ml

Instrument :
ECD_S
ClientSampleId :

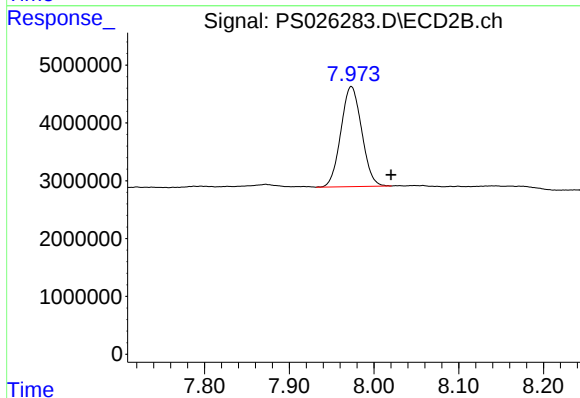


#6 MCP

R.T.: 7.973 min
Delta R.T.: -0.047 min
Response: 29551086
Conc: 9.25 ug/ml

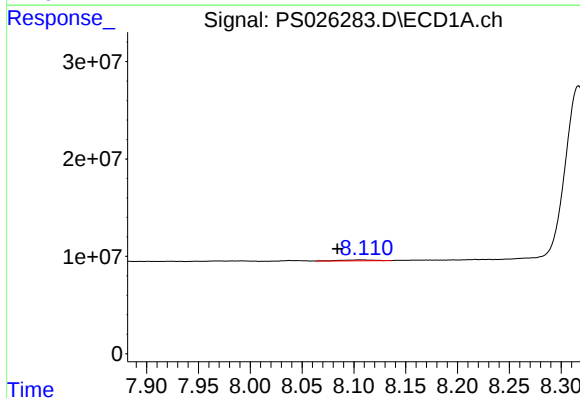


#8 DICHLORPROP

R.T.: 8.106 min
Delta R.T.: 0.021 min
Response: 2051341
Conc: N.D.

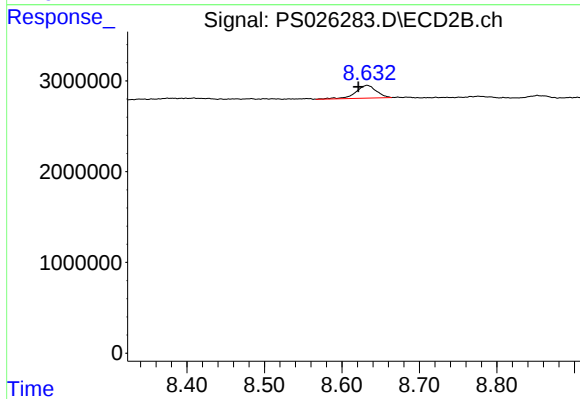

#8 DICHLORPROP


R.T.: 8.633 min
Delta R.T.: 0.011 min
Response: 2613148
Conc: 2.41 ng/ml

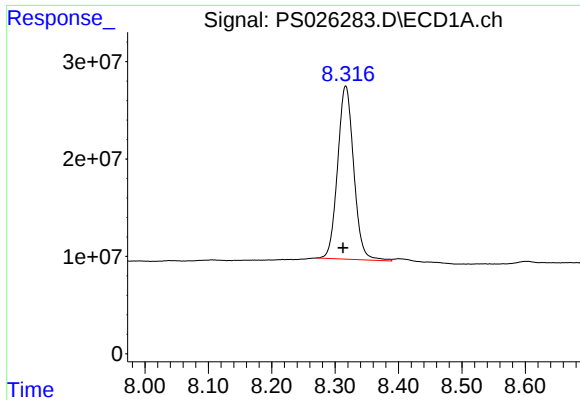

#9 2,4-D


R.T.: 8.317 min
Delta R.T.: 0.004 min
Response: 314377469
Conc: 88.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

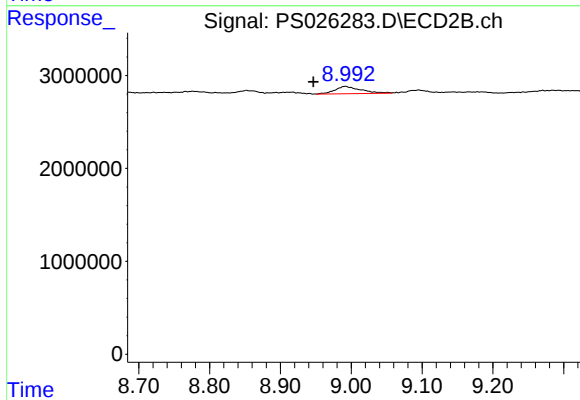


#9 2,4-D

R.T.: 8.992 min
Delta R.T.: 0.045 min
Response: 1990113
Conc: 1.93 ng/ml

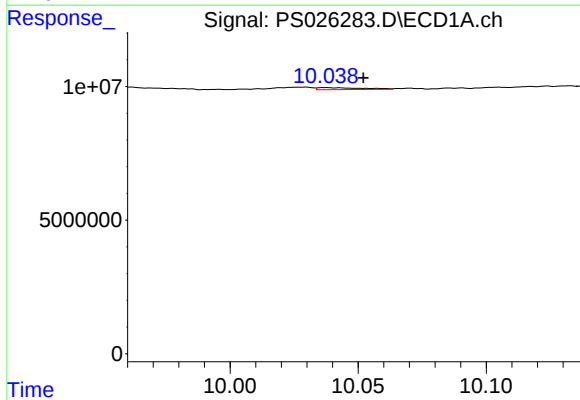


#13 2,4-DB

R.T.: 10.037 min
Delta R.T.: -0.015 min
Response: 874493
Conc: N.D.

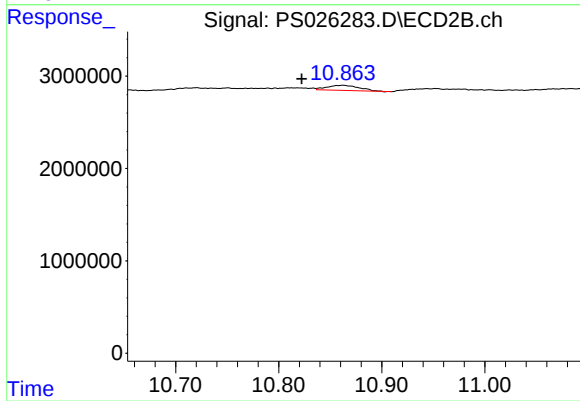

#13 2,4-DB


R.T.: 10.862 min
Delta R.T.: 0.040 min
Response: 1207394
Conc: 2.01 ng/ml

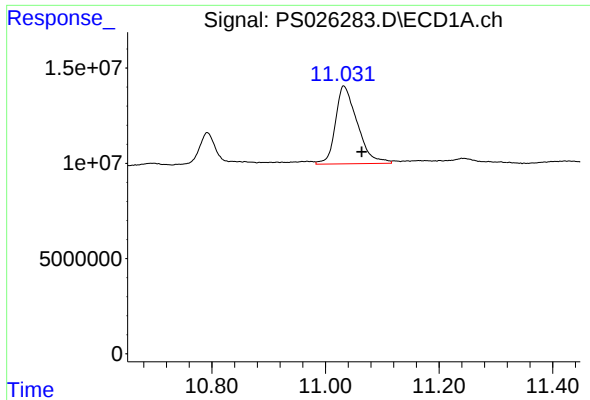

#15 Picloram

R.T.: 11.032 min
Delta R.T.: -0.032 min
Response: 109087334
Conc: 4.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

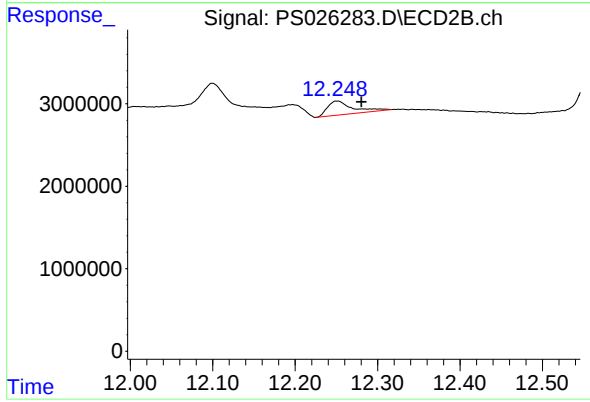

#15 Picloram

R.T.: 12.251 min
Delta R.T.: -0.029 min
Response: 3576358
Conc: N.D.