

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032925\
Data File : PS029623.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2025 16:05
Operator : AR\AJ
Sample : Q1662-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-7

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/31/2025
Supervised By :mohammad ahmed 04/01/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 23:16:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032825.M
Quant Title : 8080.M
QLast Update : Thu Mar 27 12:24:58 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.114	7.532	1177.0E6	204.6E6	306.490m	237.042

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032925\
Data File : PS029623.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2025 16:05
Operator : AR\AJ
Sample : Q1662-05
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
TP-7


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/31/2025
Supervised By : mohammad ahmed 04/01/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 23:16:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032825.M
Quant Title : 8080.M
QLast Update : Thu Mar 27 12:24:58 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

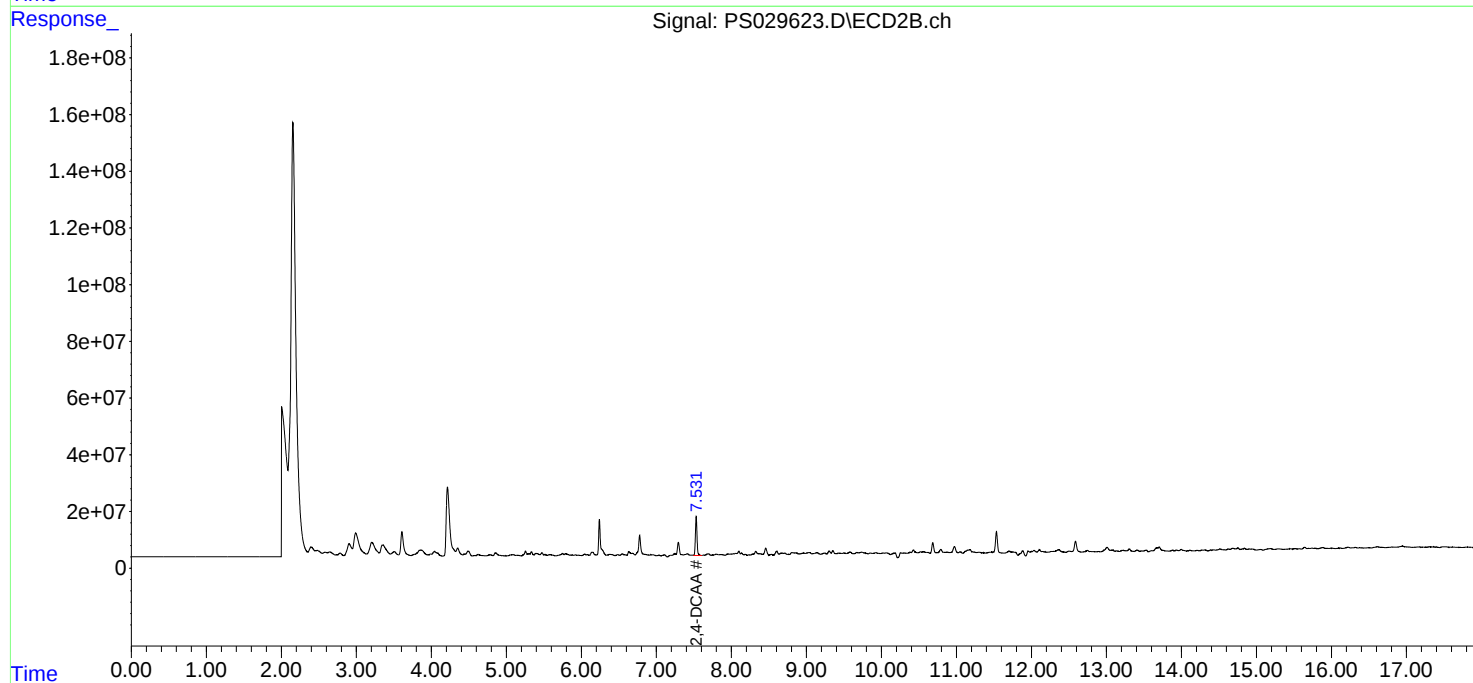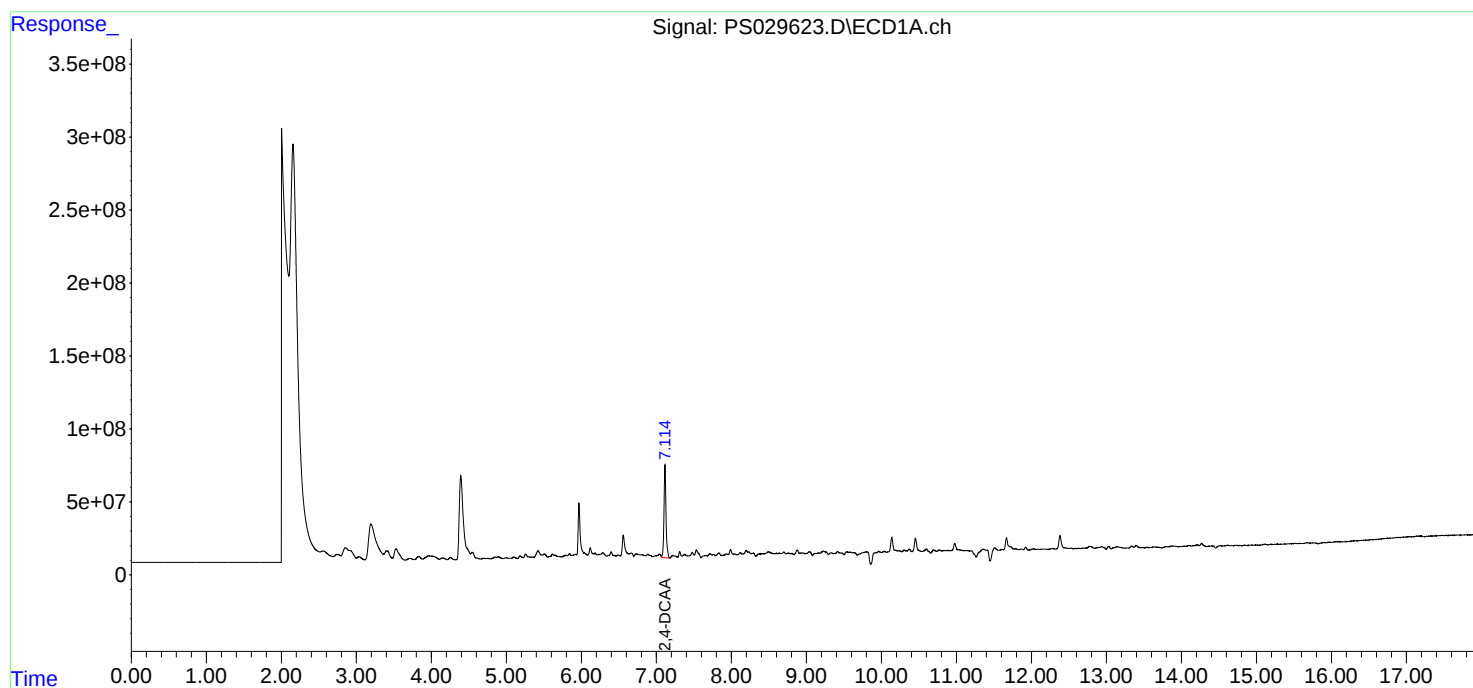

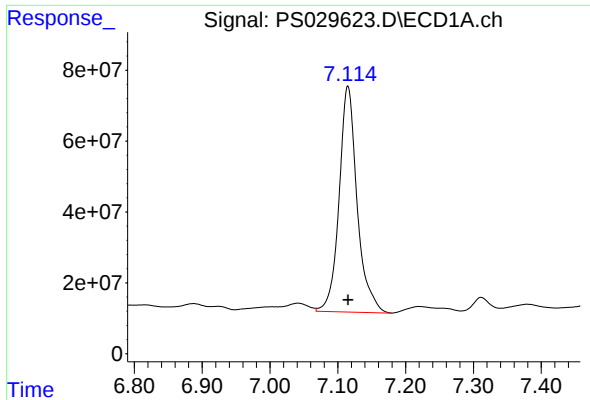


#4 2,4-DCAA

R.T.: 7.114 min
Delta R.T.: 0.000 min
Response: 1176951477
Conc: 306.49 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-7

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/31/2025
Supervised By :mohammad ahmed 04/01/2025

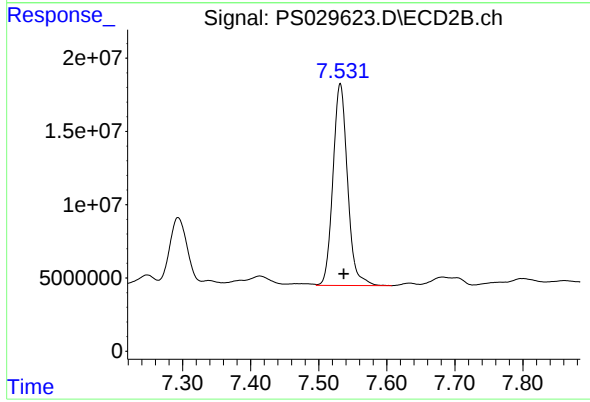

#4 2,4-DCAA

R.T.: 7.532 min
Delta R.T.: -0.005 min
Response: 204637940
Conc: 237.04 ng/ml