

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS033019\
 Data File : PS003850.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2019 08:20
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 01:43:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.769	0	78065	N.D.	0.159 #
Target Compounds							
2) T	3,5-DICHL...	0.000	8.918	0	256679	N.D.	0.402 #
3) T	4-Nitroph...	0.000	9.918	0	52524	N.D.	0.231 #
6) T	MCP	0.000	11.294	0	357066	N.D.	0.302 #
7) T	MCPA	0.000	11.690	0	105604	N.D.	0.059 #
8) T	DICHLORPROP	0.000	12.235	0	47578	N.D.	0.102 #
9) T	2,4-D	0.000	12.670	0	122677	N.D.	0.231 #
10) T	Pentachlo...	0.000	13.168	0	151627	N.D.	0.022 #
11) T	2,4,5-TP ...	0.000	13.799	0	403905	N.D.	0.153 #
12) T	2,4,5-T	0.000	14.355	0	241427	N.D.	0.111 #
13) T	2,4-DB	0.000	14.968	0	235196	N.D.	0.792 #
14) T	DINOSEB	0.000	15.442	0	79441	N.D.	0.041 #
15) T	Picloram	0.000	16.619	0	6734041	N.D.	2.123 #
16) T	DCPA	0.000	16.619	0	6734041	N.D.	1.992 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS033019\
Data File : PS003850.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Mar 2019 08:20
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 01:43:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

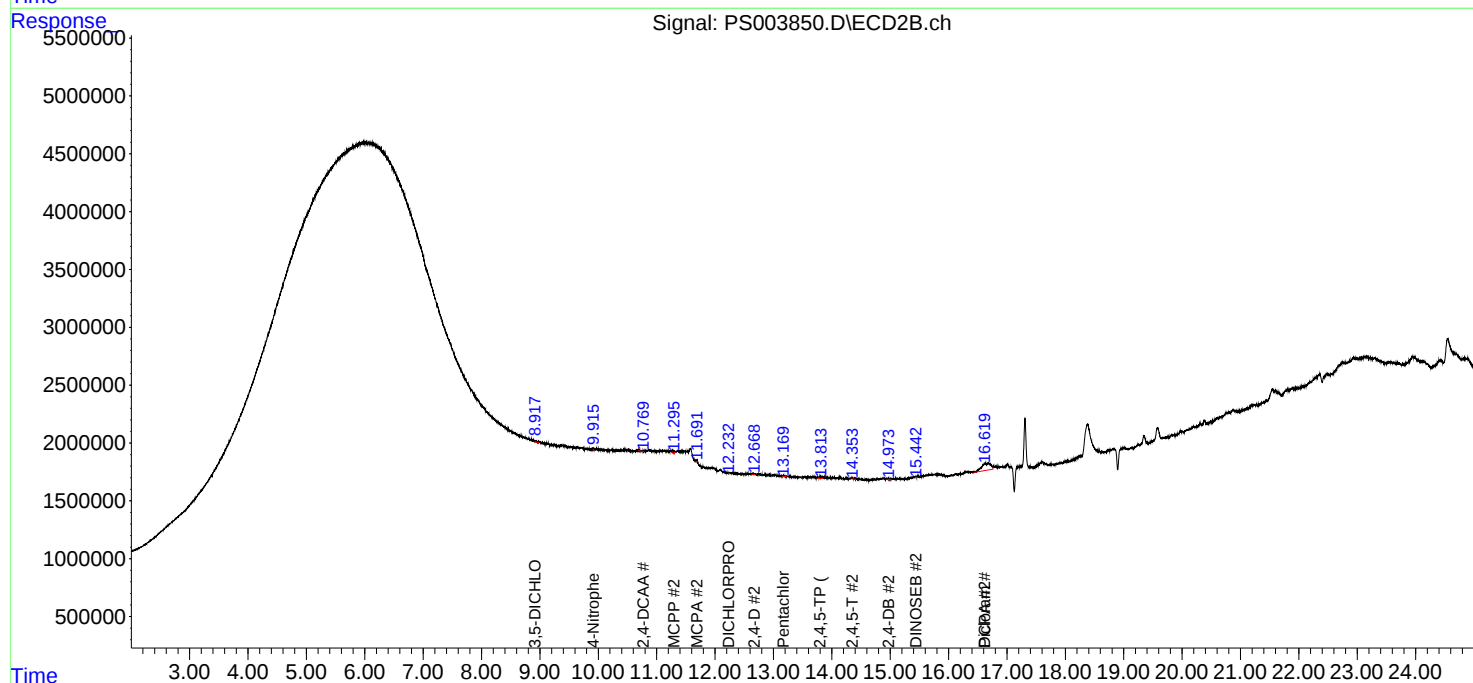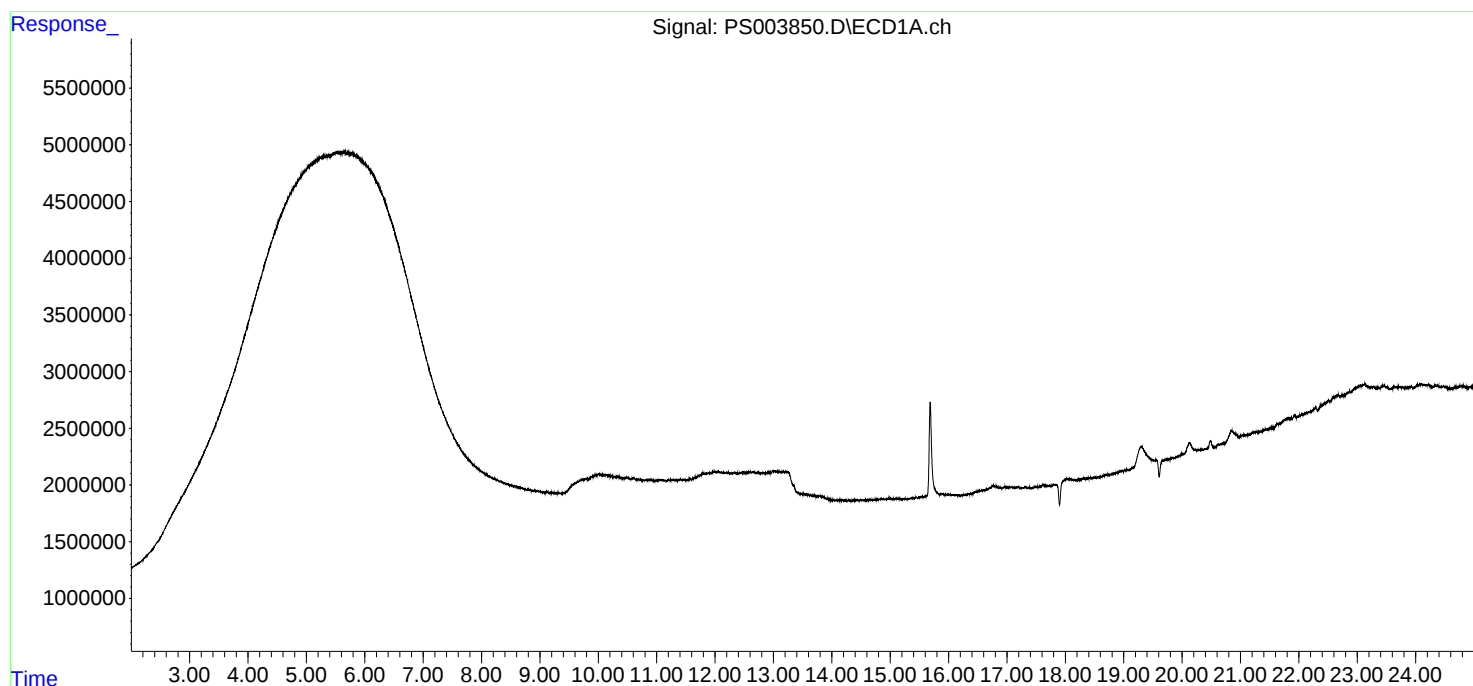


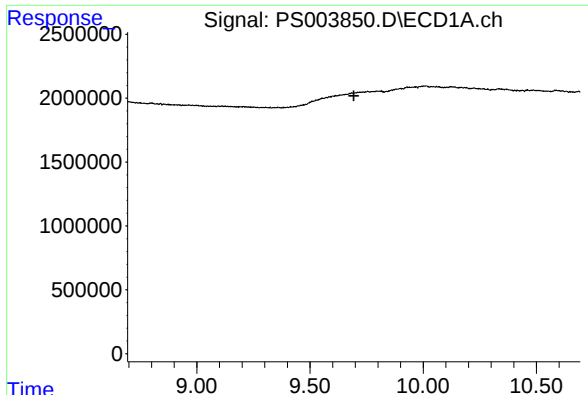

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.693 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

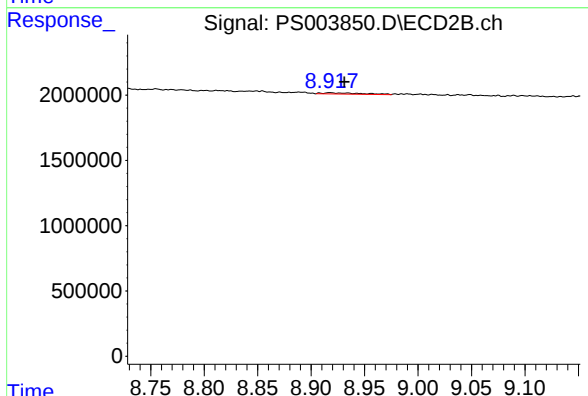


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.918 min
Delta R.T.: -0.013 min
Response: 256679
Conc: 0.40 ng/ml

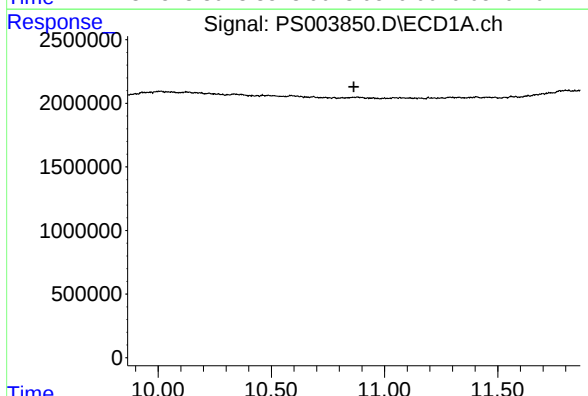


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

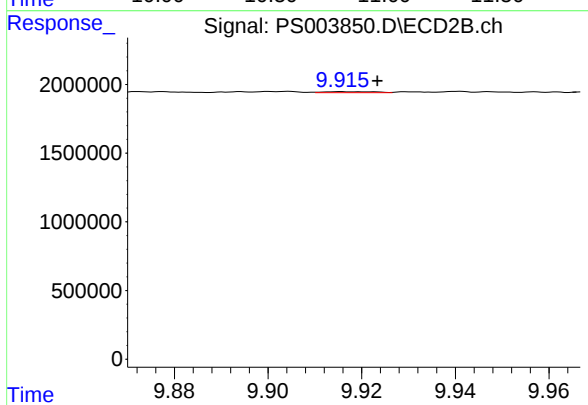

#3 4-Nitrophenol


R.T.: 9.918 min
Delta R.T.: -0.006 min
Response: 52524
Conc: 0.23 ng/ml

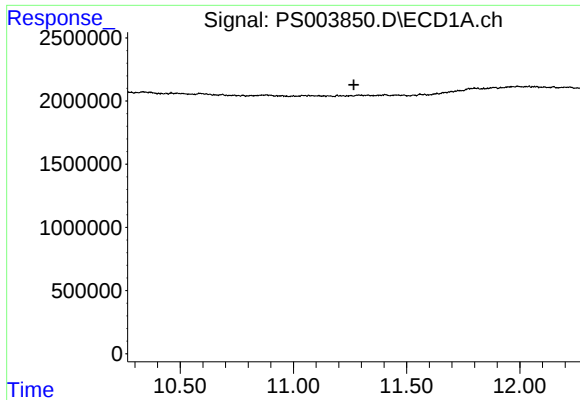

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 11.267 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

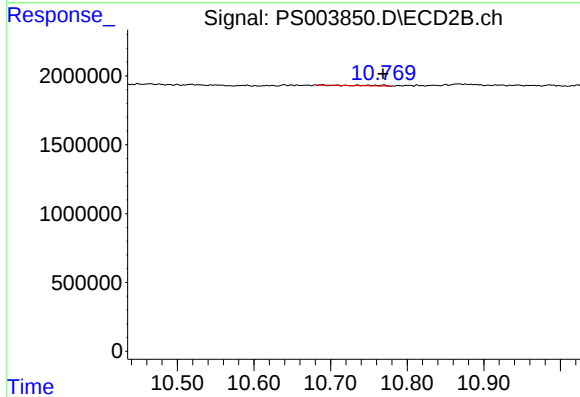


#4 2,4-DCAA

R.T.: 10.769 min
Delta R.T.: 0.000 min
Response: 78065
Conc: 0.16 ng/ml

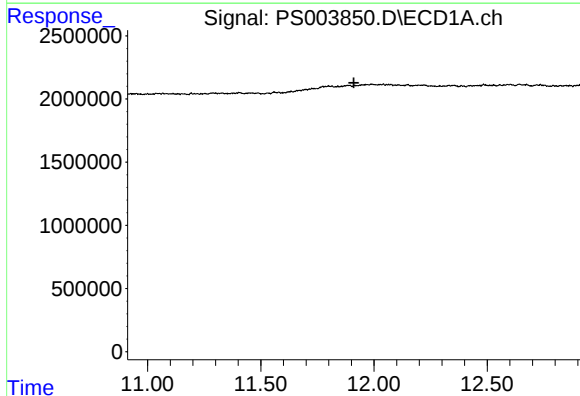


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 11.911 min
Response: 0
Conc: N.D.

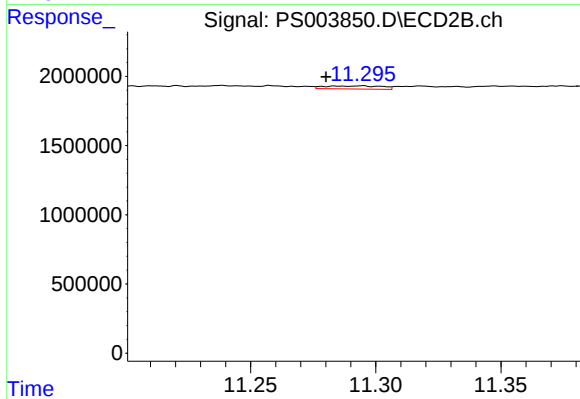

#6 MCPP


R.T.: 11.294 min
Delta R.T.: 0.014 min
Response: 357066
Conc: 0.30 ug/ml

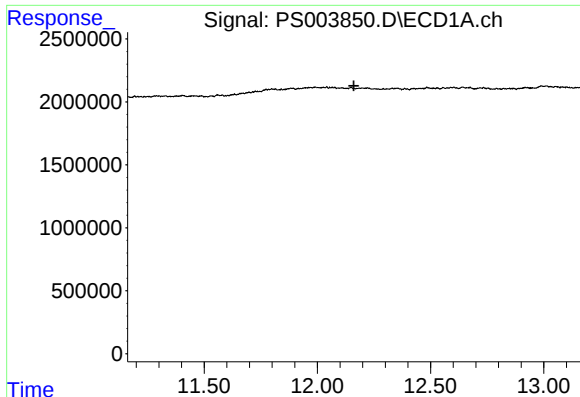

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.162 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

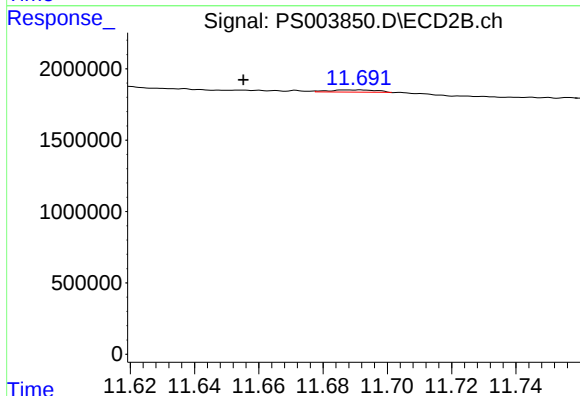


#7 MCPA

R.T.: 11.690 min
Delta R.T.: 0.034 min
Response: 105604
Conc: 0.06 ug/ml

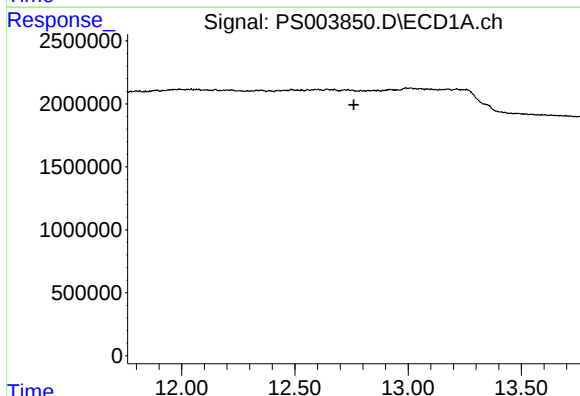


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 12.760 min
Response: 0
Conc: N.D.

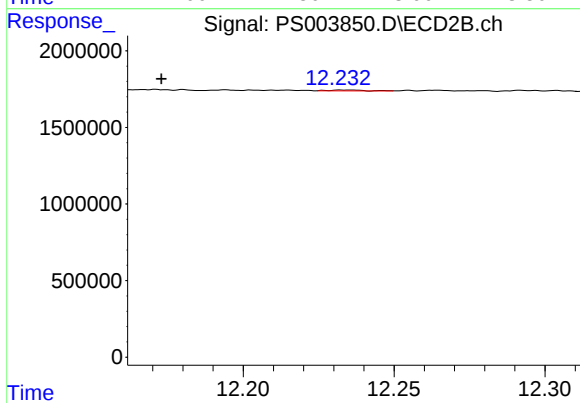

#8 DICHLORPROP


R.T.: 12.235 min
Delta R.T.: 0.062 min
Response: 47578
Conc: 0.10 ng/ml

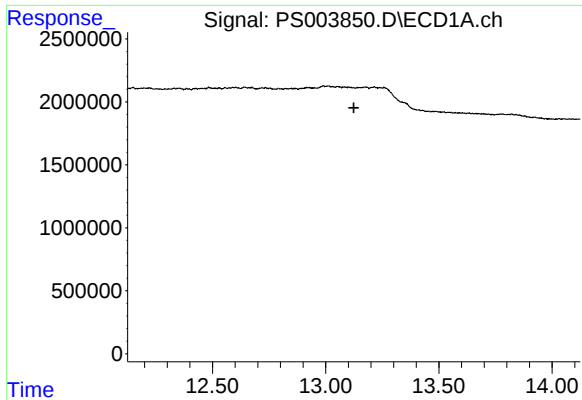

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

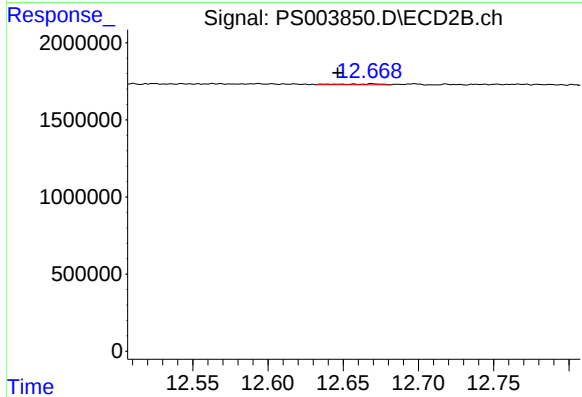


#9 2,4-D

R.T.: 12.670 min
Delta R.T.: 0.023 min
Response: 122677
Conc: 0.23 ng/ml

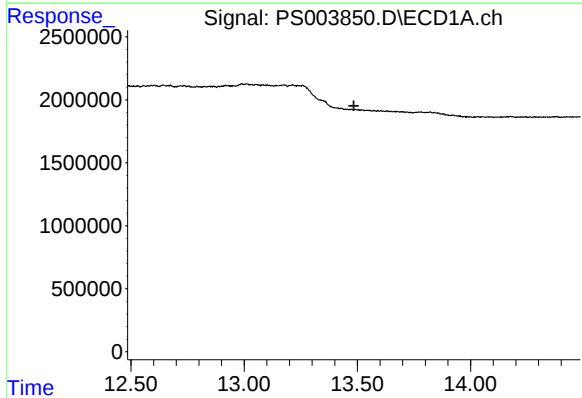


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.485 min
Response: 0
Conc: N.D.

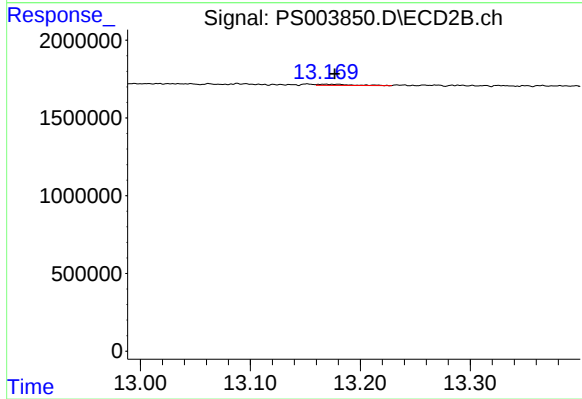

#10 Pentachlorophenol


R.T.: 13.168 min
Delta R.T.: -0.009 min
Response: 151627
Conc: 0.02 ng/ml

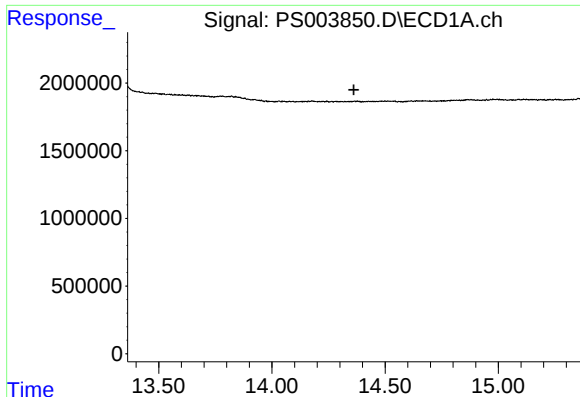

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

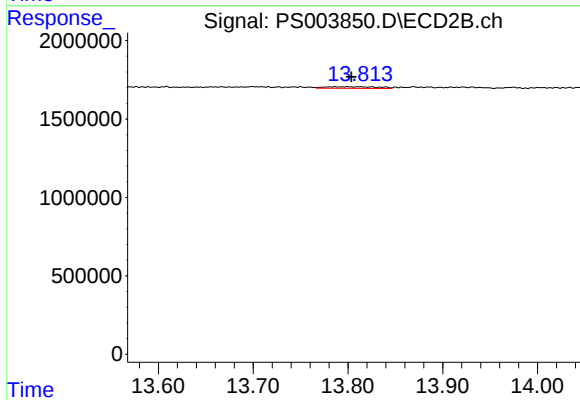


#11 2,4,5-TP (SILVEX)

R.T.: 13.799 min
Delta R.T.: -0.005 min
Response: 403905
Conc: 0.15 ng/ml

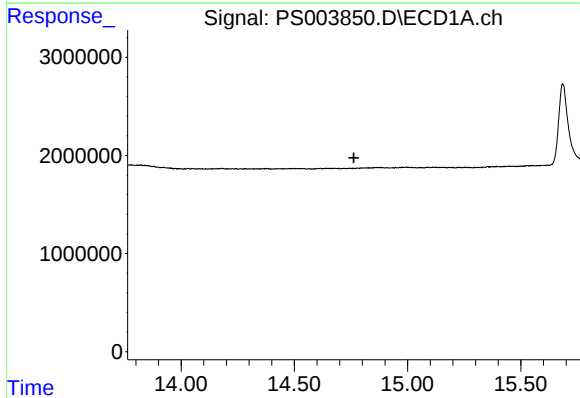


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.763 min
Response: 0
Conc: N.D.

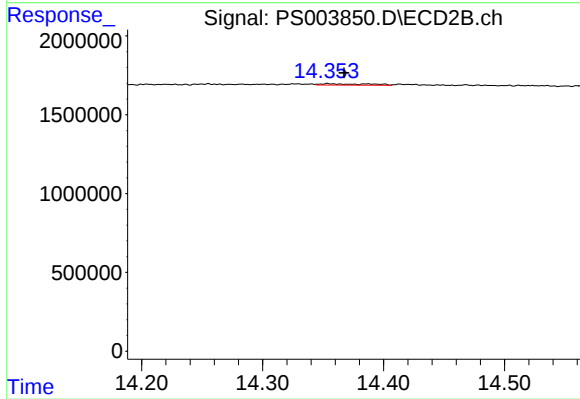

#12 2,4,5-T


R.T.: 14.355 min
Delta R.T.: -0.013 min
Response: 241427
Conc: 0.11 ng/ml

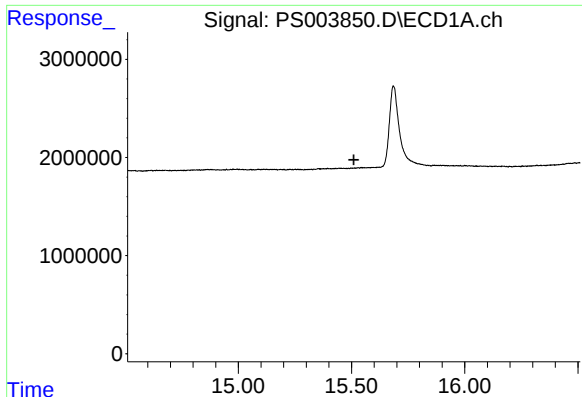

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

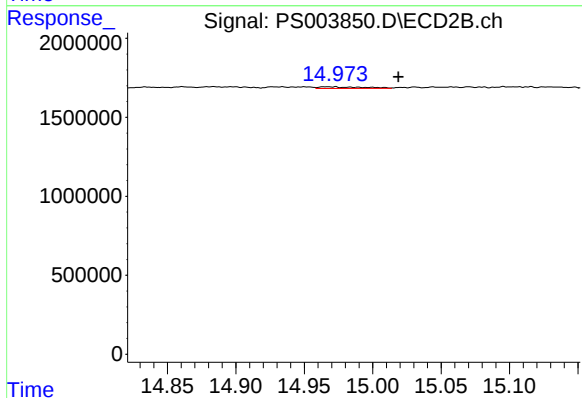


#13 2,4-DB

R.T.: 14.968 min
Delta R.T.: -0.051 min
Response: 235196
Conc: 0.79 ng/ml

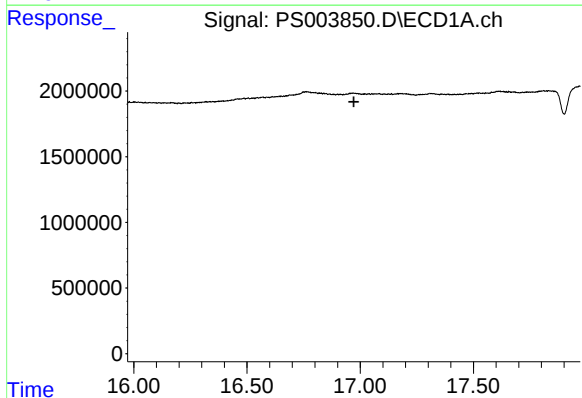


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.972 min
Response: 0
Conc: N.D.

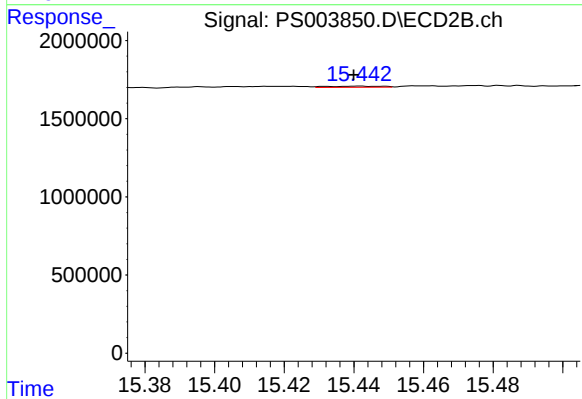

#14 DINOSEB


R.T.: 15.442 min
Delta R.T.: 0.002 min
Response: 79441
Conc: 0.04 ng/ml

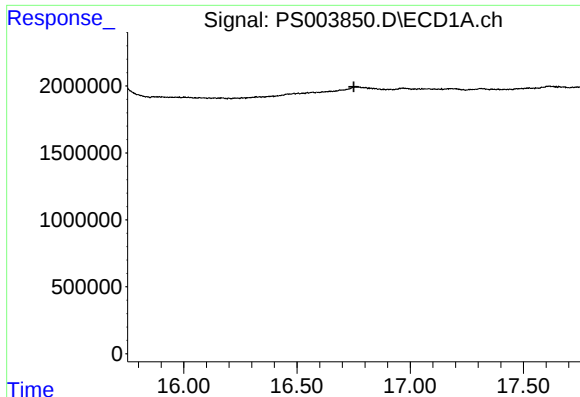

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.752 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

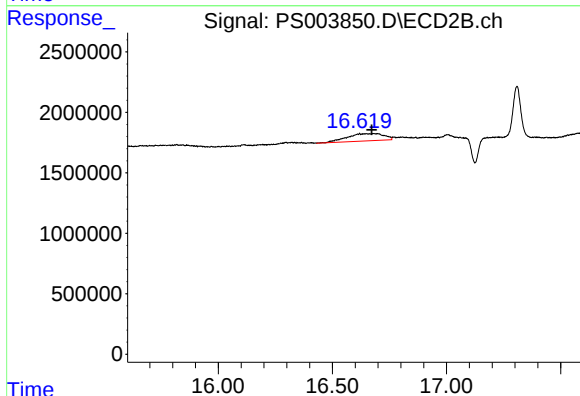


#15 Picloram

R.T.: 16.619 min
Delta R.T.: -0.054 min
Response: 6734041
Conc: 2.12 ng/ml

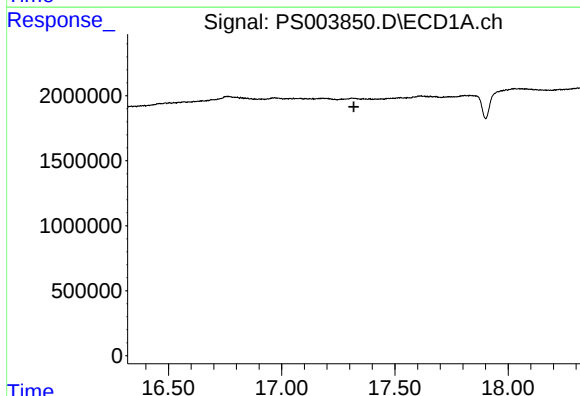

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

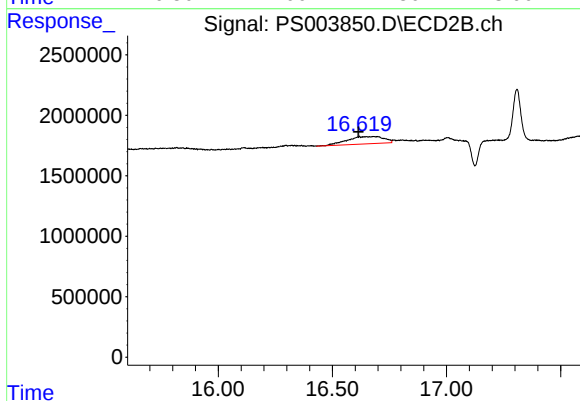

#16 DCPA

R.T.: 16.619 min
Delta R.T.: 0.004 min
Response: 6734041
Conc: 1.99 ng/ml