

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS033019\
 Data File : PS003851.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2019 08:51
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 01:43:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.303	10.735	198.1E6	20383	454.089	0.042 #
Target Compounds							
6) T	MCP	0.000	11.328	0	97433	N.D.	0.083 #
7) T	MCPA	0.000	11.690	0	238177	N.D.	0.134 #
8) T	DICHLORPROP	0.000	12.169	0	6100965	N.D.	13.105 #
9) T	2,4-D	0.000	12.615	0	409908	N.D.	0.771 #
10) T	Pentachlo...	0.000	13.217	0	1026308	N.D.	0.148 #
11) T	2,4,5-TP ...	0.000	13.785	0	10335	N.D.	0.004 #
12) T	2,4,5-T	0.000	14.334	0	65222	N.D.	0.030 #
13) T	2,4-DB	0.000	15.002	0	1981911	N.D.	6.674 #
14) T	DINOSEB	0.000	15.470	0	5581277	N.D.	2.909 #
15) T	Picloram	16.766	16.694	56645425	305004	16.675	0.096 #
16) T	DCPA	0.000	16.650	0	1709540	N.D.	0.506 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS033019\
Data File : PS003851.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Mar 2019 08:51
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 01:43:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

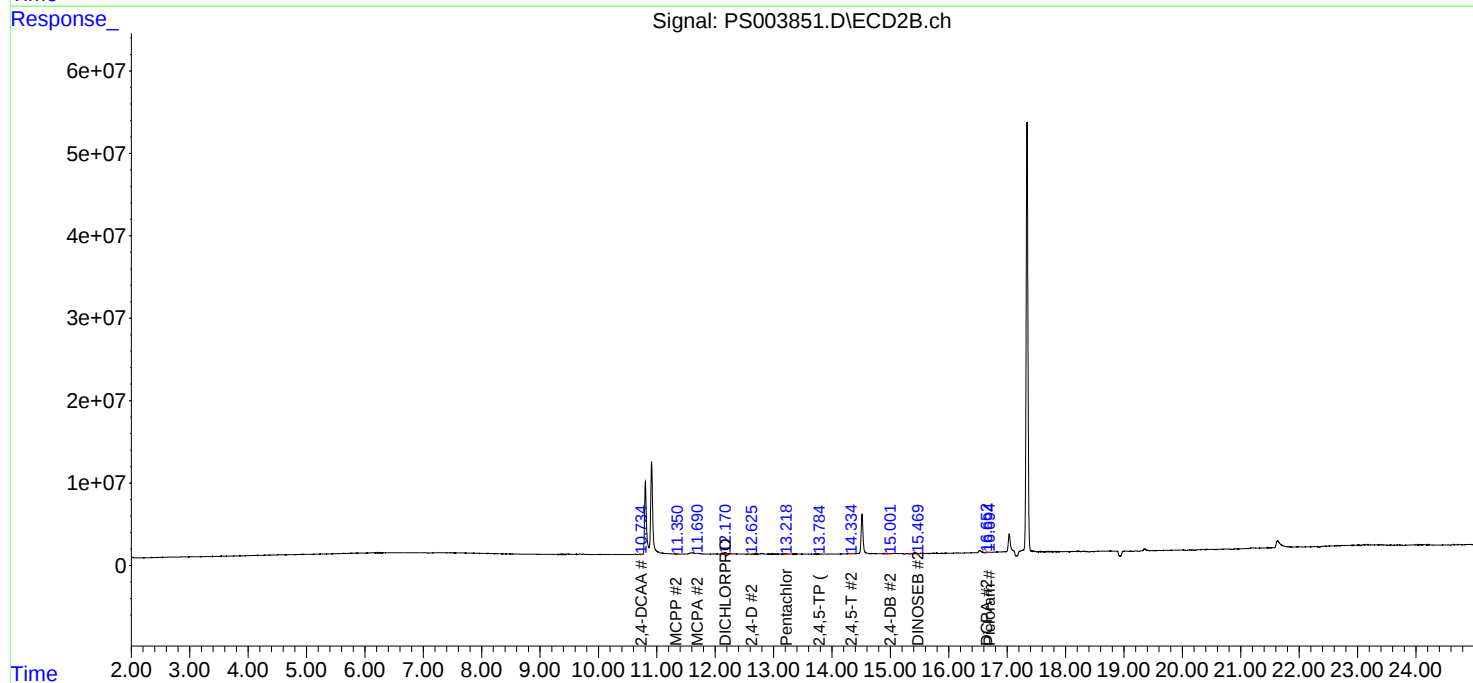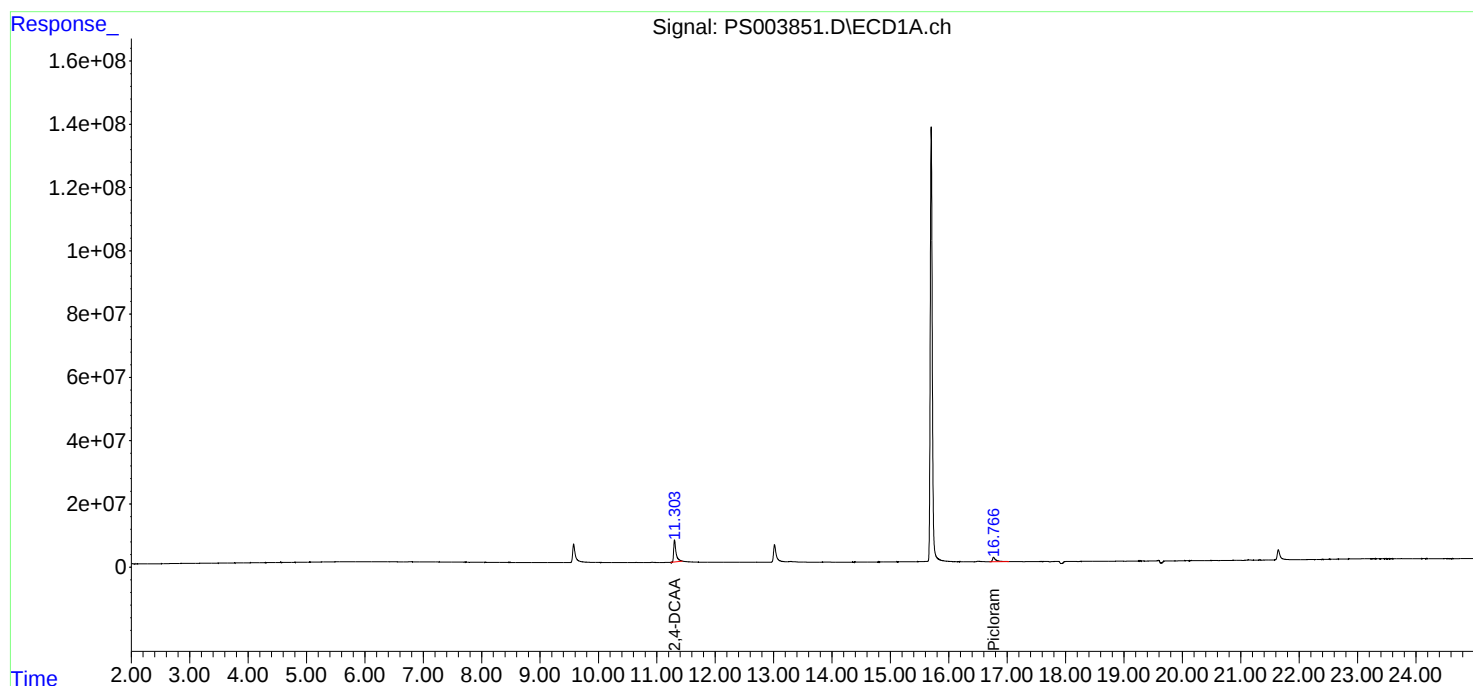


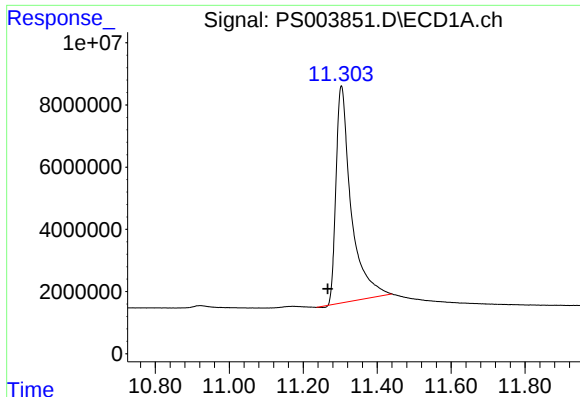

#4 2,4-DCAA


R.T.: 11.303 min
Delta R.T.: 0.037 min
Response: 198079051
Conc: 454.09 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

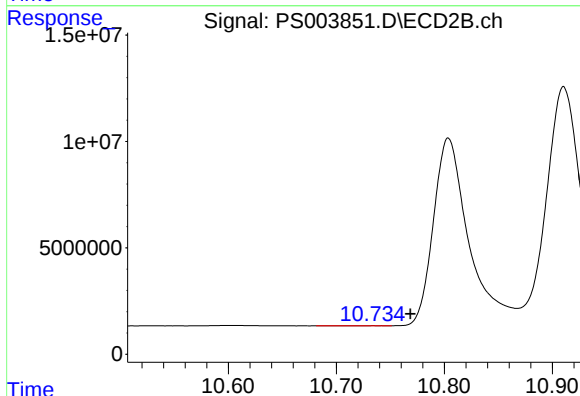


#4 2,4-DCAA

R.T.: 10.735 min
Delta R.T.: -0.034 min
Response: 20383
Conc: 0.04 ng/ml

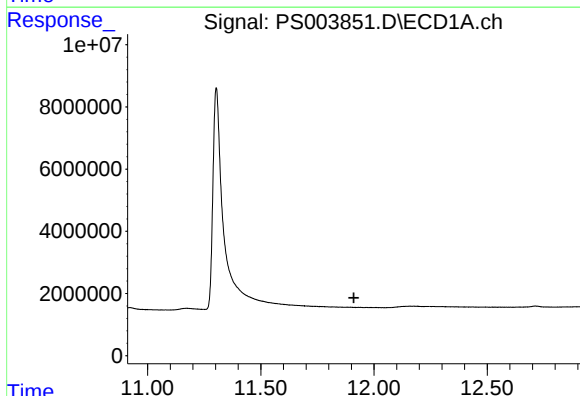


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.911 min
Response: 0
Conc: N.D.

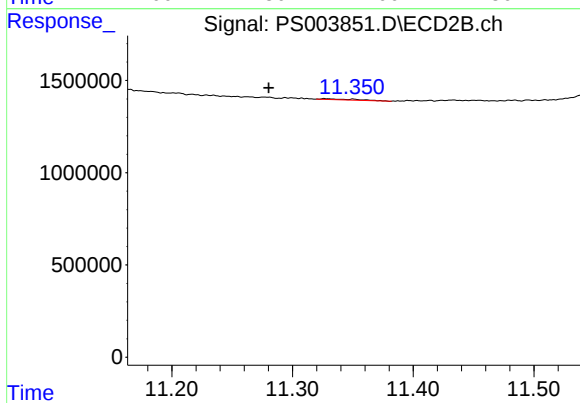

#6 MCP


R.T.: 11.328 min
Delta R.T.: 0.048 min
Response: 97433
Conc: 0.08 ug/ml

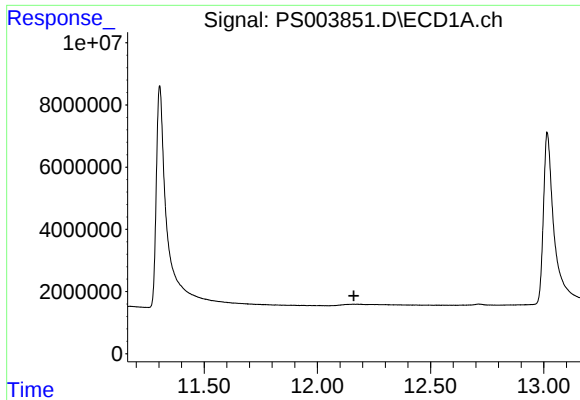

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.162 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

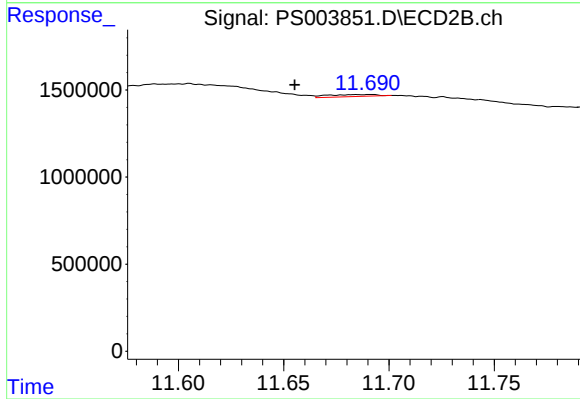


#7 MCPA

R.T.: 11.690 min
Delta R.T.: 0.034 min
Response: 238177
Conc: 0.13 ug/ml

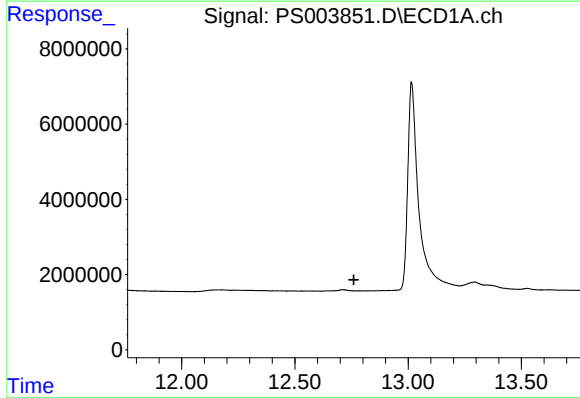


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 12.760 min
Response: 0
Conc: N.D.

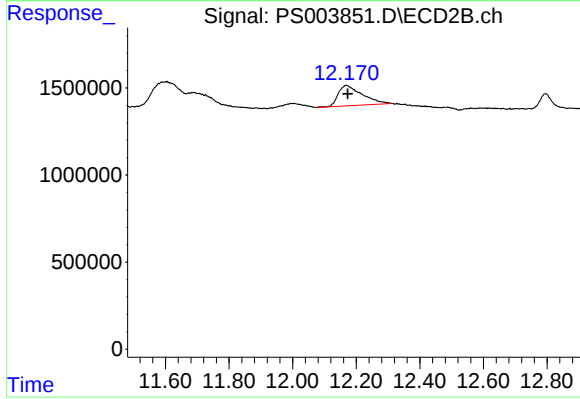

#8 DICHLORPROP


R.T.: 12.169 min
Delta R.T.: -0.004 min
Response: 6100965
Conc: 13.11 ng/ml

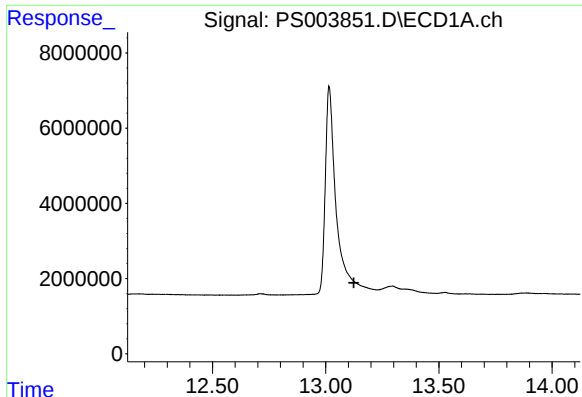

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

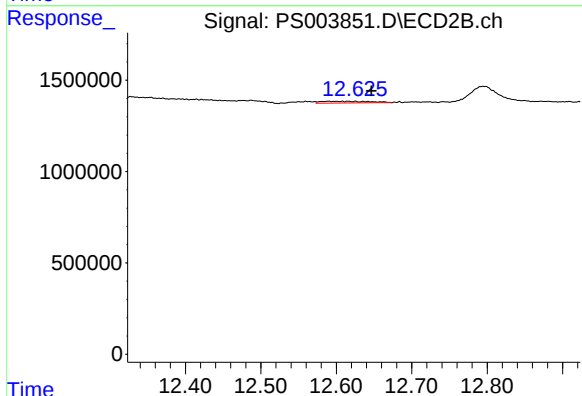


#9 2,4-D

R.T.: 12.615 min
Delta R.T.: -0.031 min
Response: 409908
Conc: 0.77 ng/ml

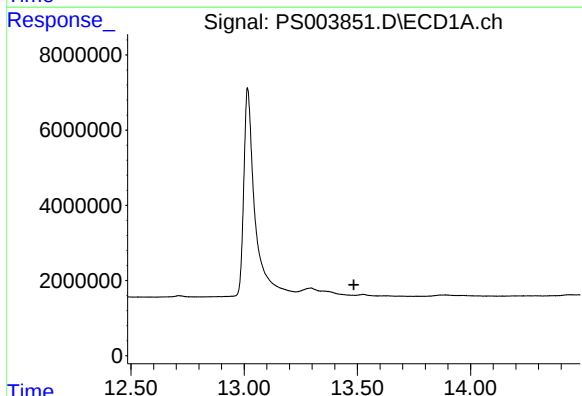


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.485 min
Response: 0
Conc: N.D.

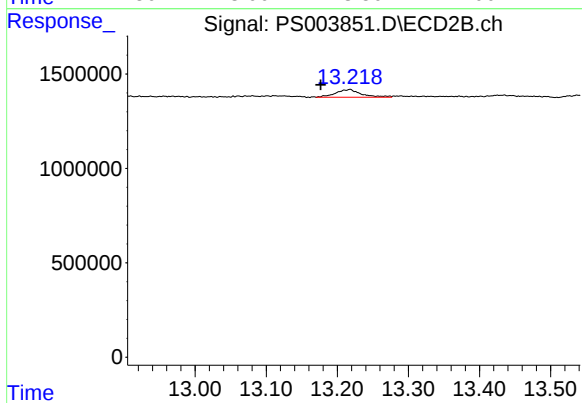

#10 Pentachlorophenol


R.T.: 13.217 min
Delta R.T.: 0.040 min
Response: 1026308
Conc: 0.15 ng/ml

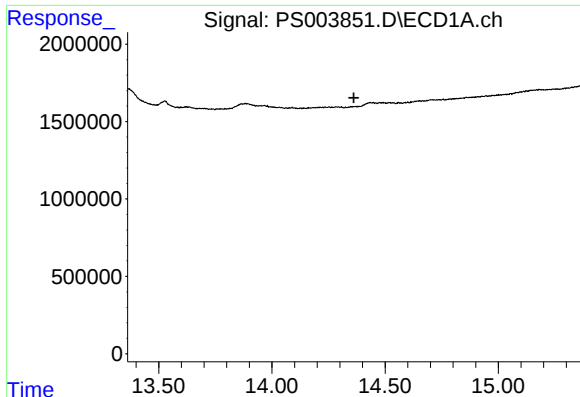

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

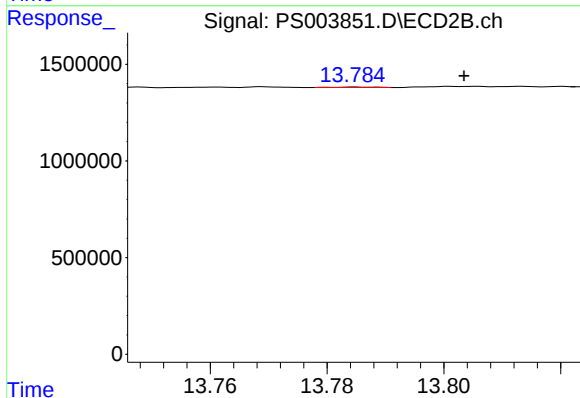


#11 2,4,5-TP (SILVEX)

R.T.: 13.785 min
Delta R.T.: -0.018 min
Response: 10335
Conc: 0.00 ng/ml

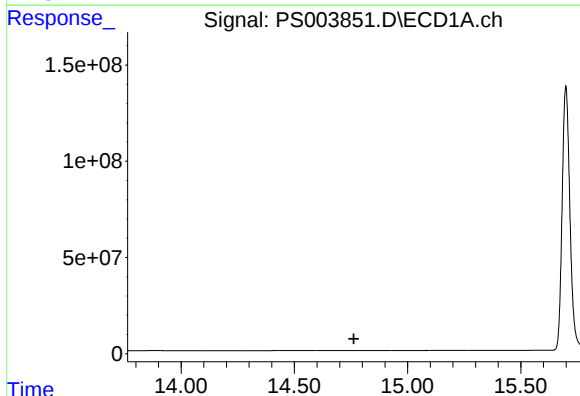


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.763 min
Response: 0
Conc: N.D.

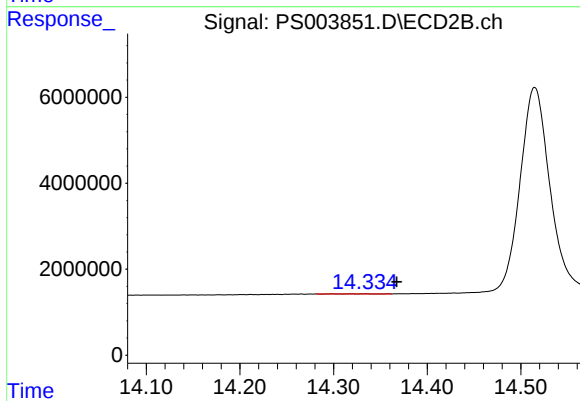

#12 2,4,5-T


R.T.: 14.334 min
Delta R.T.: -0.033 min
Response: 65222
Conc: 0.03 ng/ml

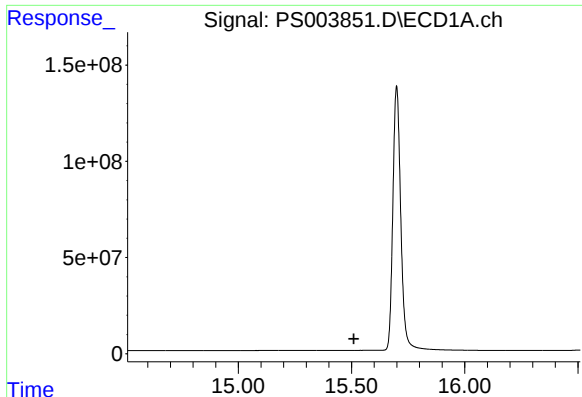

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

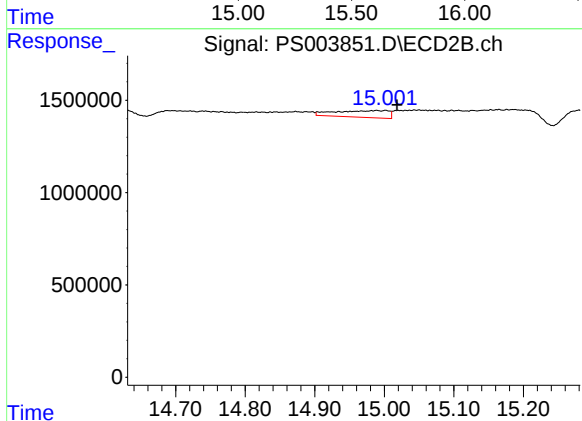


#13 2,4-DB

R.T.: 15.002 min
Delta R.T.: -0.017 min
Response: 1981911
Conc: 6.67 ng/ml

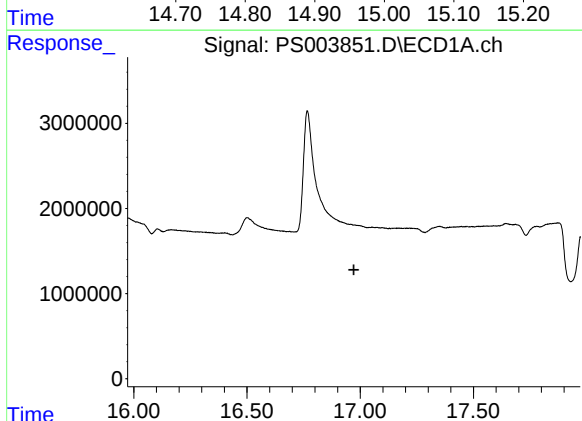


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.972 min
Response: 0
Conc: N.D.

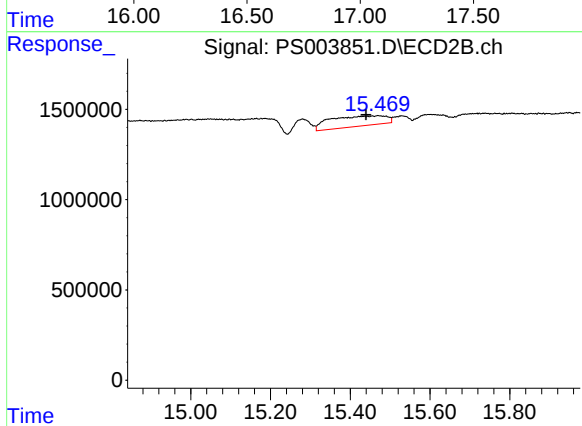

#14 DINOSEB


R.T.: 15.470 min
Delta R.T.: 0.030 min
Response: 5581277
Conc: 2.91 ng/ml

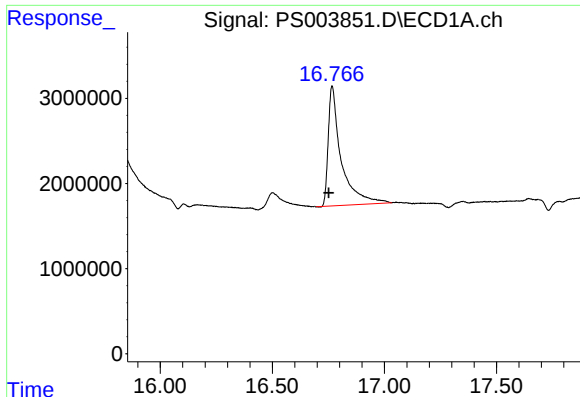

#15 Picloram


R.T.: 16.766 min
Delta R.T.: 0.015 min
Response: 56645425
Conc: 16.67 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

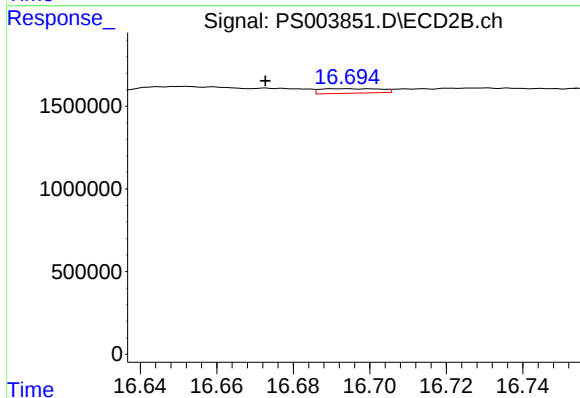


#15 Picloram

R.T.: 16.694 min
Delta R.T.: 0.021 min
Response: 305004
Conc: 0.10 ng/ml

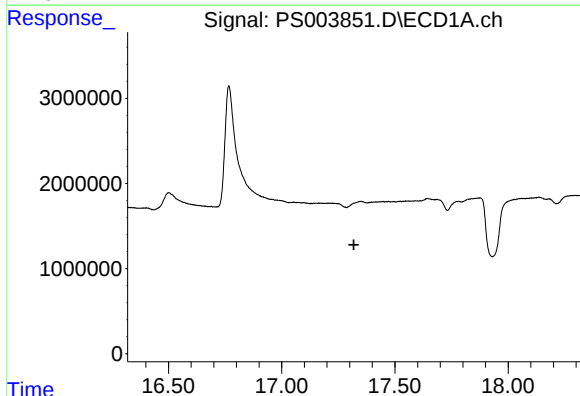

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.319 min
Response: 0
Conc: N.D.

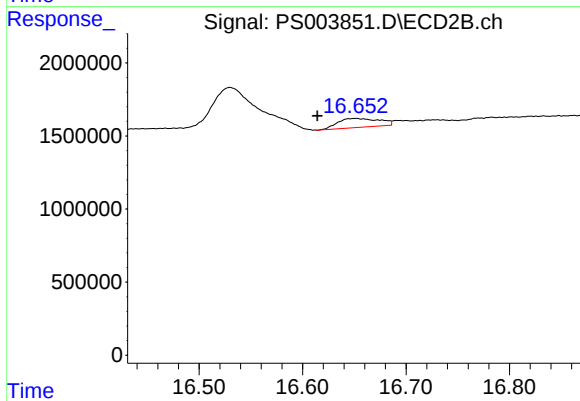

#16 DCPA

R.T.: 16.650 min
Delta R.T.: 0.036 min
Response: 1709540
Conc: 0.51 ng/ml