

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS033019\
 Data File : PS003863.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2019 16:04
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 01:47:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.282	10.784	225.6E6	191.3E6	517.124	389.883
Target Compounds							
3) T	4-Nitroph...	10.898	9.876	2645345	428383	12.210	1.887 #
6) T	MCP	0.000	11.292	0	85152	N.D.	0.072 #
7) T	MCPA	0.000	11.672	0	1168255	N.D.	0.655 #
8) T	DICHLORPROP	0.000	12.123	0	13013153	N.D.	27.953 #
9) T	2,4-D	0.000	12.596	0	987266	N.D.	1.856 #
10) T	Pentachlo...	0.000	13.193	0	1493419	N.D.	0.216 #
11) T	2,4,5-TP ...	0.000	13.869	0	1072288	N.D.	0.405 #
14) T	DINOSEB	0.000	15.443	0	8578251	N.D.	4.471 #
15) T	Picloram	16.741	16.638	73440587	1635064	21.619	0.516 #
16) T	DCPA	0.000	16.638	0	1635064	N.D.	0.484 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS033019\
Data File : PS003863.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Mar 2019 16:04
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 01:47:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

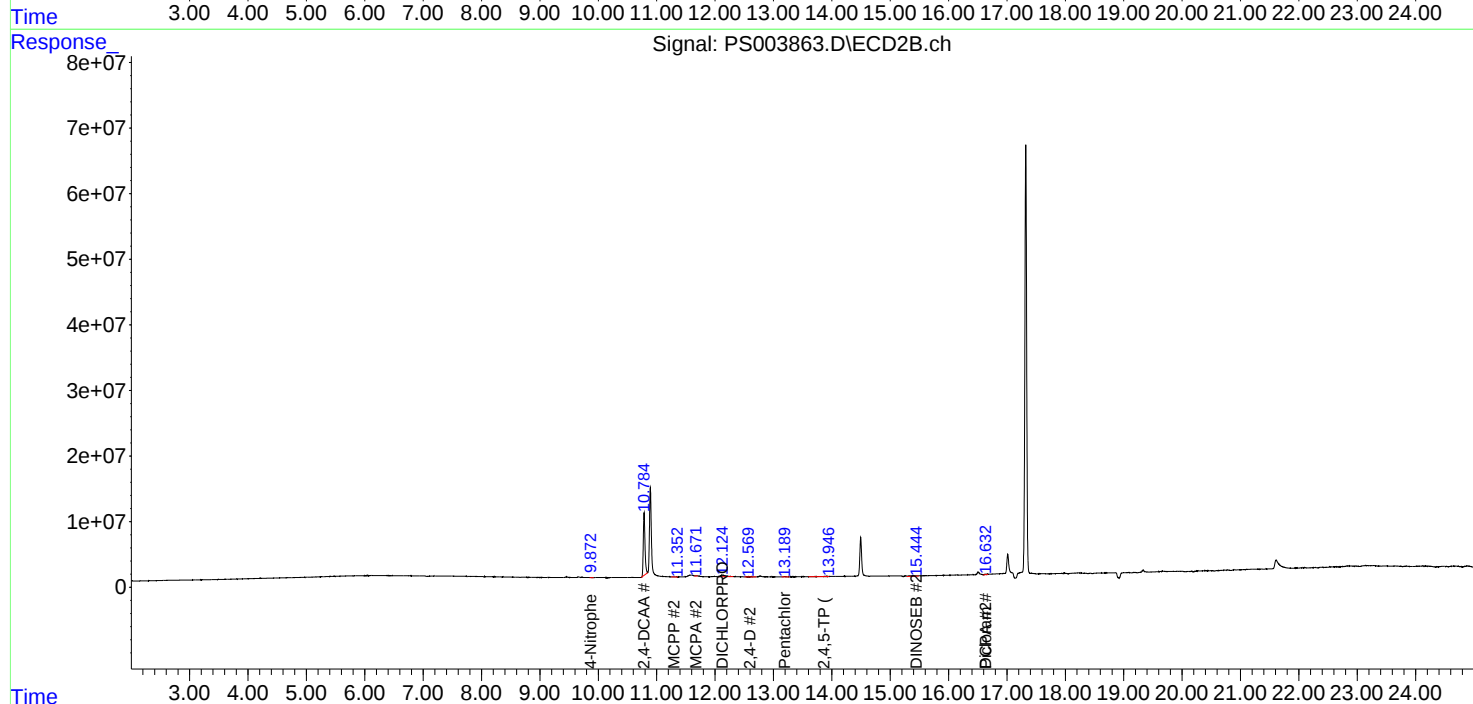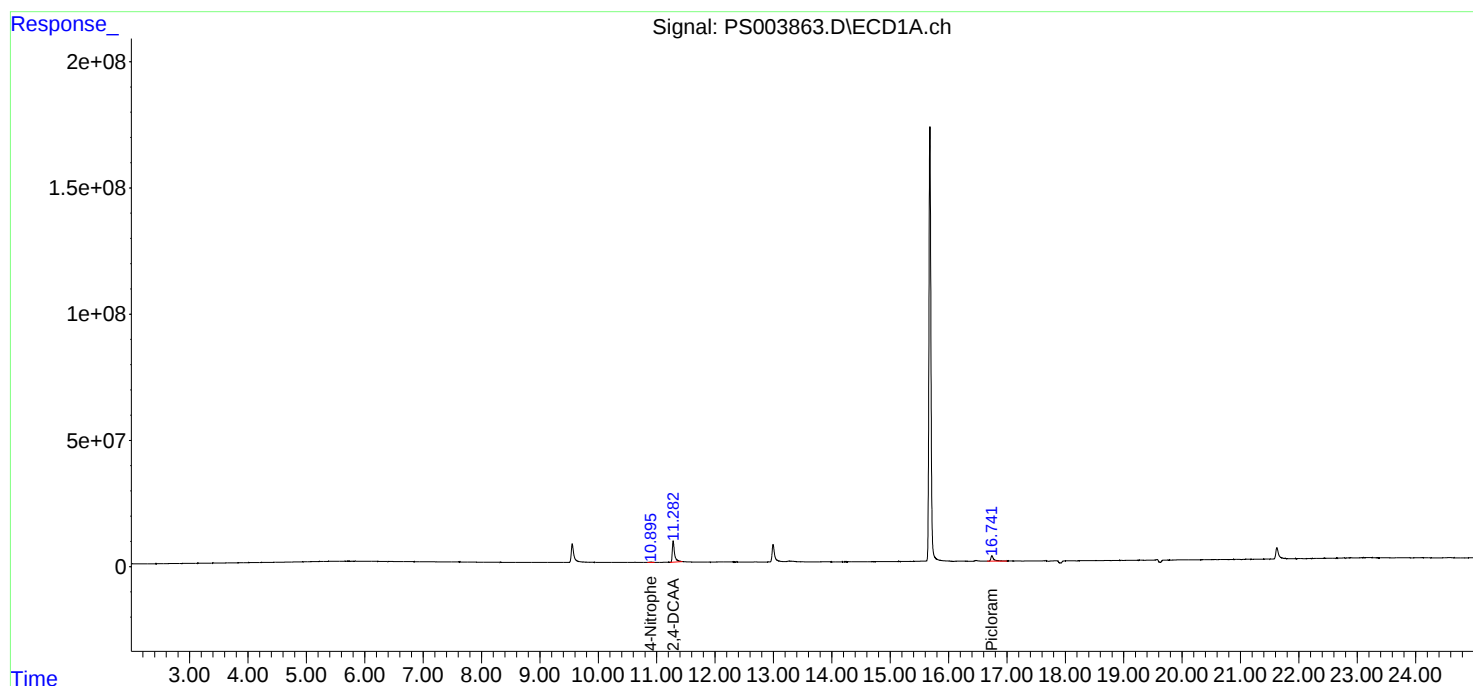


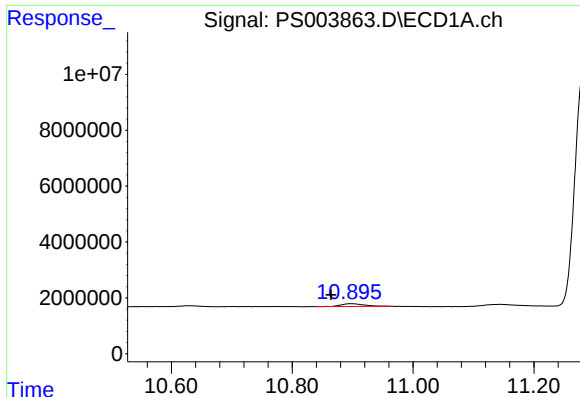

#3 4-Nitrophenol


R.T.: 10.898 min
Delta R.T.: 0.033 min
Response: 2645345
Conc: 12.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

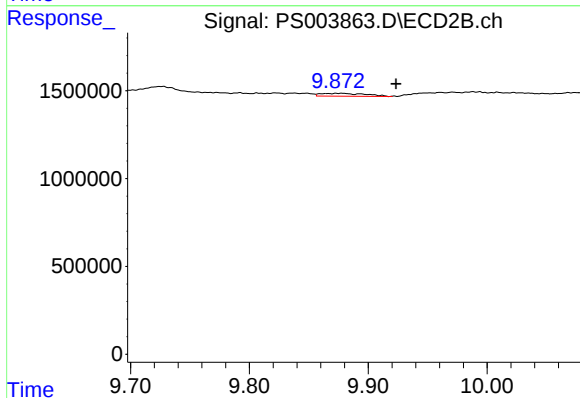


#3 4-Nitrophenol

R.T.: 9.876 min
Delta R.T.: -0.047 min
Response: 428383
Conc: 1.89 ng/ml

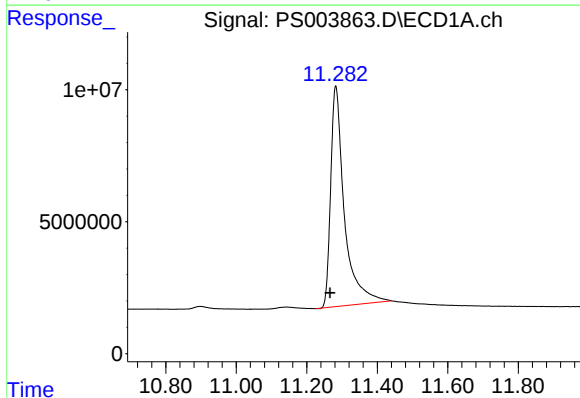


#4 2,4-DCAA

R.T.: 11.282 min
Delta R.T.: 0.016 min
Response: 225576051
Conc: 517.12 ng/ml

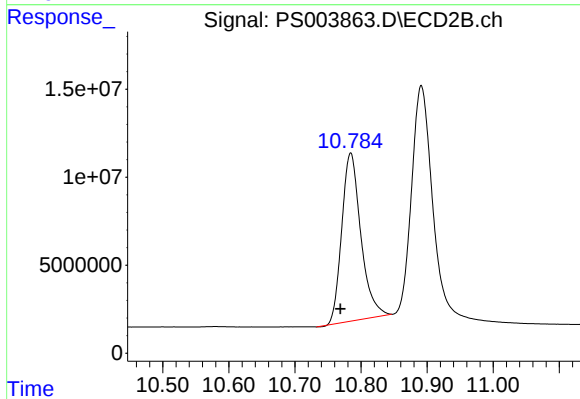

#4 2,4-DCAA


R.T.: 10.784 min
Delta R.T.: 0.016 min
Response: 191299512
Conc: 389.88 ng/ml

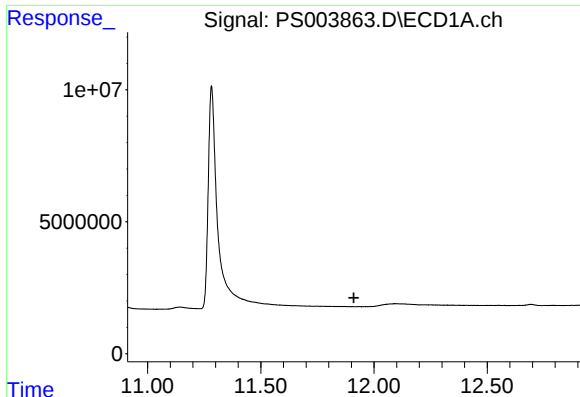

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 11.911 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

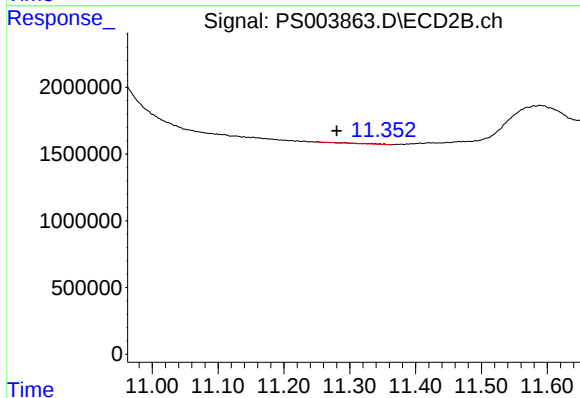


#6 MCPP

R.T.: 11.292 min
Delta R.T.: 0.011 min
Response: 85152
Conc: 0.07 ug/ml

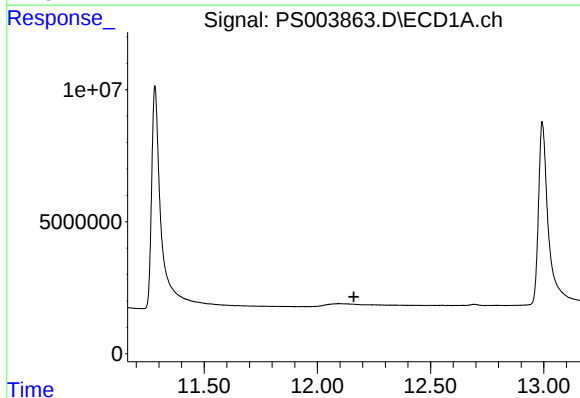


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 12.162 min
Response: 0
Conc: N.D.

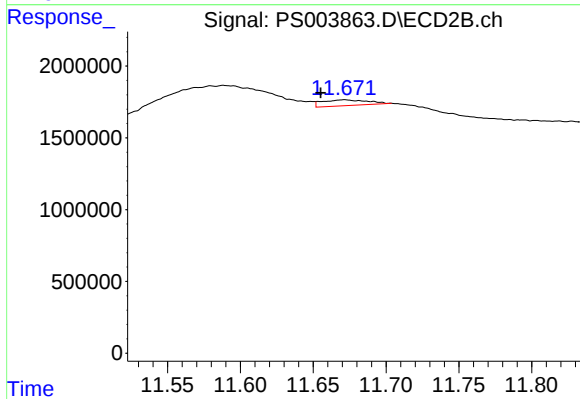

#7 MCPA


R.T.: 11.672 min
Delta R.T.: 0.017 min
Response: 1168255
Conc: 0.66 ug/ml

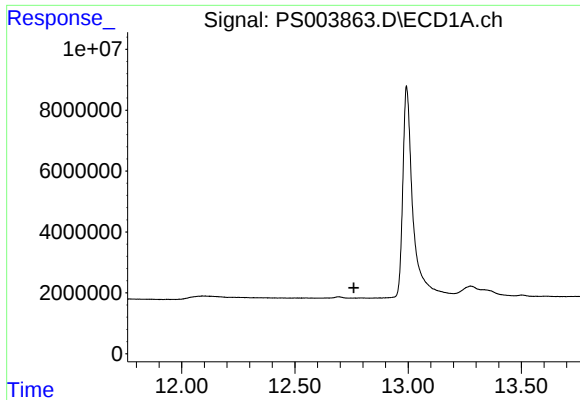

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.760 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

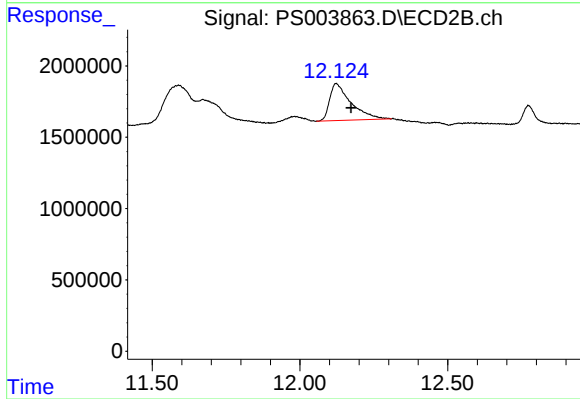


#8 DICHLORPROP

R.T.: 12.123 min
Delta R.T.: -0.049 min
Response: 13013153
Conc: 27.95 ng/ml

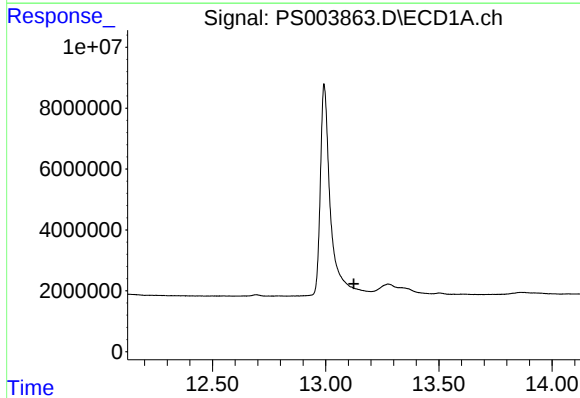


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

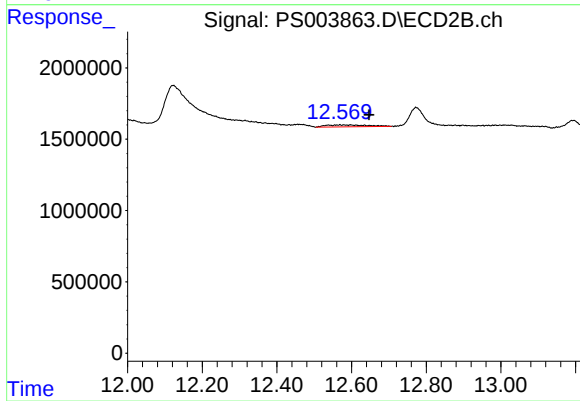

#9 2,4-D


R.T.: 12.596 min
Delta R.T.: -0.050 min
Response: 987266
Conc: 1.86 ng/ml

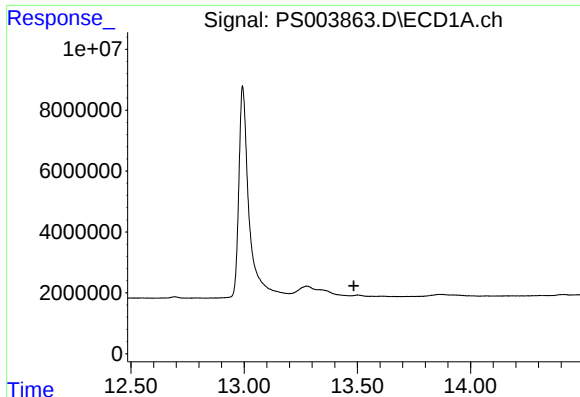

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 13.485 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

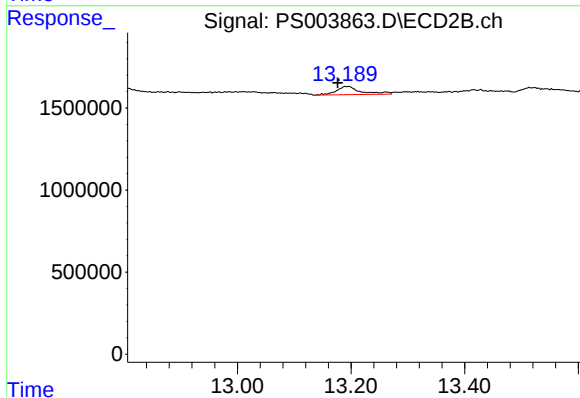


#10 Pentachlorophenol

R.T.: 13.193 min
Delta R.T.: 0.016 min
Response: 1493419
Conc: 0.22 ng/ml

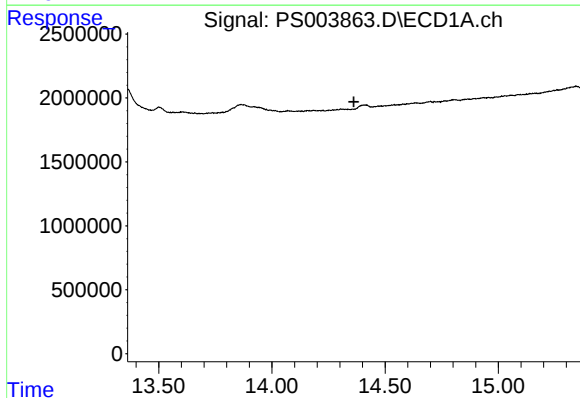


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.362 min
Response: 0
Conc: N.D.

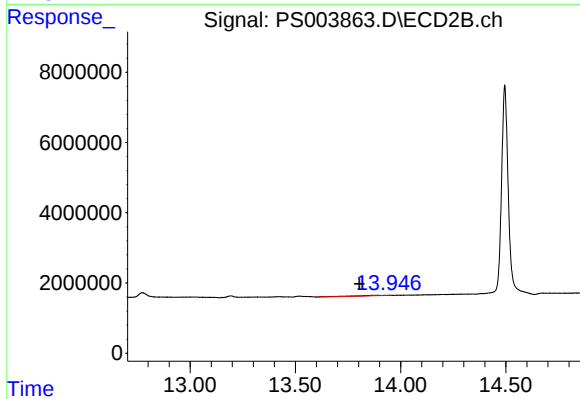

#11 2,4,5-TP (SILVEX)


R.T.: 13.869 min
Delta R.T.: 0.066 min
Response: 1072288
Conc: 0.40 ng/ml

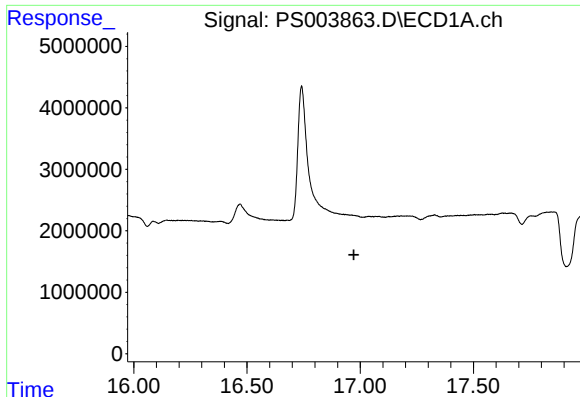

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.972 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

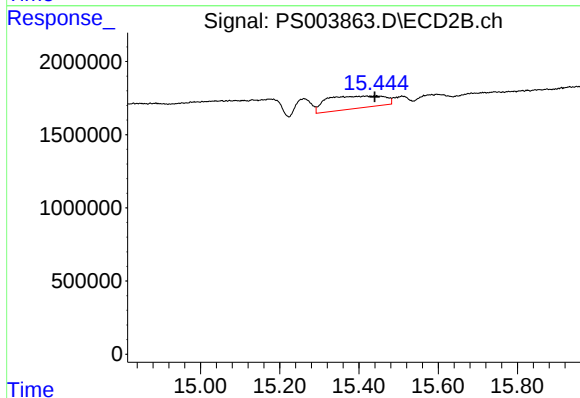


#14 DINOSEB

R.T.: 15.443 min
Delta R.T.: 0.003 min
Response: 8578251
Conc: 4.47 ng/ml

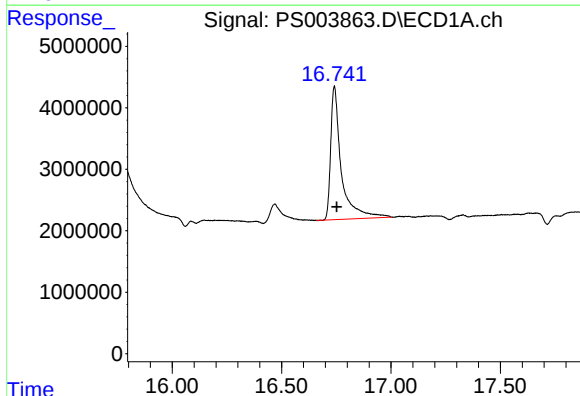


#15 Picloram

R.T.: 16.741 min
Delta R.T.: -0.011 min
Response: 73440587
Conc: 21.62 ng/ml

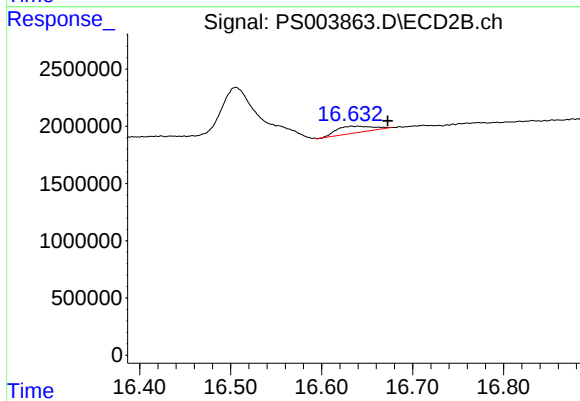

#15 Picloram


R.T.: 16.638 min
Delta R.T.: -0.034 min
Response: 1635064
Conc: 0.52 ng/ml

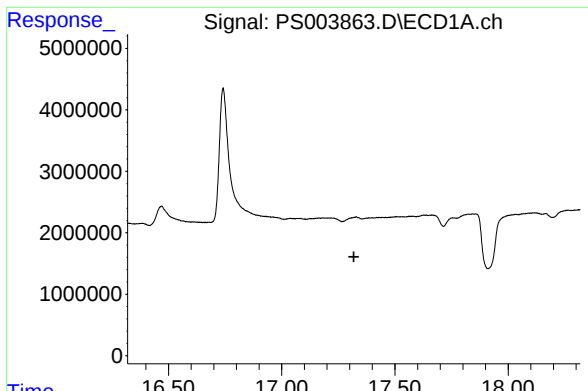

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

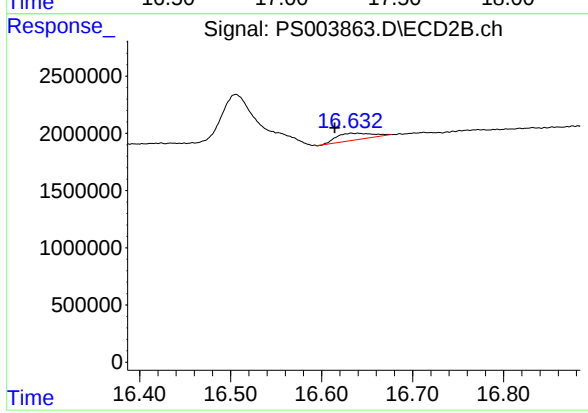

#16 DCPA

R.T.: 16.638 min
Delta R.T.: 0.024 min
Response: 1635064
Conc: 0.48 ng/ml