

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS033019\
 Data File : PS003874.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2019 21:48
 Operator : EI\SJ
 Sample : PB118400BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB118400BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 01:51:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.263	10.767	427.3E6	398.2E6	979.569	811.574
Target Compounds							
1) T	Dalapon	2.789	2.282	44709034	139.8E6	59.969	191.603 #
2) T	3,5-DICHL...	0.000	8.933	0	1035565	N.D.	1.624 #
3) T	4-Nitroph...	0.000	9.943	0	13146978	N.D.	57.907 #
5) T	DICAMBA	0.000	11.008	0	3492837	N.D.	1.878 #
7) T	MCPA	12.220	11.620	8155925	11309932	3.866	6.342 #
9) T	2,4-D	0.000	12.627	0	4526119	N.D.	8.509 #
11) T	2,4,5-TP ...	0.000	13.777	0	2725131	N.D.	1.029 #
13) T	2,4-DB	15.577	15.051	18848742	53436227	62.516	179.950 #
14) T	DINOSEB	0.000	15.492	0	7963327	N.D.	4.150 #
15) T	Picloram	0.000	16.717	0	17835091	N.D.	5.624 #
16) T	DCPA	0.000	16.623	0	10477498	N.D.	3.100 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS033019\
Data File : PS003874.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Mar 2019 21:48
Operator : EI\SJ
Sample : PB118400BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB118400BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 01:51:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

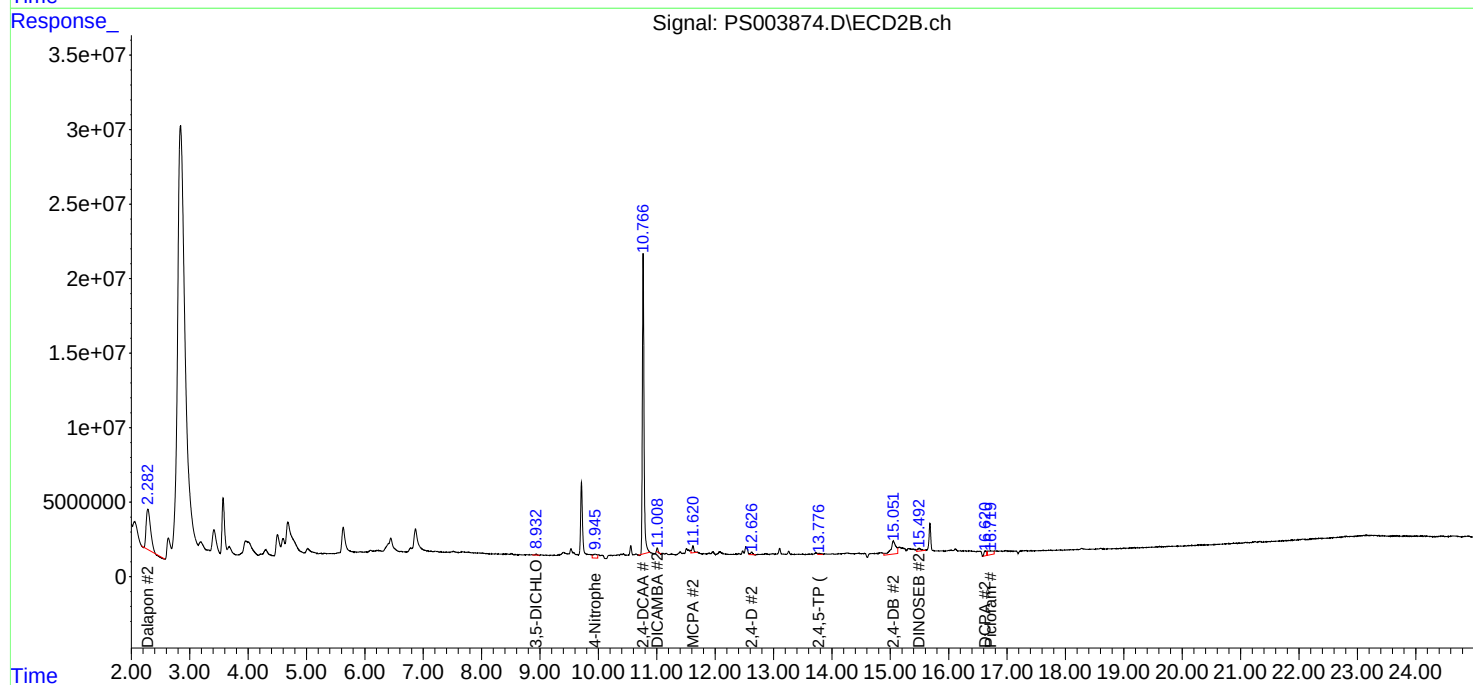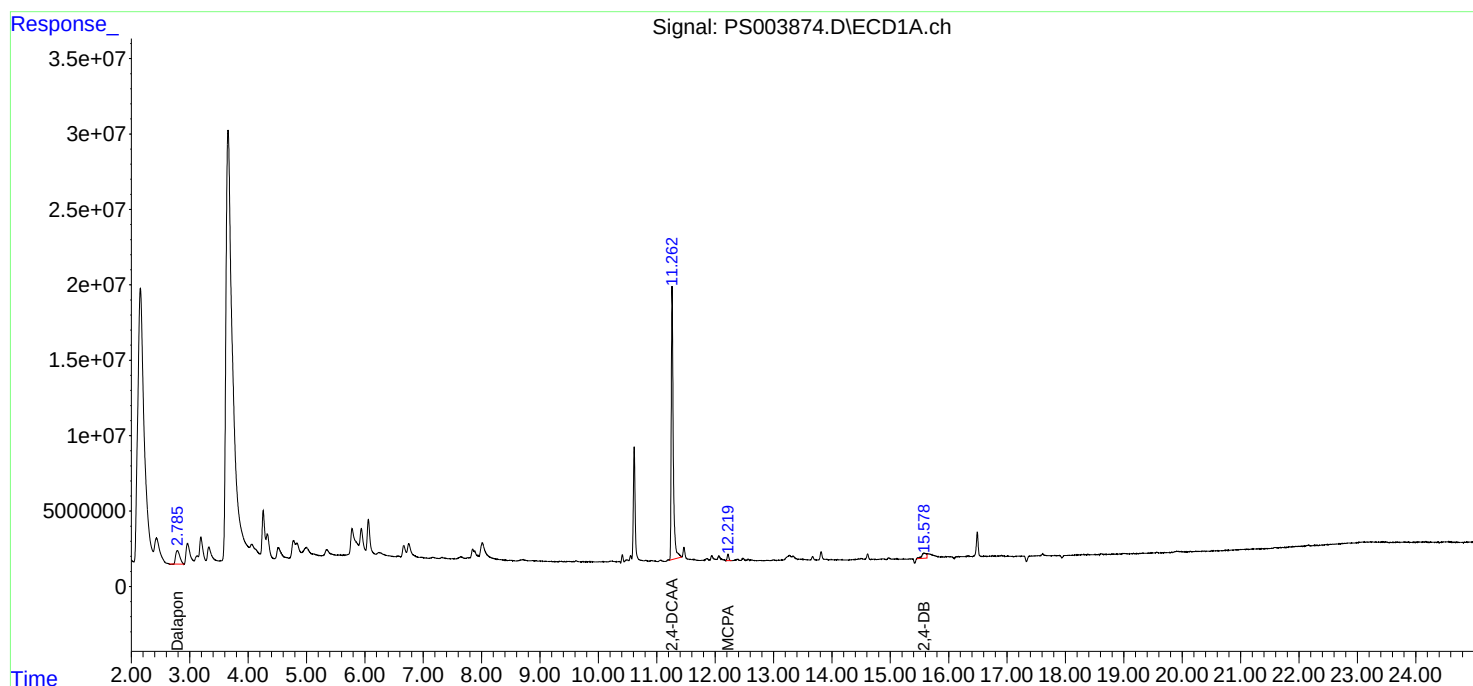


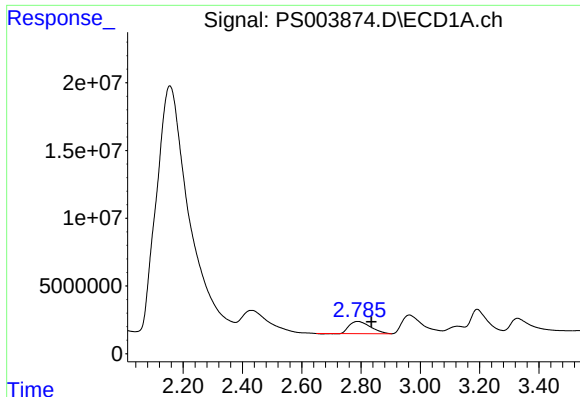

#1 Dalapon


R.T.: 2.789 min
Delta R.T.: -0.046 min
Response: 44709034
Conc: 59.97 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB118400BL

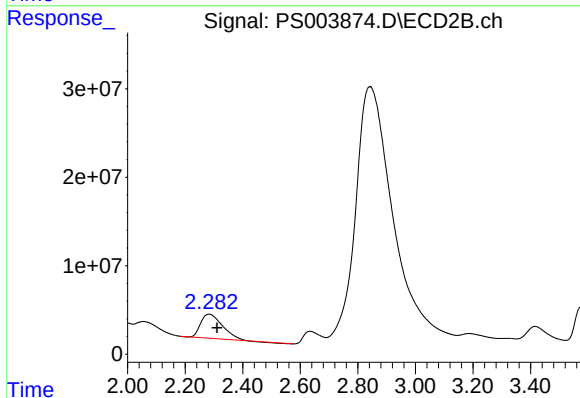


#1 Dalapon

R.T.: 2.282 min
Delta R.T.: -0.028 min
Response: 139799103
Conc: 191.60 ng/ml

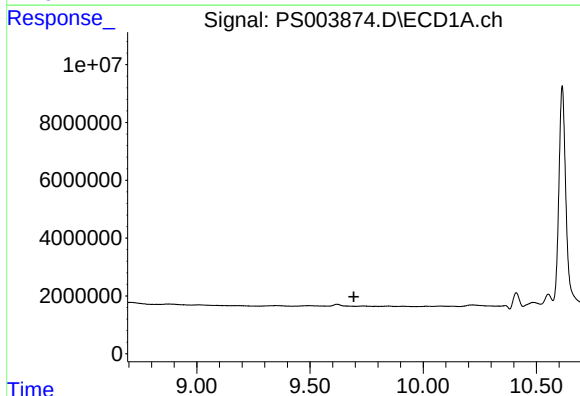


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

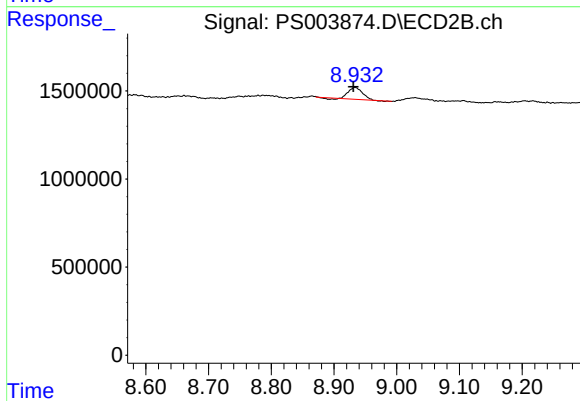

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.933 min
Delta R.T.: 0.002 min
Response: 1035565
Conc: 1.62 ng/ml

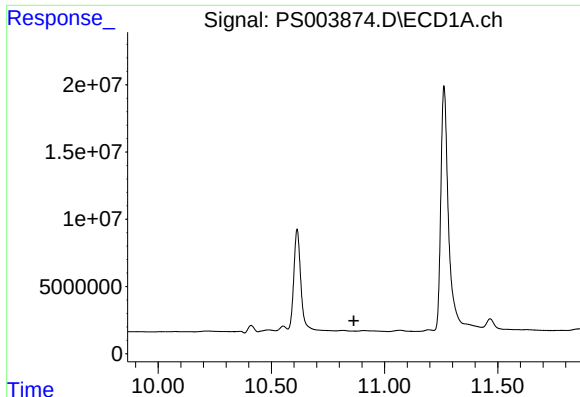

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB118400BL

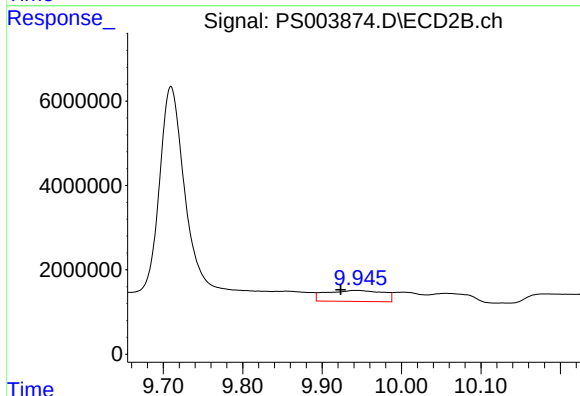


#3 4-Nitrophenol

R.T.: 9.943 min
Delta R.T.: 0.020 min
Response: 13146978
Conc: 57.91 ng/ml

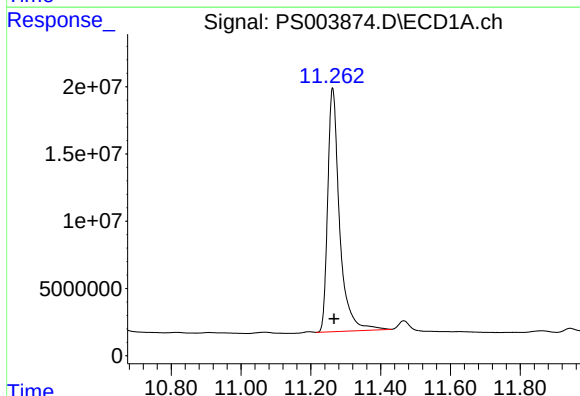


#4 2,4-DCAA

R.T.: 11.263 min
Delta R.T.: -0.004 min
Response: 427300147
Conc: 979.57 ng/ml

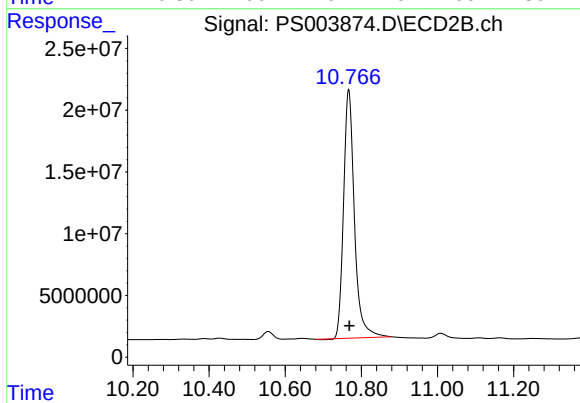

#4 2,4-DCAA


R.T.: 10.767 min
Delta R.T.: -0.002 min
Response: 398205511
Conc: 811.57 ng/ml

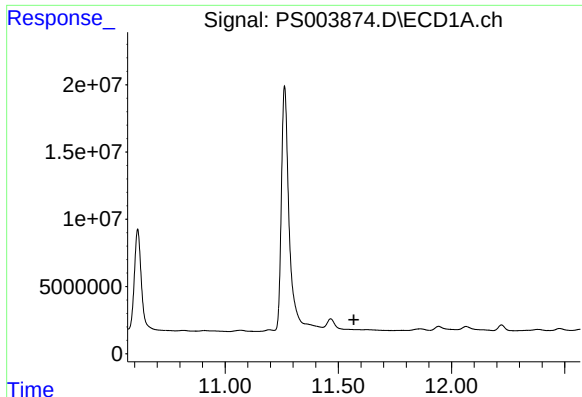

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB118400BL

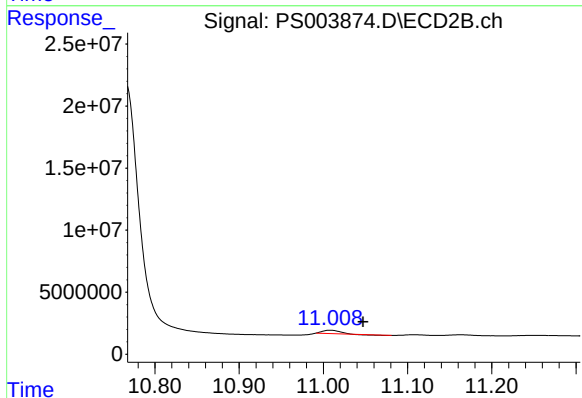


#5 DICAMBA

R.T.: 11.008 min
Delta R.T.: -0.039 min
Response: 3492837
Conc: 1.88 ng/ml

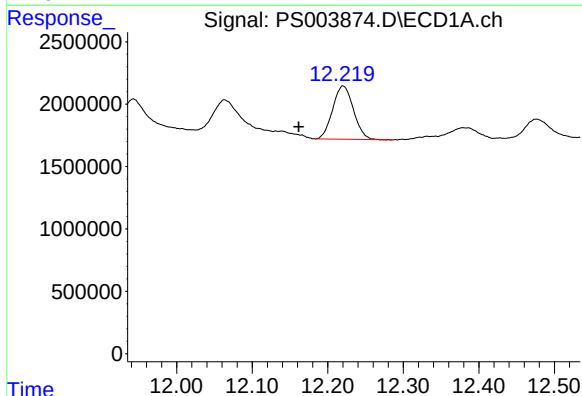


#7 MCPA

R.T.: 12.220 min
Delta R.T.: 0.059 min
Response: 8155925
Conc: 3.87 ug/ml

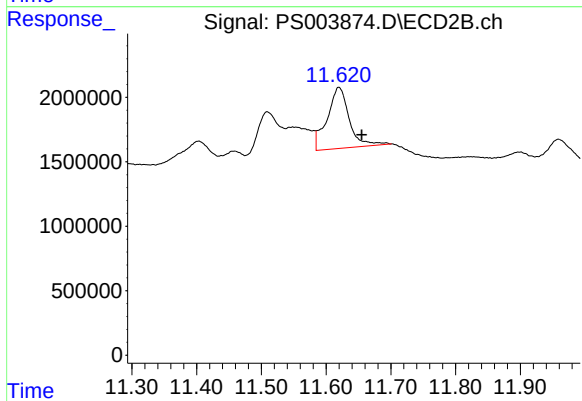

#7 MCPA


R.T.: 11.620 min
Delta R.T.: -0.035 min
Response: 11309932
Conc: 6.34 ug/ml

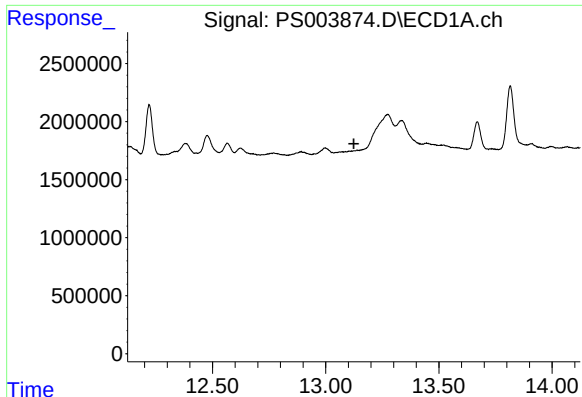

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB118400BL

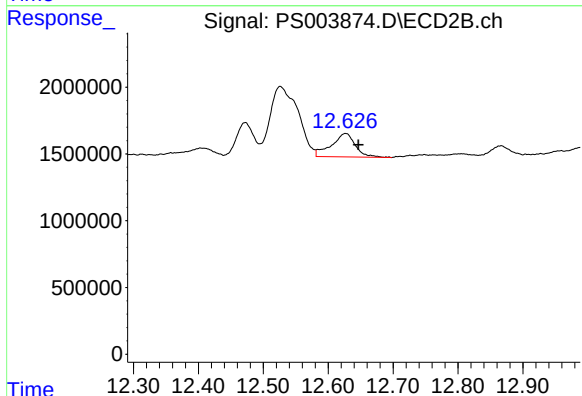


#9 2,4-D

R.T.: 12.627 min
Delta R.T.: -0.020 min
Response: 4526119
Conc: 8.51 ng/ml

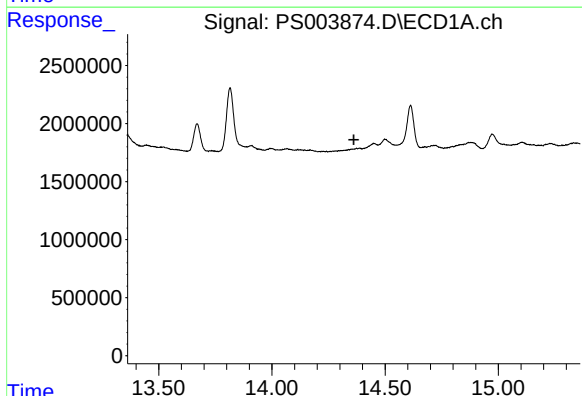


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

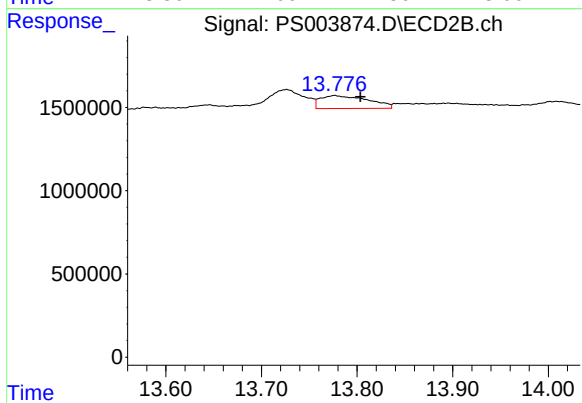

#11 2,4,5-TP (SILVEX)


R.T.: 13.777 min
Delta R.T.: -0.027 min
Response: 2725131
Conc: 1.03 ng/ml

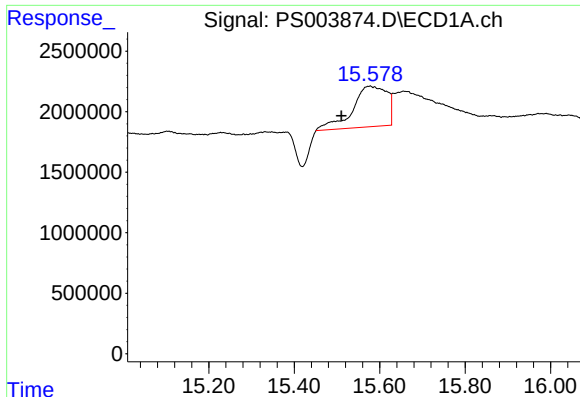

#13 2,4-DB


R.T.: 15.577 min
Delta R.T.: 0.067 min
Response: 18848742
Conc: 62.52 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB118400BL

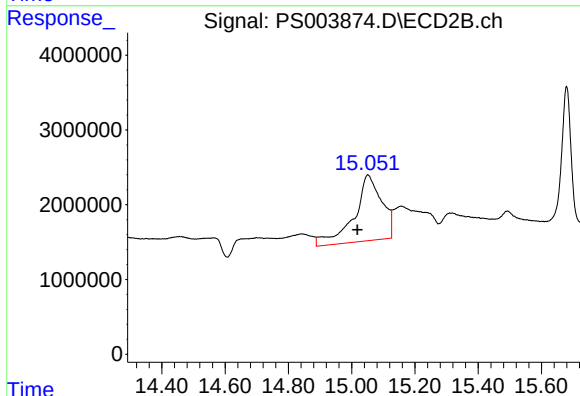


#13 2,4-DB

R.T.: 15.051 min
Delta R.T.: 0.033 min
Response: 53436227
Conc: 179.95 ng/ml

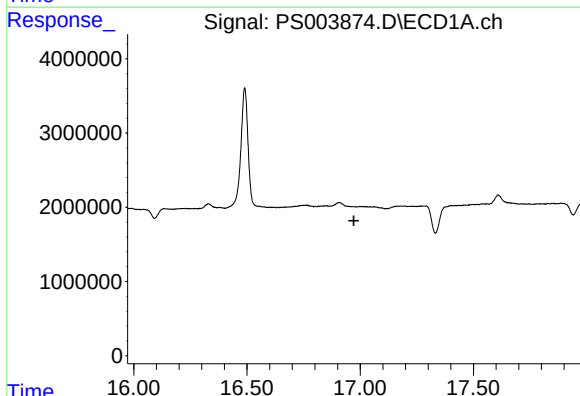


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 16.972 min
Response: 0
Conc: N.D.

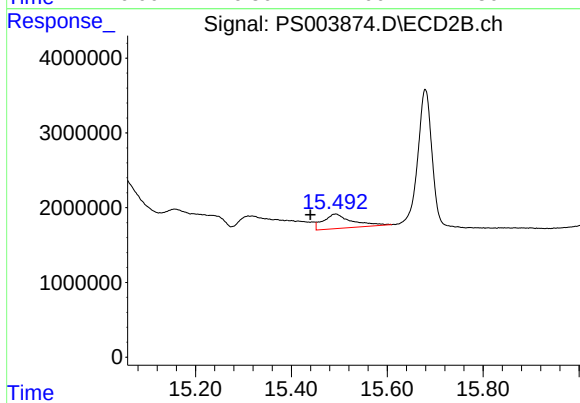

#14 DINOSEB


R.T.: 15.492 min
Delta R.T.: 0.052 min
Response: 7963327
Conc: 4.15 ng/ml

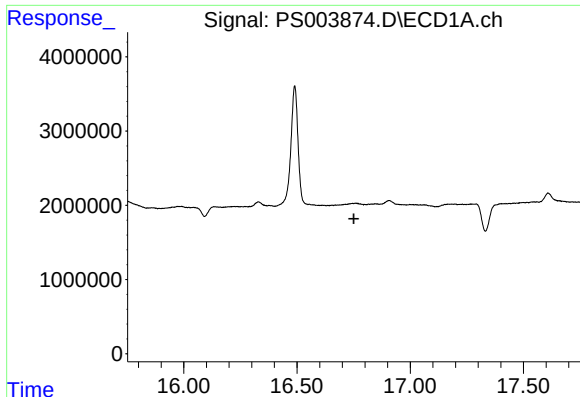

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.752 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB118400BL

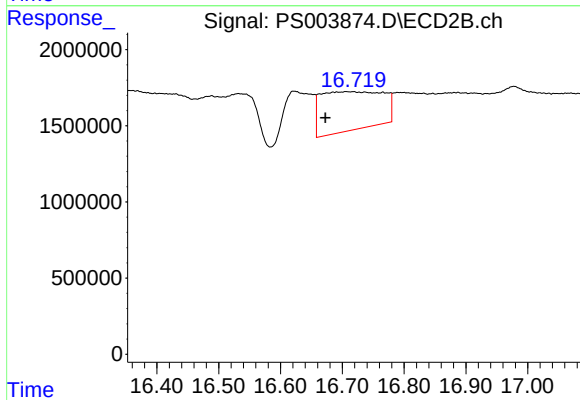


#15 Picloram

R.T.: 16.717 min
Delta R.T.: 0.044 min
Response: 17835091
Conc: 5.62 ng/ml

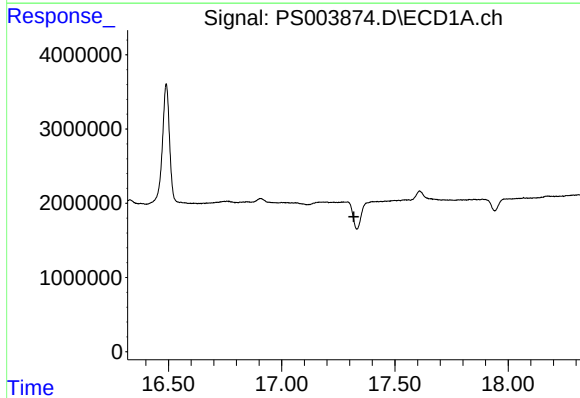

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.319 min
Response: 0
Conc: N.D.

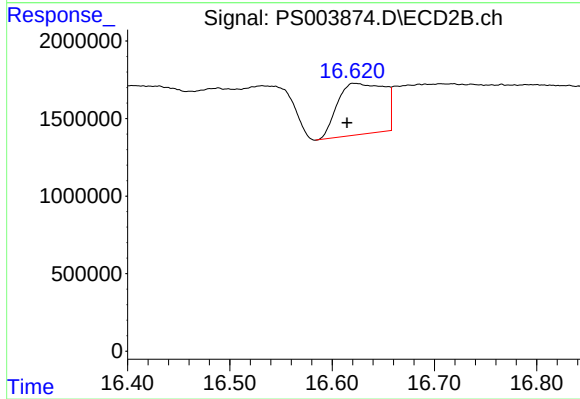

#16 DCPA

R.T.: 16.623 min
Delta R.T.: 0.008 min
Response: 10477498
Conc: 3.10 ng/ml