

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS033019\
 Data File : PS003877.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2019 23:22
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 01:52:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.264	10.764	235.6E6	183.2E6	540.102	373.371 #
Target Compounds							
3) T	4-Nitroph...	10.881	9.974	3998804	1290308	18.457	5.683 #
7) T	MCPA	0.000	11.653	0	1913685	N.D.	1.073 #
9) T	2,4-D	0.000	12.658	0	31219	N.D.	0.059 #
10) T	Pentachlo...	0.000	13.176	0	1521233	N.D.	0.220 #
11) T	2,4,5-TP ...	0.000	13.846	0	712863	N.D.	0.269 #
12) T	2,4,5-T	0.000	14.318	0	103787	N.D.	0.048 #
13) T	2,4-DB	0.000	15.005	0	5123124	N.D.	17.252 #
14) T	DINOSEB	0.000	15.427	0	10883994	N.D.	5.673 #
15) T	Picloram	16.720	16.613	123.2E6	2992428	36.273	0.944 #
16) T	DCPA	0.000	16.613	0	2992428	N.D.	0.885 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS033019\
Data File : PS003877.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Mar 2019 23:22
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 01:52:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

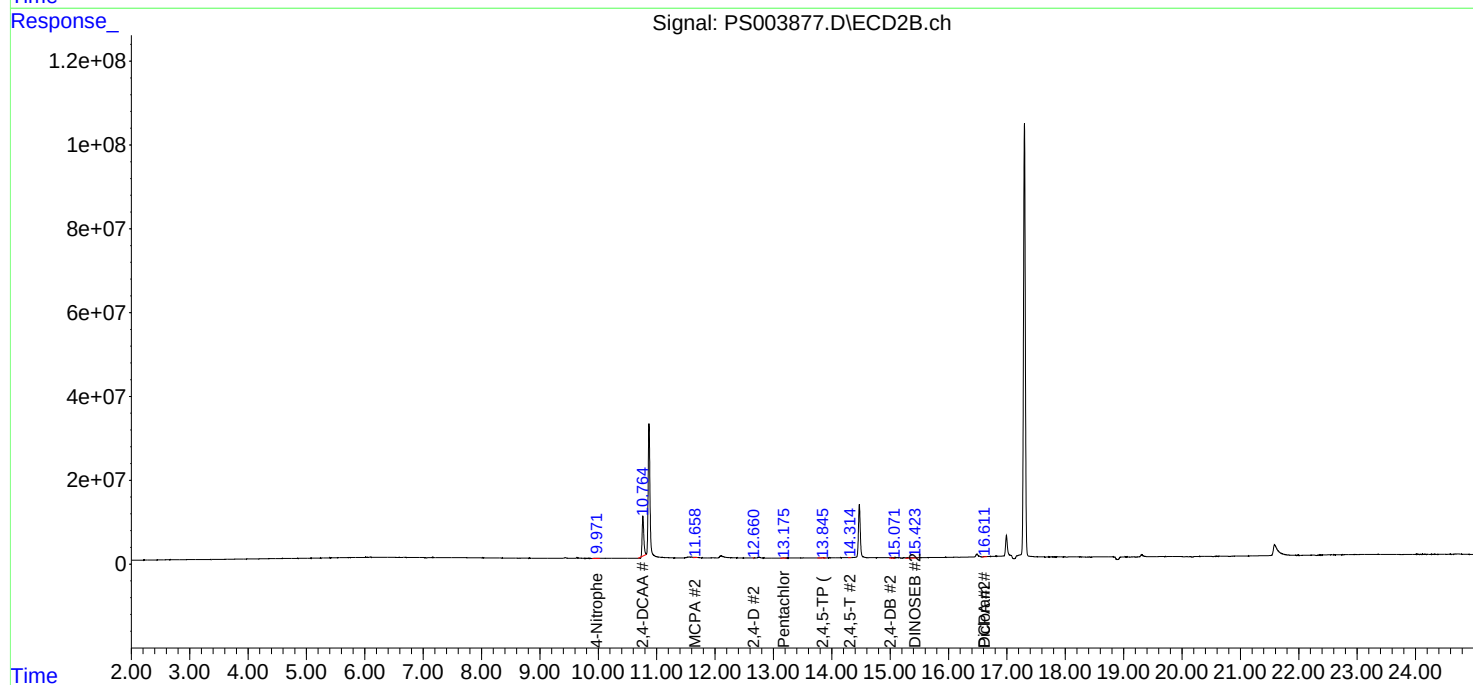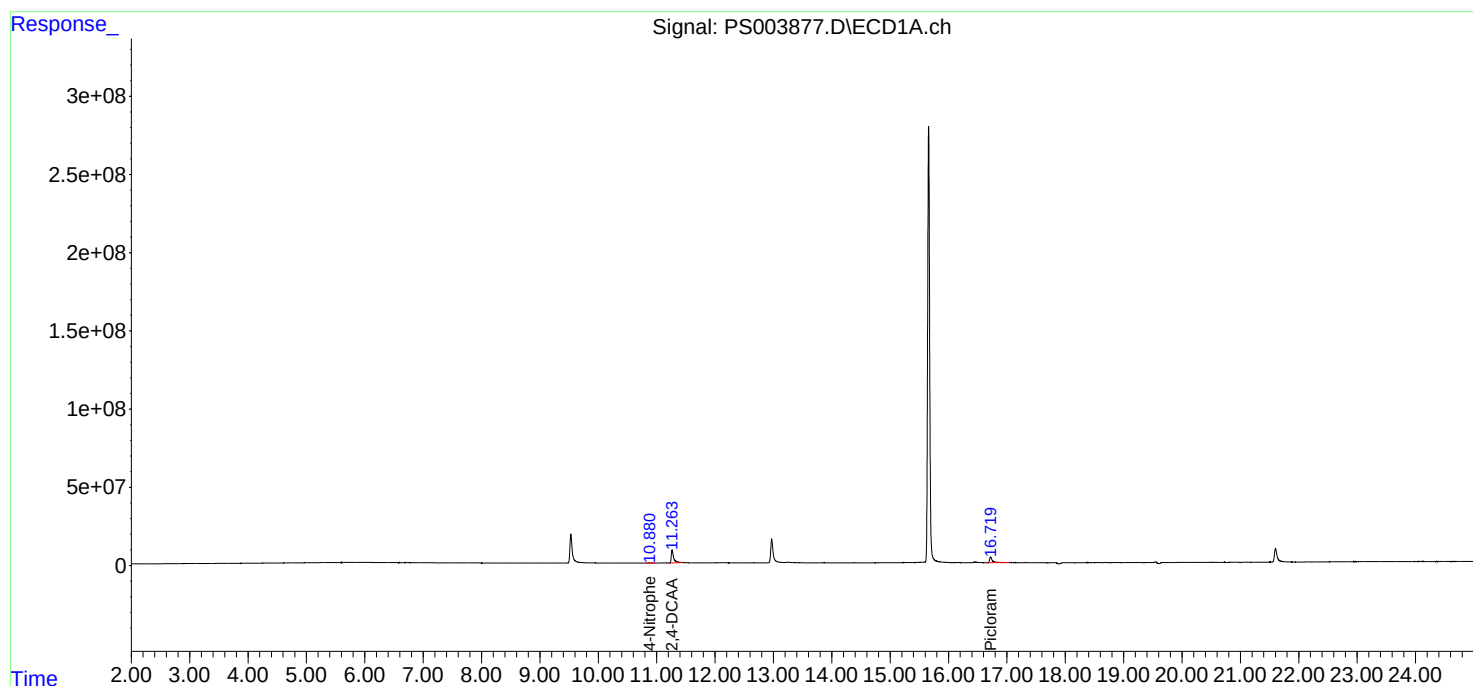


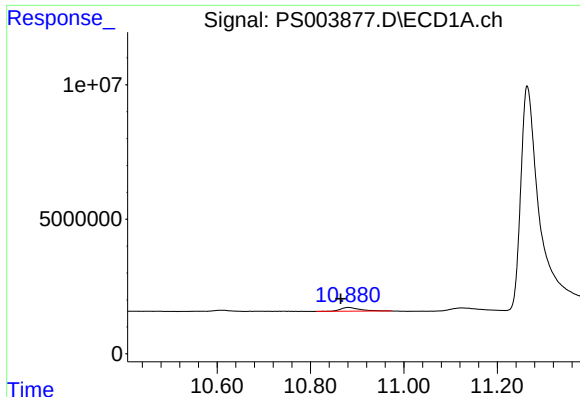

#3 4-Nitrophenol


R.T.: 10.881 min
Delta R.T.: 0.016 min
Response: 3998804
Conc: 18.46 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

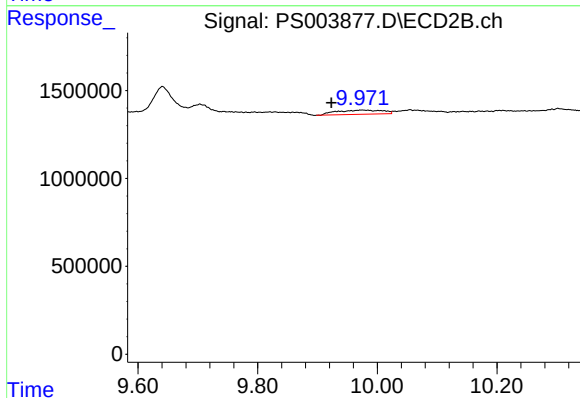


#3 4-Nitrophenol

R.T.: 9.974 min
Delta R.T.: 0.051 min
Response: 1290308
Conc: 5.68 ng/ml

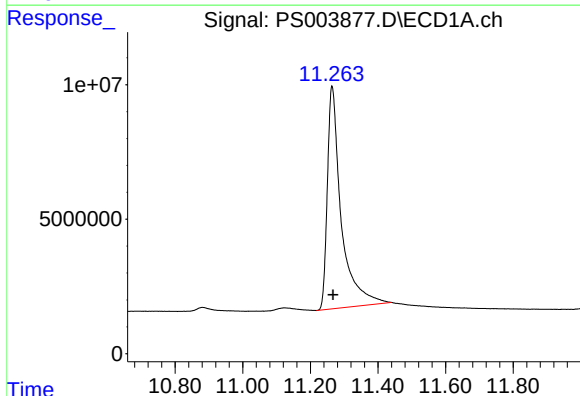


#4 2,4-DCAA

R.T.: 11.264 min
Delta R.T.: -0.002 min
Response: 235599034
Conc: 540.10 ng/ml

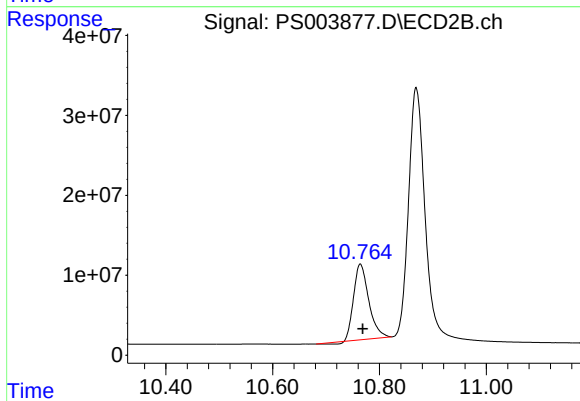

#4 2,4-DCAA


R.T.: 10.764 min
Delta R.T.: -0.005 min
Response: 183197410
Conc: 373.37 ng/ml

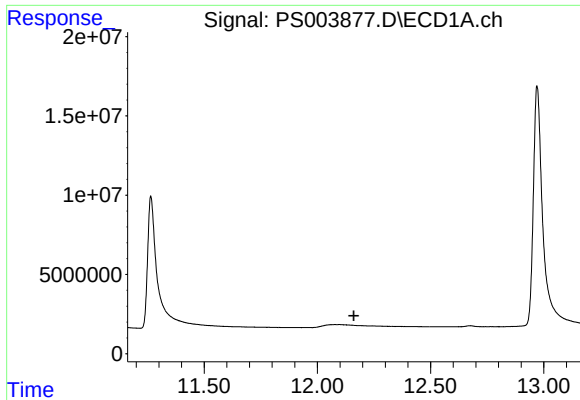

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.162 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

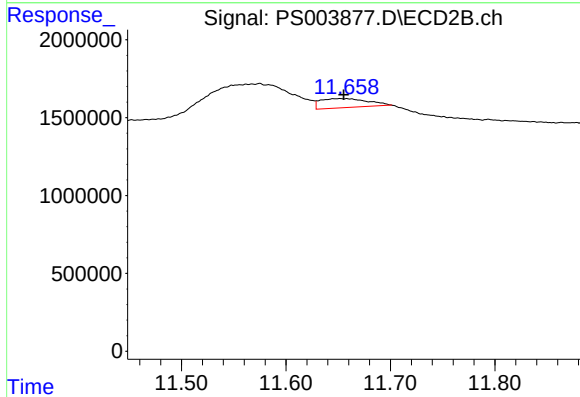


#7 MCPA

R.T.: 11.653 min
Delta R.T.: -0.002 min
Response: 1913685
Conc: 1.07 ug/ml

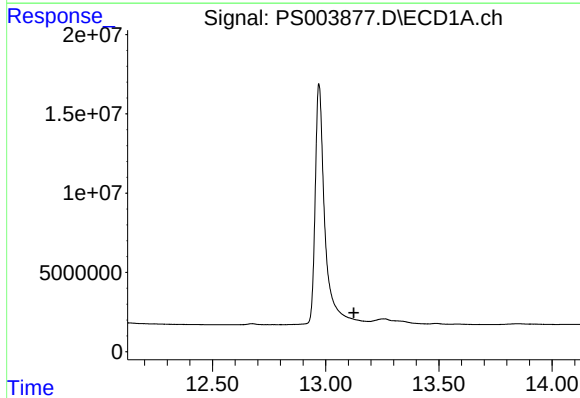


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

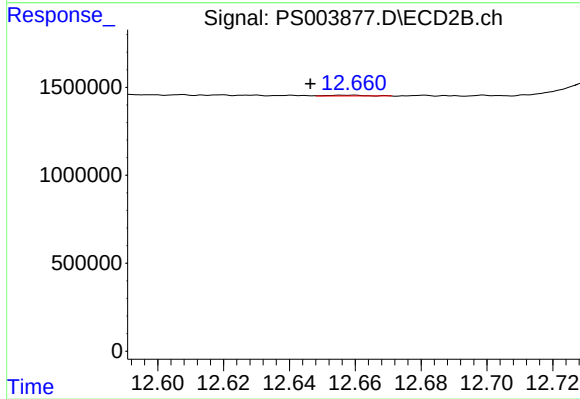

#9 2,4-D


R.T.: 12.658 min
Delta R.T.: 0.011 min
Response: 31219
Conc: 0.06 ng/ml

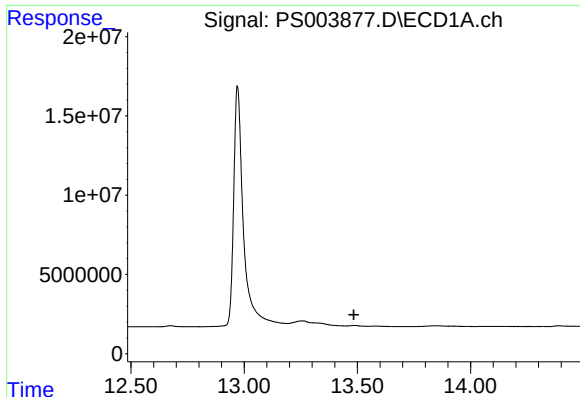

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.485 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

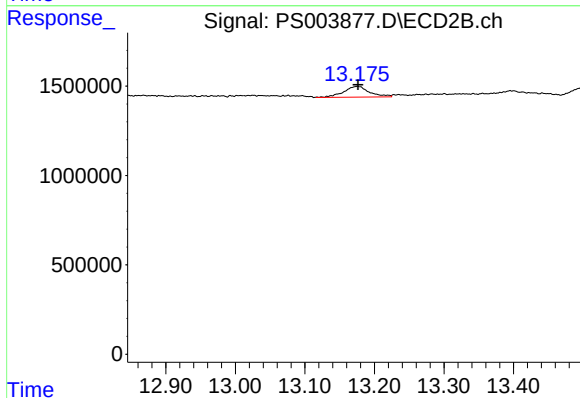


#10 Pentachlorophenol

R.T.: 13.176 min
Delta R.T.: -0.001 min
Response: 1521233
Conc: 0.22 ng/ml

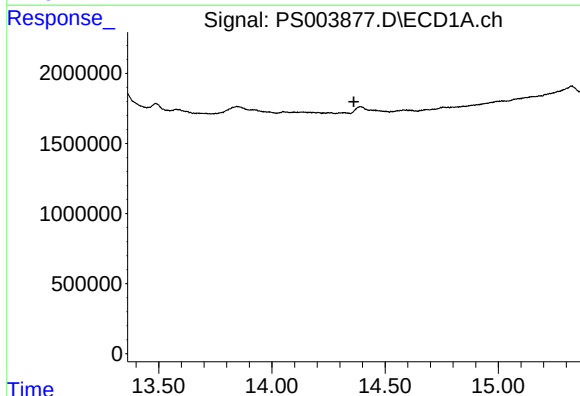


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

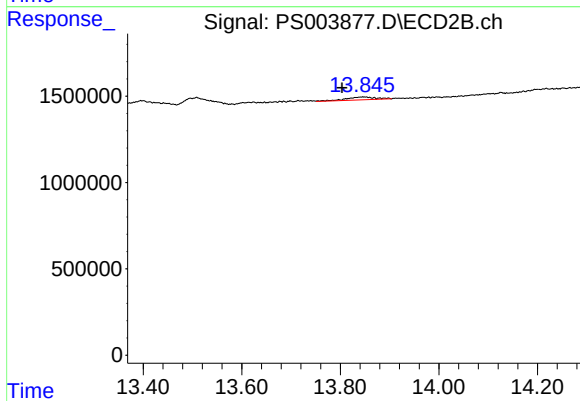

#11 2,4,5-TP (SILVEX)


R.T.: 13.846 min
Delta R.T.: 0.043 min
Response: 712863
Conc: 0.27 ng/ml

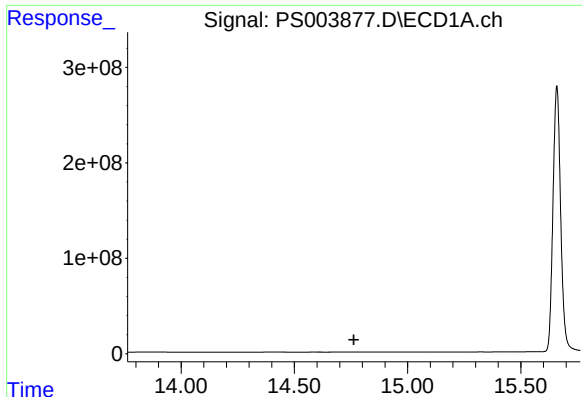

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.763 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

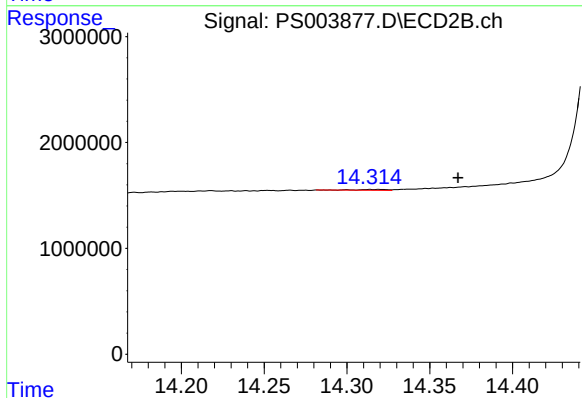


#12 2,4,5-T

R.T.: 14.318 min
Delta R.T.: -0.049 min
Response: 103787
Conc: 0.05 ng/ml

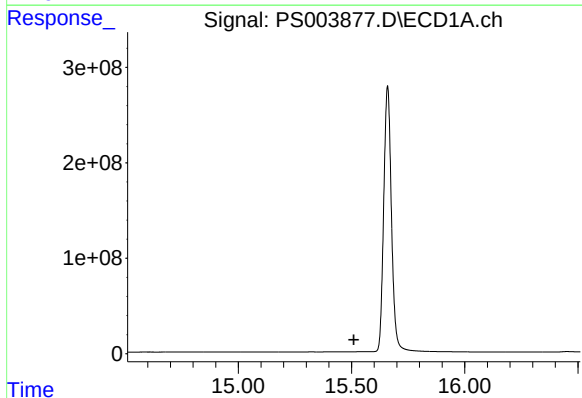


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

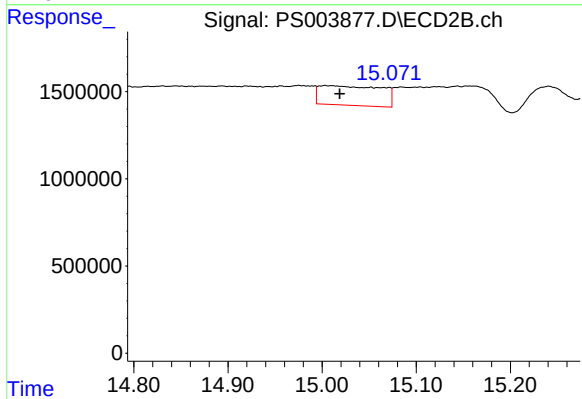

#13 2,4-DB


R.T.: 15.005 min
Delta R.T.: -0.014 min
Response: 5123124
Conc: 17.25 ng/ml

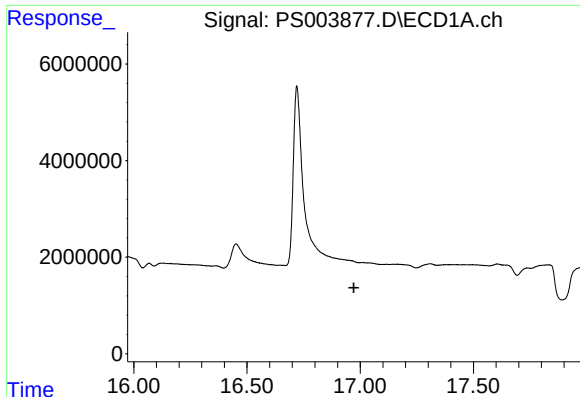

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.972 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

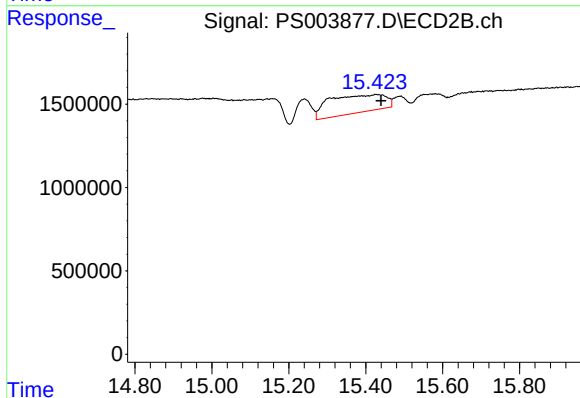


#14 DINOSEB

R.T.: 15.427 min
Delta R.T.: -0.013 min
Response: 10883994
Conc: 5.67 ng/ml

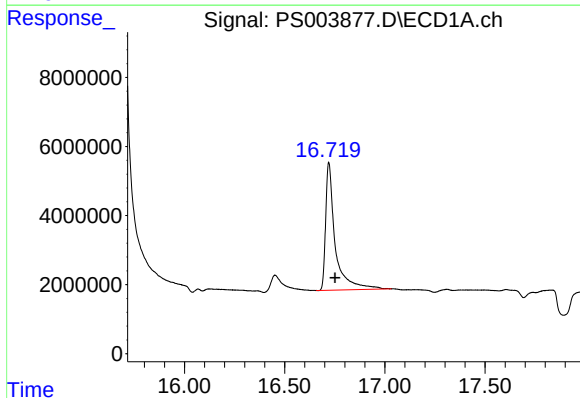


#15 Picloram

R.T.: 16.720 min
Delta R.T.: -0.032 min
Response: 123221912
Conc: 36.27 ng/ml

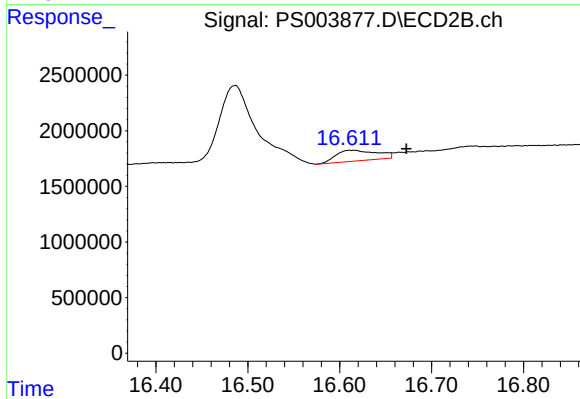

#15 Picloram


R.T.: 16.613 min
Delta R.T.: -0.060 min
Response: 2992428
Conc: 0.94 ng/ml

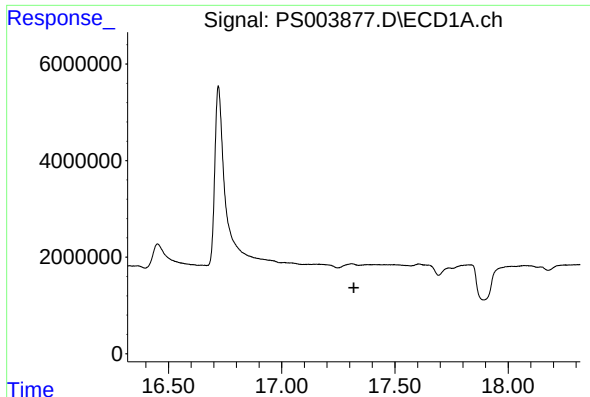

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

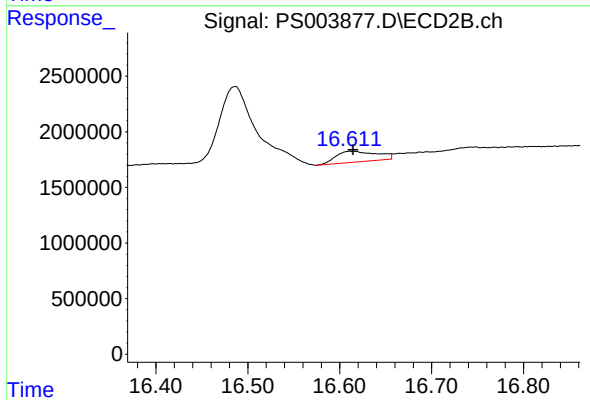

#16 DCPA

R.T.: 16.613 min
Delta R.T.: -0.001 min
Response: 2992428
Conc: 0.89 ng/ml