

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS033021\
 Data File : PS014403.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2021 09:08
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 11:20:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 18 02:23:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.165	6.890	583.1E6	237.0E6	408.079	502.457
Target Compounds							
5) T	DICAMBA	0.000	7.007f	0	486333	N.D.	<MDL
6) T	MCPD	7.553	0.000	4496667	0	1.081	N.D. #
7) T	MCPA	7.628	0.000	4687711	0	<MDL	N.D. #
9) T	2,4-D	8.338f	0.000	2919043	0	1.980	N.D. #
12) T	2,4,5-T	9.398	0.000	511614	0	<MDL	N.D. #
14) T	DINOSEB	11.047f	0.000	303885	0	<MDL	N.D. #
15) T	Picloram	10.985f	11.016f	28091632	11758714	2.690	3.100



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS033021\
Data File : PS014403.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Mar 2021 09:08
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 11:20:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
Quant Title : 8080.M
QLast Update : Thu Mar 18 02:23:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

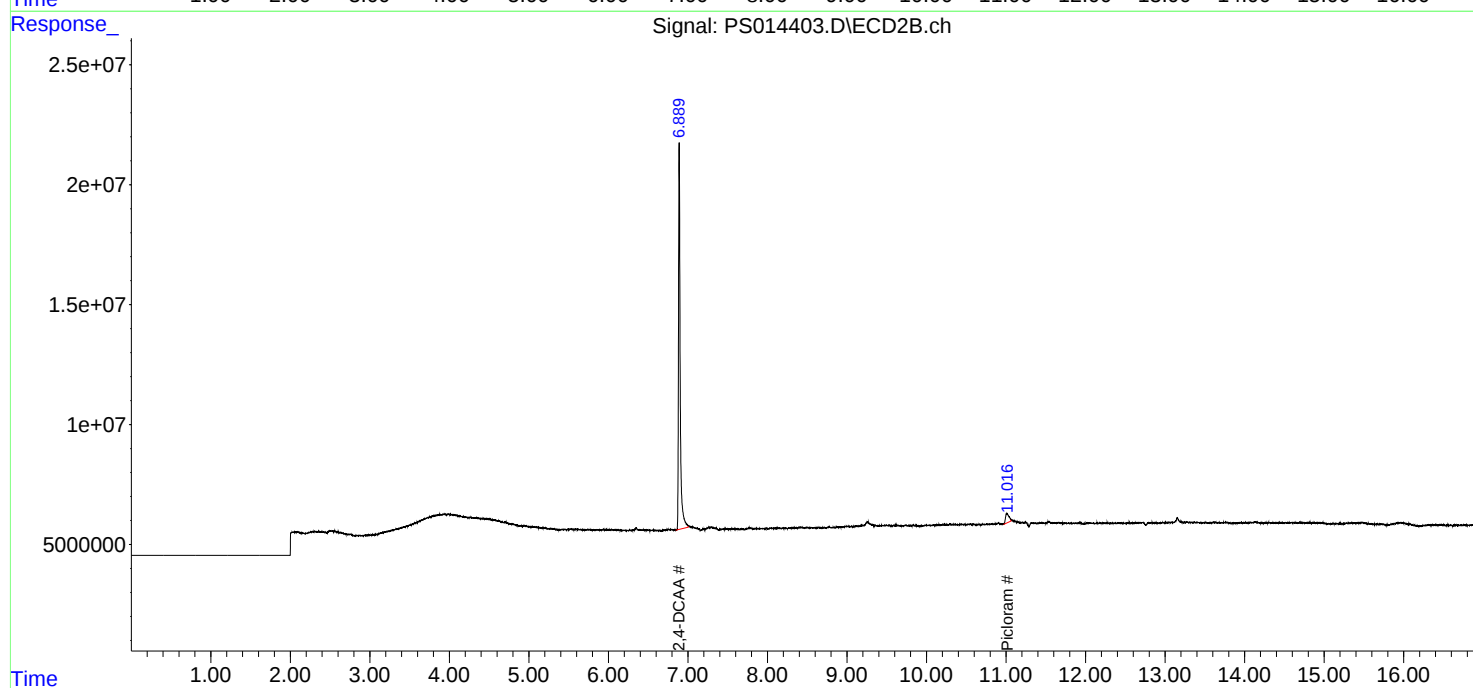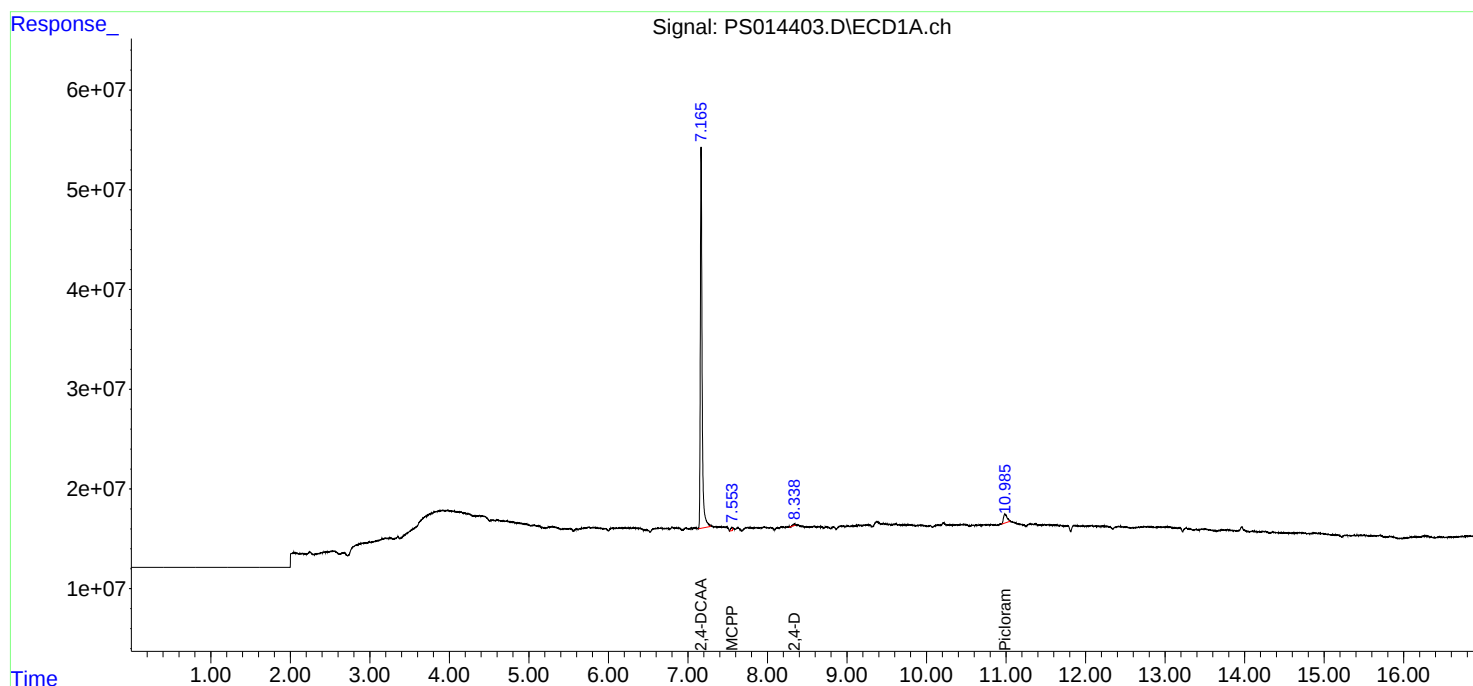


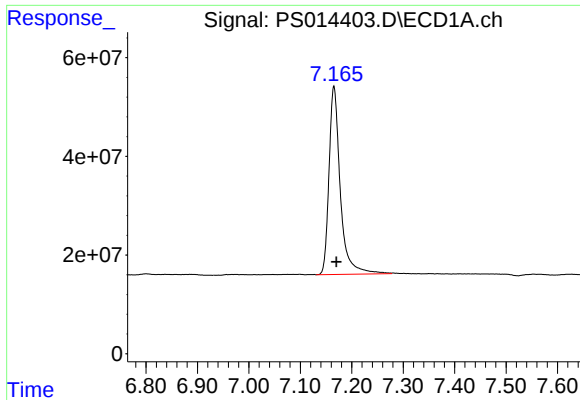

#4 2,4-DCAA


R.T.: 7.165 min
Delta R.T.: -0.005 min
Response: 583080946
Conc: 408.08 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

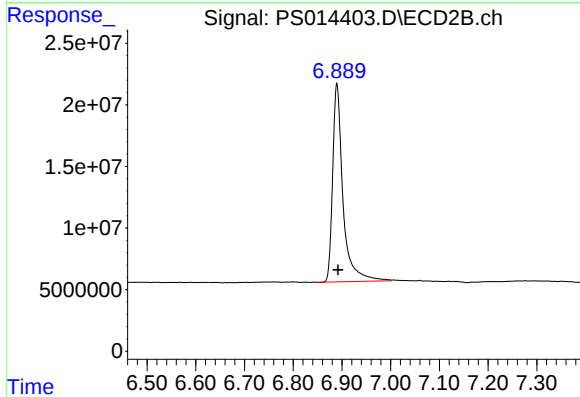


#4 2,4-DCAA

R.T.: 6.890 min
Delta R.T.: -0.002 min
Response: 237043730
Conc: 502.46 ng/ml

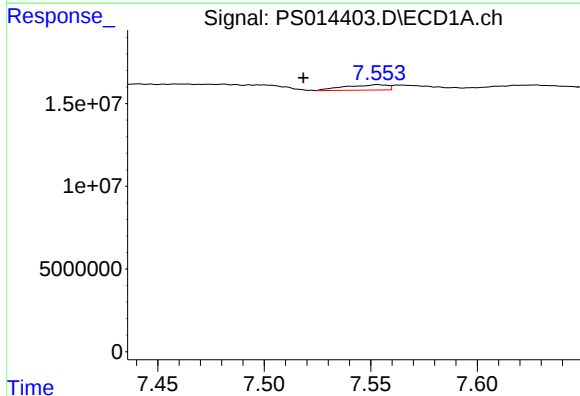


#6 MCP

R.T.: 7.553 min
Delta R.T.: 0.035 min
Response: 4496667
Conc: 1.08 ug/ml

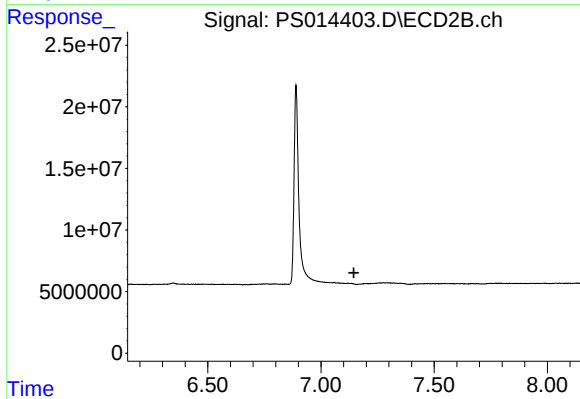

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.145 min
Response: 0
Conc: N.D.

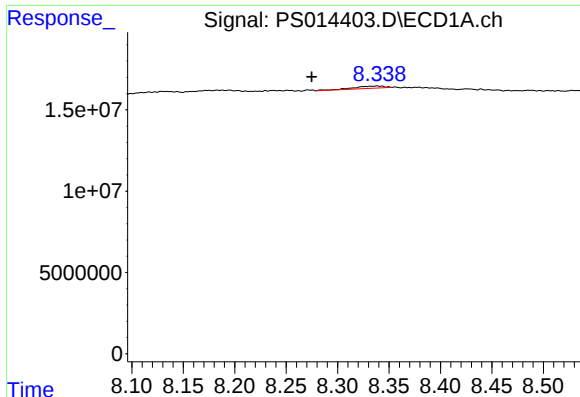

#9 2,4-D


R.T.: 8.338 min
Delta R.T.: 0.064 min
Response: 2919043
Conc: 1.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

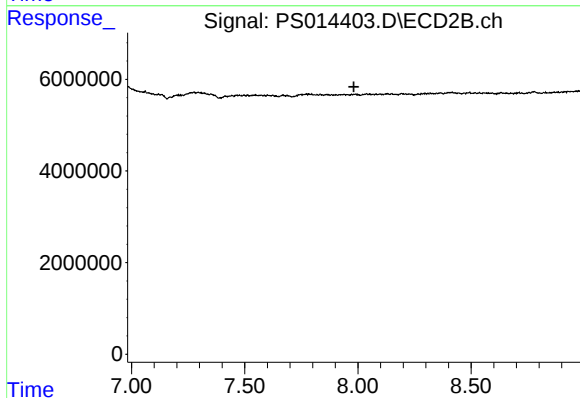


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.982 min
Response: 0
Conc: N.D.

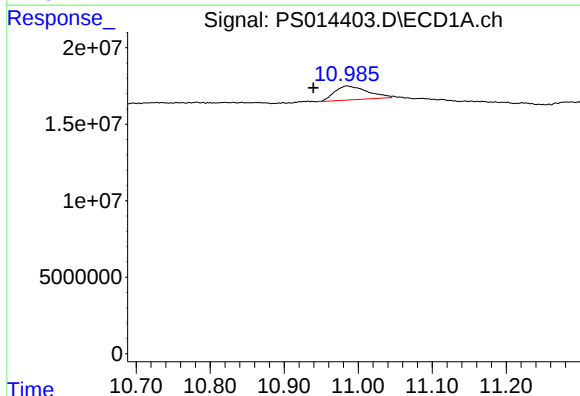

#15 Picloram

R.T.: 10.985 min
Delta R.T.: 0.046 min
Response: 28091632
Conc: 2.69 ng/ml

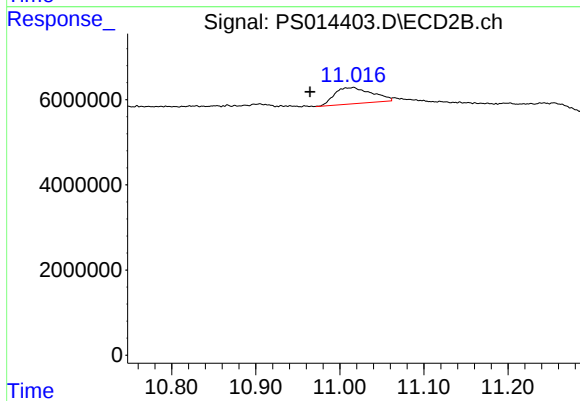

#15 Picloram

R.T.: 11.016 min
Delta R.T.: 0.052 min
Response: 11758714
Conc: 3.10 ng/ml