

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS033121\
 Data File : PS014422.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Mar 2021 17:05
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 18:25:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 18 02:23:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.161	6.887	670.9E6	255.1E6	469.567	540.792
Target Compounds							
9) T	2,4-D	8.336f	0.000	27423830	0	18.605	N.D. #
15) T	Picloram	10.975	0.000	268.3E6	0	25.689	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS033121\
Data File : PS014422.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Mar 2021 17:05
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 18:25:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
Quant Title : 8080.M
QLast Update : Thu Mar 18 02:23:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

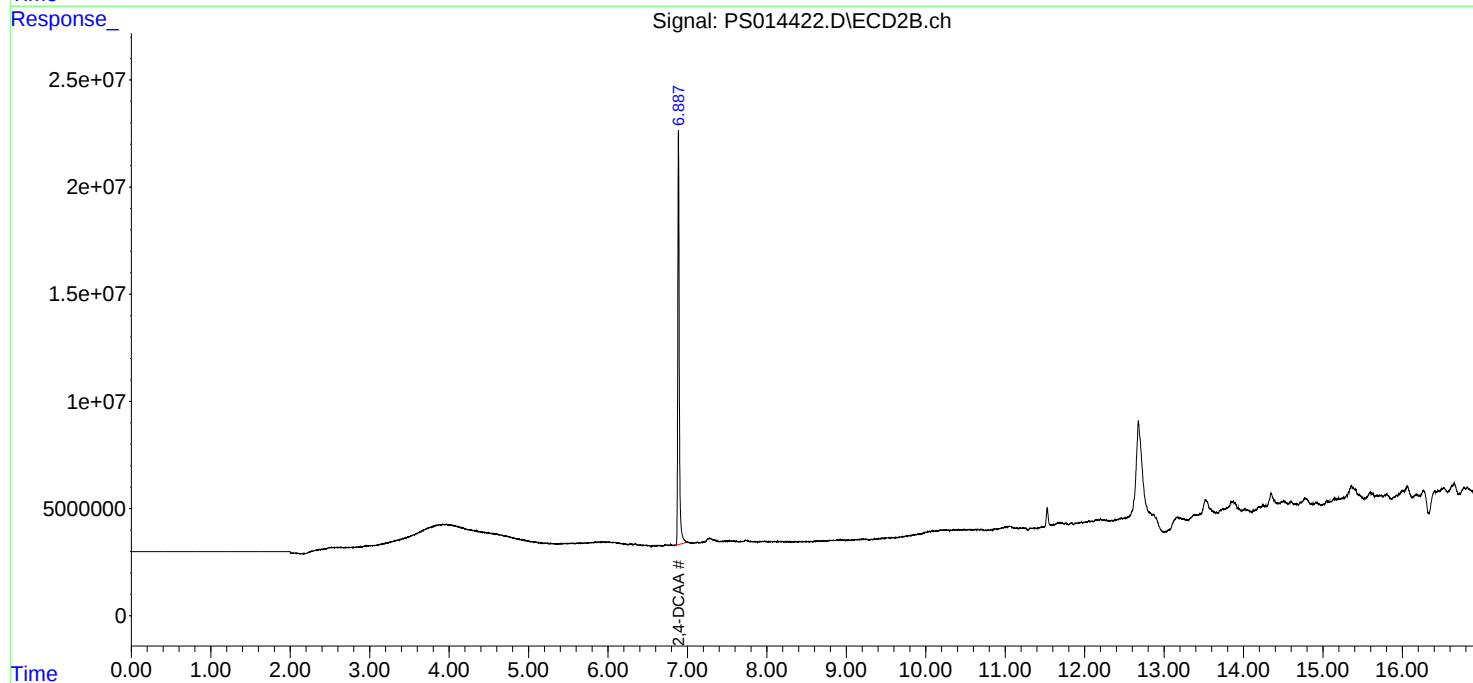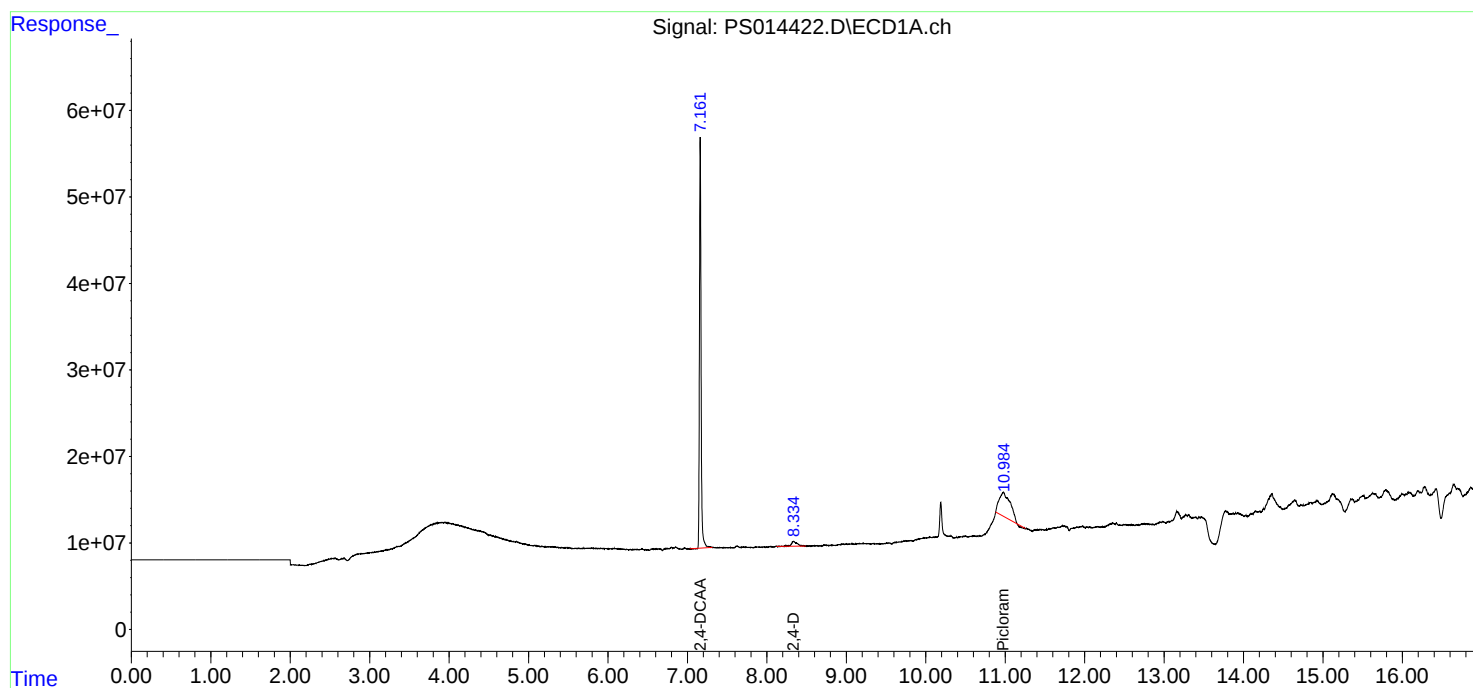


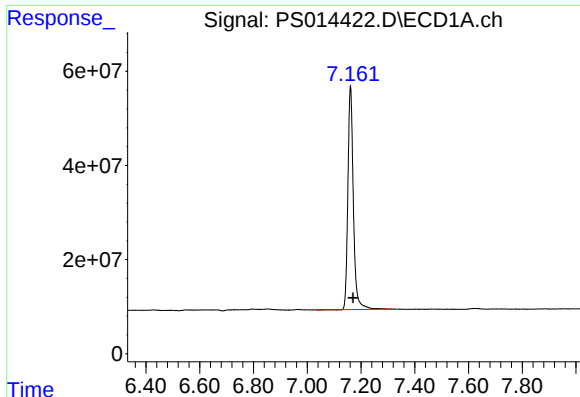

#4 2,4-DCAA


R.T.: 7.161 min
Delta R.T.: -0.009 min
Response: 670937321
Conc: 469.57 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

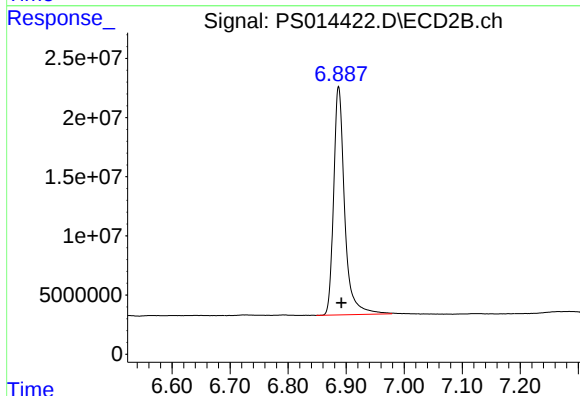


#4 2,4-DCAA

R.T.: 6.887 min
Delta R.T.: -0.005 min
Response: 255128679
Conc: 540.79 ng/ml

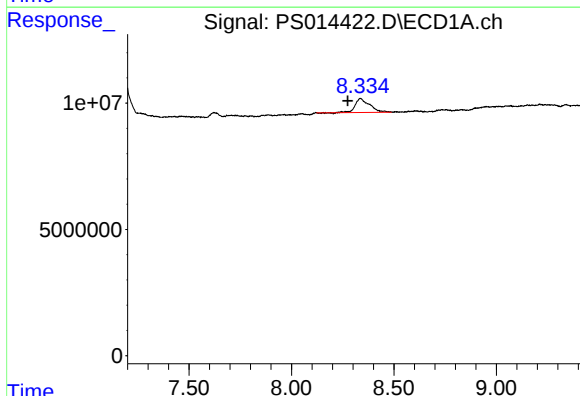


#9 2,4-D

R.T.: 8.336 min
Delta R.T.: 0.061 min
Response: 27423830
Conc: 18.61 ng/ml

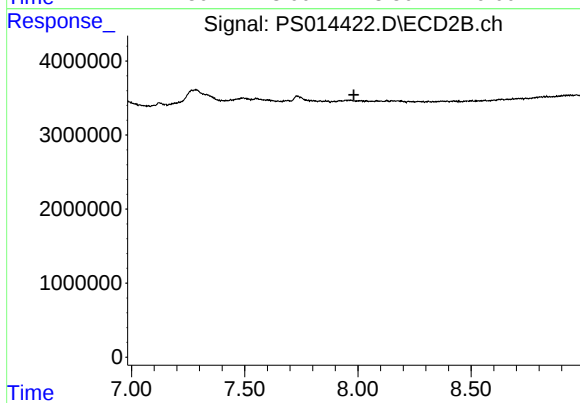

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.982 min
Response: 0
Conc: N.D.

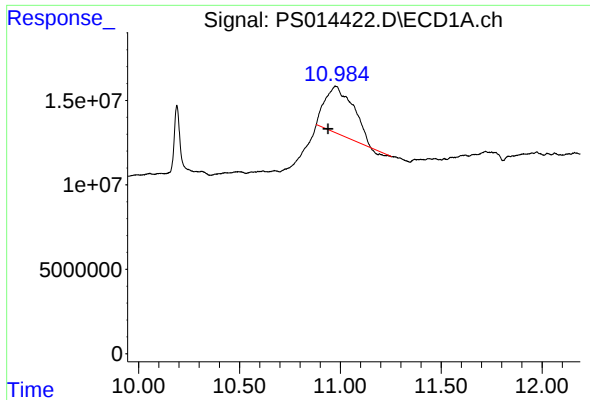

#15 Picloram

R.T.: 10.975 min
Delta R.T.: 0.036 min
Response: 268253450
Conc: 25.69 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

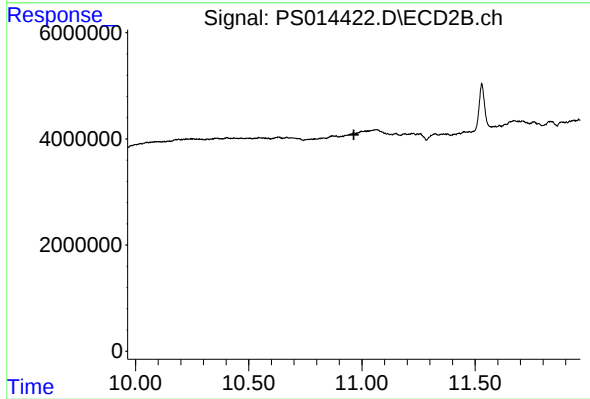

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.965 min
Response: 0
Conc: N.D.