

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS033121\
 Data File : PS014412.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Mar 2021 13:15
 Operator : DD\AJ
 Sample : M1813-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 L07

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 15:27:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 18 02:23:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.161	6.888	491.0E6	171.3E6	343.651	363.205
Target Compounds							
15) T	Picloram	10.935	10.969	446.2E6	168.3E6	42.731	44.356



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS033121\
Data File : PS014412.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Mar 2021 13:15
Operator : DD\AJ
Sample : M1813-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
L07

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 15:27:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
Quant Title : 8080.M
QLast Update : Thu Mar 18 02:23:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

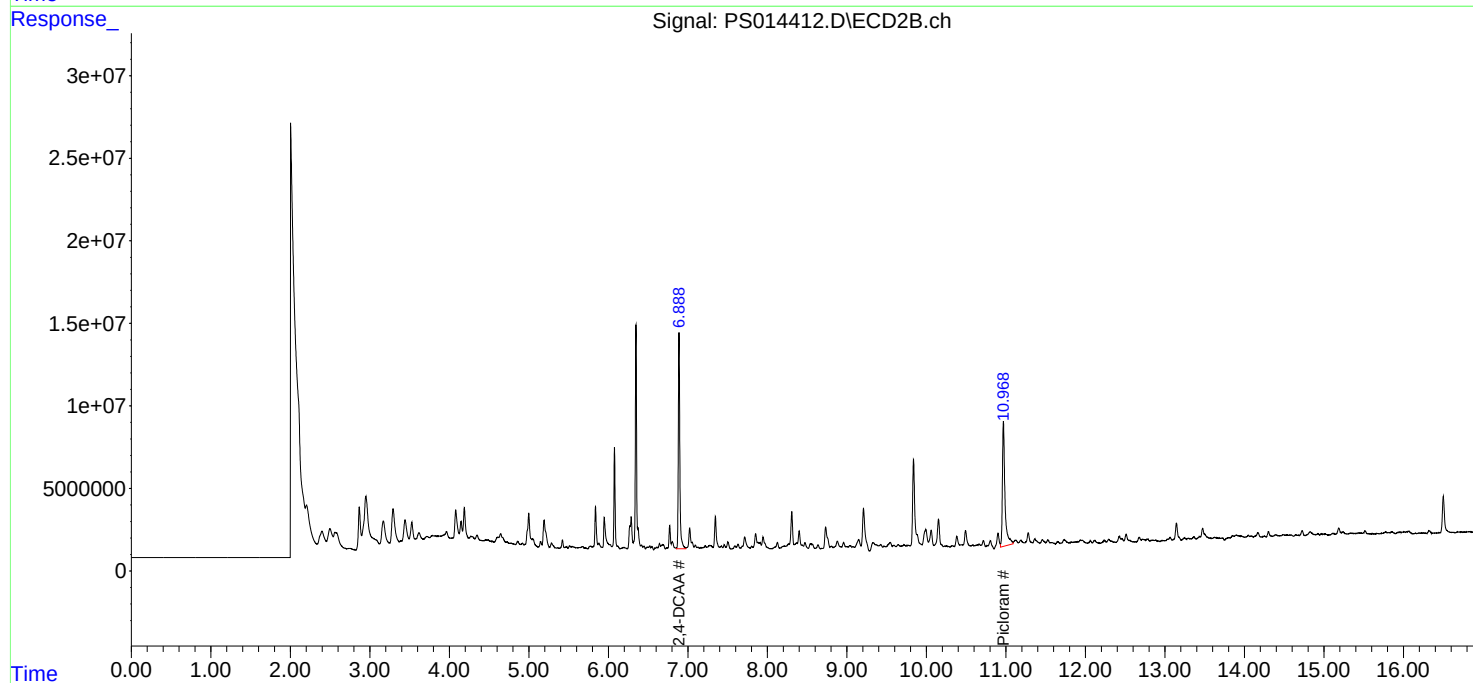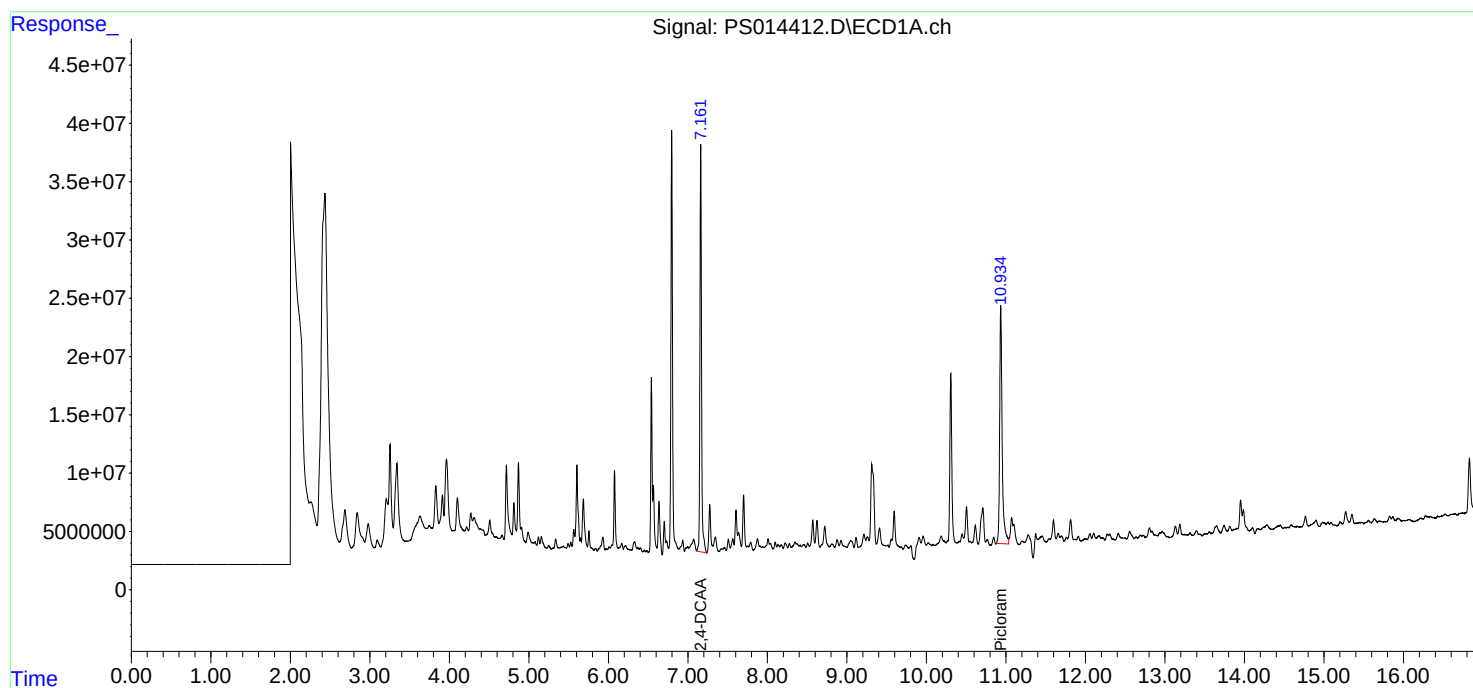


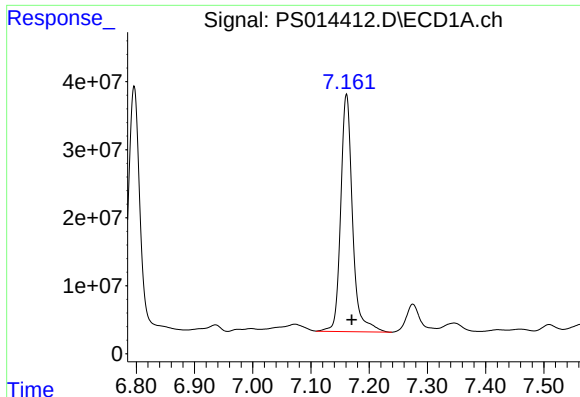

#4 2,4-DCAA


R.T.: 7.161 min
Delta R.T.: -0.009 min
Response: 491023545
Conc: 343.65 ng/ml

Instrument :
ECD_S
ClientSampleId :
L07

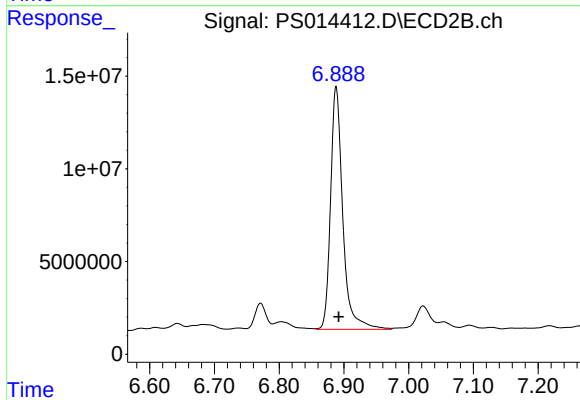


#4 2,4-DCAA

R.T.: 6.888 min
Delta R.T.: -0.004 min
Response: 171348881
Conc: 363.21 ng/ml

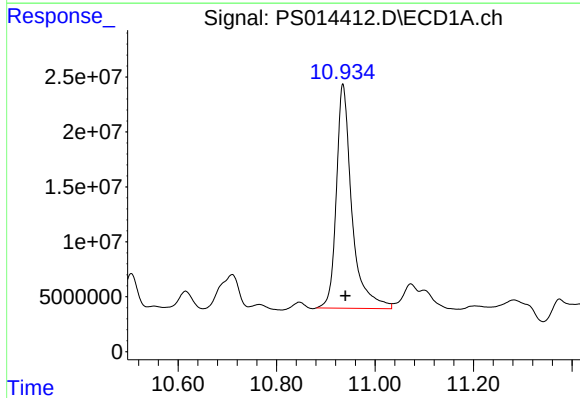

#15 Picloram

R.T.: 10.935 min
Delta R.T.: -0.005 min
Response: 446217020
Conc: 42.73 ng/ml

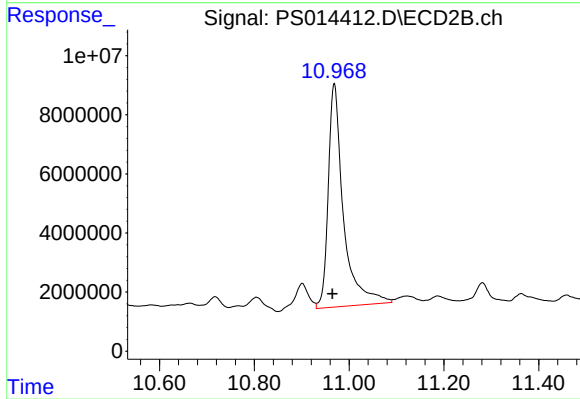

#15 Picloram

R.T.: 10.969 min
Delta R.T.: 0.004 min
Response: 168273541
Conc: 44.36 ng/ml