Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS033121\
Data File : PS014429.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Mar 2021 19:47
Operator : DD\AJ
Sample : M1855-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
EMBANKMENT-FILL-COMPOSITE

Manual Integrations APPROVED
Ankita
4/1/2021 12:54:47 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 02:07:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
Quant Title : 8080.M
QLast Update : Thu Mar 18 02:23:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
	System Monitoring Compounds						
4) S	2,4-DCAA	7.159	6.886	237.4E6	89424133	166.142m	189.551
	Target Compounds						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS033121\
Data File : PS014429.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Mar 2021 19:47
Operator : DD\AJ
Sample : M1855-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
EMBANKMENT-FILL-COMPOSITE

Manual Integrations APPROVED
Ankita
4/1/2021 12:54:47 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 02:07:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
Quant Title : 8080.M
QLast Update : Thu Mar 18 02:23:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

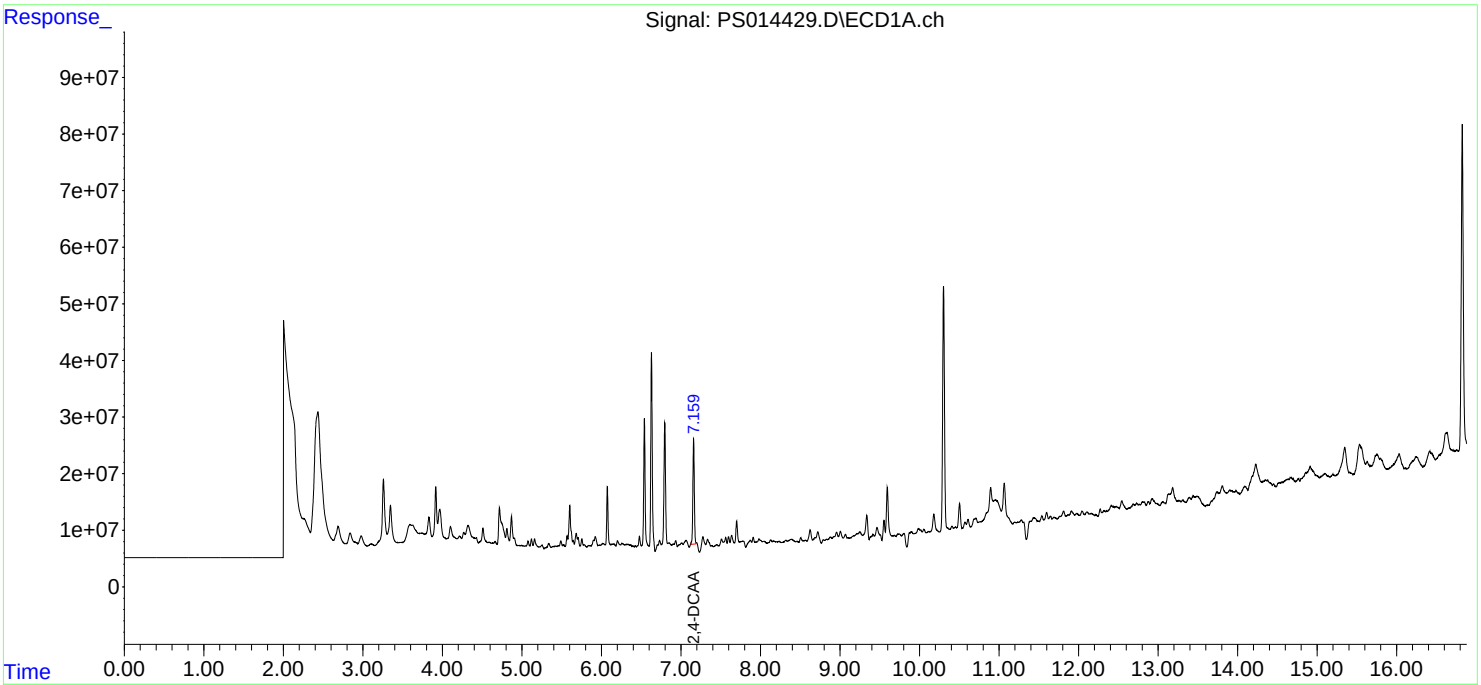

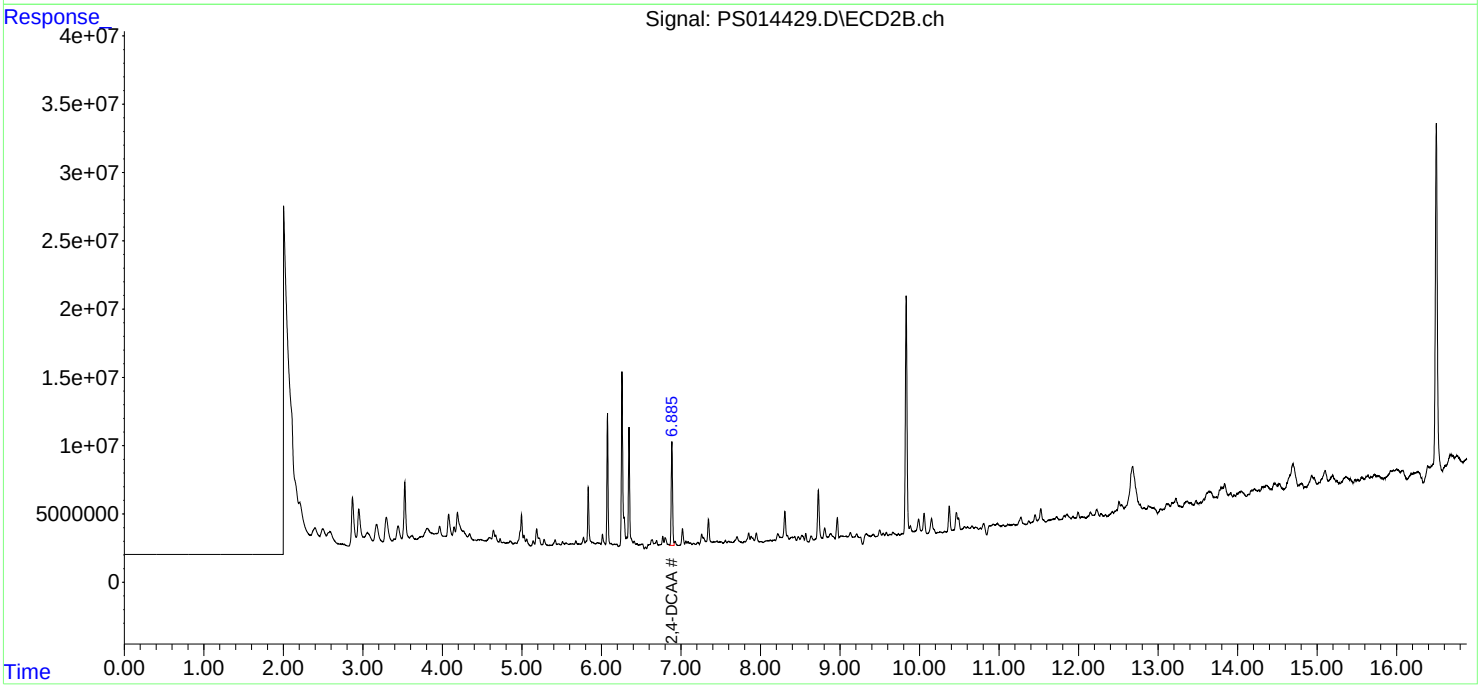

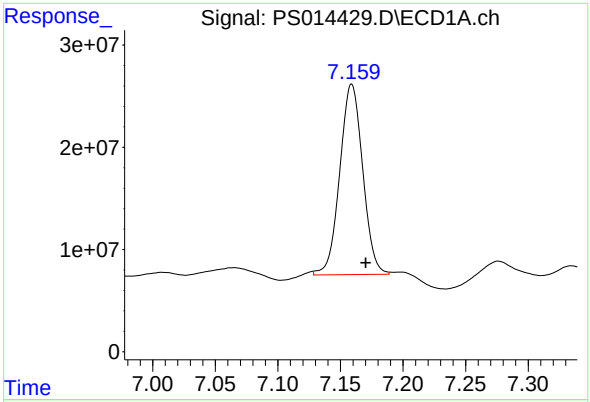

#4 2,4-DCAA

R.T.: 7.159 min
Delta R.T.: -0.012 min
Response: 237390674
Conc: 166.14 ng/ml m

Instrument :
ECD_S
ClientSampleId :
EMBANKMENT-FILL-COMPOSITE

Manual Integrations APPROVED

Ankita
4/1/2021 12:54:47 PM

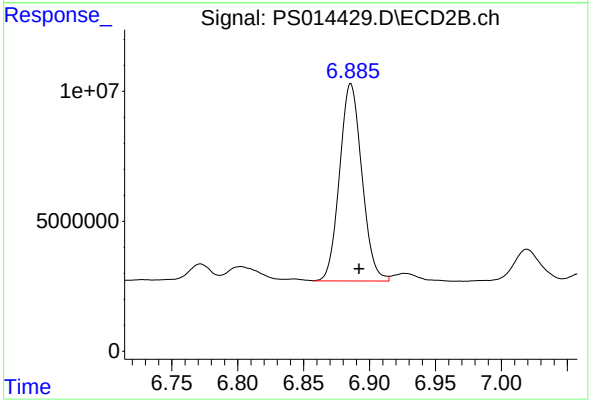

#4 2,4-DCAA

R.T.: 6.886 min
Delta R.T.: -0.006 min
Response: 89424133
Conc: 189.55 ng/ml