

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS033123\
 Data File : PS022557.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Mar 2023 08:49
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 22:00:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032023.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 20 15:46:44 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.305	0.000	1637837	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.366	0.000	157568	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.694	0.000	1490163	0	<MDL	N.D. #
3) T	4-Nitroph...	6.116	0.000	125690	0	<MDL	N.D. #
6) T	MCP	0.000	6.948	0	1977893	N.D.	<MDL
8) T	DICHLORPROP	6.971f	0.000	170545	0	<MDL	N.D. #
9) T	2,4-D	7.205	0.000	39403	0	<MDL	N.D. #
10) T	Pentachlo...	7.448	0.000	500188	0	<MDL	N.D. #
11) T	2,4,5-TP ...	7.965	0.000	1401910	0	<MDL	N.D. #
13) T	2,4-DB	8.668f	9.432	717398	1920887	<MDL	1.144 #
14) T	DINOSEB	9.780	0.000	141236	0	<MDL	N.D. #
15) T	Picloram	9.628	10.703	181362	12903710	<MDL	<MDL #
16) T	DCPA	0.000	10.703	0	12903710	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS033123\
Data File : PS022557.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Mar 2023 08:49
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 22:00:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032023.M
Quant Title : 8080.M
QLast Update : Mon Mar 20 15:46:44 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

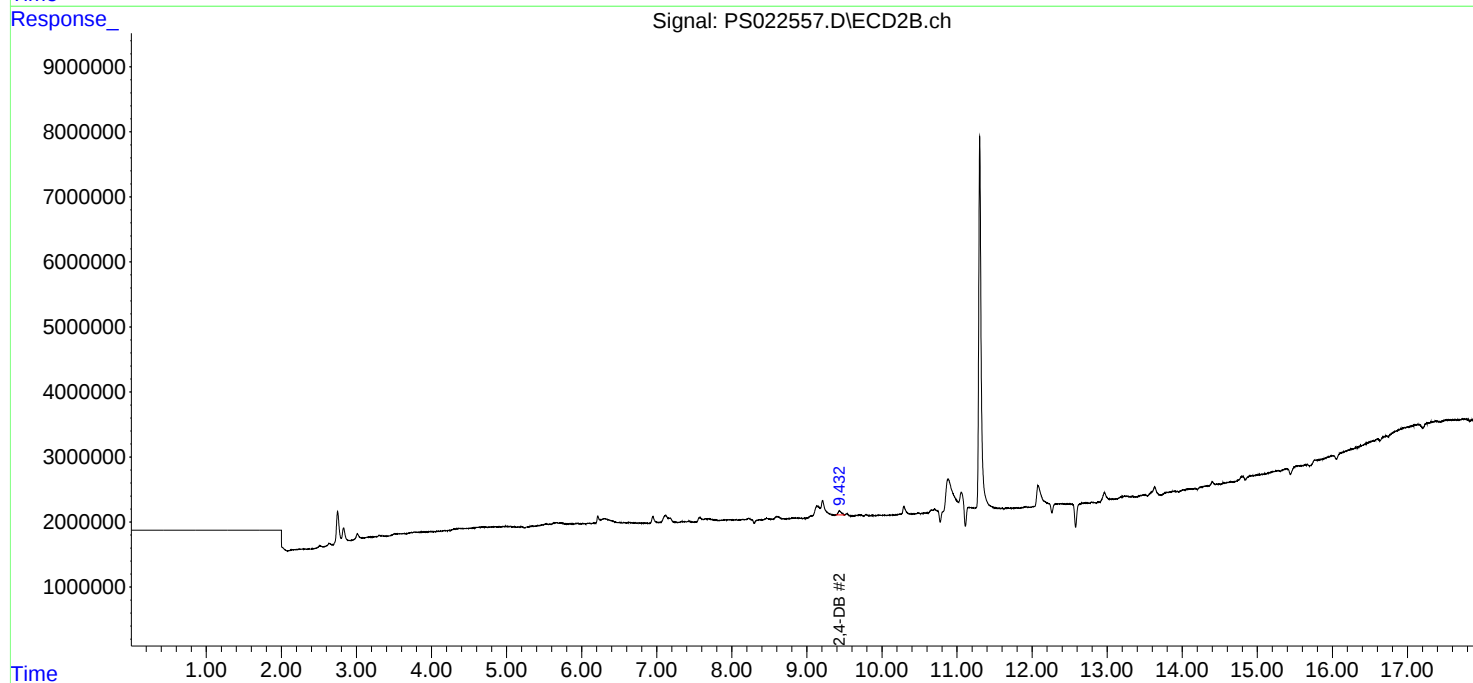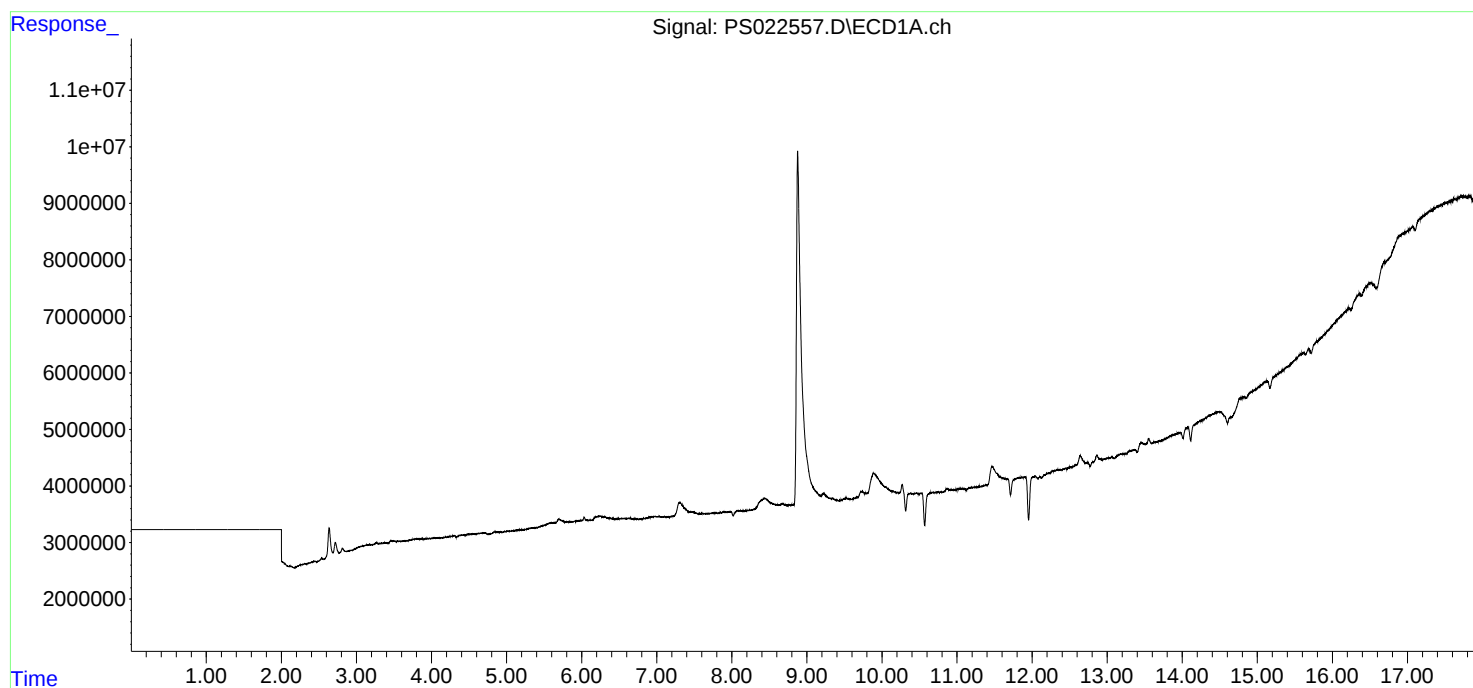


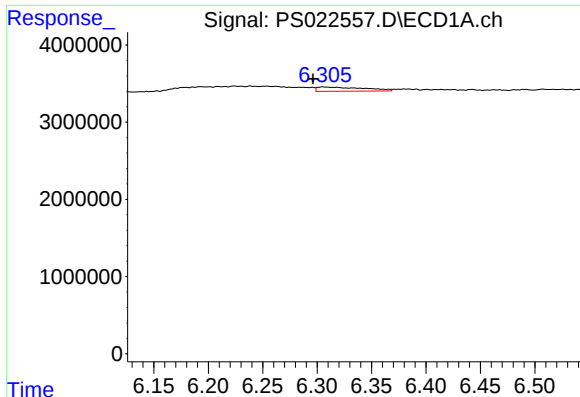

#4 2,4-DCAA


R.T.: 6.305 min
Delta R.T.: 0.009 min
Response: 1637837
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

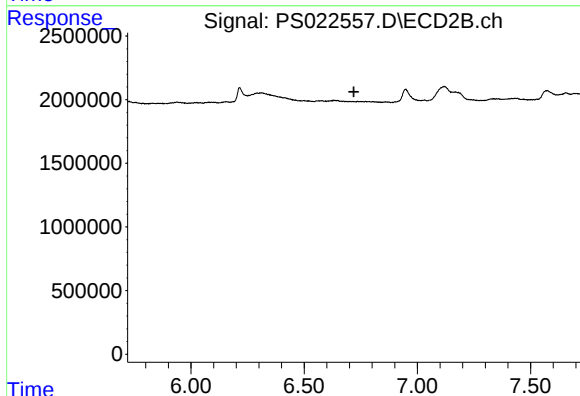


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.719 min
Response: 0
Conc: N.D.

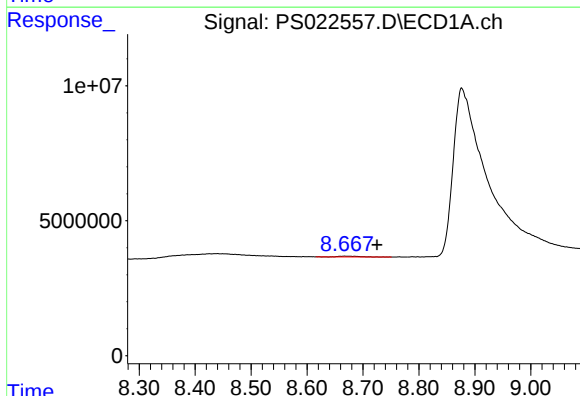

#13 2,4-DB

R.T.: 8.668 min
Delta R.T.: -0.057 min
Response: 717398
Conc: N.D.

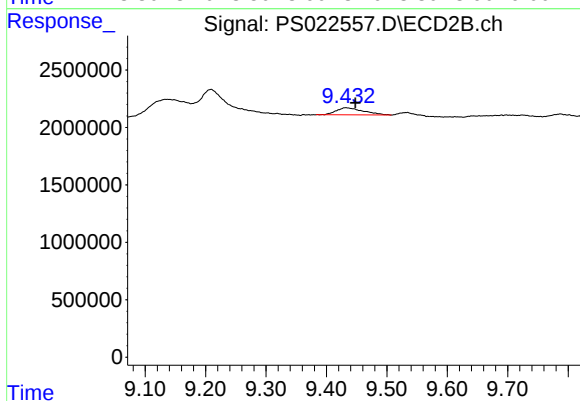

#13 2,4-DB

R.T.: 9.432 min
Delta R.T.: -0.017 min
Response: 1920887
Conc: 1.14 ng/ml