

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040119\
 Data File : PS003879.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Apr 2019 08:38
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 05:17:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.770	0	195067	N.D.	<MDL
Target Compounds							
2) T	3,5-DICHL...	0.000	8.914	0	3405	N.D.	<MDL
3) T	4-Nitroph...	10.870	9.959	2654827	2282530	12.253	10.054
5) T	DICAMBA	0.000	11.075	0	118139	N.D.	<MDL
6) T	MCP	0.000	11.284	0	189364	N.D.	<MDL
9) T	2,4-D	0.000	12.634	0	467088	N.D.	<MDL
10) T	Pentachlo...	0.000	13.203	0	241744	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.786	0	360699	N.D.	<MDL
12) T	2,4,5-T	0.000	14.368	0	994757	N.D.	<MDL
13) T	2,4-DB	0.000	14.989	0	6434794	N.D.	21.670
14) T	DINOSEB	0.000	15.411	0	4223213	N.D.	2.201
15) T	Picloram	16.717	16.678	85055040	3012055	25.038	<MDL #
16) T	DCPA	0.000	16.613	0	2906571	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040119\
Data File : PS003879.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Apr 2019 08:38
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 05:17:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

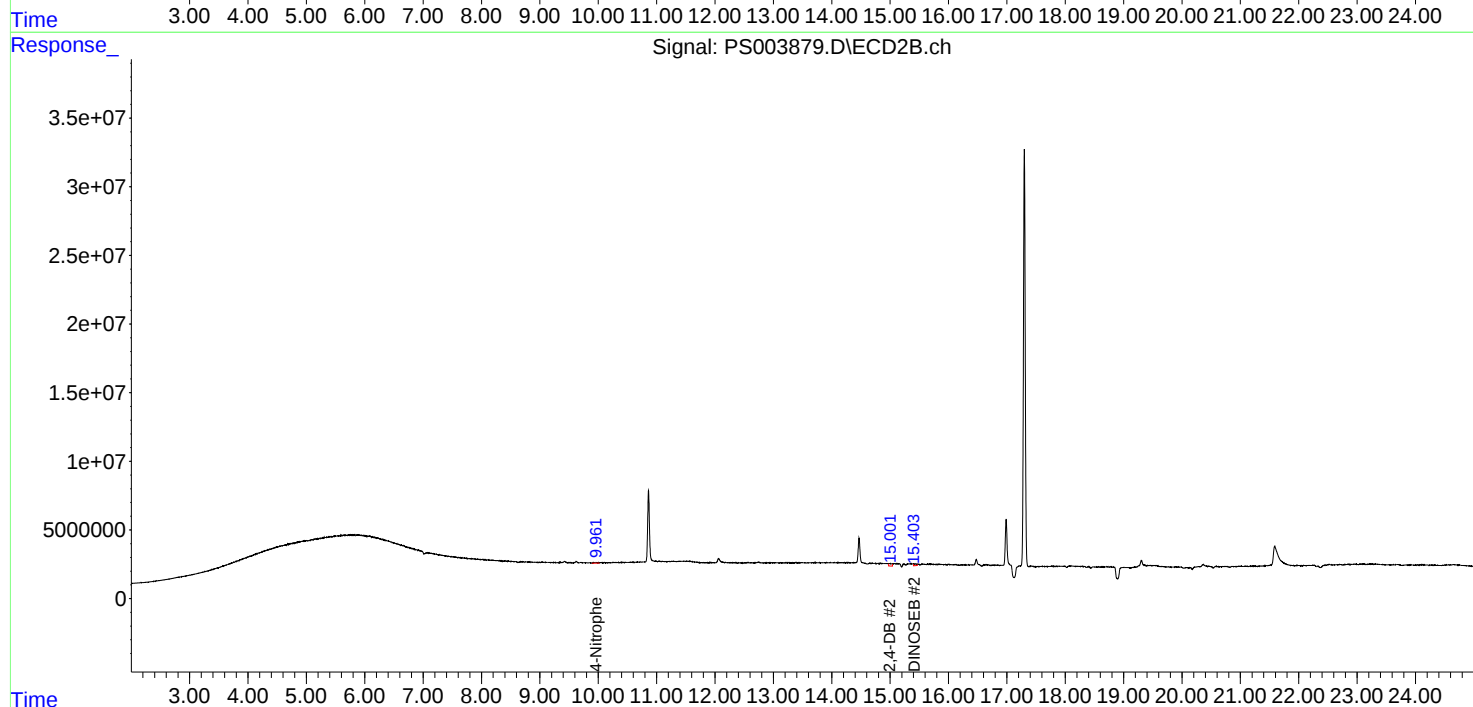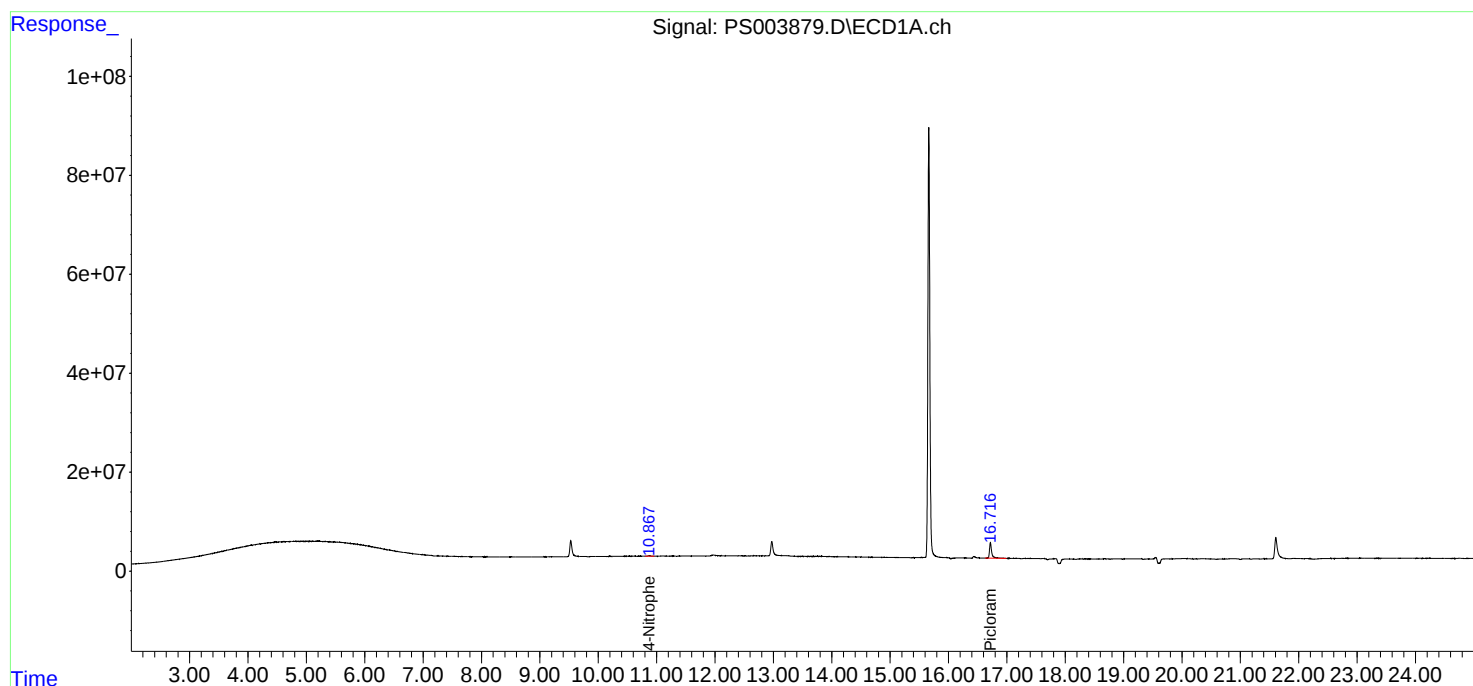


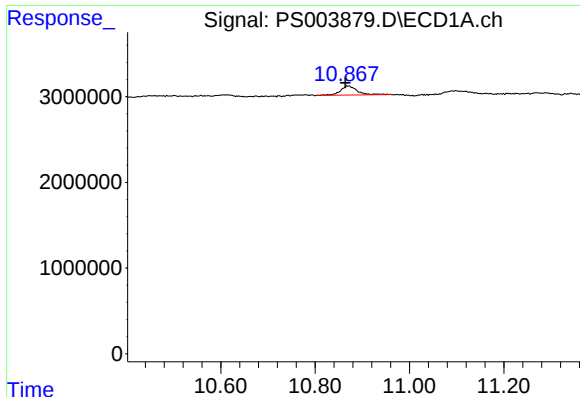

#3 4-Nitrophenol


R.T.: 10.870 min
Delta R.T.: 0.006 min
Response: 2654827
Conc: 12.25 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

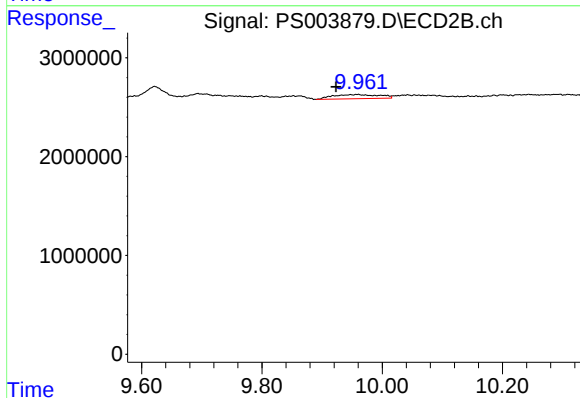


#3 4-Nitrophenol

R.T.: 9.959 min
Delta R.T.: 0.035 min
Response: 2282530
Conc: 10.05 ng/ml

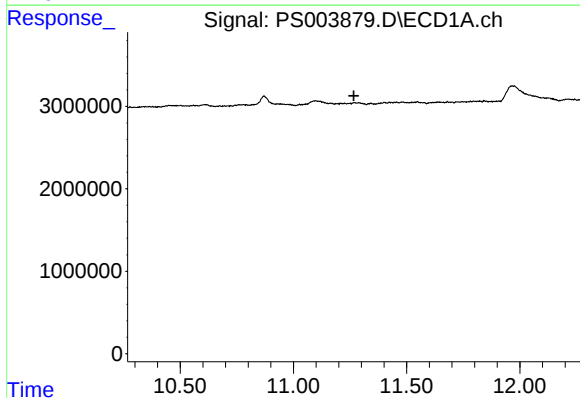


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 11.267 min
Response: 0
Conc: N.D.

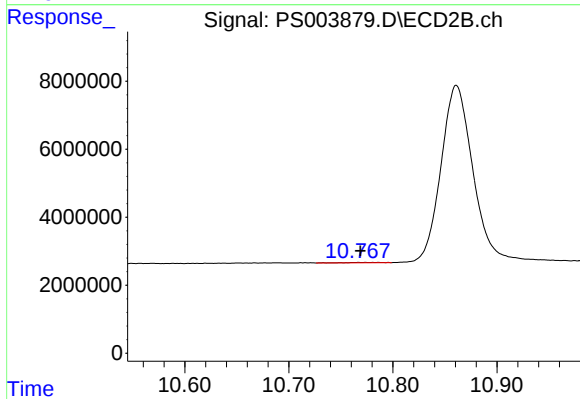

#4 2,4-DCAA


R.T.: 10.770 min
Delta R.T.: 0.001 min
Response: 195067
Conc: N.D.

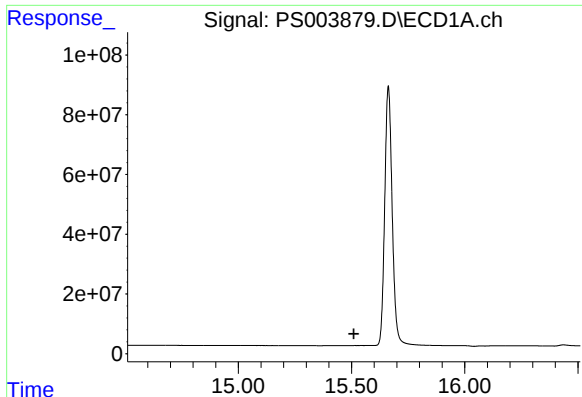

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

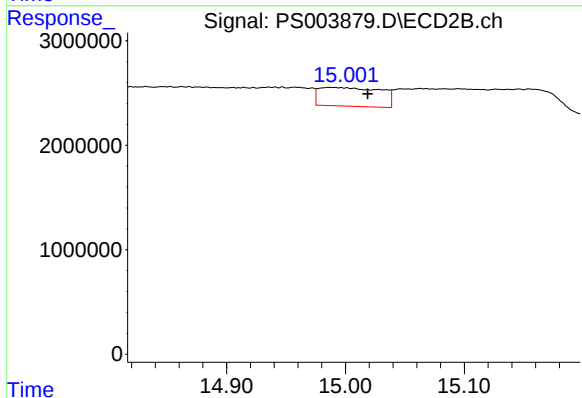


#13 2,4-DB

R.T.: 14.989 min
Delta R.T.: -0.030 min
Response: 6434794
Conc: 21.67 ng/ml

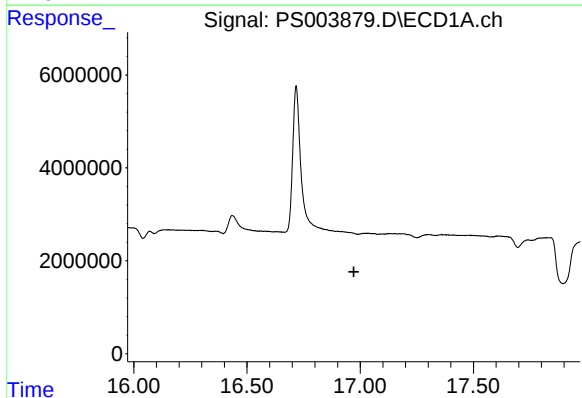


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.972 min
Response: 0
Conc: N.D.

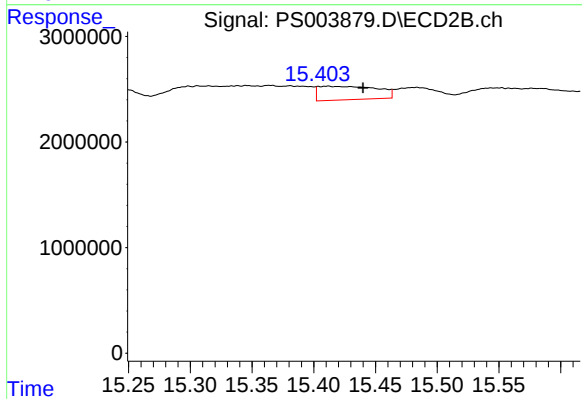

#14 DINOSEB


R.T.: 15.411 min
Delta R.T.: -0.029 min
Response: 4223213
Conc: 2.20 ng/ml

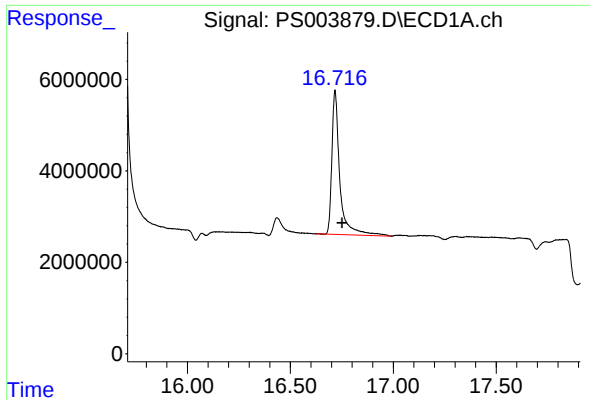

#15 Picloram

R.T.: 16.717 min
Delta R.T.: -0.034 min
Response: 85055040
Conc: 25.04 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

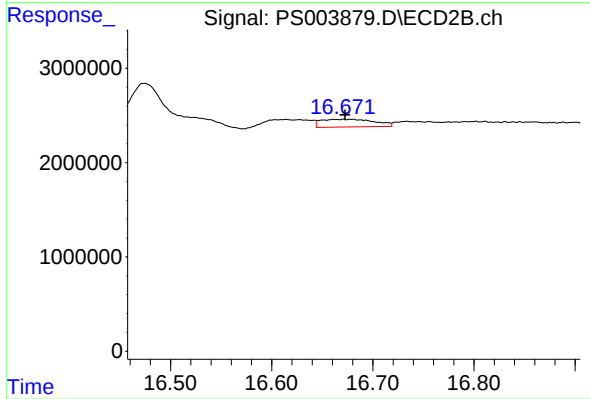

#15 Picloram

R.T.: 16.678 min
Delta R.T.: 0.005 min
Response: 3012055
Conc: N.D.