

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040119\
 Data File : PS003880.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Apr 2019 09:09
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 05:17:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.287	10.785	184.5E6	174.4E6	422.983	355.528
Target Compounds							
2) T	3,5-DICHL...	0.000	8.992	0	50553	N.D.	<MDL
3) T	4-Nitroph...	0.000	9.948	0	388560	N.D.	1.711
6) T	MCP	0.000	11.275	0	55304	N.D.	<MDL
7) T	MCPA	0.000	11.670	0	476165	N.D.	<MDL
8) T	DICHLORPROP	0.000	12.143	0	20569	N.D.	<MDL
9) T	2,4-D	0.000	12.666	0	90174	N.D.	<MDL
10) T	Pentachlo...	0.000	13.198	0	1076560	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.799	0	78686	N.D.	<MDL
12) T	2,4,5-T	0.000	14.381	0	37438	N.D.	<MDL
13) T	2,4-DB	0.000	15.035	0	421006	N.D.	1.418
14) T	DINOSEB	0.000	15.406	0	66299	N.D.	<MDL
15) T	Picloram	0.000	16.699	0	92430	N.D.	<MDL
16) T	DCPA	0.000	16.629	0	596347	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040119\
Data File : PS003880.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Apr 2019 09:09
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 05:17:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

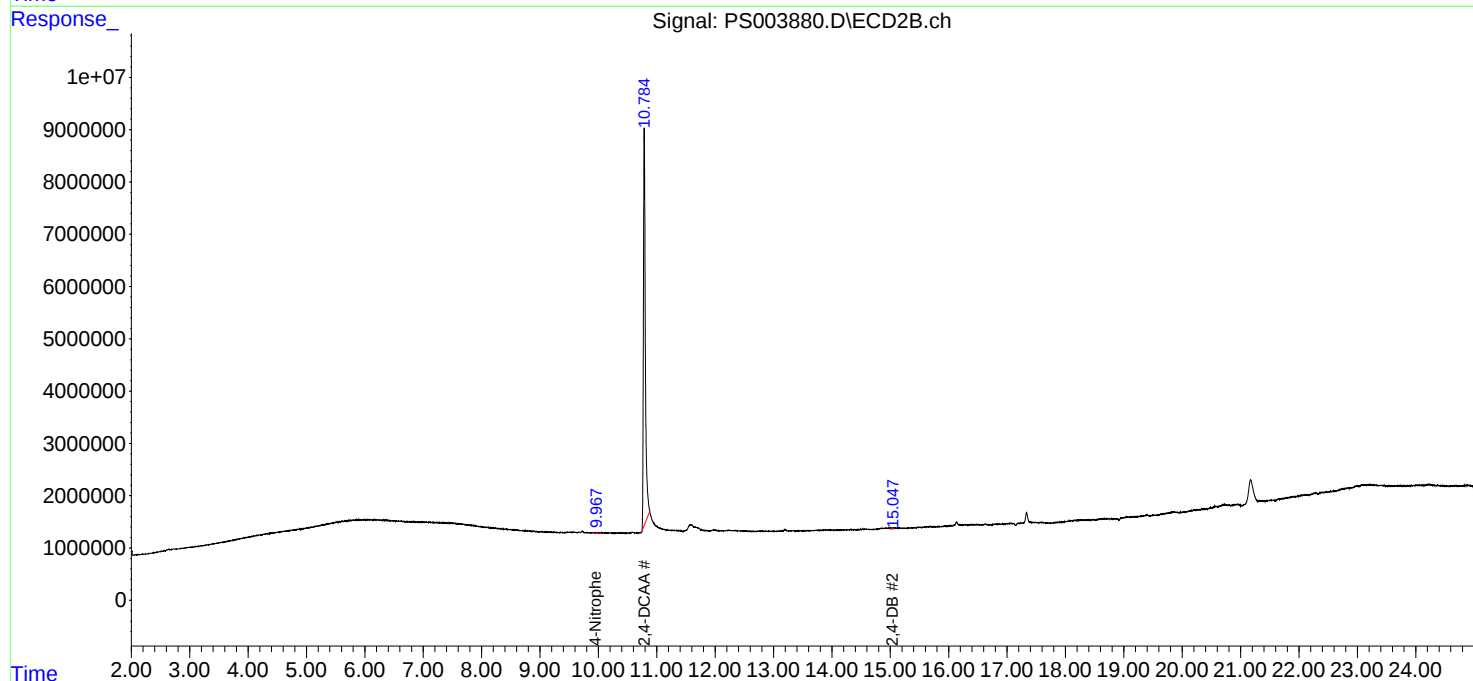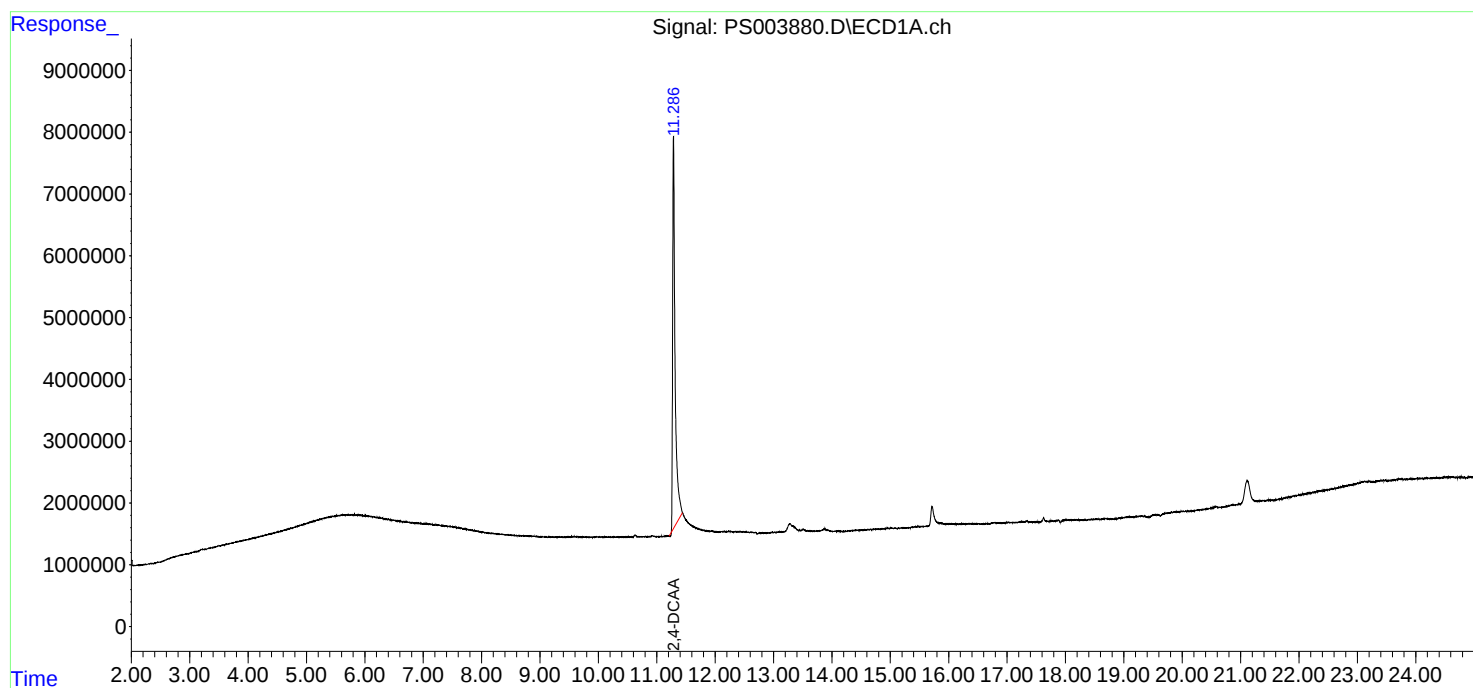


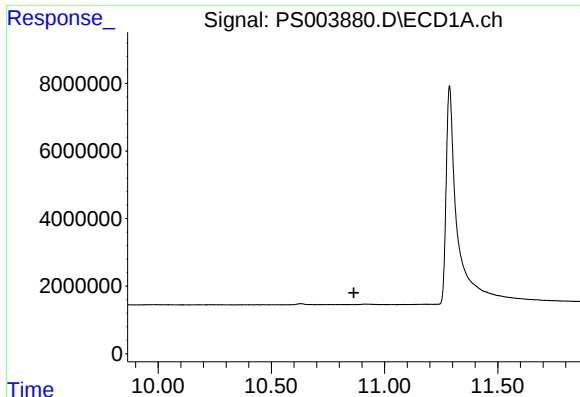

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

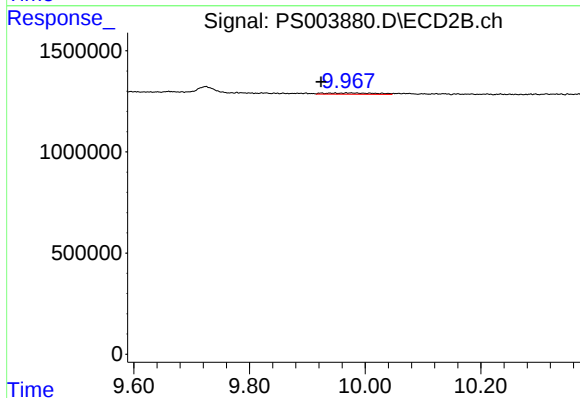


#3 4-Nitrophenol

R.T.: 9.948 min
Delta R.T.: 0.024 min
Response: 388560
Conc: 1.71 ng/ml

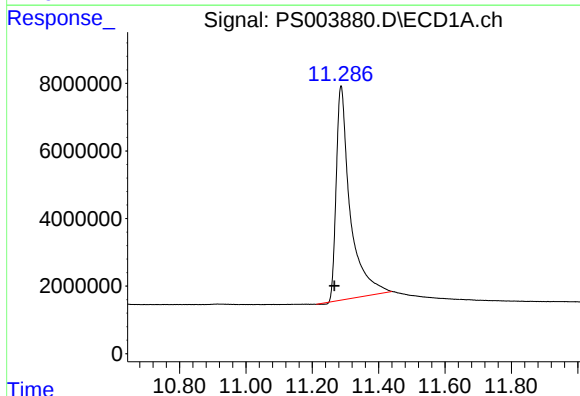


#4 2,4-DCAA

R.T.: 11.287 min
Delta R.T.: 0.020 min
Response: 184510354
Conc: 422.98 ng/ml

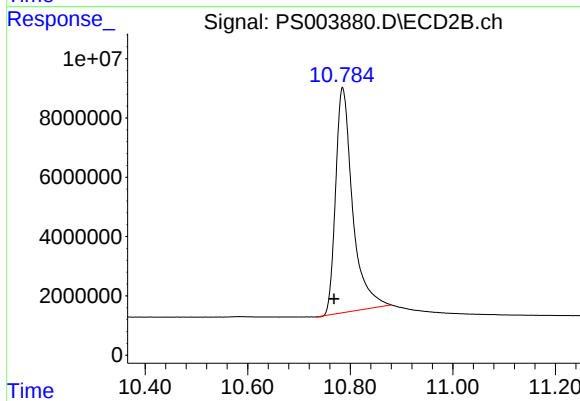

#4 2,4-DCAA


R.T.: 10.785 min
Delta R.T.: 0.017 min
Response: 174442586
Conc: 355.53 ng/ml

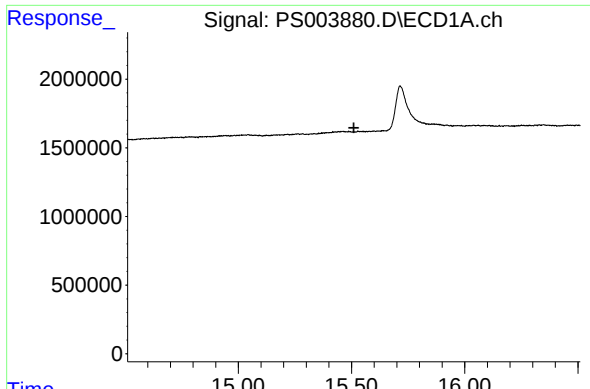

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

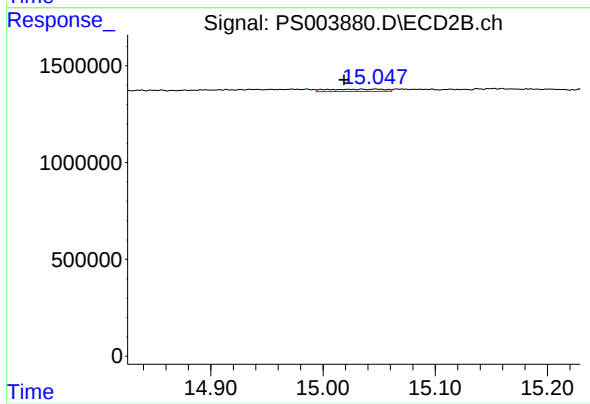

#13 2,4-DB

R.T.: 15.035 min
Delta R.T.: 0.016 min
Response: 421006
Conc: 1.42 ng/ml