

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040119\
 Data File : PS003883.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Apr 2019 13:46
 Operator : EI\SJ
 Sample : MDL-Herb-S-BL-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 MDL-Herb-S-BL-04

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 05:18:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.273	10.764	211.2E6	209.6E6	484.160	427.191
Target Compounds							
2) T	3,5-DICHL...	0.000	8.940	0	45262	N.D.	<MDL
3) T	4-Nitroph...	0.000	9.934	0	35697	N.D.	<MDL
7) T	MCPA	0.000	11.689	0	154223	N.D.	<MDL
8) T	DICHLORPROP	0.000	12.165	0	107094	N.D.	<MDL
9) T	2,4-D	13.193	12.609	23575044	25010	48.481	<MDL #
10) T	Pentachlo...	0.000	13.134	0	647679	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.812	0	85960	N.D.	<MDL
12) T	2,4,5-T	0.000	14.328	0	153374	N.D.	<MDL
13) T	2,4-DB	0.000	15.046	0	186744	N.D.	<MDL
14) T	DINOSEB	0.000	15.438	0	563612	N.D.	<MDL
15) T	Picloram	0.000	16.603	0	342085	N.D.	<MDL
16) T	DCPA	0.000	16.603	0	342085	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040119\
Data File : PS003883.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Apr 2019 13:46
Operator : EI\SJ
Sample : MDL-Herb-S-BL-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
MDL-Herb-S-BL-04

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 05:18:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

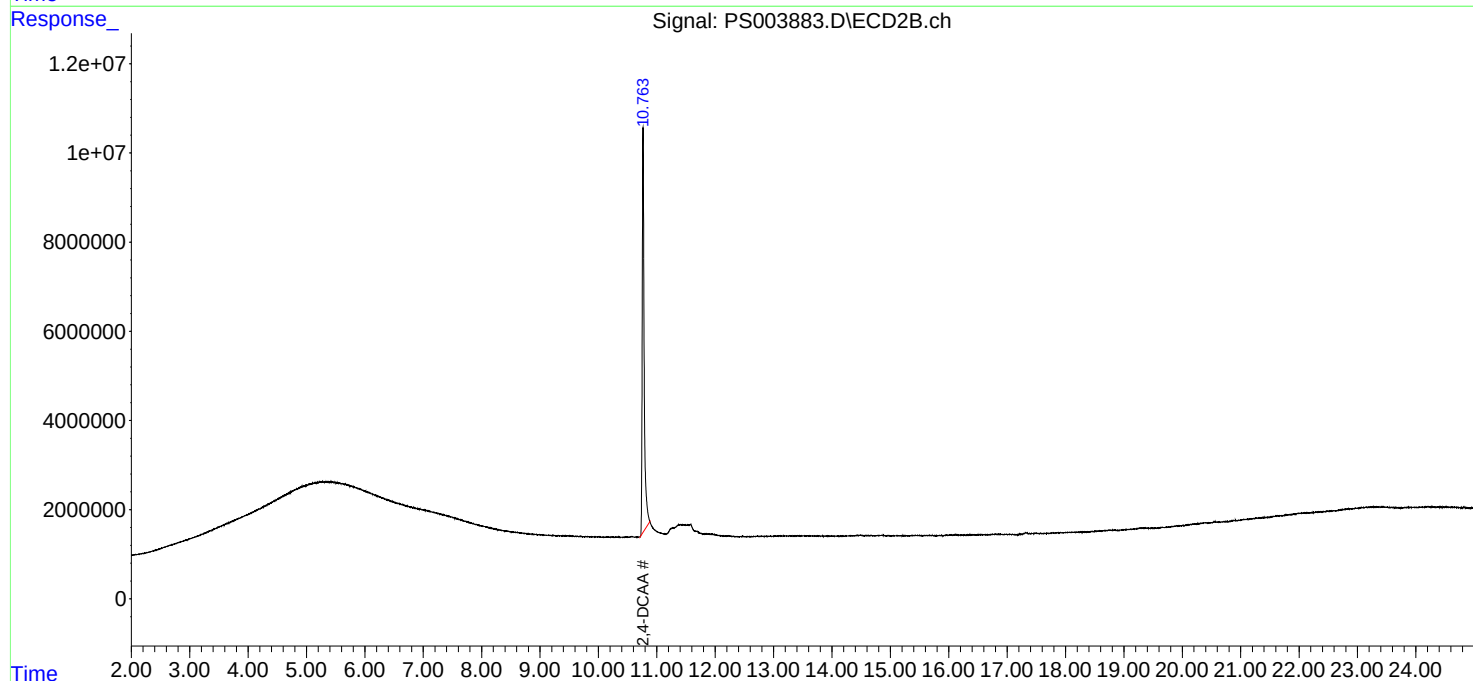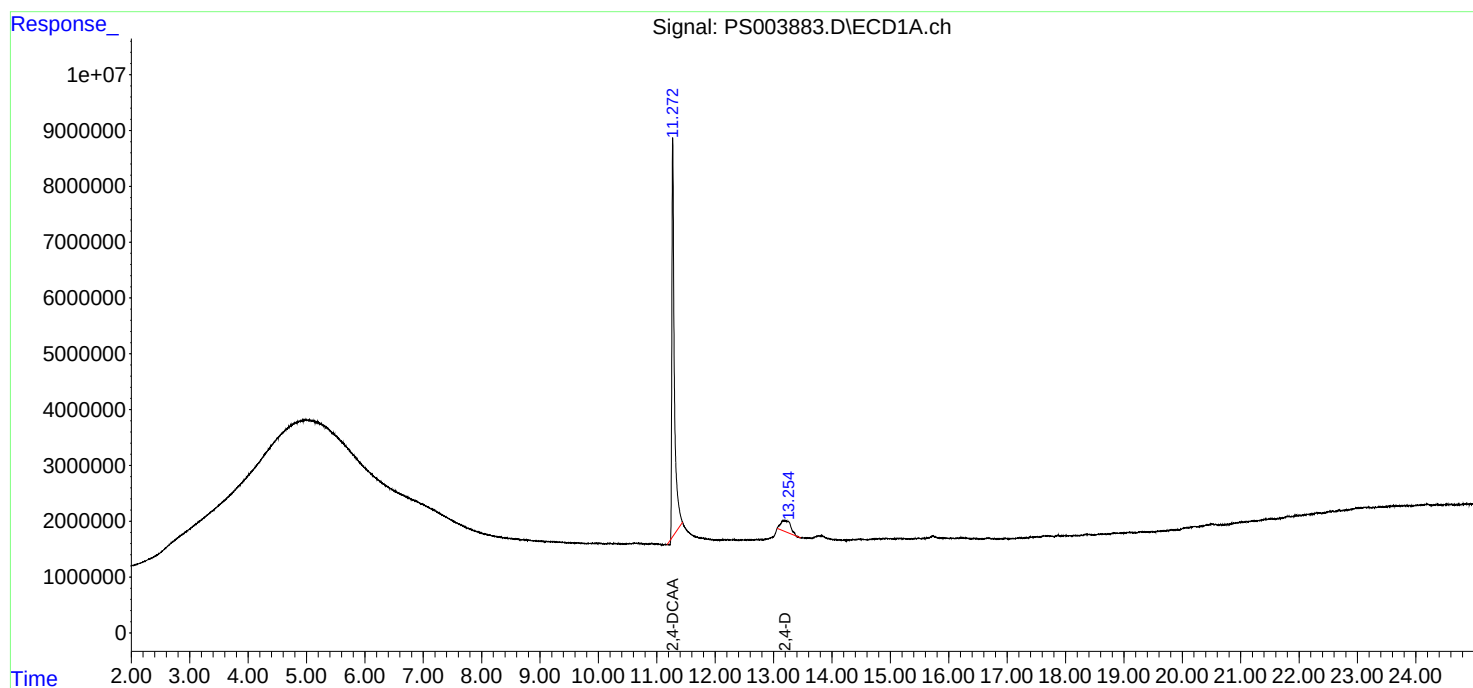


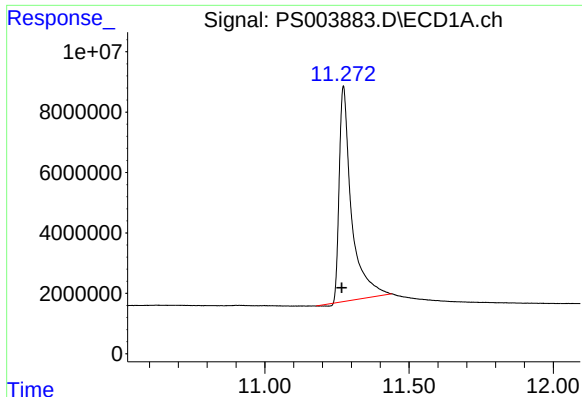

#4 2,4-DCAA


R.T.: 11.273 min
Delta R.T.: 0.006 min
Response: 211196560
Conc: 484.16 ng/ml

Instrument :
ECD_S
ClientSampleId :
MDL-Herb-S-BL-04

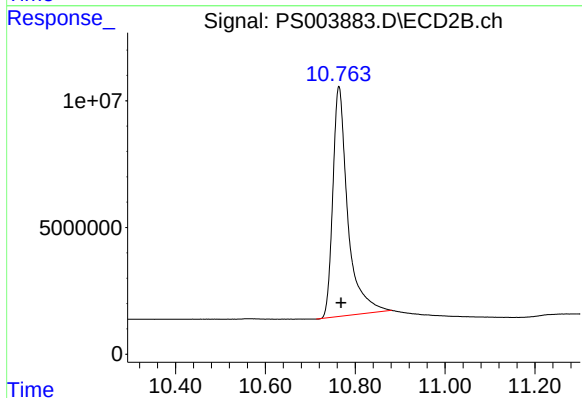


#4 2,4-DCAA

R.T.: 10.764 min
Delta R.T.: -0.005 min
Response: 209605052
Conc: 427.19 ng/ml

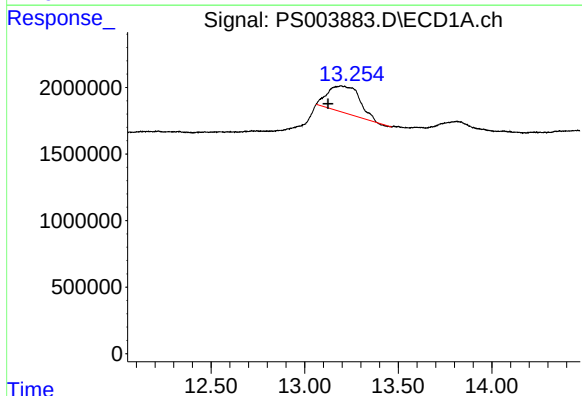

#9 2,4-D

R.T.: 13.193 min
Delta R.T.: 0.068 min
Response: 23575044
Conc: 48.48 ng/ml

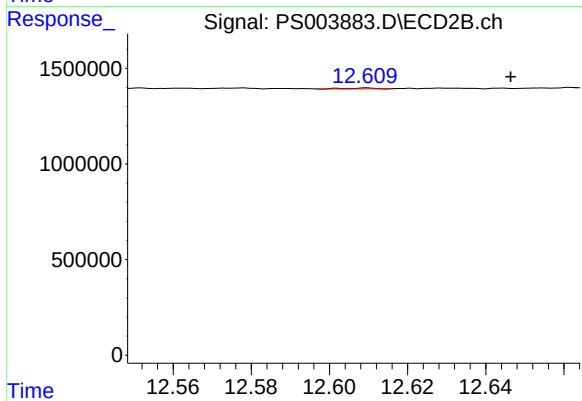

#9 2,4-D

R.T.: 12.609 min
Delta R.T.: -0.038 min
Response: 25010
Conc: N.D.