

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040120\
 Data File : PS009533.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Apr 2020 18:11
 Operator : DD\AJ
 Sample : L2072-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 MECHANIC-BUS-LIFT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 02:04:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.241	6.930	213.4E6	192.2E6	385.814	349.959
Target Compounds							
1) T	Dalapon	3.001	2.589	20361574	94818025	26.110	120.425 #
2) T	3,5-DICHL...	0.000	6.107	0	60825553	N.D.	74.788
5) T	DICAMBA	0.000	7.152	0	7890576	N.D.	3.437
6) T	MCP	0.000	7.152	0	7890576	N.D.	4.338
7) T	MCPA	7.686	7.409	146.1E6	3885461	47.971	1.440 #
8) T	DICHLORPROP	0.000	7.749	0	28184894	N.D.	50.800
10) T	Pentachlo...	0.000	8.523	0	5744544	N.D.	<MDL
12) T	2,4,5-T	9.445	9.252	44127820	6224455	17.347	2.108 #
13) T	2,4-DB	0.000	9.721	0	2617350	N.D.	6.895
14) T	DINOSEB	11.186	10.082	29065545	53916574	14.219	24.547 #
15) T	Picloram	11.012	11.046	30422296	9791630	10.024	2.405 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040120\
Data File : PS009533.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Apr 2020 18:11
Operator : DD\AJ
Sample : L2072-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
MECHANIC-BUS-LIFT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 02:04:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

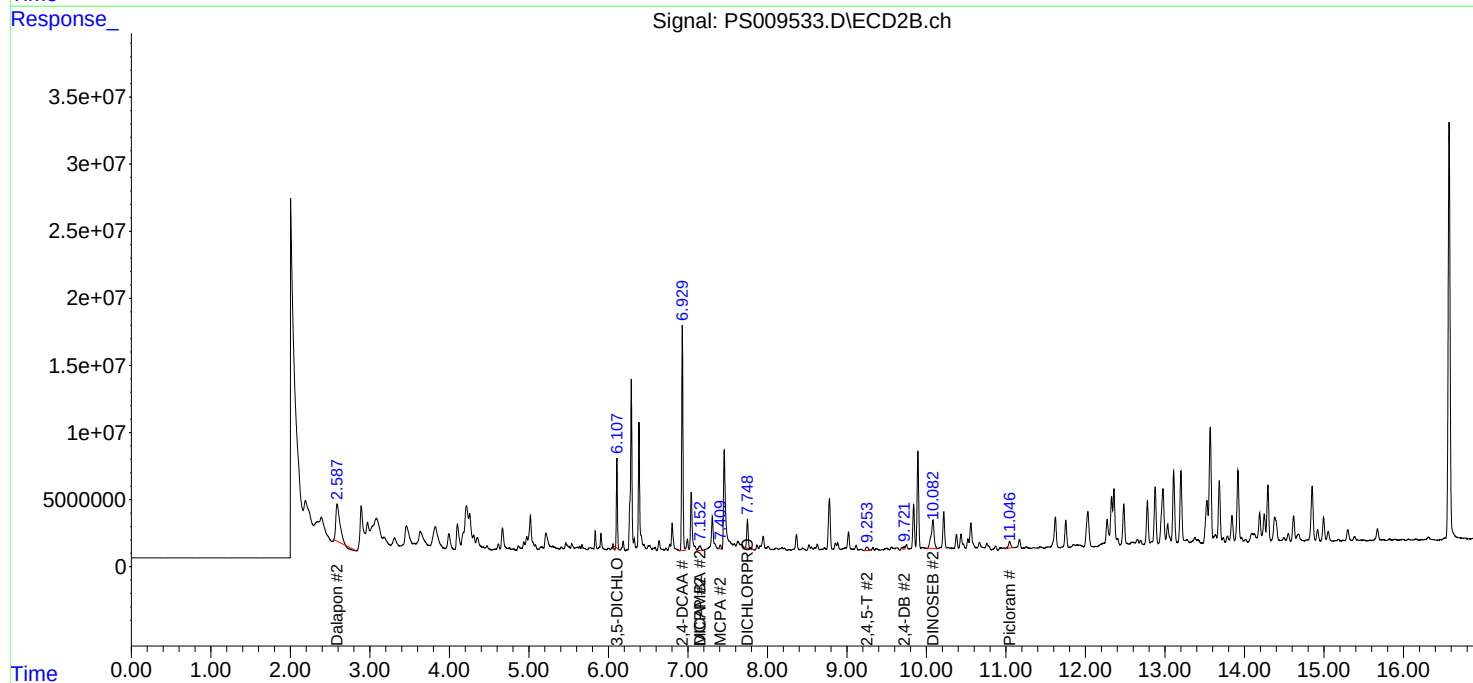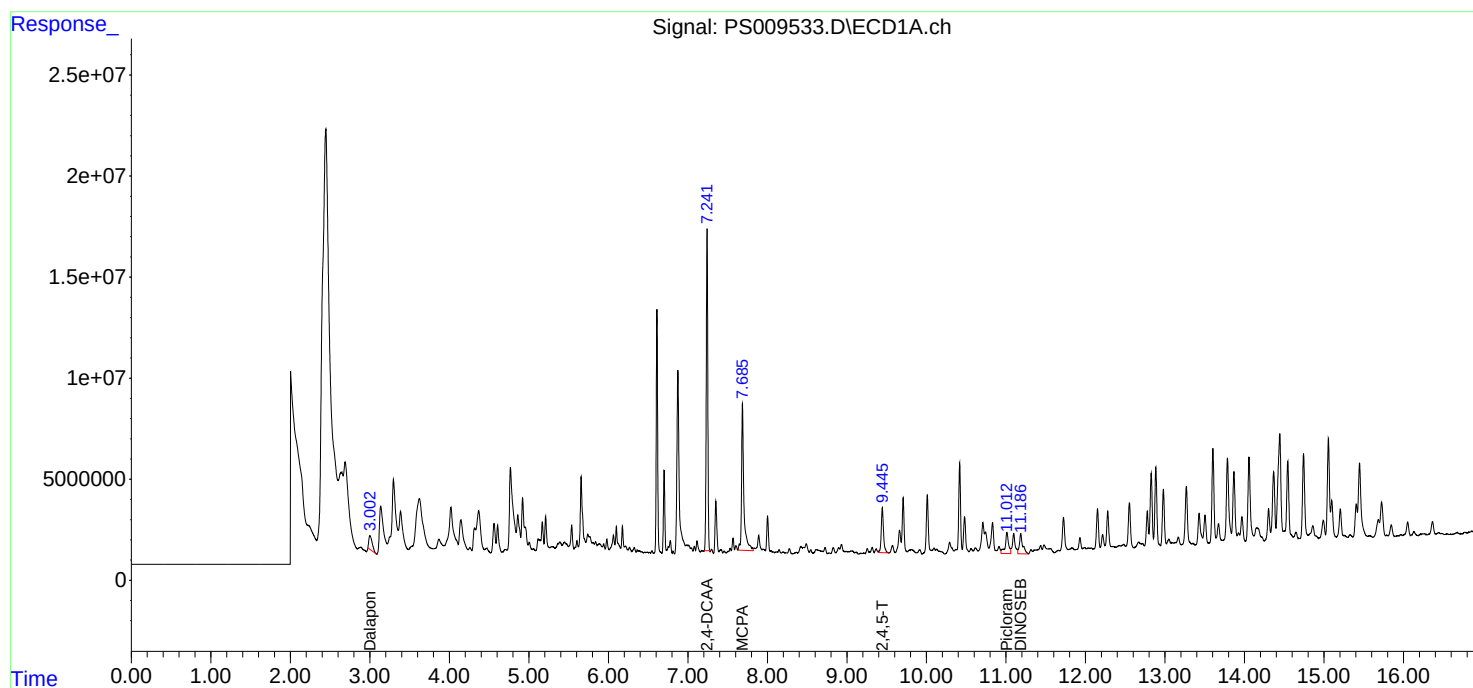


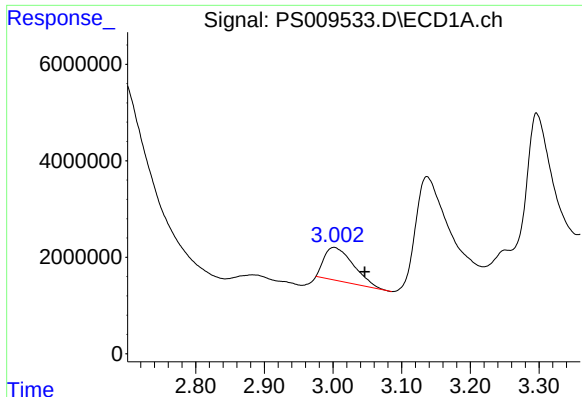

#1 Dalapon


R.T.: 3.001 min
Delta R.T.: -0.045 min
Response: 20361574
Conc: 26.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
MECHANIC-BUS-LIFT

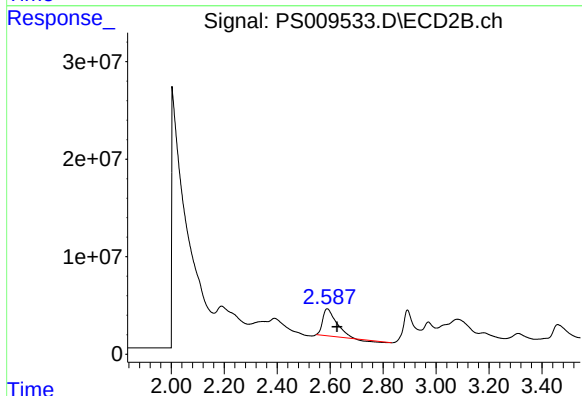


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.037 min
Response: 94818025
Conc: 120.42 ng/ml

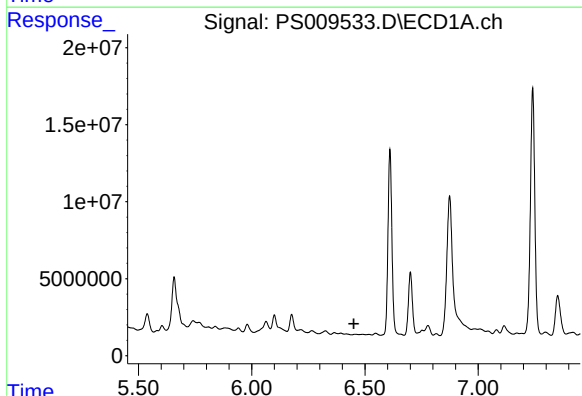


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

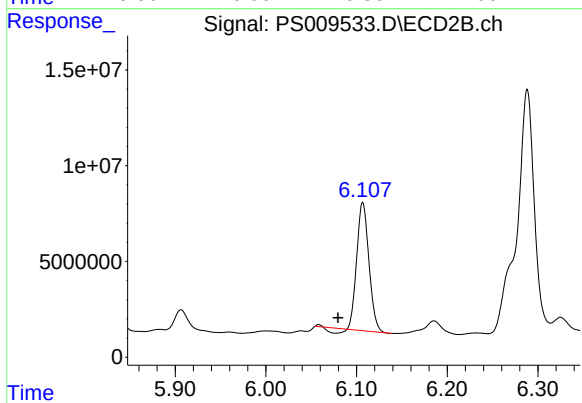

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.107 min
Delta R.T.: 0.027 min
Response: 60825553
Conc: 74.79 ng/ml

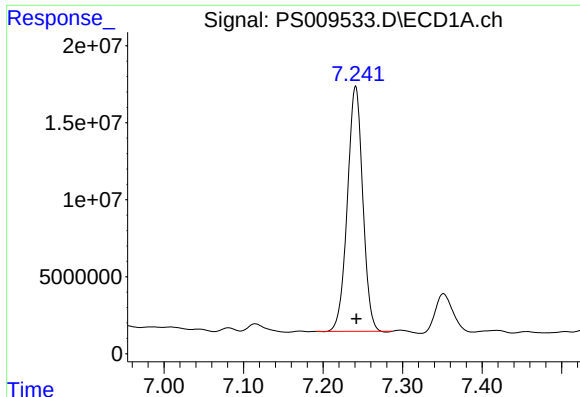

#4 2,4-DCAA


R.T.: 7.241 min
Delta R.T.: -0.001 min
Response: 213420906
Conc: 385.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
MECHANIC-BUS-LIFT

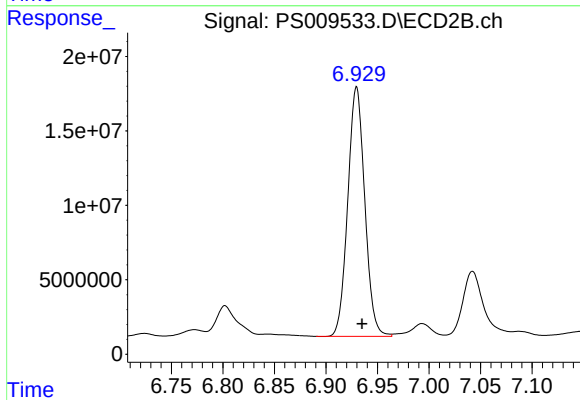


#4 2,4-DCAA

R.T.: 6.930 min
Delta R.T.: -0.005 min
Response: 192196529
Conc: 349.96 ng/ml

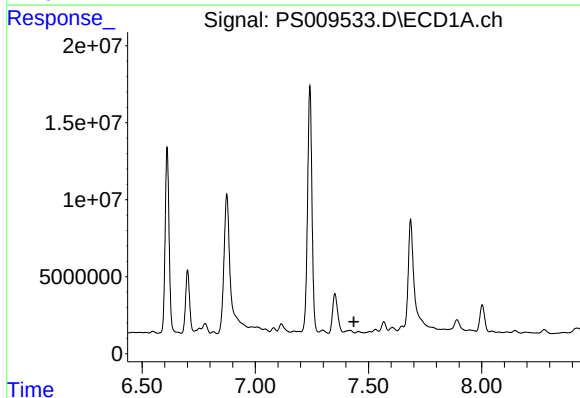


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.435 min
Response: 0
Conc: N.D.

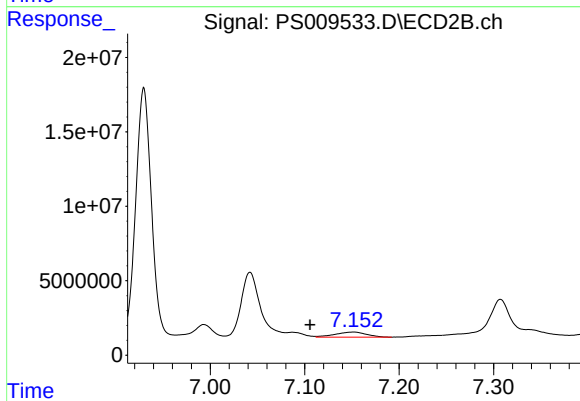

#5 DICAMBA


R.T.: 7.152 min
Delta R.T.: 0.046 min
Response: 7890576
Conc: 3.44 ng/ml

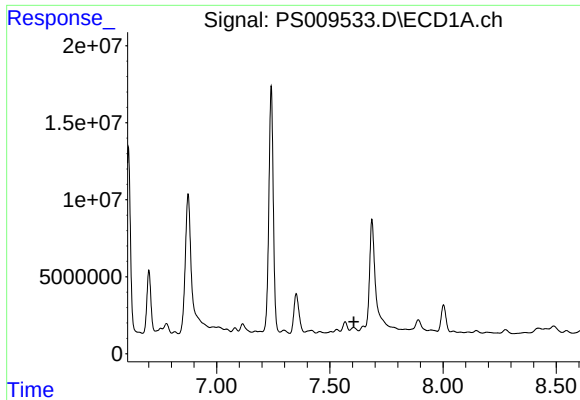

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 7.606 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
MECHANIC-BUS-LIFT

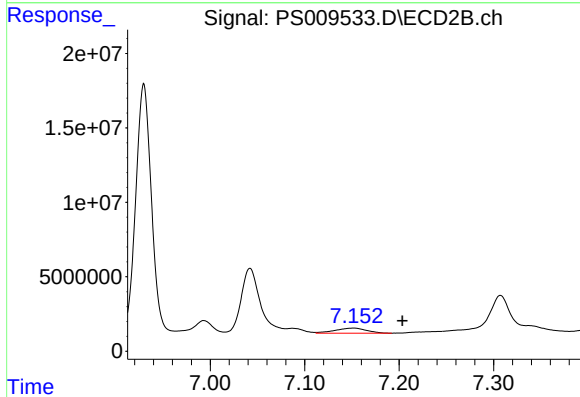


#6 MCPP

R.T.: 7.152 min
Delta R.T.: -0.052 min
Response: 7890576
Conc: 4.34 ug/ml

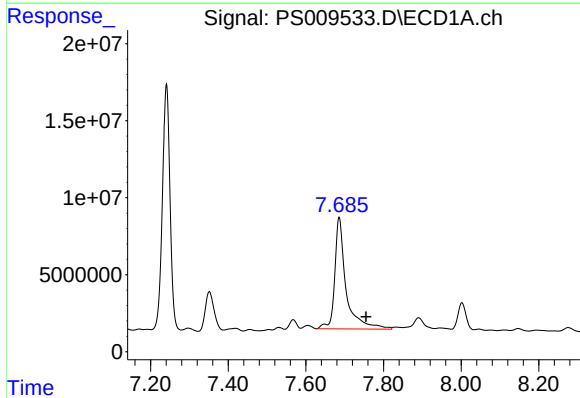


#7 MCPA

R.T.: 7.686 min
Delta R.T.: -0.070 min
Response: 146105737
Conc: 47.97 ug/ml

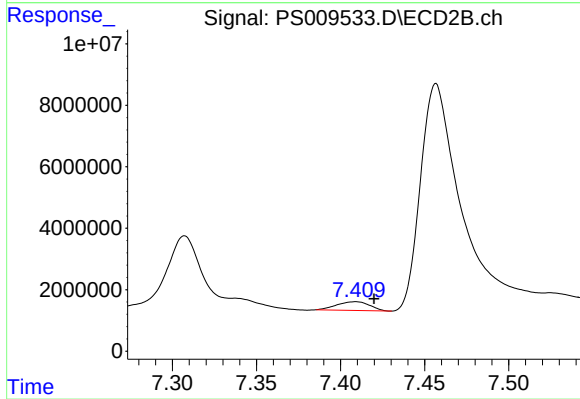

#7 MCPA


R.T.: 7.409 min
Delta R.T.: -0.011 min
Response: 3885461
Conc: 1.44 ug/ml

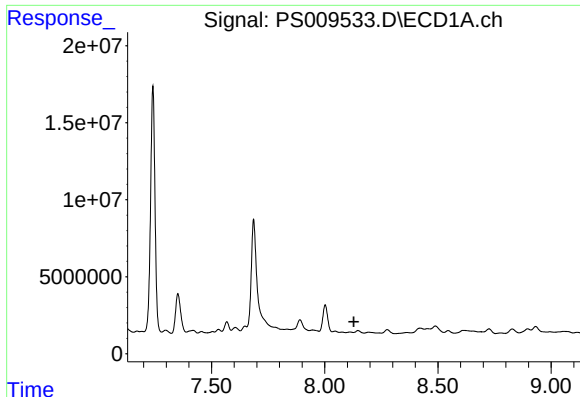

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
MECHANIC-BUS-LIFT

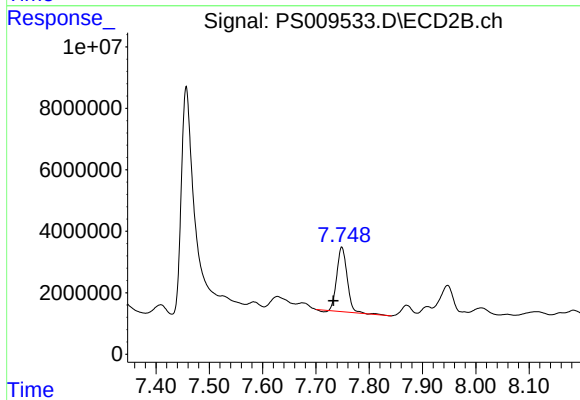


#8 DICHLORPROP

R.T.: 7.749 min
Delta R.T.: 0.016 min
Response: 28184894
Conc: 50.80 ng/ml

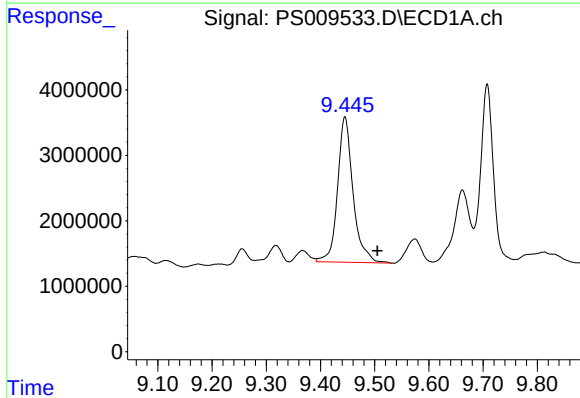


#12 2,4,5-T

R.T.: 9.445 min
Delta R.T.: -0.060 min
Response: 44127820
Conc: 17.35 ng/ml

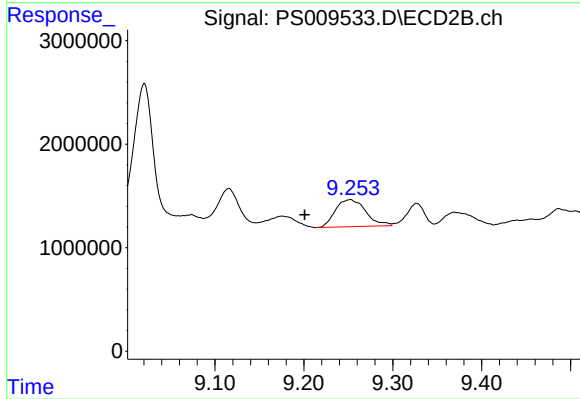

#12 2,4,5-T


R.T.: 9.252 min
Delta R.T.: 0.051 min
Response: 6224455
Conc: 2.11 ng/ml

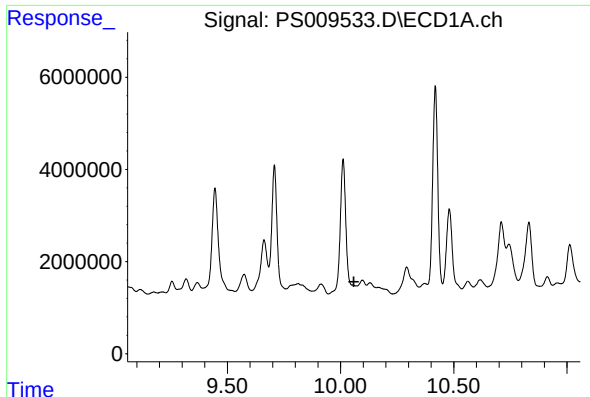

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.059 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
MECHANIC-BUS-LIFT

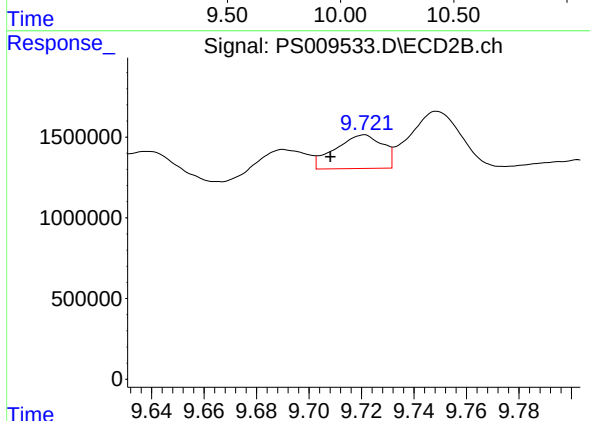


#13 2,4-DB

R.T.: 9.721 min
Delta R.T.: 0.012 min
Response: 2617350
Conc: 6.89 ng/ml

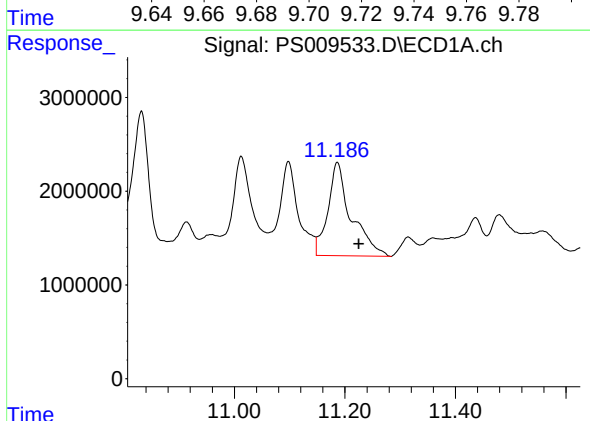


#14 DINOSEB

R.T.: 11.186 min
Delta R.T.: -0.039 min
Response: 29065545
Conc: 14.22 ng/ml

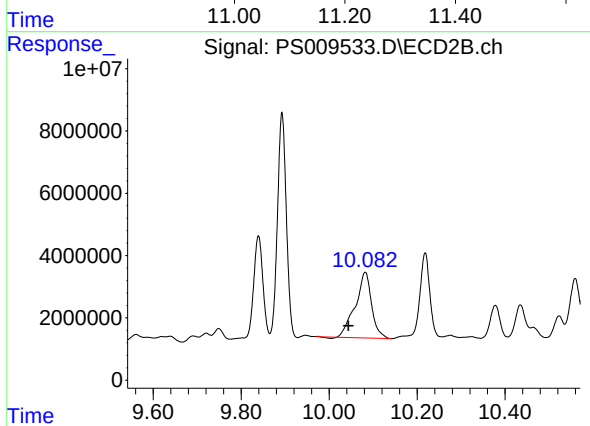

#14 DINOSEB

R.T.: 10.082 min
Delta R.T.: 0.038 min
Response: 53916574
Conc: 24.55 ng/ml

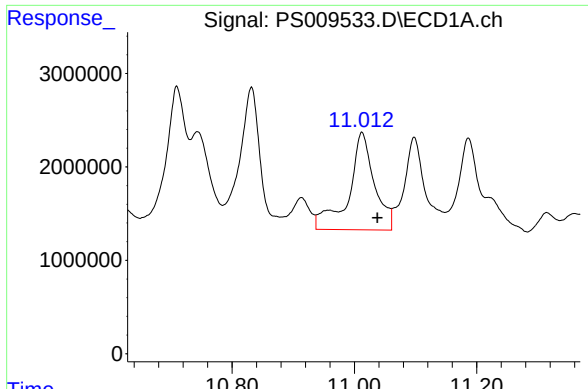

#15 Picloram


R.T.: 11.012 min

Delta R.T.: -0.025 min

Response: 30422296

Conc: 10.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
MECHANIC-BUS-LIFT

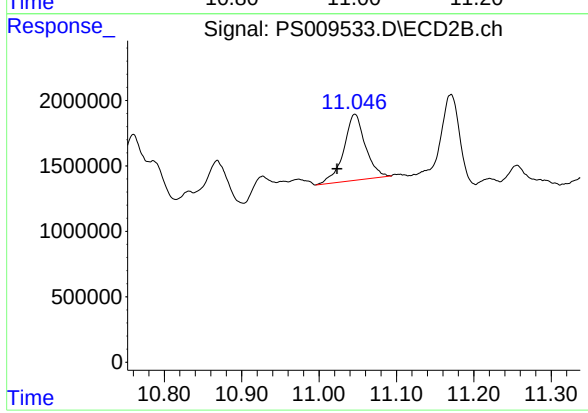

#15 Picloram

R.T.: 11.046 min

Delta R.T.: 0.023 min

Response: 9791630

Conc: 2.40 ng/ml