

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040120\
 Data File : PS009536.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Apr 2020 19:20
 Operator : DD\AJ
 Sample : L1758-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PL-03-033020

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 02:05:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.240	6.930	327.0E6	258.0E6	591.094	469.761
Target Compounds							
1) T	Dalapon	3.002	2.587	19819788	59101697	25.415	75.063 #
2) T	3,5-DICHL...	0.000	6.107	0	23067081	N.D.	28.362
7) T	MCPA	7.688	7.470	37811744	15514066	12.415	5.749 #
8) T	DICHLORPROP	0.000	7.749	0	11232349	N.D.	20.245
9) T	2,4-D	8.291	0.000	11411095	0	21.644	N.D. #
12) T	2,4,5-T	9.445	9.261	34959572	4513493	13.743	1.529 #
13) T	2,4-DB	0.000	9.641	0	2963102	N.D.	7.806
14) T	DINOSEB	11.186	10.082	27587544	98390878	13.496	44.795 #
15) T	Picloram	11.012	0.000	33530513	0	11.048	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040120\
Data File : PS009536.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Apr 2020 19:20
Operator : DD\AJ
Sample : L1758-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
PL-03-033020

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 02:05:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

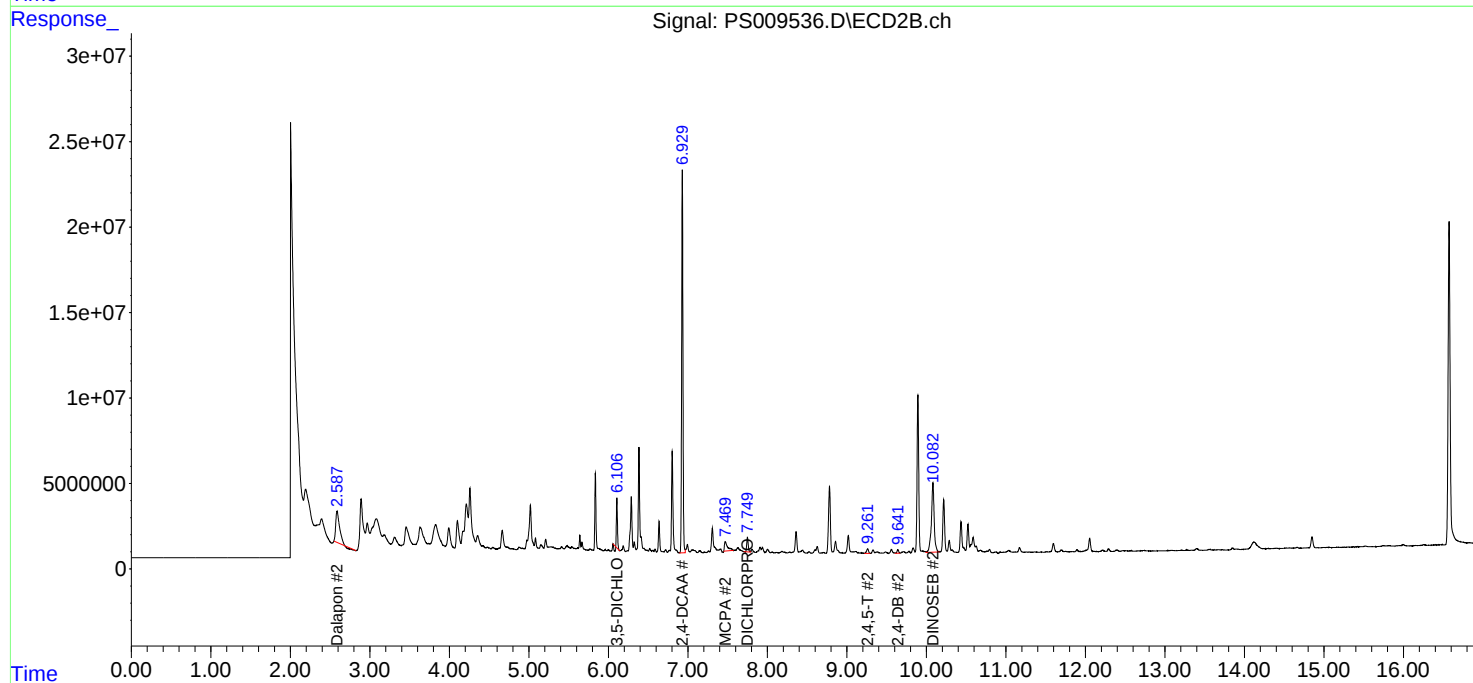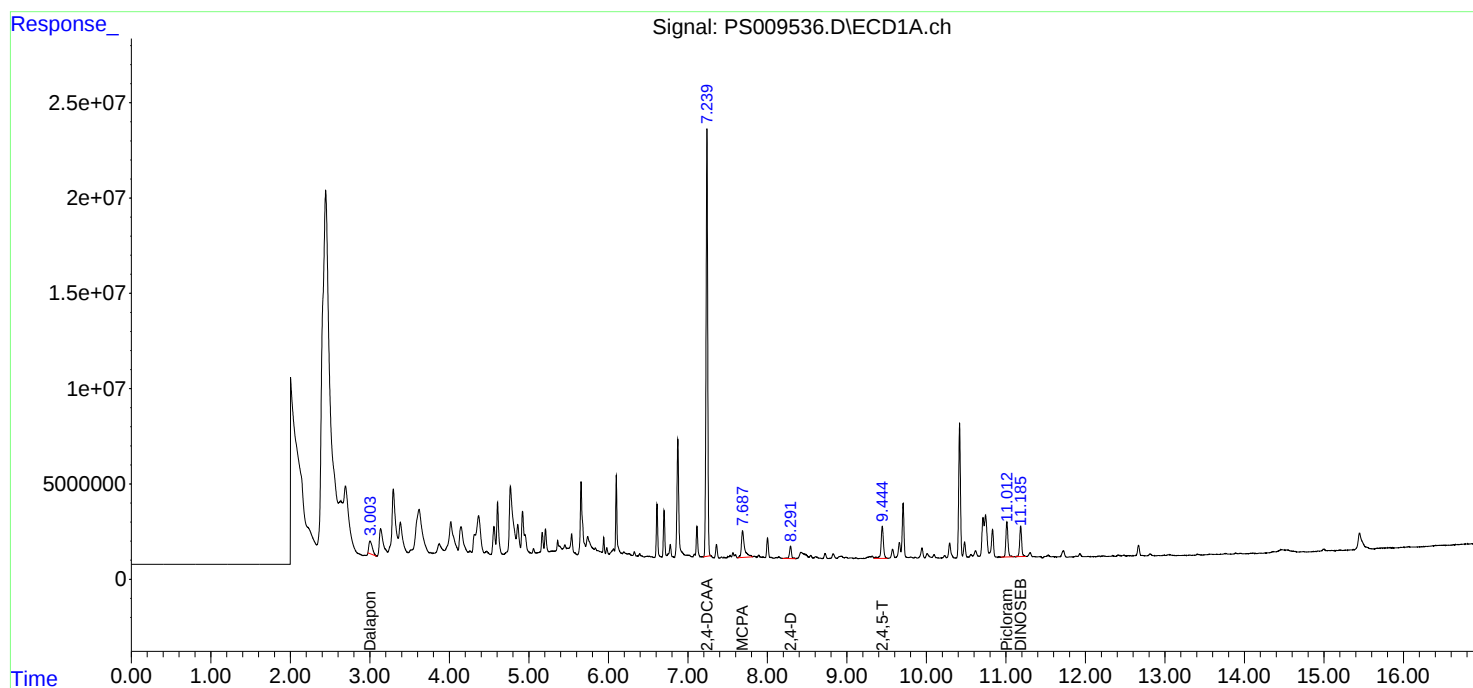


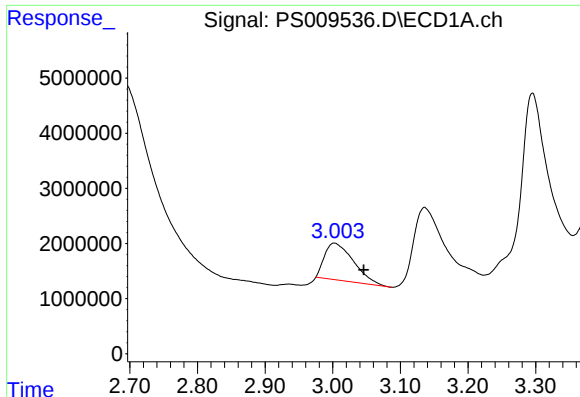

#1 Dalapon


R.T.: 3.002 min
Delta R.T.: -0.044 min
Response: 19819788
Conc: 25.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
PL-03-033020

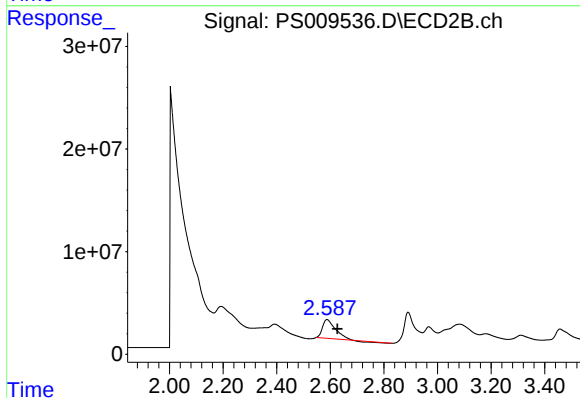


#1 Dalapon

R.T.: 2.587 min
Delta R.T.: -0.039 min
Response: 59101697
Conc: 75.06 ng/ml

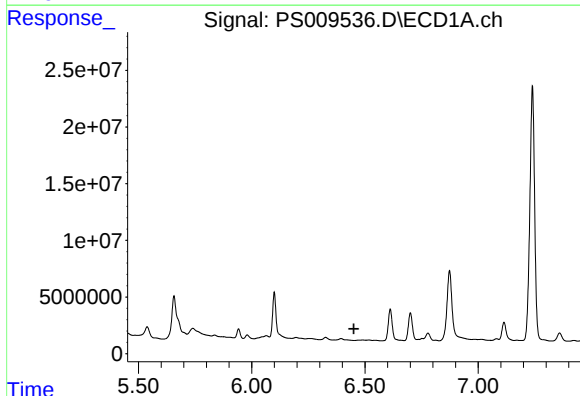


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

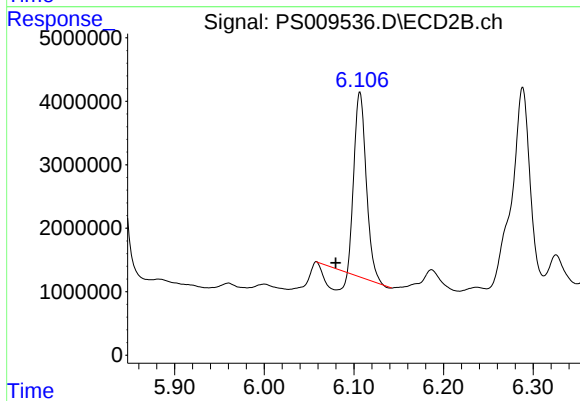

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.107 min
Delta R.T.: 0.027 min
Response: 23067081
Conc: 28.36 ng/ml

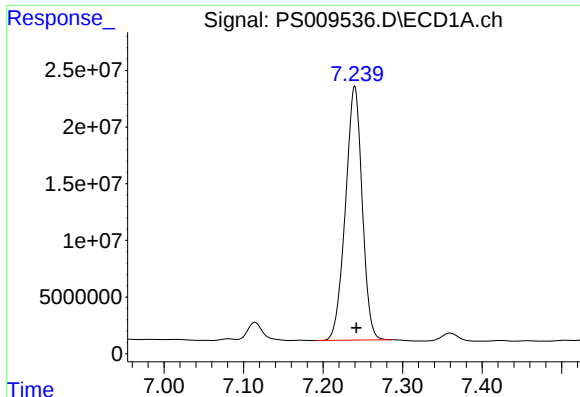

#4 2,4-DCAA


R.T.: 7.240 min
Delta R.T.: -0.002 min
Response: 326975765
Conc: 591.09 ng/ml

Instrument :
ECD_S
ClientSampleId :
PL-03-033020

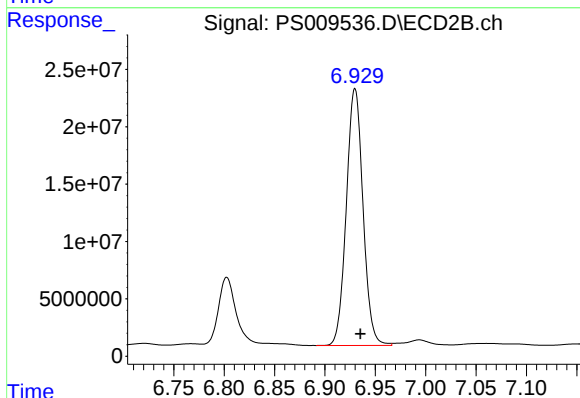


#4 2,4-DCAA

R.T.: 6.930 min
Delta R.T.: -0.005 min
Response: 257991562
Conc: 469.76 ng/ml

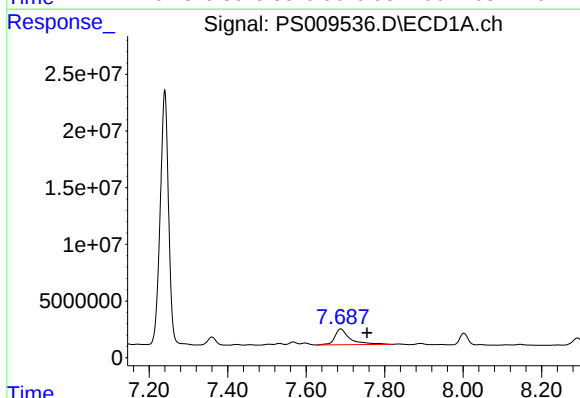


#7 MCPA

R.T.: 7.688 min
Delta R.T.: -0.068 min
Response: 37811744
Conc: 12.41 ug/ml

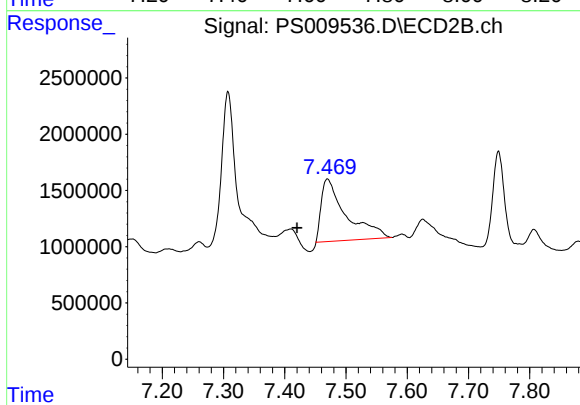

#7 MCPA


R.T.: 7.470 min
Delta R.T.: 0.050 min
Response: 15514066
Conc: 5.75 ug/ml

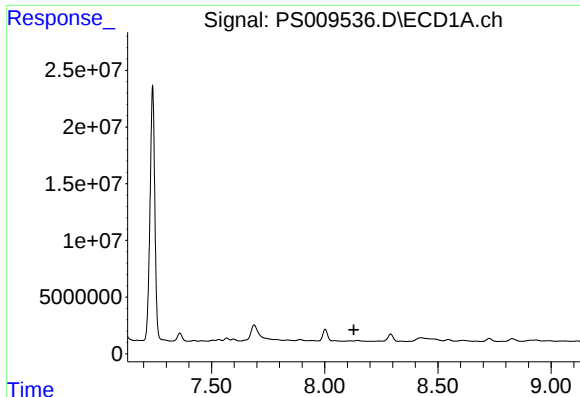

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PL-03-033020

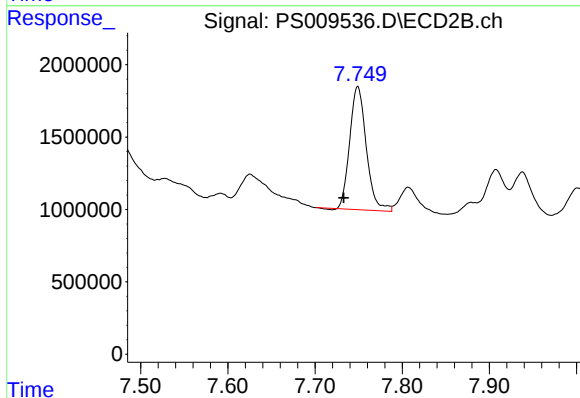


#8 DICHLORPROP

R.T.: 7.749 min
Delta R.T.: 0.016 min
Response: 11232349
Conc: 20.24 ng/ml

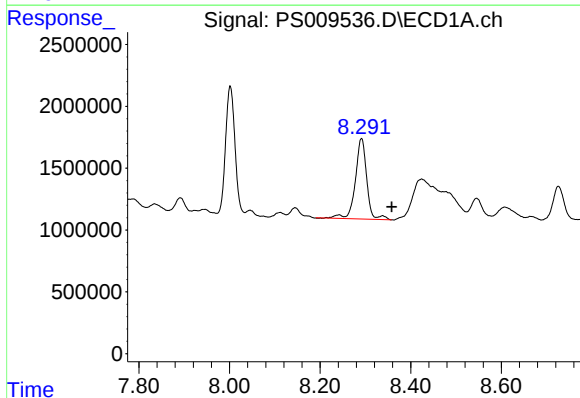


#9 2,4-D

R.T.: 8.291 min
Delta R.T.: -0.067 min
Response: 11411095
Conc: 21.64 ng/ml

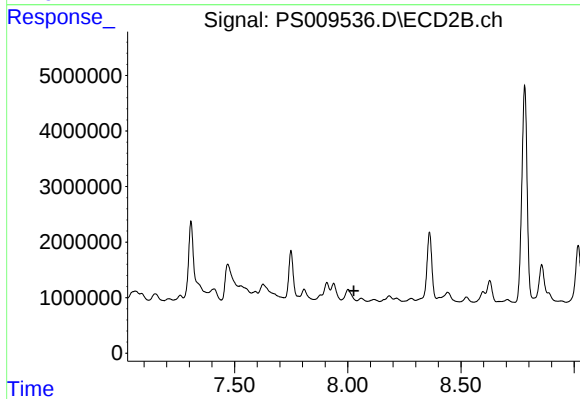

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.027 min
Response: 0
Conc: N.D.

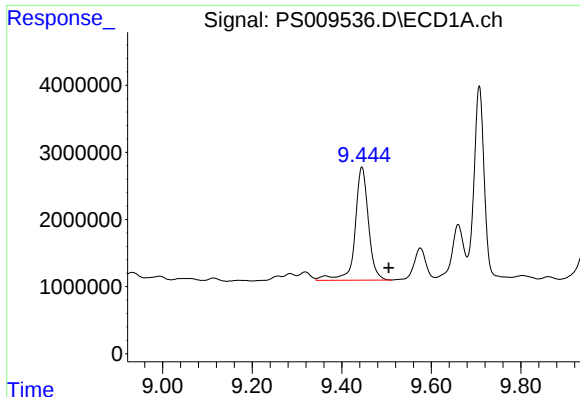

#12 2,4,5-T


R.T.: 9.445 min
Delta R.T.: -0.060 min
Response: 34959572
Conc: 13.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
PL-03-033020

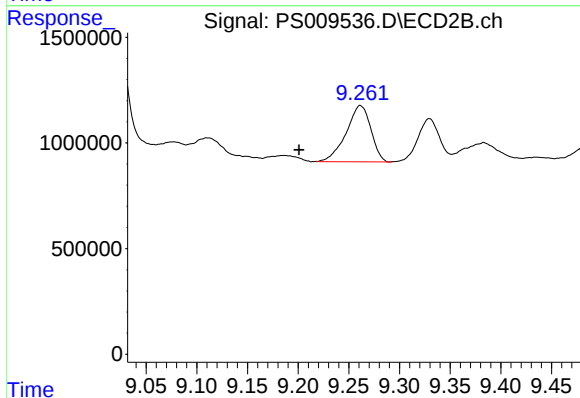


#12 2,4,5-T

R.T.: 9.261 min
Delta R.T.: 0.061 min
Response: 4513493
Conc: 1.53 ng/ml

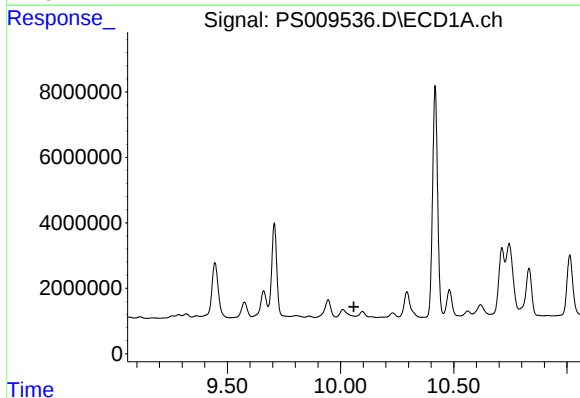


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.059 min
Response: 0
Conc: N.D.

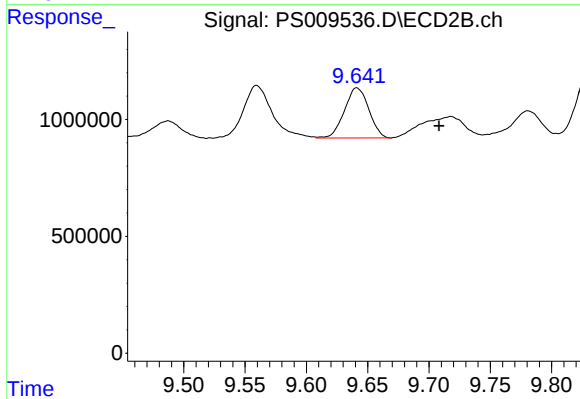

#13 2,4-DB


R.T.: 9.641 min
Delta R.T.: -0.067 min
Response: 2963102
Conc: 7.81 ng/ml

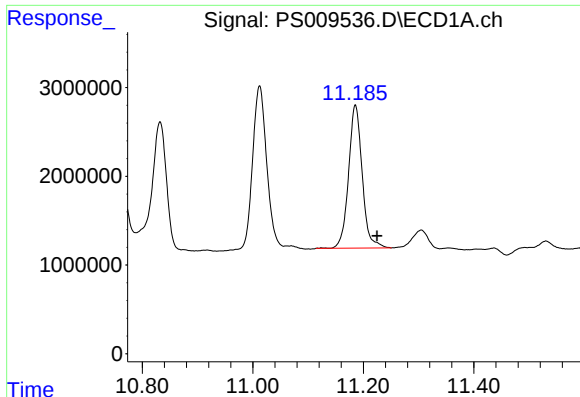

#14 DINOSEB


R.T.: 11.186 min
Delta R.T.: -0.039 min
Response: 27587544
Conc: 13.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
PL-03-033020

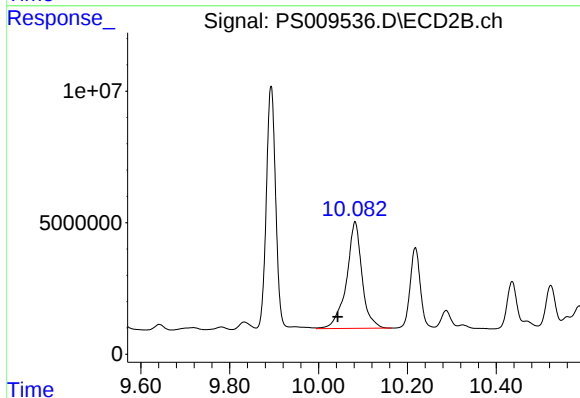


#14 DINOSEB

R.T.: 10.082 min
Delta R.T.: 0.039 min
Response: 98390878
Conc: 44.79 ng/ml

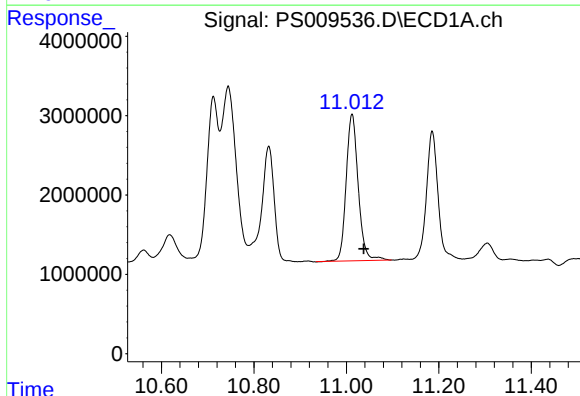

#15 Picloram

R.T.: 11.012 min
Delta R.T.: -0.025 min
Response: 33530513
Conc: 11.05 ng/ml

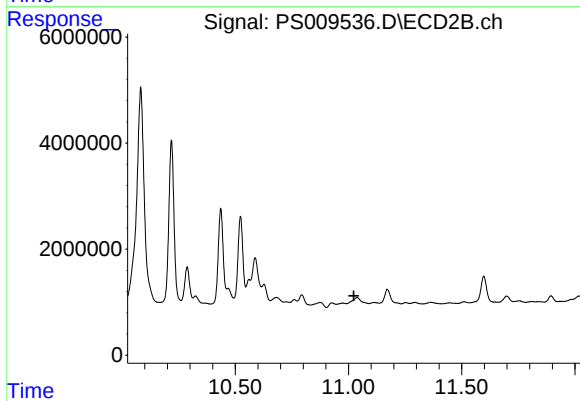

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.023 min
Response: 0
Conc: N.D.