

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040120\
 Data File : PS009538.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Apr 2020 20:06
 Operator : DD\AJ
 Sample : L1752-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HD-02-033020

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 02:05:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.241	6.930	384.2E6	372.3E6	694.524	677.892
Target Compounds							
1) T	Dalapon	3.004	2.589	21893355	85818457	28.074	108.995 #
2) T	3,5-DICHL...	0.000	6.107	0	76659798	N.D.	94.257
7) T	MCPA	7.686	0.000	17040543	0	5.595	N.D. #
8) T	DICHLORPROP	0.000	7.749	0	9650730	N.D.	17.394
12) T	2,4,5-T	9.444	9.262	50447236	5002657	19.831	1.695 #
13) T	2,4-DB	0.000	9.642	0	3487710	N.D.	9.187
14) T	DINOSEB	11.186	10.081	23635757	103.1E6	11.563	46.919 #
15) T	Picloram	11.013	0.000	40039455	0	13.193	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040120\
Data File : PS009538.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Apr 2020 20:06
Operator : DD\AJ
Sample : L1752-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
HD-02-033020

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 02:05:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

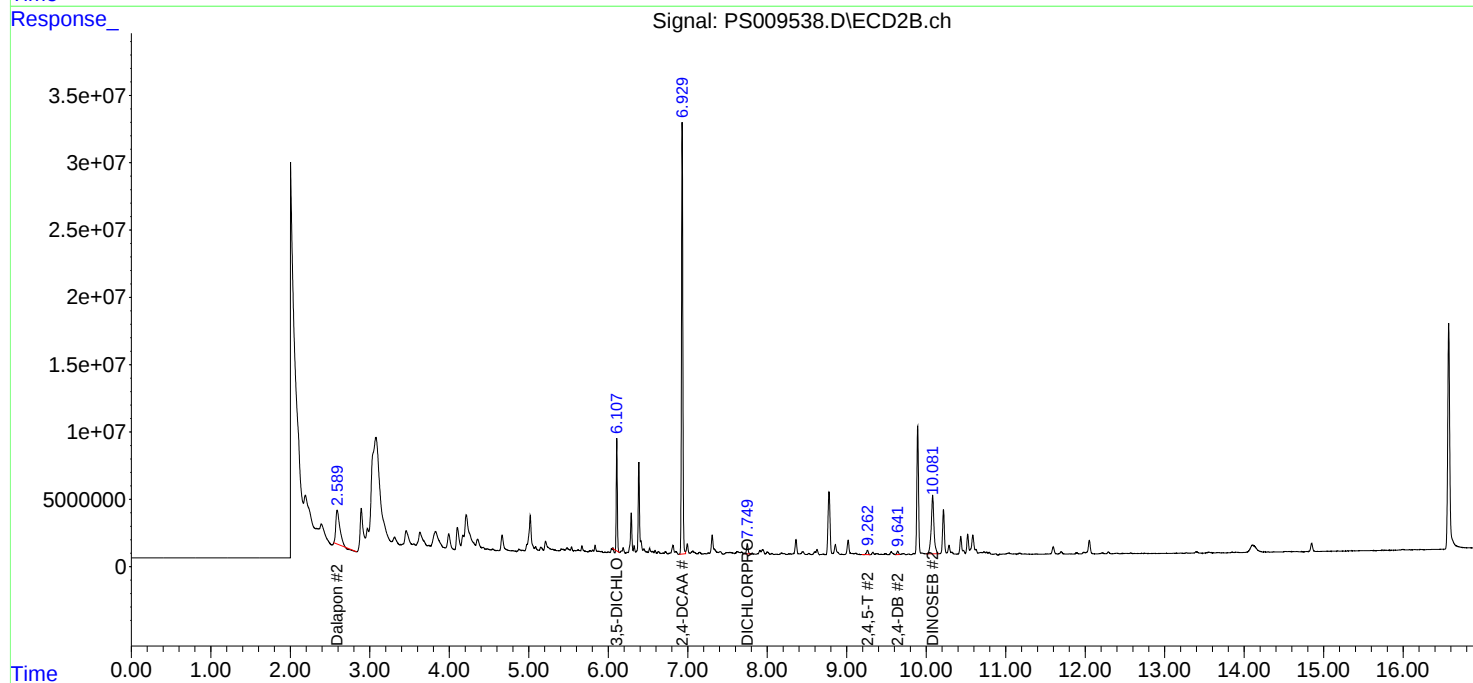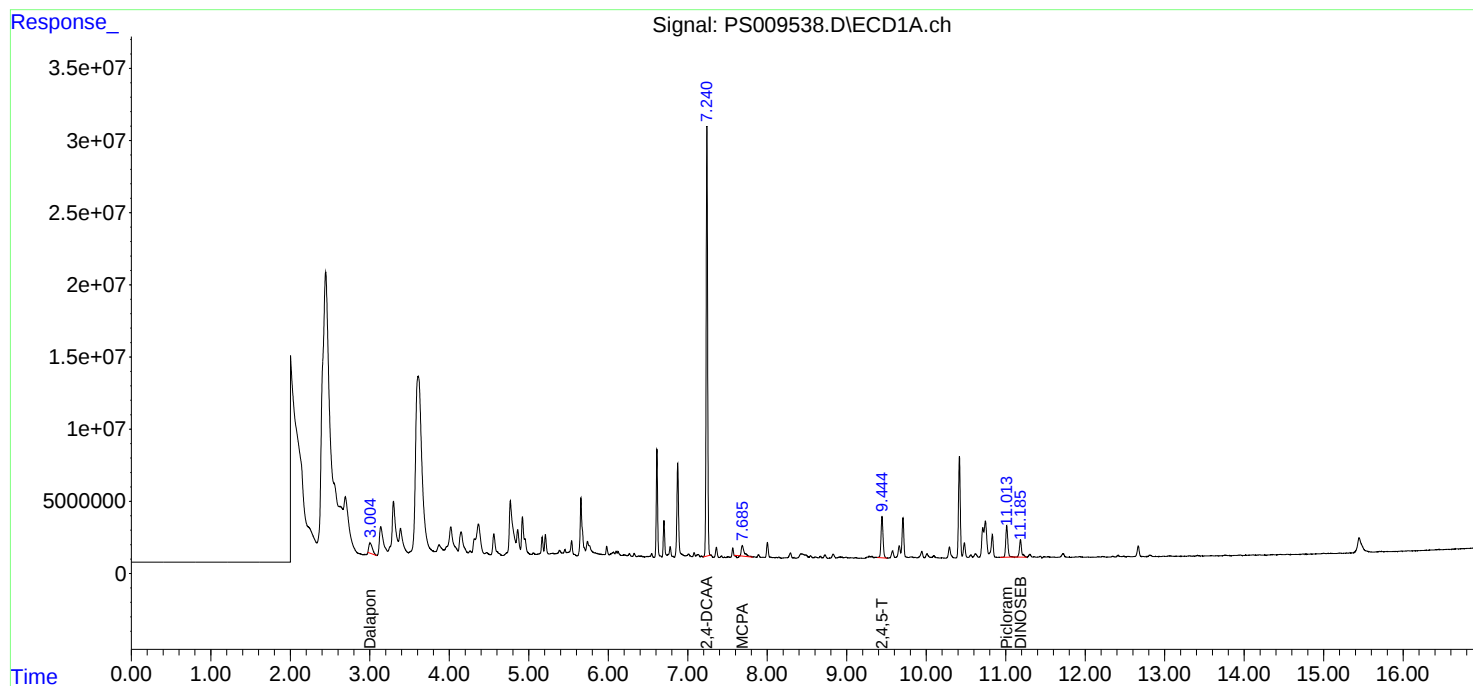


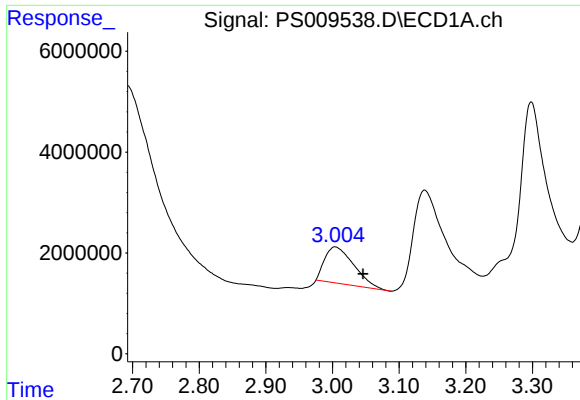

#1 Dalapon


R.T.: 3.004 min
Delta R.T.: -0.042 min
Response: 21893355
Conc: 28.07 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-02-033020

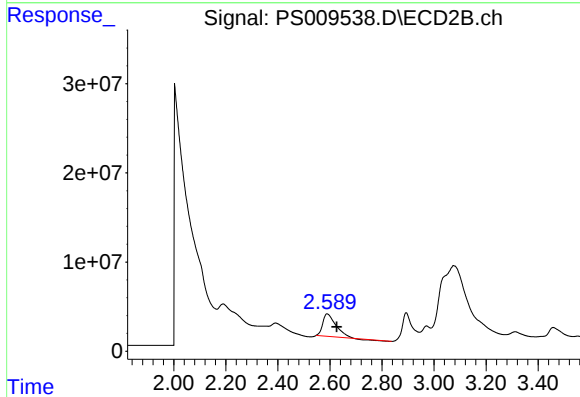


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.037 min
Response: 85818457
Conc: 108.99 ng/ml

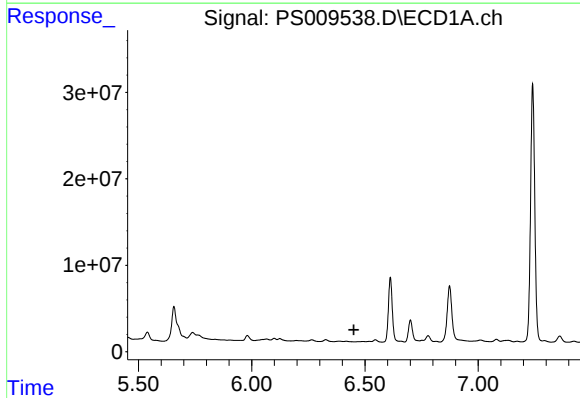


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

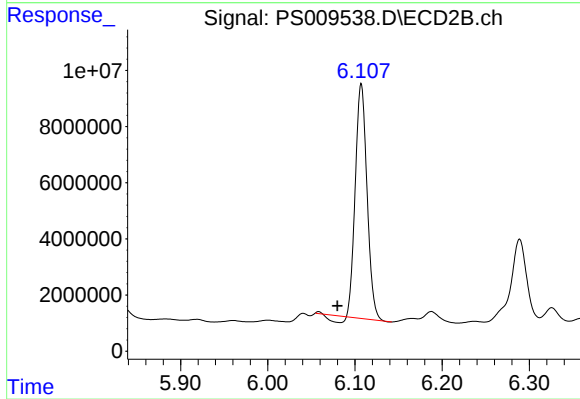

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.107 min
Delta R.T.: 0.028 min
Response: 76659798
Conc: 94.26 ng/ml

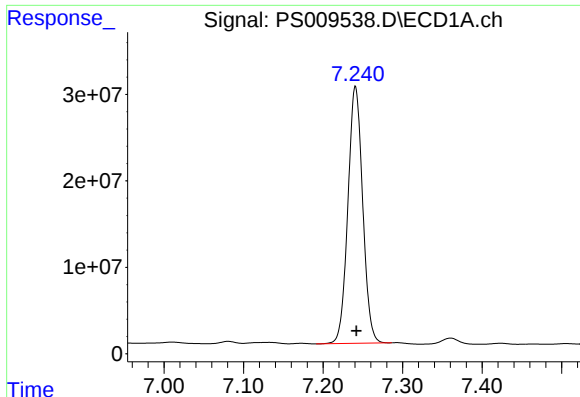

#4 2,4-DCAA


R.T.: 7.241 min
Delta R.T.: -0.001 min
Response: 384189877
Conc: 694.52 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-02-033020

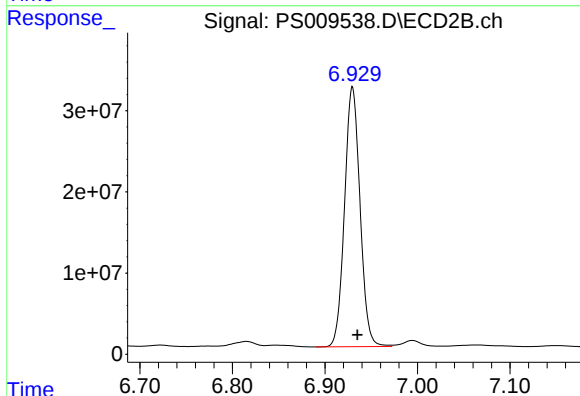


#4 2,4-DCAA

R.T.: 6.930 min
Delta R.T.: -0.005 min
Response: 372296611
Conc: 677.89 ng/ml

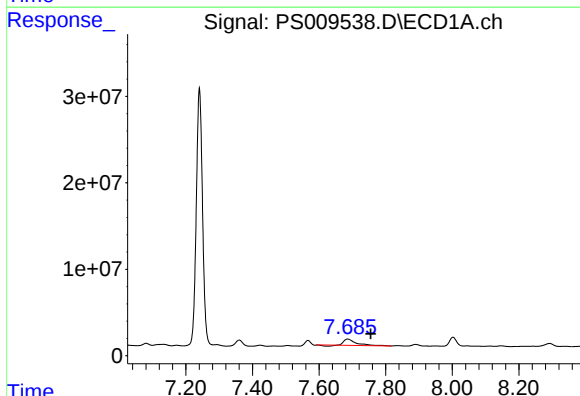


#7 MCPA

R.T.: 7.686 min
Delta R.T.: -0.070 min
Response: 17040543
Conc: 5.59 ug/ml

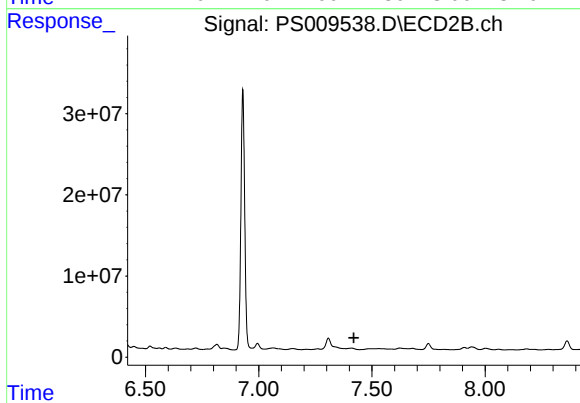

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.420 min
Response: 0
Conc: N.D.

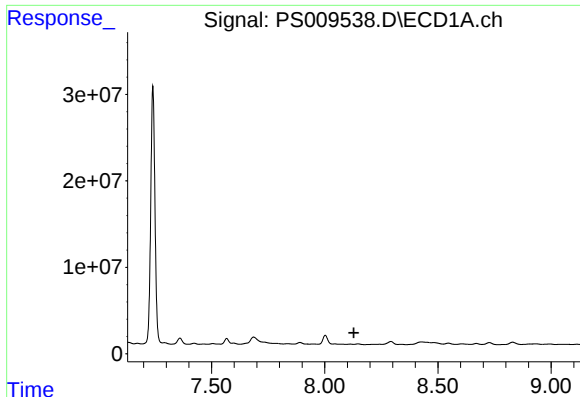

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HD-02-033020

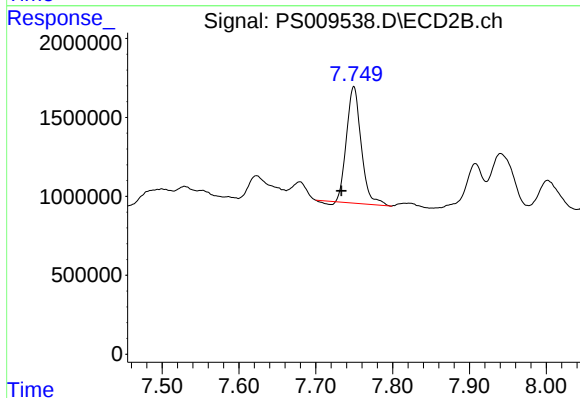


#8 DICHLORPROP

R.T.: 7.749 min
Delta R.T.: 0.016 min
Response: 9650730
Conc: 17.39 ng/ml

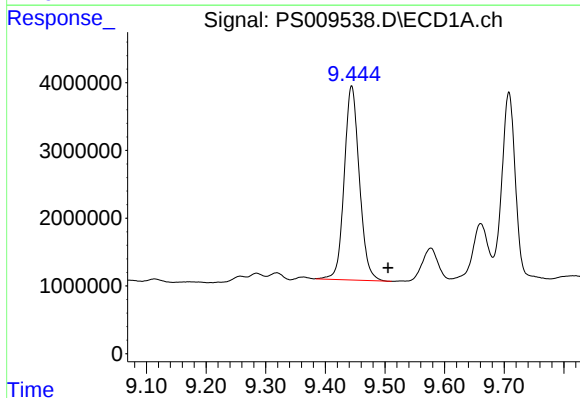


#12 2,4,5-T

R.T.: 9.444 min
Delta R.T.: -0.061 min
Response: 50447236
Conc: 19.83 ng/ml

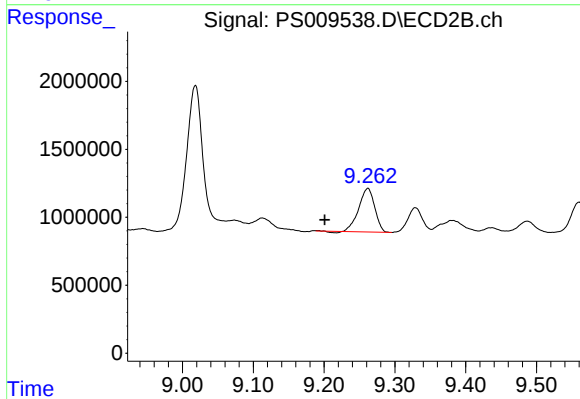

#12 2,4,5-T


R.T.: 9.262 min
Delta R.T.: 0.061 min
Response: 5002657
Conc: 1.69 ng/ml

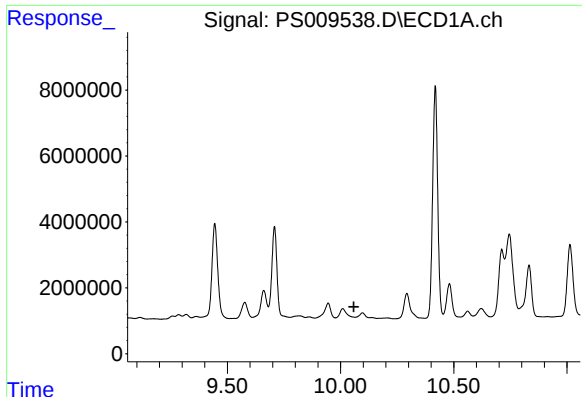

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.059 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HD-02-033020

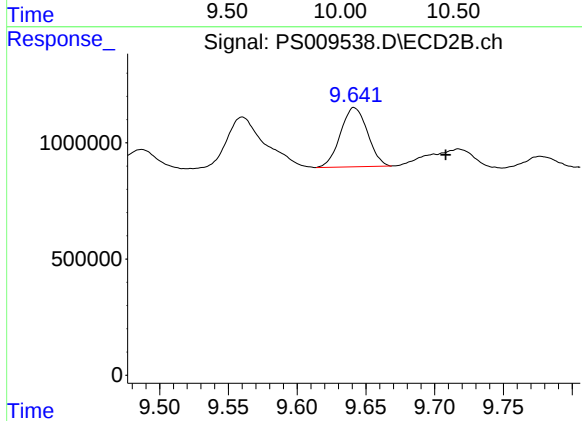


#13 2,4-DB

R.T.: 9.642 min
Delta R.T.: -0.067 min
Response: 3487710
Conc: 9.19 ng/ml

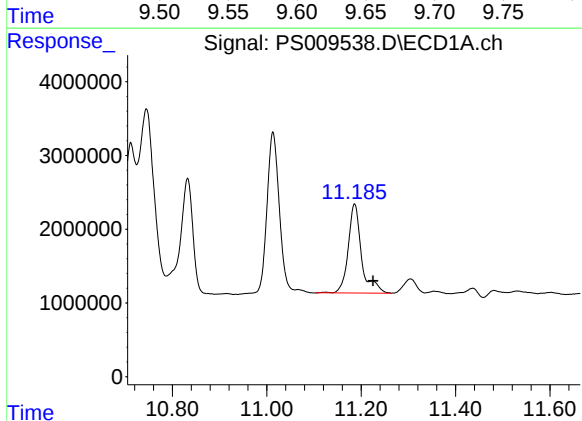


#14 DINOSEB

R.T.: 11.186 min
Delta R.T.: -0.039 min
Response: 23635757
Conc: 11.56 ng/ml

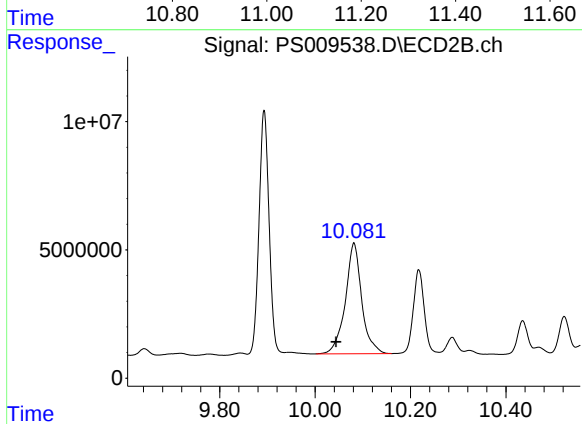

#14 DINOSEB


R.T.: 10.081 min
Delta R.T.: 0.038 min
Response: 103056807
Conc: 46.92 ng/ml

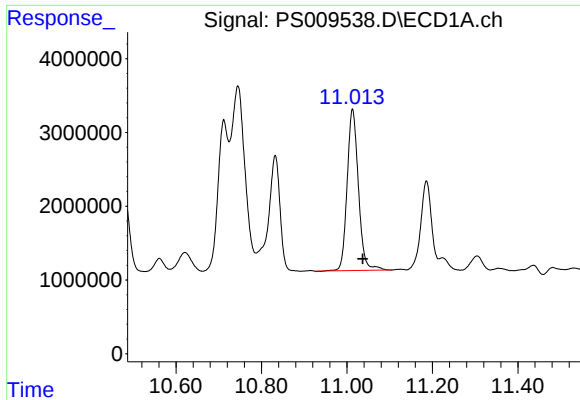

#15 Picloram

R.T.: 11.013 min
Delta R.T.: -0.024 min
Response: 40039455
Conc: 13.19 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-02-033020

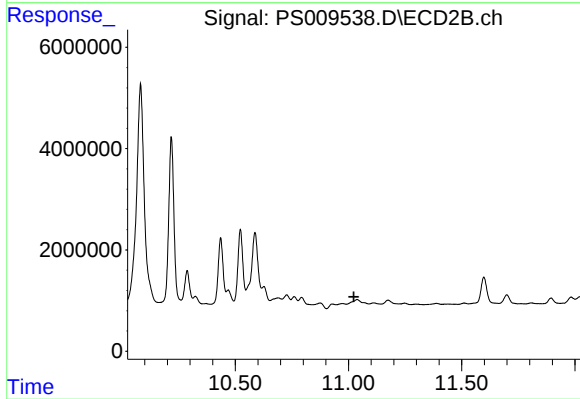

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.023 min
Response: 0
Conc: N.D.