

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040122\
 Data File : PS018857.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Apr 2022 09:15
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 22:49:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 31 16:06:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.480f	0.000	2787345	0	<MDL	N.D. #
3) T	4-Nitroph...	7.021	0.000	1651481	0	1.447	N.D. #
11) T	2,4,5-TP ...	9.222	8.642	4131278	6097253	<MDL	1.334 #
12) T	2,4,5-T	9.506	0.000	4064121	0	<MDL	N.D. #
13) T	2,4-DB	0.000	9.497f	0	50219306	N.D.	88.170
15) T	Picloram	11.012	10.898	30859364	25613952	1.103	4.530 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040122\
Data File : PS018857.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Apr 2022 09:15
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 22:49:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
Quant Title : 8080.M
QLast Update : Thu Mar 31 16:06:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

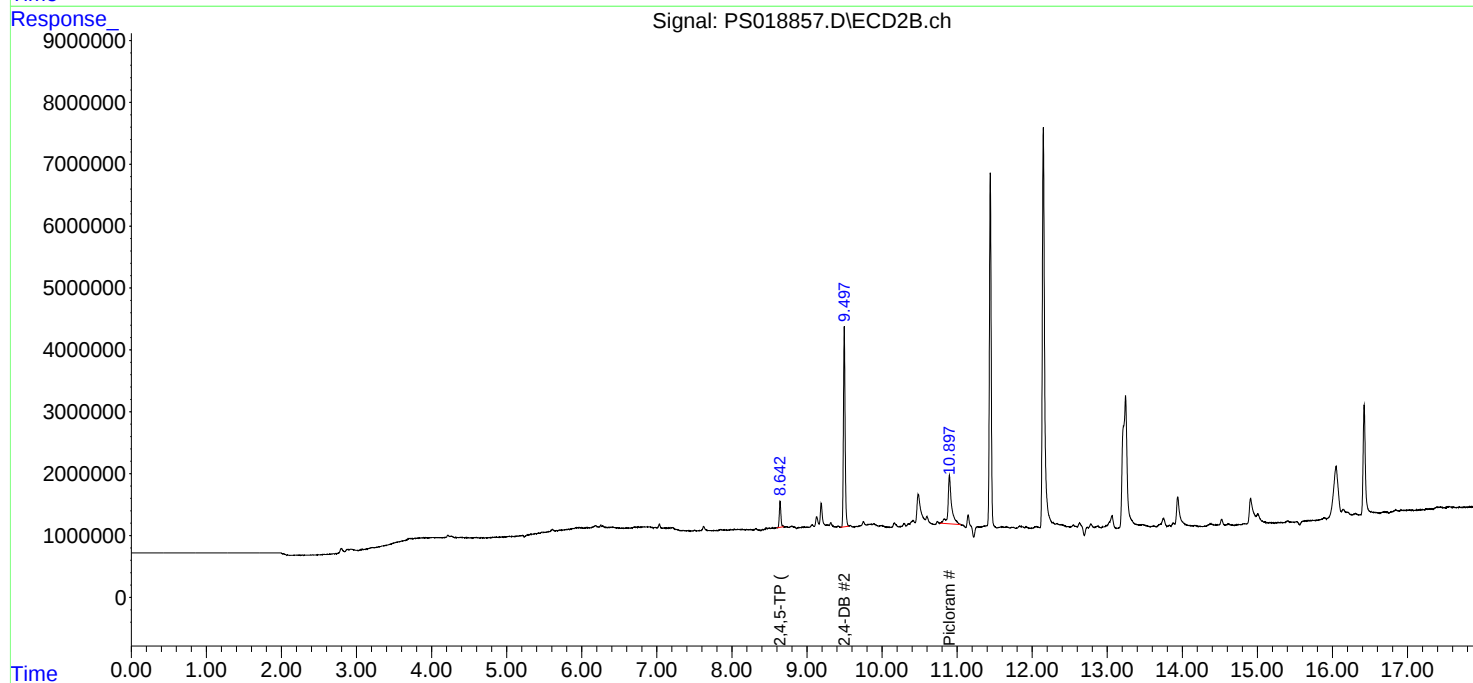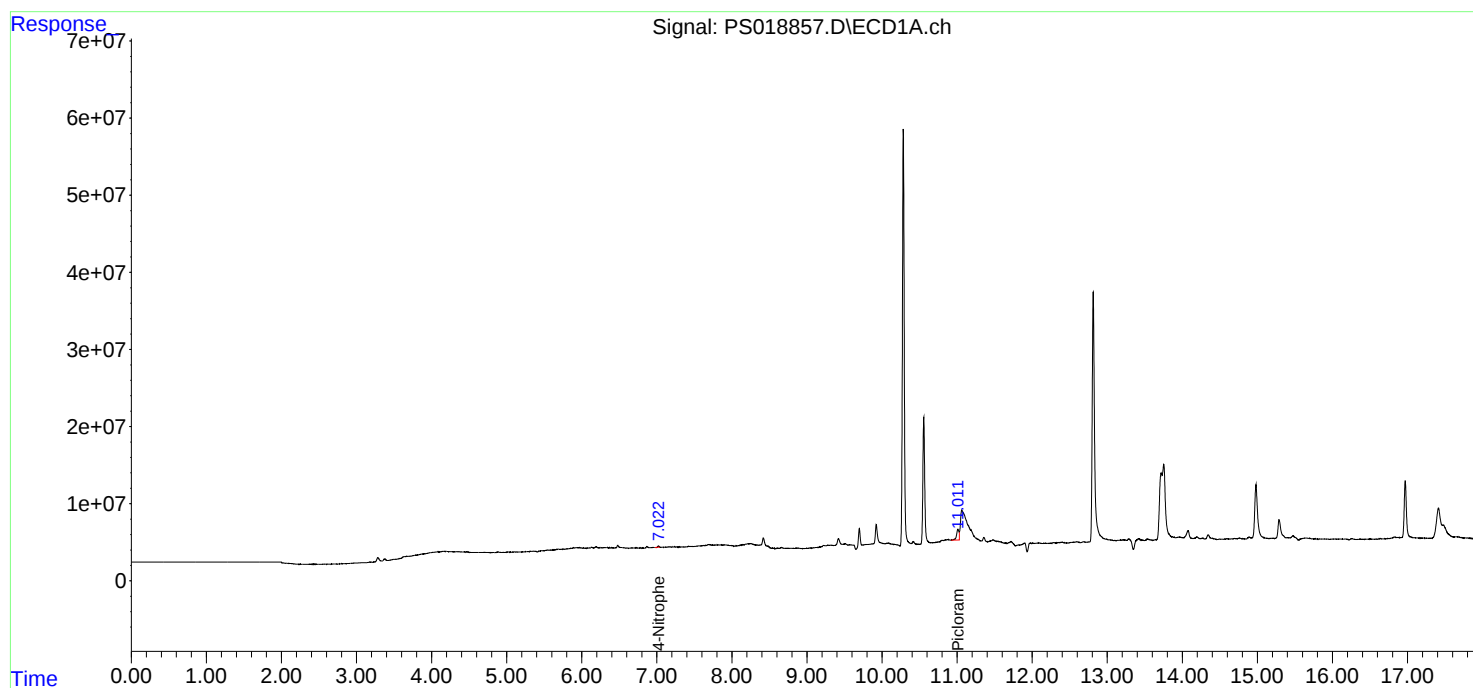


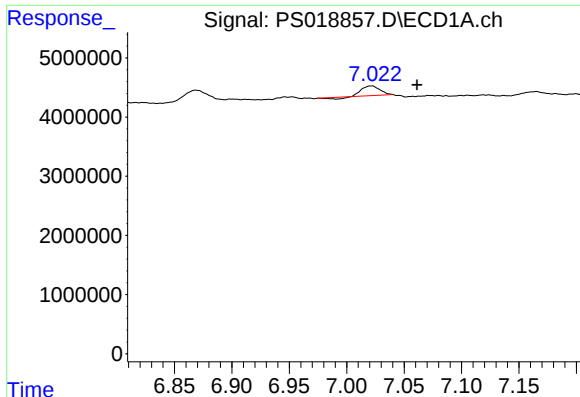

#3 4-Nitrophenol


R.T.: 7.021 min
Delta R.T.: -0.040 min
Response: 1651481
Conc: 1.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

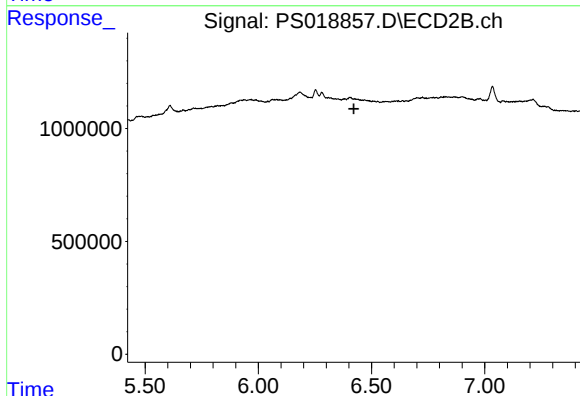


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.422 min
Response: 0
Conc: N.D.

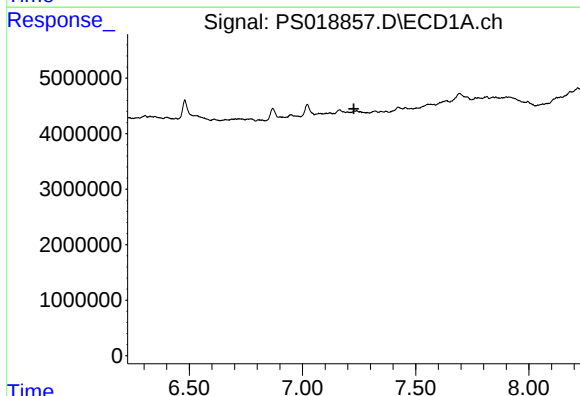


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.227 min
Response: 0
Conc: N.D.

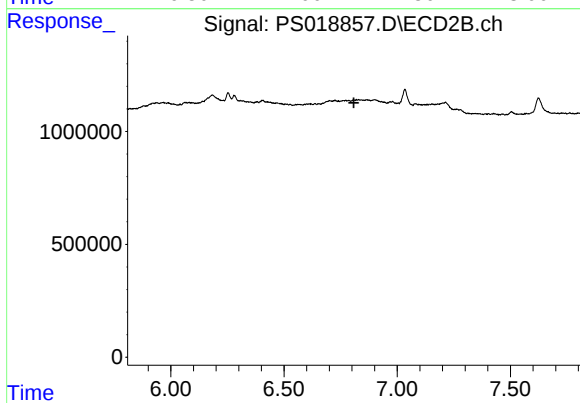

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.808 min
Response: 0
Conc: N.D.

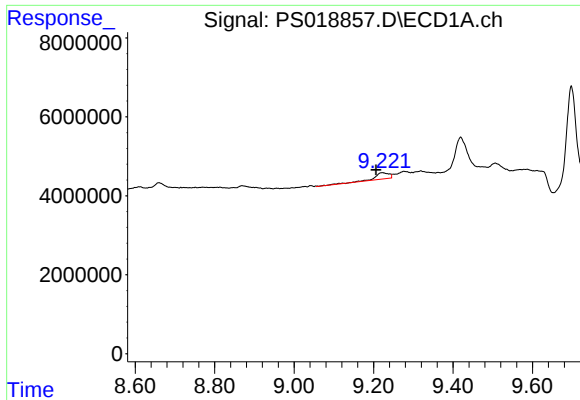

#11 2,4,5-TP (SILVEX)


R.T.: 9.222 min
Delta R.T.: 0.016 min
Response: 4131278
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

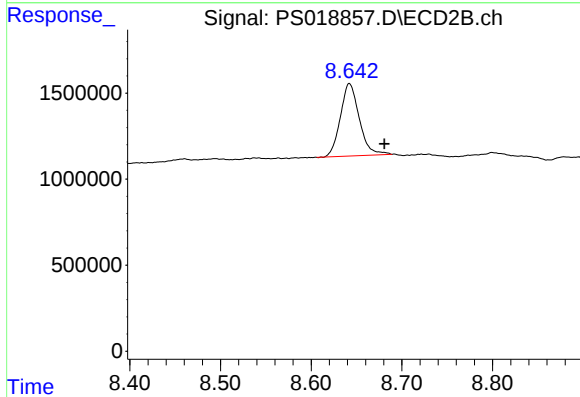


#11 2,4,5-TP (SILVEX)

R.T.: 8.642 min
Delta R.T.: -0.039 min
Response: 6097253
Conc: 1.33 ng/ml

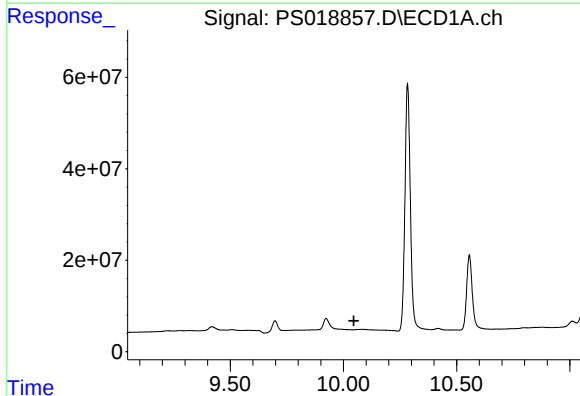


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.046 min
Response: 0
Conc: N.D.

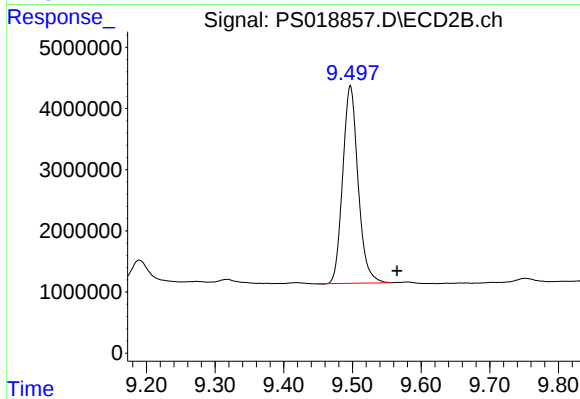

#13 2,4-DB


R.T.: 9.497 min
Delta R.T.: -0.068 min
Response: 50219306
Conc: 88.17 ng/ml

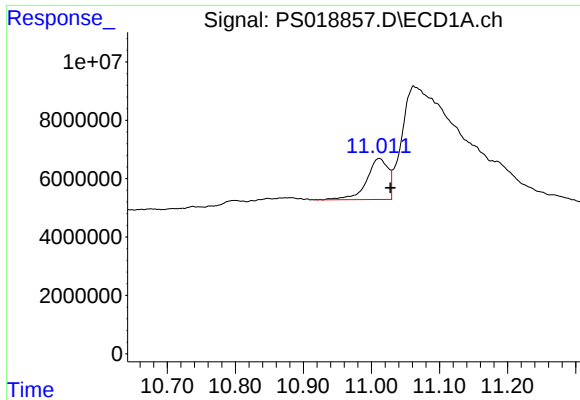

#15 Picloram

R.T.: 11.012 min
Delta R.T.: -0.016 min
Response: 30859364
Conc: 1.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

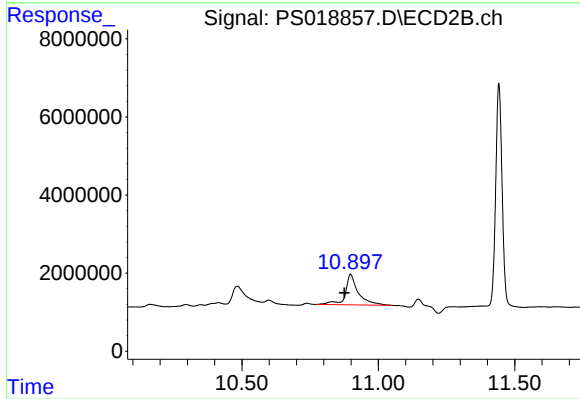

#15 Picloram

R.T.: 10.898 min
Delta R.T.: 0.023 min
Response: 25613952
Conc: 4.53 ng/ml