

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040122\
 Data File : PS018858.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Apr 2022 09:39
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 22:49:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 31 16:06:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.230	6.809	1647.2E6	357.6E6	564.200	500.839
Target Compounds							
3) T	4-Nitroph...	7.035	0.000	197759	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.649	0	5171070	N.D.	1.131
12) T	2,4,5-T	9.483	0.000	4416871	0	<MDL	N.D. #
13) T	2,4-DB	0.000	9.500f	0	29284113	N.D.	51.414
14) T	DINOSEB	11.141f	0.000	59716287	0	3.658	N.D. #
15) T	Picloram	0.000	10.925f	0	8771078	N.D.	1.551



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040122\
Data File : PS018858.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Apr 2022 09:39
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 22:49:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
Quant Title : 8080.M
QLast Update : Thu Mar 31 16:06:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

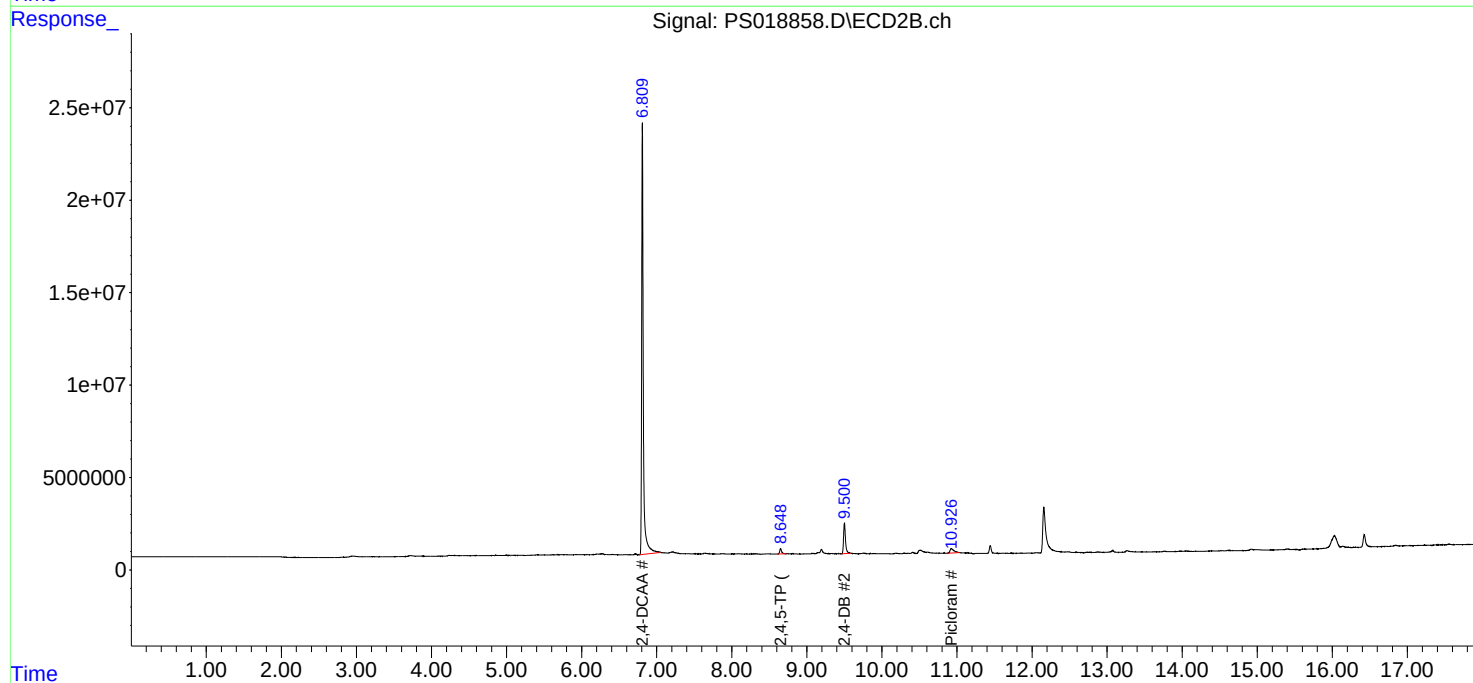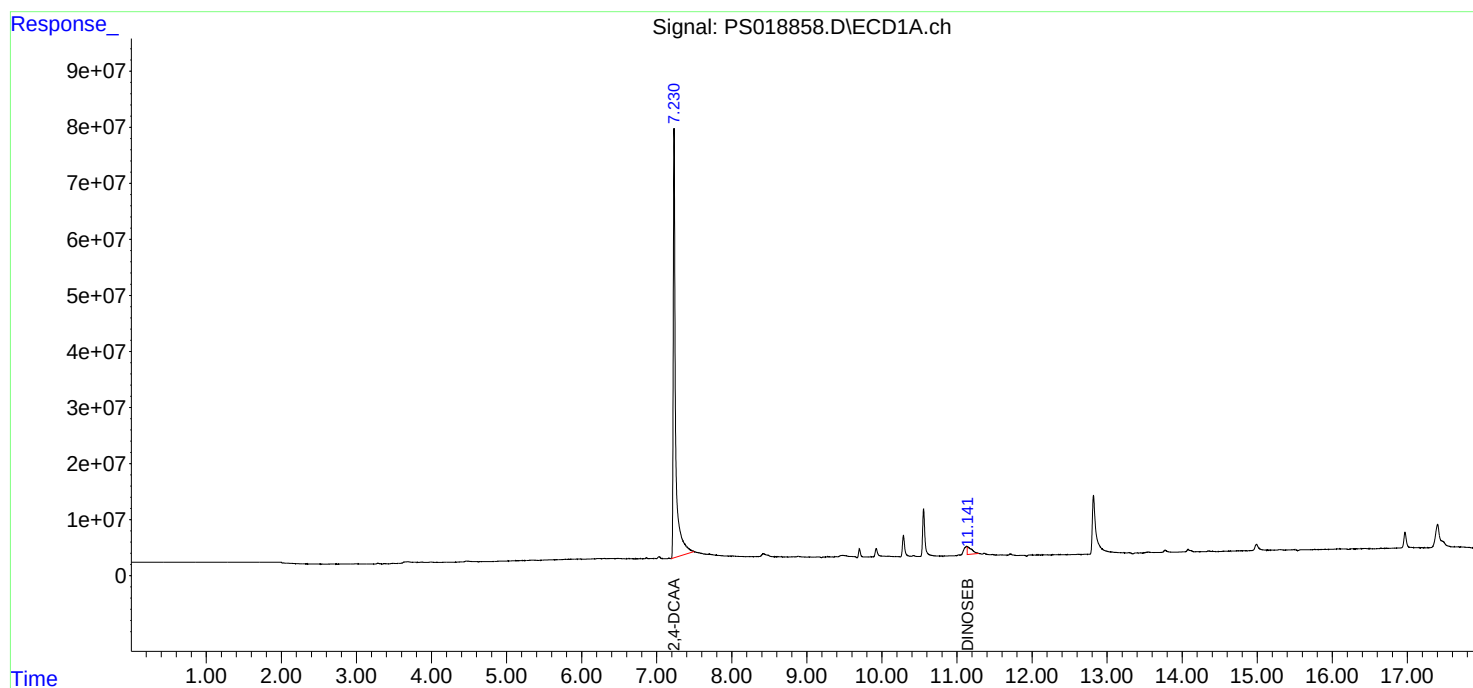


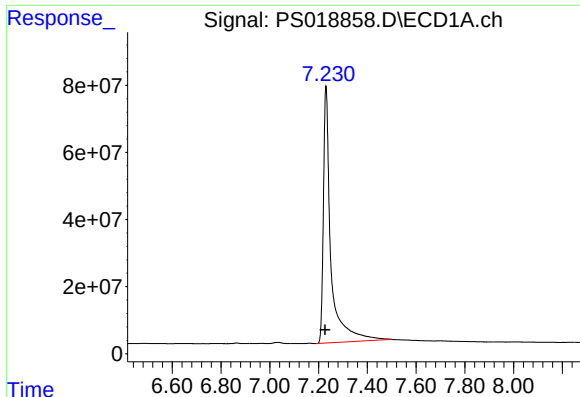

#4 2,4-DCAA


R.T.: 7.230 min
Delta R.T.: 0.003 min
Response: 1647159873
Conc: 564.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

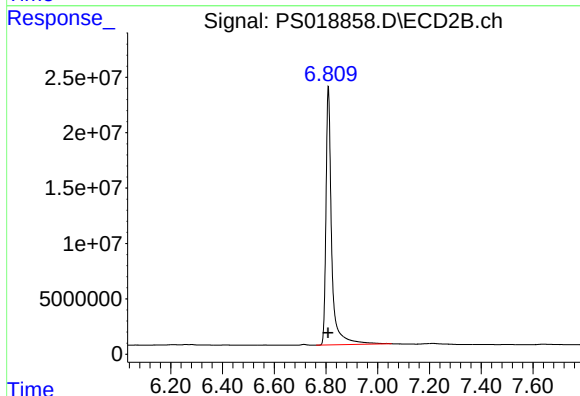


#4 2,4-DCAA

R.T.: 6.809 min
Delta R.T.: 0.000 min
Response: 357570369
Conc: 500.84 ng/ml

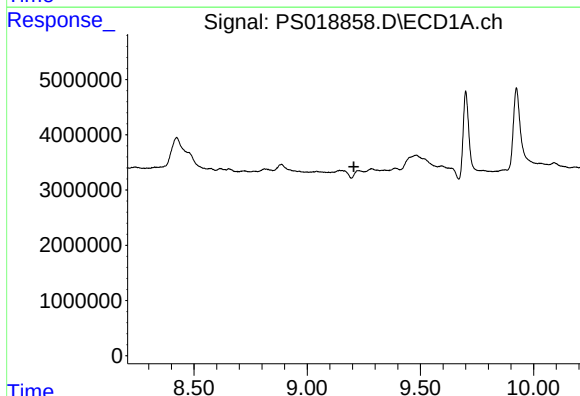


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.206 min
Response: 0
Conc: N.D.

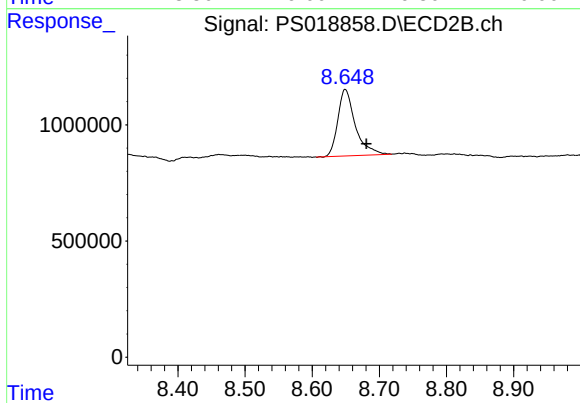

#11 2,4,5-TP (SILVEX)


R.T.: 8.649 min
Delta R.T.: -0.032 min
Response: 5171070
Conc: 1.13 ng/ml

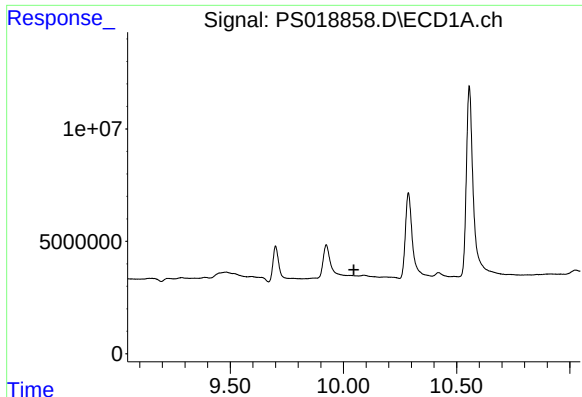

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.046 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

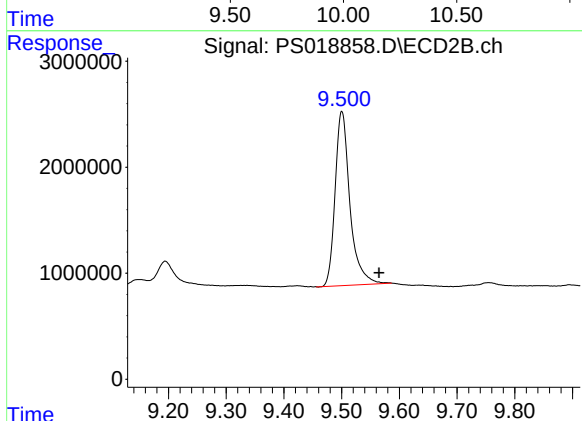


#13 2,4-DB

R.T.: 9.500 min
Delta R.T.: -0.064 min
Response: 29284113
Conc: 51.41 ng/ml

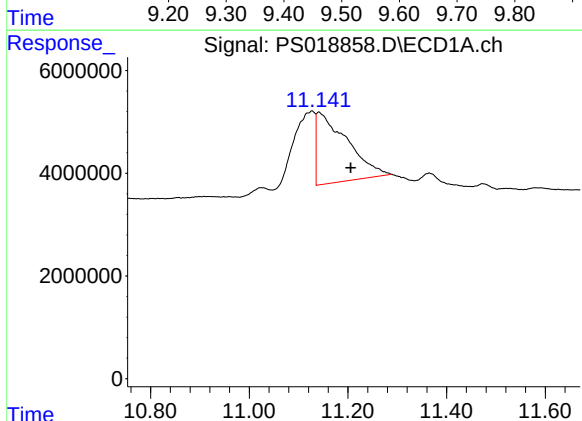


#14 DINOSEB

R.T.: 11.141 min
Delta R.T.: -0.065 min
Response: 59716287
Conc: 3.66 ng/ml

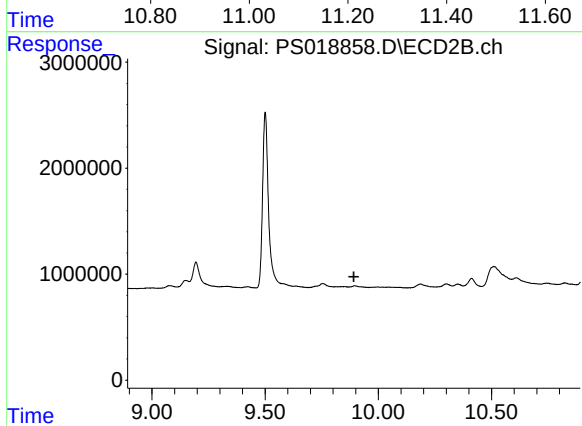

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.892 min
Response: 0
Conc: N.D.

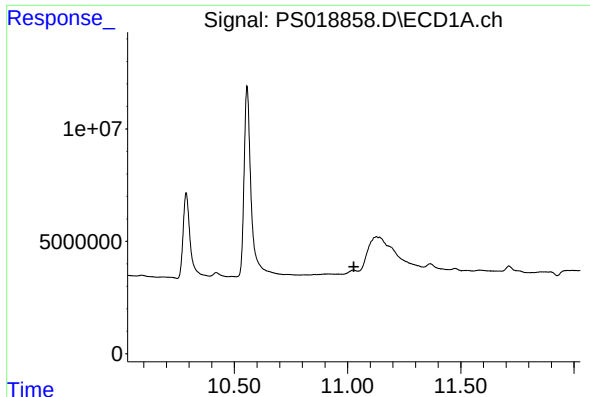

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 11.028 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

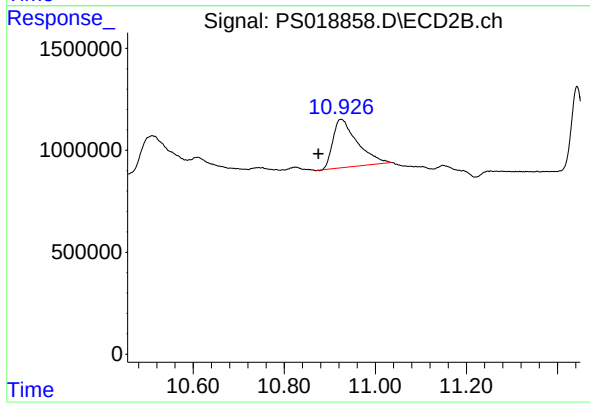

#15 Picloram

R.T.: 10.925 min
Delta R.T.: 0.050 min
Response: 8771078
Conc: 1.55 ng/ml