

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040122\
 Data File : PS018863.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Apr 2022 15:44
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 22:51:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 31 16:06:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.227	6.808	1537.6E6	343.2E6	526.672	480.747
Target Compounds							
3) T	4-Nitroph...	7.029	0.000	1256461	0	1.101	N.D. #
5) T	DICAMBA	7.413	0.000	3774263	0	<MDL	N.D. #
7) T	MCPA	7.681f	0.000	4204860	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.220	8.641f	8553645	18690331	<MDL	4.089 #
12) T	2,4,5-T	9.496	9.066	11416550	841817	<MDL	<MDL #
13) T	2,4-DB	10.085	0.000	4347519	0	1.281	N.D. #
14) T	DINOSEB	11.168	0.000	72150694	0	4.419	N.D. #
15) T	Picloram	11.007	10.896	5541643	75239594	<MDL	13.307 #
16) T	DCPA	11.476	0.000	6185343	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040122\
Data File : PS018863.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Apr 2022 15:44
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 22:51:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
Quant Title : 8080.M
QLast Update : Thu Mar 31 16:06:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

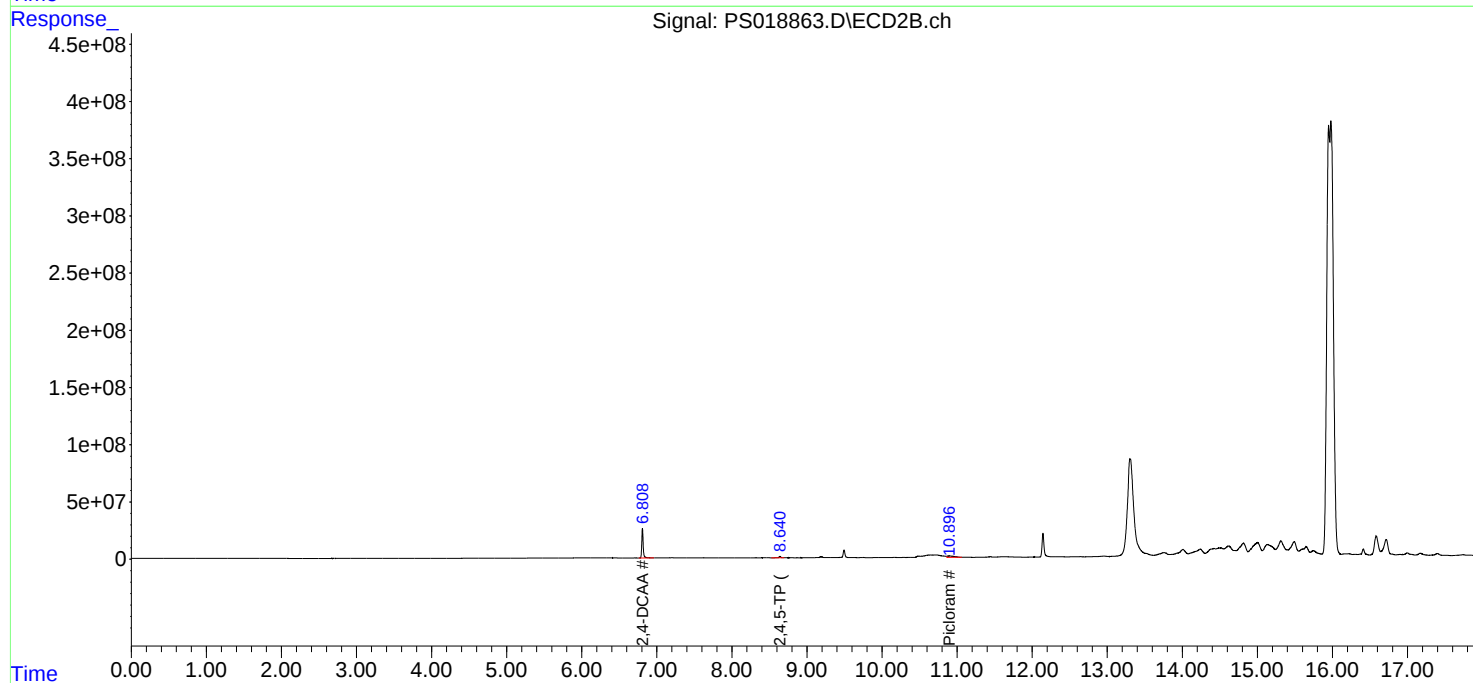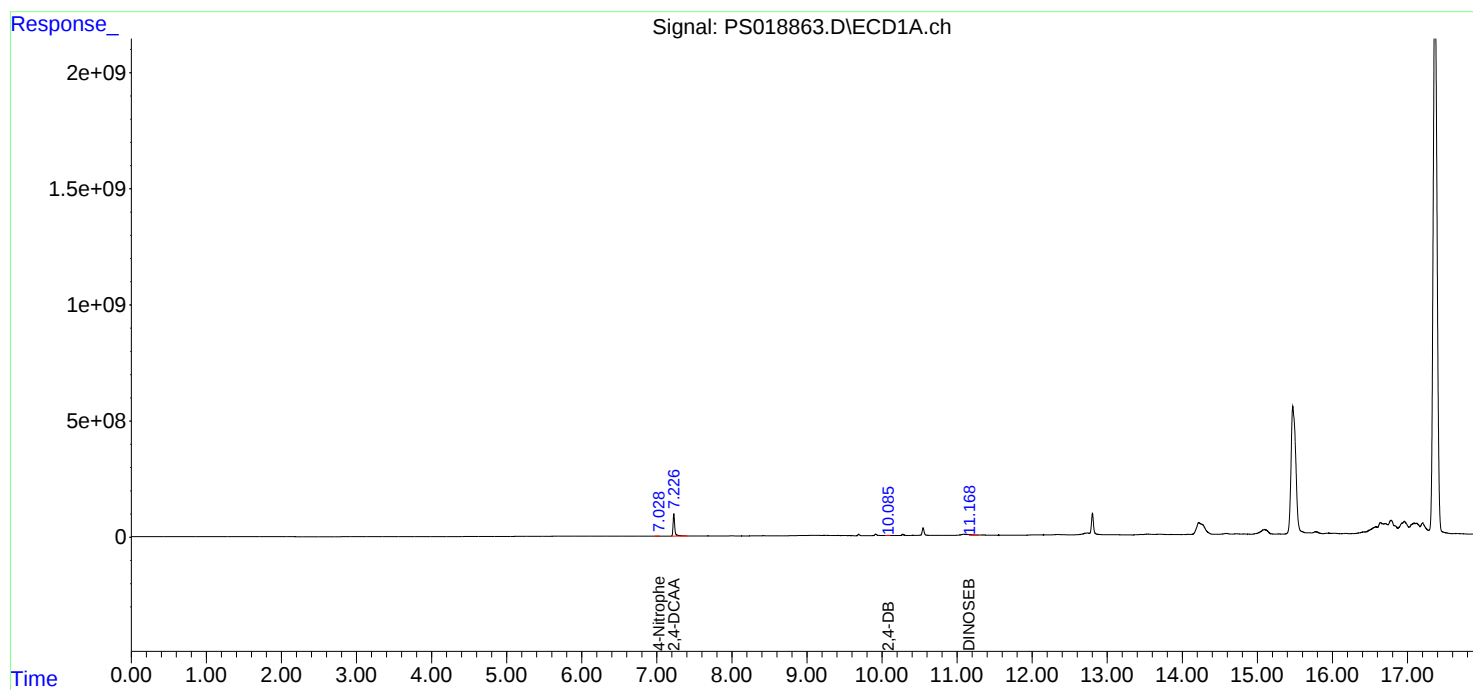


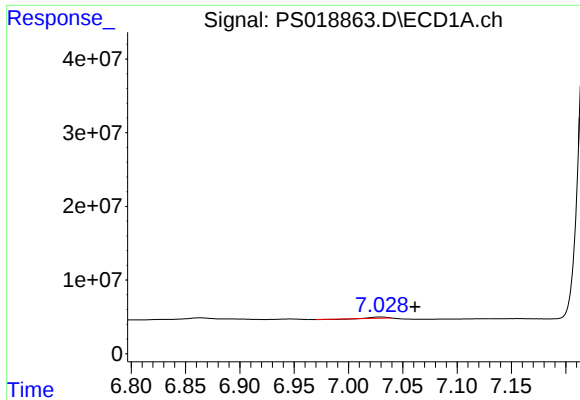

#3 4-Nitrophenol


R.T.: 7.029 min
Delta R.T.: -0.032 min
Response: 1256461
Conc: 1.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

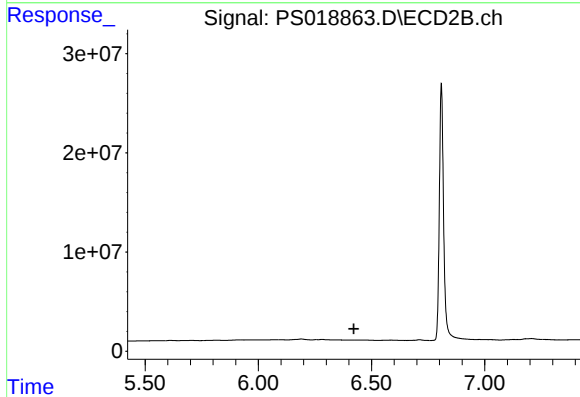


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.422 min
Response: 0
Conc: N.D.

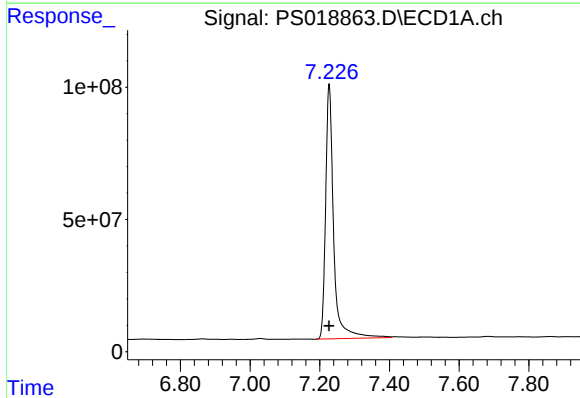


#4 2,4-DCAA

R.T.: 7.227 min
Delta R.T.: 0.000 min
Response: 1537597228
Conc: 526.67 ng/ml

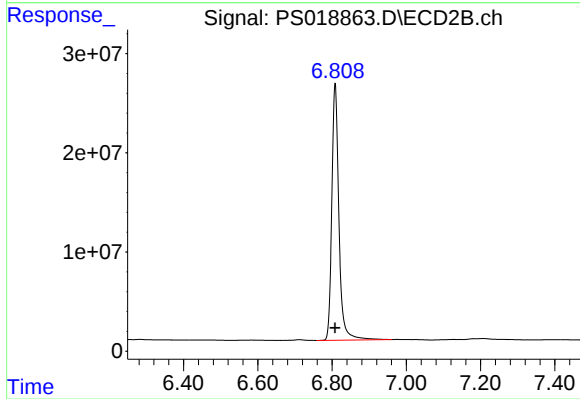

#4 2,4-DCAA


R.T.: 6.808 min
Delta R.T.: 0.000 min
Response: 343225430
Conc: 480.75 ng/ml

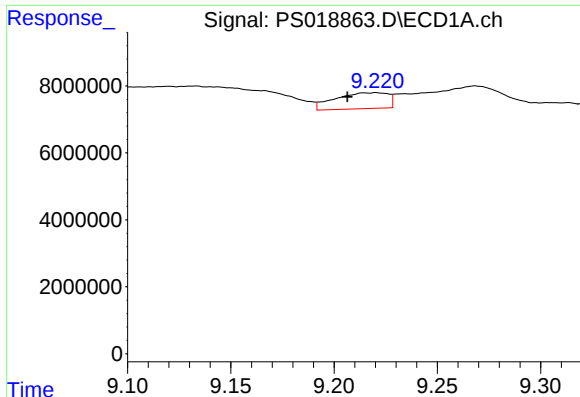

#11 2,4,5-TP (SILVEX)


R.T.: 9.220 min
Delta R.T.: 0.014 min
Response: 8553645
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

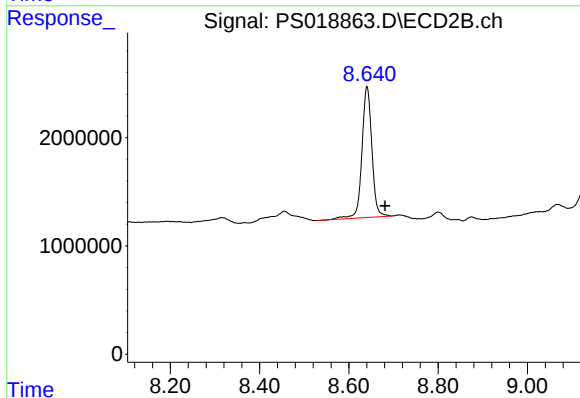


#11 2,4,5-TP (SILVEX)

R.T.: 8.641 min
Delta R.T.: -0.040 min
Response: 18690331
Conc: 4.09 ng/ml

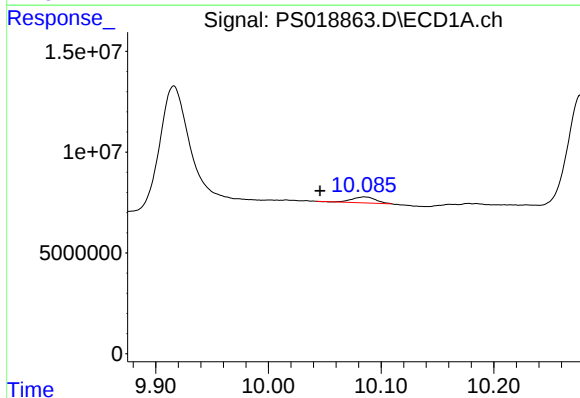


#13 2,4-DB

R.T.: 10.085 min
Delta R.T.: 0.040 min
Response: 4347519
Conc: 1.28 ng/ml

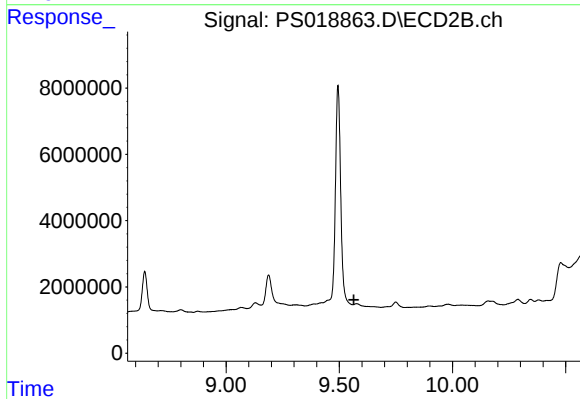

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.565 min
Response: 0
Conc: N.D.

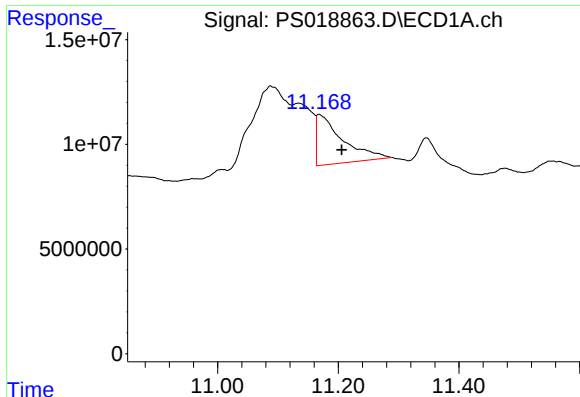

#14 DINoseb


R.T.: 11.168 min
Delta R.T.: -0.037 min
Response: 72150694
Conc: 4.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

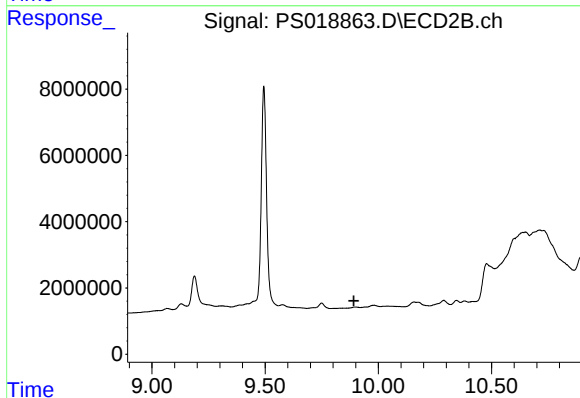


#14 DINoseb

R.T.: 0.000 min
Exp R.T. : 9.892 min
Response: 0
Conc: N.D.

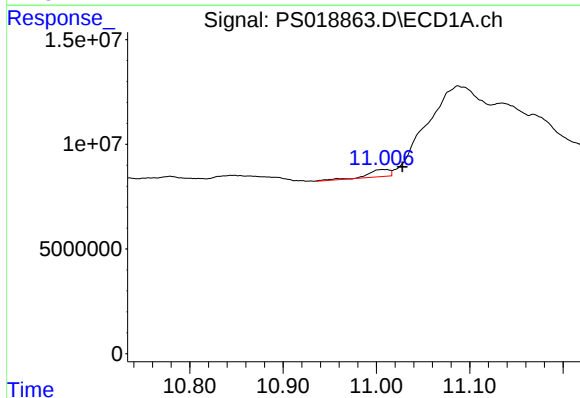

#15 Picloram

R.T.: 11.007 min
Delta R.T.: -0.021 min
Response: 5541643
Conc: N.D.

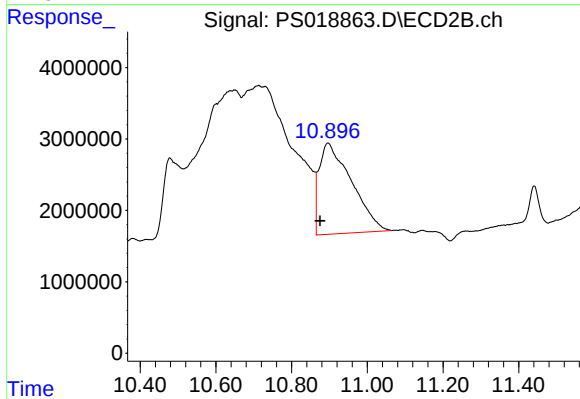

#15 Picloram

R.T.: 10.896 min
Delta R.T.: 0.021 min
Response: 75239594
Conc: 13.31 ng/ml