

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040122\
 Data File : PS018875.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Apr 2022 21:19
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 22:54:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 31 16:06:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.808	1645.5E6	346.9E6	563.626	485.860
Target Compounds							
3) T	4-Nitroph...	7.031	0.000	356788	0	<MDL	N.D. #
7) T	MCPA	7.689f	0.000	1868445	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.630	0	2748400	N.D.	3.342
11) T	2,4,5-TP ...	9.272f	8.643	7776527	11070862	<MDL	2.422 #
12) T	2,4,5-T	9.426f	0.000	4575631	0	<MDL	N.D. #
13) T	2,4-DB	0.000	9.496f	0	50417714	N.D.	88.518
14) T	DINOSEB	11.140f	0.000	48576181	0	2.975	N.D. #
15) T	Picloram	11.012	10.906	7645850	8135539	<MDL	1.439 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040122\
Data File : PS018875.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Apr 2022 21:19
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 22:54:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
Quant Title : 8080.M
QLast Update : Thu Mar 31 16:06:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

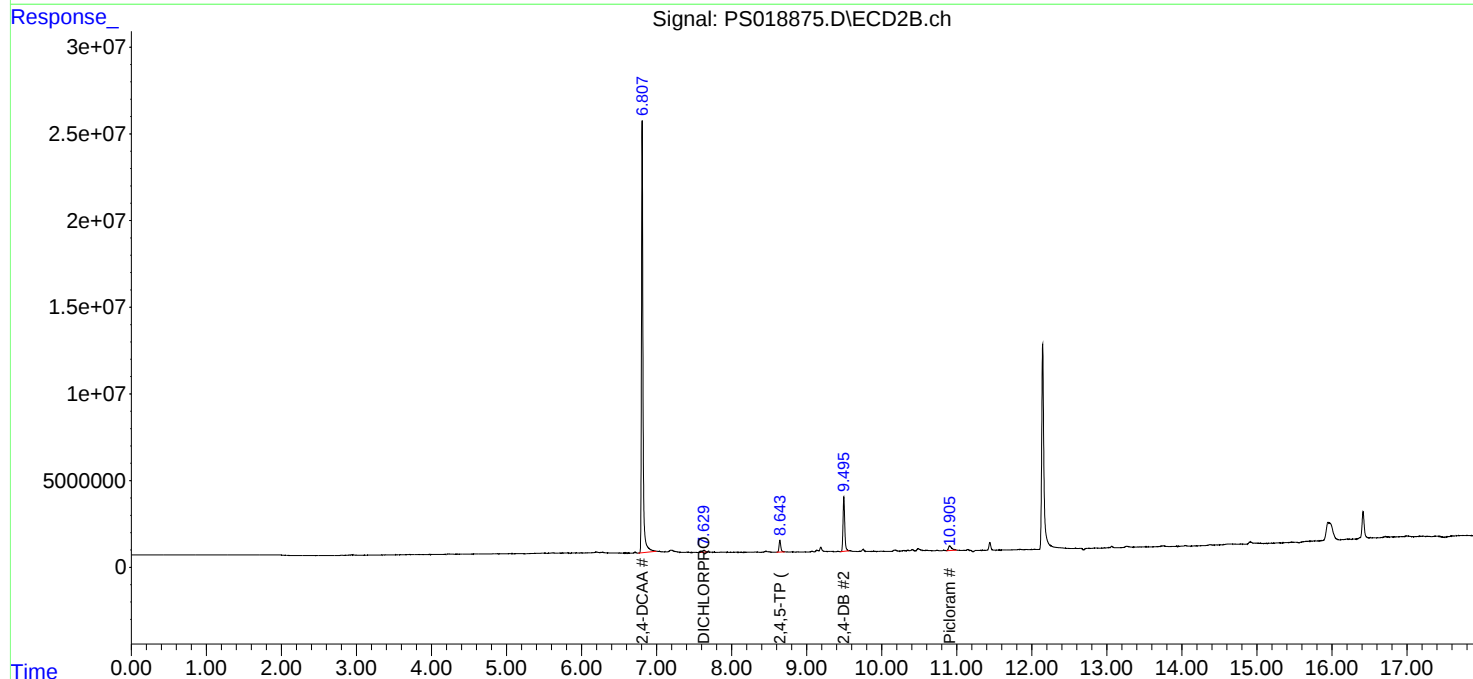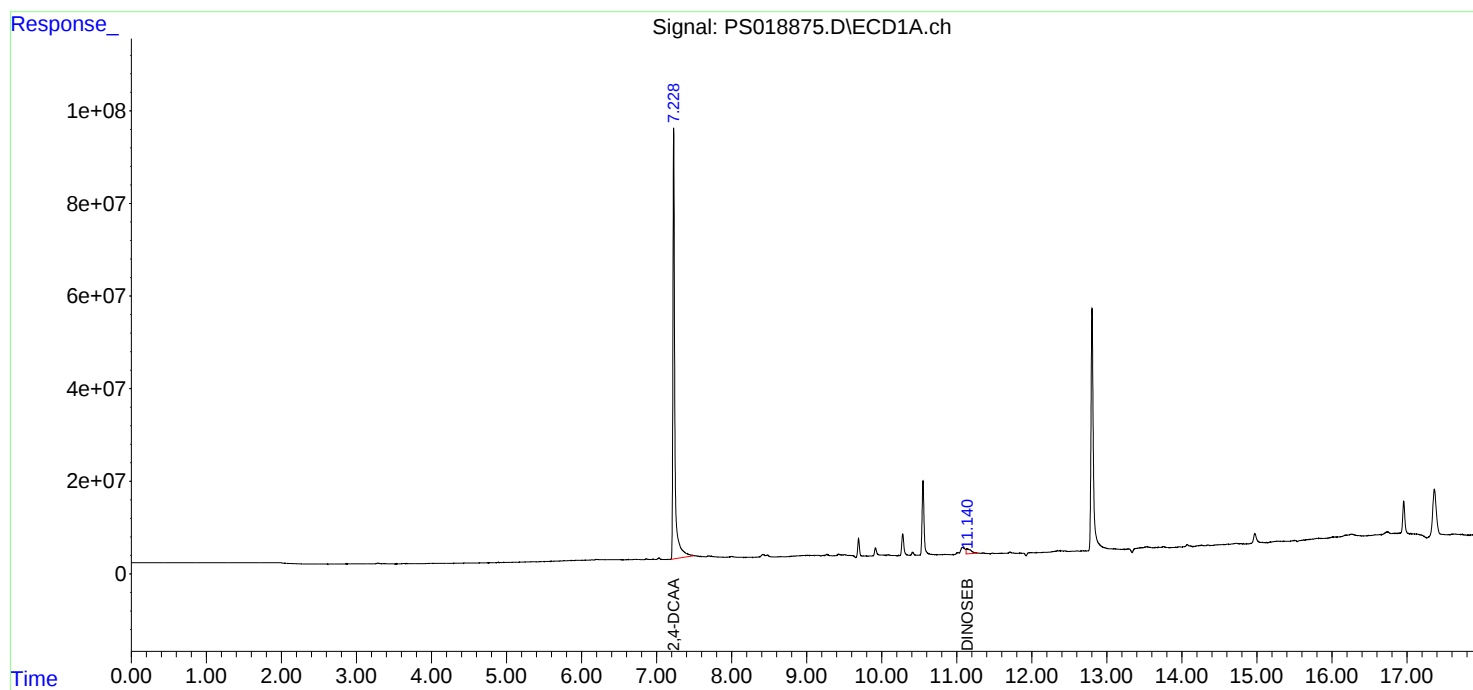


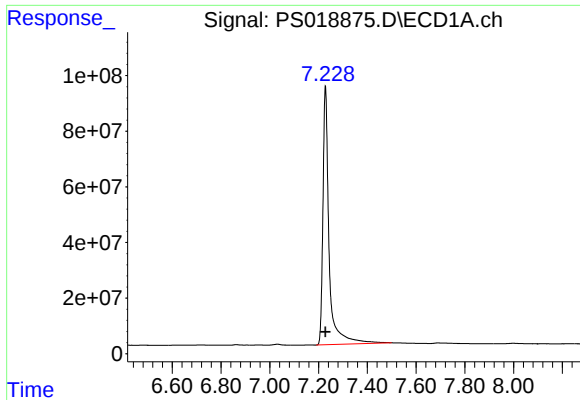

#4 2,4-DCAA


R.T.: 7.228 min
Delta R.T.: 0.000 min
Response: 1645483300
Conc: 563.63 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

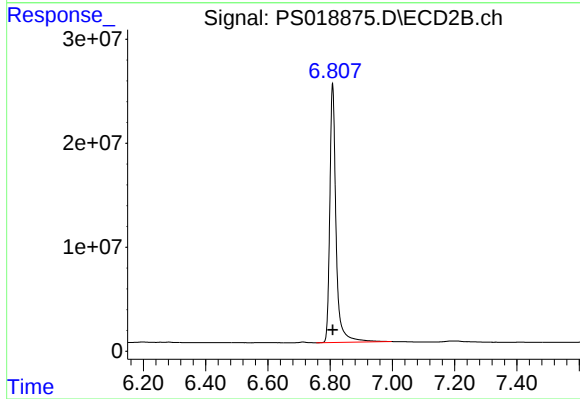


#4 2,4-DCAA

R.T.: 6.808 min
Delta R.T.: 0.000 min
Response: 346876132
Conc: 485.86 ng/ml

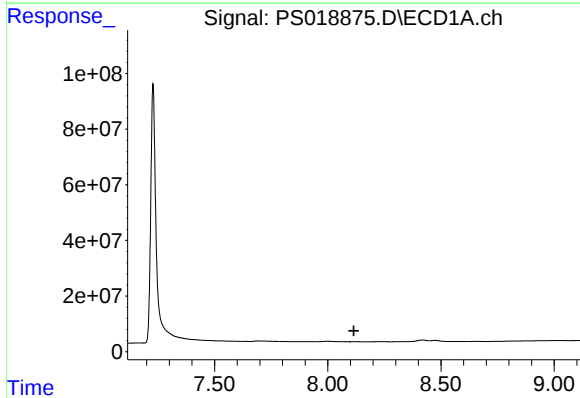


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.115 min
Response: 0
Conc: N.D.

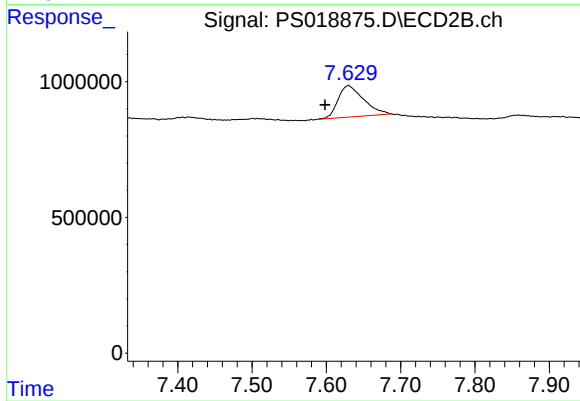

#8 DICHLORPROP


R.T.: 7.630 min
Delta R.T.: 0.032 min
Response: 2748400
Conc: 3.34 ng/ml

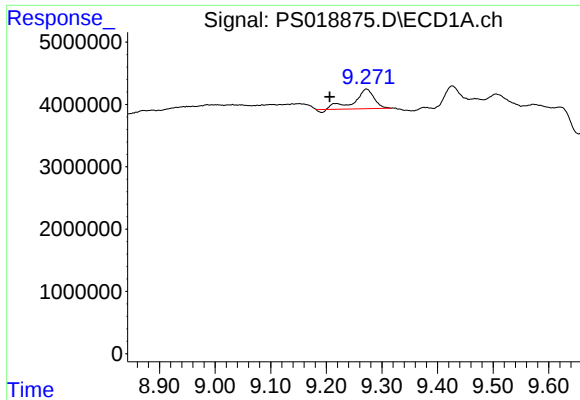

#11 2,4,5-TP (SILVEX)


R.T.: 9.272 min
Delta R.T.: 0.065 min
Response: 7776527
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

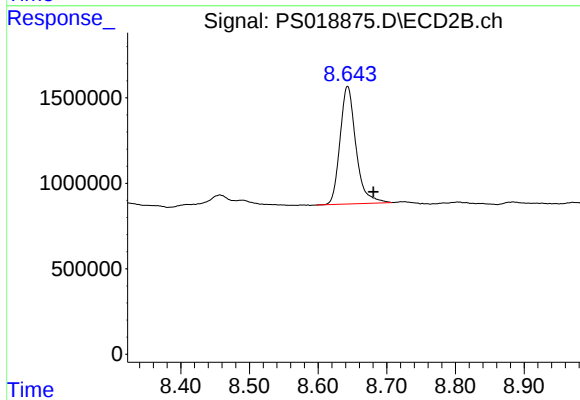


#11 2,4,5-TP (SILVEX)

R.T.: 8.643 min
Delta R.T.: -0.038 min
Response: 11070862
Conc: 2.42 ng/ml

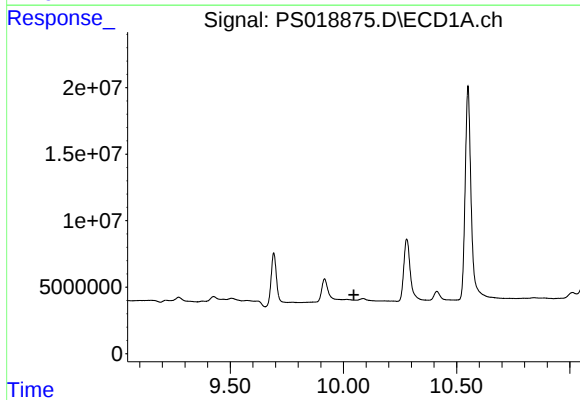


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.046 min
Response: 0
Conc: N.D.

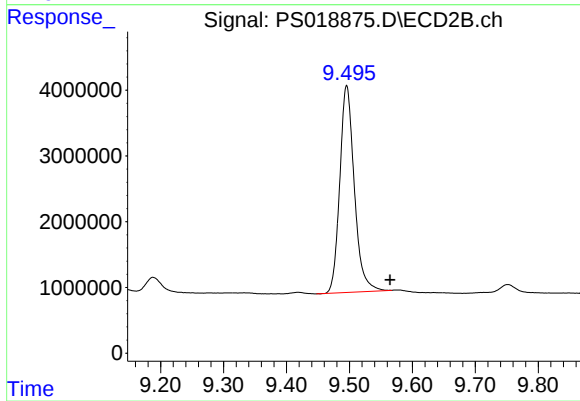

#13 2,4-DB


R.T.: 9.496 min
Delta R.T.: -0.069 min
Response: 50417714
Conc: 88.52 ng/ml

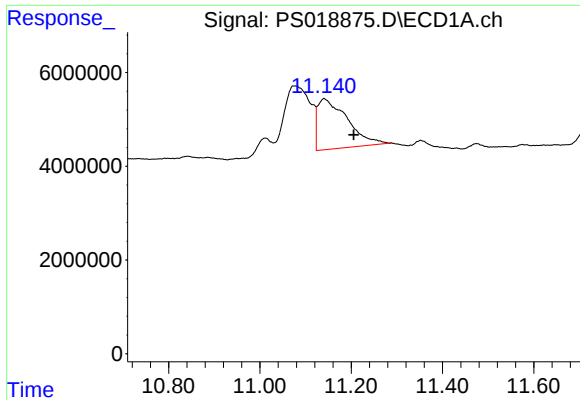

#14 DINoseb


R.T.: 11.140 min
Delta R.T.: -0.065 min
Response: 48576181
Conc: 2.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

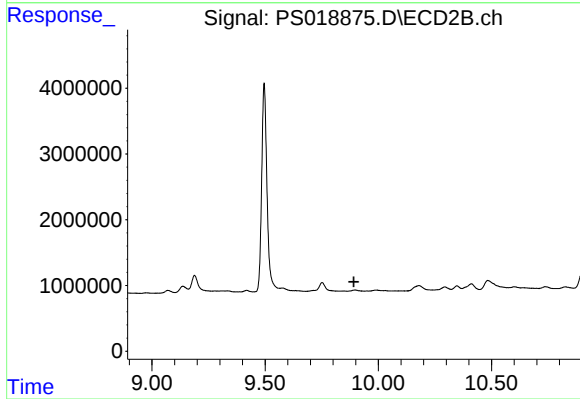


#14 DINoseb

R.T.: 0.000 min
Exp R.T. : 9.892 min
Response: 0
Conc: N.D.

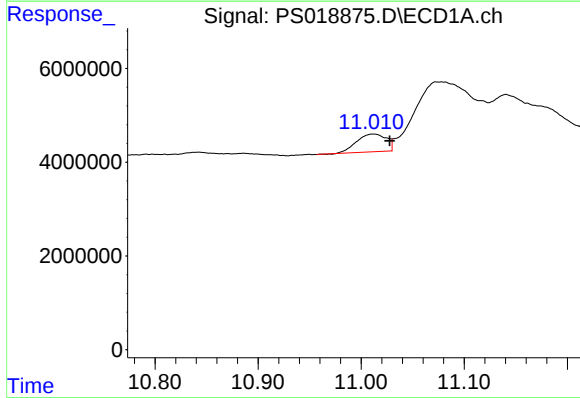

#15 Picloram

R.T.: 11.012 min
Delta R.T.: -0.016 min
Response: 7645850
Conc: N.D.

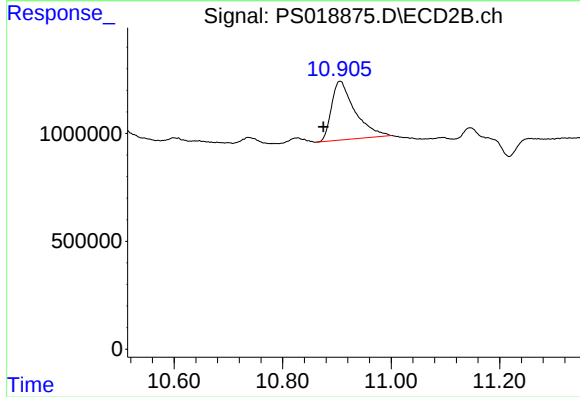

#15 Picloram

R.T.: 10.906 min
Delta R.T.: 0.031 min
Response: 8135539
Conc: 1.44 ng/ml