

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040122\
 Data File : PS018883.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2022 00:30
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 01:16:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 31 16:06:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.227	6.808	1605.7E6	346.3E6	549.992	485.093
Target Compounds							
3) T	4-Nitroph...	7.032	0.000	1653241	0	1.448	N.D. #
7) T	MCPA	7.695f	0.000	2730284	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.630	0	3270453	N.D.	3.977
11) T	2,4,5-TP ...	9.273f	8.642	4545929	14928537	<MDL	3.266 #
12) T	2,4,5-T	9.505	0.000	7495760	0	<MDL	N.D. #
13) T	2,4-DB	0.000	9.496f	0	47510804	N.D.	83.415
14) T	DINOSEB	11.140f	0.000	47249885	0	2.894	N.D. #
15) T	Picloram	11.011	10.902	12292232	7892302	<MDL	1.396 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040122\
Data File : PS018883.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2022 00:30
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 01:16:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
Quant Title : 8080.M
QLast Update : Thu Mar 31 16:06:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

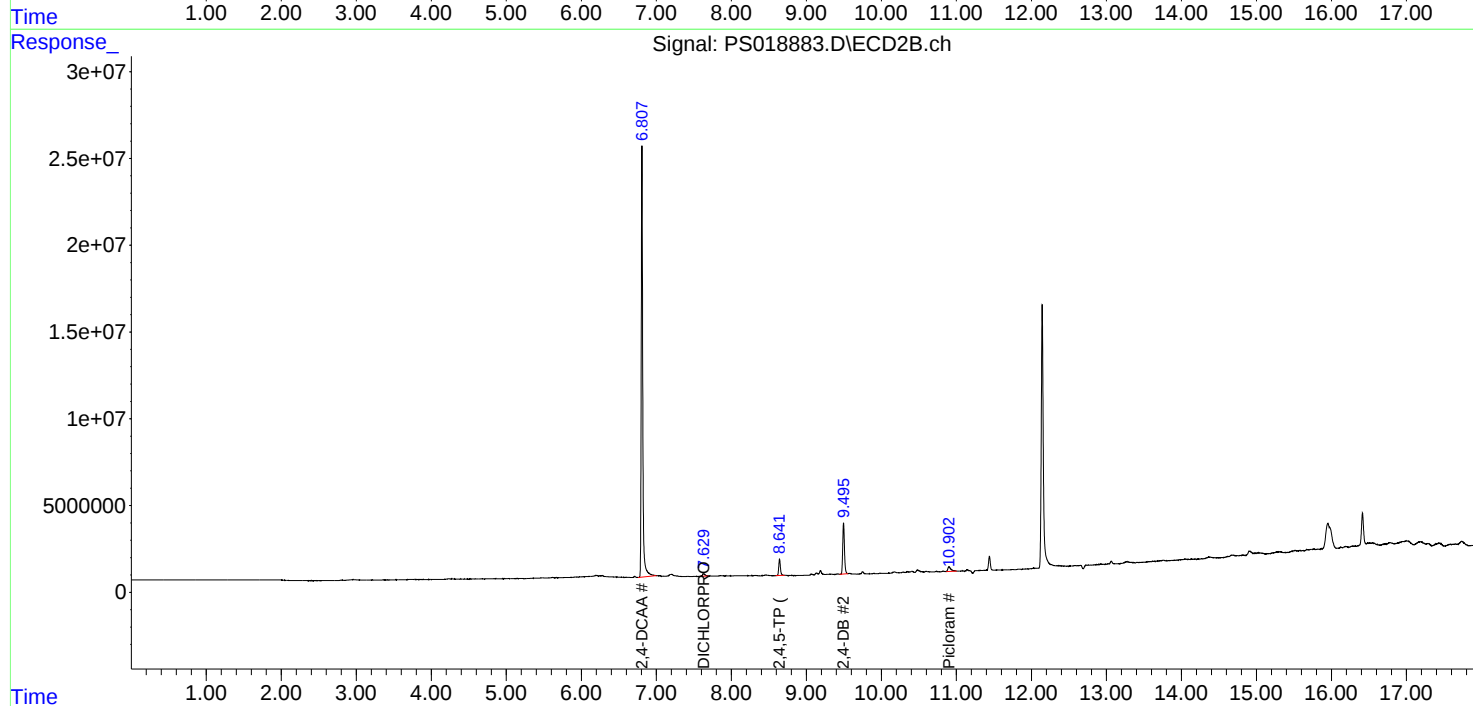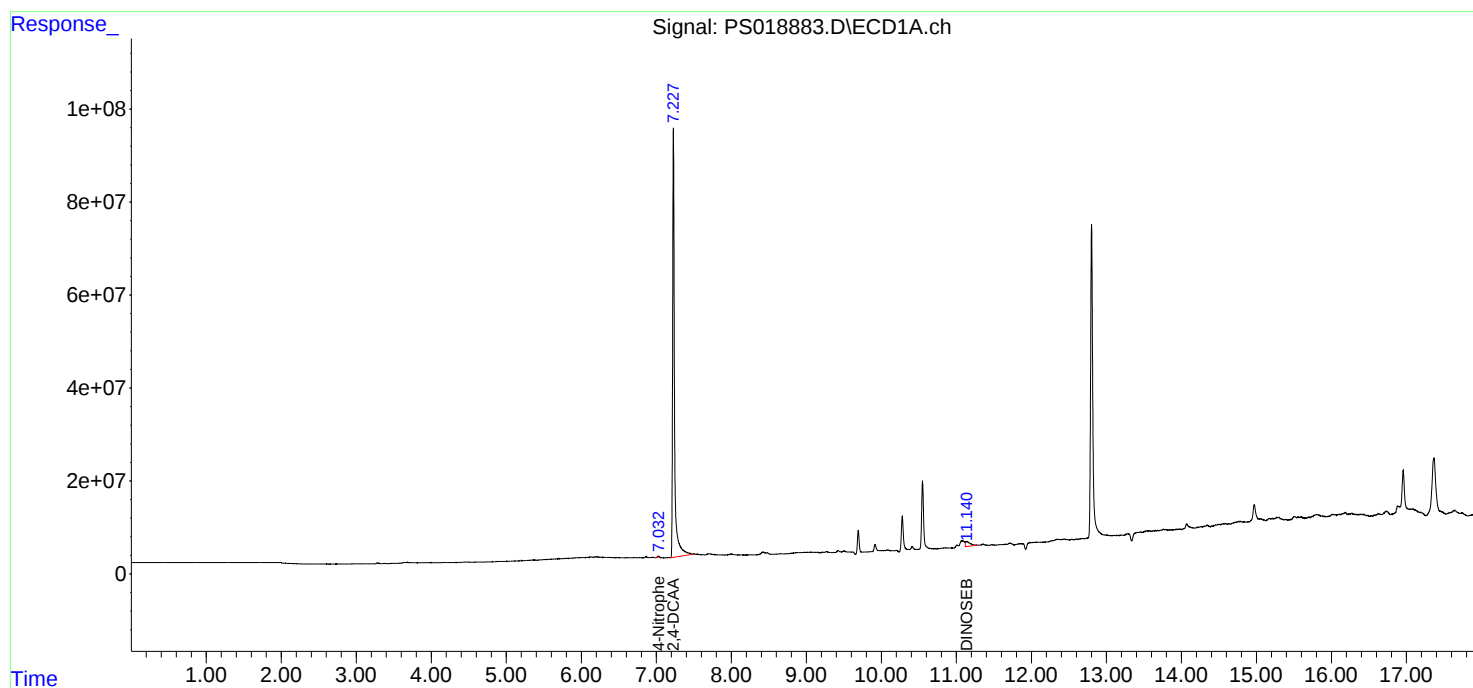


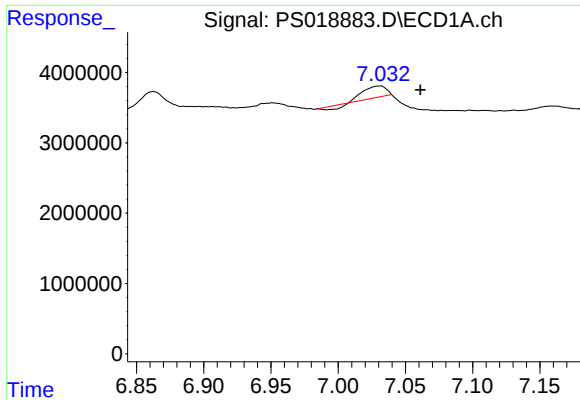

#3 4-Nitrophenol


R.T.: 7.032 min
Delta R.T.: -0.030 min
Response: 1653241
Conc: 1.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

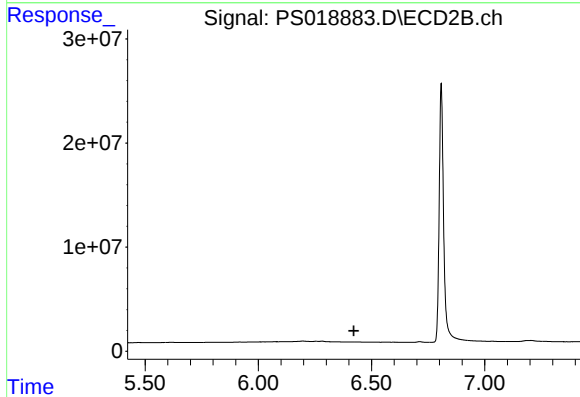


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.422 min
Response: 0
Conc: N.D.

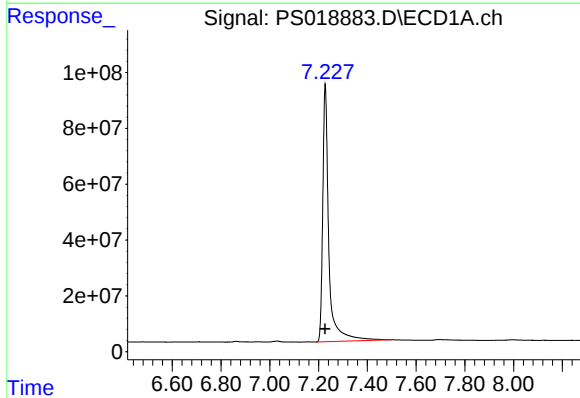


#4 2,4-DCAA

R.T.: 7.227 min
Delta R.T.: 0.000 min
Response: 1605678599
Conc: 549.99 ng/ml

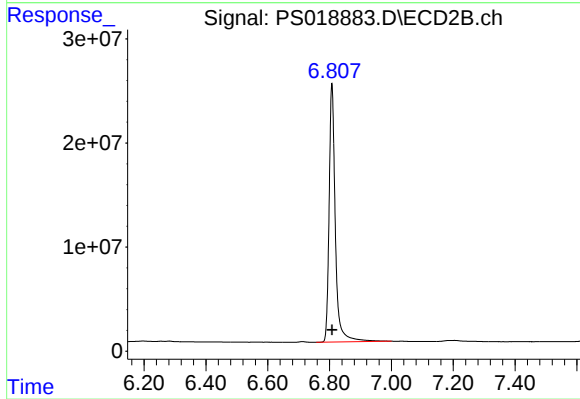

#4 2,4-DCAA


R.T.: 6.808 min
Delta R.T.: 0.000 min
Response: 346328688
Conc: 485.09 ng/ml

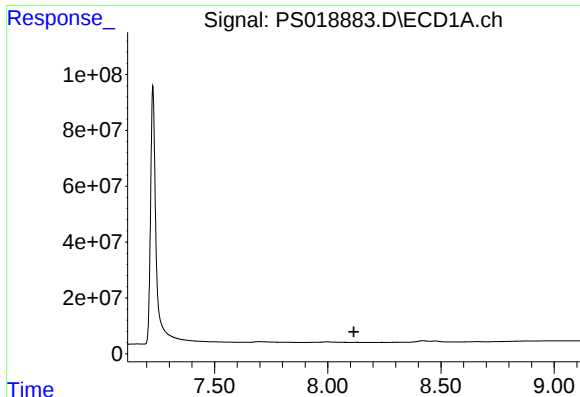

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.115 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

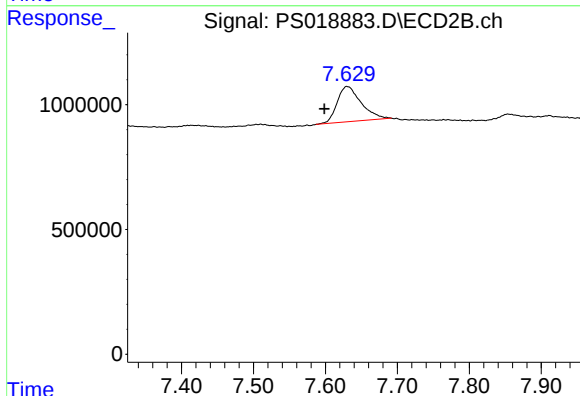


#8 DICHLORPROP

R.T.: 7.630 min
Delta R.T.: 0.031 min
Response: 3270453
Conc: 3.98 ng/ml

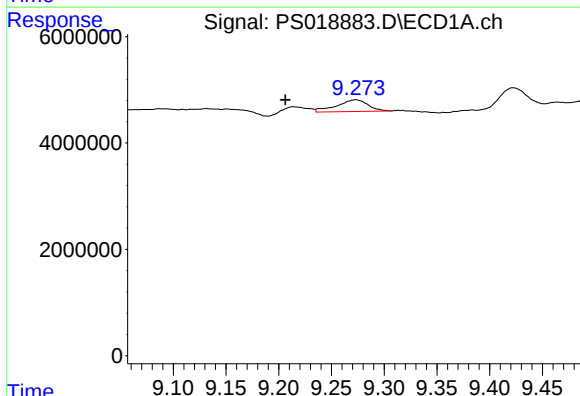


#11 2,4,5-TP (SILVEX)

R.T.: 9.273 min
Delta R.T.: 0.067 min
Response: 4545929
Conc: N.D.

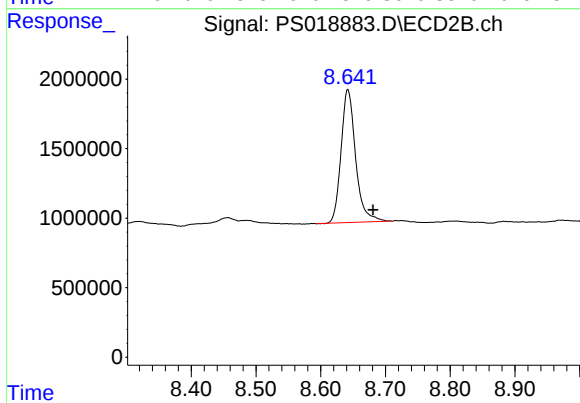

#11 2,4,5-TP (SILVEX)


R.T.: 8.642 min
Delta R.T.: -0.039 min
Response: 14928537
Conc: 3.27 ng/ml

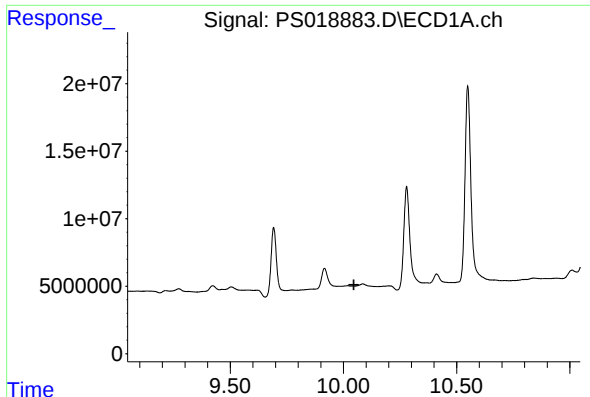

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.046 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

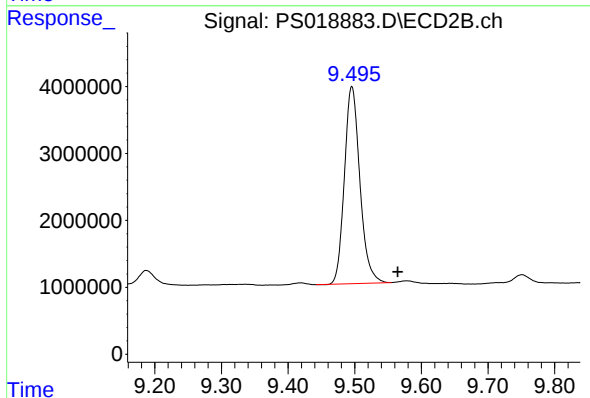


#13 2,4-DB

R.T.: 9.496 min
Delta R.T.: -0.069 min
Response: 47510804
Conc: 83.41 ng/ml

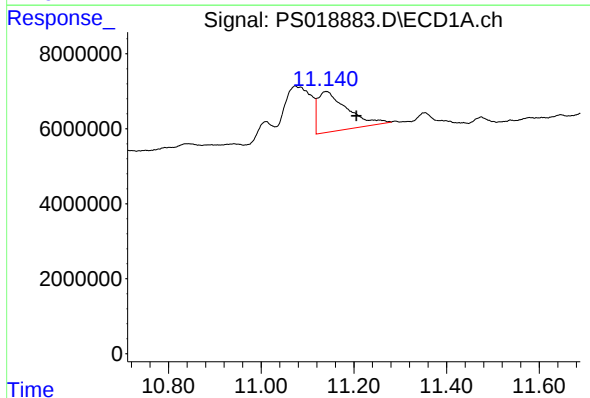


#14 DINOSEB

R.T.: 11.140 min
Delta R.T.: -0.065 min
Response: 47249885
Conc: 2.89 ng/ml

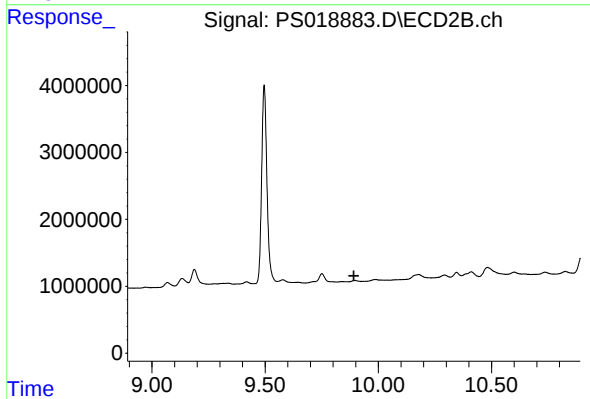

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.892 min
Response: 0
Conc: N.D.

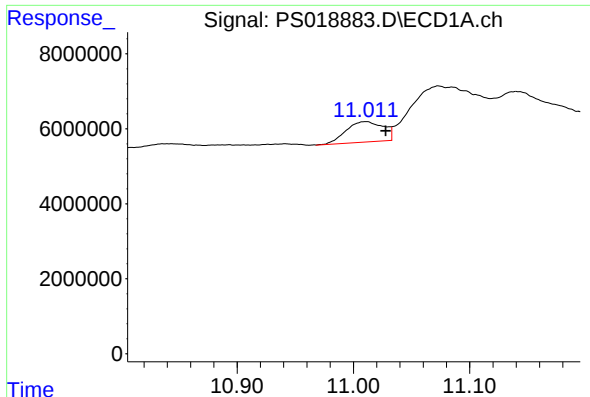

#15 Picloram

R.T.: 11.011 min
Delta R.T.: -0.017 min
Response: 12292232
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

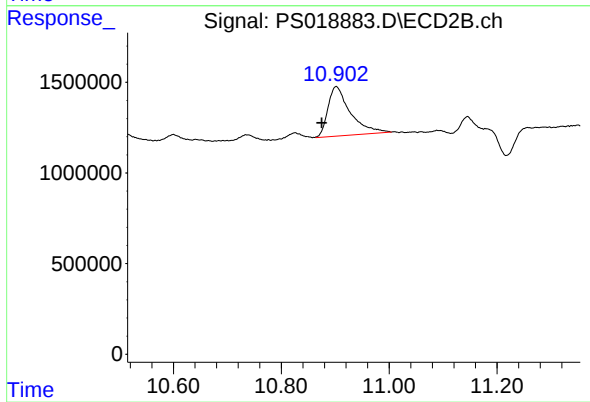

#15 Picloram

R.T.: 10.902 min
Delta R.T.: 0.027 min
Response: 7892302
Conc: 1.40 ng/ml