

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040220\
 Data File : PS009550.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2020 17:03
 Operator : DD\AJ
 Sample : PB127979BS
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 03:26:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.244	6.928	318.6E6	301.1E6	576.011	548.183
Target Compounds							
1) T	Dalapon	3.045	2.621	370.6E6	304.1E6	475.246	386.240
2) T	3,5-DICHL...	6.452	0.000	404.9E6	0	536.439	N.D. #
3) T	4-Nitroph...	7.073	0.000	132.9E6	0	556.751	N.D. #
5) T	DICAMBA	7.438	7.098	1138.9E6	1023.4E6	535.176	445.799
6) T	MCPD	7.606	7.194	89131644	81504949	36.223	44.812
7) T	MCPA	7.755	7.409	122.9E6	111.1E6	40.358	41.185
8) T	DICHLORPROP	8.132	7.726	270.3E6	240.7E6	524.133	433.909
9) T	2,4-D	8.361	8.020	283.5E6	286.7E6	537.635	436.196
10) T	Pentachlo...	8.674	8.453	3888.3E6	3284.8E6	553.008	432.787
11) T	2,4,5-TP ...	9.224	8.814	1492.5E6	1385.2E6	544.464	464.644
12) T	2,4,5-T	9.508	9.193	1362.7E6	1344.8E6	535.673	455.523
13) T	2,4-DB	10.061	9.701	171.1E6	178.6E6	494.657	470.534
14) T	DINOSEB	11.227	10.036	1079.4E6	1012.5E6	528.058	460.960
15) T	Picloram	11.041	11.016	931.1E6	1037.6E6	306.802	254.802
16) T	DCPA	11.491	10.967	1883.2E6	1819.6E6	543.298	469.807



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040220\
Data File : PS009550.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2020 17:03
Operator : DD\AJ
Sample : PB127979BS
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 03:26:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

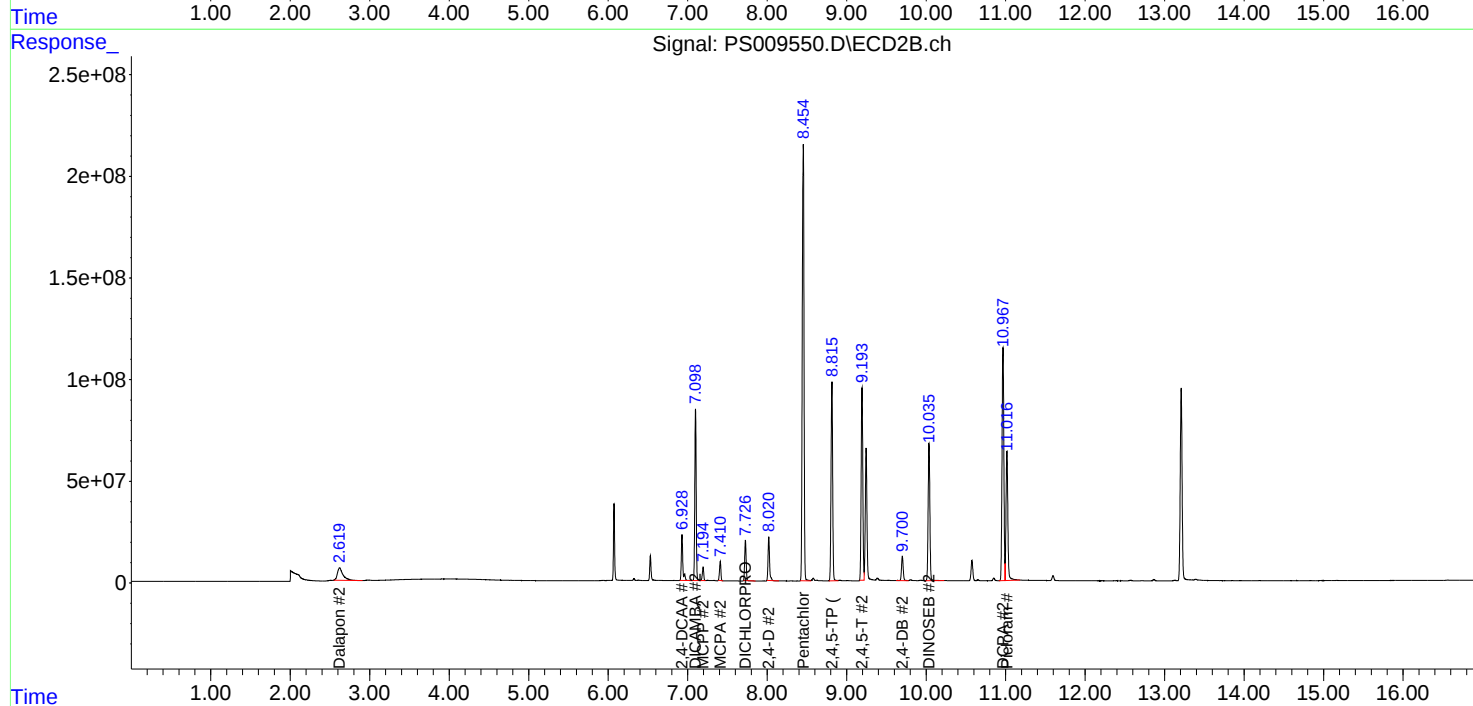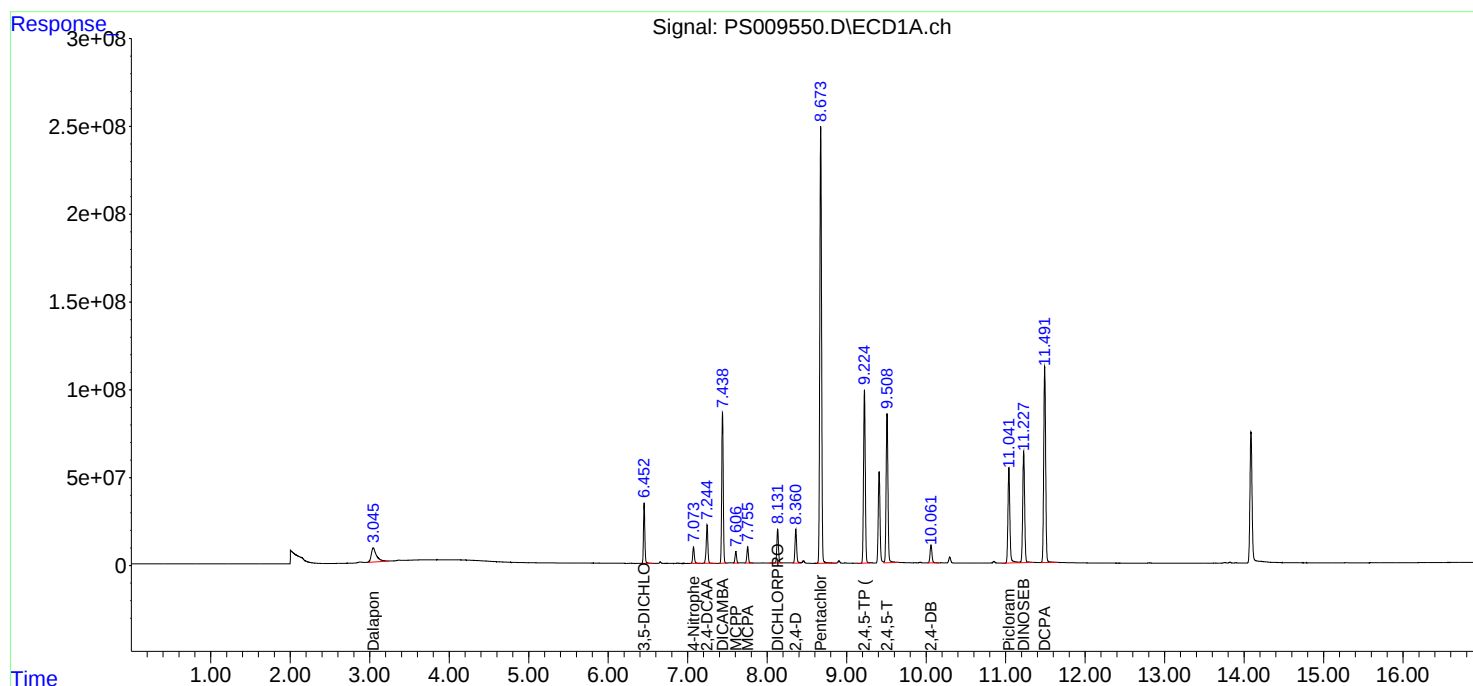


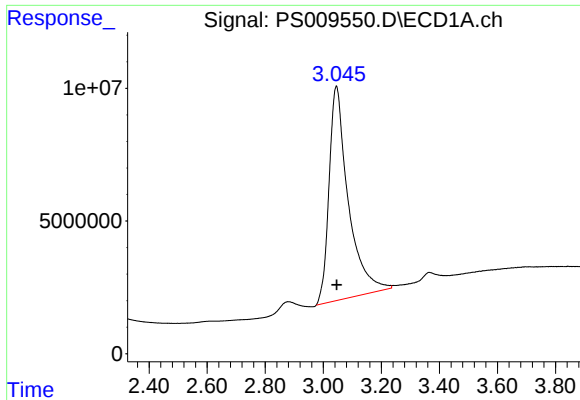

#1 Dalapon


R.T.: 3.045 min
Delta R.T.: 0.000 min
Response: 370613243
Conc: 475.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

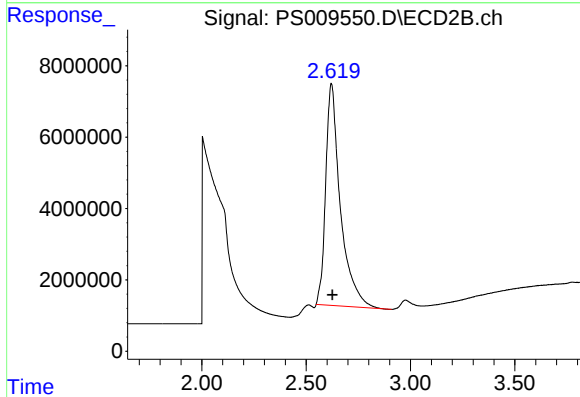


#1 Dalapon

R.T.: 2.621 min
Delta R.T.: -0.006 min
Response: 304110752
Conc: 386.24 ng/ml

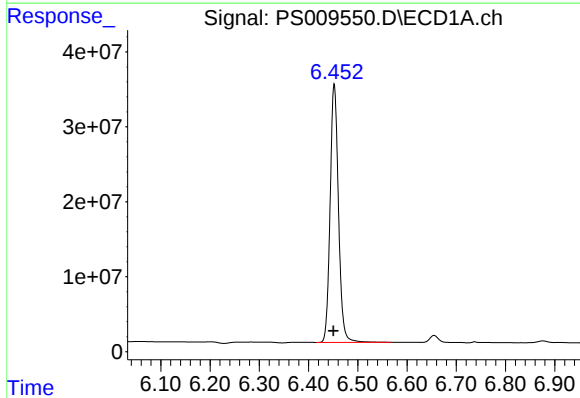


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.452 min
Delta R.T.: 0.001 min
Response: 404902851
Conc: 536.44 ng/ml

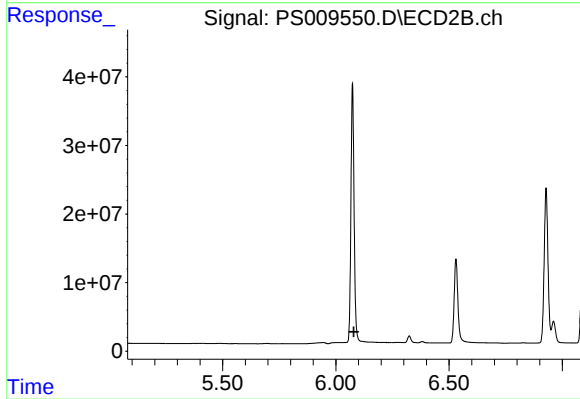

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.080 min
Response: 0
Conc: N.D.

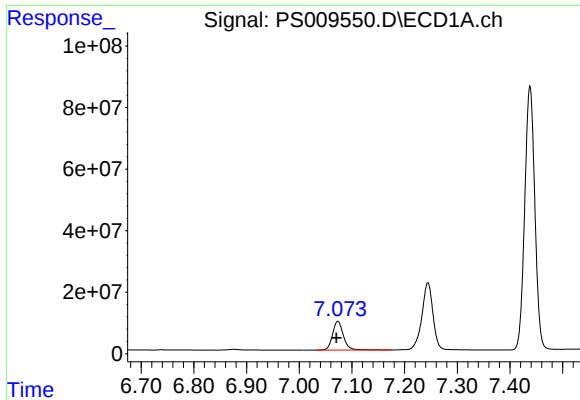

#3 4-Nitrophenol


R.T.: 7.073 min
Delta R.T.: 0.003 min
Response: 132903606
Conc: 556.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

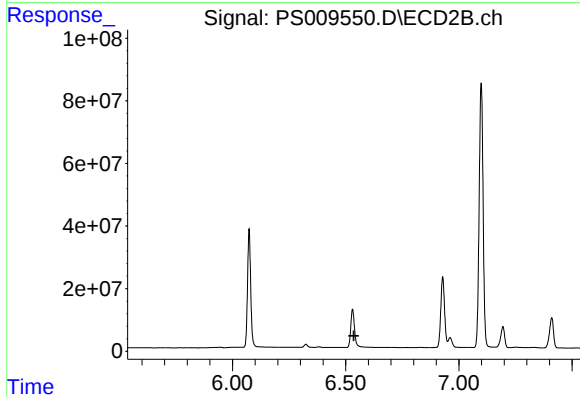


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.536 min
Response: 0
Conc: N.D.

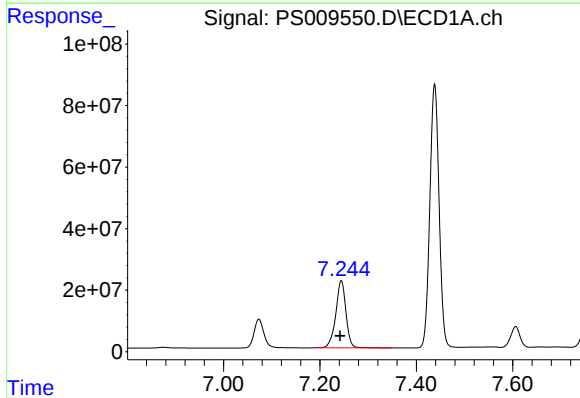


#4 2,4-DCAA

R.T.: 7.244 min
Delta R.T.: 0.002 min
Response: 318632312
Conc: 576.01 ng/ml

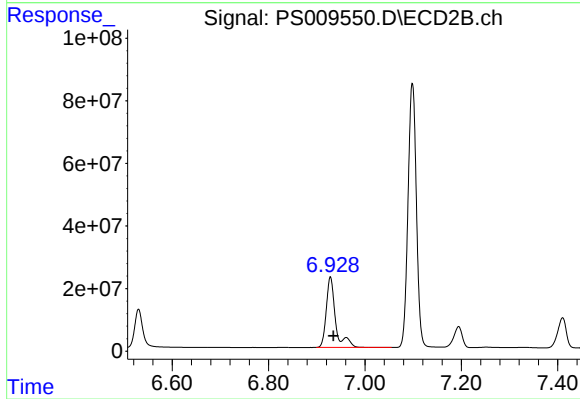

#4 2,4-DCAA


R.T.: 6.928 min
Delta R.T.: -0.007 min
Response: 301060985
Conc: 548.18 ng/ml

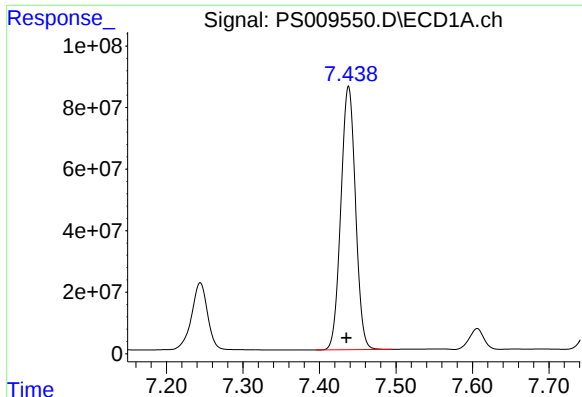

#5 DICAMBA


R.T.: 7.438 min
Delta R.T.: 0.003 min
Response: 1138943740
Conc: 535.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

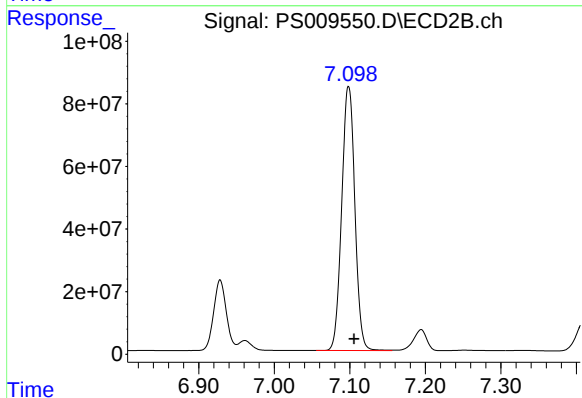


#5 DICAMBA

R.T.: 7.098 min
Delta R.T.: -0.007 min
Response: 1023377224
Conc: 445.80 ng/ml

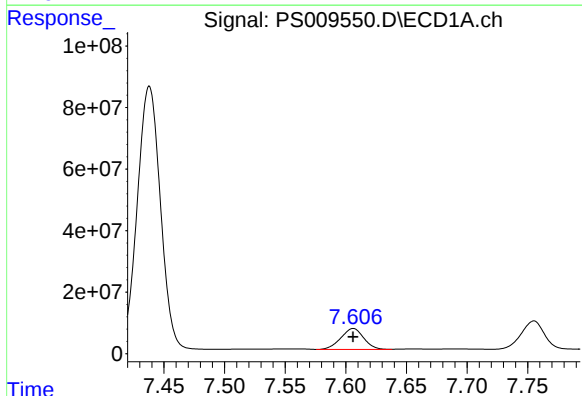


#6 MCP

R.T.: 7.606 min
Delta R.T.: 0.000 min
Response: 89131644
Conc: 36.22 ug/ml

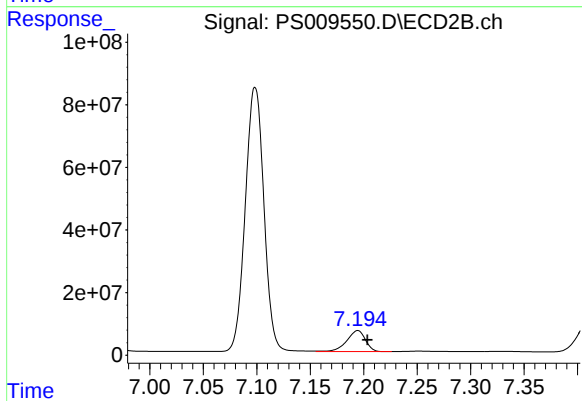

#6 MCP


R.T.: 7.194 min
Delta R.T.: -0.010 min
Response: 81504949
Conc: 44.81 ug/ml

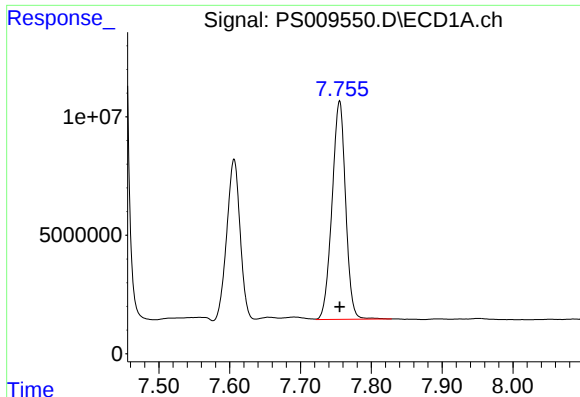

#7 MCPA


R.T.: 7.755 min
Delta R.T.: 0.000 min
Response: 122917027
Conc: 40.36 ug/ml

Instrument :
ECD_S
ClientSampleId :

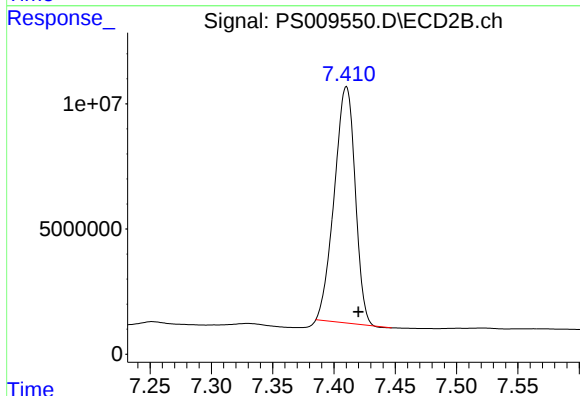


#7 MCPA

R.T.: 7.409 min
Delta R.T.: -0.011 min
Response: 111143160
Conc: 41.19 ug/ml

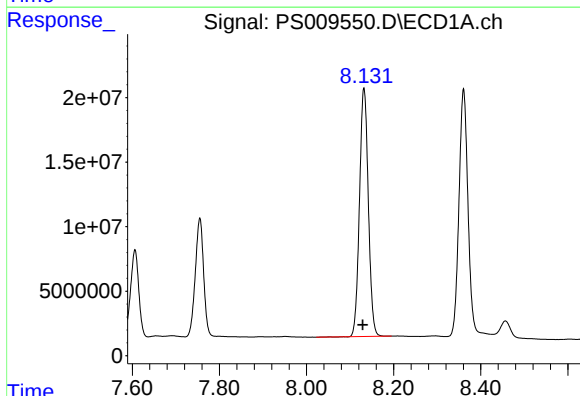


#8 DICHLORPROP

R.T.: 8.132 min
Delta R.T.: 0.003 min
Response: 270318065
Conc: 524.13 ng/ml

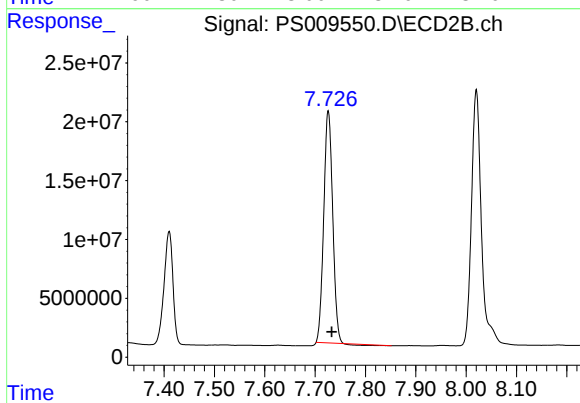

#8 DICHLORPROP


R.T.: 7.726 min
Delta R.T.: -0.007 min
Response: 240742471
Conc: 433.91 ng/ml

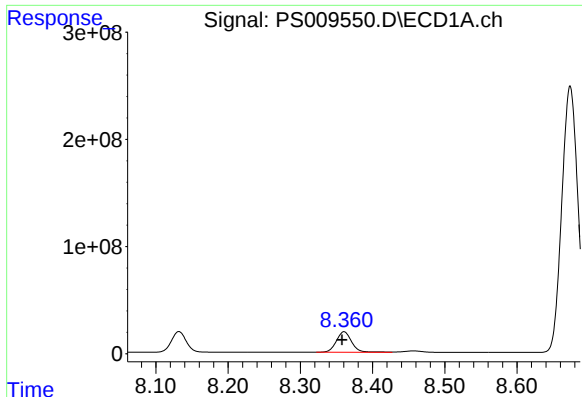

#9 2,4-D


R.T.: 8.361 min
Delta R.T.: 0.003 min
Response: 283454652
Conc: 537.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

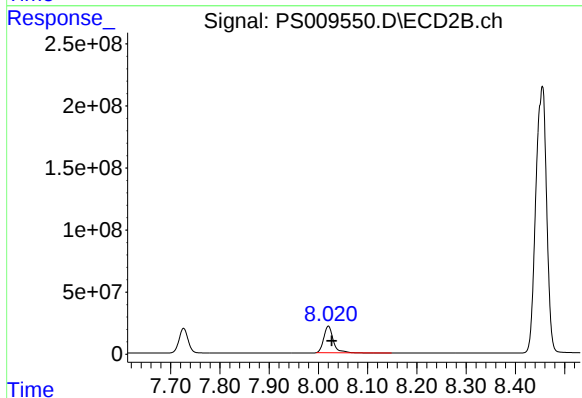


#9 2,4-D

R.T.: 8.020 min
Delta R.T.: -0.007 min
Response: 286738304
Conc: 436.20 ng/ml

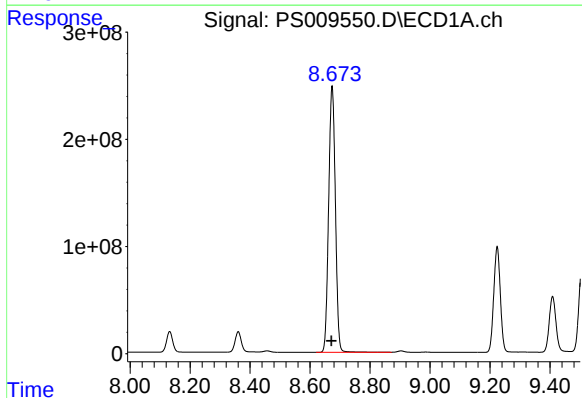


#10 Pentachlorophenol

R.T.: 8.674 min
Delta R.T.: 0.002 min
Response: 3888328194
Conc: 553.01 ng/ml

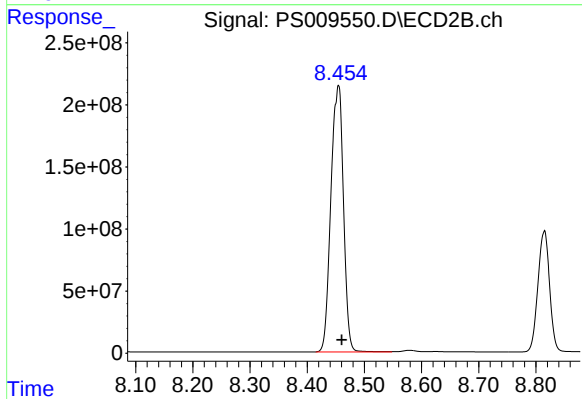

#10 Pentachlorophenol


R.T.: 8.453 min
Delta R.T.: -0.008 min
Response: 3284845663
Conc: 432.79 ng/ml

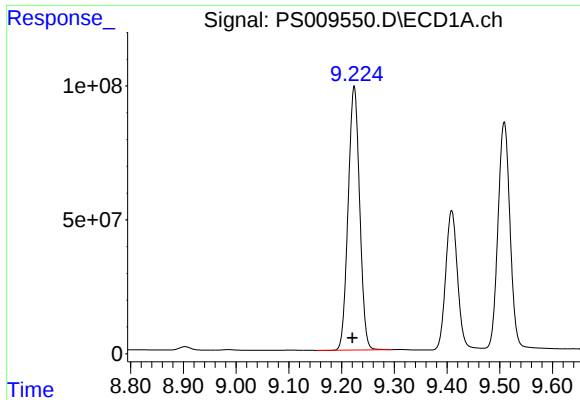

#11 2,4,5-TP (SILVEX)


R.T.: 9.224 min
Delta R.T.: 0.003 min
Response: 1492488016
Conc: 544.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

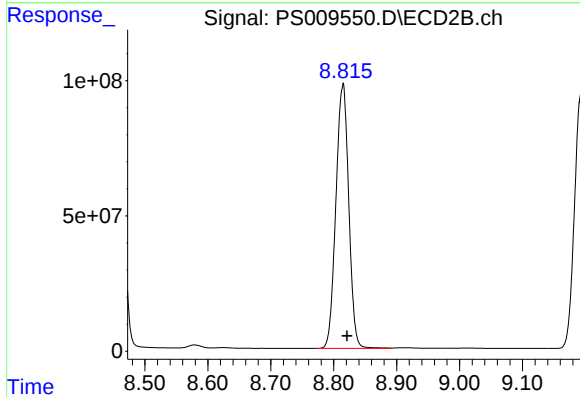


#11 2,4,5-TP (SILVEX)

R.T.: 8.814 min
Delta R.T.: -0.007 min
Response: 1385159860
Conc: 464.64 ng/ml

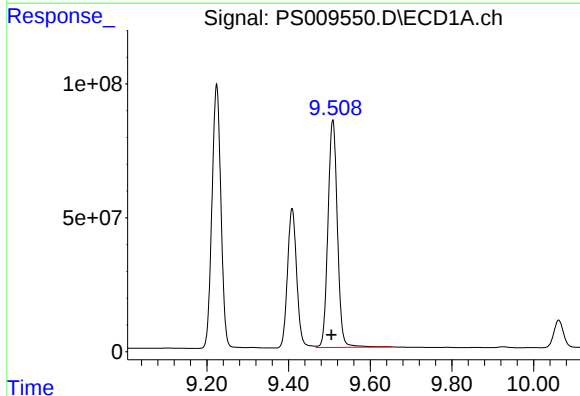


#12 2,4,5-T

R.T.: 9.508 min
Delta R.T.: 0.003 min
Response: 1362671854
Conc: 535.67 ng/ml

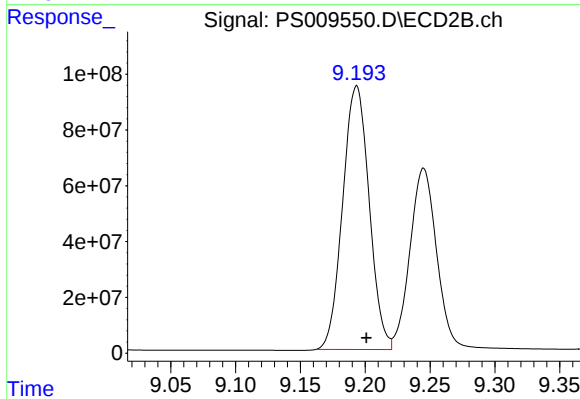

#12 2,4,5-T


R.T.: 9.193 min
Delta R.T.: -0.008 min
Response: 1344784680
Conc: 455.52 ng/ml

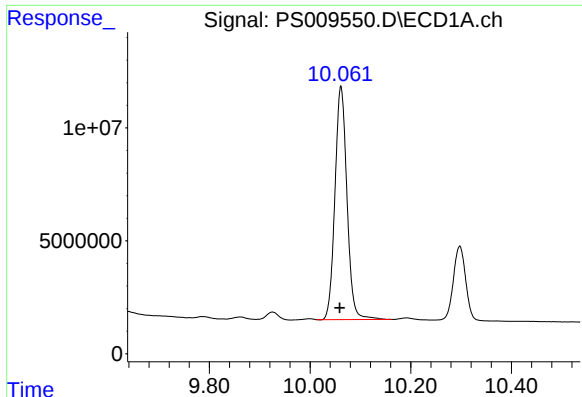

#13 2,4-DB


R.T.: 10.061 min
Delta R.T.: 0.003 min
Response: 171128877
Conc: 494.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

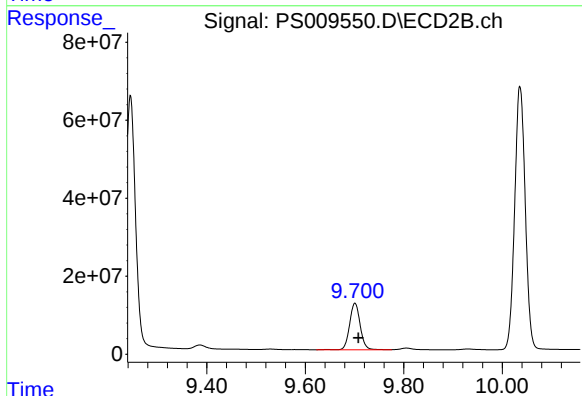


#13 2,4-DB

R.T.: 9.701 min
Delta R.T.: -0.007 min
Response: 178622153
Conc: 470.53 ng/ml

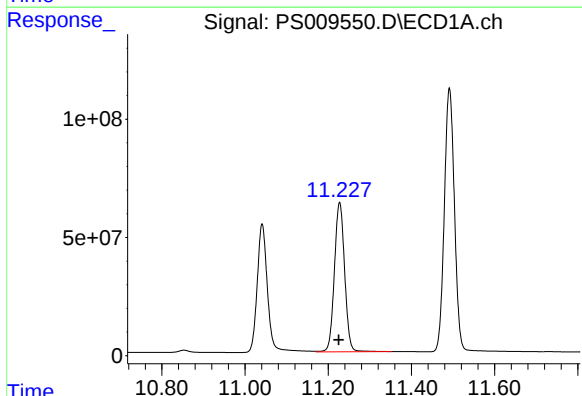


#14 DINOSEB

R.T.: 11.227 min
Delta R.T.: 0.002 min
Response: 1079429407
Conc: 528.06 ng/ml

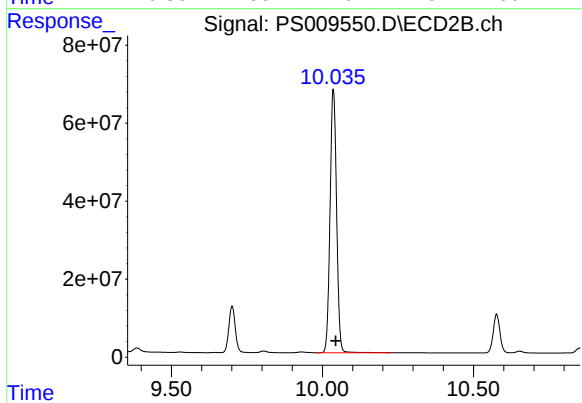

#14 DINOSEB


R.T.: 10.036 min
Delta R.T.: -0.007 min
Response: 1012489716
Conc: 460.96 ng/ml

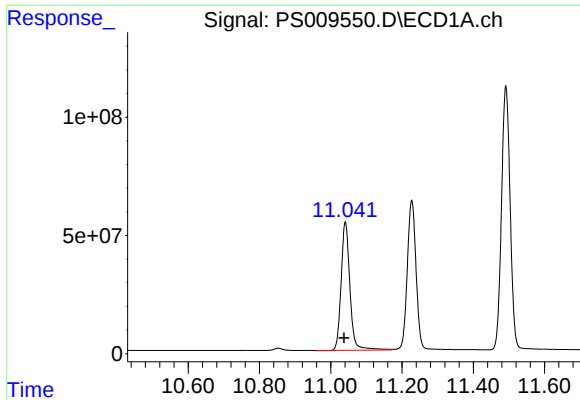

#15 Picloram


R.T.: 11.041 min
Delta R.T.: 0.004 min
Response: 931121192
Conc: 306.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

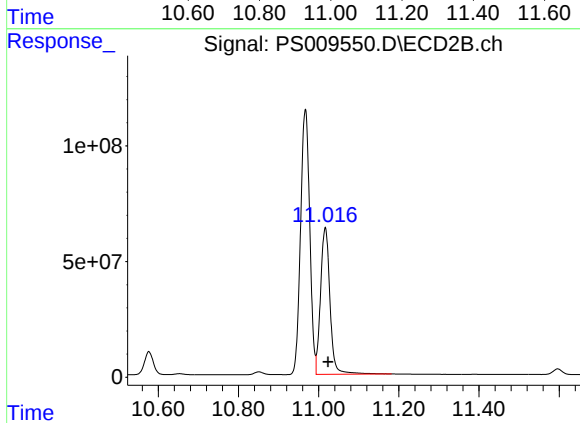


#15 Picloram

R.T.: 11.016 min
Delta R.T.: -0.007 min
Response: 1037600250
Conc: 254.80 ng/ml

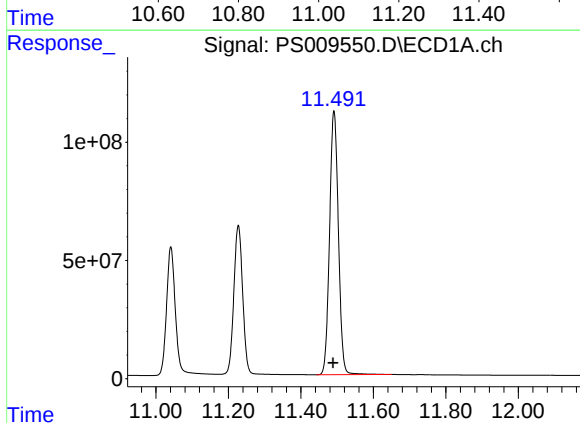

#16 DCPA

R.T.: 11.491 min
Delta R.T.: 0.002 min
Response: 1883207738
Conc: 543.30 ng/ml

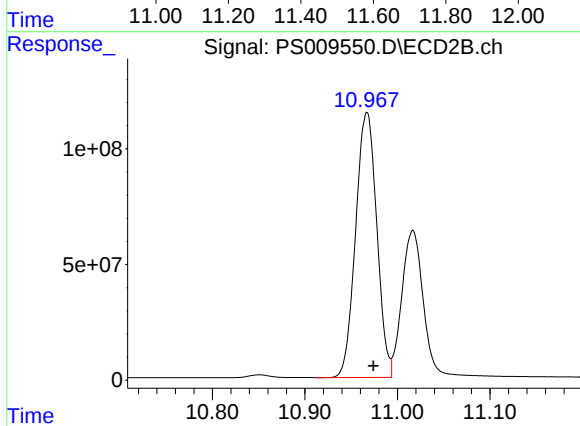

#16 DCPA

R.T.: 10.967 min
Delta R.T.: -0.007 min
Response: 1819582050
Conc: 469.81 ng/ml