

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040220\
 Data File : PS009552.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2020 17:49
 Operator : DD\AJ
 Sample : PB127979TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 03:27:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.241	6.930	333.5E6	317.1E6	602.951	577.369
Target Compounds							
1) T	Dalapon	3.001	2.587	16434445	109.6E6	21.074	139.236 #
2) T	3,5-DICHL...	0.000	6.107	0	27888229	N.D.	34.290
7) T	MCPA	7.792	0.000	34171581	0	11.220	N.D. #
8) T	DICHLORPROP	0.000	7.750	0	10301652	N.D.	18.567
10) T	Pentachlo...	8.727	0.000	7717050	0	1.098	N.D. #
11) T	2,4,5-TP ...	0.000	8.858	0	10221640	N.D.	3.429
12) T	2,4,5-T	9.448	0.000	24323384	0	9.562	N.D. #
13) T	2,4-DB	0.000	9.643	0	3737001	N.D.	9.844
14) T	DINOSEB	11.187	10.046	21842555	12870373	10.685	5.860 #
15) T	Picloram	0.000	11.022	0	4072138	N.D.	<MDL
16) T	DCPA	0.000	11.022	0	4072138	N.D.	1.051



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040220\
Data File : PS009552.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2020 17:49
Operator : DD\AJ
Sample : PB127979TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 03:27:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

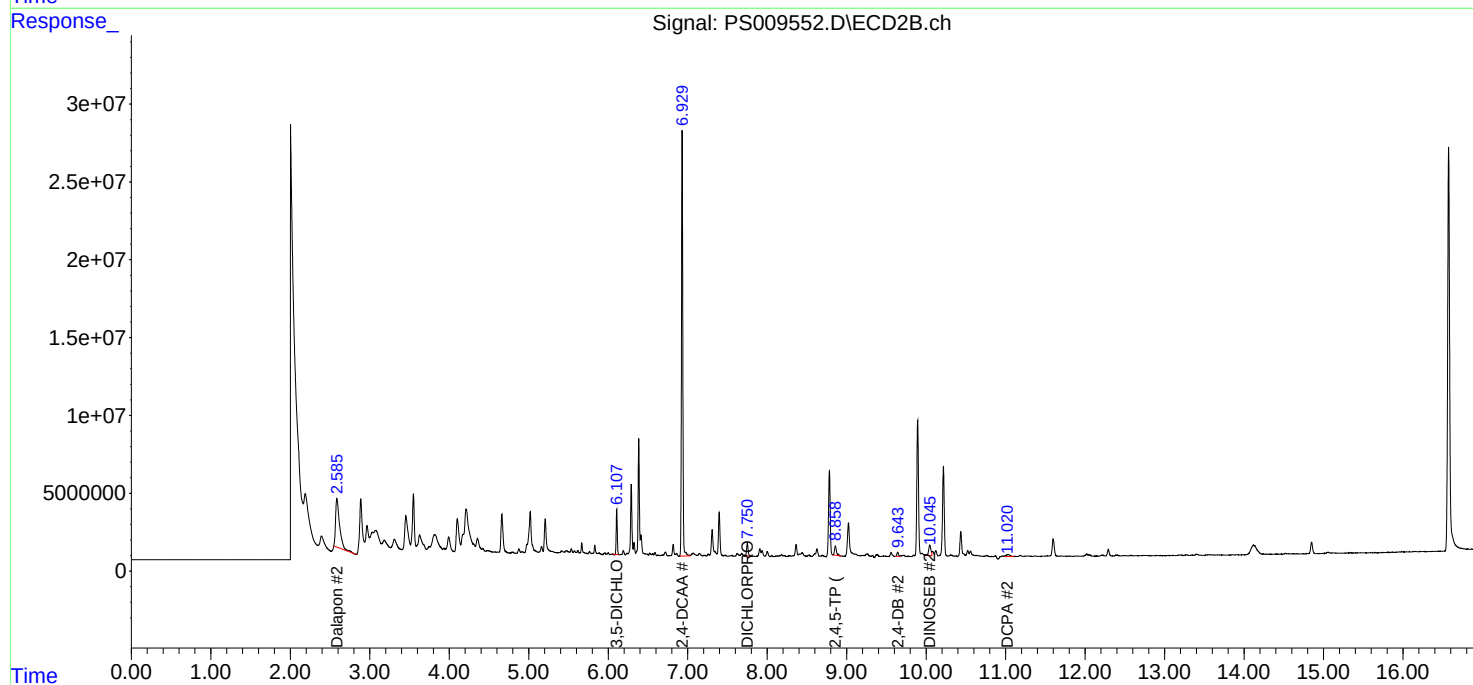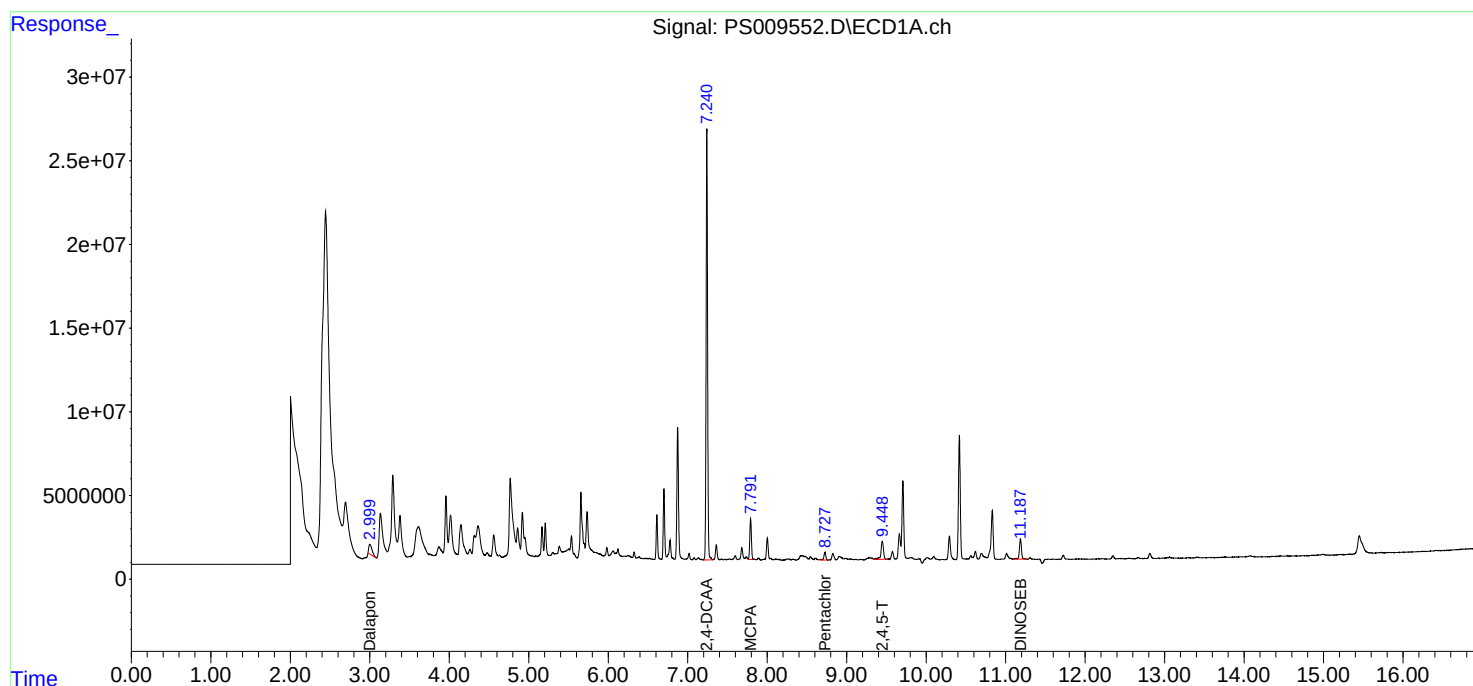


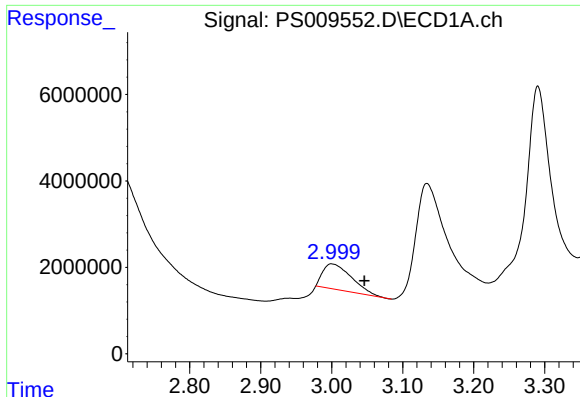

#1 Dalapon


R.T.: 3.001 min
Delta R.T.: -0.045 min
Response: 16434445
Conc: 21.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

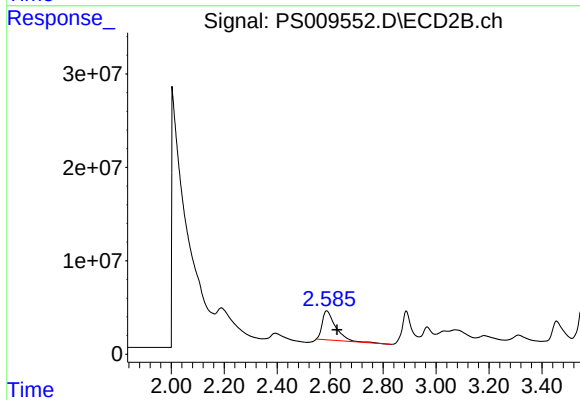


#1 Dalapon

R.T.: 2.587 min
Delta R.T.: -0.040 min
Response: 109628953
Conc: 139.24 ng/ml

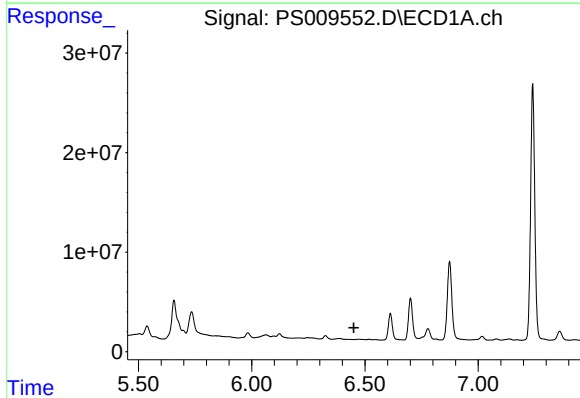


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

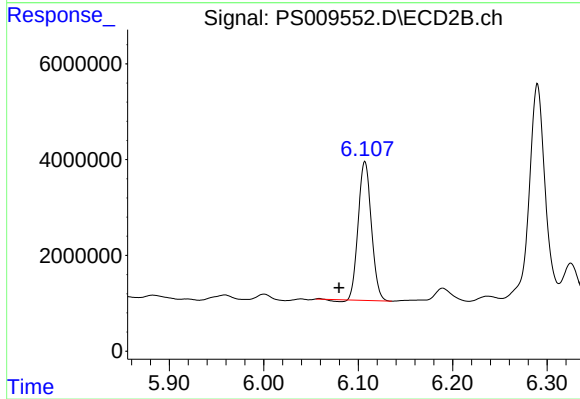

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.107 min
Delta R.T.: 0.027 min
Response: 27888229
Conc: 34.29 ng/ml

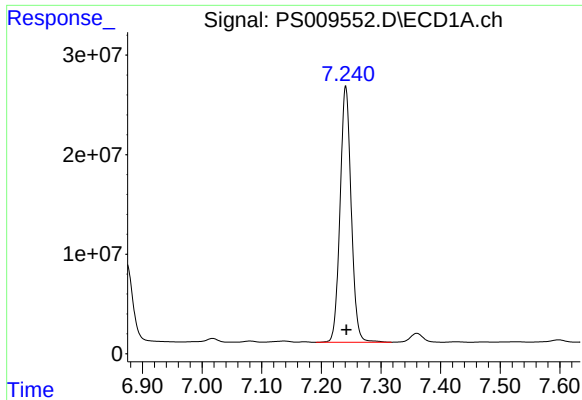

#4 2,4-DCAA


R.T.: 7.241 min
Delta R.T.: -0.001 min
Response: 333534345
Conc: 602.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

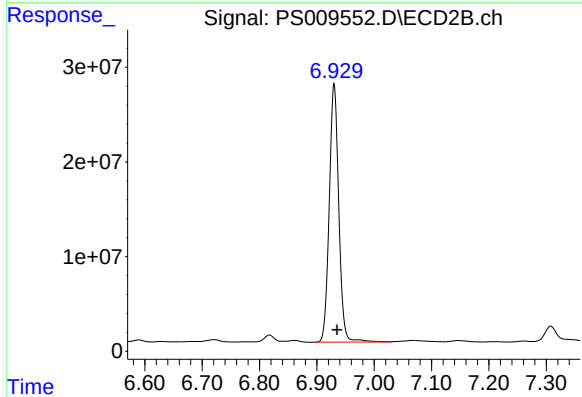


#4 2,4-DCAA

R.T.: 6.930 min
Delta R.T.: -0.005 min
Response: 317089530
Conc: 577.37 ng/ml

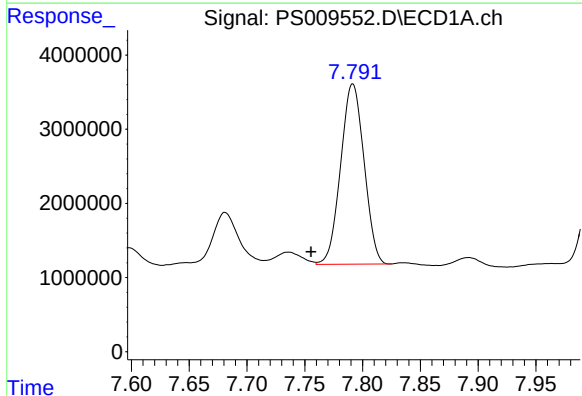


#7 MCPA

R.T.: 7.792 min
Delta R.T.: 0.036 min
Response: 34171581
Conc: 11.22 ug/ml

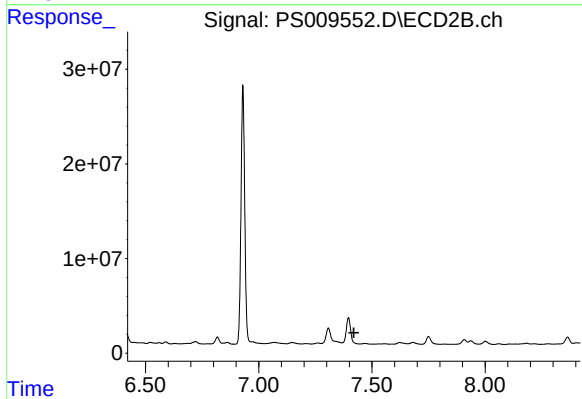

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.420 min
Response: 0
Conc: N.D.

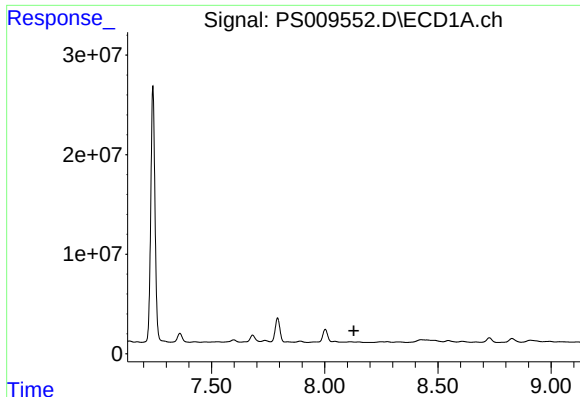

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

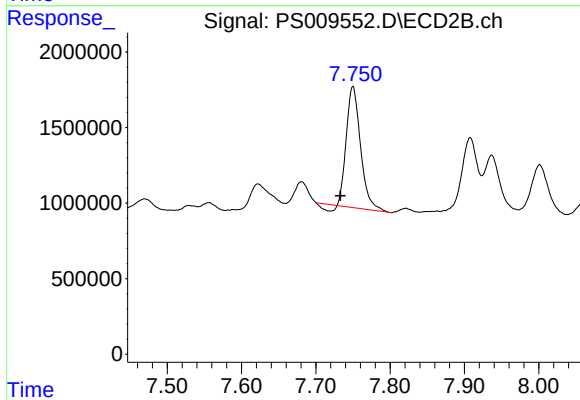


#8 DICHLORPROP

R.T.: 7.750 min
Delta R.T.: 0.017 min
Response: 10301652
Conc: 18.57 ng/ml

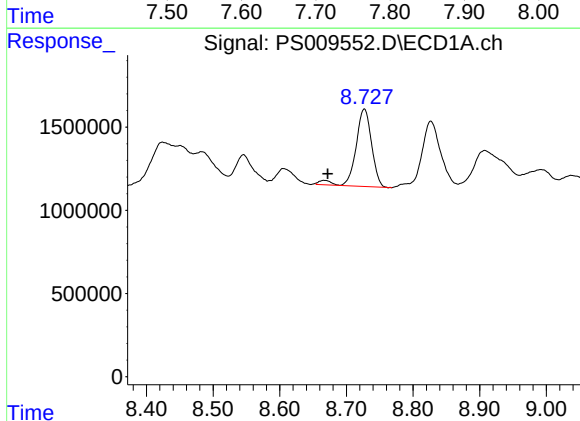


#10 Pentachlorophenol

R.T.: 8.727 min
Delta R.T.: 0.055 min
Response: 7717050
Conc: 1.10 ng/ml

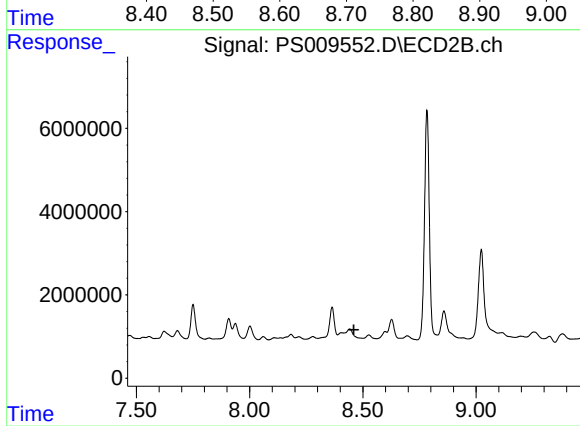

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 8.461 min
Response: 0
Conc: N.D.

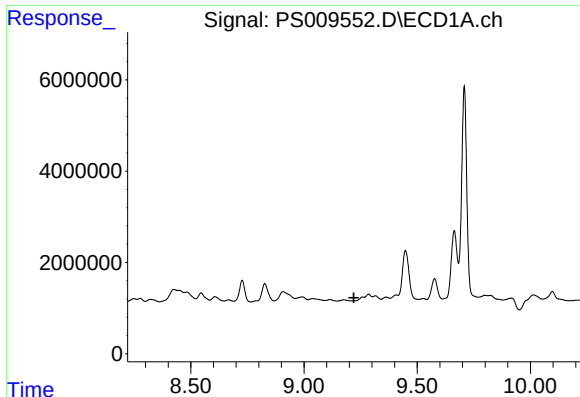

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.221 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

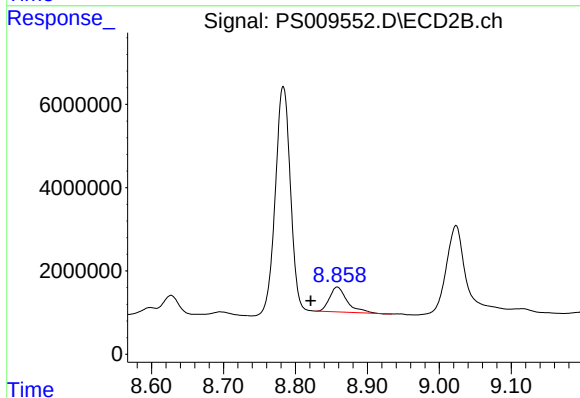


#11 2,4,5-TP (SILVEX)

R.T.: 8.858 min
Delta R.T.: 0.037 min
Response: 10221640
Conc: 3.43 ng/ml

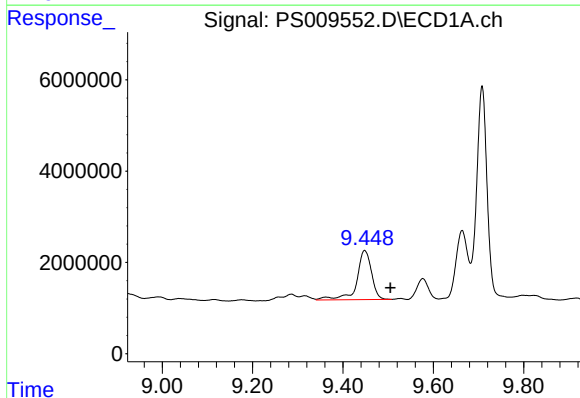


#12 2,4,5-T

R.T.: 9.448 min
Delta R.T.: -0.057 min
Response: 24323384
Conc: 9.56 ng/ml

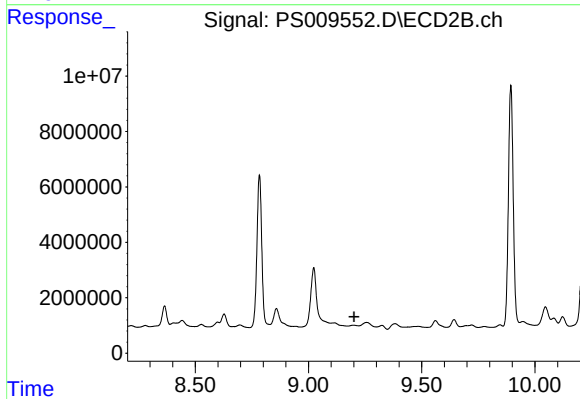

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.201 min
Response: 0
Conc: N.D.

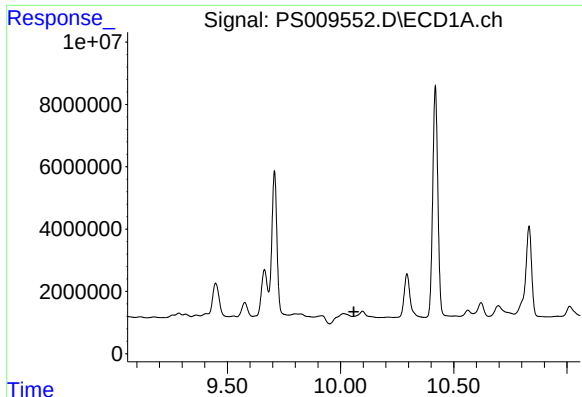

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.059 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

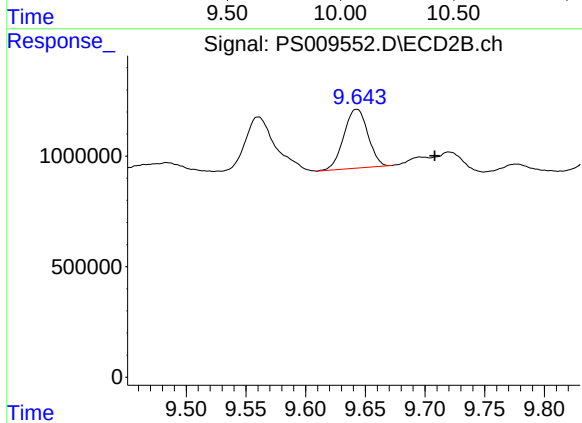


#13 2,4-DB

R.T.: 9.643 min
Delta R.T.: -0.065 min
Response: 3737001
Conc: 9.84 ng/ml

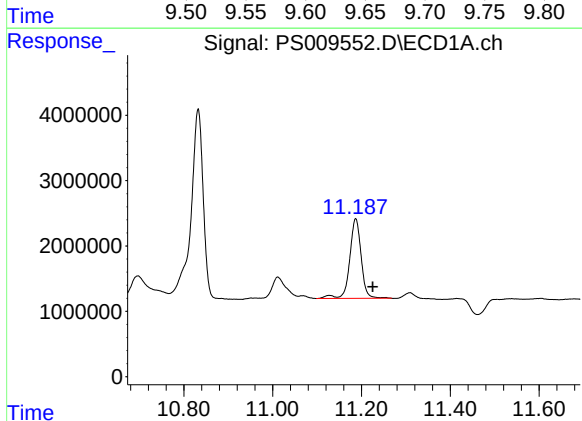


#14 DINOSEB

R.T.: 11.187 min
Delta R.T.: -0.038 min
Response: 21842555
Conc: 10.69 ng/ml

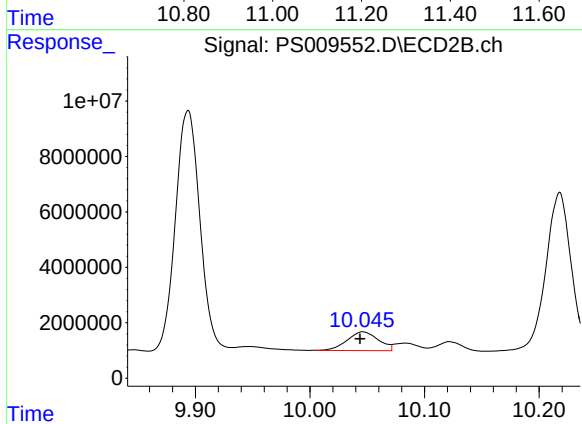

#14 DINOSEB


R.T.: 10.046 min
Delta R.T.: 0.003 min
Response: 12870373
Conc: 5.86 ng/ml

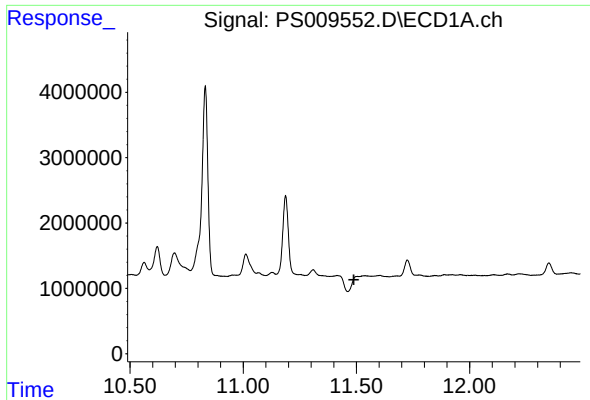

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

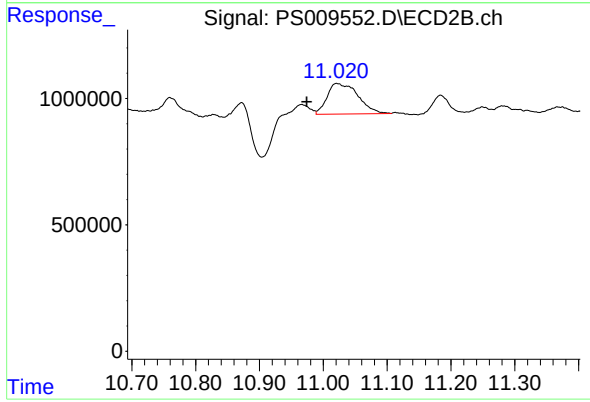

#16 DCPA

R.T.: 11.022 min
Delta R.T.: 0.047 min
Response: 4072138
Conc: 1.05 ng/ml