

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040220\
 Data File : PS009553.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2020 18:12
 Operator : DD\AJ
 Sample : L2101-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 03:27:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.241	6.930	182.6E6	167.6E6	330.174	305.224
Target Compounds							
1) T	Dalapon	2.999	2.588	19124500	130.4E6	24.524	165.585 #
2) T	3,5-DICHL...	0.000	6.107	0	68313045	N.D.	83.994
3) T	4-Nitroph...	7.129	6.586	10714968	5228973	44.886	16.433 #
5) T	DICAMBA	0.000	7.059	0	8567274	N.D.	3.732
7) T	MCPA	7.689	7.404	35360854	4725653	11.610	1.751 #
8) T	DICHLORPROP	0.000	7.749	0	15852014	N.D.	28.571
10) T	Pentachlo...	0.000	8.451	0	6276251	N.D.	<MDL
12) T	2,4,5-T	9.444	9.258	54830439	4236044	21.554	1.435 #
14) T	DINOSEB	11.186	10.047	18110895	5043187	8.860	2.296 #
15) T	Picloram	11.012	0.000	14526715	0	4.787	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040220\
Data File : PS009553.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2020 18:12
Operator : DD\AJ
Sample : L2101-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 03:27:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

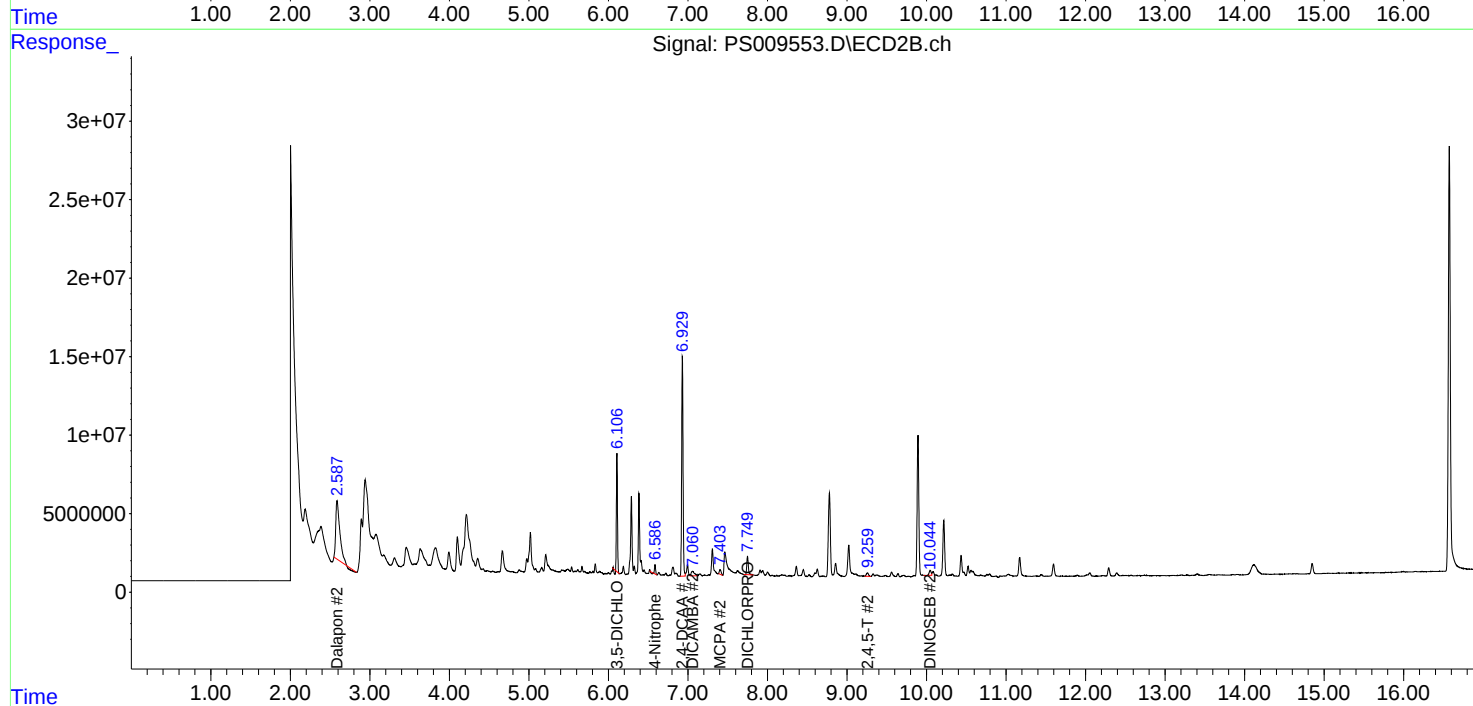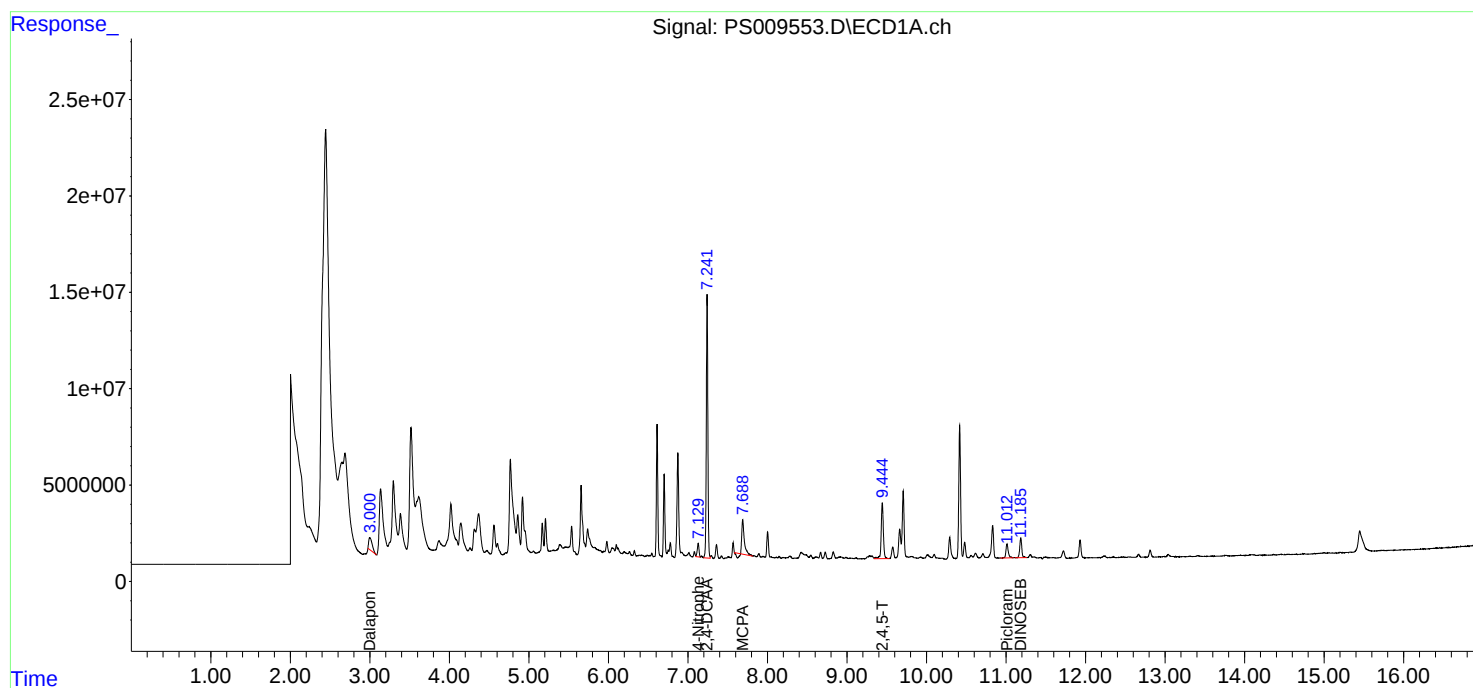


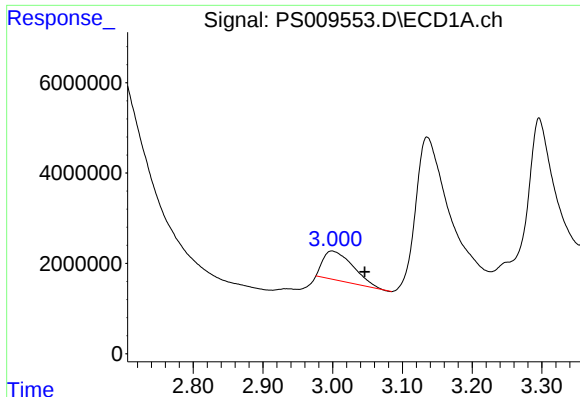

#1 Dalapon


R.T.: 2.999 min
Delta R.T.: -0.047 min
Response: 19124500
Conc: 24.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

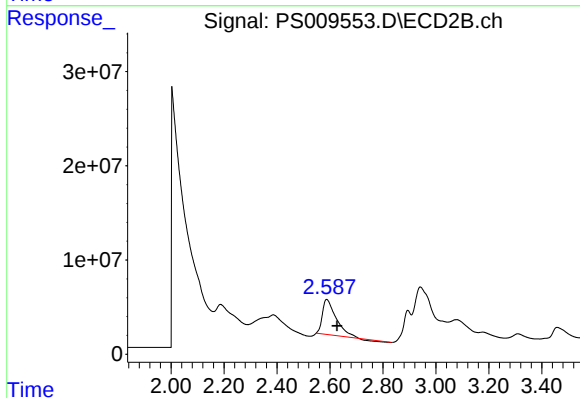


#1 Dalapon

R.T.: 2.588 min
Delta R.T.: -0.039 min
Response: 130375588
Conc: 165.59 ng/ml

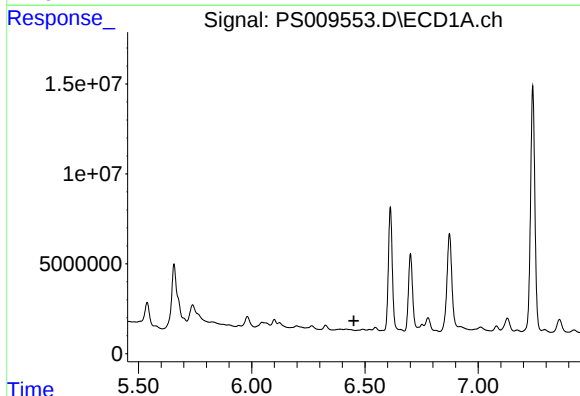


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

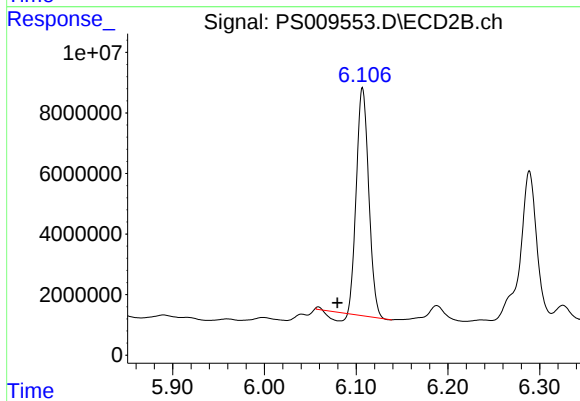

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.107 min
Delta R.T.: 0.027 min
Response: 68313045
Conc: 83.99 ng/ml

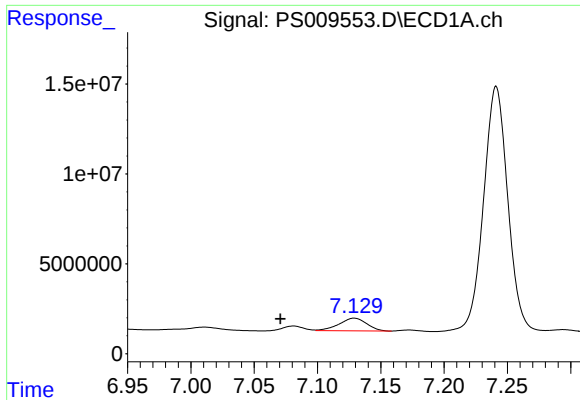

#3 4-Nitrophenol


R.T.: 7.129 min
Delta R.T.: 0.058 min
Response: 10714968
Conc: 44.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

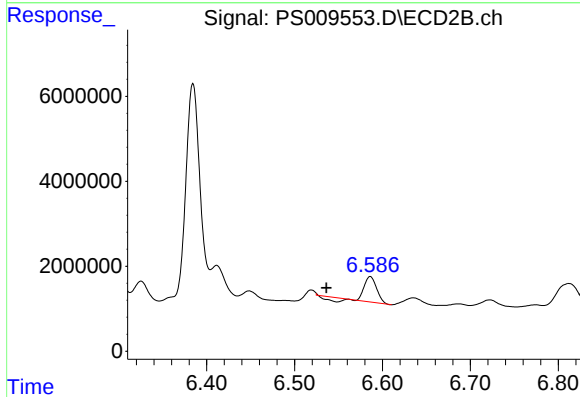


#3 4-Nitrophenol

R.T.: 6.586 min
Delta R.T.: 0.050 min
Response: 5228973
Conc: 16.43 ng/ml

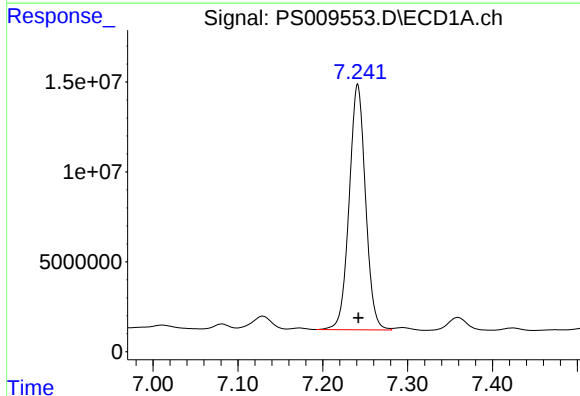


#4 2,4-DCAA

R.T.: 7.241 min
Delta R.T.: 0.000 min
Response: 182642266
Conc: 330.17 ng/ml

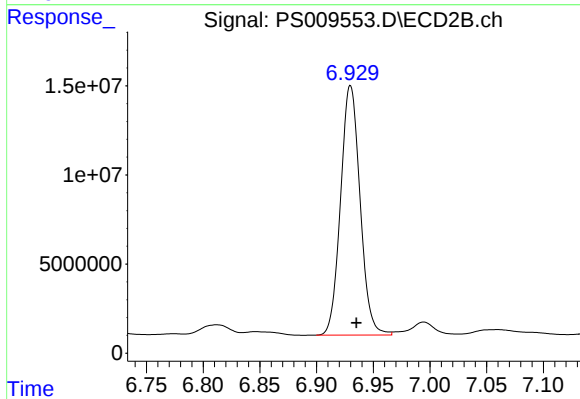

#4 2,4-DCAA


R.T.: 6.930 min
Delta R.T.: -0.005 min
Response: 167628116
Conc: 305.22 ng/ml

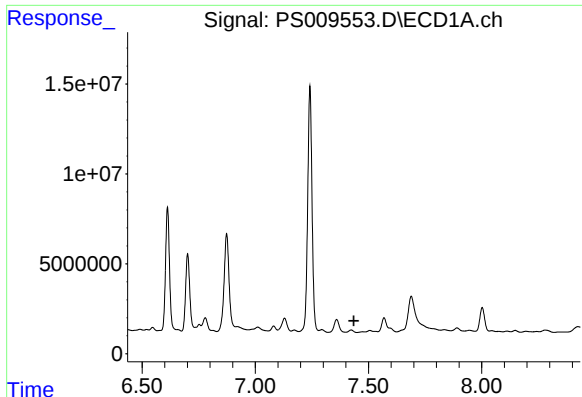

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.435 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

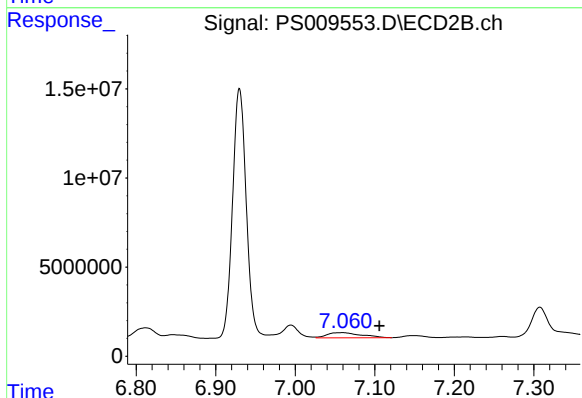


#5 DICAMBA

R.T.: 7.059 min
Delta R.T.: -0.047 min
Response: 8567274
Conc: 3.73 ng/ml

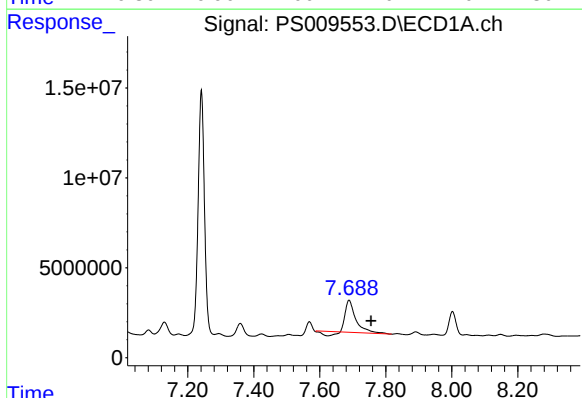


#7 MCPA

R.T.: 7.689 min
Delta R.T.: -0.067 min
Response: 35360854
Conc: 11.61 ug/ml

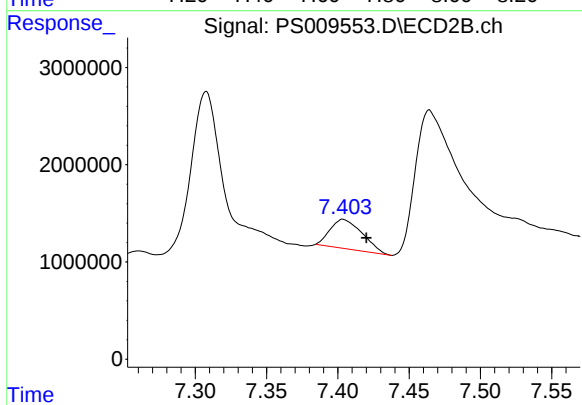

#7 MCPA


R.T.: 7.404 min
Delta R.T.: -0.016 min
Response: 4725653
Conc: 1.75 ug/ml

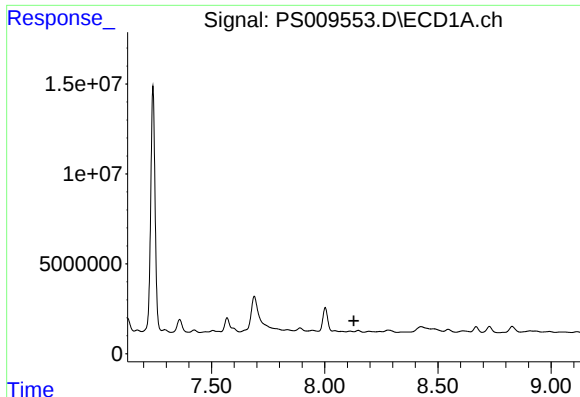

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

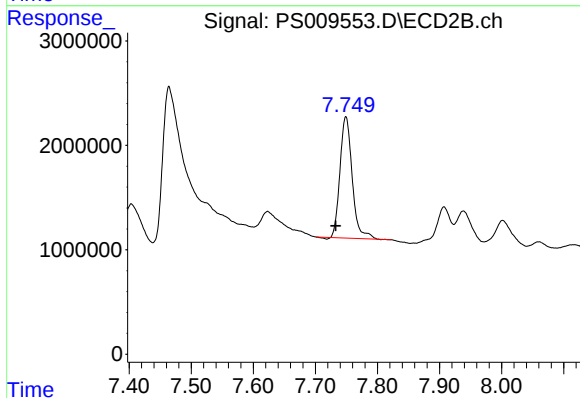


#8 DICHLORPROP

R.T.: 7.749 min
Delta R.T.: 0.016 min
Response: 15852014
Conc: 28.57 ng/ml

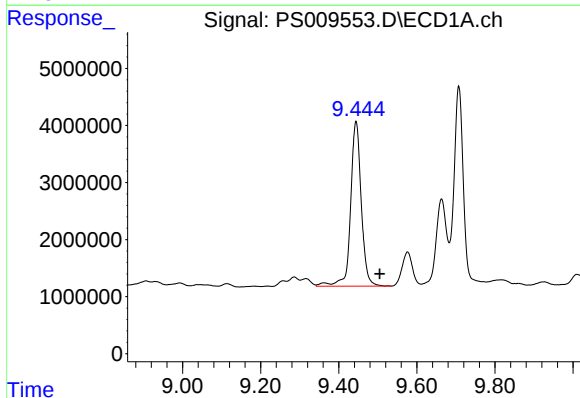


#12 2,4,5-T

R.T.: 9.444 min
Delta R.T.: -0.061 min
Response: 54830439
Conc: 21.55 ng/ml

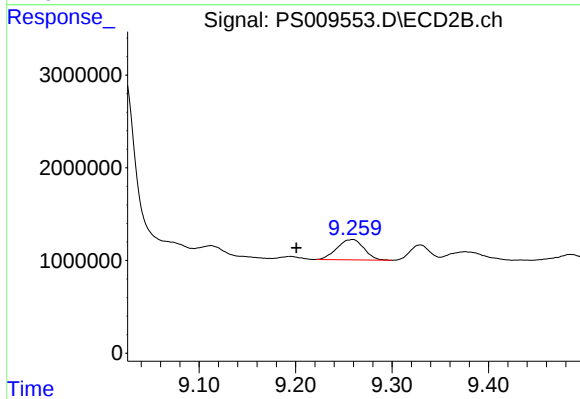

#12 2,4,5-T


R.T.: 9.258 min
Delta R.T.: 0.057 min
Response: 4236044
Conc: 1.43 ng/ml

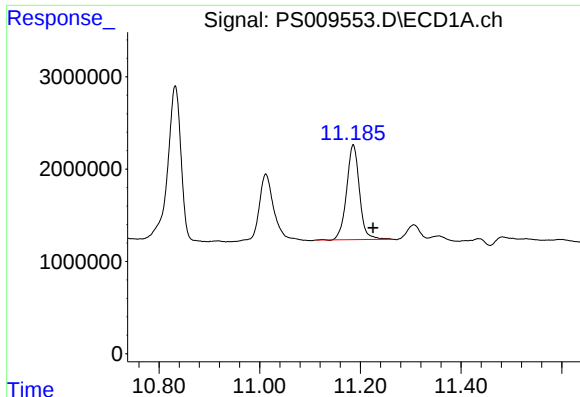

#14 DINOSEB


R.T.: 11.186 min
Delta R.T.: -0.039 min
Response: 18110895
Conc: 8.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

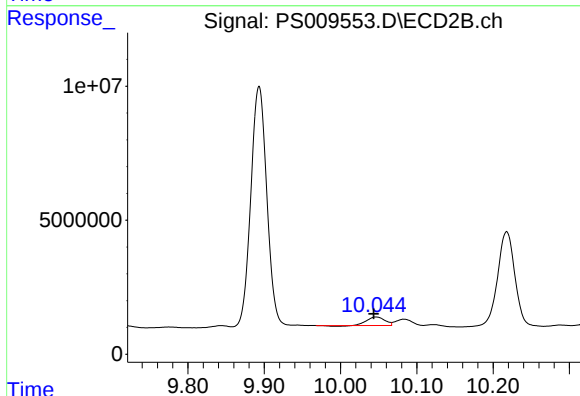


#14 DINOSEB

R.T.: 10.047 min
Delta R.T.: 0.003 min
Response: 5043187
Conc: 2.30 ng/ml

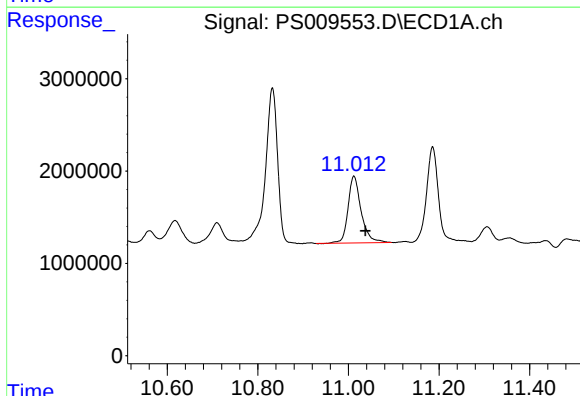

#15 Picloram

R.T.: 11.012 min
Delta R.T.: -0.025 min
Response: 14526715
Conc: 4.79 ng/ml

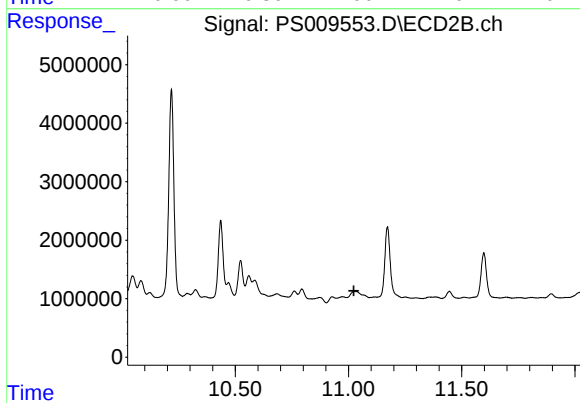

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.023 min
Response: 0
Conc: N.D.