

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040220\
 Data File : PS009557.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2020 19:44
 Operator : DD\AJ
 Sample : L2101-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 03:28:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.240	6.930	197.9E6	172.1E6	357.704	313.299
Target Compounds							
1) T	Dalapon	3.001	2.588	20280253	95916463	26.006	121.820 #
2) T	3,5-DICHL...	0.000	6.107	0	54830670	N.D.	67.417
3) T	4-Nitroph...	7.128	6.586	14429074	5744632	60.445	18.054 #
7) T	MCPA	7.690	7.466	28061615	31425268	9.214	11.645 #
8) T	DICHLORPROP	0.000	7.749	0	10354995	N.D.	18.664
12) T	2,4,5-T	9.444	0.000	51248472	0	20.146	N.D. #
13) T	2,4-DB	0.000	9.642	0	4255163	N.D.	11.209
14) T	DINOSEB	11.186	10.082	25680838	56559726	12.563	25.750 #
15) T	Picloram	11.013	0.000	17300339	0	5.700	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040220\
Data File : PS009557.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2020 19:44
Operator : DD\AJ
Sample : L2101-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 03:28:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

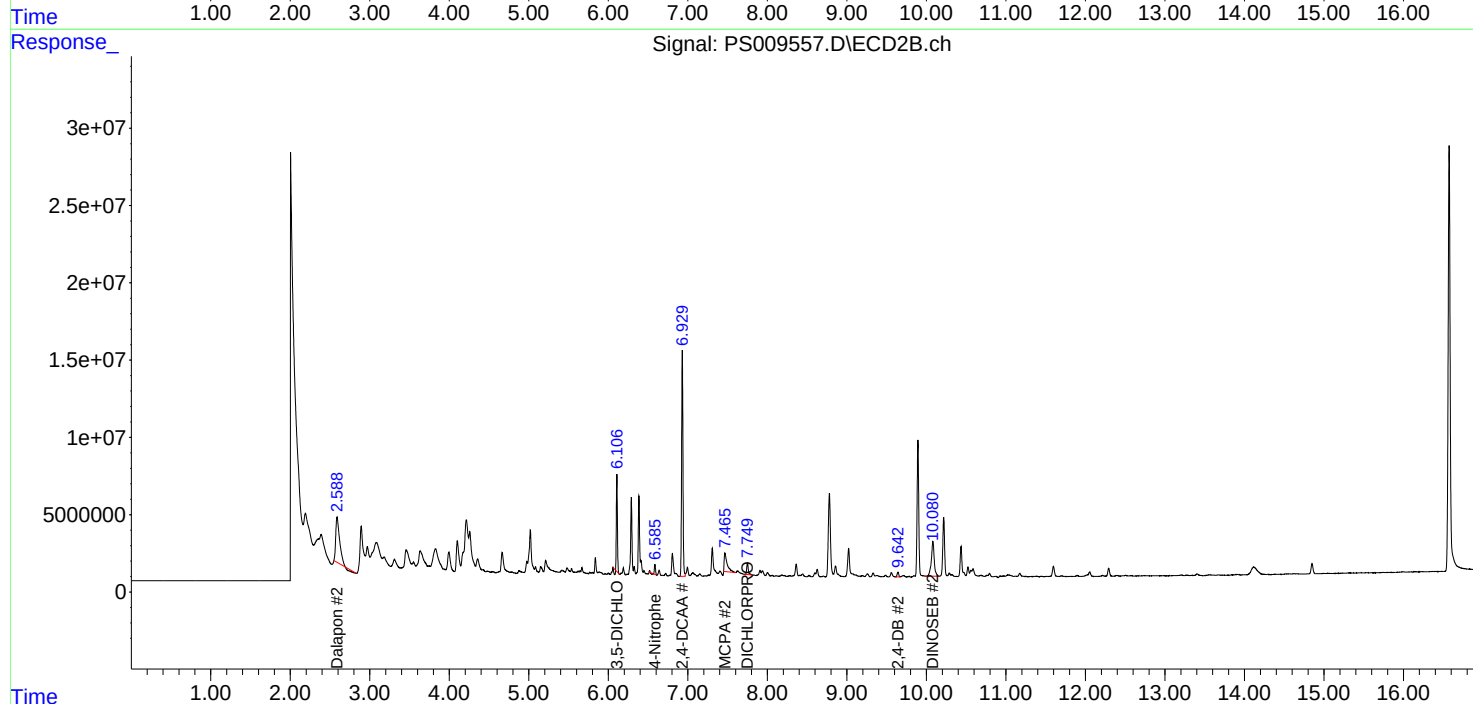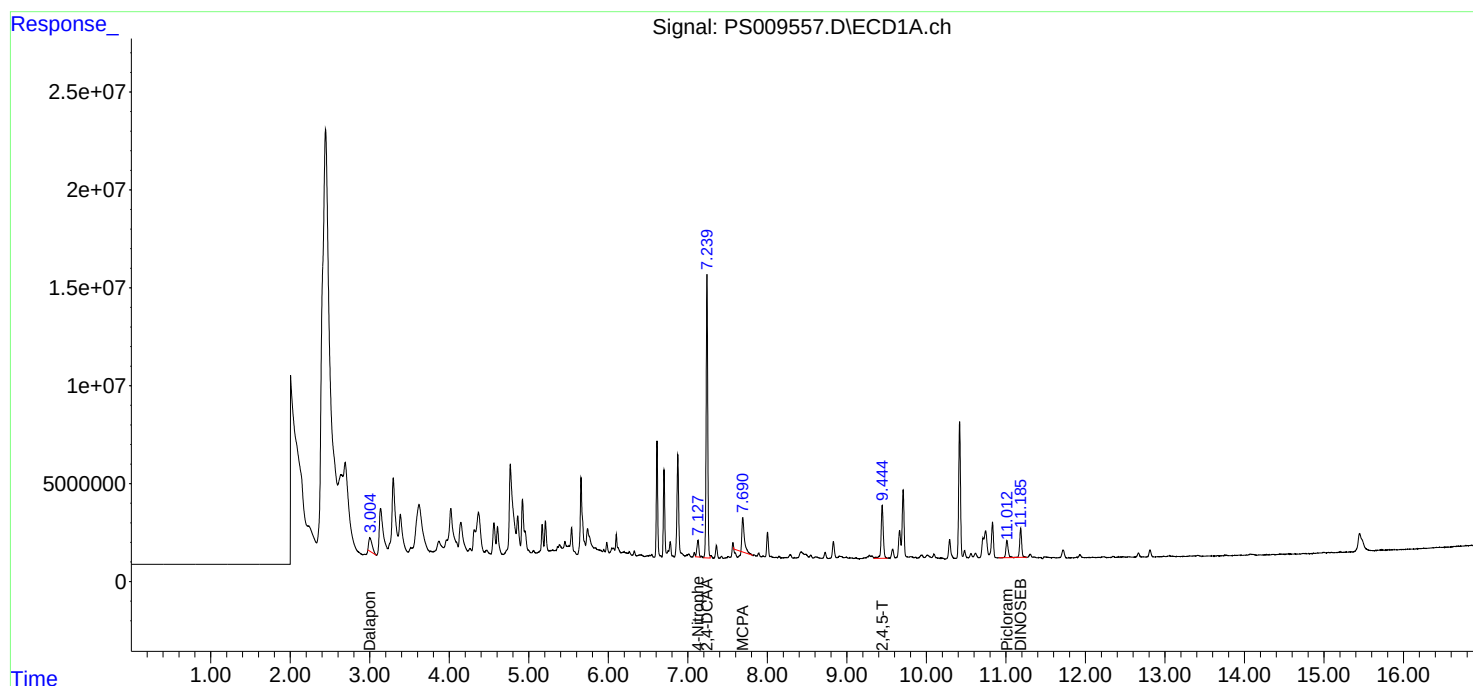


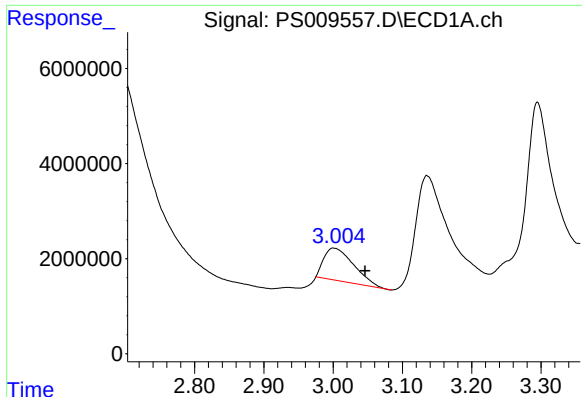

#1 Dalapon


R.T.: 3.001 min
Delta R.T.: -0.045 min
Response: 20280253
Conc: 26.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

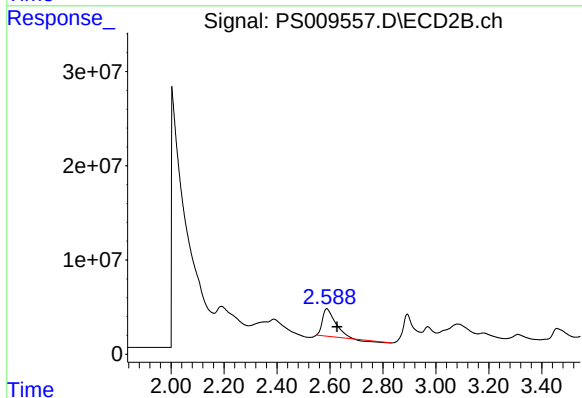


#1 Dalapon

R.T.: 2.588 min
Delta R.T.: -0.038 min
Response: 95916463
Conc: 121.82 ng/ml

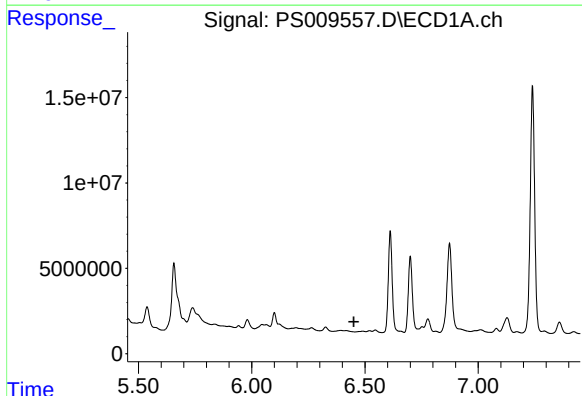


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

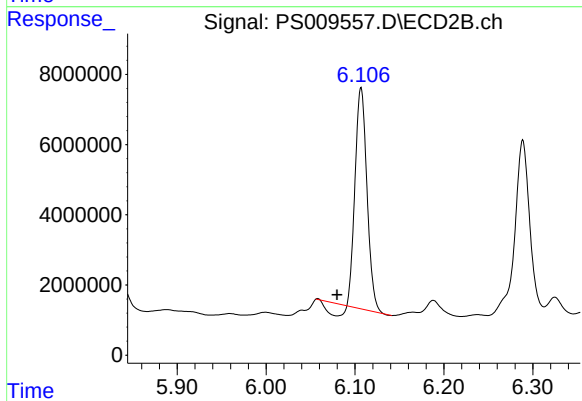

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.107 min
Delta R.T.: 0.027 min
Response: 54830670
Conc: 67.42 ng/ml

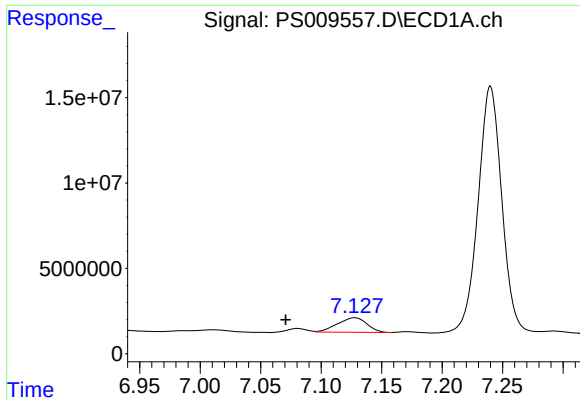

#3 4-Nitrophenol


R.T.: 7.128 min
Delta R.T.: 0.057 min
Response: 14429074
Conc: 60.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

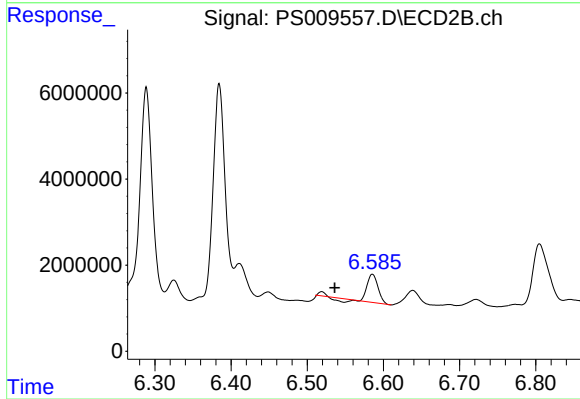


#3 4-Nitrophenol

R.T.: 6.586 min
Delta R.T.: 0.049 min
Response: 5744632
Conc: 18.05 ng/ml

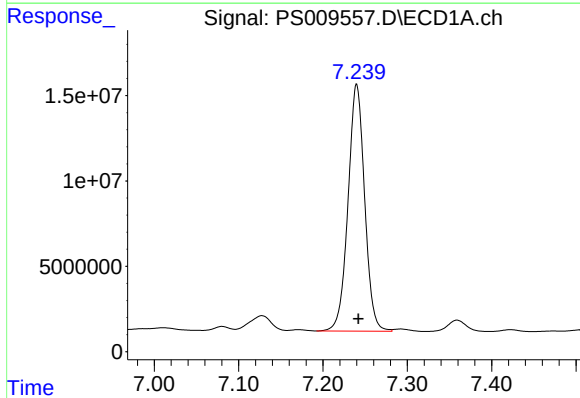


#4 2,4-DCAA

R.T.: 7.240 min
Delta R.T.: -0.002 min
Response: 197870986
Conc: 357.70 ng/ml

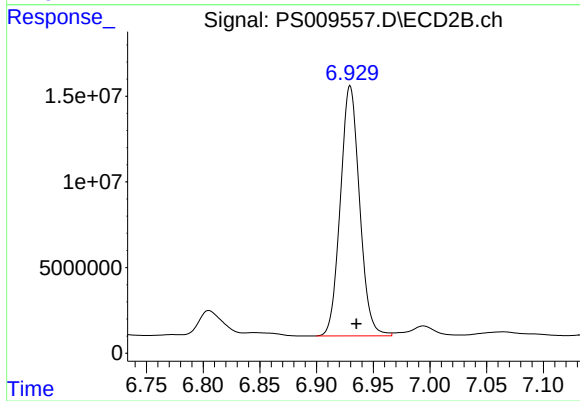

#4 2,4-DCAA


R.T.: 6.930 min
Delta R.T.: -0.005 min
Response: 172062967
Conc: 313.30 ng/ml

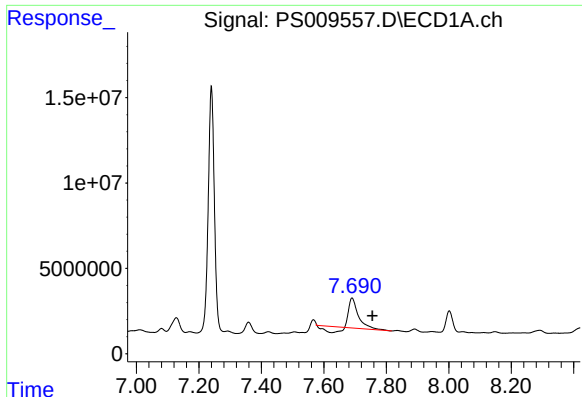

#7 MCPA


R.T.: 7.690 min
Delta R.T.: -0.065 min
Response: 28061615
Conc: 9.21 ug/ml

Instrument :
ECD_S
ClientSampleId :

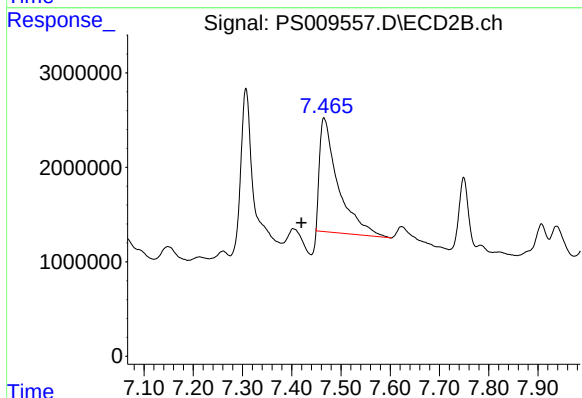


#7 MCPA

R.T.: 7.466 min
Delta R.T.: 0.046 min
Response: 31425268
Conc: 11.64 ug/ml

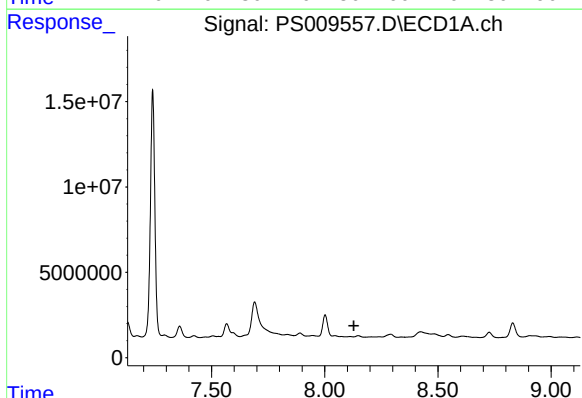


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.129 min
Response: 0
Conc: N.D.

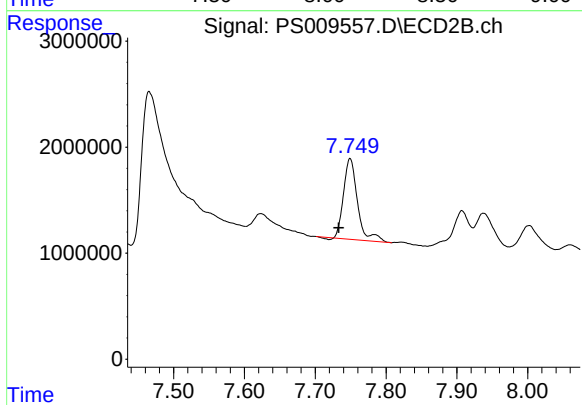

#8 DICHLORPROP


R.T.: 7.749 min
Delta R.T.: 0.016 min
Response: 10354995
Conc: 18.66 ng/ml

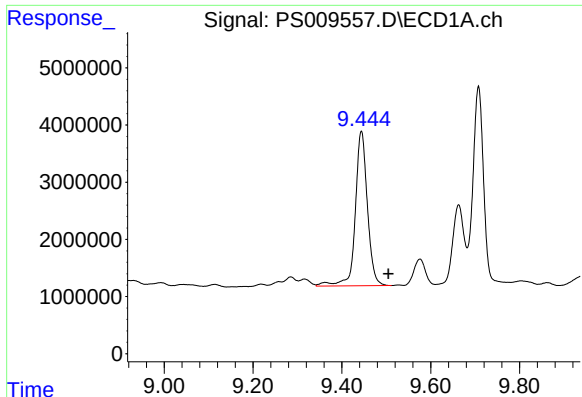

#12 2,4,5-T


R.T.: 9.444 min
Delta R.T.: -0.061 min
Response: 51248472
Conc: 20.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

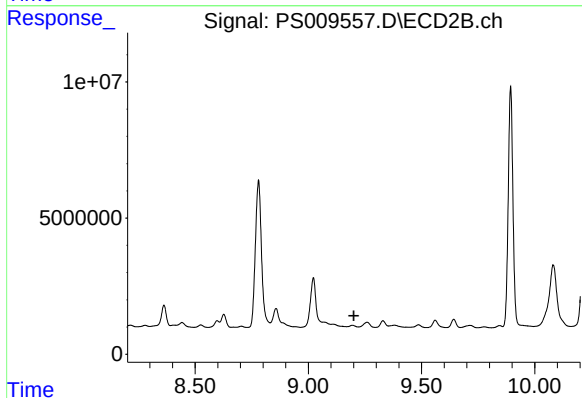


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.201 min
Response: 0
Conc: N.D.

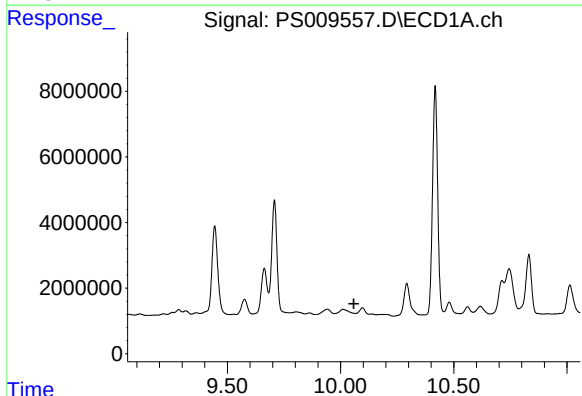


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.059 min
Response: 0
Conc: N.D.

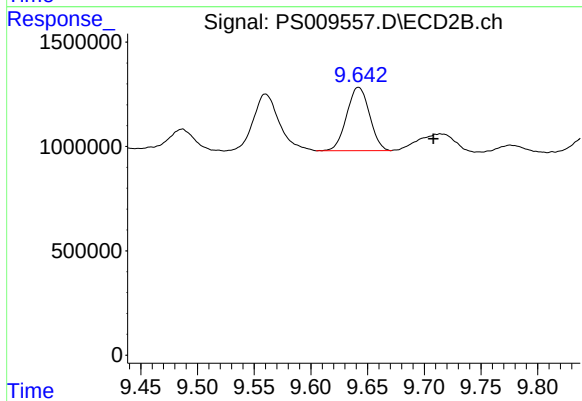

#13 2,4-DB


R.T.: 9.642 min
Delta R.T.: -0.066 min
Response: 4255163
Conc: 11.21 ng/ml

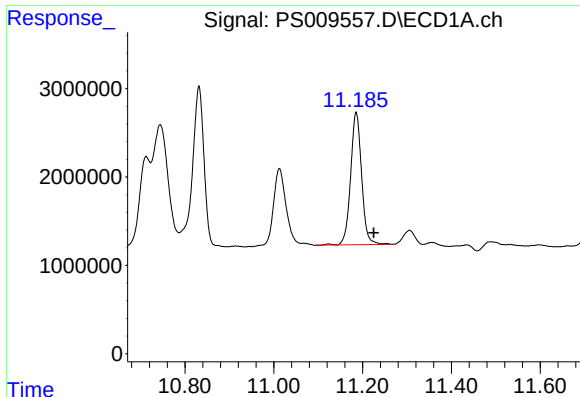

#14 DINOSEB


R.T.: 11.186 min
Delta R.T.: -0.040 min
Response: 25680838
Conc: 12.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

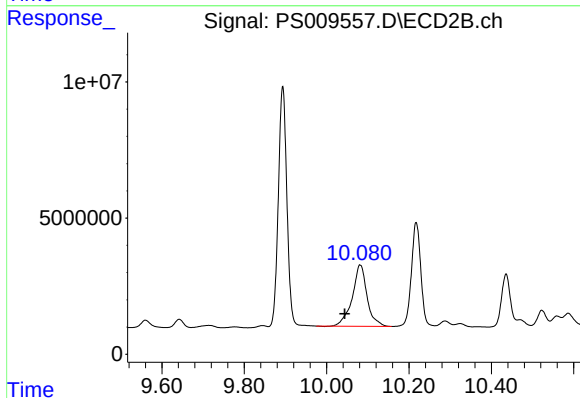


#14 DINOSEB

R.T.: 10.082 min
Delta R.T.: 0.038 min
Response: 56559726
Conc: 25.75 ng/ml

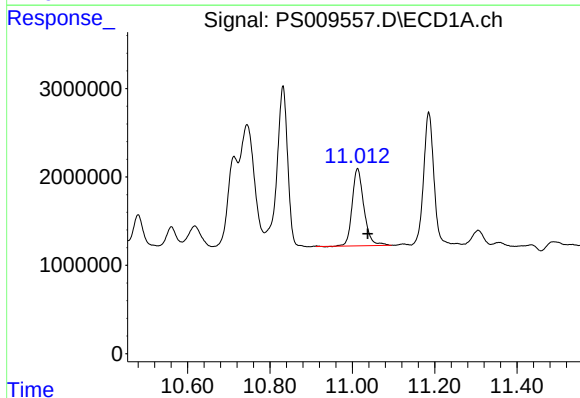

#15 Picloram

R.T.: 11.013 min
Delta R.T.: -0.025 min
Response: 17300339
Conc: 5.70 ng/ml

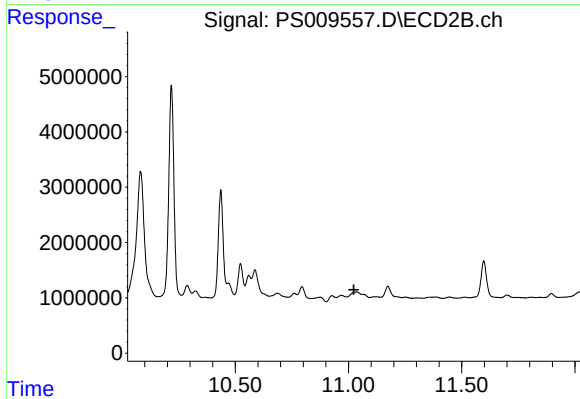

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.023 min
Response: 0
Conc: N.D.