

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040220\
 Data File : PS009558.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2020 20:07
 Operator : DD\AJ
 Sample : L2103-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 03:29:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.240	6.929	182.5E6	153.2E6	329.853	278.992
Target Compounds							
1) T	Dalapon	3.002	2.588	17142212	59149851	21.982	75.124 #
2) T	3,5-DICHL...	0.000	6.106	0	52224536	N.D.	64.213
3) T	4-Nitroph...	7.121	6.586	11846828	3363792	49.628	10.571 #
6) T	MCP	7.567	0.000	457433	0	<MDL	N.D. #
7) T	MCPA	7.691	7.468	39242603	37956625	12.885	14.065
8) T	DICHLORPROP	0.000	7.749	0	9317904	N.D.	16.794
12) T	2,4,5-T	9.444	9.261	39673505	4436799	15.596	1.503 #
13) T	2,4-DB	0.000	9.642	0	3441572	N.D.	9.066
14) T	DINOSEB	11.186	10.081	15009874	66417677	7.343	30.238 #
15) T	Picloram	11.012	0.000	13492759	0	4.446	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040220\
Data File : PS009558.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2020 20:07
Operator : DD\AJ
Sample : L2103-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 03:29:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

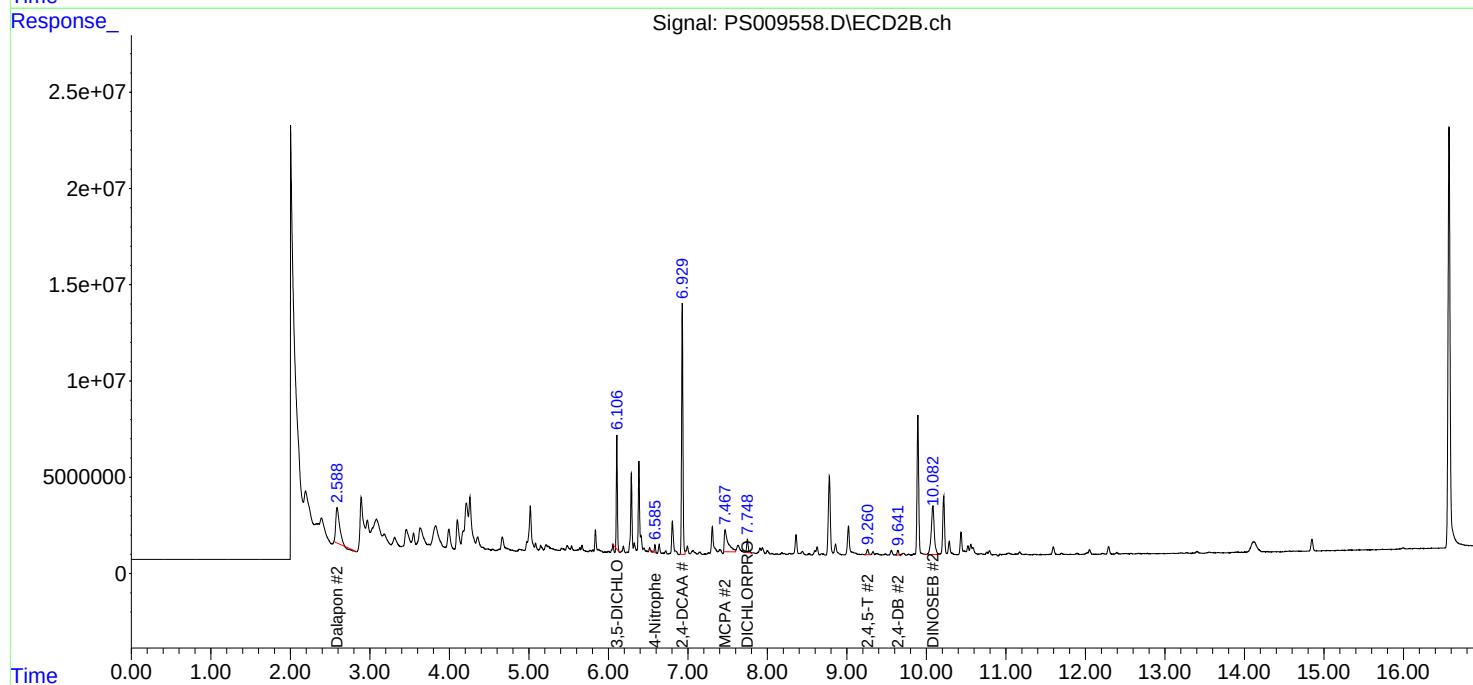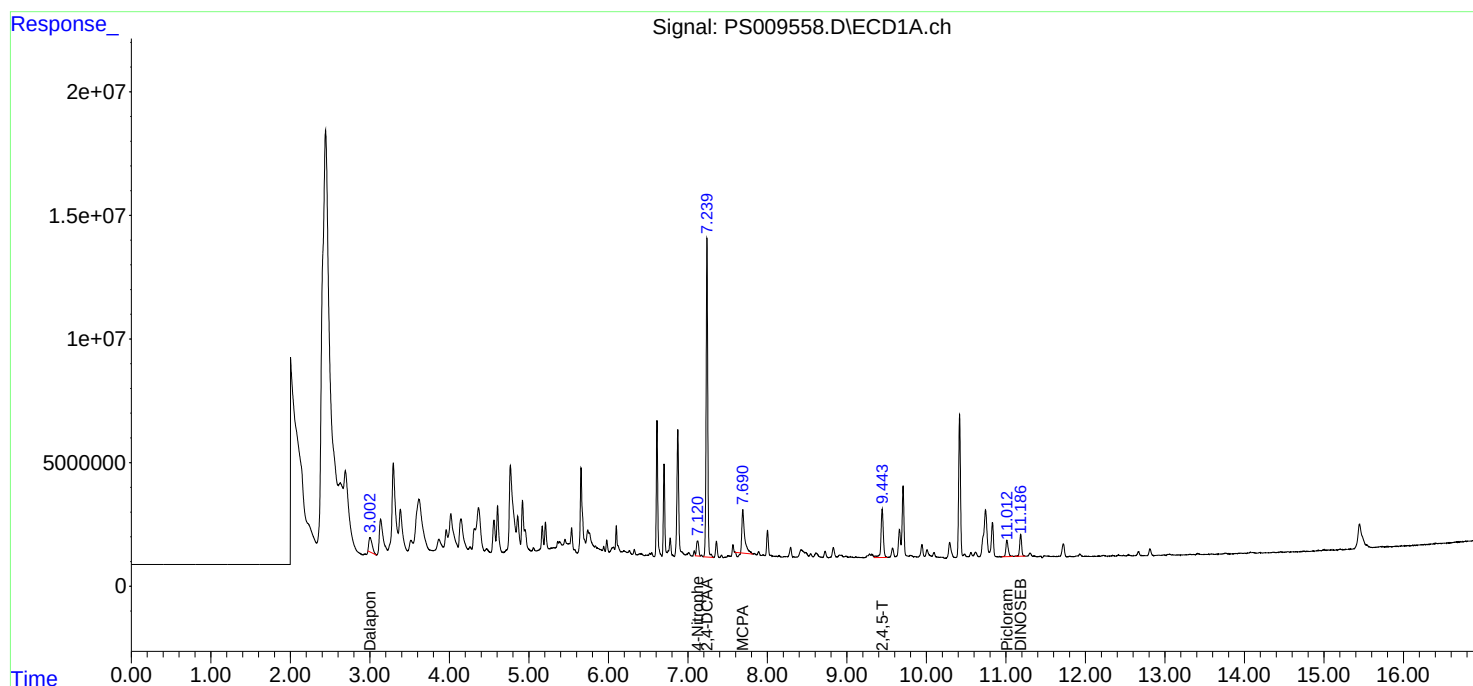


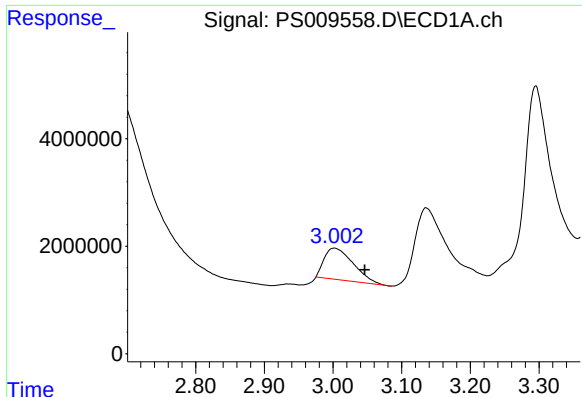

#1 Dalapon


R.T.: 3.002 min
Delta R.T.: -0.044 min
Response: 17142212
Conc: 21.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

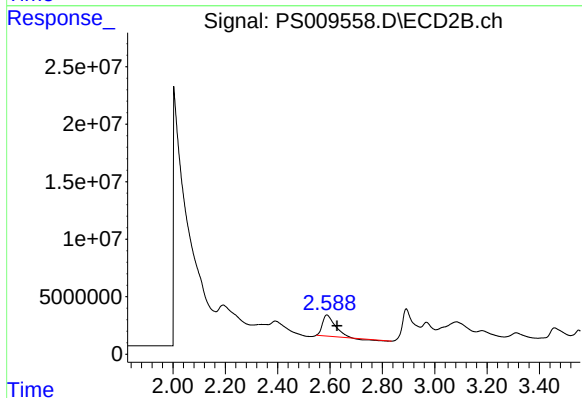


#1 Dalapon

R.T.: 2.588 min
Delta R.T.: -0.038 min
Response: 59149851
Conc: 75.12 ng/ml

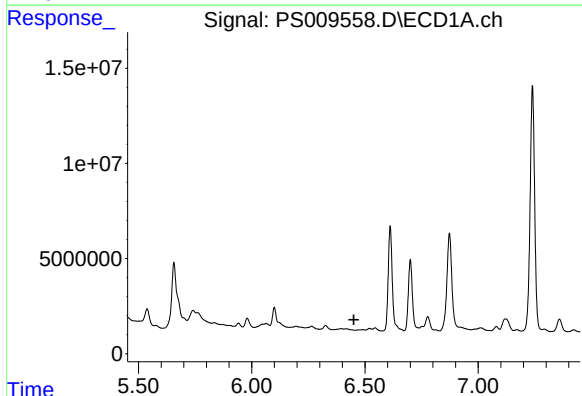


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

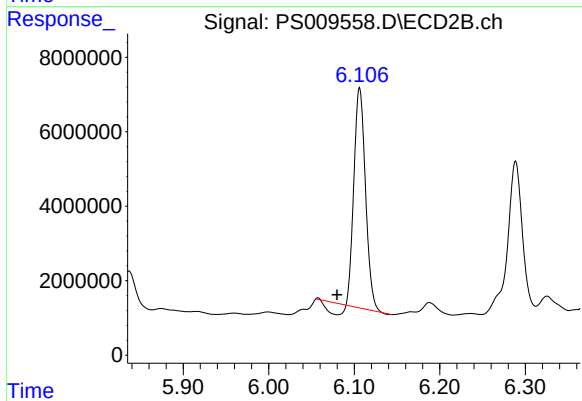

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.106 min
Delta R.T.: 0.027 min
Response: 52224536
Conc: 64.21 ng/ml

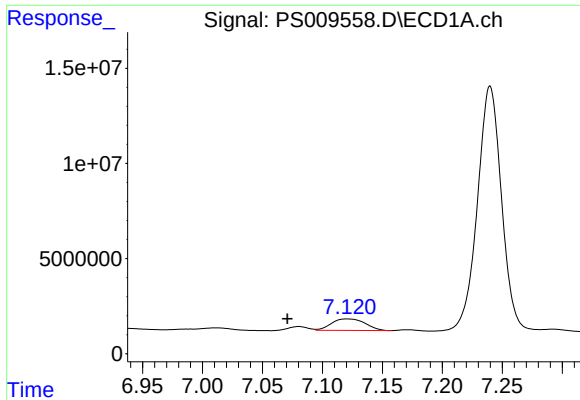

#3 4-Nitrophenol


R.T.: 7.121 min
Delta R.T.: 0.050 min
Response: 11846828
Conc: 49.63 ng/ml

Instrument :
ECD_S
ClientSampleId :

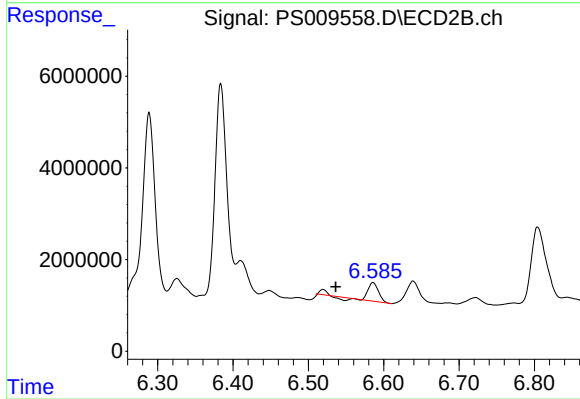


#3 4-Nitrophenol

R.T.: 6.586 min
Delta R.T.: 0.050 min
Response: 3363792
Conc: 10.57 ng/ml

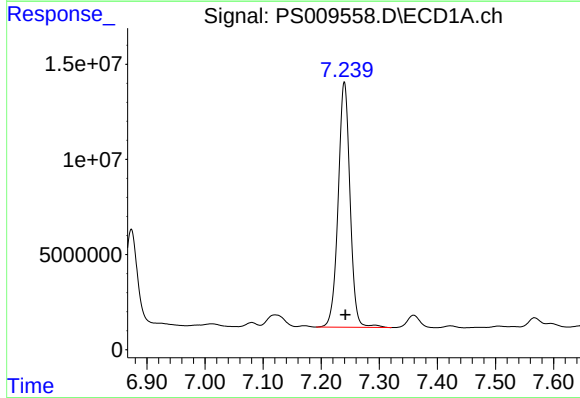


#4 2,4-DCAA

R.T.: 7.240 min
Delta R.T.: -0.002 min
Response: 182464563
Conc: 329.85 ng/ml

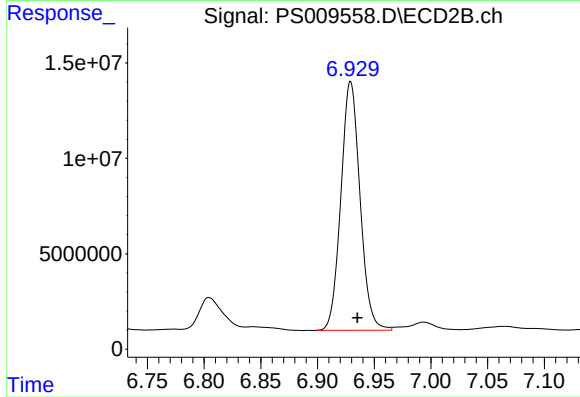

#4 2,4-DCAA


R.T.: 6.929 min
Delta R.T.: -0.006 min
Response: 153221498
Conc: 278.99 ng/ml

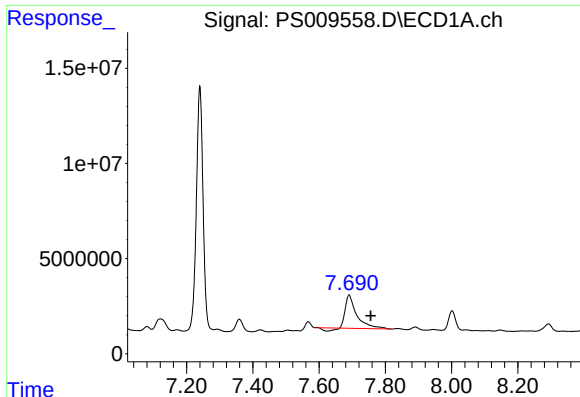

#7 MCPA


R.T.: 7.691 min
Delta R.T.: -0.065 min
Response: 39242603
Conc: 12.88 ug/ml

Instrument :
ECD_S
ClientSampleId :

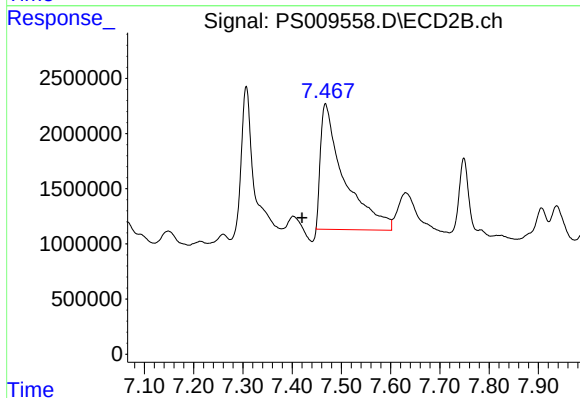


#7 MCPA

R.T.: 7.468 min
Delta R.T.: 0.048 min
Response: 37956625
Conc: 14.07 ug/ml

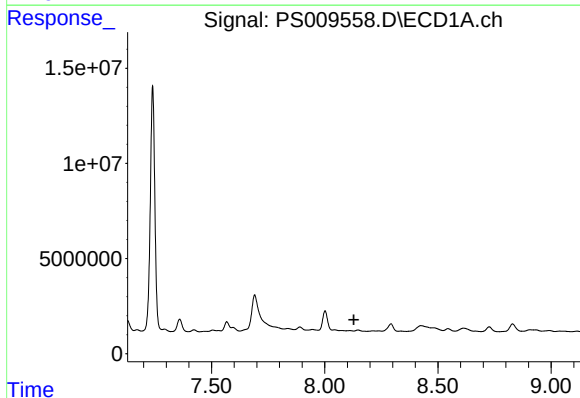


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.129 min
Response: 0
Conc: N.D.

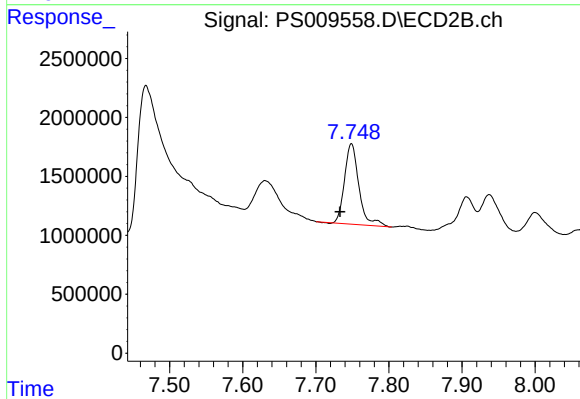

#8 DICHLORPROP


R.T.: 7.749 min
Delta R.T.: 0.016 min
Response: 9317904
Conc: 16.79 ng/ml

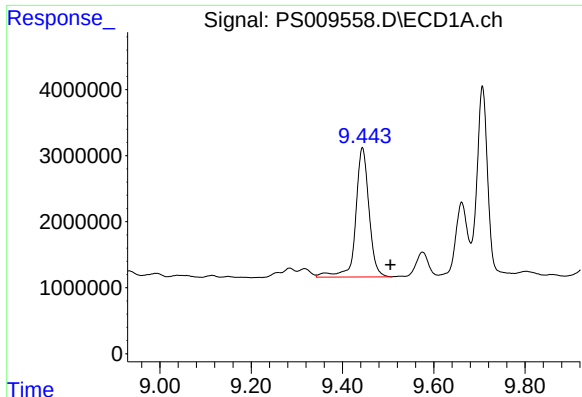

#12 2,4,5-T


R.T.: 9.444 min
Delta R.T.: -0.061 min
Response: 39673505
Conc: 15.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

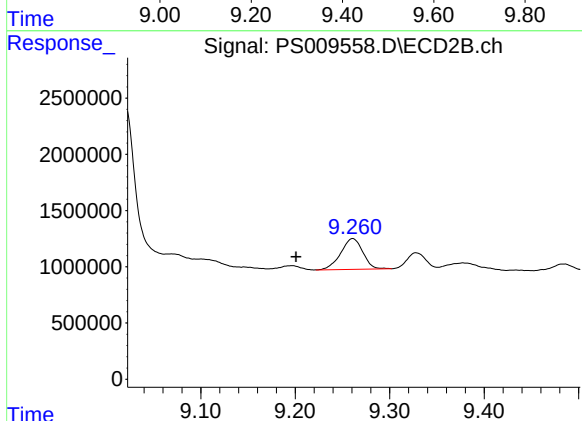


#12 2,4,5-T

R.T.: 9.261 min
Delta R.T.: 0.060 min
Response: 4436799
Conc: 1.50 ng/ml

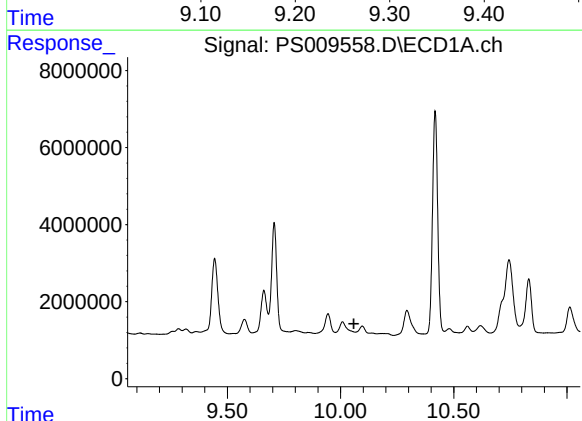


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.059 min
Response: 0
Conc: N.D.

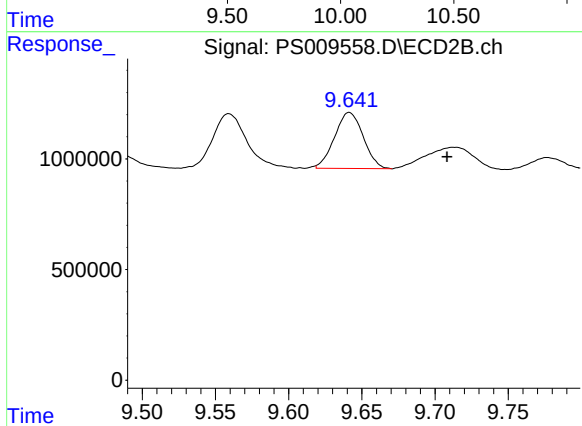

#13 2,4-DB


R.T.: 9.642 min
Delta R.T.: -0.067 min
Response: 3441572
Conc: 9.07 ng/ml

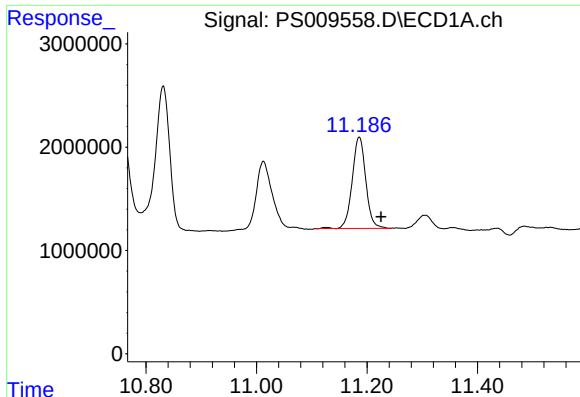

#14 DINOSEB


R.T.: 11.186 min
Delta R.T.: -0.039 min
Response: 15009874
Conc: 7.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

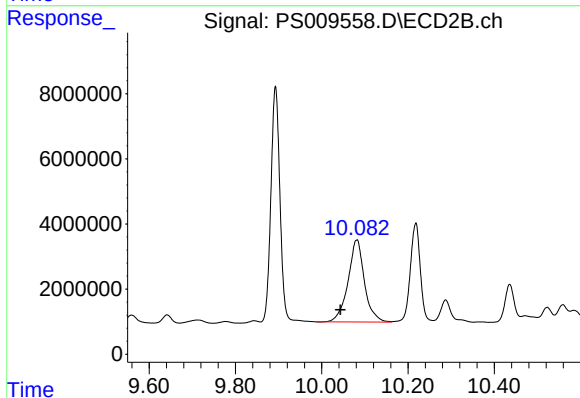


#14 DINOSEB

R.T.: 10.081 min
Delta R.T.: 0.038 min
Response: 66417677
Conc: 30.24 ng/ml

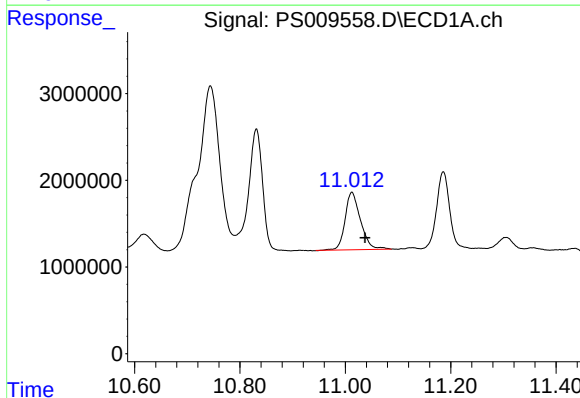

#15 Picloram

R.T.: 11.012 min
Delta R.T.: -0.025 min
Response: 13492759
Conc: 4.45 ng/ml

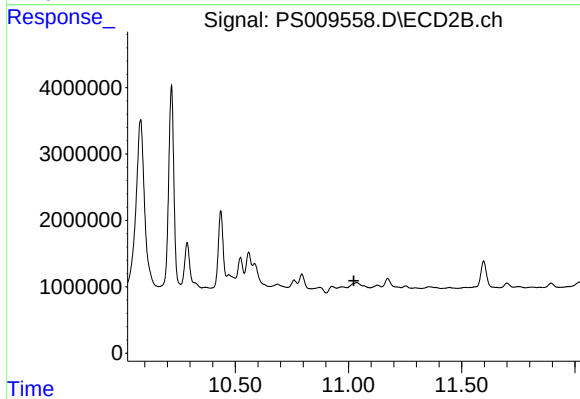

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.023 min
Response: 0
Conc: N.D.