

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040221\
 Data File : PS014453.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2021 12:47
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 01:02:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 18 02:23:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.162	6.887	700.4E6	256.4E6	490.201	543.413
Target Compounds							
9) T	2,4-D	8.333f	0.000	36384882	0	24.685	N.D. #
12) T	2,4,5-T	9.348f	0.000	4314298	0	<MDL	N.D. #
15) T	Picloram	10.914	11.002	5563140	10646829	<MDL	2.806 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040221\
Data File : PS014453.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2021 12:47
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 01:02:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
Quant Title : 8080.M
QLast Update : Thu Mar 18 02:23:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

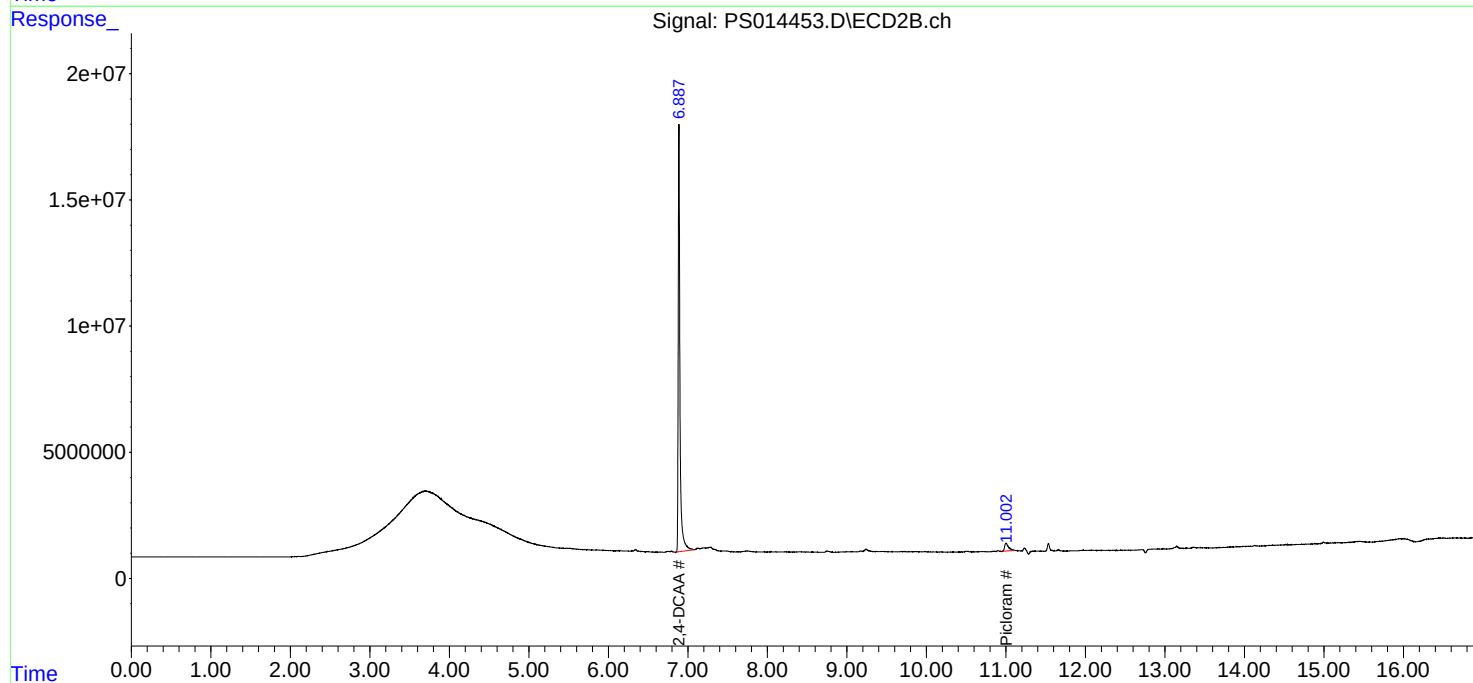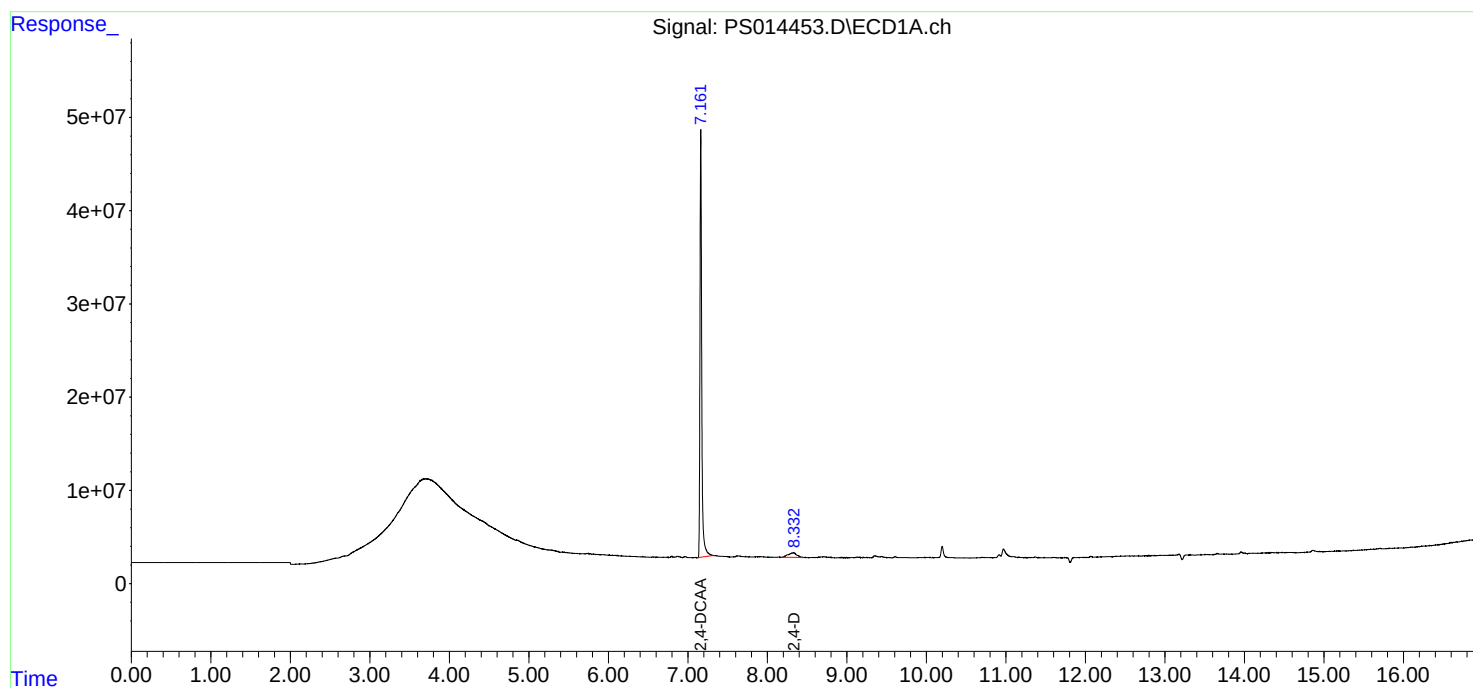


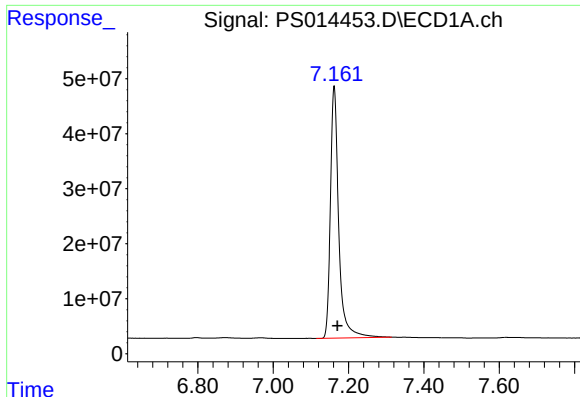

#4 2,4-DCAA


R.T.: 7.162 min
Delta R.T.: -0.008 min
Response: 700420432
Conc: 490.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

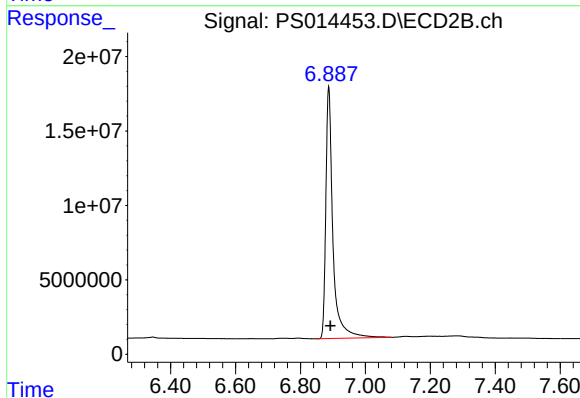


#4 2,4-DCAA

R.T.: 6.887 min
Delta R.T.: -0.005 min
Response: 256365420
Conc: 543.41 ng/ml

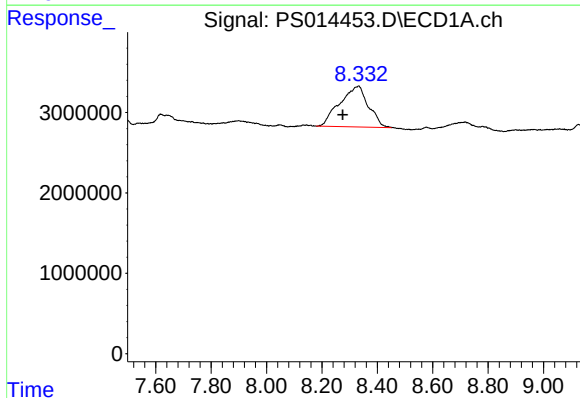


#9 2,4-D

R.T.: 8.333 min
Delta R.T.: 0.058 min
Response: 36384882
Conc: 24.68 ng/ml

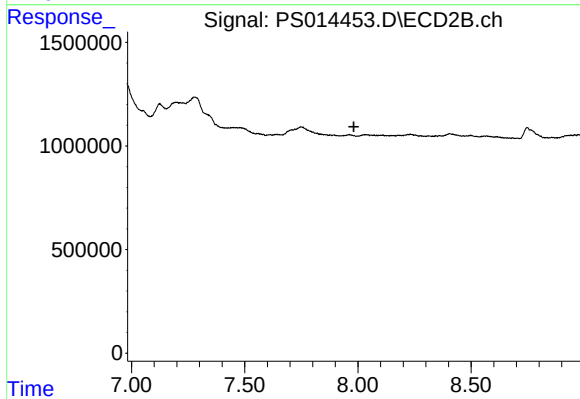

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.982 min
Response: 0
Conc: N.D.

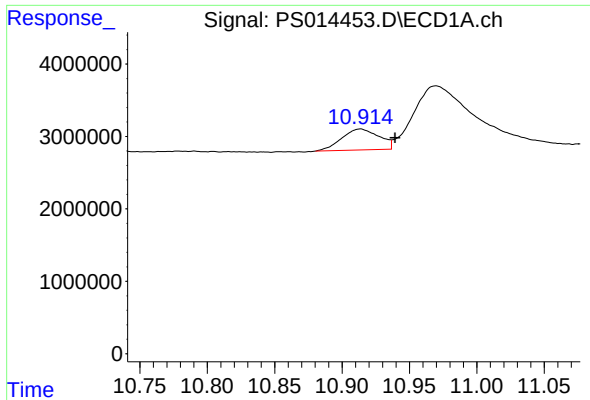

#15 Picloram

R.T.: 10.914 min
Delta R.T.: -0.026 min
Response: 5563140
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

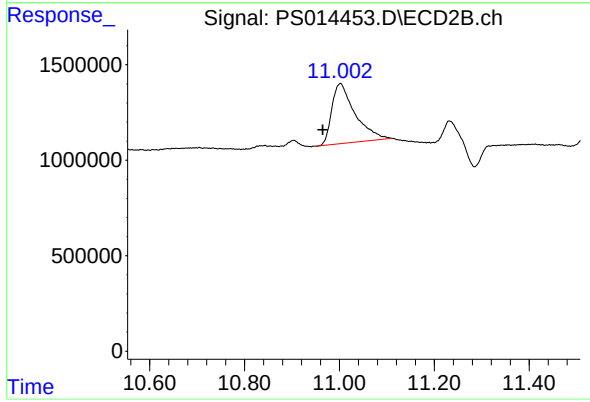

#15 Picloram

R.T.: 11.002 min
Delta R.T.: 0.037 min
Response: 10646829
Conc: 2.81 ng/ml