

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040323\
 Data File : PS022569.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2023 09:27
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 11:57:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032023.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 20 15:46:44 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.305	0.000	1009705	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.406	0.000	57377	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.736f	0.000	289191	0	<MDL	N.D. #
3) T	4-Nitroph...	6.139	0.000	1882845	0	1.374	N.D. #
5) T	DICAMBA	6.434	0.000	203007	0	<MDL	N.D. #
6) T	MCPD	6.658f	0.000	56741	0	<MDL	N.D. #
7) T	MCPA	6.658f	0.000	56741	0	<MDL	N.D. #
8) T	DICHLORPROP	7.019	7.535	397778	1199153	<MDL	<MDL #
9) T	2,4-D	7.223	0.000	491889	0	<MDL	N.D. #
10) T	Pentachlo...	7.436	0.000	1017520	0	<MDL	N.D. #
11) T	2,4,5-TP ...	7.987	0.000	1753908	0	<MDL	N.D. #
12) T	2,4,5-T	8.247	0.000	1263783	0	<MDL	N.D. #
13) T	2,4-DB	8.714	0.000	220022	0	<MDL	N.D. #
14) T	DINOSEB	9.792	0.000	613006	0	<MDL	N.D. #
15) T	Picloram	9.604	10.775	1431230	9144651	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040323\
Data File : PS022569.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2023 09:27
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 11:57:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032023.M
Quant Title : 8080.M
QLast Update : Mon Mar 20 15:46:44 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

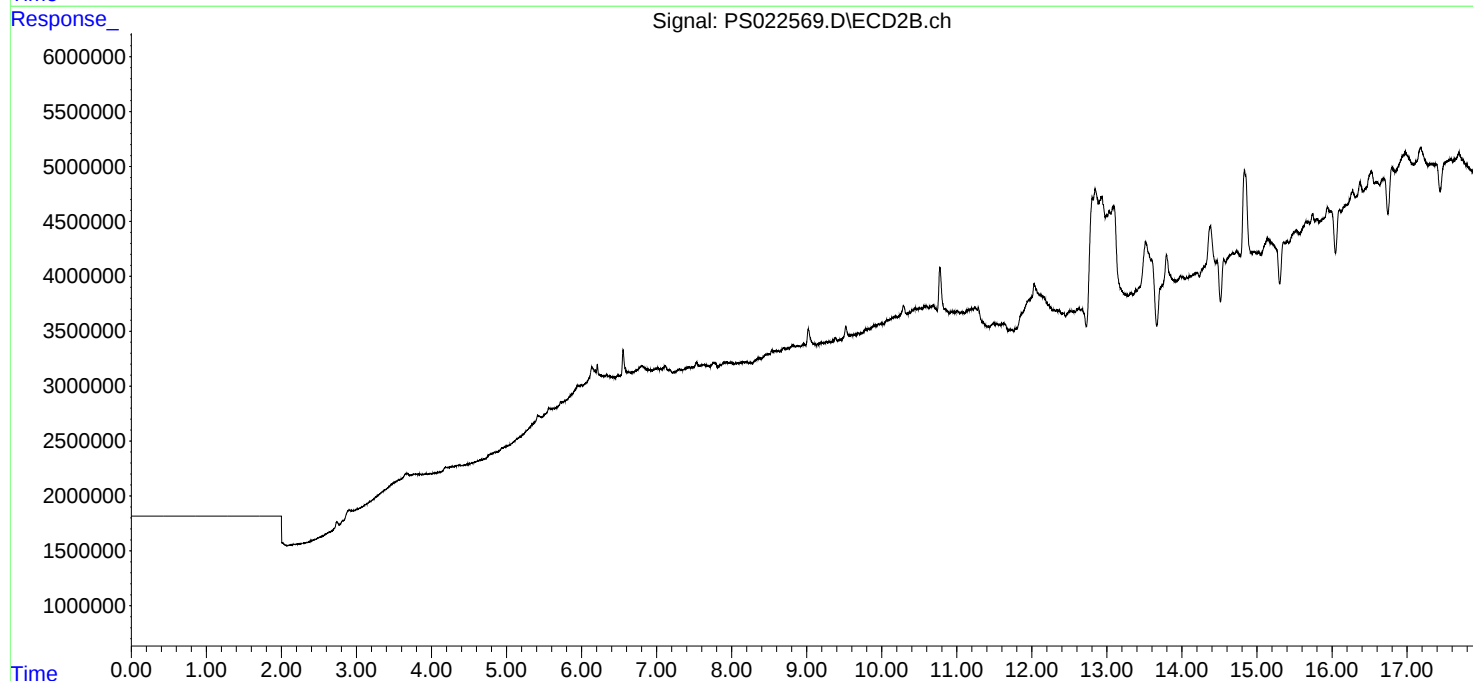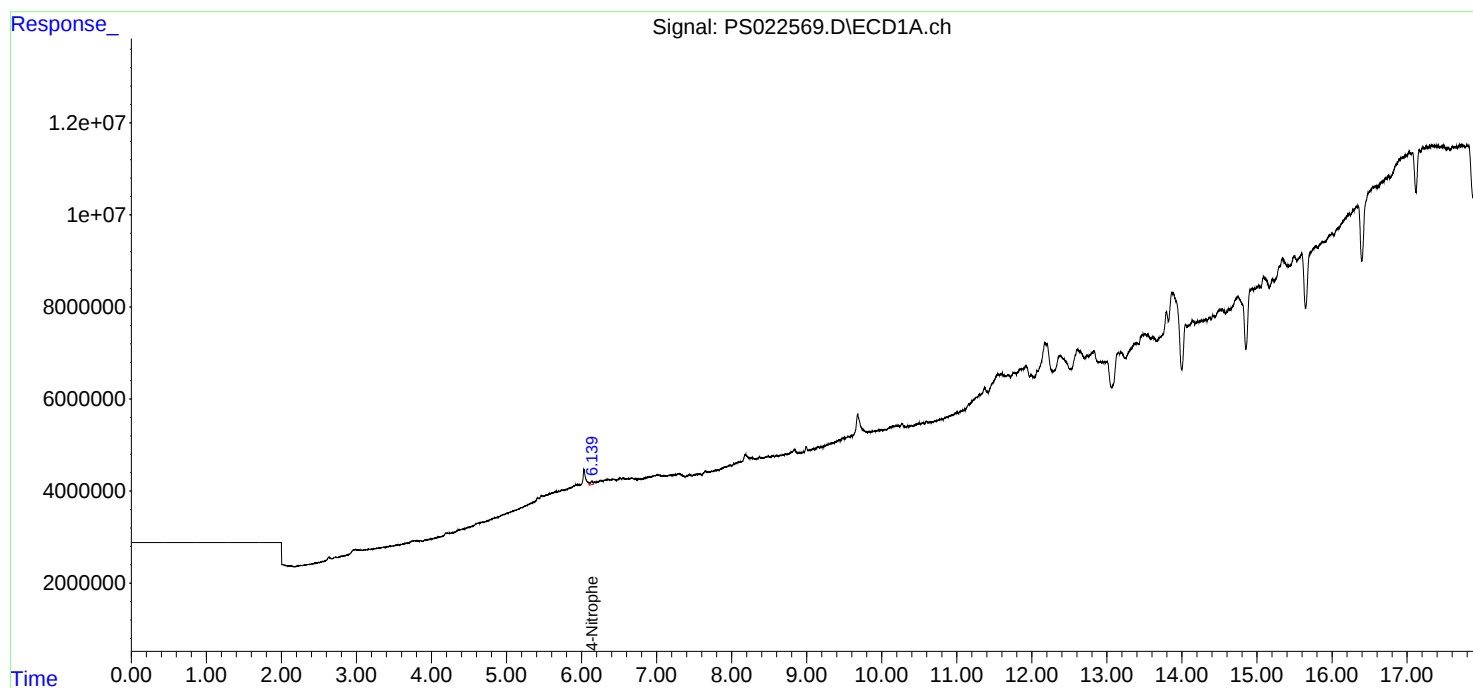


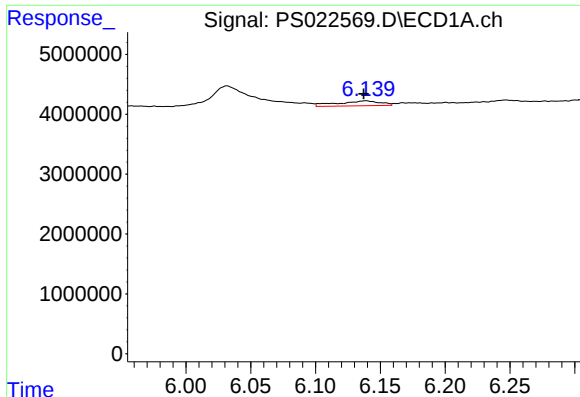

#3 4-Nitrophenol


R.T.: 6.139 min
Delta R.T.: 0.002 min
Response: 1882845
Conc: 1.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

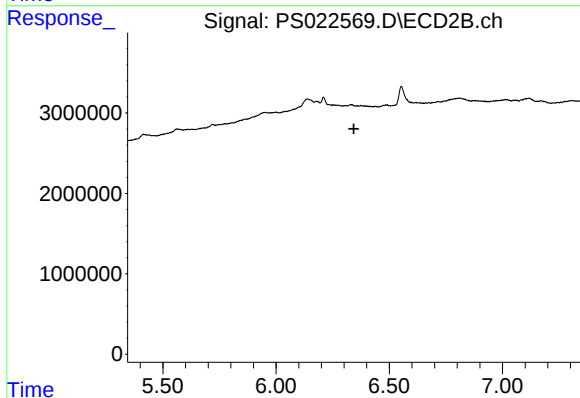


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.344 min
Response: 0
Conc: N.D.

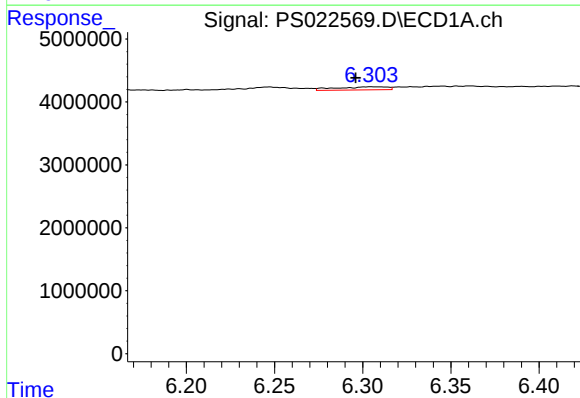

#4 2,4-DCAA

R.T.: 6.305 min
Delta R.T.: 0.009 min
Response: 1009705
Conc: N.D.

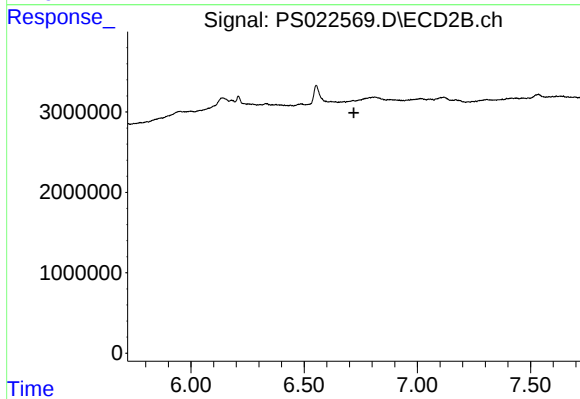

#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.719 min
Response: 0
Conc: N.D.